


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100825\
Data File : BF143886.D
Acq On : 08 Oct 2025 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 06 15:29:47 2025

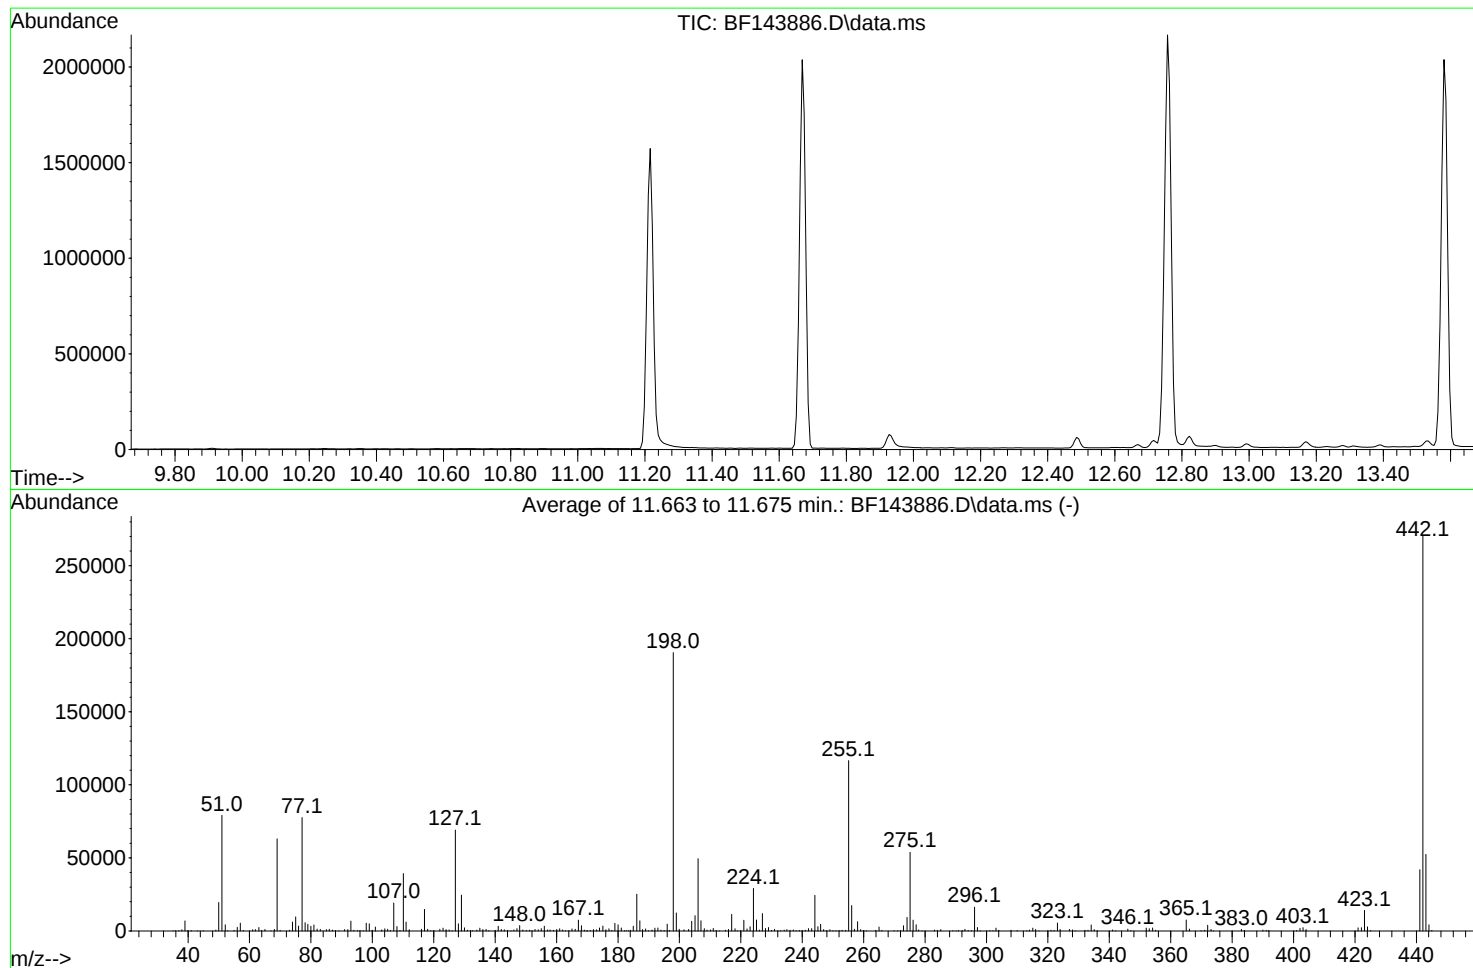




AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1604

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	1041	PASS
69	69	100	100	100.0	63059	PASS
70	69	0.00	2	0.6	363	PASS
197	198	0.00	2	0.2	431	PASS
198	198	100	100	100.0	190485	PASS
199	198	5	9	6.5	12350	PASS
365	198	1	100	3.9	7472	PASS
441	443	0.01	150	79.9	41901	PASS
442	442	100	100	100.0	270251	PASS
443	442	15	24	19.4	52419	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100825\
Data File : BF143886.D
Acq On : 08 Oct 2025 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 08 09:56:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

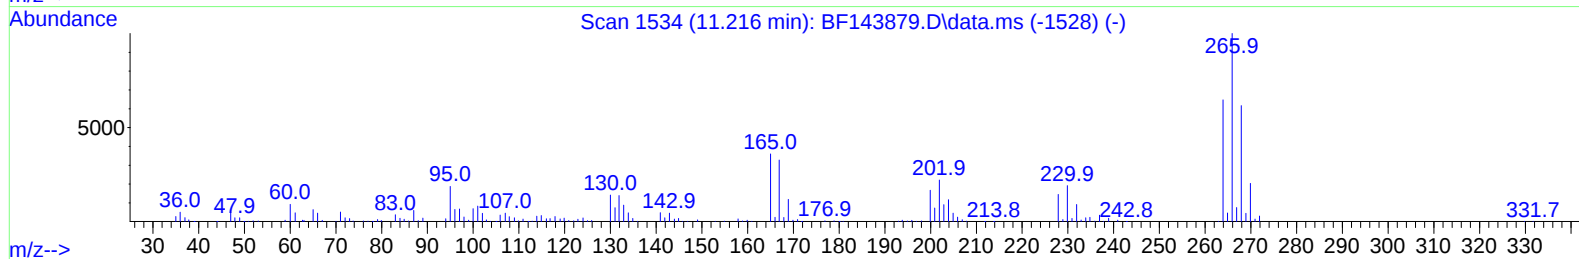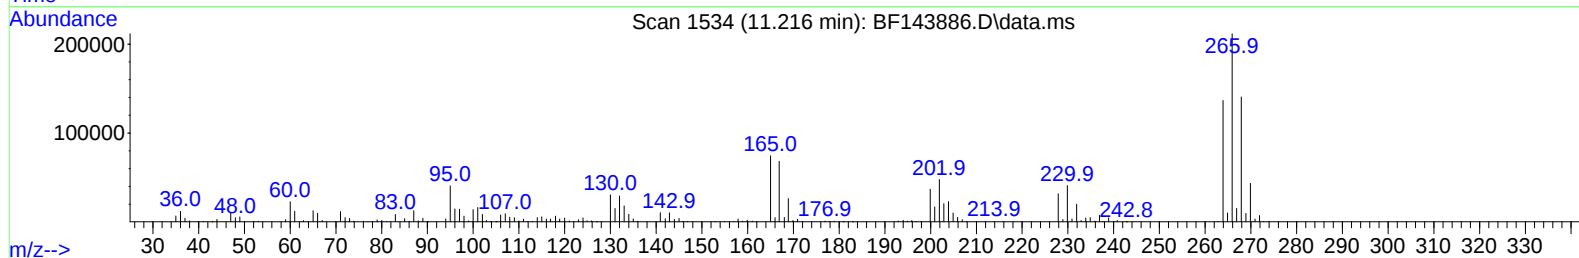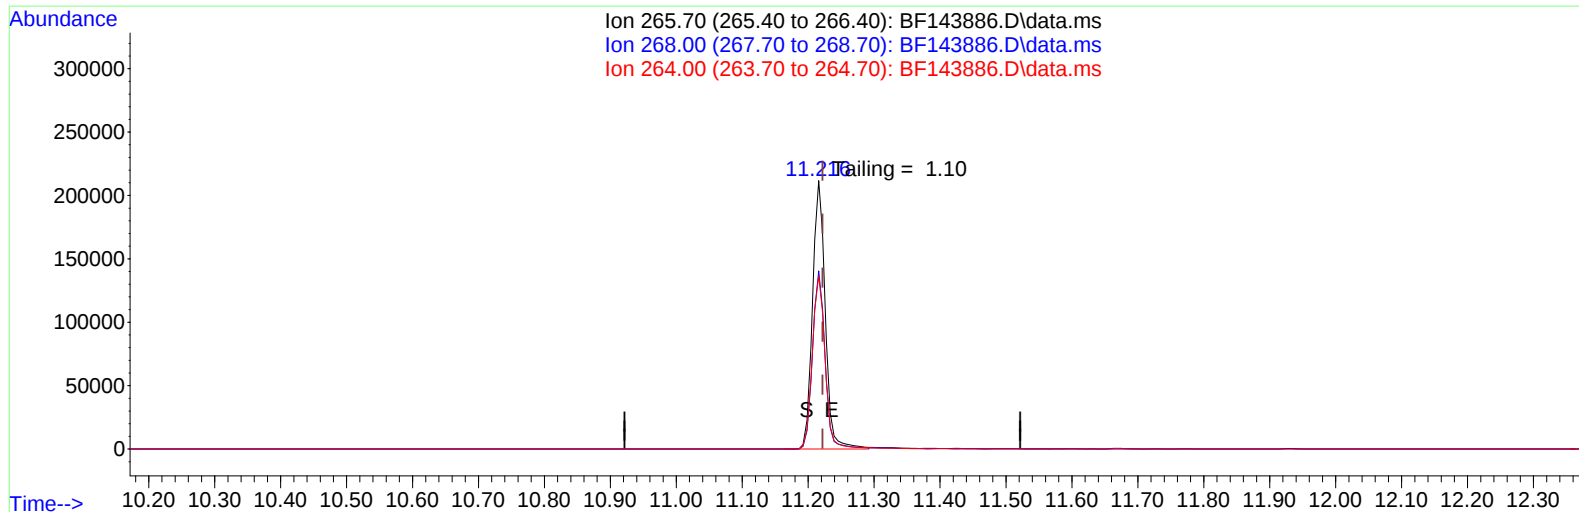

TIC: BF143886.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.006) 29768.94 ng




response 287874

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	66.38
264.00	64.70	64.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100825\
Data File : BF143886.D
Acq On : 08 Oct 2025 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 08 09:56:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

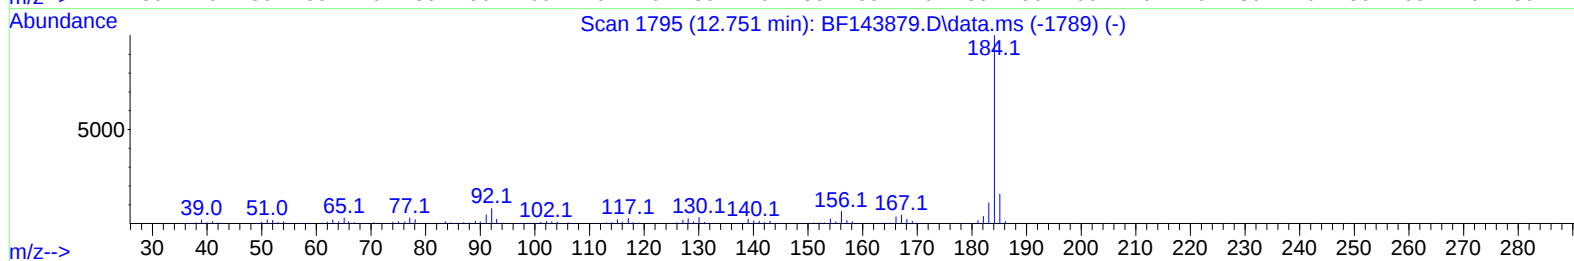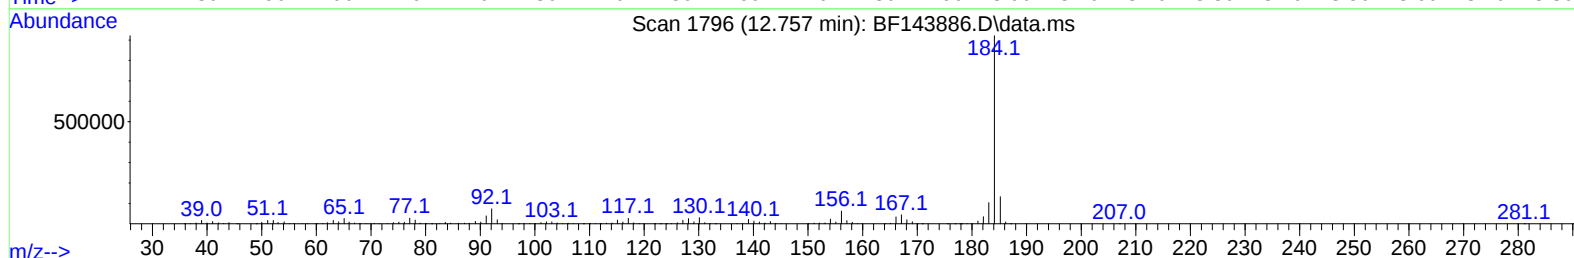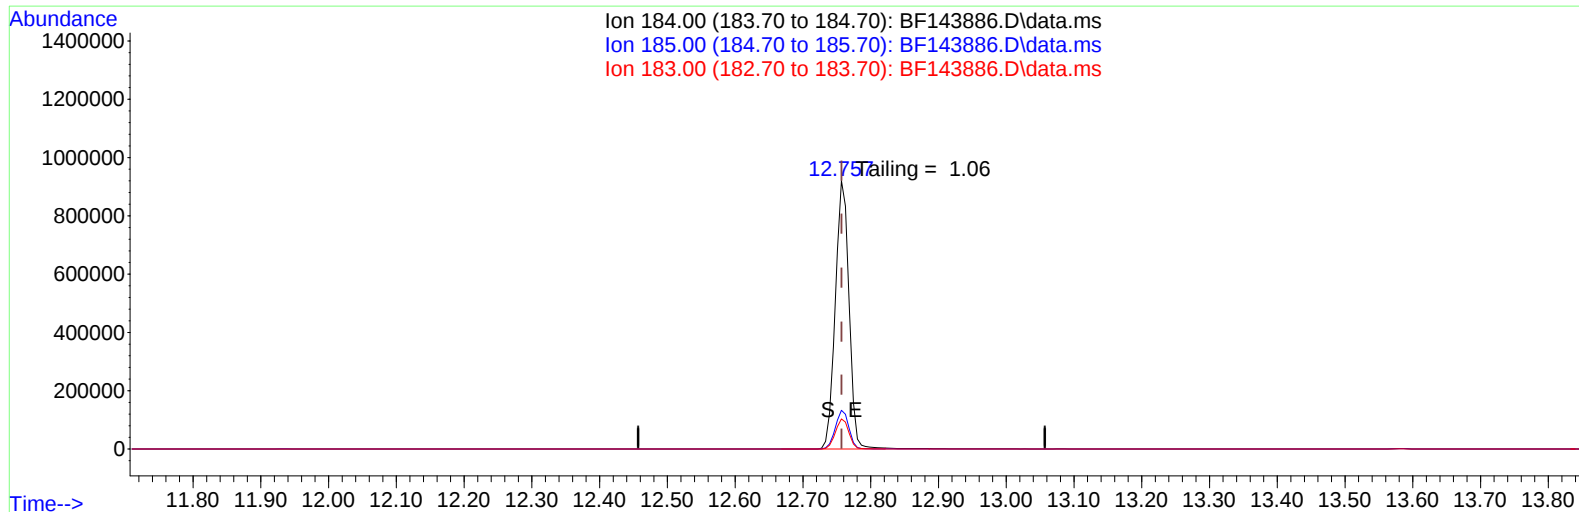

TIC: BF143886.D\data.ms

(77) Benzidine

12.757min (-0.000) 0.00 ng

response 1295126

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.44
183.00	11.00	11.22
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/8/2025	BNA_F	<u>BF143886.D</u>
Compound Name	Response	Retention Time
DDT	524359	13.58
DDD	4870	13.28
DDE	181	12.992
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5051	529410	0.95

Instrument :
BNA_F
ClientSampleId :
DFTPP