


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100625\
Data File : BP025923.D
Acq On : 06 Oct 2025 14:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 06 19:16:54 2025

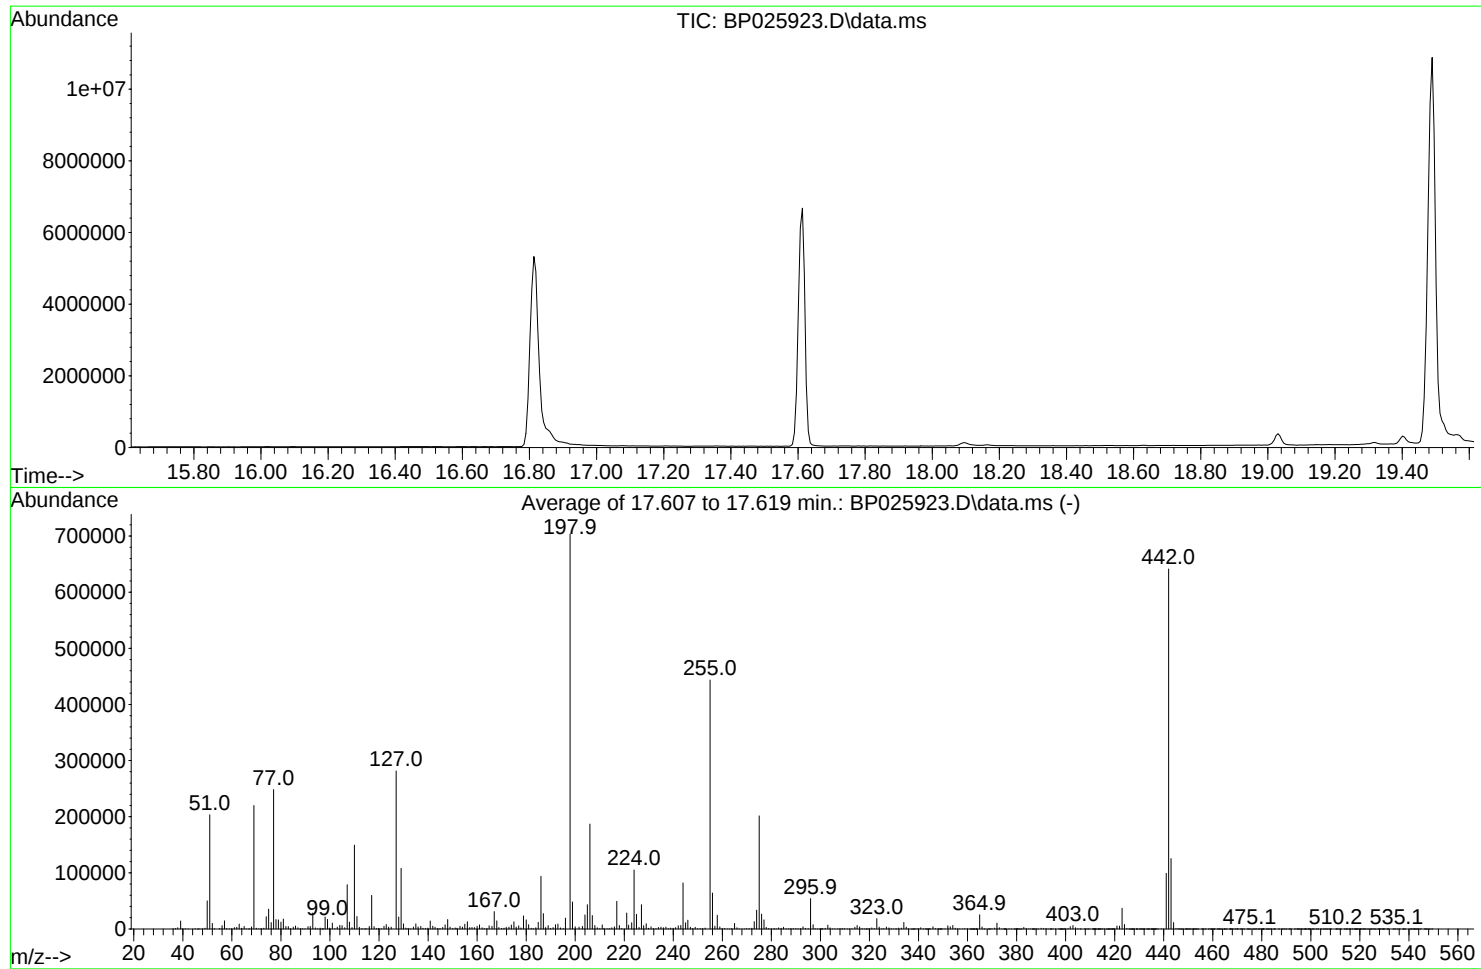


AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2483

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	3681	PASS
69	69	100	100	100.0	220105	PASS
70	69	0.00	2	0.6	1214	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	703552	PASS
199	198	5	9	6.8	48102	PASS
365	198	1	100	3.6	25214	PASS
441	443	0.01	150	78.9	98955	PASS
442	442	100	100	100.0	641402	PASS
443	442	15	24	19.6	125427	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100625\
Data File : BP025923.D
Acq On : 06 Oct 2025 14:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Oct 06 14:34:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

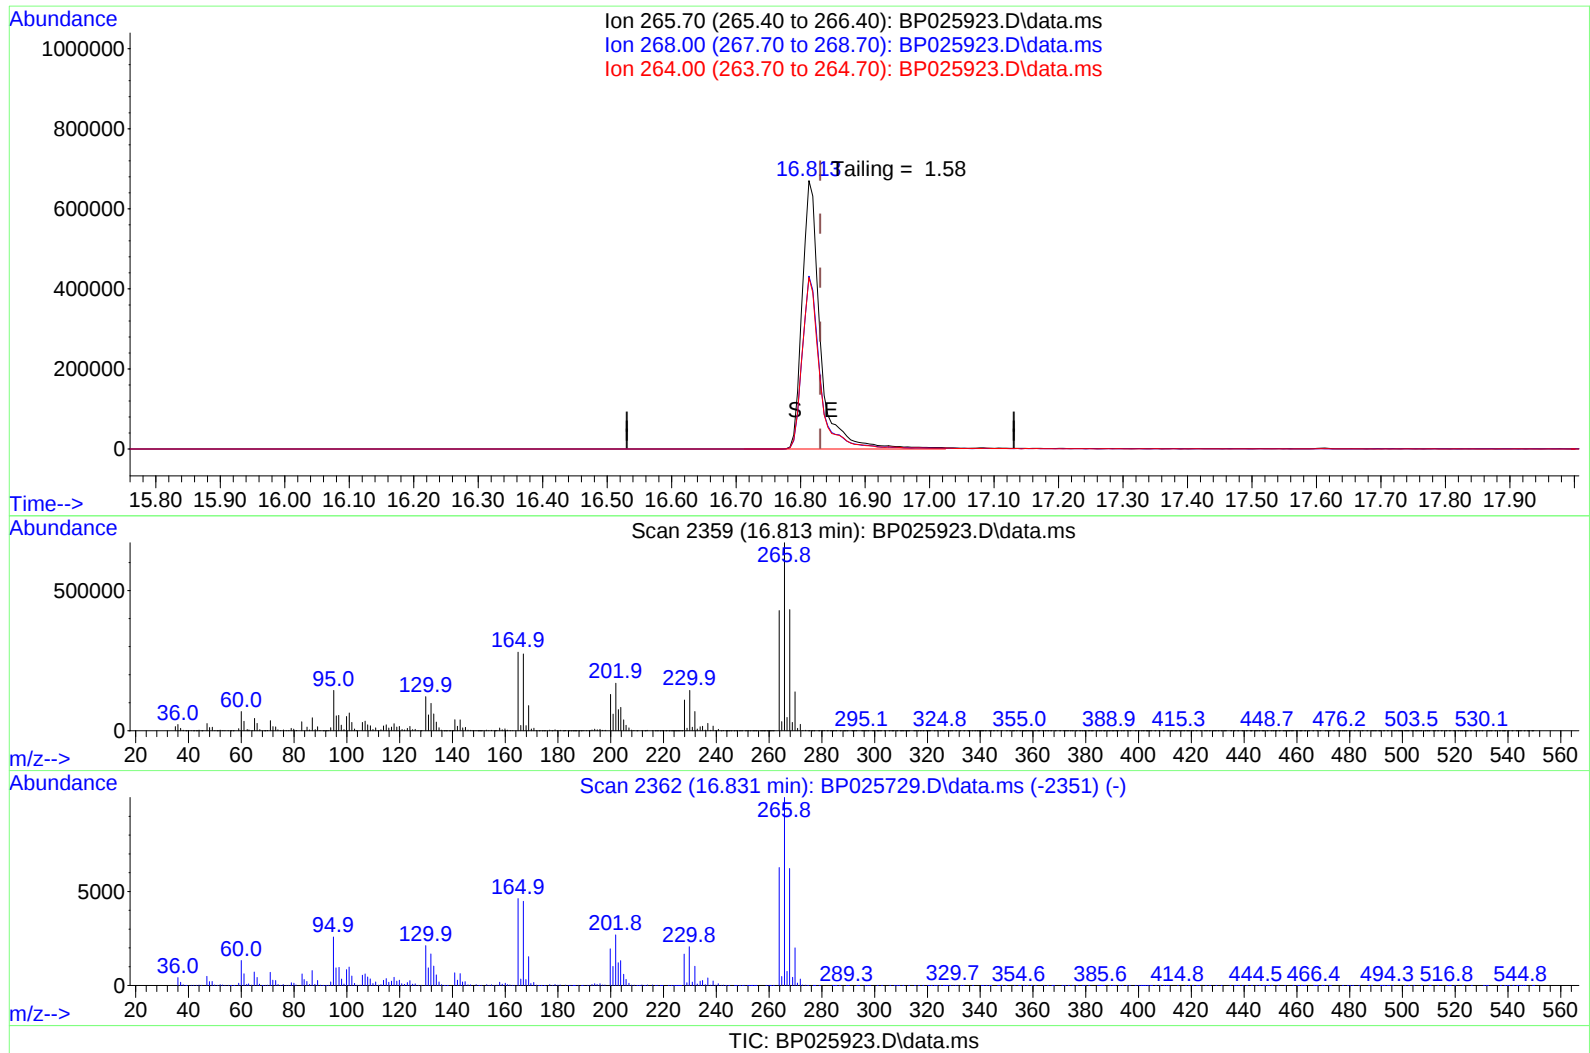

(70) Pentachlorophenol (C)

16.813min (-0.018) 3783600.35 ng




response 1315500

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.39
264.00	62.70	63.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100625\
Data File : BP025923.D
Acq On : 06 Oct 2025 14:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Oct 06 14:34:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

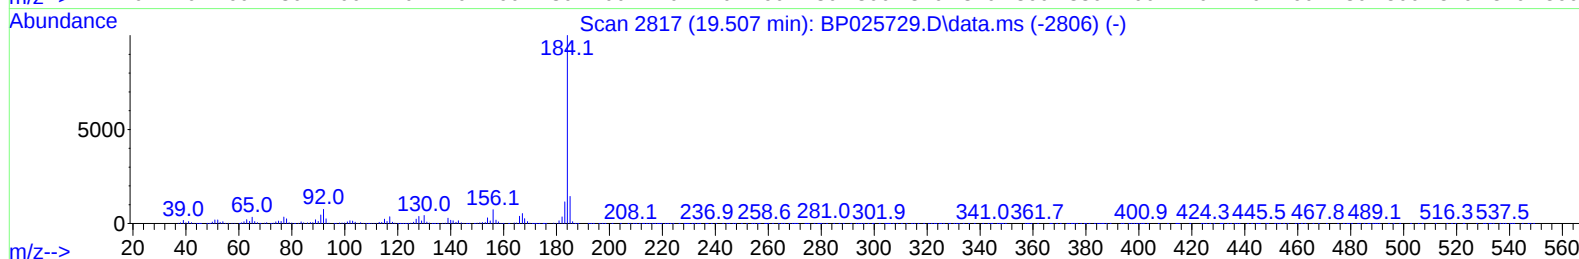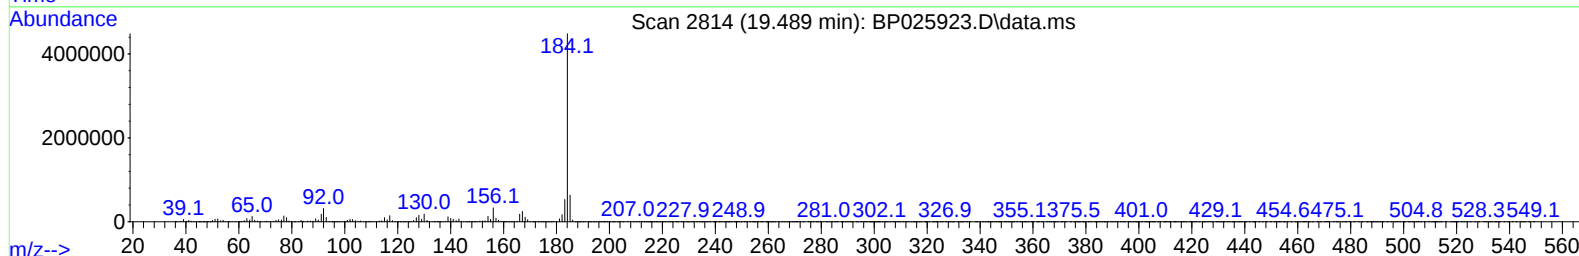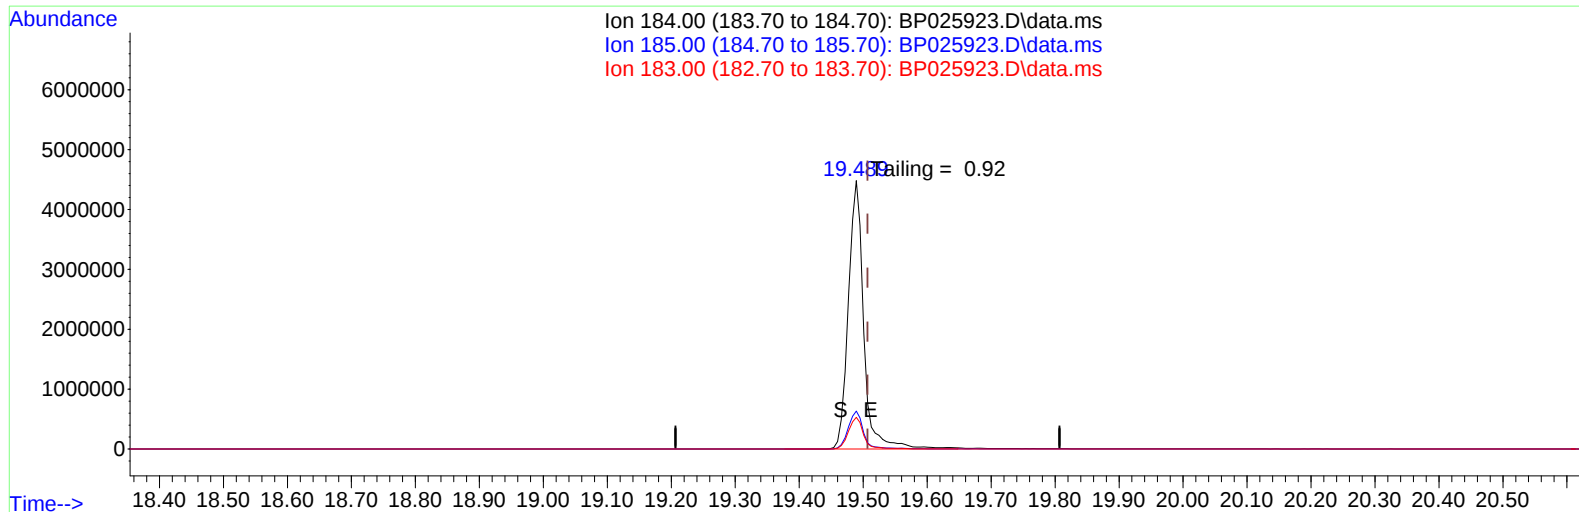

TIC: BP025923.D\data.ms

(77) Benzidine

19.489min (-0.018) 1941205.77 ng

response 7492893

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.14
183.00	11.50	11.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/6/2025	BNA_P	<u>BP025923.D</u>
Compound Name	Response	Retention Time
DDT	2978921	20.772
DDD	61119	20.313
DDE	18694	19.717
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
79813	3058734	2.61

Instrument :
BNA_P
ClientSampleId :
DFTPP