

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100825\
 Data File : BF143890.D
 Acq On : 08 Oct 2025 12:20
 Operator : RC/JU
 Sample : PB169953BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB169953BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143890.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.240	3	8	15	rVB	72033	119620	2.68%	0.437%
2	5.134	491	500	514	rBV	39313	68465	1.53%	0.250%
3	5.504	556	563	569	rBV	2633943	3738044	83.59%	13.642%
4	6.504	726	733	738	rBV	2583918	3950296	88.34%	14.416%
5	6.881	792	797	802	rBV	633259	776635	17.37%	2.834%
6	7.440	885	892	898	rBV	1721662	2453350	54.86%	8.953%
7	8.163	1009	1015	1020	rBV	768993	1008045	22.54%	3.679%
8	9.239	1191	1198	1203	rBV	3020258	4175379	93.37%	15.238%
9	9.922	1307	1314	1319	rBV	887882	1153184	25.79%	4.208%
10	10.710	1442	1448	1471	rBV	1986601	2675373	59.83%	9.764%
11	11.410	1562	1567	1574	rBV	957685	1204334	26.93%	4.395%
12	13.004	1832	1838	1843	rBV	3316771	4471676	100.00%	16.319%
13	14.057	2011	2017	2026	rBV	692372	899024	20.10%	3.281%
14	15.533	2262	2268	2284	rVB	429184	707966	15.83%	2.584%




Sum of corrected areas: 27401391

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100825\
Data File : BF143890.D
Acq On : 08 Oct 2025 12:20
Operator : RC/JU
Sample : PB169953BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB169953BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

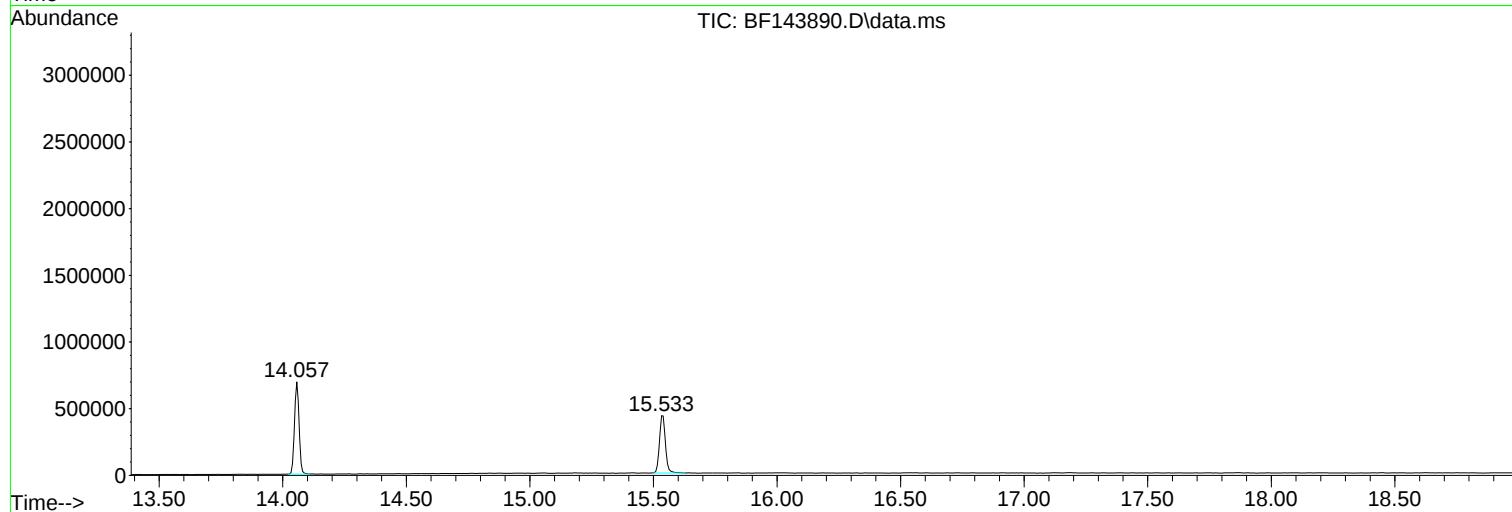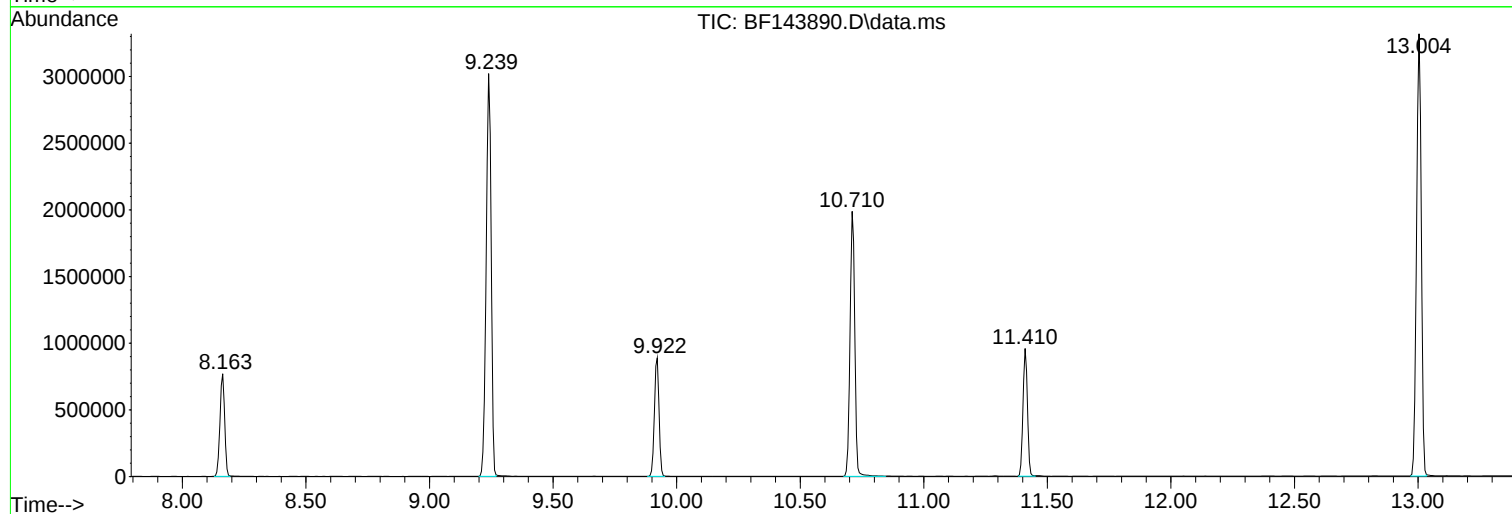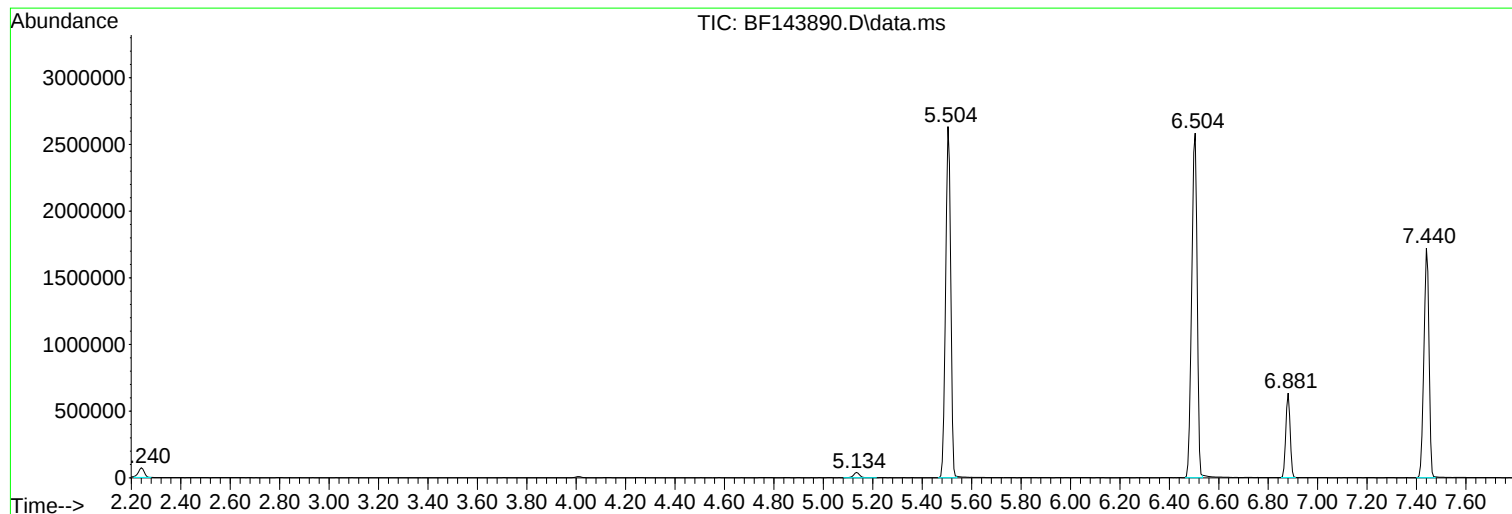

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100825\
Data File : BF143890.D
Acq On : 08 Oct 2025 12:20
Operator : RC/JU
Sample : PB169953BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB169953BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100825\
Data File : BF143890.D
Acq On : 08 Oct 2025 12:20
Operator : RC/JU
Sample : PB169953BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB169953BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------