Alliance TECHNICAL GROUP

284 Sheffield Street, Mountainside NJ 07092
Tel. 908-789-8900 Fax: 908-789-8922

DATA REPORTING QUALIFIERS- INORGANIC

For reporting results, the following " Results Qualifiers" are used:

J	Indicates the reported value was obtained from a reading that was less than the Contract Required Detection Limit (CRDL), but greater than or equal to the Instrument Detection Limit (IDL).
U	Indicates the analyte was analyzed for, but not detected.
ND	Indicates the analyte was analyzed for, but not detected
E	Indicates the reported value is estimated because of the presence of interference
M	Indicates Duplicate injection precision not met.
N	Indicates the spiked sample recovery is not within control limits.
S	Indicates the reported value was determined by the Method of Standard Addition (MSA).
*	Indicates that the duplicate analysis is not within control limits.
+	Indicates the correlation coefficient for the MSA is less than 0.995.
D	Indicates the reported value is from a secondary analysis with a dilution factor. The original analysis exceeded the calibration range.
M	Method qualifiers **"P"** for ICP instrument **"PM"** for ICP when Microwave Digestion is used **"CV"** for Manual Cold Vapor AA **"AV"** for automated Cold Vapor AA **"CA"** for MIDI-Distillation Spectrophotometric **"AS"** for Semi –Automated Spectrophotometric **"C"** for Manual Spectrophotometric **"T"** for Titrimetric **"NR"** for analyte not required to be analyzed
OR	Indicates the analyte's concentration exceeds the calibrated range of the instrument for that specific analysis.
Q	Indicates the LCS did not meet the control limits requirements
H	Sample Analysis Out Of Hold Time

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

LAB CHRONICLE

OrderID:	Q3267	**OrderDate:**	10/1/2025 3:37:00 PM
Client:	METEM A GE POWER Business	**Project:**	Parsippany Wastewater Quarterly 2025
Contact:	Sundas Pervez	**Location:**	D31

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q3267-01	**Q4**	**WATER**			**10/01/25 15:00**			**10/01/25**
			Cyanide	SM4500-CN C,E		10/06/25	10/06/25 14:51	
			Field pH	SM4500-H B			10/01/25 15:02	

Alliance
TECHNICAL GROUP

SAMPLE DATA

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	METEM A GE POWER Business	Date Collected:	10/01/25 15:00
Project:	Parsippany Wastewater Quarterly 2025	Date Received:	10/01/25
Client Sample ID:	Q4	SDG No.:	Q3267
Lab Sample ID:	Q3267-01	Matrix:	WATER
		% Solid:	0

Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Prep Date	Date Ana.	Ana Met.
Cyanide	0.0012	U	1	0.0012	0.0050	mg/L	10/06/25 11:05	10/06/25 14:51	SM 4500-CN C-21 plus E-21
Field pH	7.64		1	0	0	pH		10/01/25 15:02	SM4500-H B

Comments:

U = Not Detected
LOQ = Limit of Quantitation
MDL = Method Detection Limit
LOD = Limit of Detection
D = Dilution
Q = indicates LCS control criteria did not meet requirements
H = Sample Analysis Out Of Hold Time

J = Estimated Value
B = Analyte Found in Associated Method Blank
* = indicates the duplicate analysis is not within control limits.
E = Indicates the reported value is estimated because of the presence of interference.
OR = Over Range
N =Spiked sample recovery not within control limits

QC RESULT SUMMARY

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Initial and Continuing Calibration Verification

Client:	METEM A GE POWER Business	**SDG No.:**	Q3267
Project:	Parsippany Wastewater Quarterly 2025	**RunNo.:**	LB137435

Analyte		Units	Result	True Value	% Recovery	Acceptance Window (%R)	Analysis Date
Sample ID:	**ICV1**						
Cyanide		mg/L	0.095	0.099	96	85-115	10/06/2025
Sample ID:	**CCV1**						
Cyanide		mg/L	0.24	0.25	96	90-110	10/06/2025
Sample ID:	**CCV2**						
Cyanide		mg/L	0.24	0.25	96	90-110	10/06/2025

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Initial and Continuing Calibration Verification

Client:	METEM A GE POWER Business	**SDG No.:**	Q3267
Project:	Parsippany Wastewater Quarterly 2025	**RunNo.:**	LB137498

Analyte	Units	Result	True Value	% Recovery	Acceptance Window (%R)	Analysis Date
Sample ID: **ICV**						
Field pH	pH	7.01	7	100	90-110	10/01/2025
Sample ID: **CCV1**						
Field pH	pH	7.00	7	100	90-110	10/01/2025
Sample ID: **CCV2**						
Field pH	pH	7.01	7	100	90-110	10/01/2025

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Initial and Continuing Calibration Verification

Client:	METEM A GE POWER Business	**SDG No.:**	Q3267
Project:	Parsippany Wastewater Quarterly 2025	**RunNo.:**	LB137498

Analyte	Units	Result	True Value	% Recovery	Acceptance Window (%R)	Analysis Date

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Initial and Continuing Calibration Blank Summary

Client: METEM A GE POWER Business **SDG No.:** Q3267

Project: Parsippany Wastewater Quarterly 2025 **RunNo.:** LB137435

Analyte		Units	Result	Acceptance Limits	Conc Qual	MDL	RDL	Analysis Date
Sample ID:	ICB1							
Cyanide		mg/L	< 0.0025	0.0025	U	0.0012	0.005	10/06/2025
Sample ID:	CCB1							
Cyanide		mg/L	< 0.0025	0.0025	U	0.0012	0.005	10/06/2025
Sample ID:	CCB2							
Cyanide		mg/L	< 0.0025	0.0025	U	0.0012	0.005	10/06/2025

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Initial and Continuing Calibration Blank Summary

Client:	METEM A GE POWER Business	**SDG No.:**	Q3267
Project:	Parsippany Wastewater Quarterly 2025	**RunNo.:**	LB137435

Analyte	Units	Result	Acceptance Limits	Conc Qual	MDL	RDL	Analysis Date

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Preparation Blank Summary

Client: METEM A GE POWER Business **SDG No.:** Q3267

Project: Parsippany Wastewater Quarterly 2025

Analyte	Units	Result	Acceptance Limits	Conc Qual	MDL	RDL	Analysis Date
Sample ID:	**PB169962BL**						
Cyanide	mg/L	< 0.0025	0.0025	U	0.0012	0.005	10/06/2025

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Matrix Spike Summary

Client: METEM A GE POWER Business
SDG No.: Q3267
Project: Parsippany Wastewater Quarterly 2025
Sample ID: Q3258-01
Client ID: MONTHLY-CYANIDE MS
Percent Solids for Spike Sample: 0

Analyte	Units	Acceptance Limit %R	Spiked Result	Conc. Qualifier	Sample Result	Conc. Qualifier	Spike Added	Dilution Factor	% Rec	Qual	Analysis Date
Cyanide	mg/L	75-125	0.28		0.25		0.04	1	75		10/06/2025

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Matrix Spike Summary

Client: METEM A GE POWER Business
SDG No.: Q3267
Project: Parsippany Wastewater Quarterly 2025
Sample ID: Q3258-01
Client ID: MONTHLY-CYANIDE MSD
Percent Solids for Spike Sample: 0

Analyte	Units	Acceptance Limit %R	Spiked Result	Conc. Qualifier	Sample Result	Conc. Qualifier	Spike Added	Dilution Factor	% Rec	Qual	Analysis Date
Cyanide	mg/L	75-125	0.28		0.25		0.04	1	75		10/06/2025

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Duplicate Sample Summary

Client: METEM A GE POWER Business
SDG No.: Q3267
Project: Parsippany Wastewater Quarterly 2025
Sample ID: Q3258-01
Client ID: MONTHLY-CYANIDE DUP
Percent Solids for Spike Sample: 0

Analyte	Units	Acceptance Limit	Sample Result	Conc. Qualifier	Duplicate Result	Conc. Qualifier	Dilution Factor	RPD/ AD	Qual	Analysis Date
Cyanide	mg/L	+/-20	0.25		0.24		1	4		10/06/2025

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Duplicate Sample Summary

Client: METEM A GE POWER Business
SDG No.: Q3267
Project: Parsippany Wastewater Quarterly 2025
Sample ID: Q3258-01
Client ID: MONTHLY-CYANIDE MSD
Percent Solids for Spike Sample: 0

Analyte	Units	Acceptance Limit	Sample Result	Conc. Qualifier	Duplicate Result	Conc. Qualifier	Dilution Factor	RPD/ AD	Qual	Analysis Date
Cyanide	mg/L	+/-20	0.28		0.28		1	0		10/06/2025

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Duplicate Sample Summary

Client: METEM A GE POWER Business
SDG No.: Q3267
Project: Parsippany Wastewater Quarterly 2025
Sample ID: Q3267-01
Client ID: Q4DUP
Percent Solids for Spike Sample: 0

Analyte	Units	Acceptance Limit	Sample Result	Conc. Qualifier	Duplicate Result	Conc. Qualifier	Dilution Factor	RPD/ AD	Qual	Analysis Date
Field pH	pH	+/-20	7.64		7.64		1	0		10/01/2025

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Laboratory Control Sample Summary

Client:	METEM A GE POWER Business	**SDG No.:**	Q3267
Project:	Parsippany Wastewater Quarterly 2025	**Run No.:**	LB137435

Analyte	Units	True Value	Result	Conc. Qualifier	% Recovery	Dilution Factor	Acceptance Limit %R	Analysis Date
Sample ID **PB169962BS**								
Cyanide	mg/L	0.1	0.096		96	1	85-115	10/06/2025

RAW DATA

LB137435

Test results | Aquakem 7.2AQ1 | Page: 1

Alliance Technical Group
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM | Instrument ID : Konelab

10/6/2025 14:54

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.404	0.0	0.084	
ICB1	0.529	0.0	0.001	
CCV1	240.797	0.0	0.212	
CCB1	0.363	0.0	0.001	
RL CHECK	5.266	0.0	0.005	105% (50-150)
PB169962BL	0.096	0.0	0.001	
PB169962BS	96.246	0.0	0.085	
MIDPB169962	240.808	0.0	0.212	96% (90-110) 10/06/2025 RM
Q3258-01	245.338	0.0	0.216	
Q3258-01DUP	243.665	0.0	0.215	
Q3258-02MS	282.012	0.0	0.248	
Q3258-03MSD	281.906	0.0	0.248	
Q3258-04	2.433	0.0	0.003	
Q3267-01	0.491	0.0	0.001	
CCV2	240.656	0.0	0.212	
CCB2	0.108	0.0	0.001	

N	16
Mean	123.507
SD	122.9600
CV%	99.56

Aquakem v. 7.2AQ1
Results from time period:
Mon Oct 06 14:36:09 2025
Mon Oct 06 14:54:04 2025

Sample Id	Sam/Ctr/cA	Test short r	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.1146	µg/l	10/6/2025 11:48:33	
5.0PPBCN	A	Total CN	P	5.1765	µg/l	10/6/2025 11:48:34	
10PPBCN	A	Total CN	P	10.0597	µg/l	10/6/2025 11:48:35	
50PPBCN	A	Total CN	P	48.076	µg/l	10/6/2025 11:48:36	
100PPBCN	A	Total CN	P	101.2694	µg/l	10/6/2025 11:48:37	
250PPBCN	A	Total CN	P	251.1949	µg/l	10/6/2025 11:48:38	
500PPBCN	A	Total CN	P	499.3381	µg/l	10/6/2025 11:48:39	
ICV1	S	Total CN	P	95.4036	µg/l	10/6/2025 14:36:10	
ICB1	S	Total CN	P	0.5289	µg/l	10/6/2025 14:36:12	
CCV1	S	Total CN	P	240.7973	µg/l	10/6/2025 14:36:14	
CCB1	S	Total CN	P	0.3632	µg/l	10/6/2025 14:36:16	
RL CHECK	S	Total CN	P	5.2656	µg/l	10/6/2025 14:36:17	
PB169962BL	S	Total CN	P	0.0959	µg/l	10/6/2025 14:43:42	
PB169962BS	S	Total CN	P	96.2458	µg/l	10/6/2025 14:43:44	
MIDPB169962	S	Total CN	P	240.8082	µg/l	10/6/2025 14:43:46	
Q3258-01	S	Total CN	P	245.3385	µg/l	10/6/2025 14:43:48	
Q3258-01DUP	S	Total CN	P	243.6653	µg/l	10/6/2025 14:43:51	
Q3258-02MS	S	Total CN	P	282.0124	µg/l	10/6/2025 14:51:18	
Q3258-03MSD	S	Total CN	P	281.9064	µg/l	10/6/2025 14:51:19	
Q3258-04	S	Total CN	P	2.4328	µg/l	10/6/2025 14:51:20	
Q3267-01	S	Total CN	P	0.4914	µg/l	10/6/2025 14:51:21	
CCV2	S	Total CN	P	240.6565	µg/l	10/6/2025 14:51:24	
CCB2	S	Total CN	P	0.1076	µg/l	10/6/2025 14:51:26	

Calibration results Aquakem 7.2AQ1 Page: 1

Alliance Technical Group
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM Instrument ID : Konelab

10/6/2025 11:49

Test Total CN

Accepted 10/6/2025 11:49

Factor 1138
Bias 0.001

Coeff. of det. 0.999965

Errors

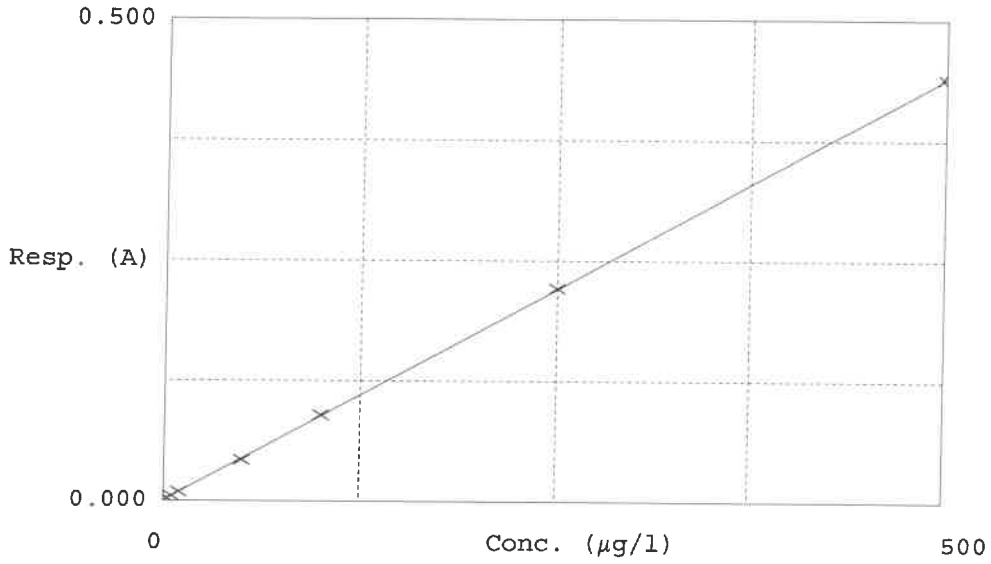

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.1146	0.0000	-
2	5.0PPBCN	0.005	5.1765	5.0000	3.5
3	10PPBCN	0.009	10.0597	10.0000	0.6
4	50PPBCN	0.043	48.0760	50.0000	-3.8
5	100PPBCN	0.090	101.2694	100.0000	1.3
6	250PPBCN	0.221	251.1949	250.0000	0.5
7	500PPBCN	0.439	499.3381	500.0000	-0.1

10/06/2025
RM

Alliance TECHNICAL GROUP

Water Cyanide Preparation Sheet

PB169962

SOP ID : MSM4500-CN C,E-Cyanide-13

SDG No : N/A

Start Digest Date: 10/06/2025 **Time :** 11:05 **Temp :** 123 °C

Matrix : WATER

End Digest Date: 10/06/2025 **Time :** 12:35 **Temp :** 127 °C

Pippete ID : WC

Balance ID : N/A

Hood ID : HOOD#1 **Digestion tube ID :** M5595 **Block Thermometer ID :** WC CYANIDE

Block ID : MC-1,MC-2 **Filter paper ID :** N/A **Prep Technician Signature:** JP

Weigh By : N/A **pH Meter ID :** N/A **Supervisor Signature:** 12

Standared Name	MLS USED	STD REF. # FROM LOG
LCSW	1.0ML	WP113838
MS/MSD SPIKE SOL.	0.40ML	WP113837
PBW	50.0ML	W3112
RL CHECK	50.0ML	WP115062
N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
0.25N NaOH	50.0ML	WP113836
50% v/v H2SO4	5.0ML	WP112826
51% w/v MgCL2	2.0ML	WP112827
pH Paper 0-14	N/A	W3215
Nitrate/Nitrite Strip	N/A	W3182
Lead Acetate strip	N/A	W3134
KI-starch paper	N/A	W3155
0.4N Sulfamic Acid	5.ML	WP112829
N/A	N/A	N/A
N/A	N/A	N/A

LAB SAMPLE ID	CLIENT SAMPLE ID	Wt(g)/Vol(ml)	Comment
S0	S0	N/A	N/A
S5.0	S5.0	N/A	N/A
S10.0	S10.0	N/A	N/A
S100.0	S100.0	N/A	N/A
S250.0	S250.0	N/A	N/A
S500.0	S500.0	N/A	N/A
ICV	ICV	0.5ML	W3012
ICB	ICB	N/A	N/A
CCV	CCV	N/A	N/A
CCB	CCB	N/A	N/A
Midrange	Midrange	2.5ML	WP113837
HIGHSTD	HIGHSTD	N/A	N/A
LOWSTD	LOWSTD	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

N/A

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
10/06/2025 12:50	JP / WC	RM (WC)
	Preparation Group	Analysis Group

Alliance TECHNICAL GROUP

Water Cyanide Preparation Sheet

PB169962

Lab Sample ID	Client Sample ID	Initial Vol (ml)	Final Vol (ml)	pH	Sulfide	Oxidizing	Nitrate/ Nitrite	Comment	Prep Pos
PB169962BL	PBW962	50	50	>12	Negative	Negative	Negative	N/A	N/A
PB169962BS	LCS962	50	50	>12	Negative	Negative	Negative	N/A	N/A
Q3258-01DUP	MONTHLY-CYANIDE DUP	50	50	>12	Negative	Negative	Negative	N/A	N/A
Q3258-01	MONTHLY-CYANIDE	50	50	>12	Negative	Negative	Negative	N/A	N/A
Q3258-02	Q3258-01MS	50	50	>12	Negative	Negative	Negative	N/A	N/A
Q3258-03	Q3258-01MSD	50	50	>12	Negative	Negative	Negative	N/A	N/A
Q3258-04	ADDTIONAL-CYANIDE-3	50	50	>12	Negative	Negative	Negative	N/A	N/A
Q3267-01	Q4	50	50	>12	Negative	Negative	Positive	N/A	N/A

WORKLIST(Hardcopy Internal Chain)

WorkList Name : cn-10-06 **WorkList ID :** 192302 **Department :** Distillation **Date :** 10-06-2025 07:42:42

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q3258-01	MONTHLY-CYANIDE	Water	Cyanide	Cool 4 deg C	DALT01	D31	09/29/2025	SM4500-CN C
Q3258-02	Q3258-01MS	Water	Cyanide	Cool 4 deg C	DALT01	D31	09/29/2025	SM4500-CN C
Q3258-03	Q3258-01MSD	Water	Cyanide	Cool 4 deg C	DALT01	D31	09/29/2025	SM4500-CN C
Q3258-04	ADDTIONAL-CYANIDE-3	Water	Cyanide	Cool 4 deg C	DALT01	D31	09/30/2025	SM4500-CN C
Q3267-01	Q4	Water	Cyanide	1:1 NaOH to pH >12	METE01	D31	10/01/2025	SM4500-CN C

Date/Time 10/06/2025 10.00
Raw Sample Received by:
Raw Sample Relinquished by:

Date/Time 10/06/2025 11.45
Raw Sample Received by:
Raw Sample Relinquished by:

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Instrument ID: KONELAB

Daily Analysis Runlog For Sequence/QCBatch ID # LB137435

Review By	rubina	Review On	10/7/2025 3:23:29 PM
Supervise By	Iwona	Supervise On	10/7/2025 3:24:02 PM
SubDirectory	LB137435	Test	Cyanide

STD. NAME	STD REF.#
ICAL Standard	WP115057,WP115058,WP115059,WP115060,WP115061,WP115062,WP115063
ICV Standard	W3012
CCV Standard	WP115058
ICSA Standard	N/A
CRI Standard	N/A
LCS Standard	WP113838
Chk Standard	WP112643,WP114324,WP115065

Sr#	SampleId	ClientID	QcType	Date	Comment	Operator	Status
1	0.0PPBCN	0.0PPBCN	CAL1	10/06/25 11:48		rubina	OK
2	5.0PPBCN	5.0PPBCN	CAL2	10/06/25 11:48		rubina	OK
3	10PPBCN	10PPBCN	CAL3	10/06/25 11:48		rubina	OK
4	50PPBCN	50PPBCN	CAL4	10/06/25 11:48		rubina	OK
5	100PPBCN	100PPBCN	CAL5	10/06/25 11:48		rubina	OK
6	250PPBCN	250PPBCN	CAL6	10/06/25 11:48		rubina	OK
7	500PPBCN	500PPBCN	CAL7	10/06/25 11:48		rubina	OK
8	ICV1	ICV1	ICV	10/06/25 14:36		rubina	OK
9	ICB1	ICB1	ICB	10/06/25 14:36		rubina	OK
10	CCV1	CCV1	CCV	10/06/25 14:36		rubina	OK
11	CCB1	CCB1	CCB	10/06/25 14:36		rubina	OK
12	RL	RL	SAM	10/06/25 14:36		rubina	OK
13	PB169962BL	PB169962BL	MB	10/06/25 14:43		rubina	OK
14	PB169962BS	PB169962BS	LCS	10/06/25 14:43		rubina	OK
15	MIDPB169962	MIDPB169962	SAM	10/06/25 14:43		rubina	OK
16	Q3258-01	MONTHLY-CYANIDE	SAM	10/06/25 14:43		rubina	OK
17	Q3258-01DUP	MONTHLY-CYANIDE	DUP	10/06/25 14:43		rubina	OK
18	Q3258-02	MONTHLY-CYANIDE	MS	10/06/25 14:51		rubina	OK

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Instrument ID: KONELAB

Daily Analysis Runlog For Sequence/QCBatch ID # LB137435

Review By	rubina	Review On	10/7/2025 3:23:29 PM
Supervise By	Iwona	Supervise On	10/7/2025 3:24:02 PM
SubDirectory	LB137435	Test	Cyanide

STD. NAME	STD REF.#
ICAL Standard	WP115057,WP115058,WP115059,WP115060,WP115061,WP115062,WP115063
ICV Standard	W3012
CCV Standard	WP115058
ICSA Standard	N/A
CRI Standard	N/A
LCS Standard	WP113838
Chk Standard	WP112643,WP114324,WP115065

19	Q3258-03	MONTHLY-CYANIDE	MSD	10/06/25 14:51		rubina	OK
20	Q3258-04	ADDTIONAL-CYANID	SAM	10/06/25 14:51		rubina	OK
21	Q3267-01	Q4	SAM	10/06/25 14:51		rubina	OK
22	CCV2	CCV2	CCV	10/06/25 14:51		rubina	OK
23	CCB2	CCB2	CCB	10/06/25 14:51		rubina	OK

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Instrument ID: WC PH METER-1

Daily Analysis Runlog For Sequence/QCBatch ID # LB137498

Review By	rubina	Review On	10/14/2025 2:54:59 PM
Supervise By	Iwona	Supervise On	10/14/2025 2:55:06 PM
SubDirectory	LB137498	Test	Field pH

STD. NAME	STD REF.#
ICAL Standard	N/A
ICV Standard	N/A
CCV Standard	N/A
ICSA Standard	N/A
CRI Standard	N/A
LCS Standard	N/A
Chk Standard	W3178,W3217,W3191,W3093,W3093,W3093

Sr#	SampleId	ClientID	QcType	Date	Comment	Operator	Status
1	CAL2	CAL2	CAL	10/01/25 14:50		Ayul	OK
2	CAL1	CAL1	CAL	10/01/25 14:52		Ayul	OK
3	CAL3	CAL3	CAL	10/01/25 14:54		Ayul	OK
4	ICV	ICV	ICV	10/01/25 14:56		Ayul	OK
5	CCV1	CCV1	CCV	10/01/25 15:00		Ayul	OK
6	Q3267-01	Q4	SAM	10/01/25 15:02		Ayul	OK
7	Q3267-01DUP	Q4DUP	DUP	10/01/25 15:07		Ayul	OK
8	CCV2	CCV2	CCV	10/01/25 15:11		Ayul	OK

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

Prep Standard - Chemical Standard Summary

Order ID : Q3267

Test : Cyanide,Field pH

Prepbatch ID : PB169962,

Sequence ID/Qc Batch ID: LB137435,LB137498,

Standard ID :
WP112643,WP112826,WP112827,WP113836,WP113837,WP113838,WP114324,WP115056,WP115057,WP115058,WP115059,WP115060,WP115061,WP115062,WP115063,WP115065,

Chemical ID :
M6041,M6151,W2668,W3012,W3019,W3093,W3112,W3113,W3139,W3152,W3178,W3182,W3191,W3203,W3214,W3215,W3217,W3224,

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Wet Chemistry STANDARD PREPARATION LOG

Recipe ID	NAME	NO.	Prep Date	Expiration Date	Prepared By	ScaleID	PipetteID	Supervised By
539	CN BUFFER	WP112643	04/09/2025	10/09/2025	Niha Farheen Shaik	WETCHEM_SCALE_5 (WCSC-5)	None	Iwona Zarych 04/09/2025

FROM 138.00000gram of W2668 + 862.00000ml of W3112 = Final Quantity: 1000.000 ml

Recipe ID	NAME	NO.	Prep Date	Expiration Date	Prepared By	ScaleID	PipetteID	Supervised By
1714	Sulfuric Acid, 50% (v/v)	WP112826	04/25/2025	10/25/2025	Rubina Mughal	None	None	Iwona Zarych 04/25/2025

FROM 1000.00000ml of M6041 + 1000.00000ml of W3112 = Final Quantity: 2000.000 ml

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Wet Chemistry STANDARD PREPARATION LOG

Recipe ID	NAME	NO.	Prep Date	Expiration Date	Prepared By	ScaleID	PipetteID	Supervised By
3214	Magnesium Chloride For Cyanide 2.5M(51%W/V)	WP112827	04/25/2025	10/25/2025	Rubina Mughal	WETCHEM_SCALE_8 (WCSC-7)	None	Iwona Zarych 04/25/2025

FROM 500.00000ml of W3112 + 510.00000gram of W3152 = Final Quantity: 1000.000 ml

Recipe ID	NAME	NO.	Prep Date	Expiration Date	Prepared By	ScaleID	PipetteID	Supervised By
11	Sodium hydroxide absorbing solution 0.25 N	WP113836	07/08/2025	12/31/2025	Rubina Mughal	WETCHEM_SCALE_8 (WCSC-7)	None	Iwona Zarych 07/08/2025

FROM 21.00000L of W3112 + 210.00000gram of W3113 = Final Quantity: 21.000 L

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Wet Chemistry STANDARD PREPARATION LOG

Recipe ID	NAME	NO.	Prep Date	Expiration Date	Prepared By	ScaleID	PipetteID	Supervised By
3850	Cyanide MS-MSD spiking solution, 5PPM	WP113837	07/08/2025	11/30/2025	Rubina Mughal	None	WETCHEM_PIPETTE_3 (WC)	Iwona Zarych 07/08/2025

FROM 1.00000ml of W3214 + 199.00000ml of WP113836 = Final Quantity: 200.000 ml

Recipe ID	NAME	NO.	Prep Date	Expiration Date	Prepared By	ScaleID	PipetteID	Supervised By
3371	Cyanide LCS Spike Solution, 5PPM	WP113838	07/08/2025	12/24/2025	Rubina Mughal	None	WETCHEM_PIPETTE_3 (WC)	Iwona Zarych 07/08/2025

FROM 1.00000ml of W3224 + 199.00000ml of WP113836 = Final Quantity: 200.000 ml

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Wet Chemistry STANDARD PREPARATION LOG

Recipe ID	NAME	NO.	Prep Date	Expiration Date	Prepared By	ScaleID	PipetteID	Supervised By
607	PYRIDINE-BARBITURIC ACID	WP114324	08/19/2025	02/17/2026	Rubina Mughal	WETCHEM_SCALE_5 (WCSC-5)	Glass Pipette-A	Jignesh Parikh 08/19/2025

FROM 145.00000ml of W3112 + 15.00000gram of W3203 + 15.00000ml of M6151 + 75.00000ml of W3019 = Final Quantity: 250.000 ml

Recipe ID	NAME	NO.	Prep Date	Expiration Date	Prepared By	ScaleID	PipetteID	Supervised By
3456	Cyanide Intermediate Working Std, 5PPM	WP115056	10/06/2025	10/07/2025	Rubina Mughal	None	WETCHEM_PIPETTE_3 (WC)	Iwona Zarych 10/06/2025

FROM 0.25000ml of W3214 + 49.75000ml of WP113836 = Final Quantity: 50.000 ml

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Wet Chemistry STANDARD PREPARATION LOG

Recipe ID	NAME	NO.	Prep Date	Expiration Date	Prepared By	ScaleID	PipetteID	Supervised By
4	Calibation standard 500 ppb	WP115057	10/06/2025	10/07/2025	Rubina Mughal	None	WETCHEM_PIPETTE_3 (WC)	Iwona Zarych 10/06/2025

FROM 45.00000ml of WP113836 + 5.00000ml of WP115056 = Final Quantity: 50.000 ml

Recipe ID	NAME	NO.	Prep Date	Expiration Date	Prepared By	ScaleID	PipetteID	Supervised By
3761	Calibration-CCV CN Standard 250 ppb	WP115058	10/06/2025	10/07/2025	Rubina Mughal	None	WETCHEM_PIPETTE_3 (WC)	Iwona Zarych 10/06/2025

FROM 2.50000ml of WP115056 + 47.50000ml of WP113836 = Final Quantity: 50.000 ml

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Wet Chemistry STANDARD PREPARATION LOG

Recipe ID	NAME	NO.	Prep Date	Expiration Date	Prepared By	ScaleID	PipetteID	Supervised By
6	Calibration Standard 100 ppb	WP115059	10/06/2025	10/07/2025	Rubina Mughal	None	WETCHEM_PIPETTE_3 (WC)	Iwona Zarych 10/06/2025

FROM 1.00000ml of WP115056 + 49.00000ml of WP113836 = Final Quantity: 50.000 ml

Recipe ID	NAME	NO.	Prep Date	Expiration Date	Prepared By	ScaleID	PipetteID	Supervised By
7	Calibration Standard 50 ppb	WP115060	10/06/2025	10/07/2025	Rubina Mughal	None	WETCHEM_PIPETTE_3 (WC)	Iwona Zarych 10/06/2025

FROM 0.50000ml of WP115056 + 49.50000ml of WP113836 = Final Quantity: 50.000 ml

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Wet Chemistry STANDARD PREPARATION LOG

Recipe ID	NAME	NO.	Prep Date	Expiration Date	Prepared By	ScaleID	PipetteID	Supervised By
8	Calibration Standard 10 ppb	WP115061	10/06/2025	10/07/2025	Rubina Mughal	None	WETCHEM_PIPETTE_3 (WC)	Iwona Zarych 10/06/2025

FROM 1.00000ml of WP115057 + 49.00000ml of WP113836 = Final Quantity: 50.000 ml

Recipe ID	NAME	NO.	Prep Date	Expiration Date	Prepared By	ScaleID	PipetteID	Supervised By
9	Calibration Standard 5 ppb	WP115062	10/06/2025	10/07/2025	Rubina Mughal	None	WETCHEM_PIPETTE_3 (WC)	Iwona Zarych 10/06/2025

FROM 0.50000ml of WP115057 + 49.50000ml of WP113836 = Final Quantity: 50.000 ml

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Wet Chemistry STANDARD PREPARATION LOG

Recipe ID	NAME	NO.	Prep Date	Expiration Date	Prepared By	ScaleID	PipetteID	Supervised By
167	0 ppb CN calibration std	WP115063	10/06/2025	10/07/2025	Rubina Mughal	None	None	Iwona Zarych 10/06/2025

FROM 50.00000ml of WP113836 = Final Quantity: 50.000 ml

Recipe ID	NAME	NO.	Prep Date	Expiration Date	Prepared By	ScaleID	PipetteID	Supervised By
1582	Chloramine T solution, 0.014M	WP115065	10/06/2025	10/07/2025	Rubina Mughal	WETCHEM_SCALE_5 (WCSC-5)	Glass Pipette-A	Iwona Zarych 10/06/2025

FROM 0.08000gram of W3139 + 20.00000ml of W3112 = Final Quantity: 20.000 ml

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	23D2462010	03/20/2028	08/16/2024 / mohan	08/16/2024 / mohan	M6041

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9530-33 / Hydrochloric Acid, Instra-Analyzed (cs/6x2.5L)	22G2862015	02/17/2026	02/18/2025 / Sagar	01/15/2025 / Sagar	M6151

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	J3818-5 / SODIUM PHOSPHATE, MONOBAS/HYD, CRYS, ACS, 2.5 KG	0000225799	12/03/2025	04/05/2021 / Alexander	02/10/2020 / apatel	W2668

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
EPA	/ ICV-CN	ICV6-400	12/31/2025	01/08/2025 / Iwona	02/20/2020 / Iwona	W3012

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
SIGMA ALDRICH	270970-1L / Pyridine 1L	SHBQ2113	04/03/2028	04/03/2023 / Iwona	04/03/2023 / Iwona	W3019

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	566002 / BUFFER PH 7.00 GREEN 1PINT PK6	44001f99	12/31/2025	04/03/2024 / jignesh	04/02/2024 / jignesh	W3093

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / Iwona	07/03/2024 / Iwona	W3112

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19510-7 / Sodium Hydroxide Pellets 12 Kg	23B1556310	12/31/2025	07/08/2024 / Iwona	07/08/2024 / Iwona	W3113

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	JTE494-6 / CHLORAMINE-T BAKER 250GM	10239484	09/09/2029	09/09/2024 / Iwona	09/09/2024 / Iwona	W3139

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	01237-10KG / Megnasium Chloride Hexahydrate ACS 10KG	002126-2019-201	11/25/2029	11/25/2024 / Iwona	11/25/2024 / Iwona	W3152

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	AL14055-3 / PH 4 BUFFER SOLUTION	2411A93	10/30/2026	04/01/2025 / JIGNESH	01/27/2025 / jignesh	W3178

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	470112-662 / TEST STRIPES, NITRATE/NITRITE, PK50	436101	04/30/2027	08/05/2025 / Iwona	02/26/2025 / Iwona	W3182

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	1601-1 / PH 10.01 BUFFER,COLOR CD 475ML	2410F80	03/31/2026	04/01/2025 / JIGNESH	03/13/2025 / jignesh	W3191

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	EM-BX0035-3 / Barbituric Acid, 100 gms	WXBF3271V	05/16/2029	04/21/2025 / Iwona	04/21/2025 / Iwona	W3203

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	RC2543-4 / CYANIDE STD 1000PPM 4OZ	1505H73	11/30/2025	05/21/2025 / Iwona	05/21/2025 / Iwona	W3214

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	140444 / TEST PAPERS,PH 0-14,.5 SENSI,100PK	10D3242	12/31/2028	06/09/2025 / Iwona	06/09/2025 / Iwona	W3215

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	AL14455-3 / buffer solution pH 7 yellow	2504D34	03/31/2027	07/02/2025 / jignesh	06/26/2025 / Iwona	W3217

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	LC135457 / Cyanide Standard, 1000 PPM, Second Source	45060288	12/24/2025	07/07/2025 / Iwona	07/07/2025 / Iwona	W3224

Sigma-Aldrich.

W3019
Rec 4/3/23

3050 Spruce Street, Saint Louis, MO 63103, USA
Website: www.sigmaaldrich.com
Email USA: techserv@sial.com
Outside USA: eurtechserv@sial.com

Certificate of Analysis

Product Name:
Pyridine - anhydrous, 99.8%

Product Number:	**270970**
Batch Number:	**SHBQ2113**
Brand:	SIAL
CAS Number:	110-86-1
MDL Number:	MFCD00011732
Formula:	C5H5N
Formula Weight:	79.10 g/mol
Quality Release Date:	15 DEC 2022



Test	Specification	Result
Appearance (Color)	Colorless	Colorless
Appearance (Form)	Liquid	Liquid
Infrared Spectrum	Conforms to Structure	Conforms
Purity (GC)	≥ 99.75 %	99.99 %
Water (by Karl Fischer)	≤ 0.003 %	0.002 %
Residue on Evaporation	≤ 0.0005 %	< 0.0001 %

Larry Coers, Director
Quality Control
Sheboygan Falls, WI US

W3011
W3012
W3013
W3014
W3015

For ICP-MS use: dilute the ICV1 concentrate 50-fold with 1% (v/v) nitric acid; pipet 2 mL of the concentrate into a 100 mL volumetric flask and dilute to volume with 1% (v/v) nitric acid.

ICV5-0415 For the cold vapor analysis of mercury by AA: dilute the ICV5 concentrate 100-fold with 2% (v/v) nitric acid; pipet 1 mL of the concentrate into a 100 mL volumetric flask and dilute to volume with 2% (v/v) nitric acid. The ICV5 concentrate is prepared in 0.05% (w/v) $K_2Cr_2O_7$ and 5% (v/v) nitric acid.

ICV6-0400 For the analysis of cyanide: dilute the ICV6 concentrate 100-fold with Type II water; pipet 1 mL of the concentrate into a 100 mL volumetric flask and dilute to volume with Type II water. Distill this solution along with the samples before analysis. The cyanide concentrate is prepared from $K_3Fe(CN)_6$, Type II water, and 0.1 % sodium hydroxide, and will decompose rapidly if exposed to light.

NOTE: USE TYPE II WATER AND HIGH-PURITY ACIDS FOR ALL DILUTIONS.

(D) *CERTIFIED CONCENTRATIONS OF QATS ICV1, ICV5, AND ICV6 SOLUTIONS*

ICV1-1014		
Element	**Concentration (µg/L) (after 10-fold dilution)**	**Concentration (µg/L) (after 50-fold dilution)**
Al	2520	504
Sb	1010	202
As	997	199
Ba	518	104
Be	514	103
Cd	514	103
Ca	10000	2000
Cr	517	103
Co	521	104
Cu	505	101
Fe	10100	2020
Pb	1030	206
Mg	5990	1198
Mn	524	105
Ni	525	105
K	9940	1988
Se	1030	206
Ag	252	50
Na	10100	2020
Tl	1040	208
V	504	101
Zn	1010	202

ICV5-0415		ICV6-0400	
Element	**Concentration (µg/L) (after 100-fold dilution)**	**Analyte**	**Concentration (µg/L) (after 100-fold dilution)**
Hg	4.0	**CN^-**	99

Sulfuric Acid
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis
Low Selenium

M 6041-46
MS

avantor™ | J.T.Baker®

Material No.: 9673-33
Batch No.: 23D2462010
Manufactured Date: 2023-03-22
Retest Date: 2028-03-20
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
ACS – Assay (H_2SO_4)	95.0 – 98.0 %	96.1 %
Appearance	Passes Test	Passes Test
ACS – Color (APHA)	≤ 10	5
ACS – Residue after Ignition	≤ 3 ppm	< 1 ppm
ACS – Substances Reducing Permanganate (as SO2)	≤ 2 ppm	< 2 ppm
Ammonium (NH_4)	≤ 1 ppm	1 ppm
Chloride (Cl)	≤ 0.1 ppm	< 0.1 ppm
Nitrate (NO_3)	≤ 0.2 ppm	< 0.1 ppm
Phosphate (PO_4)	≤ 0.5 ppm	< 0.1 ppm
Trace Impurities – Aluminum (Al)	≤ 30.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 4.0 ppb	< 2.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	8.5 ppb
Trace Impurities – Cadmium (Cd)	≤ 2.0 ppb	< 0.3 ppb
Trace Impurities – Chromium (Cr)	≤ 6.0 ppb	< 0.4 ppb
Trace Impurities – Cobalt (Co)	≤ 0.5 ppb	< 0.3 ppb
Trace Impurities – Copper (Cu)	≤ 1.0 ppb	< 0.1 ppb
Trace Impurities – Gold (Au)	≤ 10.0 ppb	0.5 ppb
Heavy Metals (as Pb)	≤ 500.0 ppb	< 100.0 ppb
Trace Impurities – Iron (Fe)	≤ 50.0 ppb	1.3 ppb
Trace Impurities – Lead (Pb)	≤ 0.5 ppb	< 0.5 ppb
Trace Impurities – Magnesium (Mg)	≤ 7.0 ppb	0.8 ppb
Trace Impurities – Manganese (Mn)	≤ 1.0 ppb	< 0.4 ppb
Trace Impurities – Mercury (Hg)	≤ 0.5 ppb	< 0.1 ppb
Trace Impurities – Nickel (Ni)	≤ 2.0 ppb	0.3 ppb
Trace Impurities – Potassium (K)	≤ 500.0 ppb	< 2.0 ppb
Trace Impurities – Selenium (Se)	≤ 50.0 ppb	< 0.1 ppb
Trace Impurities – Silicon (Si)	≤ 100.0 ppb	31.5 ppb
Trace Impurities – Silver (Ag)	≤ 1.0 ppb	< 0.3 ppb

>>> Continued on page 2 >>>

Sulfuric Acid
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis
Low Selenium

avantor™ | J.T.Baker®

Material No.: 9673-33
Batch No.: 23D2462010

Test	Specification	Result
Trace Impurities - Sodium (Na)	≤ 500.0 ppb	5.4 ppb
Trace Impurities - Strontium (Sr)	≤ 5.0 ppb	< 0.2 ppb
Trace Impurities - Tin (Sn)	≤ 5.0 ppb	< 0.8 ppb
Trace Impurities - Zinc (Zn)	≤ 5.0 ppb	0.4 ppb

For Laboratory,Research,or Manufacturing Use

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

James T Ethier

Jamie Ethier
Vice President Global Quality

Hydrochloric Acid, 36.5–38.0%
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis

avantor™ | J.T.Baker®

M6151

R→ 1/15/25

Material No.: 9530-33
Batch No.: 22G2862015
Manufactured Date: 2022-06-15
Retest Date: 2027-06-14
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
ACS – Assay (as HCl) (by acid-base titrn)	36.5 – 38.0 %	37.9 %
ACS – Color (APHA)	≤ 10	5
ACS – Residue after Ignition	≤ 3 ppm	< 1 ppm
ACS – Specific Gravity at 60°/60°F	1.185 – 1.192	1.191
ACS – Bromide (Br)	≤ 0.005 %	< 0.005 %
ACS – Extractable Organic Substances	≤ 5 ppm	< 1 ppm
ACS – Free Chlorine (as Cl_2)	≤ 0.5 ppm	< 0.5 ppm
Phosphate (PO_4)	≤ 0.05 ppm	< 0.03 ppm
Sulfate (SO_4)	≤ 0.5 ppm	< 0.3 ppm
Sulfite (SO_3)	≤ 0.8 ppm	0.3 ppm
Ammonium (NH_4)	≤ 3 ppm	< 1 ppm
Trace Impurities – Arsenic (As)	≤ 0.010 ppm	< 0.003 ppm
Trace Impurities – Aluminum (Al)	≤ 10.0 ppb	1.3 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 3.0 ppb
Trace Impurities – Barium (Ba)	≤ 1.0 ppb	0.2 ppb
Trace Impurities – Beryllium (Be)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities – Bismuth (Bi)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Boron (B)	≤ 20.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 1.0 ppb	< 0.3 ppb
Trace Impurities – Calcium (Ca)	≤ 50.0 ppb	163.0 ppb
Trace Impurities – Chromium (Cr)	≤ 1.0 ppb	0.7 ppb
Trace Impurities – Cobalt (Co)	≤ 1.0 ppb	< 0.3 ppb
Trace Impurities – Copper (Cu)	≤ 1.0 ppb	< 0.1 ppb
Trace Impurities – Gallium (Ga)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities – Germanium (Ge)	≤ 3.0 ppb	< 2.0 ppb
Trace Impurities – Gold (Au)	≤ 4.0 ppb	0.6 ppb
Heavy Metals (as Pb)	≤ 100 ppb	< 50 ppb
Trace Impurities – Iron (Fe)	≤ 15 ppb	6 ppb

>>> Continued on page 2 >>>

Hydrochloric Acid, 36.5-38.0%
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis

avantor™ | J.T.Baker®

Material No.: 9530-33
Batch No.: 22G2862015

Test	Specification	Result
Trace Impurities - Lead (Pb)	≤ 1.0 ppb	< 0.5 ppb
Trace Impurities - Lithium (Li)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities - Magnesium (Mg)	≤ 10.0 ppb	2.9 ppb
Trace Impurities - Manganese (Mn)	≤ 1.0 ppb	< 0.4 ppb
Trace Impurities - Mercury (Hg)	≤ 0.5 ppb	0.1 ppb
Trace Impurities - Molybdenum (Mo)	≤ 10.0 ppb	< 3.0 ppb
Trace Impurities - Nickel (Ni)	≤ 4.0 ppb	< 0.3 ppb
Trace Impurities - Niobium (Nb)	≤ 1.0 ppb	0.8 ppb
Trace Impurities - Potassium (K)	≤ 9.0 ppb	< 2.0 ppb
Trace Impurities - Selenium (Se), For Information Only		< 1.0 ppb
Trace Impurities - Silicon (Si)	≤ 100.0 ppb	< 10.0 ppb
Trace Impurities - Silver (Ag)	≤ 1.0 ppb	0.5 ppb
Trace Impurities - Sodium (Na)	≤ 100.0 ppb	2.3 ppb
Trace Impurities - Strontium (Sr)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities - Tantalum (Ta)	≤ 1.0 ppb	1.6 ppb
Trace Impurities - Thallium (Tl)	≤ 5.0 ppb	< 2.0 ppb
Trace Impurities - Tin (Sn)	≤ 5.0 ppb	4.0 ppb
Trace Impurities - Titanium (Ti)	≤ 1.0 ppb	1.5 ppb
Trace Impurities - Vanadium (V)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities - Zinc (Zn)	≤ 5.0 ppb	0.8 ppb
Trace Impurities - Zirconium (Zr)	≤ 1.0 ppb	0.3 ppb

>>> Continued on page 3 >>>

Hydrochloric Acid, 36.5-38.0%
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis

avantor™ | J.T.Baker®

Material No.: 9530-33
Batch No.: 22G2862015

Test	Specification	Result

For Laboratory,Research,or Manufacturing Use
Product Information (not specifications):
Appearance (clear, fuming liquid)
Meets ACS Specifications
Storage Condition: Store below 25 °C.

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

James T Ethier

Jamie Ethier
Vice President Global Quality

Sodium Phosphate, Monobasic, Monohydrate,
Crystal
BAKER ANALYZED® A.C.S. Reagent

(sodium dihydrogen phosphate, monohydrate)

Material No.: 3818-05
Batch No.: 0000225799
Manufactured Date: 2018/12/05
Retest Date: 2025/12/03
Revision No: 1

Certificate of Analysis

Meets ACS Reagent Chemical Requirements,

Test	Specification	Result
Assay ($NaH_2PO_4 \cdot H_2O$)	98.0 - 102.0 %	99.5
pH of 5% Solution at 25°C	4.1 - 4.5	4.3
Insoluble Matter	<= 0.01 %	< 0.01
Chloride (Cl)	<= 5 ppm	< 5
ACS - Sulfate (SO_4)	<= 0.003 %	< 0.003
Calcium (Ca)	<= 0.005 %	<0.005
Potassium (K)	<= 0.01 %	< 0.01
Heavy Metals (as Pb)	<= 0.001 %	< 0.001
Trace Impurities - Iron (Fe)	<= 0.001 %	< 0.001

For Laboratory, Research or Manufacturing Use
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: IN
Packaging Site: Paris Mfg Ctr & DC

Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

RICCA CHEMICAL COMPANY®

1490 Lammers Pike
Batesville, IN 47006
http://www.riccachemical.com
1-888-GO-RICCA
customerservice@riccachemical.com

W3093 0941 04/03/2024 LG

Certificate of Analysis

Buffer, Reference Standard, pH 7.00 ± 0.01 at 25°C (Color Coded Yellow)

Lot Number: 4401F99 **Product Number:** 1551

Manufacture Date: JAN 08, 2024
Expiration Date: DEC 2025

The certified value for this product is confirmed in independent testing by a second qualified chemist.
The NIST traceable pH value is certified to ±0.01 at 25 °C only. All other pH values at their corresponding temperatures are accurate to ± 0.05.

°C	0	5	10	15	20	25	30	35	40	45	50
pH	7.12	7.09	7.06	7.04	7.02	7.00	6.99	6.98	6.98	6.97	6.97

Name	CAS#	Grade
Water	7732-18-5	ACS/ASTM/USP/EP
Sodium Phosphate Dibasic	7558-79-4	ACS
Potassium Dihydrogen Phosphate	7778-77-0	ACS
Preservative	Proprietary	
Yellow Dye	Proprietary	
Sodium Hydroxide	1310-73-2	

Test	Specification	Result	
Appearance	Yellow liquid	Passed	*Not a certified value.

Test	Certified Value	Uncertainty	NIST SRM#
pH at 25°C (Method: SQCP027, SQCP033)	7.004	0.02	186-I-g, 186-II-g, 191d

Specification	Reference
Commercial Buffer Solutions	ASTM (D 1293 B)
Buffer A	ASTM (D 5464)
Buffer A	ASTM (D 5128)

pH measurements were performed in our Batesville, IN laboratory under ISO/IEC 17025 accreditation (ANAB Certificate L2387.02) and are certified traceable to National Institute of Standards and Technology (NIST) Standard Reference Material as indicated above via an unbroken chain of comparisons. The uncertainty is calculated from the uncertainty of the measurement variation from sample to sample, the uncertainty in the NIST Standard Reference Material, and the uncertainty of the measurement process. The uncertainty is multiplied by k=2, corresponding to 95% coverage in a normal distribution. Volumetric glassware complies with Class A tolerance requirements of ASTM E 288 and NIST Circular 434; it is calibrated before first use and recalibrated regularly in accordance with ASTM E 542 and NIST Procedure NBSIR 74-461. Balances are calibrated regularly with weights certified traceable to the NIST national mass standard. Thermometers and temperature probes are calibrated before first use and recalibrated regularly with a thermometer traceable to NIST standards. All products are prepared according to master documents that assure manufacture according to validated methods. Batch records document raw material traceability and production and testing history for each lot manufactured.

Part Number	Size / Package Type	Shelf Life (Unopened Container)
1551-1	4 L natural poly	24 months
1551-1CT	4 L Cubitainer®	24 months
1551-2.5	10 L Cubitainer®	24 months
1551-5	20 L Cubitainer®	24 months

Recommended Storage: 15°C - 30°C (59°F - 86°F)

Paul Brandon (01/08/2024)
Production Manager
This document is designed to comply with ISO Guide 31 "Reference Materials -- Contents of Certificates and Labels."

This product was tested in an ISO 17025 Accredited Laboratory

Certificate of Analysis

Sodium Hydroxide (Pellets)

Material: 0583

Grade: ACS GRADE

Batch Number: 23B1556310

Chemical Formula: NaOH
Molecular Weight: 40
CAS #: 1310-73-2
Appearance:

Pellets

Manufacture Date: 12/14/2022
Expiration Date: 12/31/2025

Storage: Room Temperature

TEST	SPECIFICATION	ANALYSIS	DISPOSITION
Calcium	<= 0.005 %	<0.005 %	PASS
Chloride	<= 0.005 %	0.002 %	PASS
Heavy Metals	<= 0.002 %	<0.002 %	PASS
Iron	<= 0.001 %	<0.001 %	PASS
Magnesium	<= 0.002 %	<0.002 %	PASS
Mercury	<= 0.1 ppm	<0.1 ppm	PASS
Nickel	<= 0.001 %	<0.001 %	PASS
Nitrogen Compounds	<= 0.001 %	<0.001 %	PASS
Phosphate	<= 0.001 %	<0.001 %	PASS
Potassium	<= 0.02 %	<0.02 %	PASS
Purity	>= 97.0 %	99.2 %	PASS
Sodium Carbonate	<= 1.0 %	0.5 %	PASS
Sulfate	<= 0.003 %	<0.003 %	PASS

Internal ID #: 710

Signature

We certify that this batch conforms to the specifications listed.

This document has been electronically produced and is valid without a signature.

Leona Edwardson, Quality Control Sr. Manager - Solon
VWR Chemicals, LLC.
28600 Fountain Parkway, Solon OH 44139 USA

Additional Information

Analysis may have been rounded to significant digits in specification limits.

Product meets analytical specifications of the grades listed.

Certificate of Analysis

Sodium Hydroxide (Pellets)

Material: **0583**

Grade: **ACS GRADE**

Batch Number: **23B1556310**

Chemical Formula:	NaOH	Manufacture Date:	12/14/2022
Molecular Weight:	40	Expiration Date:	12/31/2025
CAS #:	1310-73-2		
Appearance:		Storage:	Room Temperature

Pellets

Spec Set: 0583ACS

Internal ID #: 710

Signature

We certify that this batch conforms to the specifications listed.

This document has been electronically produced and is valid without a signature.

Leona Edwardson, Quality Control Sr. Manager - Solon
VWR Chemicals, LLC.
28600 Fountain Parkway, Solon OH 44139 USA

Additional Information

Analysis may have been rounded to significant digits in specification limits.

Product meets analytical specifications of the grades listed.

ThermoFisher SCIENTIFIC

Certificate of Analysis

W3139 Received on 9/9/24 by IZ

Product No.:	A12044
Product:	Chloramine-T trihydrate, 98%
Lot No.:	10239484

Appearance:	White powder
Melting Point:	166°C(dec)
Assay (Iodometric titration):	100.5%
Identification (FTIR):	Conforms

W3152 Received on 11/25/24 by IZ

Chem-Impex International, Inc.

Tel: (630) 766-2112
Fax: (630) 766-2218
E-mail: sales@chemimpex.com
Web site: www.chemimpex.com
Shipping and Correspondence:
935 Dillon Drive
Wood Dale, IL 60191
Manufacturing site:
825 Dillon Drive
Wood Dale, IL 60191

Certificate of Analysis

Catalogue Number	01237
Lot Number	002126-2019-201
Product	**Magnesium chloride hexahydrate**
	Magnesium chloride•$6H_2O$
CAS Number	7791-18-6
Molecular Formula	$MgCl_2$•$6H_2O$
Molecular Weight	203.3

Appearance	White crystals
Solubility	167 g in 100 mL water
Melting Point	~ 115 °C
Heavy Metals	4.393 ppm
Anion	Nitrate (NO_3) : < 0.001% Phosphate (PO_4) : < 5 ppm Sulfate (SO_4) : < 0.002%
Cation	Ammonium (NH_4) : < 0.002% Barium (Ba) : 0.005% Calcium (Ca) : 0.01% Iron (Fe) : 4.5 ppm Manganese (Mn) : 0.624 ppm Potassium (K) : 0.004% Sodium (Na) : 0.000003% Strontium (Sr) : 0.005%
Insoluble material	0.0021%
Assay by titration	100.83%
Grade	ACS reagent
Storage	Store at RT

Certificate of Analysis

Catalog Number: 01237 **Lot Number: 002126-2019-201**

Remarks	See material safety data sheet for additional information
	For laboratory use only

The foregoing is a copy of the Certificate of Analysis as provided by our supplier

Bala Kumar
Quality Control Manager

RICCA CHEMICAL COMPANY®

1841 Broad Street
Pocomoke City, MD 21851
http://www.riccachemical.com
1-888-GO-RICCA
customerservice@riccachemical.com

Certificate of Analysis

W3178 58

Buffer, Reference Standard, pH 4.00 ± 0.01 at 25°C (Color Coded Red)

Lot Number: 2411A93 **Product Number:** 1501 **Manufacture Date:** NOV 04, 2024
Expiration Date: OCT 2026

The certified value for this product is confirmed in independent testing by a second qualified chemist.
The NIST Traceable pH value is certified to ±0.01 at 25 °C only. All other pH values at their corresponding temperatures are accurate to ± 0.05.

°C	0	5	10	15	20	25	30	35	40	45	50
pH	4.00	4.00	4.00	4.00	4.00	4.00	4.01	4.02	4.03	4.04	4.06

Name	CAS#	Grade
Water	7732-18-5	ACS/ASTM/USP/EP
Potassium Acid Phthalate	877-24-7	Buffer
Preservative	Proprietary	Commercial
Red Dye	Proprietary	Purified

Test	Specification	Result	
Appearance	Red liquid	Passed	*Not a certified value.

Test	Certified Value	Uncertainty	NIST SRM#
pH at 25°C (Method: SQCP027, SQCP033)	4.008	0.02	185i, 186-I-g, 186-II-g

Specification	Reference
Commercial Buffer Solutions	ASTM (D 1293 B)
Buffer B	ASTM (D 5464)
Buffer B	ASTM (D 5128)

pH measurements were performed in our Pocomoke City, MD laboratory under ISO/IEC 17025 accreditation (ANAB Certificate L2387.01) and are certified traceable to National Institute of Standards and Technology (NIST) Standard Reference Material as indicated above via an unbroken chain of comparisons. The uncertainty is calculated from the uncertainty of the measurement variation from sample to sample, the uncertainty in the NIST Standard Reference Material, and the uncertainty of the measurement process. The uncertainty is multiplied by k=2, corresponding to 95% coverage in a normal distribution. Volumetric glassware complies with Class A tolerance requirements of ASTM E 288 and NIST Circular 434; it is calibrated before first use and recalibrated regularly in accordance with ASTM E 542 and NIST Procedure NBSIR 74-461. Balances are calibrated regularly with weights certified traceable to the NIST national mass standard. Thermometers and temperature probes are calibrated before first use and recalibrated regularly with a thermometer traceable to NIST standards. All products are prepared according to master documents that assure manufacture according to validated methods. Batch records document raw material traceability and production and testing history for each lot manufactured.

Part Number	Size / Package Type	Shelf Life (Unopened Container)
1501-16	500 mL natural poly	24 months
1501-2.5	10 L Cubitainer®	24 months
1501-5	20 L Cubitainer®	24 months

Recommended Storage: 15°C - 30°C (59°F - 86°F)

RICCA CHEMICAL COMPANY®
1841 Broad Street
Pocomoke City, MD 21851
http://www.riccachemical.com
1-888-GO-RICCA
customerservice@riccachemical.com

W3191 W3191 Receive Date: 03/18/25 JP

Certificate of Analysis

Buffer, Reference Standard, pH 10.00 ± 0.01 at 25°C (Color Coded Blue)

Lot Number: 2410F80 **Product Number:** 1601 **Manufacture Date:** OCT 09, 2024

Expiration Date: MAR 2026

The certified value for this product is confirmed in independent testing by a second qualified chemist.
The NIST traceable pH value is certified to ±0.01 at 25 °C only. All other pH values at their corresponding temperatures are accurate to ± 0.05.

°C	0	5	10	15	20	25	30	35	40	50
pH	10.31	10.23	10.17	10.11	10.05	10.00	9.95	9.91	9.87	9.81

Name	CAS#	Grade
Water	7732-18-5	ACS/ASTM/USP/EP
Sodium Carbonate	497-19-8	ACS
Sodium Bicarbonate	144-55-8	ACS
Sodium Hydroxide	1310-73-2	Reagent
Preservative	Proprietary	
Blue Dye	Proprietary	

Test	Specification	Result	
Appearance	Blue liquid	Passed	*Not a certified value.

Test	Certified Value	Uncertainty	NIST SRM#
pH at 25°C (Method: SQCP027, SQCP033)	10.009	0.02	186-I-g, 186-II-g, 191d

Specification	Reference
Commercial Buffer Solutions	
Buffer C	ASTM (D 1293 B)
Buffer C	ASTM (D 5464)
	ASTM (D 5128)

pH measurements were performed in our Pocomoke City, MD laboratory under ISO/IEC 17025 accreditation (ANAB Certificate L2387.01) and are certified traceable to National Institute of Standards and Technology (NIST) Standard Reference Material as indicated above via an unbroken chain of comparisons. The uncertainty is calculated from the uncertainty of the measurement variation from sample to sample, the uncertainty in the NIST Standard Reference Material, and the uncertainty of the measurement process. The uncertainty is multiplied by k=2, corresponding to 95% coverage in a normal distribution. Volumetric glassware complies with Class A tolerance requirements of ASTM E 288 and NIST Circular 434; it is calibrated before first use and recalibrated regularly in accordance with ASTM E 542 and NIST Procedure NBSIR 74-461. Balances are calibrated regularly with weights certified traceable to the NIST national mass standard. Thermometers and temperature probes are calibrated before first use and recalibrated regularly with a thermometer traceable to NIST standards. All products are prepared according to master documents that assure manufacture according to validated methods. Batch records document raw material traceability and production and testing history for each lot manufactured.

Part Number	Size / Package Type	Shelf Life (Unopened Container)
1601-1	4 L natural poly	18 months
1601-16	500 mL natural poly	18 months
1601-1CT	4 L Cubitainer®	18 months
1601-2.5	10 L Cubitainer®	18 months
1601-32	1 L natural poly	18 months
1601-5	20 L Cubitainer®	18 months

3050 Spruce Street, Saint Louis, MO 63103, USA
Website: www.sigmaaldrich.com
Email USA: techserv@sial.com
Outside USA: eurtechserv@sial.com

Certificate of Analysis

Product Name:
Barbituric acid - ReagentPlus® , 99%

Product Number:	**185698**
Batch Number:	**WXBF3271V**
Brand:	SIAL
CAS Number:	67-52-7
Formula:	C4H4N2O3
Formula Weight:	128,09 g/mol
Quality Release Date:	16 MAY 2024



Test	Specification	Result
Appearance (Colour)	White to Off-White	White
Appearance (Form)	Powder	Powder
Infrared spectrum	Conforms to Structure	Conforms
Purity (Titration by NaOH)	98.5 - 101.5 %	100.4 %
GC (area %) VPCT	≥ 98 %	100 %

Kang Chen
Quality Manager
Wuxi , China CN

RICCA CHEMICAL COMPANY®

W3214 Received on 5/21/25 by IZ

448 West Fork Dr
Arlington, TX 76012
http://www.riccachemical.com
1-888-GO-RICCA
customerservice@riccachemical.com

Certificate of Analysis

Cyanide Standard, 1000 ppm CN^-

Lot Number: 1505H73 **Product Number:** 2543

Manufacture Date: MAY 08, 2025
Expiration Date: NOV 2025

This standard is prepared using accurate volumetric techniques from material that has been assayed against Silver Nitrate solution certifiec traceable to NIST Standard Reference Material 999. The certified value reported is the prepared value based upon the method of preparation of the material. The uncertainty in the prepared value is the combined uncertainty based on the stability of the assayed Potassium Cyanide, and the uncertainty in the mass and volume measurements.
Use 0.16% (w/v) (0.04 N) Sodium Hydroxide or 0.225 % (w/v) (0.04 N) Potassium Hydroxide to make dilutions of this standard. Restandardize weekly if extreme accuracy is required.

Name	CAS#	Grade
Water	7732-18-5	ACS/ASTM/USP/EP
Potassium Cyanide	151-50-8	ACS
Sodium Hydroxide	1310-73-2	Reagent (from ACS)

Test	Specification	Result
Appearance	Colorless liquid	Passed
Cyanide (CN^-)	995-1005 ppm	1000 ppm

Specification	Reference
Stock Standard Cyanide Solution	APHA (4500-CN- F)
Stock Cyanide Solution	APHA (4500-CN- E)
Stock Cyanide Solution	APHA (4500-CN- K)
Stock Cyanide Solution	APHA (4500-CN- H)
Cyanide Reference Solution (1000 mg/L)	EPA (SW-846) (7.3.3.2)
Cyanide Calibration Stock Solution (1,000 mg/L CN-)	EPA (SW-846) (9213)
Stock Cyanide Solution	EPA (335.3)
Stock Cyanide Solution	EPA (335.2)
Cyanide Solution Stock	ASTM (D 4282)
Simple Cyanide Solution, Stock (1.0 g/L CN)	ASTM (D 4374)

Volumetric glassware complies with Class A tolerance requirements of ASTM E 288 and NIST Circular 434; it is calibrated before first use and recalibrated regularly in accordance with ASTM E 542 and NIST Procedure NBSIR 74-461. Balances are calibrated regularly with weights certified traceable to the NIST national mass standard. Thermometers and temperature probes are calibrated before first use and recalibrated regularly with a thermometer traceable to NIST standards. All products are prepared according to master documents that assure manufacture according to validated methods. Batch records document raw material traceability and production and testing history for each lot manufactured.

Part Number	Size / Package Type	Shelf Life (Unopened Container)
2543-16	500 mL amber poly	6 months
2543-32	1 L amber poly	6 months
2543-4	120 mL amber poly	6 months

Recommended Storage: 2°C - 8°C (36°F - 46°F)

Ernest Mahan (05/08/2025)
Plant Manager

RICCA CHEMICAL COMPANY®

1841 Broad Street
Pocomoke City, MD 21851
http://www.riccachemical.com
1-888-GO-RICCA
customerservice@riccachemical.com

Certificate of Analysis

Buffer, Reference Standard, pH 7.00 ± 0.01 at 25°C (Color Coded Yellow)

Lot Number: 2504D34 **Product Number:** 1551

Manufacture Date: APR 03, 2025
Expiration Date: MAR 2027

The certified value for this product is confirmed in independent testing by a second qualified chemist.
The NIST traceable pH value is certified to ±0.01 at 25 °C only. All other pH values at their corresponding temperatures are accurate to ± 0.05.

°C	0	5	10	15	20	25	30	35	40	45	50
pH	7.12	7.09	7.06	7.04	7.02	7.00	6.99	6.98	6.98	6.97	6.97

Name	CAS#	Grade
Water	7732-18-5	ACS/ASTM/USP/EP
Sodium Phosphate Dibasic	7558-79-4	ACS
Potassium Dihydrogen Phosphate	7778-77-0	ACS
Preservative	Proprietary	
Yellow Dye	Proprietary	
Sodium Hydroxide	1310-73-2	Reagent (from ACS)

Test	Specification	Result	
Appearance	Yellow liquid	Passed	*Not a certified value.

Test	Certified Value	Uncertainty	NIST SRM#
pH at 25°C (Method: SQCP027, SQCP033)	7.003	0.02	186-I-g, 186-II-g, 191d

Specification	Reference
Commercial Buffer Solutions	ASTM (D 1293 B)
Buffer A	ASTM (D 5464)
Buffer A	ASTM (D 5128)

pH measurements were performed in our Pocomoke City, MD laboratory under ISO/IEC 17025 accreditation (ANAB Certificate L2387.01) and are certified traceable to National Institute of Standards and Technology (NIST) Standard Reference Material as indicated above via an unbroken chain of comparisons. The uncertainty is calculated from the uncertainty of the measurement variation from sample to sample, the uncertainty in the NIST Standard Reference Material, and the uncertainty of the measurement process. The uncertainty is multiplied by k=2, corresponding to 95% coverage in a normal distribution. Volumetric glassware complies with Class A tolerance requirements of ASTM E 288 and NIST Circular 434; it is calibrated before first use and recalibrated regularly in accordance with ASTM E 542 and NIST Procedure NBSIR 74-461. Balances are calibrated regularly with weights certified traceable to the NIST national mass standard. Thermometers and temperature probes are calibrated before first use and recalibrated regularly with a thermometer traceable to NIST standards. All products are prepared according to master documents that assure manufacture according to validated methods. Batch records document raw material traceability and production and testing history for each lot manufactured.

Part Number	Size / Package Type	Shelf Life (Unopened Container)
1551-2.5	10 L Cubitainer®	24 months
1551-20	20 x 20 mL pack	24 months
1551-32	1 L natural poly	24 months
1551-5	20 L Cubitainer®	24 months

Recommended Storage: 15°C - 30°C (59°F - 86°F)

Jose Pena (04/03/2025)
Operations Manager

This product was tested in an ISO 17025 Accredited Laboratory

LabChem
Part of TCP Analytical Group
Jackson's Pointe Commerce Park- Building 1000
1010 Jackson's Pointe Court, Zelienople, PA 16063

Certificate of Analysis

Cyanide Standard 1000 ppm (1ml = 1mg CN)

Product Code: **LC13545**

Manufacture Date: June 25, 2025

Lot Number: **45060288**

Expiration Date: December 24, 2025

Test	Specification	Result
Appearance (clarity)	clear solution	clear solution
Appearance (color)	colorless	colorless
Concentration (CN)	0.990 - 1.010mg/mL	1.000mg/mL
Concentration (CN)	990 - 1,010ppm	1,000ppm
Traceable to NIST SRM	Report	999b

Intended Use *- Product is intended for use in manufacturing procedures and laboratory procedures and protocols.*

Storage Information *- Unless noted on the product label, store the product under normal lab conditions in its tightly closed, original container. Do not pipet directly from the container or return unused portions to the container.*

Instructions for Handling and Use - *Please refer to the associated product label and Safety Data Sheet (SDS) for information regarding safety and handling of this product.*

Preparation - *All products are manufactured and tested according to established, documented procedures and methodology. Production documentation records manufacturing data, raw material traceability and testing history on a per lot basis. Balances, thermometers, and glassware are calibrated before first use and on a regular schedule with references traceable to NIST*

The suffix of the product code may differ from what is on your product label. The suffix will designate the size and be associated with a numeric digit(s). Visit LabChem.com for more information

Suffix	1	2	3/3S/36/36S	4/4C	5	6	7	8	9	20	44	200	246	486
Size	500mL or g	1L or 1kg	2.5L/2.5L Coated/6x2.5L/6x2.5L Coated	4L	20L	10L	125mL	25g	100g	20x20mL	4x4L	200L	24x6mL	48x6mL

Michael Monteleone

Michael Monteleone
Chemistry Supervisor - Quality Control
2025070315:30:45ahoffman-0-0

ISO9001:2015 Registration #0306-01

SHIPPING DOCUMENTS

Alliance TECHNICAL GROUP

284 Sheffield Street, Mountainside, NJ 07092
(908) 789-8900 · Fax (908) 789-8922
www.chemtech.net

ALLIANCE PROJECT NO.
QUOTE NO. Q32267
COC Number 2045153

CLIENT INFORMATION

REPORT TO BE SENT TO:
COMPANY: Metcm A GE Power Business
ADDRESS: 700 Parsippany Road
CITY: Parsippany STATE: NJ ZIP: 07054
ATTENTION: Sundas Perez
PHONE: FAX:

CLIENT PROJECT INFORMATION

PROJECT NAME: Parsippany Wastewater Quarterly 2025
PROJECT NO.: LOCATION:
PROJECT MANAGER:
e-mail:
PHONE: FAX:

CLIENT BILLING INFORMATION

BILL TO: PO#:
ADDRESS:
CITY STATE: ZIP:
ATTENTION: PHONE:

DATA TURNAROUND INFORMATION

FAX (RUSH) _____ DAYS*
HARDCOPY (DATA PACKAGE): _____ DAYS*
EDD: _____ DAYS*
*TO BE APPROVED BY CHEMTECH
STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS

DATA DELIVERABLE INFORMATION

- ☐ Level 1 (Results Only)
- ☐ Level 2 (Results + QC)
- ☐ Level 3 (Results + QC + Raw Data)
- ☐ EDD FORMAT _____
- ☐ Level 4 (QC + Full Raw Data)
- ☐ NJ Reduced ☐ US EPA CLP
- ☐ NYS ASP A ☐ NYS ASP B
- ☐ Other _____

ANALYSIS

1: Metals 6 trap 2: Cyanide 3: Field pH 4 5 6 7 8 9

ALLIANCE SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE COMP	SAMPLE TYPE GRAB	SAMPLE COLLECTION DATE	SAMPLE COLLECTION TIME	# OF BOTTLES	PRESERVATIVES 1 (B)	2 (D)	3 (E)	4	5	6	7	8	9	COMMENTS
1.	Q4	W	✓		10-1-25	1500	4	✓	✓	✓							PH 7.64
2.																	
3.																	
4.																	
5.																	
6.																	
7.																	
8.																	
9.																	
10.																	

← Specify Preservatives
A-HCl D-NaOH
B-HN03 E-ICE
C-H2SO4 F-OTHER

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER:	DATE/TIME:	RECEIVED BY:	DATE/TIME:
1.	10.1.25 1515	1.	10-1-25 1515
2.		2.	
3.	10-1-25 1615	3.	

Conditions of bottles or coolers at receipt: ☐ COMPLIANT ☐ NON COMPLIANT ☐ COOLER TEMP 3.7 °C
Comments:

Page _____ of

CLIENT: ☐ Hand Delivered ☐ Other

Shipment Complete ☐ YES ☐ NO

WHITE - ALLIANCE COPY FOR RETURN TO CLIENT YELLOW - ALLIANCE COPY PINK - SAMPLER COPY

Alliance Technical Group, LLC-Newark
284 Sheffield Street, Mountainside, NJ 07092 Tel. 908-789-8900 Fax 908-789-8922

FIELD SAMPLING LOG

Project Name: ParSippany Wastewater quarterly 202
Project Location: ParSippany
Cooler Custody Seal: N/A
Temperature Correction Factor (°C): 0

Client Name: Metem A GE power Business
Client Address: 700 Parsippany Road
Client Rep on Site: Sundas Pervez
Sampling Date: 10-1-25
Arrival Time: 1435 Departure Time: 1518

FIELD EQUIPMENT CALIBRATION

pH Calibration (SM4500-H B/9040C)				
	Calibration			ICV (± 0.1 pH unit)
	7.00 Buffer	4.00 Buffer	10.00 Buffer	7.00 Buffer
	W 3217	W 3178	W 3191	W 3093
Time	1450	1452	1454	1456
Temp °C	21.6 C	21.0 C	21.2 C	21.5 C
pH	~~4.06~~ JD 7.00	4.00	10.05	7.01

FIELD EQUIPMENT CALIBRATION

Specific Conductance (mS/cm) (99% -101%)/(mmho/cm) (SM2510 B/120.1/9050A)		
	Calibration (± 1%) (99% -101%)	ICV (± 1%) (99% -101%)
	WP	WP
Time		
Temp °C		
Reading (mS/cm)		

Sampler Signature/Date: 10-1-25

Supervisor Review/Date: _____

QA Control# A3041249

Client Name: Metlife # of Park Ridge

Client Address: 700 Parsippany Road

Client Rep on Site: Sundas Pervez

Sampling Date: 10-1-25

Arrival Time: 1435 Departure Time: 1518

Project Location: Parsippany

Cooler Custody Seal: N/A

Temperature Correction Factor (°C): 0

FIELD SAMPLING INFORMATION

Sampling Location	Date/Time of sampling	Field Measurements			
		Date/Time of Analysis	pH	Temperature °C	Specific Conductance (mS/cm) (99% -101%)
CCV (C3093)	10-1-25 1458	10-1-25 1500	7.00	21.2°C	N/A
Q4	1500	1502	7.64	20.4°C	
Dup	1504	1507	7.64	20.5°C	
CCV (C3093)	1509	1511	7.01	21.3°C	

Meter: YSI MPS, Model # 556, Serial # 085A0063

Sampler Signature/Date: 10-1-25

Supervisor Review/Date: _____

QA Control# A3041249

Alliance TECHNICAL GROUP
284 Sheffield Street, Mountainside NJ 07092 (908)-789-8900 Fax : 908 789 8922

Laboratory Certification

Certified By	License No.
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255425
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	TX-C25-00189
Virginia	460312