


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100225\
Data File : BG064472.D
Acq On : 2 Oct 2025 8:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 02 16:40:42 2025

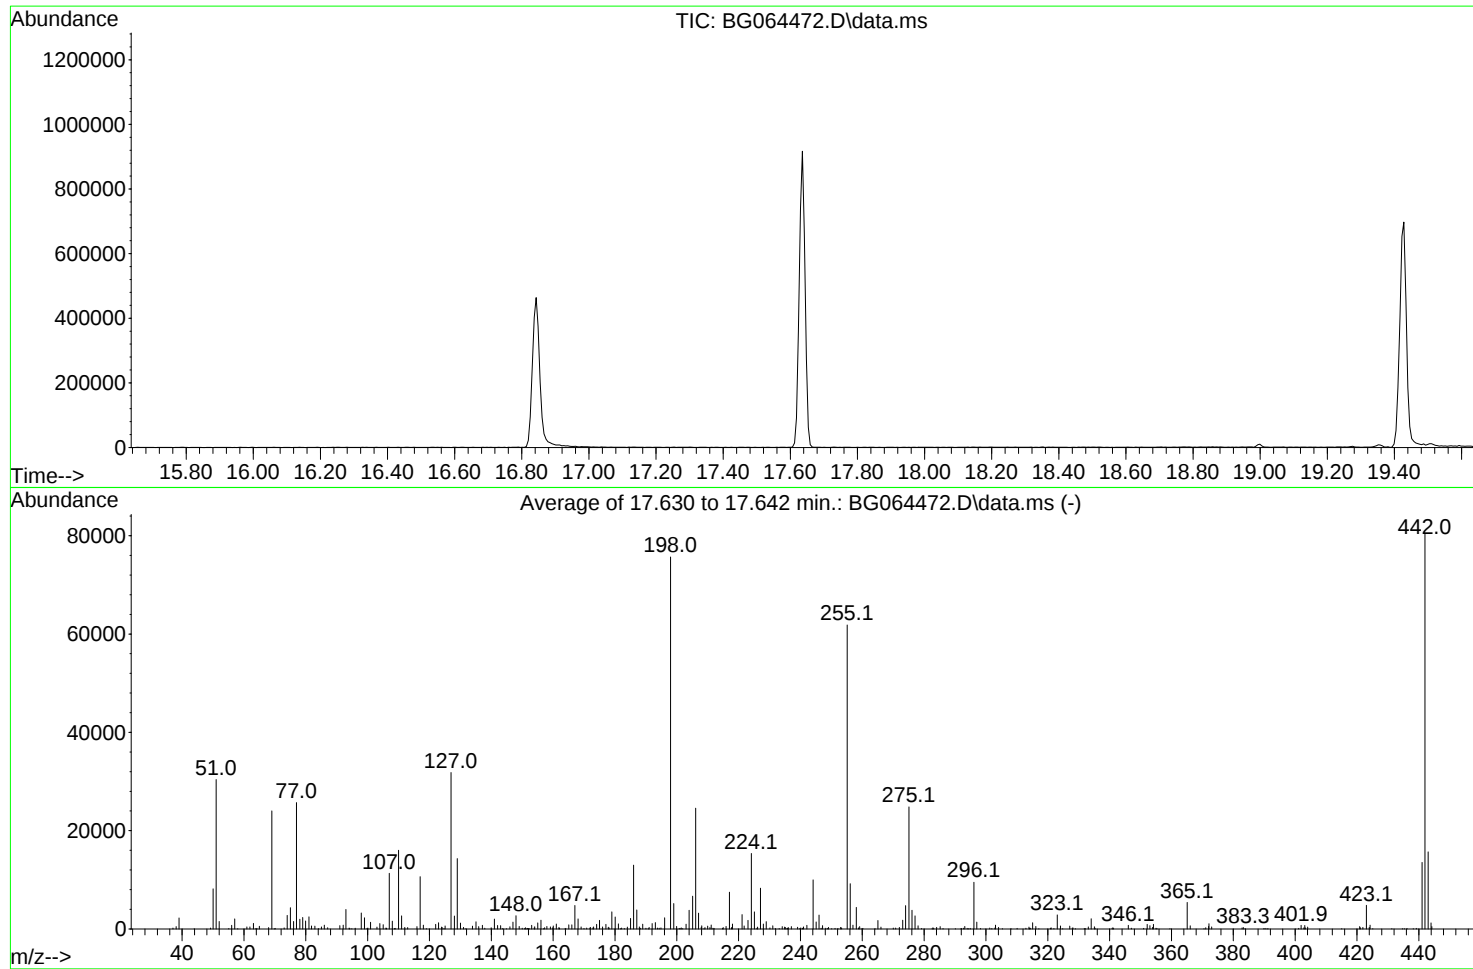

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.1	271	PASS
69	69	100	100	100.0	24008	PASS
70	69	0.00	2	0.4	100	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	75675	PASS
199	198	5	9	6.8	5168	PASS
365	198	1	100	7.1	5406	PASS
441	443	0.01	150	86.2	13521	PASS
442	442	100	100	100.0	80341	PASS
443	442	15	24	19.5	15684	PASS