


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100325\
Data File : BG064484.D
Acq On : 3 Oct 2025 12:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 02 16:40:42 2025

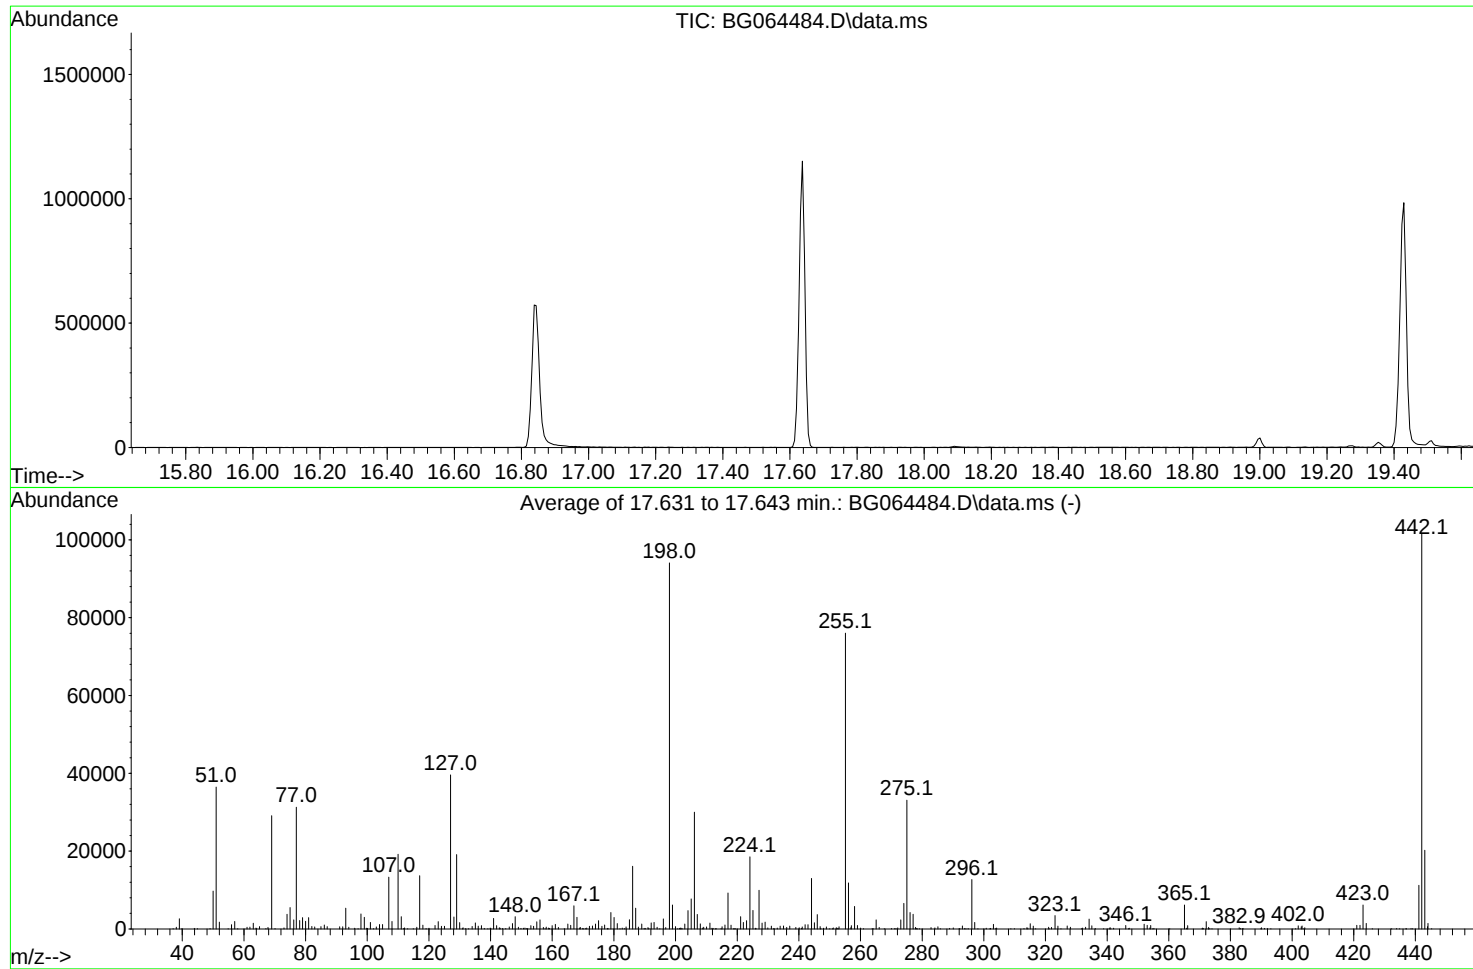




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.4	409	PASS
69	69	100	100	100.0	29101	PASS
70	69	0.00	2	0.3	85	PASS
197	198	0.00	2	0.4	350	PASS
198	198	100	100	100.0	94096	PASS
199	198	5	9	6.5	6146	PASS
365	198	1	100	6.5	6153	PASS
441	443	0.01	150	55.5	11215	PASS
442	442	100	100	100.0	101485	PASS
443	442	15	24	19.9	20196	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100325\
Data File : BG064484.D
Acq On : 3 Oct 2025 12:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 03 13:30:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 02 16:40:42 2025
Response via : Initial Calibration

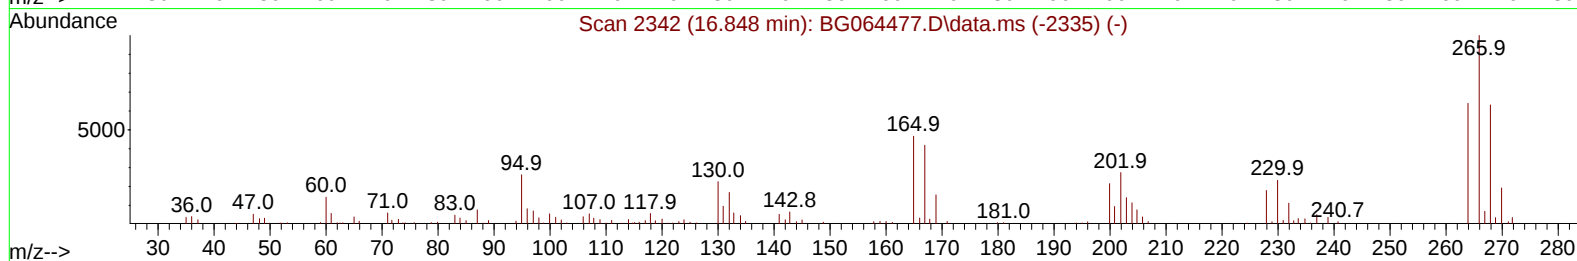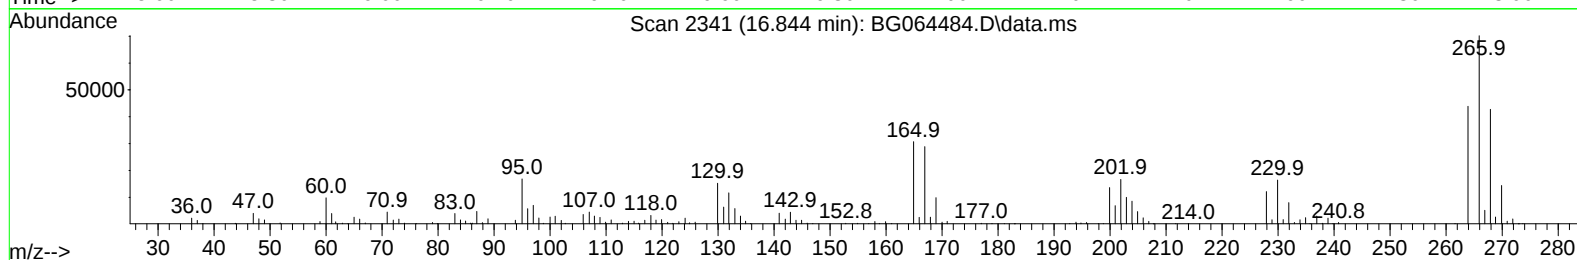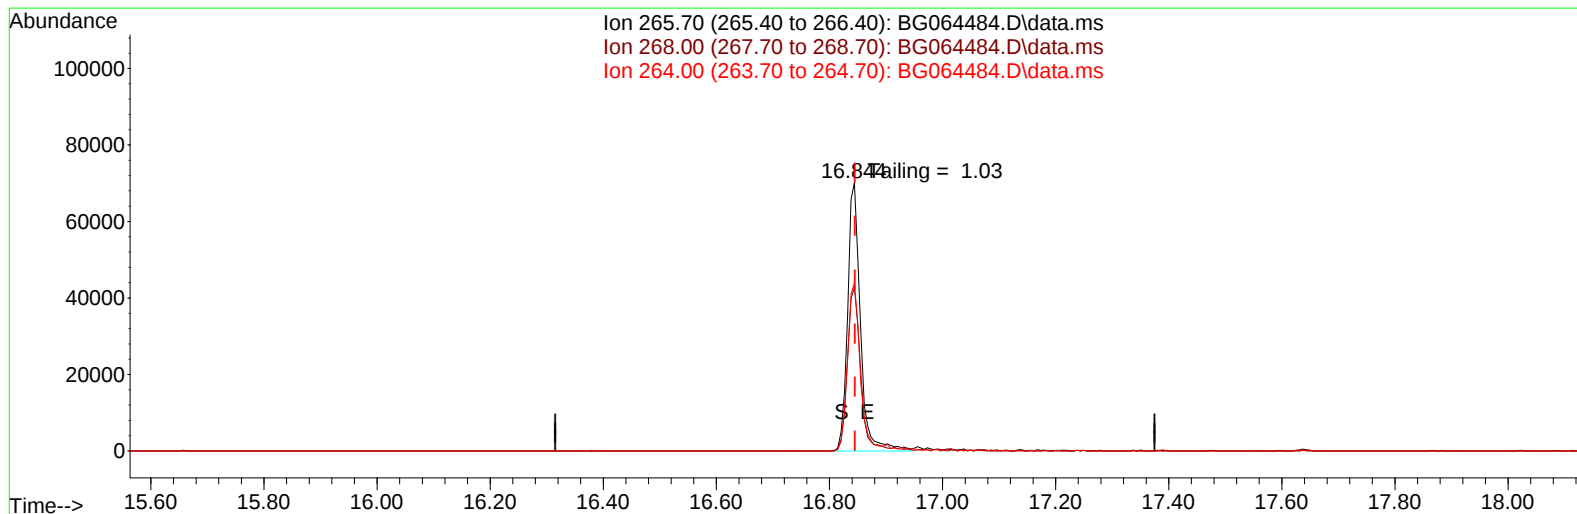

TIC: BG064484.D\data.ms

(70) Pentachlorophenol (C)

16.844min (-0.001) 67536.73 ng




response 110600

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	60.92
264.00	64.00	62.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100325\
Data File : BG064484.D
Acq On : 3 Oct 2025 12:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 03 13:30:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 02 16:40:42 2025
Response via : Initial Calibration

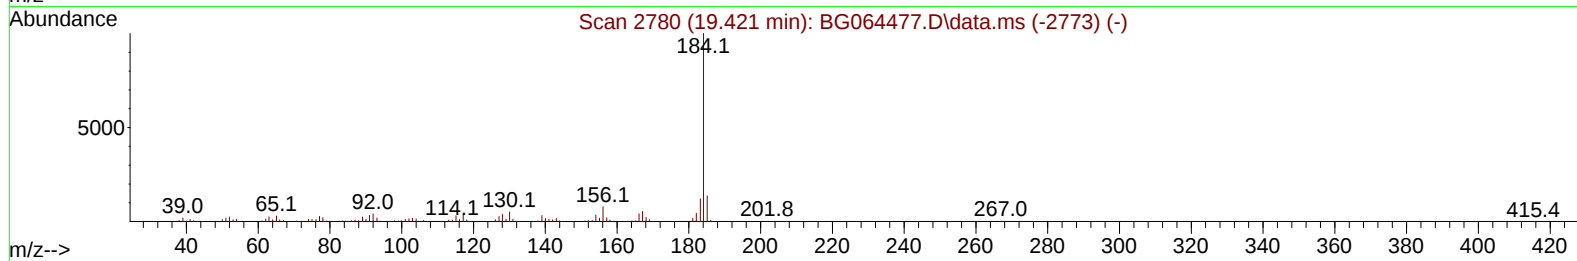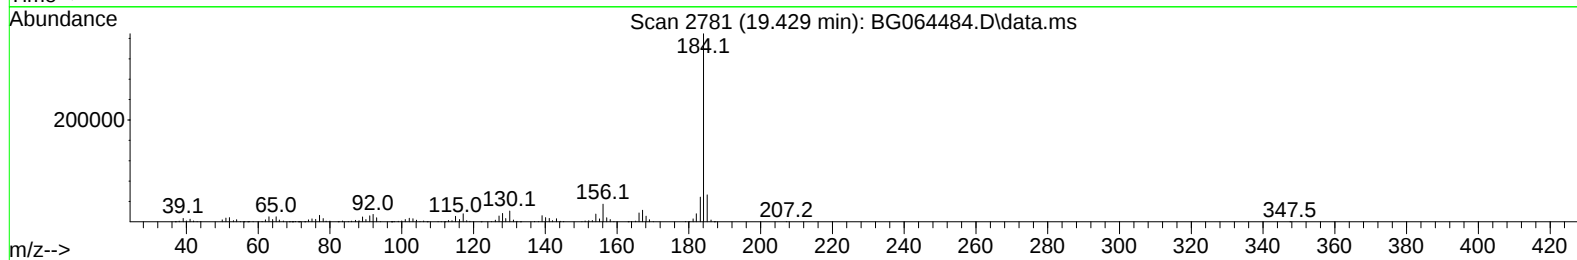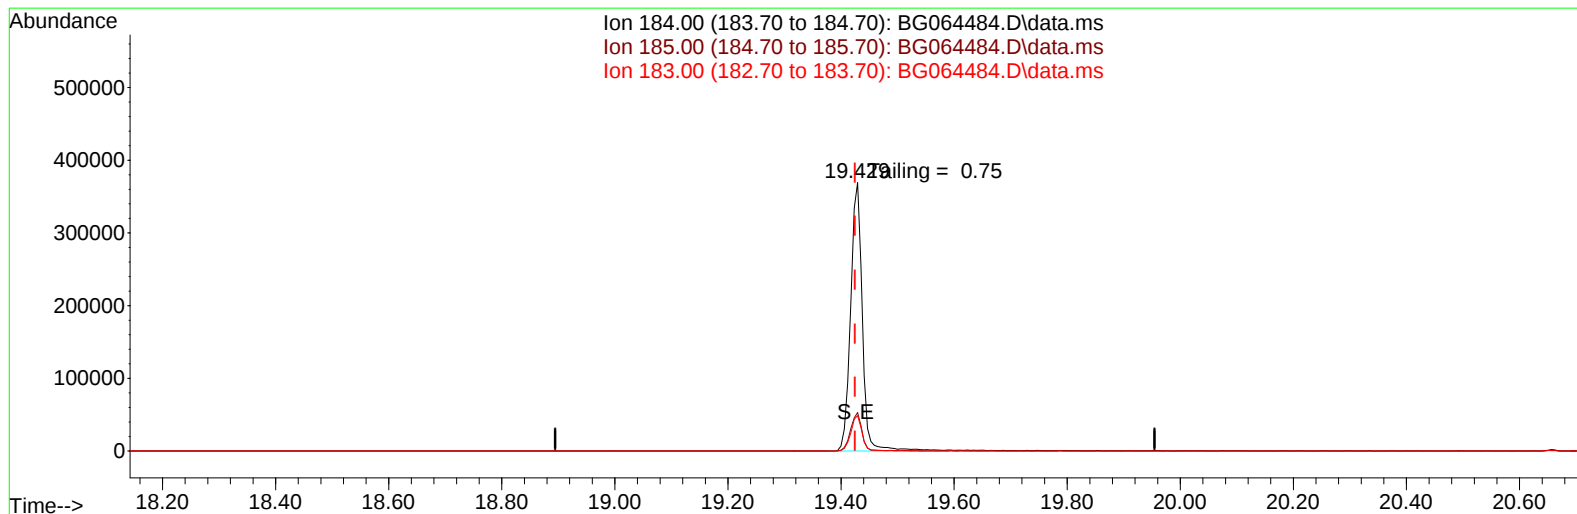

TIC: BG064484.D\data.ms

(77) Benzidine

19.429min (+ 0.004) 28542.55 ng

response 531970

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.34
183.00	12.20	13.17
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/3/2025	BNA_G	<u>BG064484.D</u>
Compound Name	Response	Retention Time
DDT	369876	20.657
DDD	5315	20.217
DDE	294	19.711
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5609	375485	1.49

Instrument :
BNA_G
ClientSampleId :
DFTPP