

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG100325\  
Data File : BG064488.D  
Acq On : 3 Oct 2025 15:35  
Operator : RC/JU  
Sample : PB169973BL  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB169973BL

Integration Parameters: rteint.p  
Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG100225.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG064488.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.415       | 389           | 396         | 404          | rBV      | 414112         | 622304        | 28.61%          | 8.093%        |
| 2         | 7.001       | 658           | 666         | 673          | rBV      | 393647         | 667108        | 30.67%          | 8.676%        |
| 3         | 7.824       | 799           | 806         | 813          | rBB      | 69950          | 113447        | 5.22%           | 1.475%        |
| 4         | 8.976       | 993           | 1002        | 1010         | rBV      | 242448         | 422134        | 19.41%          | 5.490%        |
| 5         | 10.609      | 1273          | 1280        | 1295         | rVB      | 82628          | 154573        | 7.11%           | 2.010%        |
| 6         | 13.071      | 1693          | 1699        | 1712         | rBV      | 702849         | 1080017       | 49.65%          | 14.046%       |
| 7         | 14.446      | 1927          | 1933        | 1944         | rBV      | 154134         | 244585        | 11.24%          | 3.181%        |
| 8         | 15.938      | 2180          | 2187        | 2201         | rBV      | 712709         | 1087253       | 49.99%          | 14.140%       |
| 9         | 17.189      | 2391          | 2400        | 2407         | rBV      | 242464         | 354840        | 16.31%          | 4.615%        |
| 10        | 19.810      | 2839          | 2846        | 2854         | rBV      | 1723358        | 2175065       | 100.00%         | 28.287%       |
| 11        | 21.408      | 3112          | 3118        | 3127         | rBV      | 243946         | 383387        | 17.63%          | 4.986%        |
| 12        | 24.387      | 3615          | 3625        | 3635         | rBV2     | 145265         | 384523        | 17.68%          | 5.001%        |




Sum of corrected areas: 7689236

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG100325\  
Data File : BG064488.D  
Acq On : 3 Oct 2025 15:35  
Operator : RC/JU  
Sample : PB169973BL  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB169973BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG100225.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

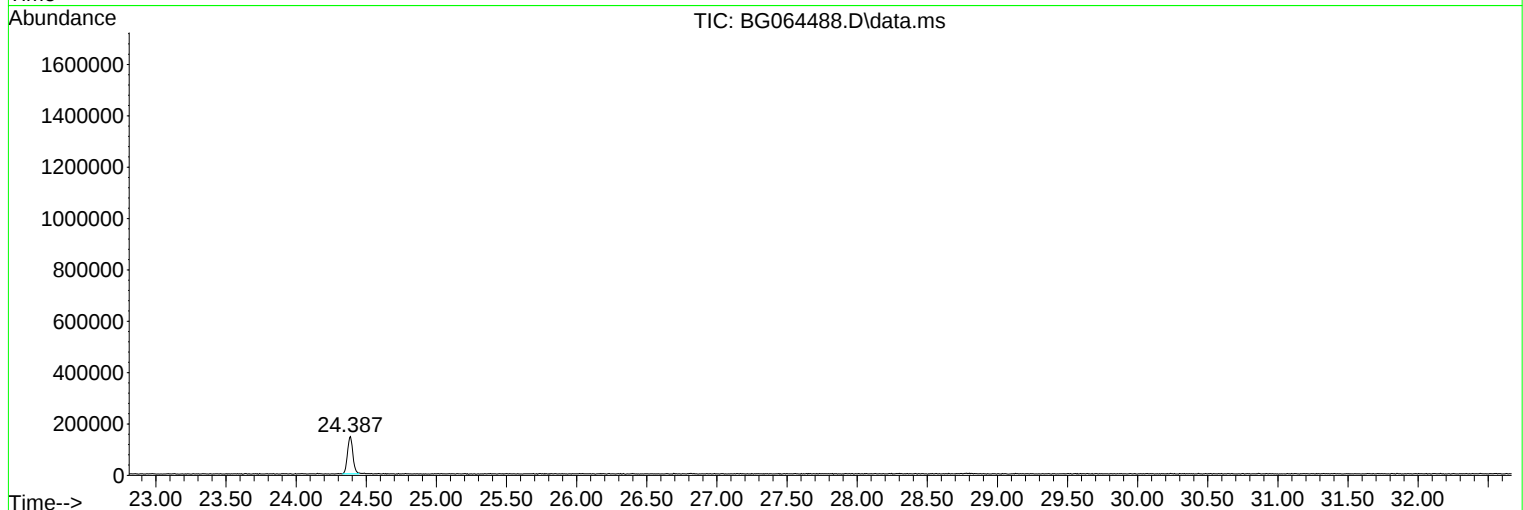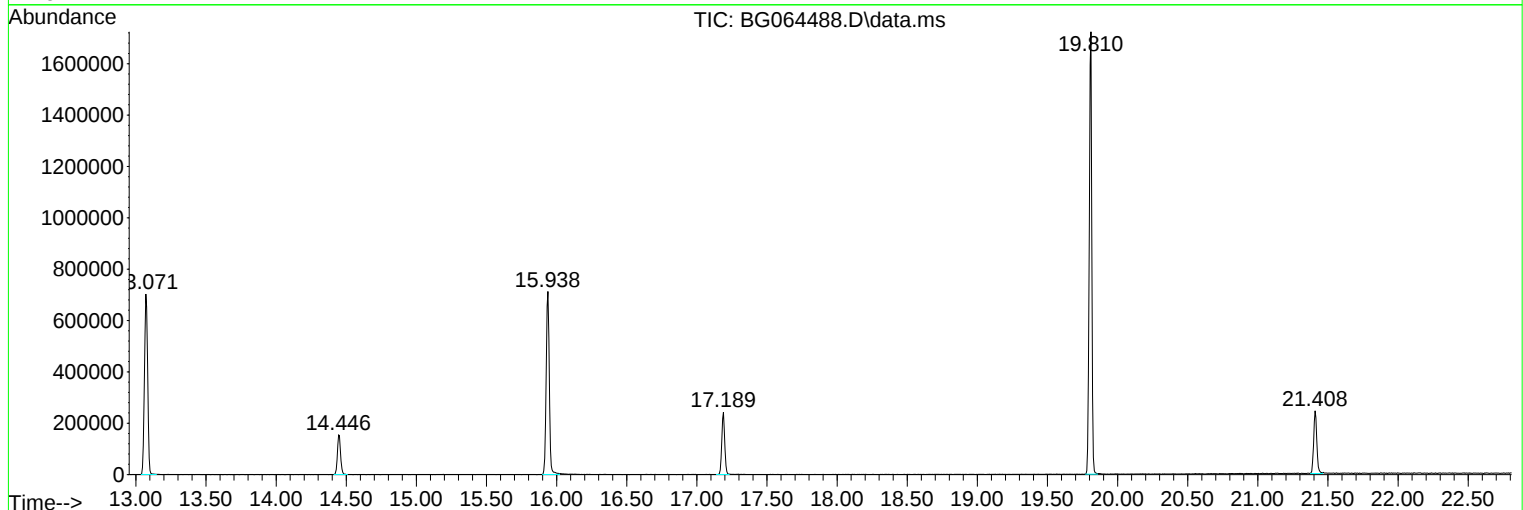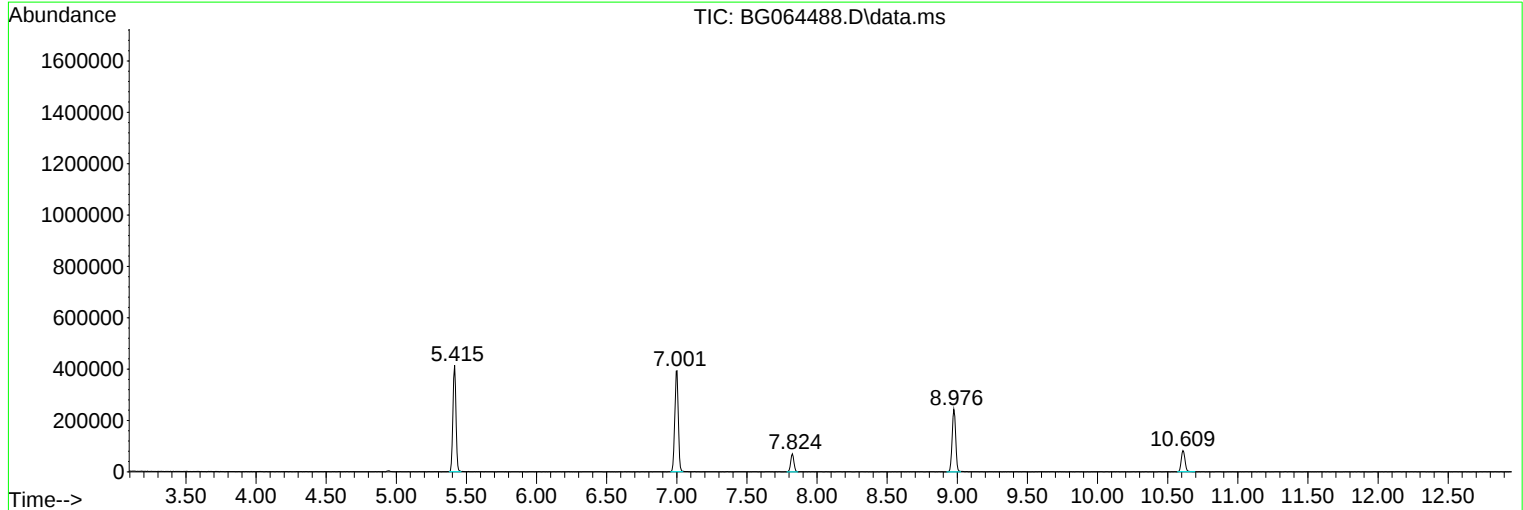

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG100325\  
Data File : BG064488.D  
Acq On : 3 Oct 2025 15:35  
Operator : RC/JU  
Sample : PB169973BL  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB169973BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG100225.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG100325\  
Data File : BG064488.D  
Acq On : 3 Oct 2025 15:35  
Operator : RC/JU  
Sample : PB169973BL  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB169973BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG100225.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|