
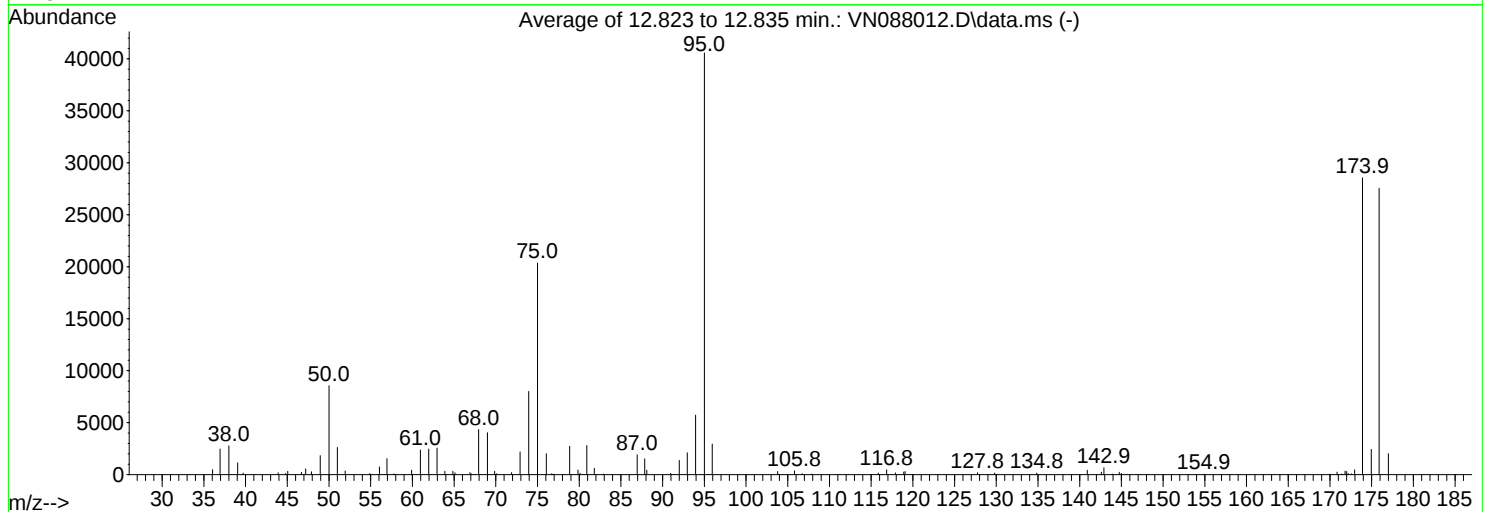


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100325\
Data File : VN088012.D
Acq On : 03 Oct 2025 09:34
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N092325W.M
Title : SW846 8260
Last Update : Wed Sep 24 05:05:30 2025

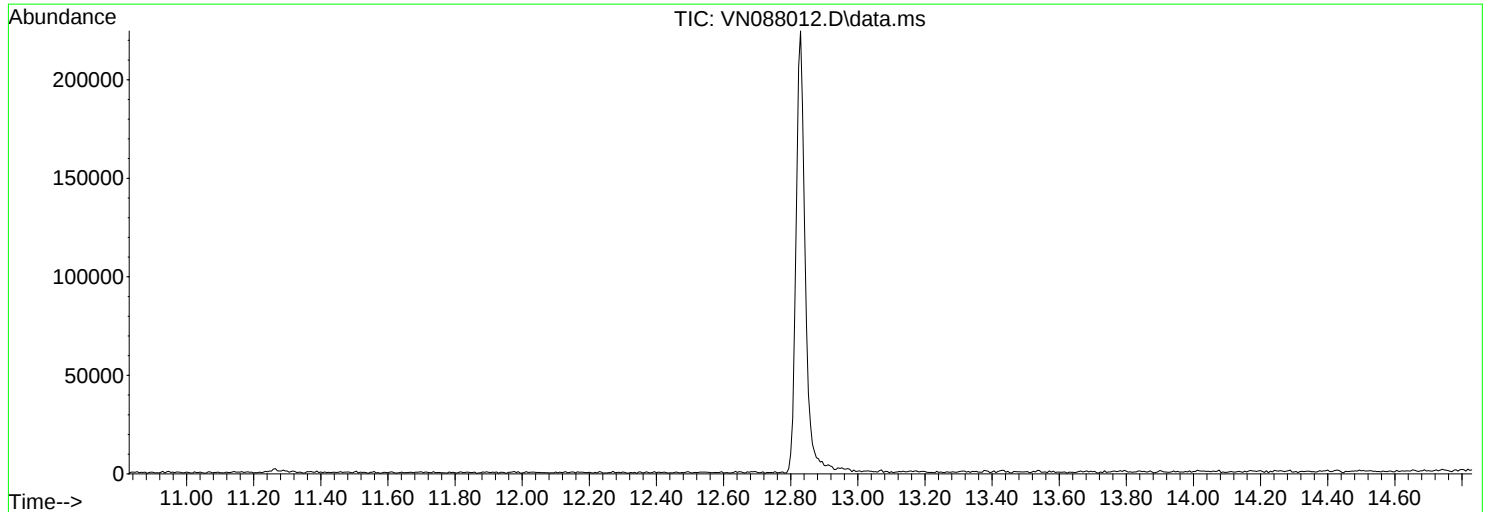

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	8567	PASS
75	95	30	60	50.2	20371	PASS
95	95	100	100	100.0	40579	PASS
96	95	5	9	7.3	2942	PASS
173	174	0.00	2	1.6	464	PASS
174	95	50	100	70.4	28557	PASS
175	174	5	9	8.5	2440	PASS
176	174	95	101	96.5	27552	PASS
177	176	5	9	7.3	2015	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	484	48.95	1838	62.95	2560	72.90	2184
36.95	2460	50.00	8567	63.90	324	73.95	800
38.00	2774	51.00	2614	64.85	322	75.00	2037
39.05	1146	51.95	358	65.10	182	76.05	201
39.70	156	54.90	105	66.90	195	76.70	94
43.90	192	56.05	741	67.10	75	76.90	55
44.80	109	56.95	1541	67.95	4346	78.85	2729
45.05	323	57.80	75	69.00	4040	79.85	453
46.70	216	59.90	429	69.85	321	80.10	137
47.20	560	60.95	2365	70.10	96	80.90	2796
47.90	285	61.95	2458	71.90	199	81.80	617

Average of 12.823 to 12.835 min.: VN088012.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
82.90	65	105.80	364	140.90	435	172.00	309
86.95	1910	106.75	101	142.60	233	172.20	103
87.85	1520	107.90	66	142.90	663	172.60	73
88.10	424	115.85	156	143.90	56	172.95	464
90.95	122	116.85	458	144.75	229	173.90	28557
92.00	1369	117.90	169	145.00	128	174.95	2440
92.95	2116	118.90	243	154.90	51	175.90	27552
93.95	5721	119.05	305	170.00	56	177.00	2015
95.00	40579	127.75	185	170.85	248		
95.95	2942	129.80	163	171.40	65		
103.80	313	134.85	148	171.80	334		

Instrument :

MSVOA_N

ClientSampleId :

BFB