

Prep Standard - Chemical Standard Summary

Order ID : Q3277

Test : EPH_NF

Prepbatch ID : PB169970,

Sequence ID/Qc Batch ID: FE100325AL,

Standard ID :

EP2641,EP2646,PP24768,PP24769,PP24770,PP24771,PP24772,PP24773,PP24774,PP24915,PP24918,PP24941,

Chemical ID :

E3875,E3951,E3956,E3966,E3972,E3973,E3974,P12364,P13280,P13281,P13620,P13690,P14029,P14030,P14031,P14032,P14058,P14059,P14060,P14061,P14074,P14075,P14076,P14077,P14078,P14079,P14080,P14081,P14082,P14083,P14094,P14095,P14096,P14097,P14098,P14099,P14100,P14101,P14102,P14103,P14147,P14148,P14149,P14150,W3234,

Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2017	1:1 ACETONE/METHYLENE CHLORIDE	EP2641	09/16/2025	03/16/2026	Evelyn Huang	None	None	Riteshkumar Patel
09/16/2025								

FROM 8000.00000ml of E3972 + 8000.00000ml of E3973 = Final Quantity: 16000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	EP2646	09/26/2025	01/28/2026	Evelyn Huang	Extraction_SC ALE_2	None	Riteshkumar Patel
(EX-SC-2)								

FROM 4000.00000gram of E3875 = Final Quantity: 4000.000 gram



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
781	100 PPM Aliphatic HC Working STD (Restek)	PP24768	08/01/2025	02/01/2026	Yogesh Patel	None	None	Abdul Mirza 08/19/2025
<u>FROM</u> 0.25000ml of P13620 + 0.25000ml of P13690 + 1.25000ml of P12364 + 23.25000ml of E3956 = Final Quantity: 25.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2900	100 PPM Aliphatic HC STD (Absolute)	PP24769	08/01/2025	02/01/2026	Yogesh Patel	None	None	Abdul Mirza 08/19/2025
<u>FROM</u> 0.22000ml of P13690 + 0.25000ml of P13620 + 1.25000ml of P13280 + 1.25000ml of P13281 + 22.00000ml of E3956 = Final Quantity: 25.000 ml								

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
783	50 PPM Aliphatic HC STD	PP24770	08/01/2025	02/01/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24768 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
784	20 PPM Aliphatic HC STD	PP24771	08/01/2025	02/01/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.80000ml of W3234 + 0.20000ml of PP24768 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
785	10 PPM Aliphatic HC STD	PP24772	08/01/2025	02/01/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.90000ml of W3234 + 0.10000ml of PP24768 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
786	5 PPM Aliphatic HC STD	PP24773	08/01/2025	02/01/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.90000ml of W3234 + 0.10000ml of PP24770 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2901	20 PPM Aliphatic HC STD ICV (Absolute)	PP24774	08/01/2025	02/01/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.80000ml of W3234 + 0.20000ml of PP24769 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1331	100 PPM NJEPH Fractionating Surrogate	PP24915	08/28/2025	02/28/2026	Abdul Mirza	None	None	Yogesh Patel
								09/17/2025

FROM 1.25000ml of P14058 + 1.25000ml of P14059 + 1.25000ml of P14060 + 1.25000ml of P14061 + 195.00000ml of E3966 = Final Quantity: 200.000 ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	417203	01/28/2026	07/28/2025 / RUPESH	01/29/2025 / Rajesh	E3875

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-3382-05 / Sand, Purified (cs/4x2.5kg)	25A2756718	12/31/2028	07/09/2025 / RUPESH	04/28/2020 / RUPESH	E3951

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	25C0362005	04/30/2026	07/16/2025 / RUPESH	07/16/2025 / RUPESH	E3956

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	25C0362005	04/30/2026	08/22/2025 / RUPESH	08/20/2025 / RUPESH	E3966

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H1462005	05/24/2027	09/16/2025 / Evelyn	09/04/2025 / Riteshkumar	E3972

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	25C1262005	04/16/2026	09/15/2025 / Riteshkumar	09/15/2025 / Riteshkumar	E3973

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	25C0362006	04/10/2027	09/26/2025 / Riteshkumar	09/26/2025 / Riteshkumar	E3974

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30540 / Custom NJEPH Aliphatics Calibration Standard	A0190424	02/01/2026	08/01/2025 / yogesh	03/16/2023 / Yogesh	P12364

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	95899 / NJ EPH Aliphatic n-Hydrocarbons-Revised, 1000 PPM	040524	02/01/2026	08/01/2025 / yogesh	04/11/2024 / yogesh	P13280

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	95899 / NJ EPH Aliphatic n-Hydrocarbons-Revised, 1000 PPM	040524	02/01/2026	08/01/2025 / yogesh	04/11/2024 / yogesh	P13281

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0213283	02/01/2026	08/01/2025 / yogesh	10/16/2024 / yogesh	P13620

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0216631	02/01/2026	08/01/2025 / yogesh	10/16/2024 / yogesh	P13690

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0225485	03/24/2026	09/24/2025 / Abdul	06/02/2025 / Rahul	P14029

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0225485	03/24/2026	09/24/2025 / Abdul	06/02/2025 / Rahul	P14030

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0225485	03/24/2026	09/24/2025 / Abdul	06/02/2025 / Rahul	P14031

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0225485	03/24/2026	09/24/2025 / Abdul	06/02/2025 / Rahul	P14032

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0224278	02/28/2026	08/28/2025 / Abdul	06/09/2025 / anahy	P14058

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0221895	02/28/2026	08/28/2025 / Abdul	06/09/2025 / anahy	P14059

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0221895	02/28/2026	08/28/2025 / Abdul	06/09/2025 / anahy	P14060

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0221895	02/28/2026	08/28/2025 / Abdul	06/09/2025 / anahy	P14061

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0225381	03/02/2026	09/02/2025 / Abdul	07/16/2025 / anahy	P14074

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0225381	03/02/2026	09/02/2025 / Abdul	07/16/2025 / anahy	P14075

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0225381	03/02/2026	09/02/2025 / Abdul	07/16/2025 / anahy	P14076

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0225381	03/02/2026	09/02/2025 / Abdul	07/16/2025 / anahy	P14077

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0225381	03/02/2026	09/02/2025 / Abdul	07/16/2025 / anahy	P14078

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0225381	03/02/2026	09/02/2025 / Abdul	07/16/2025 / anahy	P14079

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0225381	03/02/2026	09/02/2025 / Abdul	07/16/2025 / anahy	P14080

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0225381	03/02/2026	09/02/2025 / Abdul	07/16/2025 / anahy	P14081

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0225381	03/02/2026	09/02/2025 / Abdul	07/16/2025 / anahy	P14082

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0225381	03/02/2026	09/02/2025 / Abdul	07/16/2025 / anahy	P14083

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0226411	03/02/2026	09/02/2025 / Abdul	07/16/2025 / anahy	P14094

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0226411	03/02/2026	09/02/2025 / Abdul	07/16/2025 / anahy	P14095

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0226411	03/02/2026	09/02/2025 / Abdul	07/16/2025 / anahy	P14096

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0226411	03/02/2026	09/02/2025 / Abdul	07/16/2025 / anahy	P14097

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0226411	03/02/2026	09/02/2025 / Abdul	07/16/2025 / anahy	P14098

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0226411	03/02/2026	09/02/2025 / Abdul	07/16/2025 / anahy	P14099

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0226411	03/02/2026	09/02/2025 / Abdul	07/16/2025 / anahy	P14100

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0226411	03/02/2026	09/02/2025 / Abdul	07/16/2025 / anahy	P14101

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0226411	03/02/2026	09/02/2025 / Abdul	07/16/2025 / anahy	P14102

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0226411	03/02/2026	09/02/2025 / Abdul	07/16/2025 / anahy	P14103

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0216631	03/24/2026	09/24/2025 / Abdul	09/24/2025 / Abdul	P14147

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0216631	03/24/2026	09/24/2025 / Abdul	09/24/2025 / Abdul	P14148

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0216631	03/24/2026	09/24/2025 / Abdul	09/24/2025 / Abdul	P14149

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0216631	03/24/2026	09/24/2025 / Abdul	09/24/2025 / Abdul	P14150

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	25C0362005	04/30/2026	07/28/2025 / jignesh	07/25/2025 / jignesh	W3234

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03

Batch No.: 25C0362006

Manufactured Date: 2025-01-29

Expiration Date: 2026-04-30

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	6
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	4
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5\%$	100.0 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95\%$	100 %
Color (APHA)	≤ 10	10
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05\%$	$< 0.01\%$

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E 3974

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC



**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MÉXICO
CP 64070
TEL +52 81 13 52 67 67
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na ₂ SO ₄
SPECIFICATION NUMBER:	6399	RELEASE DATE:	MAY/23/2024
LOT NUMBER :	417203		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na ₂ SO ₄)	Min. 99.0%	99.8 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.2
Insoluble matter	Max. 0.01%	0.001 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO ₄)	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.001 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.001 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.2 %
Retained on US Standard No. 60 sieve	Min. 94%	96.2 %
Through US Standard No. 60 sieve	Max. 5%	3.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

RE-02-01, Ed. 3

E 3875



Material	BDH9274-2.5KG
Material Description	BDH SAND STDD OTTAWA W+I 2.5KG
Grade	NOT APPLICABLE
Batch	25A2756718
Reassay Date	12/31/2028
CAS Number	14808-60-7
Molecular Formula	SiO ₂
Molecular Mass	60.09
Date of Manufacture	12/05/2024
Storage	Room Temperature

Characteristics	Specifications	Measured Values
Appearance	Beige granules.	Beige granules.
Moisture	<= 0.1 %	0.1 %
Particle Size 30-40 mesh	>= 80 %	99 %
CUSTOMER PART # BDH9274-2.5KG		

Received on 1/12/25.

E3951

Internal ID #: 793

Signature	Additional Information
We certify that this batch conforms to the specifications listed above. This document has been electronically produced and is valid without a signature. Leona Edwardson, Quality Control Sr. Manager - Solon VWR Chemicals, LLC. 28600 Fountain Parkway, Solon OH 44139 USA	Analysis may have been rounded to significant digits in specification limits Product meets analytical specifications of the grades listed.

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03

Batch No.: 25C0362005

Manufactured Date: 2025-01-29

Expiration Date: 2026-04-30

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	≤ 10	6
ECD-Sensitive Impurities (as EthyleneDibromide) - Single Impurity Peak (ng/mL)	≤ 5	5
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	100.0 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	100 %
Color (APHA)	≤ 10	10
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	$< 0.01 \%$

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

Received on 7/16/25

E3956

Jamie Croak
Director Quality Operations, Bioscience Production

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 25C0362005
Manufactured Date: 2025-01-29
Expiration Date: 2026-04-30
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	≤ 10	6
ECD-Sensitive Impurities (as EthyleneDibromide) - Single Impurity Peak (ng/mL)	≤ 5	5
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5\%$	100.0 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95\%$	100 %
Color (APHA)	≤ 10	10
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05\%$	$< 0.01\%$

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3966

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA, 19087 U.S.A. Phone 610.386.1700

Acetone
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

avantor™



Material No.: 9254-03

Batch No.: 24H1462005

Manufactured Date: 2024-05-24

Expiration Date: 2027-05-24

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	99.8 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (µeq/g)	<= 0.3	0.2
Titration Base (µeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	0.2 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	<1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

E3972

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30540 **Lot No.:** A0190424

Description : NJEPH Aliphatics Calibration Standard

Aliphatics Calibration Standard 2000µg/mL, Hexane/Carbon Disulfide (80:20), 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : November 30, 2029 **Storage:** 25°C nominal

Handling: Sonicate prior to use. **Ship:** Ambient

P12361
↓
P12370 } Y.P.
031/6/23

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)	
1	n-Nonane (C9) CAS # 111-84-2 Purity 99% (Lot SHBN5361)	2,014.0 µg/mL	+/- 11.8193 +/- 50.0027 +/- 59.9491	µg/mL Gravimetric Unstressed Stressed
2	n-Decane (C10) CAS # 124-18-5 Purity 99% (Lot SHBN8619)	2,014.7 µg/mL	+/- 11.8232 +/- 50.0193 +/- 59.9689	µg/mL Gravimetric Unstressed Stressed
3	Naphthalene CAS # 91-20-3 Purity 99% (Lot MKCH0219)	2,015.3 µg/mL	+/- 11.8271 +/- 50.0358 +/- 59.9888	µg/mL Gravimetric Unstressed Stressed
4	n-Dodecane (C12) CAS # 112-40-3 Purity 99% (Lot SHBN7174)	2,008.0 µg/mL	+/- 11.7841 +/- 49.8538 +/- 59.7705	µg/mL Gravimetric Unstressed Stressed
5	2-Methylnaphthalene CAS # 91-57-6 Purity 96% (Lot STBK0259)	2,007.0 µg/mL	+/- 11.7784 +/- 49.8299 +/- 59.7419	µg/mL Gravimetric Unstressed Stressed
6	n-Tetradecane (C14) CAS # 629-59-4 Purity 99% (Lot STBK2282)	2,016.7 µg/mL	+/- 11.8349 +/- 50.0689 +/- 60.0284	µg/mL Gravimetric Unstressed Stressed
7	n-Hexadecane (C16) CAS # 544-76-3 Purity 98% (Lot SHBM4146)	2,014.9 µg/mL	+/- 11.8244 +/- 50.0246 +/- 59.9753	µg/mL Gravimetric Unstressed Stressed

8	n-Octadecane (C18) CAS # 593-45-3 Purity 97%	(Lot VZKOJ)	2,004.7 µg/mL	+/-	11.7645	µg/mL	Gravimetric
				+/-	49.7710	µg/mL	Unstressed
				+/-	59.6712	µg/mL	Stressed
9	n-Eicosane (C20) CAS # 112-95-8 Purity 99%	(Lot MKCF7888)	2,018.0 µg/mL	+/-	11.8428	µg/mL	Gravimetric
				+/-	50.1020	µg/mL	Unstressed
				+/-	60.0681	µg/mL	Stressed
10	n-Heneicosane (C21) CAS # 629-94-7 Purity 99%	(Lot MKCL3226)	2,000.7 µg/mL	+/-	11.7410	µg/mL	Gravimetric
				+/-	49.6717	µg/mL	Unstressed
				+/-	59.5522	µg/mL	Stressed
11	n-Docosane (C22) CAS # 629-97-0 Purity 99%	(Lot MKCL8918)	2,005.3 µg/mL	+/-	11.7684	µg/mL	Gravimetric
				+/-	49.7876	µg/mL	Unstressed
				+/-	59.6911	µg/mL	Stressed
12	n-Tetracosane (C24) CAS # 646-31-1 Purity 99%	(Lot MKCN2863)	2,018.0 µg/mL	+/-	11.8428	µg/mL	Gravimetric
				+/-	50.1020	µg/mL	Unstressed
				+/-	60.0681	µg/mL	Stressed
13	n-Hexacosane (C26) CAS # 630-01-3 Purity 99%	(Lot MKCD4540)	2,014.0 µg/mL	+/-	11.8193	µg/mL	Gravimetric
				+/-	50.0027	µg/mL	Unstressed
				+/-	59.9491	µg/mL	Stressed
14	n-Octacosane (C28) CAS # 630-02-4 Purity 99%	(Lot BCCG0084)	2,002.0 µg/mL	+/-	11.7489	µg/mL	Gravimetric
				+/-	49.7048	µg/mL	Unstressed
				+/-	59.5919	µg/mL	Stressed
15	n-Triacontane (C30) CAS # 638-68-6 Purity 97%	(Lot MKCQ9436)	2,011.1 µg/mL	+/-	11.8025	µg/mL	Gravimetric
				+/-	49.9316	µg/mL	Unstressed
				+/-	59.8637	µg/mL	Stressed
16	n-Dotriacontane (C32) CAS # 544-85-4 Purity 99%	(Lot BCBW0661)	2,012.0 µg/mL	+/-	11.8075	µg/mL	Gravimetric
				+/-	49.9531	µg/mL	Unstressed
				+/-	59.8895	µg/mL	Stressed
17	n-Tetratriacontane (C34) CAS # 14167-59-0 Purity 99%	(Lot OML4N)	2,006.7 µg/mL	+/-	11.7762	µg/mL	Gravimetric
				+/-	49.8207	µg/mL	Unstressed
				+/-	59.7308	µg/mL	Stressed
18	n-Hexatriacontane (C36) CAS # 630-06-8 Purity 99%	(Lot Z27H018)	2,017.3 µg/mL	+/-	11.8388	µg/mL	Gravimetric
				+/-	50.0855	µg/mL	Unstressed
				+/-	60.0483	µg/mL	Stressed
19	n-Octatriacontane (C38) CAS # 7194-85-6 Purity 96%	(Lot 0000145137)	2,017.3 µg/mL	+/-	11.8385	µg/mL	Gravimetric
				+/-	50.0842	µg/mL	Unstressed
				+/-	60.0467	µg/mL	Stressed
20	n-Tetracontane (C40) CAS # 4181-95-7 Purity 99%	(Lot BSBME)	2,008.7 µg/mL	+/-	11.7880	µg/mL	Gravimetric
				+/-	49.8703	µg/mL	Unstressed
				+/-	59.7903	µg/mL	Stressed
Solvent: Hexane/Carbon disulfide (80:20)							
	CAS # 110-54-3/75-15-0						
	Purity 99%						

Column:
30m x 0.25mm x 0.25µm
Pxx-5 (cat.#10223)


Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

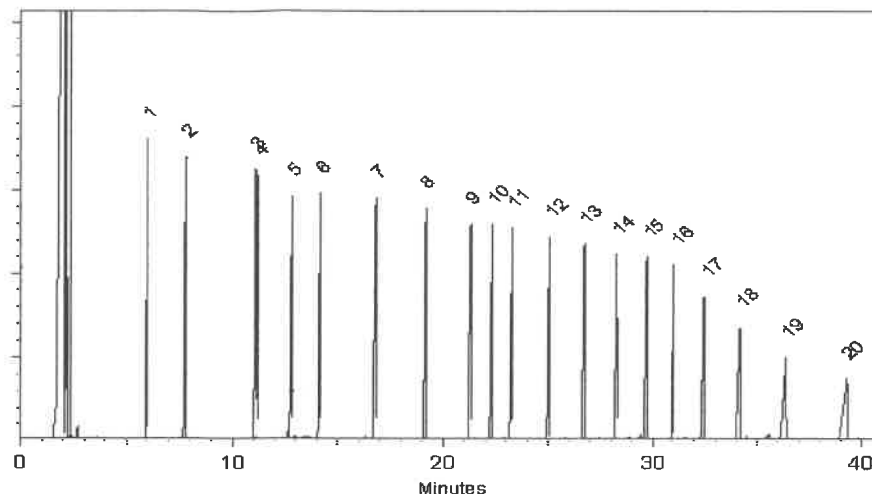

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Morgan Craighead - Mix Technician

Date Mixed: 10-Oct-2022 Balance: 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 20-Oct-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days


- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



CERTIFIED WEIGHT REPORT

Part Number: 95999

Lot Number: 040524

Description: NJ EPH Aliphatic n-Hydrocarbons - Revised
20 components

Expiration Date: 040534

Recommended Storage: Ambient (20 °C)

Nominal Concentration (µg/mL): 1000

NIST Test ID#: 6UTB

Weight(s) shown below were combined and diluted to (mL):

CAUTION: Sonicate Before Use

Solvent(s):
Cyclohexane

Lot#
28930


Formulated By:	Anthony Mahoney	040524	DATE
Reviewed By:	Pedro L. Rentas	040524	DATE

P13278
Y.P.
P13287
04/11/24

5E-05 Balance Uncertainty
0.001 Flask Uncertainty

CAUTION: Sonicate Before Use															SDS Information			
Compound															(Solvent Safety Info. On Attached pg.)			
(RM#)	Lot	Dil.	Initial	Initial	Nominal	Purity	Purity	Uncertainty	Target	Actual	Actual	Expanded						
Part Number	Number	Factor	Vol. (mL)	Conc. (µg/mL)	Conc. (µg/mL)	(%)	Uncertainty	Pipette	Weight(g)	Weight(g)	Conc. (µg/mL)	(+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50			
1. 2-Methylnaphthalene	(0214)	MKB3783V	NA	NA	NA	1000	97	0.2	NA	0.02579	0.02594	1005.7	5.7	91-57-6	N/A	or-rat 1630mg/kg		
2. Naphthalene	(0222)	MKB28680V	NA	NA	NA	1000	100	0.2	NA	0.02502	0.02511	1003.7	5.7	91-20-3	10 ppm (50mg/m3/8H)	or-rat 490mg/kg		
3. n-Nonane	95708	120222	1.00	25.00	1000.7	1000	NA	0.013	NA	NA	1000.0	4.2	111-84-2	200 ppm (1050mg/m3/8H)	ivr-mus 218mg/kg			
4. n-Decane	95708	120222	1.00	25.00	1000.9	1000	NA	0.013	NA	NA	1000.2	4.2	124-18-5	N/A	N/A			
5. n-Dodecane	95708	120222	1.00	25.00	1000.7	1000	NA	0.013	NA	NA	1000.0	4.2	112-40-3	N/A	ivr-mus 3494mg/kg			
6. n-Tetradecane	95708	120222	1.00	25.00	1002.1	1000	NA	0.013	NA	NA	1001.3	4.2	629-59-4	N/A	N/A			
7. n-Hexadecane	95708	120222	1.00	25.00	1000.5	1000	NA	0.013	NA	NA	999.7	4.2	544-76-3	N/A	N/A			
8. n-Octadecane	95708	120222	1.00	25.00	1001.0	1000	NA	0.013	NA	NA	1000.3	4.1	593-45-3	N/A	N/A			
9. n-Eicosane	95708	120222	1.00	25.00	1001.0	1000	NA	0.013	NA	NA	1000.3	4.2	112-95-8	N/A	N/A			
10. n-Heneicosane	95708	120222	1.00	25.00	1002.4	1000	NA	0.013	NA	NA	1001.6	4.2	629-94-7	N/A	N/A			
11. n-Docosane	95708	120222	1.00	25.00	1001.9	1000	NA	0.013	NA	NA	1001.2	4.2	629-97-0	N/A	N/A			
12. n-Tetracosane	95708	120222	1.00	25.00	1000.8	1000	NA	0.013	NA	NA	1000.1	4.2	646-31-1	N/A	N/A			
13. n-Hexacosane	95708	120222	1.00	25.00	1001.2	1000	NA	0.013	NA	NA	1000.4	4.2	630-01-3	N/A	N/A			
14. n-Octacosane	95708	120222	1.00	25.00	1000.5	1000	NA	0.013	NA	NA	999.8	4.2	630-02-4	N/A	N/A			
15. n-Triacontane	95708	120222	1.00	25.00	1000.5	1000	NA	0.013	NA	NA	999.8	4.2	638-68-6	N/A	N/A			
16. n-Dotriacontane	95708	120222	1.00	25.00	1000.5	1000	NA	0.013	NA	NA	999.8	4.3	544-85-4	N/A	ivr-mus 100mg/kg			
17. n-Tetra triacontane	95708	120222	1.00	25.00	1000.4	1000	NA	0.013	NA	NA	999.7	4.2	14167-59-0	N/A	N/A			
18. n-Hexatriacontane	95708	120222	1.00	25.00	1001.5	1000	NA	0.013	NA	NA	1000.8	4.2	630-06-8	N/A	N/A			
19. n-Octatriacontane	95708	120222	1.00	25.00	1000.3	1000	NA	0.013	NA	NA	999.6	4.3	7194-85-6	N/A	N/A			
20. n-Tetracontane	95708	120222	1.00	25.00	1000.6	1000	NA	0.013	NA	NA	999.9	4.3	4181-95-7	N/A	N/A			

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



CERTIFIED WEIGHT REPORT

Part Number: 95999

Lot Number: 040524

Description: NJ EPH Aliphatic n-Hydrocarbons - Revised
20 components

Expiration Date: 040534

Recommended Storage: Ambient (20 °C)

Nominal Concentration (µg/mL): 1000

NIST Test ID#: 6UTB

Weight(s) shown below were combined and diluted to (mL):

CAUTION: Sonicate Before Use

Solvent(s):
Cyclohexane

Lot#
28930

P13278
Y.P.
P13287
04/11/24

5E-05 Balance Uncertainty
0.001 Flask Uncertainty

Formulated By:	Anthony Mahoney	040524	DATE
Reviewed By:	Pedro L. Rentas	040524	DATE

Compound		Part Number	(RM#)	Lot Number	DIL Factor	Initial Vol. (mL)	Initial Conc (µg/mL)	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty	Pipette	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)		
																CAS#	OSHA PEL (TWA)	LD50
1.	2-Methylnaphthalene	(0214)	MKBF3783V	NA	NA	NA	NA	1000	97	0.2	NA	0.02579	0.02594	1005.7	5.7	91-57-6	N/A	or-rat 1630mg/kg
2.	Naphthalene	(0222)	MKB28680V	NA	NA	NA	NA	1000	100	0.2	NA	0.02502	0.02511	1003.7	5.7	91-20-3	10 ppm (50mg/m ³ /8H)	or-rat 490mg/kg
3.	n-Nonane	95708	120222	1.00	25.00	1000.7	1000.7	1000	NA	0.013	NA	NA	NA	1000.0	4.2	111-84-2	200 ppm (1050mg/m ³ /8H)	ivn-mus 218mg/kg
4.	n-Decane	95708	120222	1.00	25.00	1000.9	1000.9	1000	NA	0.013	NA	NA	NA	1000.2	4.2	124-18-5	N/A	N/A
5.	n-Dodecane	95708	120222	1.00	25.00	1000.7	1000.7	1000	NA	0.013	NA	NA	NA	1000.0	4.2	112-40-3	N/A	ivn-mus 3494mg/kg
6.	n-Tetradecane	95708	120222	1.00	25.00	1002.1	1002.1	1000	NA	0.013	NA	NA	NA	1001.3	4.2	629-59-4	N/A	N/A
7.	n-Hexadecane	95708	120222	1.00	25.00	1000.5	1000.5	1000	NA	0.013	NA	NA	NA	999.7	4.2	544-76-3	N/A	N/A
8.	n-Octadecane	95708	120222	1.00	25.00	1001.0	1001.0	1000	NA	0.013	NA	NA	NA	1000.3	4.1	583-45-3	N/A	N/A
9.	n-Eicosane	95708	120222	1.00	25.00	1001.0	1001.0	1000	NA	0.013	NA	NA	NA	1000.3	4.2	112-95-8	N/A	N/A
10.	n-Henicosane	95708	120222	1.00	25.00	1002.4	1002.4	1000	NA	0.013	NA	NA	NA	1001.6	4.2	629-94-7	N/A	N/A
11.	n-Docosane	95708	120222	1.00	25.00	1001.9	1001.9	1000	NA	0.013	NA	NA	NA	1001.2	4.2	629-97-0	N/A	N/A
12.	n-Tetracosane	95708	120222	1.00	25.00	1000.8	1000.8	1000	NA	0.013	NA	NA	NA	1000.1	4.2	646-31-1	N/A	N/A
13.	n-Hexacosane	95708	120222	1.00	25.00	1001.2	1001.2	1000	NA	0.013	NA	NA	NA	1000.4	4.2	630-01-3	N/A	N/A
14.	n-Octacosane	95708	120222	1.00	25.00	1000.5	1000.5	1000	NA	0.013	NA	NA	NA	999.8	4.2	630-02-4	N/A	N/A
15.	n-Triacontane	95708	120222	1.00	25.00	1000.5	1000.5	1000	NA	0.013	NA	NA	NA	999.8	4.2	638-68-6	N/A	N/A
16.	n-Dotriacontane	95708	120222	1.00	25.00	1000.5	1000.5	1000	NA	0.013	NA	NA	NA	999.8	4.3	544-85-4	N/A	ivn-mus 100mg/kg
17.	n-Tetracontane	95708	120222	1.00	25.00	1000.4	1000.4	1000	NA	0.013	NA	NA	NA	999.7	4.2	14167-59-0	N/A	N/A
18.	n-Hexatriacontane	95708	120222	1.00	25.00	1001.5	1001.5	1000	NA	0.013	NA	NA	NA	1000.8	4.2	630-08-8	N/A	N/A
19.	n-Octatriacontane	95708	120222	1.00	25.00	1000.3	1000.3	1000	NA	0.013	NA	NA	NA	999.6	4.3	7184-86-6	N/A	N/A
20.	n-Tetracontane	95708	120222	1.00	25.00	1000.6	1000.6	1000	NA	0.013	NA	NA	NA	999.9	4.3	4181-95-7	N/A	N/A

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31098 **Lot No.:** A0213283

Description : 1-Chlorooctadecane Standard

1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : July 31, 2031 **Storage:** 10°C or colder

Ship: Ambient

P13595
↓
P13624 } Y.P.
10/16/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Chlorooctadecane	3386-33-2	15018900	99%	10,058.0 µg/mL	+/- 565.0578

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-S (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

10 ml/min.

Inj. Vol

1µl

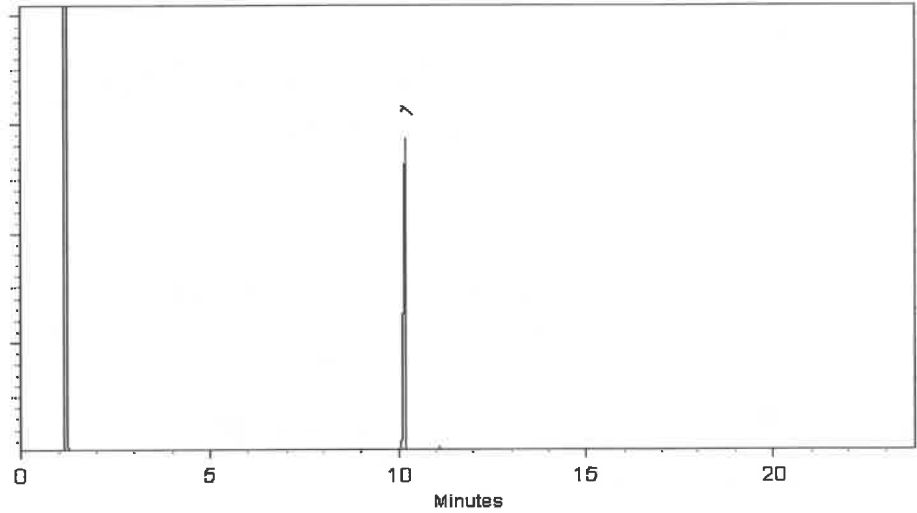

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Stacey Wanner - Operations Technician I

Date Mixed: 28-Jun-2024

Balance Serial # B345965662

Dillan Murphy - Operations Technician I

Date Passed: 01-Jul-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31097 **Lot No.:** A0216631
Description : o-Terphenyl Standard
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : April 30, 2028 **Storage:** 10°C or colder
Handling: Sonicate prior to use. **Ship:** Ambient

P13645 } Y.P.
↓
P13694 } 10/16/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	o-Terphenyl	84-15-1	GKSSA	99%	10,065.0 µg/mL	+/- 453.3336

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

10 ml/min.

Inj. Vol

1µl

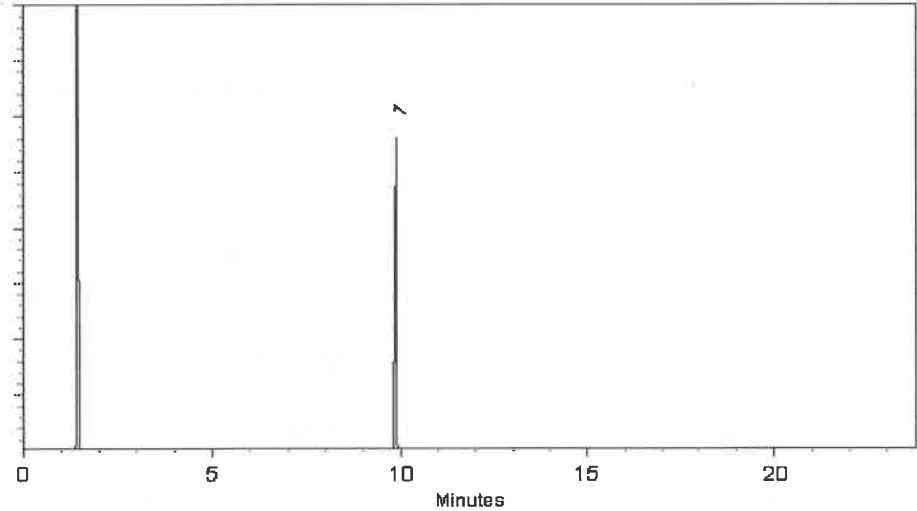

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ven Kelley - Operations Tech I

Date Mixed: 17-Sep-2024

Balance Serial # 1128353505

Dillan Murphy - Operations Technician I

Date Passed: 23-Sep-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31098 **Lot No.:** A0225485

Description : 1-Chlorooctadecane Standard

1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : June 30, 2032 **Storage:** 10°C or colder

Ship: Ambient

P14028
↓
P14042 } RC/
6/2/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Chlorooctadecane	3386-33-2	15711200	99%	10,006.8 µg/mL	+/- 562.1814

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

10 ml/min.

Inj. Vol

1µl

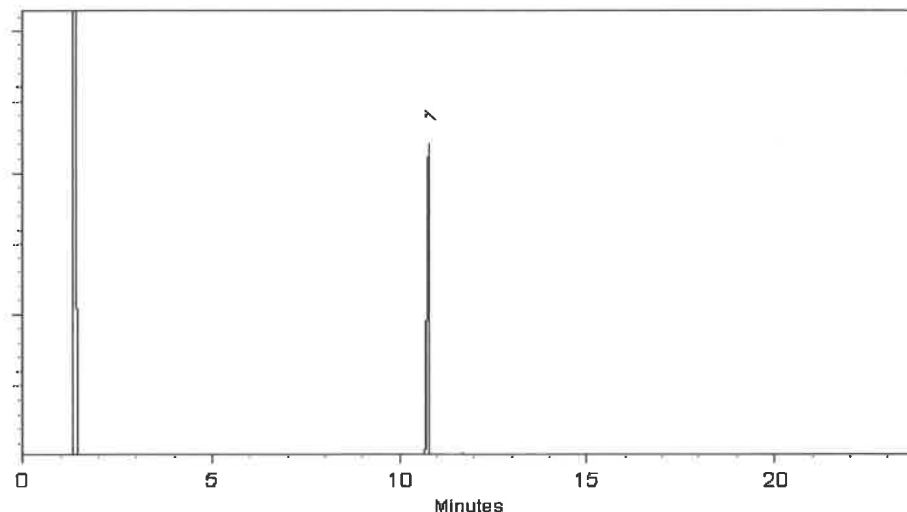

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler

Sam Moodler - Operations Tech I

Date Mixed: 08-May-2025

Balance Serial # 1128360905

Brittany Federinko

Brittany Federinko - Operations Tech II

Date Passed: 13-May-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31098 **Lot No.:** A0225485
Description : 1-Chlorooctadecane Standard
1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride,
1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : June 30, 2032 **Storage:** 10°C or colder
Ship: Ambient

P14028 } RC/
↓
P14042 } 6/2/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Chlorooctadecane	3386-33-2	15711200	99%	10,006.8 µg/mL	+/- 562.1814

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

10 ml/min.

Inj. Vol

1µl

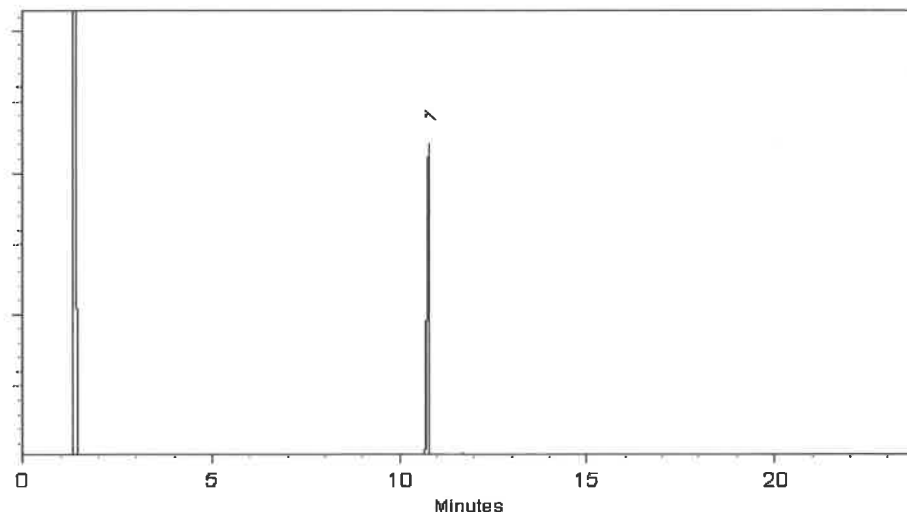

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler

Sam Moodler - Operations Tech I

Date Mixed: 08-May-2025

Balance Serial # 1128360905

Brittany Federinko

Brittany Federinko - Operations Tech II

Date Passed: 13-May-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31098 **Lot No.:** A0225485
Description : 1-Chlorooctadecane Standard
1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride,
1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : June 30, 2032 **Storage:** 10°C or colder
Ship: Ambient

P14028
↓
P14042 } RC/
6/2/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Chlorooctadecane	3386-33-2	15711200	99%	10,006.8 µg/mL	+/- 562.1814

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

10 ml/min.

Inj. Vol

1µl

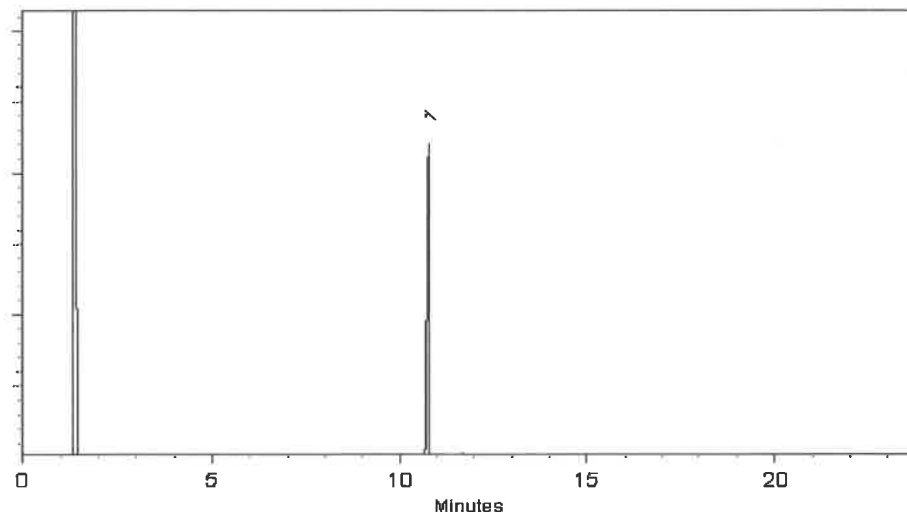

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler

Sam Moodler - Operations Tech I

Date Mixed: 08-May-2025

Balance Serial # 1128360905

Brittany Federinko

Brittany Federinko - Operations Tech II

Date Passed: 13-May-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31098 **Lot No.:** A0225485

Description : 1-Chlorooctadecane Standard

1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : June 30, 2032 **Storage:** 10°C or colder

Ship: Ambient

P14028
↓
P14042 } RC/
6/2/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Chlorooctadecane	3386-33-2	15711200	99%	10,006.8 µg/mL	+/- 562.1814

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

10 ml/min.

Inj. Vol

1µl

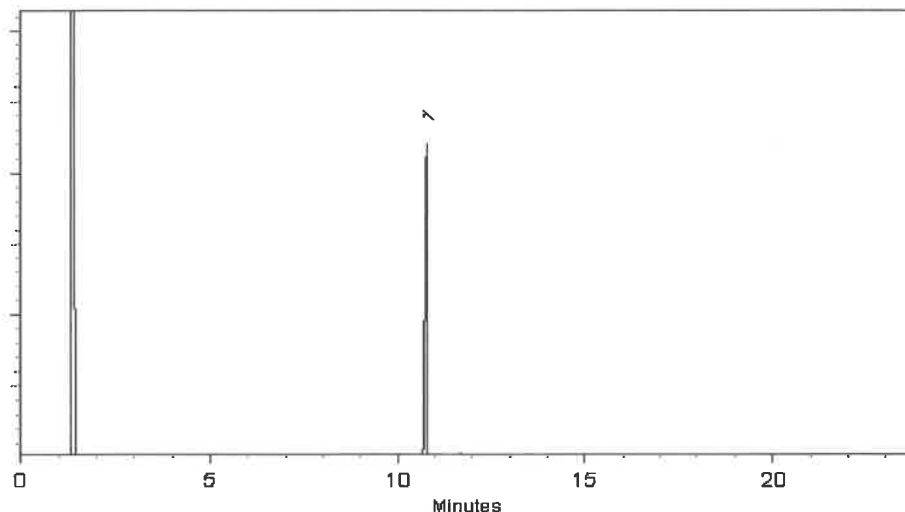

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler

Sam Moodler - Operations Tech I

Date Mixed: 08-May-2025

Balance Serial # 1128360905

Brittany Federinko

Brittany Federinko - Operations Tech II

Date Passed: 13-May-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31480 **Lot No.:** A0224278

Description : MA Fractionation Surrogate Spike Mix
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : March 31, 2031 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P14043 } AC
↓
P14058 } 6/10/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,018.5 µg/mL	+/- 181.0240
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,019.5 µg/mL	+/- 181.0691

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31480 **Lot No.:** A0221895
Description : MA Fractionation Surrogate Spike Mix
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : January 31, 2031 **Storage:** 10°C or colder
Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P14059
↓
P14062 } AC
6/10/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,032.5 µg/mL	+/- 181.6547
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,033.0 µg/mL	+/- 181.6772

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31480 **Lot No.:** A0221895
Description : MA Fractionation Surrogate Spike Mix
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : January 31, 2031 **Storage:** 10°C or colder
Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P14059
↓
P14062 } AC
6/10/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,032.5 µg/mL	+/- 181.6547
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,033.0 µg/mL	+/- 181.6772

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31480 **Lot No.:** A0221895
Description : MA Fractionation Surrogate Spike Mix
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : January 31, 2031 **Storage:** 10°C or colder
Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P14059
↓
P14062 } AC
6/10/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,032.5 µg/mL	+/- 181.6547
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,033.0 µg/mL	+/- 181.6772

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0225381

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : April 30, 2031 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P14074 } AC
↓
P14083 } 7/16/25.

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	200.3 µg/mL	+/- 9.0255
2	Naphthalene	91-20-3	STBL1057	99%	200.4 µg/mL	+/- 9.0294
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	214935V16F	97%	200.2 µg/mL	+/- 9.0208
5	Acenaphthene	83-32-9	MKCV8166	99%	200.0 µg/mL	+/- 9.0114
6	Fluorene	86-73-7	10246250	98%	200.3 µg/mL	+/- 9.0255
7	Phenanthrene	85-01-8	MKCV8193	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	101492T18R	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	A0458721	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCK2592	99%	200.8 µg/mL	+/- 9.0474
11	Benz(a)anthracene	56-55-3	I70012022BAA	99%	200.4 µg/mL	+/- 9.0294
12	Chrysene	218-01-9	RP250121RSR	99%	200.0 µg/mL	+/- 9.0114
13	Benzo(b)fluoranthene	205-99-2	022013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.4 µg/mL	+/- 9.0294
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383

17	Dibenz(a,h)anthracene	53-70-3	712061504-1-1	99%	200.4 µg/mL	+/- 9.0294
18	Benzo(g,h,i)perylene	191-24-2	RP250219RSR	99%	200.0 µg/mL	+/- 9.0114

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

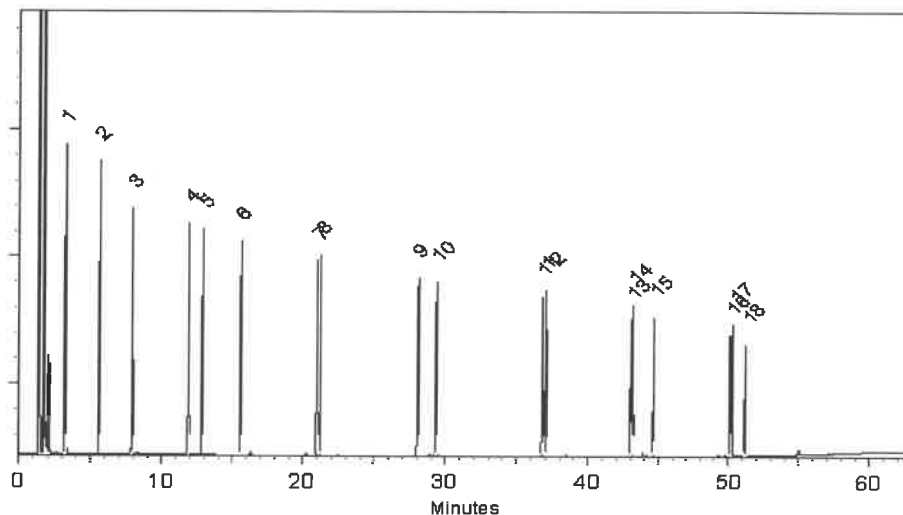

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Richard Zimmerman
Richard Zimmerman - Operations Tech I

Date Mixed: 06-May-2025 **Balance Serial #** 1128353505

Brittany Federinko
Brittany Federinko - Operations Tech II

Date Passed: 09-May-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0225381

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : April 30, 2031 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P14074 } AC
↓
P14083 } 7/16/25.

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	200.3 µg/mL	+/- 9.0255
2	Naphthalene	91-20-3	STBL1057	99%	200.4 µg/mL	+/- 9.0294
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	214935V16F	97%	200.2 µg/mL	+/- 9.0208
5	Acenaphthene	83-32-9	MKCV8166	99%	200.0 µg/mL	+/- 9.0114
6	Fluorene	86-73-7	10246250	98%	200.3 µg/mL	+/- 9.0255
7	Phenanthrene	85-01-8	MKCV8193	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	101492T18R	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	A0458721	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCK2592	99%	200.8 µg/mL	+/- 9.0474
11	Benz(a)anthracene	56-55-3	I70012022BAA	99%	200.4 µg/mL	+/- 9.0294
12	Chrysene	218-01-9	RP250121RSR	99%	200.0 µg/mL	+/- 9.0114
13	Benzo(b)fluoranthene	205-99-2	022013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.4 µg/mL	+/- 9.0294
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383

17	Dibenz(a,h)anthracene	53-70-3	712061504-1-1	99%	200.4 µg/mL	+/- 9.0294
18	Benzo(g,h,i)perylene	191-24-2	RP250219RSR	99%	200.0 µg/mL	+/- 9.0114

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

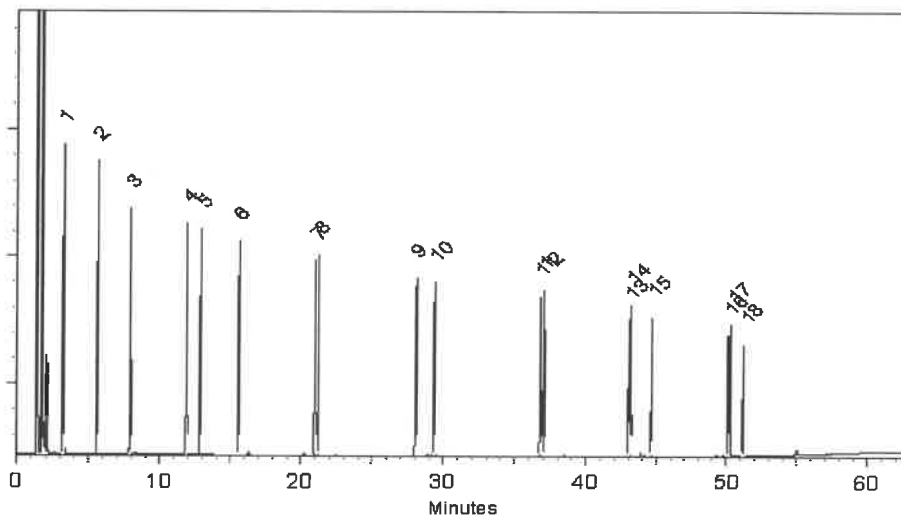

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Richard Zimmerman
Richard Zimmerman - Operations Tech I

Date Mixed: 06-May-2025 **Balance Serial #** 1128353505

Brittany Federinko
Brittany Federinko - Operations Tech II

Date Passed: 09-May-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0225381

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : April 30, 2031 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P14074 } AC
↓
P14083 } 7/16/25.

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	200.3 µg/mL	+/- 9.0255
2	Naphthalene	91-20-3	STBL1057	99%	200.4 µg/mL	+/- 9.0294
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	214935V16F	97%	200.2 µg/mL	+/- 9.0208
5	Acenaphthene	83-32-9	MKCV8166	99%	200.0 µg/mL	+/- 9.0114
6	Fluorene	86-73-7	10246250	98%	200.3 µg/mL	+/- 9.0255
7	Phenanthrene	85-01-8	MKCV8193	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	101492T18R	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	A0458721	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCK2592	99%	200.8 µg/mL	+/- 9.0474
11	Benz(a)anthracene	56-55-3	I70012022BAA	99%	200.4 µg/mL	+/- 9.0294
12	Chrysene	218-01-9	RP250121RSR	99%	200.0 µg/mL	+/- 9.0114
13	Benzo(b)fluoranthene	205-99-2	022013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.4 µg/mL	+/- 9.0294
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383

17	Dibenz(a,h)anthracene	53-70-3	712061504-1-1	99%	200.4 µg/mL	+/- 9.0294
18	Benzo(g,h,i)perylene	191-24-2	RP250219RSR	99%	200.0 µg/mL	+/- 9.0114

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

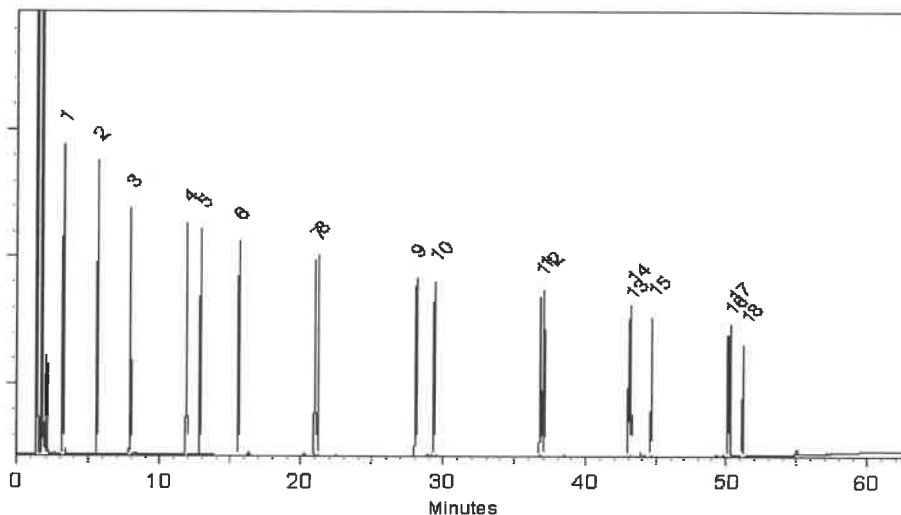

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Richard Zimmerman
Richard Zimmerman - Operations Tech I

Date Mixed: 06-May-2025 **Balance Serial #** 1128353505

Brittany Federinko
Brittany Federinko - Operations Tech II

Date Passed: 09-May-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0225381

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : April 30, 2031 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P14074 } AC
↓
P14083 } 7/16/25.

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	200.3 µg/mL	+/- 9.0255
2	Naphthalene	91-20-3	STBL1057	99%	200.4 µg/mL	+/- 9.0294
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	214935V16F	97%	200.2 µg/mL	+/- 9.0208
5	Acenaphthene	83-32-9	MKCV8166	99%	200.0 µg/mL	+/- 9.0114
6	Fluorene	86-73-7	10246250	98%	200.3 µg/mL	+/- 9.0255
7	Phenanthrene	85-01-8	MKCV8193	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	101492T18R	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	A0458721	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCK2592	99%	200.8 µg/mL	+/- 9.0474
11	Benz(a)anthracene	56-55-3	I70012022BAA	99%	200.4 µg/mL	+/- 9.0294
12	Chrysene	218-01-9	RP250121RSR	99%	200.0 µg/mL	+/- 9.0114
13	Benzo(b)fluoranthene	205-99-2	022013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.4 µg/mL	+/- 9.0294
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383

17	Dibenz(a,h)anthracene	53-70-3	712061504-1-1	99%	200.4 µg/mL	+/- 9.0294
18	Benzo(g,h,i)perylene	191-24-2	RP250219RSR	99%	200.0 µg/mL	+/- 9.0114

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

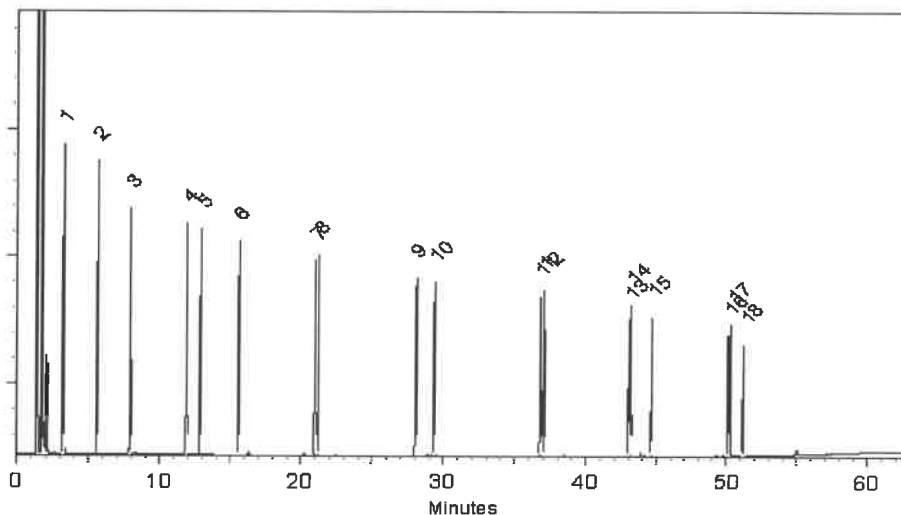

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Richard Zimmerman
Richard Zimmerman - Operations Tech I

Date Mixed: 06-May-2025 **Balance Serial #** 1128353505

Brittany Federinko
Brittany Federinko - Operations Tech II

Date Passed: 09-May-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0225381

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : April 30, 2031 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P14074 } AC
↓
P14083 } 7/16/25.

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	200.3 µg/mL	+/- 9.0255
2	Naphthalene	91-20-3	STBL1057	99%	200.4 µg/mL	+/- 9.0294
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	214935V16F	97%	200.2 µg/mL	+/- 9.0208
5	Acenaphthene	83-32-9	MKCV8166	99%	200.0 µg/mL	+/- 9.0114
6	Fluorene	86-73-7	10246250	98%	200.3 µg/mL	+/- 9.0255
7	Phenanthrene	85-01-8	MKCV8193	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	101492T18R	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	A0458721	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCK2592	99%	200.8 µg/mL	+/- 9.0474
11	Benz(a)anthracene	56-55-3	I70012022BAA	99%	200.4 µg/mL	+/- 9.0294
12	Chrysene	218-01-9	RP250121RSR	99%	200.0 µg/mL	+/- 9.0114
13	Benzo(b)fluoranthene	205-99-2	022013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.4 µg/mL	+/- 9.0294
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383

17	Dibenz(a,h)anthracene	53-70-3	712061504-1-1	99%	200.4 µg/mL	+/- 9.0294
18	Benzo(g,h,i)perylene	191-24-2	RP250219RSR	99%	200.0 µg/mL	+/- 9.0114

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

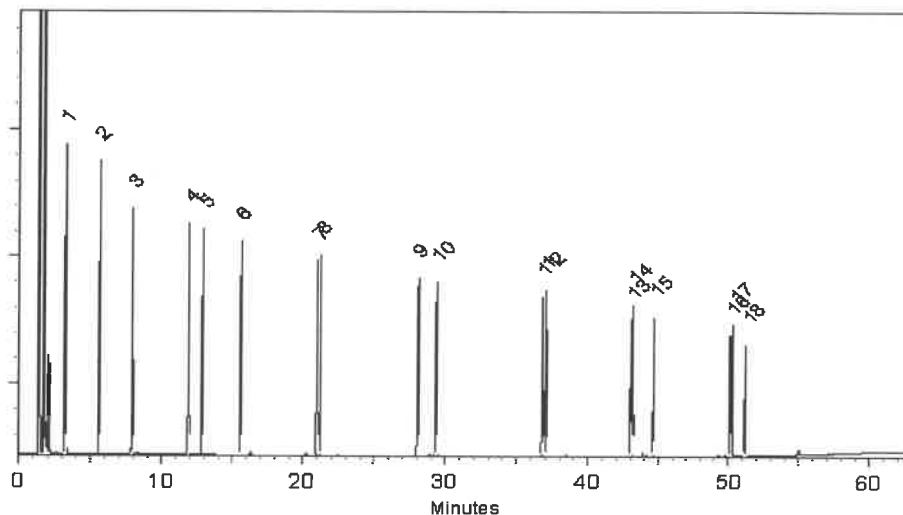

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Richard Zimmerman
Richard Zimmerman - Operations Tech I

Date Mixed: 06-May-2025 **Balance Serial #** 1128353505

Brittany Federinko
Brittany Federinko - Operations Tech II

Date Passed: 09-May-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0225381

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : April 30, 2031 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P14074 } AC
↓
P14083 } 7/16/25.

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	200.3 µg/mL	+/- 9.0255
2	Naphthalene	91-20-3	STBL1057	99%	200.4 µg/mL	+/- 9.0294
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	214935V16F	97%	200.2 µg/mL	+/- 9.0208
5	Acenaphthene	83-32-9	MKCV8166	99%	200.0 µg/mL	+/- 9.0114
6	Fluorene	86-73-7	10246250	98%	200.3 µg/mL	+/- 9.0255
7	Phenanthrene	85-01-8	MKCV8193	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	101492T18R	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	A0458721	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCK2592	99%	200.8 µg/mL	+/- 9.0474
11	Benz(a)anthracene	56-55-3	I70012022BAA	99%	200.4 µg/mL	+/- 9.0294
12	Chrysene	218-01-9	RP250121RSR	99%	200.0 µg/mL	+/- 9.0114
13	Benzo(b)fluoranthene	205-99-2	022013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.4 µg/mL	+/- 9.0294
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383

17	Dibenz(a,h)anthracene	53-70-3	712061504-1-1	99%	200.4 µg/mL	+/- 9.0294
18	Benzo(g,h,i)perylene	191-24-2	RP250219RSR	99%	200.0 µg/mL	+/- 9.0114

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

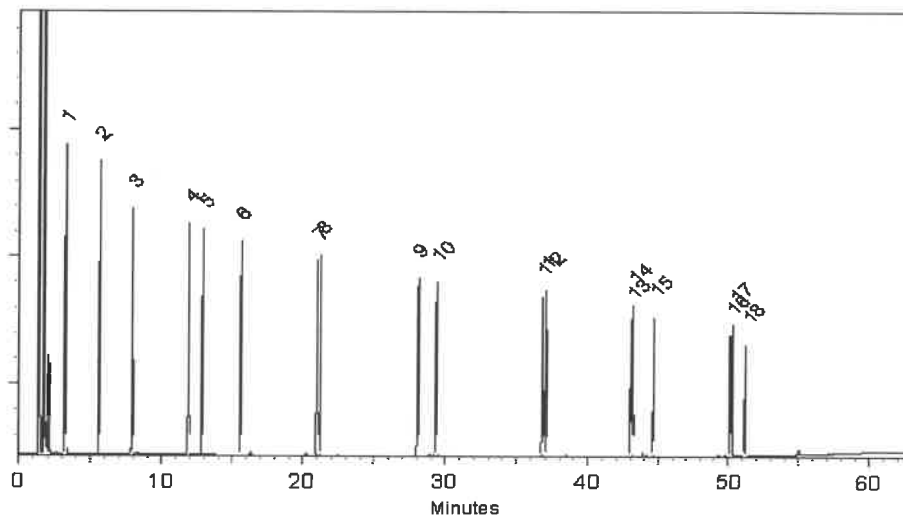

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Richard Zimmerman
Richard Zimmerman - Operations Tech I

Date Mixed: 06-May-2025 **Balance Serial #** 1128353505

Brittany Federinko
Brittany Federinko - Operations Tech II

Date Passed: 09-May-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0225381

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : April 30, 2031 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P14074 } AC
↓
P14083 } 7/16/25.

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	200.3 µg/mL	+/- 9.0255
2	Naphthalene	91-20-3	STBL1057	99%	200.4 µg/mL	+/- 9.0294
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	214935V16F	97%	200.2 µg/mL	+/- 9.0208
5	Acenaphthene	83-32-9	MKCV8166	99%	200.0 µg/mL	+/- 9.0114
6	Fluorene	86-73-7	10246250	98%	200.3 µg/mL	+/- 9.0255
7	Phenanthrene	85-01-8	MKCV8193	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	101492T18R	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	A0458721	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCK2592	99%	200.8 µg/mL	+/- 9.0474
11	Benz(a)anthracene	56-55-3	I70012022BAA	99%	200.4 µg/mL	+/- 9.0294
12	Chrysene	218-01-9	RP250121RSR	99%	200.0 µg/mL	+/- 9.0114
13	Benzo(b)fluoranthene	205-99-2	022013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.4 µg/mL	+/- 9.0294
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383

17	Dibenz(a,h)anthracene	53-70-3	712061504-1-1	99%	200.4 µg/mL	+/- 9.0294
18	Benzo(g,h,i)perylene	191-24-2	RP250219RSR	99%	200.0 µg/mL	+/- 9.0114

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

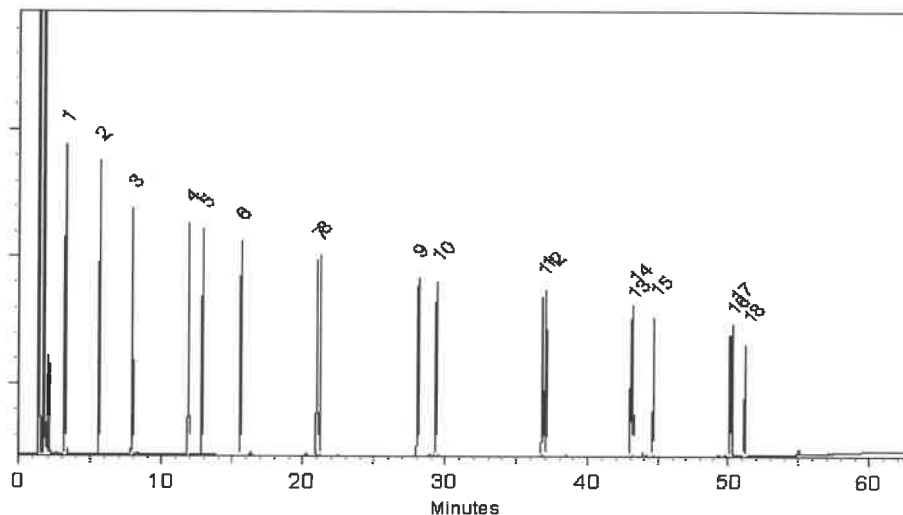

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Richard Zimmerman
Richard Zimmerman - Operations Tech I

Date Mixed: 06-May-2025 **Balance Serial #** 1128353505

Brittany Federinko
Brittany Federinko - Operations Tech II

Date Passed: 09-May-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0225381

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : April 30, 2031 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P14074 } AC
↓
P14083 } 7/16/25.

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	200.3 µg/mL	+/- 9.0255
2	Naphthalene	91-20-3	STBL1057	99%	200.4 µg/mL	+/- 9.0294
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	214935V16F	97%	200.2 µg/mL	+/- 9.0208
5	Acenaphthene	83-32-9	MKCV8166	99%	200.0 µg/mL	+/- 9.0114
6	Fluorene	86-73-7	10246250	98%	200.3 µg/mL	+/- 9.0255
7	Phenanthrene	85-01-8	MKCV8193	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	101492T18R	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	A0458721	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCK2592	99%	200.8 µg/mL	+/- 9.0474
11	Benz(a)anthracene	56-55-3	I70012022BAA	99%	200.4 µg/mL	+/- 9.0294
12	Chrysene	218-01-9	RP250121RSR	99%	200.0 µg/mL	+/- 9.0114
13	Benzo(b)fluoranthene	205-99-2	022013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.4 µg/mL	+/- 9.0294
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383

17	Dibenz(a,h)anthracene	53-70-3	712061504-1-1	99%	200.4 µg/mL	+/- 9.0294
18	Benzo(g,h,i)perylene	191-24-2	RP250219RSR	99%	200.0 µg/mL	+/- 9.0114

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

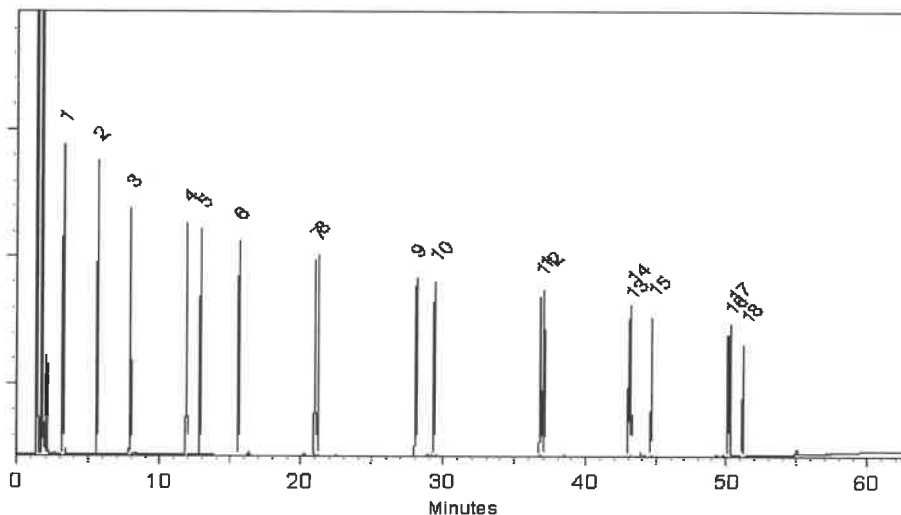

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Richard Zimmerman
Richard Zimmerman - Operations Tech I

Date Mixed: 06-May-2025 **Balance Serial #** 1128353505

Brittany Federinko
Brittany Federinko - Operations Tech II

Date Passed: 09-May-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0225381

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : April 30, 2031 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P14074 } AC
↓
P14083 } 7/16/25.

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	200.3 µg/mL	+/- 9.0255
2	Naphthalene	91-20-3	STBL1057	99%	200.4 µg/mL	+/- 9.0294
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	214935V16F	97%	200.2 µg/mL	+/- 9.0208
5	Acenaphthene	83-32-9	MKCV8166	99%	200.0 µg/mL	+/- 9.0114
6	Fluorene	86-73-7	10246250	98%	200.3 µg/mL	+/- 9.0255
7	Phenanthrene	85-01-8	MKCV8193	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	101492T18R	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	A0458721	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCK2592	99%	200.8 µg/mL	+/- 9.0474
11	Benz(a)anthracene	56-55-3	I70012022BAA	99%	200.4 µg/mL	+/- 9.0294
12	Chrysene	218-01-9	RP250121RSR	99%	200.0 µg/mL	+/- 9.0114
13	Benzo(b)fluoranthene	205-99-2	022013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.4 µg/mL	+/- 9.0294
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383

17	Dibenz(a,h)anthracene	53-70-3	712061504-1-1	99%	200.4 µg/mL	+/- 9.0294
18	Benzo(g,h,i)perylene	191-24-2	RP250219RSR	99%	200.0 µg/mL	+/- 9.0114

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

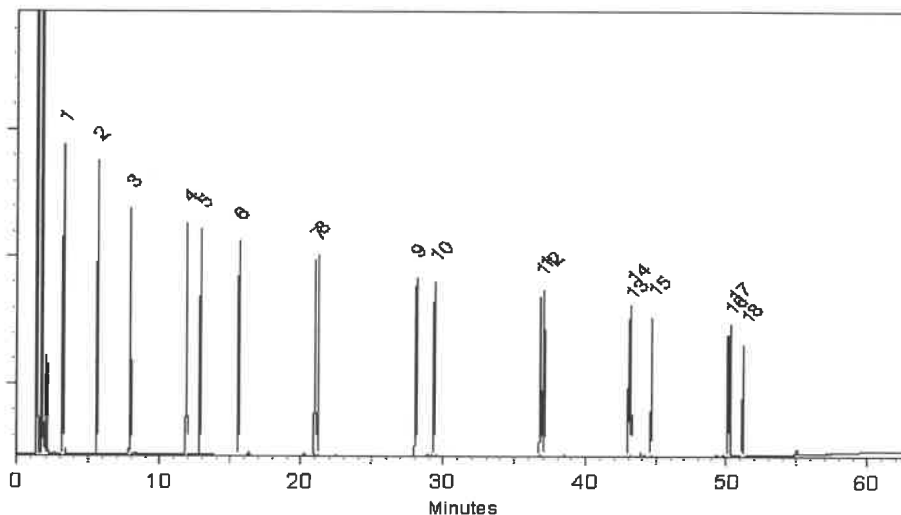

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Richard Zimmerman
Richard Zimmerman - Operations Tech I

Date Mixed: 06-May-2025 **Balance Serial #** 1128353505

Brittany Federinko
Brittany Federinko - Operations Tech II

Date Passed: 09-May-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0225381

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : April 30, 2031 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P14074 } AC
↓
P14083 } 7/16/25.

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	200.3 µg/mL	+/- 9.0255
2	Naphthalene	91-20-3	STBL1057	99%	200.4 µg/mL	+/- 9.0294
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	214935V16F	97%	200.2 µg/mL	+/- 9.0208
5	Acenaphthene	83-32-9	MKCV8166	99%	200.0 µg/mL	+/- 9.0114
6	Fluorene	86-73-7	10246250	98%	200.3 µg/mL	+/- 9.0255
7	Phenanthrene	85-01-8	MKCV8193	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	101492T18R	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	A0458721	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCK2592	99%	200.8 µg/mL	+/- 9.0474
11	Benz(a)anthracene	56-55-3	I70012022BAA	99%	200.4 µg/mL	+/- 9.0294
12	Chrysene	218-01-9	RP250121RSR	99%	200.0 µg/mL	+/- 9.0114
13	Benzo(b)fluoranthene	205-99-2	022013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.4 µg/mL	+/- 9.0294
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383

17	Dibenz(a,h)anthracene	53-70-3	712061504-1-1	99%	200.4 µg/mL	+/- 9.0294
18	Benzo(g,h,i)perylene	191-24-2	RP250219RSR	99%	200.0 µg/mL	+/- 9.0114

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

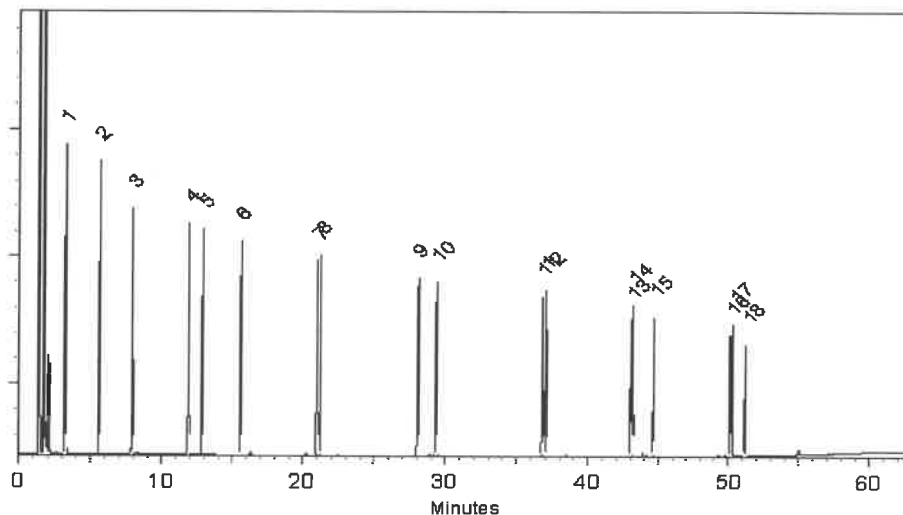

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Richard Zimmerman
Richard Zimmerman - Operations Tech I

Date Mixed: 06-May-2025 **Balance Serial #** 1128353505

Brittany Federinko
Brittany Federinko - Operations Tech II

Date Passed: 09-May-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0226411

Description : NJEPH Aliphatics Matrix Spike Mix
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : July 31, 2032 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P14094
↓
P14103 } AC
7/16/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.3 µg/mL	+/- 5.1753
2	n-Decane (C10)	124-18-5	SHBS1019	99%	200.3 µg/mL	+/- 5.1753
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.0 µg/mL	+/- 5.1667
4	n-Tetradecane (C14)	629-59-4	STBL2522	99%	200.0 µg/mL	+/- 5.1667
5	n-Hexadecane (C16)	544-76-3	SHBR0670	99%	200.0 µg/mL	+/- 5.1667
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.0 µg/mL	+/- 5.1667
7	n-Eicosane (C20)	112-95-8	MKCN8767	99%	200.0 µg/mL	+/- 5.1667
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.3 µg/mL	+/- 5.1753
9	n-Docosane (C22)	629-97-0	MKCQ3729	99%	200.0 µg/mL	+/- 5.1667
10	n-Tetracosane (C24)	646-31-1	UH5GN	99%	200.0 µg/mL	+/- 5.1667
11	n-Hexacosane (C26)	630-01-3	MKCV0107	99%	200.0 µg/mL	+/- 5.1667
12	n-Octacosane (C28)	630-02-4	BCCM2091	99%	200.0 µg/mL	+/- 5.1667
13	n-Triacontane (C30)	638-68-6	MKCW9459	99%	200.0 µg/mL	+/- 5.1667
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.0 µg/mL	+/- 5.1667
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.0 µg/mL	+/- 5.1667
16	n-Hexatriacontane (C36)	630-06-8	U30H007	99%	200.0 µg/mL	+/- 5.1667
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	200.0 µg/mL	+/- 5.1667

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

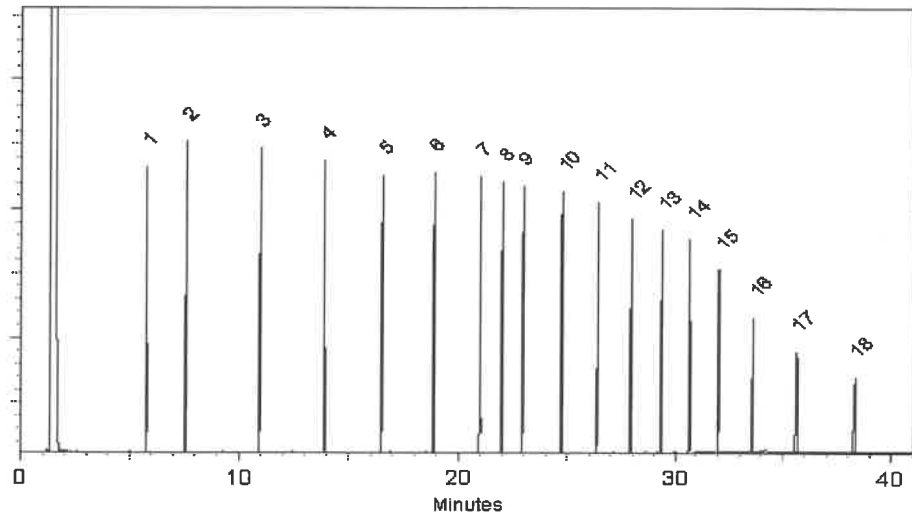

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

A.O.E.
Aaron Enyart - Operations Tech I

Date Mixed: 05-Jun-2025 **Balance Serial #** 1128353505

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-Jun-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0226411

Description : NJEPH Aliphatics Matrix Spike Mix
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : July 31, 2032 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P14094
↓
P14103 } AC
7/16/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.3 µg/mL	+/- 5.1753
2	n-Decane (C10)	124-18-5	SHBS1019	99%	200.3 µg/mL	+/- 5.1753
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.0 µg/mL	+/- 5.1667
4	n-Tetradecane (C14)	629-59-4	STBL2522	99%	200.0 µg/mL	+/- 5.1667
5	n-Hexadecane (C16)	544-76-3	SHBR0670	99%	200.0 µg/mL	+/- 5.1667
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.0 µg/mL	+/- 5.1667
7	n-Eicosane (C20)	112-95-8	MKCN8767	99%	200.0 µg/mL	+/- 5.1667
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.3 µg/mL	+/- 5.1753
9	n-Docosane (C22)	629-97-0	MKCQ3729	99%	200.0 µg/mL	+/- 5.1667
10	n-Tetracosane (C24)	646-31-1	UH5GN	99%	200.0 µg/mL	+/- 5.1667
11	n-Hexacosane (C26)	630-01-3	MKCV0107	99%	200.0 µg/mL	+/- 5.1667
12	n-Octacosane (C28)	630-02-4	BCCM2091	99%	200.0 µg/mL	+/- 5.1667
13	n-Triacontane (C30)	638-68-6	MKCW9459	99%	200.0 µg/mL	+/- 5.1667
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.0 µg/mL	+/- 5.1667
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.0 µg/mL	+/- 5.1667
16	n-Hexatriacontane (C36)	630-06-8	U30H007	99%	200.0 µg/mL	+/- 5.1667
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	200.0 µg/mL	+/- 5.1667

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

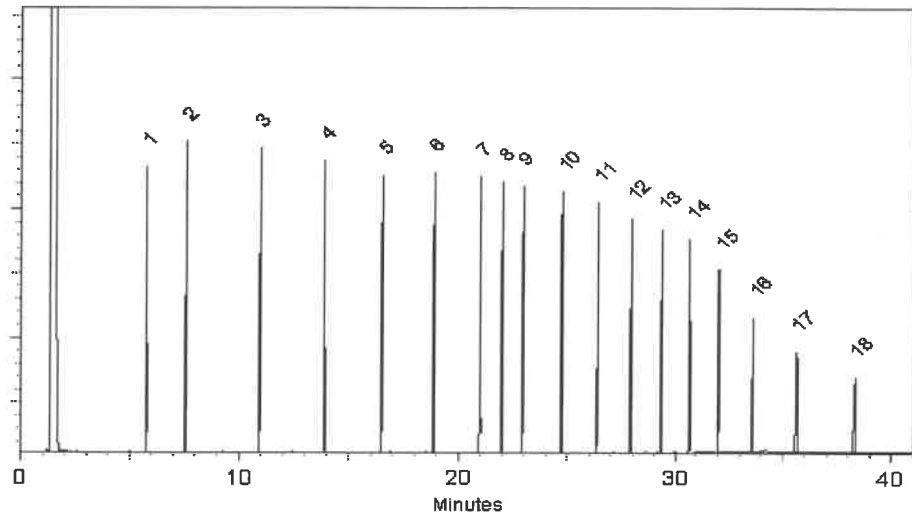

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

A.O.E.
Aaron Enyart - Operations Tech I

Date Mixed: 05-Jun-2025 **Balance Serial #** 1128353505

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-Jun-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0226411

Description : NJEPH Aliphatics Matrix Spike Mix
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : July 31, 2032 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P14094
↓
P14103 } AC
7/16/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.3 µg/mL	+/- 5.1753
2	n-Decane (C10)	124-18-5	SHBS1019	99%	200.3 µg/mL	+/- 5.1753
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.0 µg/mL	+/- 5.1667
4	n-Tetradecane (C14)	629-59-4	STBL2522	99%	200.0 µg/mL	+/- 5.1667
5	n-Hexadecane (C16)	544-76-3	SHBR0670	99%	200.0 µg/mL	+/- 5.1667
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.0 µg/mL	+/- 5.1667
7	n-Eicosane (C20)	112-95-8	MKCN8767	99%	200.0 µg/mL	+/- 5.1667
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.3 µg/mL	+/- 5.1753
9	n-Docosane (C22)	629-97-0	MKCQ3729	99%	200.0 µg/mL	+/- 5.1667
10	n-Tetracosane (C24)	646-31-1	UH5GN	99%	200.0 µg/mL	+/- 5.1667
11	n-Hexacosane (C26)	630-01-3	MKCV0107	99%	200.0 µg/mL	+/- 5.1667
12	n-Octacosane (C28)	630-02-4	BCCM2091	99%	200.0 µg/mL	+/- 5.1667
13	n-Triacontane (C30)	638-68-6	MKCW9459	99%	200.0 µg/mL	+/- 5.1667
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.0 µg/mL	+/- 5.1667
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.0 µg/mL	+/- 5.1667
16	n-Hexatriacontane (C36)	630-06-8	U30H007	99%	200.0 µg/mL	+/- 5.1667
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	200.0 µg/mL	+/- 5.1667

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

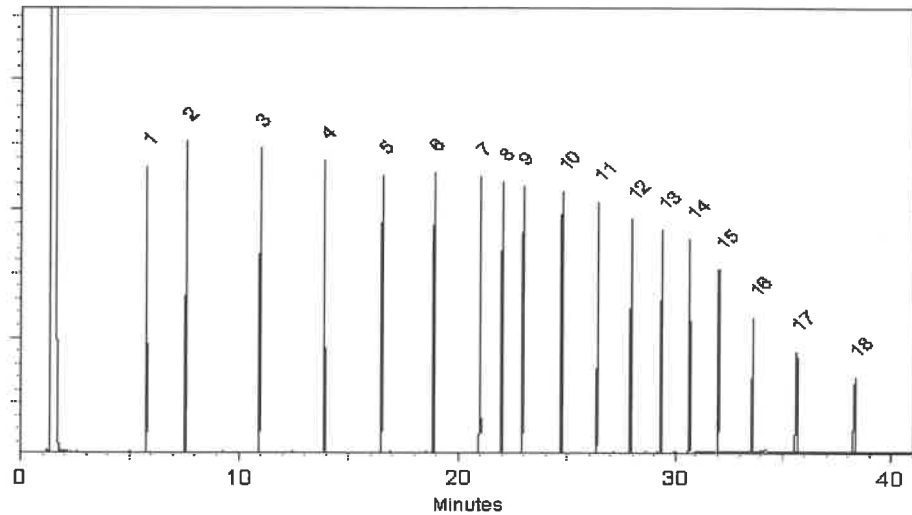

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

A.O.E.
Aaron Enyart - Operations Tech I

Date Mixed: 05-Jun-2025 **Balance Serial #** 1128353505

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-Jun-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0226411

Description : NJEPH Aliphatics Matrix Spike Mix
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : July 31, 2032 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P14094
↓
P14103 } AC
7/16/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.3 µg/mL	+/- 5.1753
2	n-Decane (C10)	124-18-5	SHBS1019	99%	200.3 µg/mL	+/- 5.1753
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.0 µg/mL	+/- 5.1667
4	n-Tetradecane (C14)	629-59-4	STBL2522	99%	200.0 µg/mL	+/- 5.1667
5	n-Hexadecane (C16)	544-76-3	SHBR0670	99%	200.0 µg/mL	+/- 5.1667
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.0 µg/mL	+/- 5.1667
7	n-Eicosane (C20)	112-95-8	MKCN8767	99%	200.0 µg/mL	+/- 5.1667
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.3 µg/mL	+/- 5.1753
9	n-Docosane (C22)	629-97-0	MKCQ3729	99%	200.0 µg/mL	+/- 5.1667
10	n-Tetracosane (C24)	646-31-1	UH5GN	99%	200.0 µg/mL	+/- 5.1667
11	n-Hexacosane (C26)	630-01-3	MKCV0107	99%	200.0 µg/mL	+/- 5.1667
12	n-Octacosane (C28)	630-02-4	BCCM2091	99%	200.0 µg/mL	+/- 5.1667
13	n-Triacontane (C30)	638-68-6	MKCW9459	99%	200.0 µg/mL	+/- 5.1667
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.0 µg/mL	+/- 5.1667
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.0 µg/mL	+/- 5.1667
16	n-Hexatriacontane (C36)	630-06-8	U30H007	99%	200.0 µg/mL	+/- 5.1667
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	200.0 µg/mL	+/- 5.1667

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

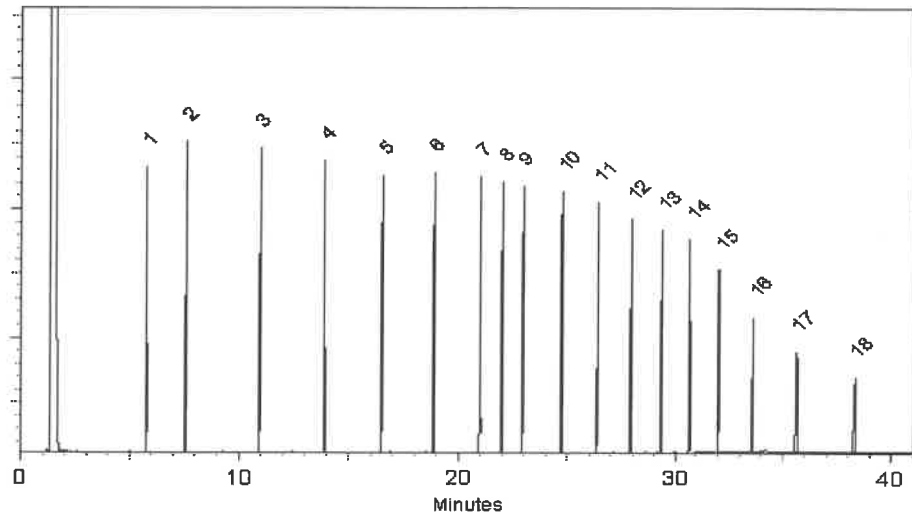

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

A.O.E.
Aaron Enyart - Operations Tech I

Date Mixed: 05-Jun-2025 **Balance Serial #** 1128353505

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-Jun-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0226411

Description : NJEPH Aliphatics Matrix Spike Mix
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : July 31, 2032 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P14094
↓
P14103 } AC
7/16/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.3 µg/mL	+/- 5.1753
2	n-Decane (C10)	124-18-5	SHBS1019	99%	200.3 µg/mL	+/- 5.1753
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.0 µg/mL	+/- 5.1667
4	n-Tetradecane (C14)	629-59-4	STBL2522	99%	200.0 µg/mL	+/- 5.1667
5	n-Hexadecane (C16)	544-76-3	SHBR0670	99%	200.0 µg/mL	+/- 5.1667
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.0 µg/mL	+/- 5.1667
7	n-Eicosane (C20)	112-95-8	MKCN8767	99%	200.0 µg/mL	+/- 5.1667
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.3 µg/mL	+/- 5.1753
9	n-Docosane (C22)	629-97-0	MKCQ3729	99%	200.0 µg/mL	+/- 5.1667
10	n-Tetracosane (C24)	646-31-1	UH5GN	99%	200.0 µg/mL	+/- 5.1667
11	n-Hexacosane (C26)	630-01-3	MKCV0107	99%	200.0 µg/mL	+/- 5.1667
12	n-Octacosane (C28)	630-02-4	BCCM2091	99%	200.0 µg/mL	+/- 5.1667
13	n-Triacontane (C30)	638-68-6	MKCW9459	99%	200.0 µg/mL	+/- 5.1667
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.0 µg/mL	+/- 5.1667
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.0 µg/mL	+/- 5.1667
16	n-Hexatriacontane (C36)	630-06-8	U30H007	99%	200.0 µg/mL	+/- 5.1667
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	200.0 µg/mL	+/- 5.1667

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

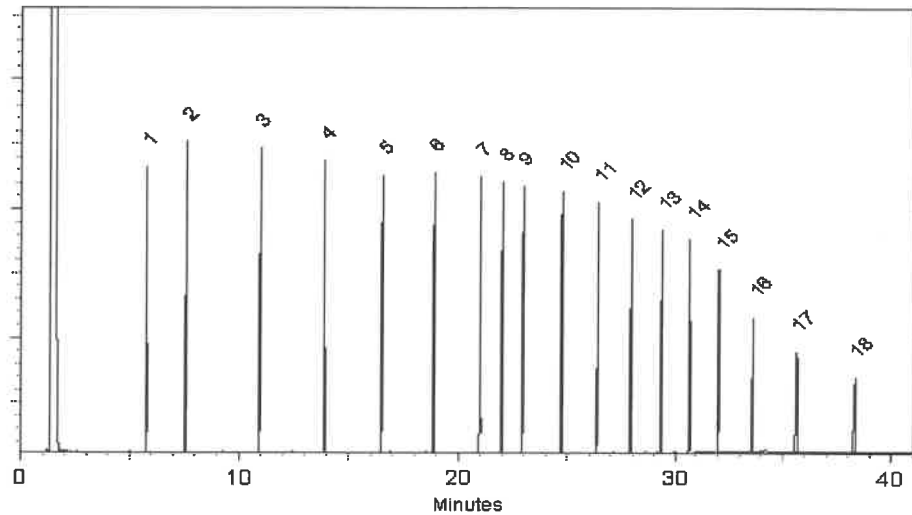

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

A.O.E.
Aaron Enyart - Operations Tech I

Date Mixed: 05-Jun-2025 **Balance Serial #** 1128353505

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-Jun-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0226411

Description : NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : July 31, 2032 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P14094
↓
P14103 } AC
7/16/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.3 µg/mL	+/- 5.1753
2	n-Decane (C10)	124-18-5	SHBS1019	99%	200.3 µg/mL	+/- 5.1753
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.0 µg/mL	+/- 5.1667
4	n-Tetradecane (C14)	629-59-4	STBL2522	99%	200.0 µg/mL	+/- 5.1667
5	n-Hexadecane (C16)	544-76-3	SHBR0670	99%	200.0 µg/mL	+/- 5.1667
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.0 µg/mL	+/- 5.1667
7	n-Eicosane (C20)	112-95-8	MKCN8767	99%	200.0 µg/mL	+/- 5.1667
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.3 µg/mL	+/- 5.1753
9	n-Docosane (C22)	629-97-0	MKCQ3729	99%	200.0 µg/mL	+/- 5.1667
10	n-Tetracosane (C24)	646-31-1	UH5GN	99%	200.0 µg/mL	+/- 5.1667
11	n-Hexacosane (C26)	630-01-3	MKCV0107	99%	200.0 µg/mL	+/- 5.1667
12	n-Octacosane (C28)	630-02-4	BCCM2091	99%	200.0 µg/mL	+/- 5.1667
13	n-Triacontane (C30)	638-68-6	MKCW9459	99%	200.0 µg/mL	+/- 5.1667
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.0 µg/mL	+/- 5.1667
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.0 µg/mL	+/- 5.1667
16	n-Hexatriacontane (C36)	630-06-8	U30H007	99%	200.0 µg/mL	+/- 5.1667
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	200.0 µg/mL	+/- 5.1667

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

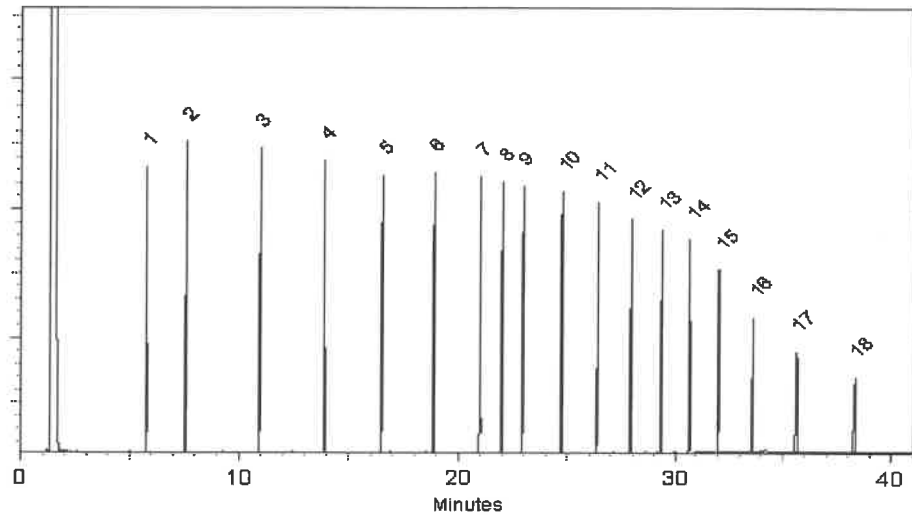

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

A.O.E.
Aaron Enyart - Operations Tech I

Date Mixed: 05-Jun-2025 **Balance Serial #** 1128353505

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-Jun-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0226411

Description : NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : July 31, 2032 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P14094
↓
P14103 } AC
7/16/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.3 µg/mL	+/- 5.1753
2	n-Decane (C10)	124-18-5	SHBS1019	99%	200.3 µg/mL	+/- 5.1753
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.0 µg/mL	+/- 5.1667
4	n-Tetradecane (C14)	629-59-4	STBL2522	99%	200.0 µg/mL	+/- 5.1667
5	n-Hexadecane (C16)	544-76-3	SHBR0670	99%	200.0 µg/mL	+/- 5.1667
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.0 µg/mL	+/- 5.1667
7	n-Eicosane (C20)	112-95-8	MKCN8767	99%	200.0 µg/mL	+/- 5.1667
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.3 µg/mL	+/- 5.1753
9	n-Docosane (C22)	629-97-0	MKCQ3729	99%	200.0 µg/mL	+/- 5.1667
10	n-Tetracosane (C24)	646-31-1	UH5GN	99%	200.0 µg/mL	+/- 5.1667
11	n-Hexacosane (C26)	630-01-3	MKCV0107	99%	200.0 µg/mL	+/- 5.1667
12	n-Octacosane (C28)	630-02-4	BCCM2091	99%	200.0 µg/mL	+/- 5.1667
13	n-Triacontane (C30)	638-68-6	MKCW9459	99%	200.0 µg/mL	+/- 5.1667
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.0 µg/mL	+/- 5.1667
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.0 µg/mL	+/- 5.1667
16	n-Hexatriacontane (C36)	630-06-8	U30H007	99%	200.0 µg/mL	+/- 5.1667
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	200.0 µg/mL	+/- 5.1667

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

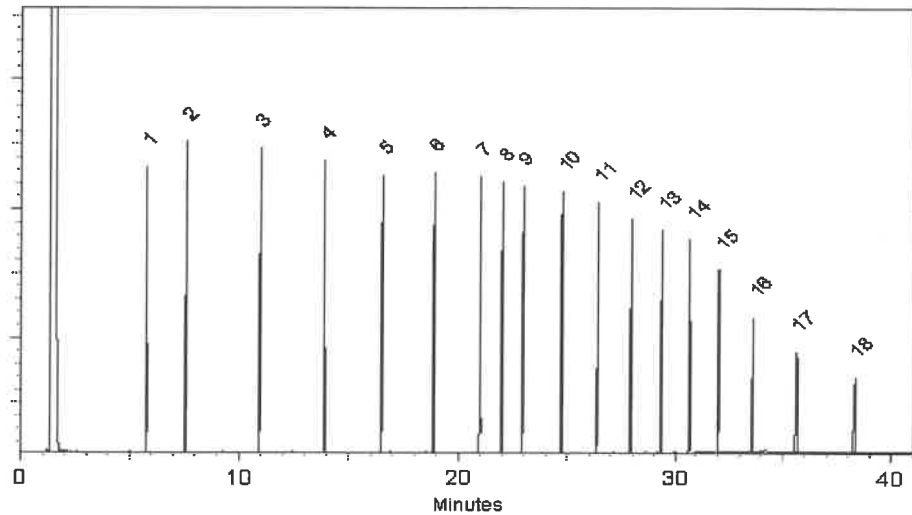

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

A.O.E.
Aaron Enyart - Operations Tech I

Date Mixed: 05-Jun-2025 Balance Serial # 1128353505

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-Jun-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0226411

Description : NJEPH Aliphatics Matrix Spike Mix
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : July 31, 2032 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P14094
↓
P14103 } AC
7/16/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.3 µg/mL	+/- 5.1753
2	n-Decane (C10)	124-18-5	SHBS1019	99%	200.3 µg/mL	+/- 5.1753
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.0 µg/mL	+/- 5.1667
4	n-Tetradecane (C14)	629-59-4	STBL2522	99%	200.0 µg/mL	+/- 5.1667
5	n-Hexadecane (C16)	544-76-3	SHBR0670	99%	200.0 µg/mL	+/- 5.1667
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.0 µg/mL	+/- 5.1667
7	n-Eicosane (C20)	112-95-8	MKCN8767	99%	200.0 µg/mL	+/- 5.1667
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.3 µg/mL	+/- 5.1753
9	n-Docosane (C22)	629-97-0	MKCQ3729	99%	200.0 µg/mL	+/- 5.1667
10	n-Tetracosane (C24)	646-31-1	UH5GN	99%	200.0 µg/mL	+/- 5.1667
11	n-Hexacosane (C26)	630-01-3	MKCV0107	99%	200.0 µg/mL	+/- 5.1667
12	n-Octacosane (C28)	630-02-4	BCCM2091	99%	200.0 µg/mL	+/- 5.1667
13	n-Triacontane (C30)	638-68-6	MKCW9459	99%	200.0 µg/mL	+/- 5.1667
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.0 µg/mL	+/- 5.1667
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.0 µg/mL	+/- 5.1667
16	n-Hexatriacontane (C36)	630-06-8	U30H007	99%	200.0 µg/mL	+/- 5.1667
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	200.0 µg/mL	+/- 5.1667

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

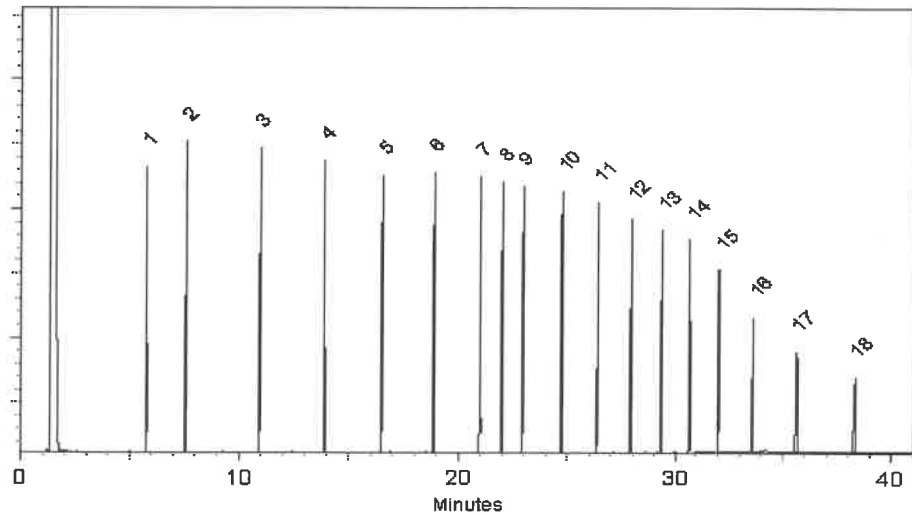

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

A.O.E.
Aaron Enyart - Operations Tech I

Date Mixed: 05-Jun-2025 **Balance Serial #** 1128353505

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-Jun-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0226411

Description : NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : July 31, 2032 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P14094
↓
P14103 } AC
7/16/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.3 µg/mL	+/- 5.1753
2	n-Decane (C10)	124-18-5	SHBS1019	99%	200.3 µg/mL	+/- 5.1753
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.0 µg/mL	+/- 5.1667
4	n-Tetradecane (C14)	629-59-4	STBL2522	99%	200.0 µg/mL	+/- 5.1667
5	n-Hexadecane (C16)	544-76-3	SHBR0670	99%	200.0 µg/mL	+/- 5.1667
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.0 µg/mL	+/- 5.1667
7	n-Eicosane (C20)	112-95-8	MKCN8767	99%	200.0 µg/mL	+/- 5.1667
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.3 µg/mL	+/- 5.1753
9	n-Docosane (C22)	629-97-0	MKCQ3729	99%	200.0 µg/mL	+/- 5.1667
10	n-Tetracosane (C24)	646-31-1	UH5GN	99%	200.0 µg/mL	+/- 5.1667
11	n-Hexacosane (C26)	630-01-3	MKCV0107	99%	200.0 µg/mL	+/- 5.1667
12	n-Octacosane (C28)	630-02-4	BCCM2091	99%	200.0 µg/mL	+/- 5.1667
13	n-Triacontane (C30)	638-68-6	MKCW9459	99%	200.0 µg/mL	+/- 5.1667
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.0 µg/mL	+/- 5.1667
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.0 µg/mL	+/- 5.1667
16	n-Hexatriacontane (C36)	630-06-8	U30H007	99%	200.0 µg/mL	+/- 5.1667
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	200.0 µg/mL	+/- 5.1667

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

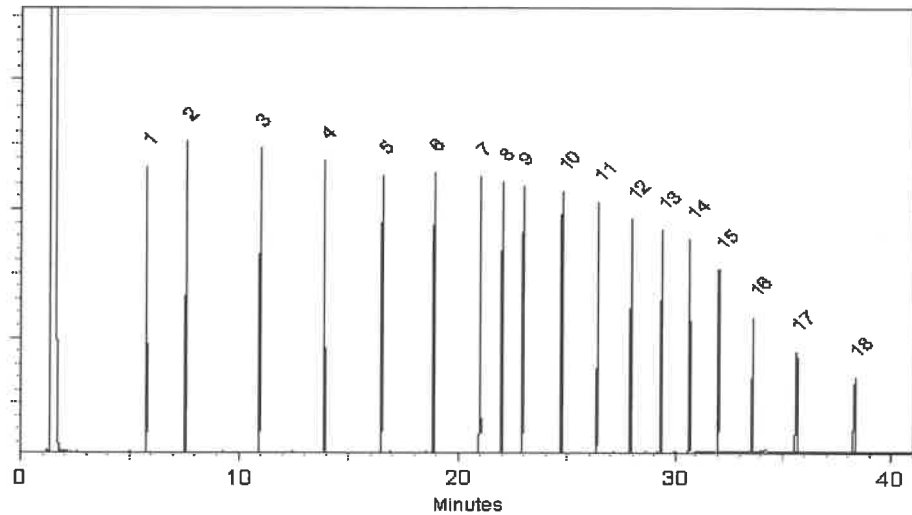

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

A.O.E.
Aaron Enyart - Operations Tech I

Date Mixed: 05-Jun-2025 **Balance Serial #** 1128353505

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-Jun-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0226411

Description : NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : July 31, 2032 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P14094
↓
P14103 } AC
7/16/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.3 µg/mL	+/- 5.1753
2	n-Decane (C10)	124-18-5	SHBS1019	99%	200.3 µg/mL	+/- 5.1753
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.0 µg/mL	+/- 5.1667
4	n-Tetradecane (C14)	629-59-4	STBL2522	99%	200.0 µg/mL	+/- 5.1667
5	n-Hexadecane (C16)	544-76-3	SHBR0670	99%	200.0 µg/mL	+/- 5.1667
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.0 µg/mL	+/- 5.1667
7	n-Eicosane (C20)	112-95-8	MKCN8767	99%	200.0 µg/mL	+/- 5.1667
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.3 µg/mL	+/- 5.1753
9	n-Docosane (C22)	629-97-0	MKCQ3729	99%	200.0 µg/mL	+/- 5.1667
10	n-Tetracosane (C24)	646-31-1	UH5GN	99%	200.0 µg/mL	+/- 5.1667
11	n-Hexacosane (C26)	630-01-3	MKCV0107	99%	200.0 µg/mL	+/- 5.1667
12	n-Octacosane (C28)	630-02-4	BCCM2091	99%	200.0 µg/mL	+/- 5.1667
13	n-Triacontane (C30)	638-68-6	MKCW9459	99%	200.0 µg/mL	+/- 5.1667
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.0 µg/mL	+/- 5.1667
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.0 µg/mL	+/- 5.1667
16	n-Hexatriacontane (C36)	630-06-8	U30H007	99%	200.0 µg/mL	+/- 5.1667
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	200.0 µg/mL	+/- 5.1667

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

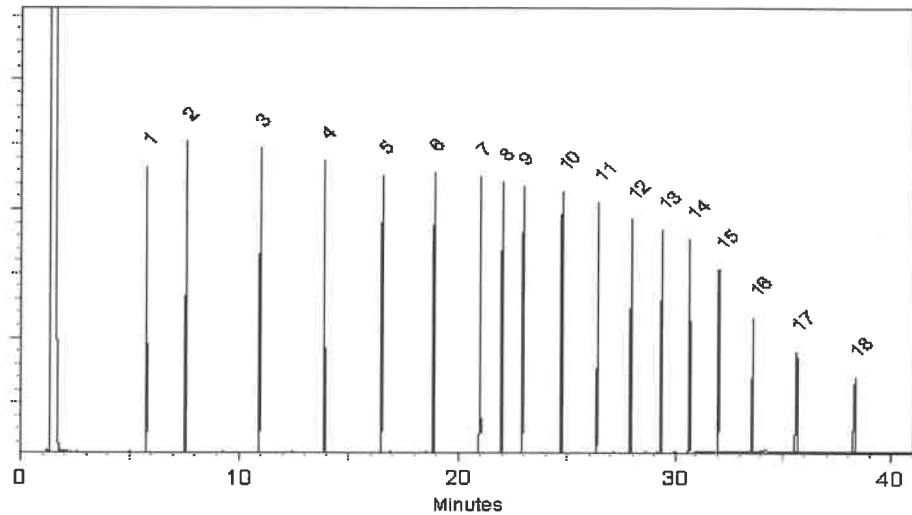

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

A.O.E.
Aaron Enyart - Operations Tech I

Date Mixed: 05-Jun-2025 **Balance Serial #** 1128353505

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-Jun-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis

 **avantor**™



Material No.: 9262-03

Batch No.: 25C0362005

Manufactured Date: 2025-01-29

Expiration Date: 2026-04-30

Revision No.: 0

W3234 JB
OP4421 07/28/2025

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	<= 10	6
ECD-Sensitive Impurities (as EthyleneDibromide) - Single Impurity Peak (ng/mL)	<= 5	5
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	>= 99.5 %	100.0 %
Assay (as n-Hexane) (by GC, corrected for water)	>= 95 %	100 %
Color (APHA)	<= 10	10
Residue after Evaporation	<= 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	<= 0.05 %	<0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC



Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC