

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following “ Results Qualifiers” are used:

Value	If the result is a value greater than or equal to the detection limit, report the value
U	Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. “10 U”. This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
ND	Indicates the analyte was analyzed for, but not detected
J	Indicates an estimated value. This flag is used: (1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.) (2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
B	Indicates the analyte was found in the blank as well as the sample report as “12 B”.
E	Indicates the analyte ‘s concentration exceeds the calibrated range of the instrument for that specific analysis.
D	This flag identifies all compounds identified in an analysis at a secondary dilution factor.
P	This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a “P”.
N	This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
A	This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
Q	Indicates the LCS did not meet the control limits requirements

LAB CHRONICLE

OrderID:	Q3277	OrderDate:	10/2/2025 3:50:00 PM
Client:	G Environmental	Project:	Newport
Contact:	Gary Landis	Location:	D31,VOA Ref. #2 Soil

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q3277-01	WC1	SOIL			09/30/25			10/02/25
			PCB	8082A		10/06/25	10/06/25	
			EPH_NF	NJEPH		10/03/25	10/04/25	



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Hit Summary Sheet
SW-846

SDG No.: Q3277

Order ID: Q3277

Client: G Environmental

Project ID: Newport

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units
-----------	-----------	--------	-----------	---------------	---	-----	-----	-------

Client ID :

Total Concentration: 0.000



QC SUMMARY

Surrogate Summary

SDG No.: Q3277

Client: G Environmental

Analytical Method: 8082A

Lab Sample ID	Client ID	Parameter	Column	Spike	Result	Recovery(%)	Qual	Limits(%)	
								Low	High
I.BLK-PO113719.D	PIBLK-PO113719.D	Tetrachloro-m-xyl	1	20	17.0	85		60	140
		Decachlorobiphen	1	20	17.3	86		60	140
		Tetrachloro-m-xyl	2	20	17.0	85		60	140
		Decachlorobiphen	2	20	18.1	91		60	140
I.BLK-PO114253.D	PIBLK-PO114253.D	Tetrachloro-m-xyl	1	20	18.2	91		60	140
		Decachlorobiphen	1	20	17.6	88		60	140
		Tetrachloro-m-xyl	2	20	17.7	89		60	140
		Decachlorobiphen	2	20	18.1	91		60	140
PB169987BL	PB169987BL	Tetrachloro-m-xyl	1	20	20.5	102		32	144
		Decachlorobiphen	1	20	20.3	102		32	175
		Tetrachloro-m-xyl	2	20	19.4	97		32	144
		Decachlorobiphen	2	20	19.6	98		32	175
PB169987BS	PB169987BS	Tetrachloro-m-xyl	1	20	19.7	99		32	144
		Decachlorobiphen	1	20	20.1	101		32	175
		Tetrachloro-m-xyl	2	20	18.5	92		32	144
		Decachlorobiphen	2	20	19.9	100		32	175
Q3277-01	WC1	Tetrachloro-m-xyl	1	20	24.4	122		32	144
		Decachlorobiphen	1	20	22.6	113		32	175
		Tetrachloro-m-xyl	2	20	22.9	115		32	144
		Decachlorobiphen	2	20	22.9	115		32	175
Q3288-01MS	TR-01-100325MS	Tetrachloro-m-xyl	1	20	12.9	65		32	144
		Decachlorobiphen	1	20	13.8	69		32	175
		Tetrachloro-m-xyl	2	20	13.6	68		32	144
		Decachlorobiphen	2	20	14.6	73		32	175
Q3288-01MSD	TR-01-100325MSD	Tetrachloro-m-xyl	1	20	13.3	67		32	144
		Decachlorobiphen	1	20	12.7	64		32	175
		Tetrachloro-m-xyl	2	20	14.1	70		32	144
		Decachlorobiphen	2	20	14.1	70		32	175
I.BLK-PO114268.D	PIBLK-PO114268.D	Tetrachloro-m-xyl	1	20	17.7	88		60	140
		Decachlorobiphen	1	20	14.6	73		60	140
		Tetrachloro-m-xyl	2	20	17.5	87		60	140
		Decachlorobiphen	2	20	16.1	81		60	140

Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.:	<u>Q3277</u>	Analytical Method:	<u>8082A</u>
Client:	<u>G Environmental</u>	DataFile :	<u>PO114259.D</u>

	Parameter	Spike	Sample Result	Result	Units	Rec	Rec Qual	RPD	RPD Qual	Low	Limits High	RPD
Lab Sample ID:	Q3288-01MS (Column 1)		Client Sample ID:	TR-01-100325MS								
	AR1016	179.2	0	143	ug/kg	80				55	146	
	AR1260	179.2	0	137	ug/kg	76				54	119	
Lab Sample ID:	Q3288-01MS (Column 2)		Client Sample ID:	TR-01-100325MS								
	AR1016	179.2	0	160	ug/kg	89				55	146	
	AR1260	179.2	0	141	ug/kg	79				54	119	

Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.:	<u>Q3277</u>	Analytical Method:	<u>8082A</u>
Client:	<u>G Environmental</u>	DataFile :	<u>PO114260.D</u>

		Sample				Rec		RPD		Limits			
	Parameter	Spike	Result	Result	Units	Rec	Qual	RPD	Qual	Low	High	RPD	
Lab Sample ID:	Q3288-01MSD	Client Sample ID:		TR-01-100325MSD									
	(Column 1)												
	AR1016			178.9	0	150	ug/kg	84		5		55	146
	AR1260	178.9	0	130	ug/kg	73		4		54	119	15	
Lab Sample ID:	Q3288-01MSD	Client Sample ID:		TR-01-100325MSD									
	(Column 2)												
	AR1016			178.9	0	158	ug/kg	88		1		55	146
	AR1260	178.9	0	135	ug/kg	75		5		54	119	15	

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.:	<u>Q3277</u>	Analytical Method:	<u>8082A</u>
Client:	<u>G Environmental</u>	Datafile :	<u>PO114255.D</u>

Lab Sample ID	Parameter	Spike	Result	Units	Rec	RPD	Qual	RPD	Low	Limits	RPD
								Qual		High	
PB169987BS (Column 1)	AR1016	166.5	180	ug/kg	108				71	120	
	AR1260	166.5	182	ug/kg	109				65	130	
PB169987BS (Column 2)	AR1016	166.5	167	ug/kg	100				71	120	
	AR1260	166.5	149	ug/kg	89				65	130	

4C

PESTICIDE METHOD BLANK SUMMARY

Client ID

PB169987BL

Lab Name: Alliance

Contract: GENV01

Lab Code: ACE

SDG NO.: Q3277

Lab Sample ID: PB169987BL

Lab File ID: PO114254.D

Matrix: (soil/water) Solid

Extraction: (Type) SOXH

Sulfur Cleanup: (Y/N) N

Date Extracted: 10/06/2025

Date Analyzed (1): 10/06/2025

Date Analyzed (2): 10/06/2025

Time Analyzed (1): 12:10

Time Analyzed (2): 12:10

Instrument ID (1): ECD_O

Instrument ID (2): ECD_O

GC Column (1): ZB-MR1 ID: 0.32 (mm)

GC Column (2): ZB-MR2 ID: 0.32 (mm)

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED 1	DATE ANALYZED 2
PB169987BS	PB169987BS	PO114255.D	10/06/2025	10/06/2025
WC1	Q3277-01	PO114257.D	10/06/2025	10/06/2025
TR-01-100325MS	Q3288-01MS	PO114259.D	10/06/2025	10/06/2025
TR-01-100325MSD	Q3288-01MSD	PO114260.D	10/06/2025	10/06/2025

COMMENTS: _____



SAMPLE DATA

Report of Analysis

Client:	G Environmental		Date Collected:	09/30/25	
Project:	Newport		Date Received:	10/02/25	
Client Sample ID:	WC1		SDG No.:	Q3277	
Lab Sample ID:	Q3277-01		Matrix:	SOIL	
Analytical Method:	8082A		% Solid:	97.6	Decanted:
Sample Wt/Vol:	30.09	Units: g	Final Vol:	10000	uL
Soil Aliquot Vol:		uL	Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	SW3541B				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO114257.D	1	10/06/25 08:43	10/06/25 13:05	PB169987

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	4.00	U	4.00	17.4	ug/kg
11104-28-2	Aroclor-1221	4.10	U	4.10	17.4	ug/kg
11141-16-5	Aroclor-1232	3.80	U	3.80	17.4	ug/kg
53469-21-9	Aroclor-1242	4.10	U	4.10	17.4	ug/kg
12672-29-6	Aroclor-1248	6.00	U	6.00	17.4	ug/kg
11097-69-1	Aroclor-1254	3.30	U	3.30	17.4	ug/kg
37324-23-5	Aroclor-1262	5.10	U	5.10	17.4	ug/kg
11100-14-4	Aroclor-1268	3.70	U	3.70	17.4	ug/kg
11096-82-5	Aroclor-1260	3.30	U	3.30	17.4	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	24.4		32 - 144	122%	SPK: 20
2051-24-3	Decachlorobiphenyl	22.9		32 - 175	115%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100625\
 Data File : PO114257.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2025 13:05
 Operator : YP/AJ
 Sample : Q3277-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WC1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 13:30:18 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:49:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.655	3.645	215.6E6	122.6E6	24.450	22.947
2) SA Decachlor...	8.659	8.603	151.5E6	47898100	22.648	22.942

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100625\
Data File : PO114257.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2025 13:05
Operator : YP/AJ
Sample : Q3277-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
WC1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 13:30:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

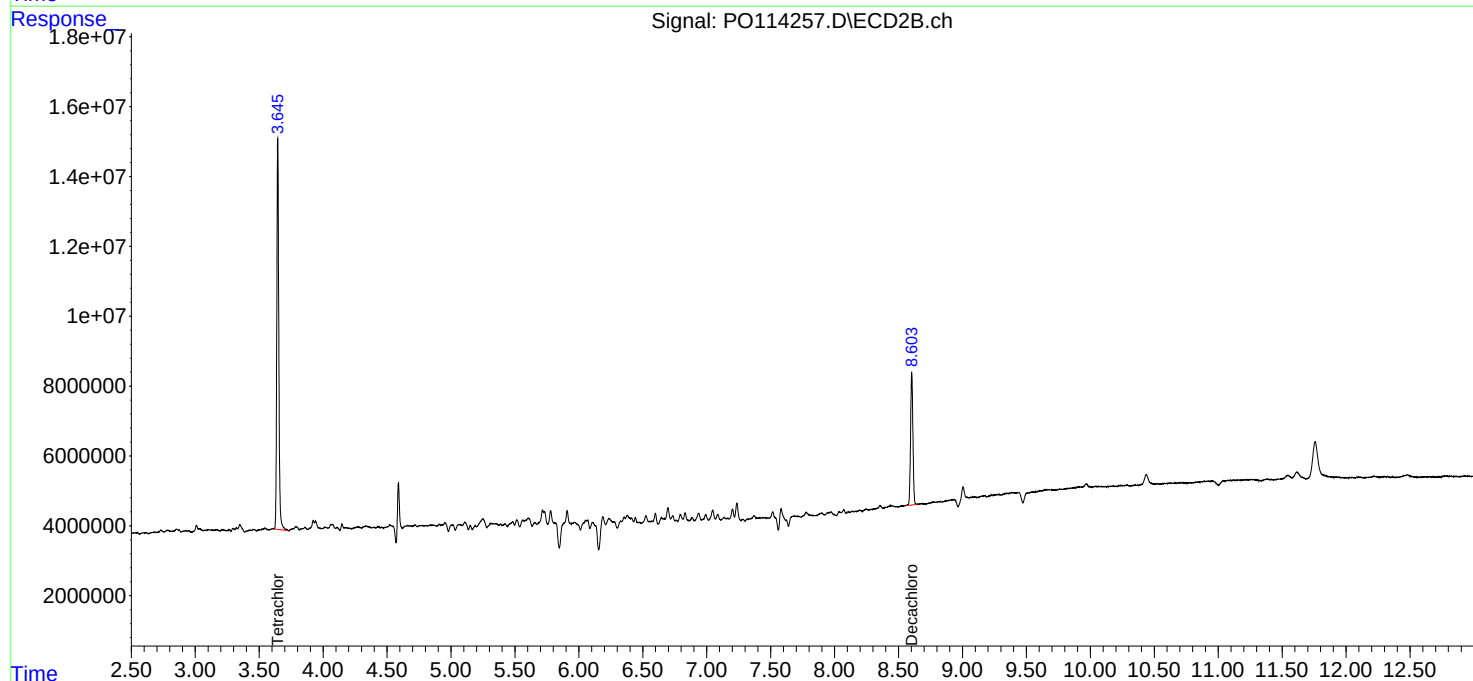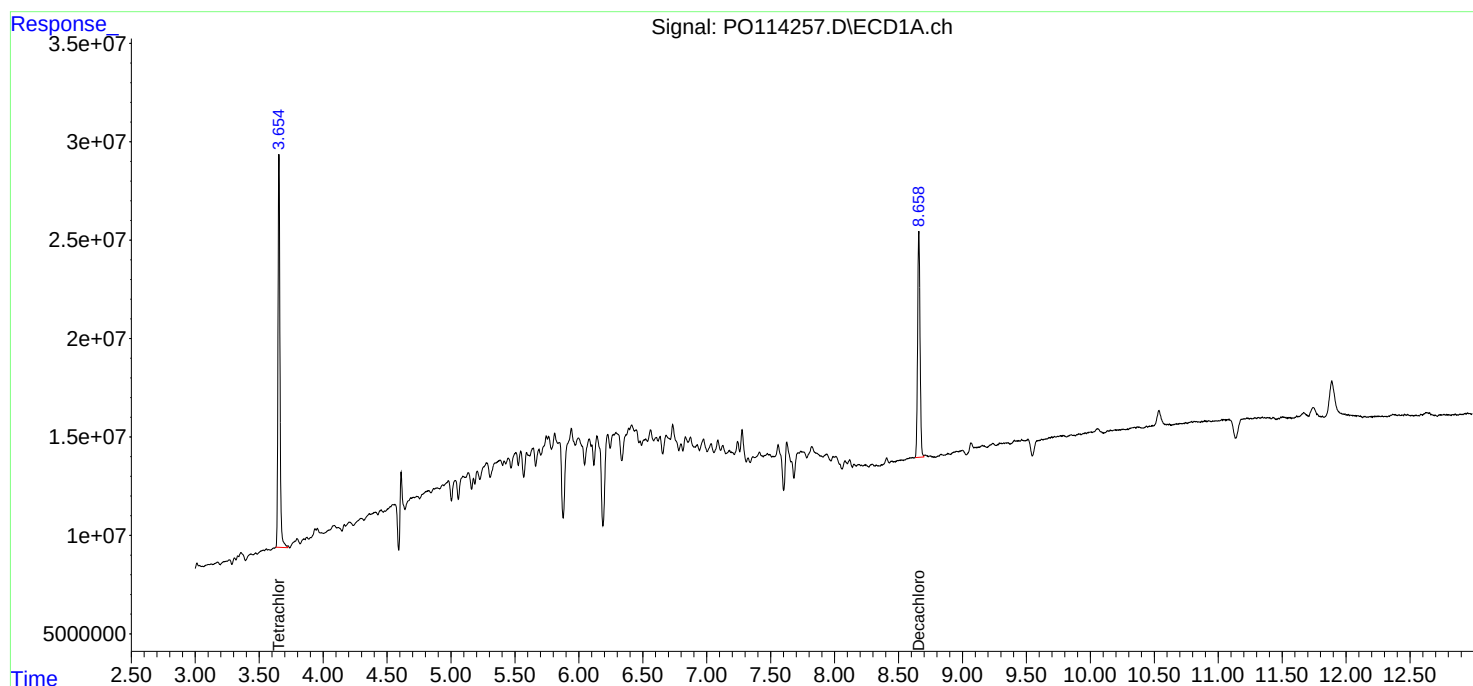


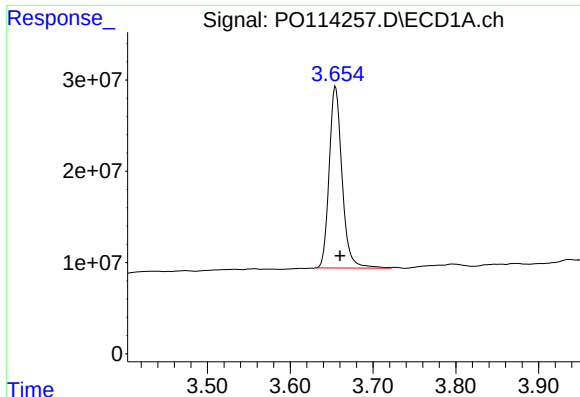

#1 Tetrachloro-m-xylene


R.T.: 3.655 min
Delta R.T.: -0.005 min
Response: 215643509
Conc: 24.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC1

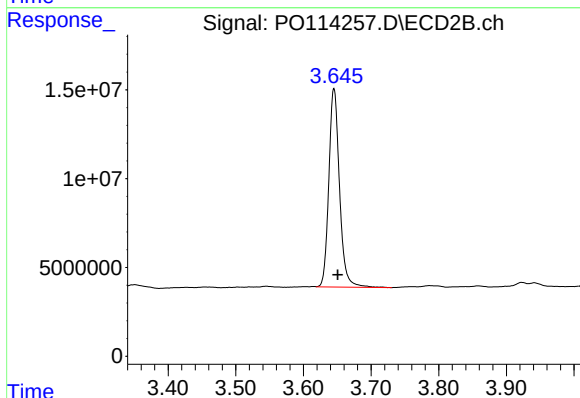


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: -0.006 min
Response: 122559183
Conc: 22.95 ng/ml

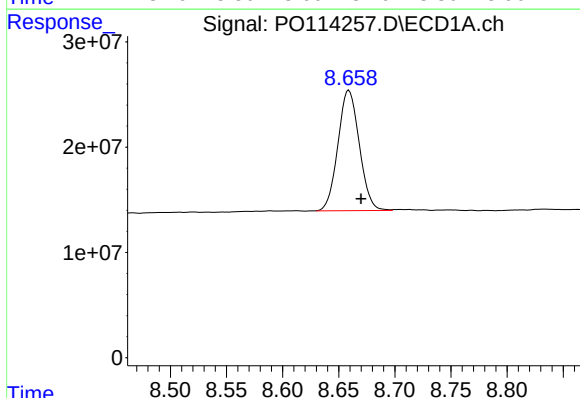

#2 Decachlorobiphenyl

R.T.: 8.659 min
Delta R.T.: -0.011 min
Response: 151523380
Conc: 22.65 ng/ml

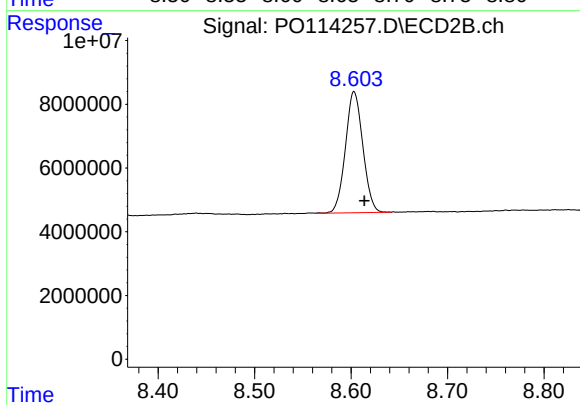

#2 Decachlorobiphenyl

R.T.: 8.603 min
Delta R.T.: -0.011 min
Response: 47898100
Conc: 22.94 ng/ml



CALIBRATION SUMMARY

Contract: **GENV01**

SDG NO.: Q3277

Calibration Date(s): **09/15/2025** **09/15/2025**

Calibration Times: 09:34 19:21

GC Column: ZB-MR1 ID: 0.32 (mm)

LAB FILE ID:		RT 1000 =	<u>PO113720.D</u>	RT 750 =	<u>PO113721.D</u>
RT 500 =	PO113722.D	RT 250 =	PO113723.D	RT 050 =	PO113724.D

[illegible]

[illegible]

Contract: **GENV01**

SDG NO.: Q3277

Calibration Date(s): **09/15/2025** **09/15/2025**

Calibration Times: 09:34 19:21

GC Column: ZB-MR2 ID: 0.32 (mm)

LAB FILE ID:		RT 1000 =	<u>PO113720.D</u>	RT 750 =	<u>PO113721.D</u>
RT 500 =	PO113722.D	RT 250 =	PO113723.D	RT 050 =	PO113724.D

[illegible]

[illegible]

CALIBRATION FACTOR OF INITIAL CALIBRATION

Lab Name: Alliance
Lab Code: ACE
Instrument ID: ECD_O

Contract: GENV01
SDG NO.: Q3277

Calibration Date(s): 09/15/2025 09/15/2025
Calibration Times: 09:34 19:21

GC Column: ZB-MR1 **ID:** 0.32 (mm)

LAB FILE ID:		CF 1000 =	PO113720.D	CF 750 =	PO113721.D			
CF 500 =		PO113722.D	CF 250 =	PO113723.D	CF 050 =	PO113724.D		
COMPOUND		CF 1000	CF 750	CF 500	CF 250	CF 050	CF	% RSD
Aroclor-1016-1	(1)	279831097	287472752	292257338	332268632	325738980	303513760	8
Aroclor-1016-2	(2)	419615441	429789385	439630440	492863176	493423100	455064308	8
Aroclor-1016-3	(3)	264606829	274358713	282734982	335166652	339181720	299209779	12
Aroclor-1016-4	(4)	220679515	227430096	236573942	251207960	266000940	240378491	8
Aroclor-1016-5	(5)	221161183	229729939	240498310	258108880	251005100	240100682	6
Aroclor-1260-1	(1)	451552761	471491176	474059886	507788164	546116300	490201657	8
Aroclor-1260-2	(2)	696304563	729550533	748950352	813407288	840985420	765839631	8
Aroclor-1260-3	(3)	574976216	607269133	635434940	723540836	822837840	672811793	15
Aroclor-1260-4	(4)	393925161	402138616	416474848	460301232	490840000	432735971	10
Aroclor-1260-5	(5)	1123652016	1096405636	1111782554	1193531308	1138663840	1132807071	3
Decachlorobiphenyl		6329905650	6344624080	6521704980	7067879800	7187292000	6690281302	6
Tetrachloro-m-xylene		8408389270	8593125013	8709615100	9391670440	8995637600	8819687485	4
Aroclor-1242-1	(1)	238599676	240720349	228247758	257159088	146270660	222199506	20
Aroclor-1242-2	(2)	362617467	360722704	342353350	393496496	221429160	336123835	20
Aroclor-1242-3	(3)	227891791	227998801	217213648	247566408	154288520	214991834	17
Aroclor-1242-4	(4)	185677557	186112447	176530238	202181048	124089440	174918146	17
Aroclor-1242-5	(5)	203750446	205780253	194932678	234457364	207956060	209375360	7
Decachlorobiphenyl		6625063440	6674671280	6788602460	7173491920	4387615000	6329888820	17
Tetrachloro-m-xylene		8568753780	8503816840	8003156340	9089751000	5283727200	7889841032	19
Aroclor-1248-1	(1)	175951880	180949771	185151304	187344088	171954220	180270253	4
Aroclor-1248-2	(2)	241204409	248355665	250410428	264222632	211901240	243218875	8
Aroclor-1248-3	(3)	311971277	319675973	325795004	350237008	314744160	324484684	5
Aroclor-1248-4	(4)	478786582	491838525	498712610	536762996	495510440	500322231	4
Aroclor-1248-5	(5)	326343326	337739332	340979574	367185960	318715000	338192638	5
Decachlorobiphenyl		6906923760	6991953907	7181732520	7612820120	5681727800	6875031621	10
Tetrachloro-m-xylene		8281619260	8465620507	8425382600	8733430400	6417874600	8064785473	12
Aroclor-1254-1	(1)	525265407	536188556	564134008	621264868	479241140	545218796	10
Aroclor-1254-2	(2)	478176368	488478569	519631638	583021712	472883720	508438401	9
Aroclor-1254-3	(3)	746637997	760372989	800603668	890308500	712603920	782105415	9
Aroclor-1254-4	(4)	554979056	565283144	587994066	646517864	379494280	546853682	18
Aroclor-1254-5	(5)	718134746	733343003	760419284	795296128	714490520	744336736	5
Decachlorobiphenyl		7203849800	7364098027	7605167340	8057726000	6076737800	7261515793	10
Tetrachloro-m-xylene		8326407670	8484622733	8619663240	9079782920	6520976600	8206290633	12
Aroclor-1268-1	(1)	1758947774	1709816927	1785772362	1945135008	1654311040	1770796622	6



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	1483041115	1450283463	1507897996	1638884712	1362761360	1488573729	7
Aroclor-1268-3	(3)	1211444046	1190914560	1240719650	1354691068	1116147840	1222783433	7
Aroclor-1268-4	(4)	446305248	439383757	459862146	499372456	429000100	454784741	6
Aroclor-1268-5	(5)	3222969842	3094367483	3187698556	3417074196	2682918220	3121005659	9
Decachlorobiphenyl		13813421760	13413455987	13885344600	15047923920	11999959200	13632021093	8
Tetrachloro-m-xylene		8650489570	8416864440	8733056840	9508670200	6744065200	8410629250	12



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Lab Name: Alliance
Lab Code: ACE
Instrument ID: ECD_O

Contract: GENV01
SDG NO.: Q3277

Calibration Date(s): 09/15/2025 09/15/2025
Calibration Times: 09:34 19:21

GC Column: ZB-MR2 ID: 0.32 (mm)

LAB FILE ID:		CF 1000 = <u>PO113720.D</u>		CF 750 = <u>PO113721.D</u>			
CF 500 = <u>PO113722.D</u>		CF 250 = <u>PO113723.D</u>		CF 050 = <u>PO113724.D</u>			
COMPOUND		CF 1000	CF 750	CF 500	CF 250	CF 050	% RSD
Aroclor-1016-1	(1)	161194959	167555515	172213236	197943584	212300180	12
Aroclor-1016-2	(2)	247660649	254215127	266109690	295452504	320788840	11
Aroclor-1016-3	(3)	132478875	137775607	144079418	158682380	173701980	11
Aroclor-1016-4	(4)	104213080	109199812	115770016	129547460	144816260	14
Aroclor-1016-5	(5)	131110272	137976827	144614834	165292304	171336360	12
Aroclor-1260-1	(1)	220737147	228186052	237294134	270069216	300160800	13
Aroclor-1260-2	(2)	290821079	295868247	313059866	353160924	400129960	14
Aroclor-1260-3	(3)	243248258	249887552	265854760	308918420	333877760	14
Aroclor-1260-4	(4)	166358067	173783024	182499490	209711196	223704380	13
Aroclor-1260-5	(5)	376721298	381888356	400424476	450051720	519309860	14
Decachlorobiphenyl		1971088000	1990798747	2046674720	2250657920	2179534400	6
Tetrachloro-m-xylene		5023699930	5127536973	5213659900	5649531080	5690644400	6
Aroclor-1242-1	(1)	140070279	141394544	137879020	161129568	101738300	16
Aroclor-1242-2	(2)	212507654	216303512	209728396	243981540	153746360	16
Aroclor-1242-3	(3)	114358137	116433633	116071012	134530132	98664540	11
Aroclor-1242-4	(4)	108951291	110656661	111486918	130110352	113781160	8
Aroclor-1242-5	(5)	137204941	140225116	141656710	164146076	126006440	10
Decachlorobiphenyl		2013236400	2036818507	2055399480	2187990440	1370225400	17
Tetrachloro-m-xylene		5081963720	5070567053	4816444880	5487100000	3160127800	19
Aroclor-1248-1	(1)	104656676	109107384	112539406	121726504	98599380	8
Aroclor-1248-2	(2)	146373463	152254041	158543364	175696640	155007980	7
Aroclor-1248-3	(3)	155110693	160619584	167536538	186260212	165045720	7
Aroclor-1248-4	(4)	182007971	188031200	194979064	215245372	191166620	7
Aroclor-1248-5	(5)	185591629	190752652	199422540	222580060	215555020	8
Decachlorobiphenyl		2031704490	2074468760	2119835620	2240995600	1660075400	11
Tetrachloro-m-xylene		4917523020	5005006120	5026178760	5438510280	4106940200	10
Aroclor-1254-1	(1)	279563251	289274152	304362018	339134132	299656300	7
Aroclor-1254-2	(2)	241241488	250685427	264723600	295034360	268710580	8
Aroclor-1254-3	(3)	370644030	380249351	395058822	433239944	357396100	8
Aroclor-1254-4	(4)	235623256	242545119	253069482	278102248	177620780	16
Aroclor-1254-5	(5)	290238808	298084172	311869266	340236600	294431680	7
Decachlorobiphenyl		2023494990	2074021307	2154035320	2293253640	1745979000	10
Tetrachloro-m-xylene		4906596160	4990801373	5101889120	5432554640	4242824600	9
Aroclor-1268-1	(1)	463812746	461069815	484852436	552413272	478530480	8



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	382551151	381395492	400241488	450975464	376701220	398372963	8
Aroclor-1268-3	(3)	309516041	307584487	322365468	361316928	330962760	326349137	7
Aroclor-1268-4	(4)	126169269	122567489	128850366	141798540	114523000	126781733	8
Aroclor-1268-5	(5)	880606144	856364473	894951184	981182000	782994000	879219560	8
Decachlorobiphenyl		3812230710	3735660987	3912512580	4347451840	3518286000	3865228423	8
Tetrachloro-m-xylene		5092073170	4970547720	5151696080	5694720080	4205757800	5022958970	11



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Lab Name: Alliance Contract: GENV01

Lab Code: ACE SDG NO.: Q3277

Instrument ID: ECD_O Date(s) Analyzed: 09/15/2025 09/15/2025

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	3.87	3.77	3.97	96855600
		2	3.96	3.86	4.06	71896200
		3	4.03	3.93	4.13	236858000
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.03	3.93	4.13	175075000
		2	4.52	4.42	4.62	95953000
		3	4.76	4.66	4.86	197025000
		4	4.94	4.84	5.04	98735000
		5	4.98	4.88	5.08	65259600
Aroclor-1262	500	1	6.78	6.68	6.88	992416000
		2	7.29	7.19	7.39	1584210000
		3	7.57	7.47	7.67	559174000
		4	7.63	7.53	7.73	1000210000
		5	8.13	8.03	8.23	399122000



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Lab Name: Alliance **Contract:** GENV01
Lab Code: ACE **SDG NO.:** Q3277
Instrument ID: ECD_O **Date(s) Analyzed:** 09/15/2025 09/15/2025
GC Column: ZB-MR2 **ID:** 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	3.86	3.76	3.96	67679000
		2	3.94	3.84	4.04	50962200
		3	4.02	3.92	4.12	156597000
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.02	3.92	4.12	118402000
		2	4.74	4.64	4.84	122831000
		3	4.91	4.81	5.01	66545800
		4	5.00	4.90	5.10	58641000
		5	5.17	5.07	5.27	61534600
Aroclor-1262	500	1	6.75	6.65	6.85	366152000
		2	7.25	7.15	7.35	456612000
		3	7.53	7.43	7.63	174199000
		4	7.59	7.49	7.69	278024000
		5	8.08	7.98	8.18	113685000

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113720.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 09:34
 Operator : YP/AJ
 Sample : AR1660ICC1000
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 11:09:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 15 11:05:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.651	840.8E6	502.4E6	98.240	98.144
2) SA Decachlor...	8.670	8.614	633.0E6	197.1E6	98.508	98.119
Target Compounds						
3) L1 AR-1016-1	4.742	4.723	279.8E6	161.2E6	978.279	966.953
4) L1 AR-1016-2	4.760	4.740	419.6E6	247.7E6	976.706	964.091
5) L1 AR-1016-3	4.818	4.915	264.6E6	132.5E6	966.880	958.054
6) L1 AR-1016-4	4.937	4.958	220.7E6	104.2E6	965.239	947.464
7) L1 AR-1016-5	5.193	5.170	221.2E6	131.1E6	958.114	951.022
31) L7 AR-1260-1	6.228	6.196	451.6E6	220.7E6	975.684	963.852
32) L7 AR-1260-2	6.418	6.384	696.3E6	290.8E6	963.573	963.174
33) L7 AR-1260-3	6.783	6.535	575.0E6	243.2E6	950.051	955.595
34) L7 AR-1260-4	7.041	7.003	393.9E6	166.4E6	972.175	953.731
35) L7 AR-1260-5	7.285	7.246	1123.7E6	376.7E6	1005.310	969.500



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113720.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 09:34
Operator : YP/AJ
Sample : AR1660ICC1000
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 11:09:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 15 11:05:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

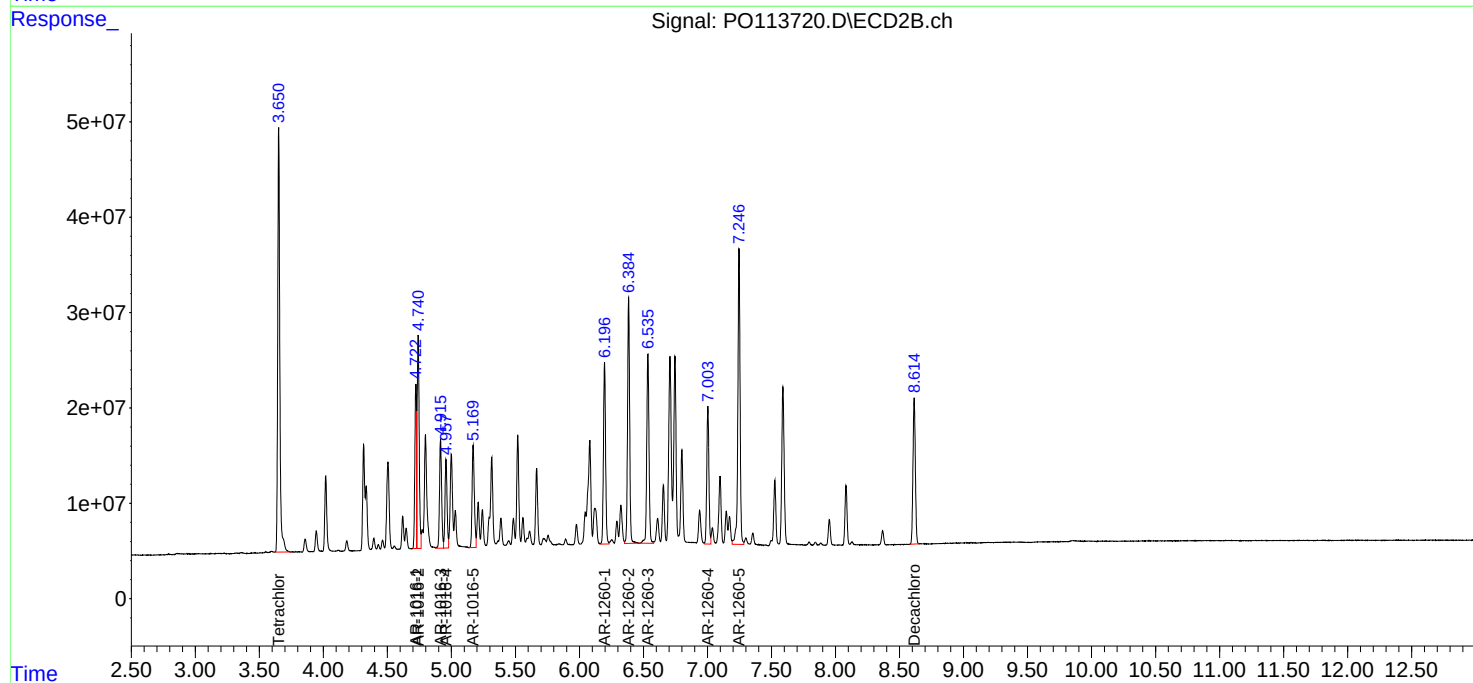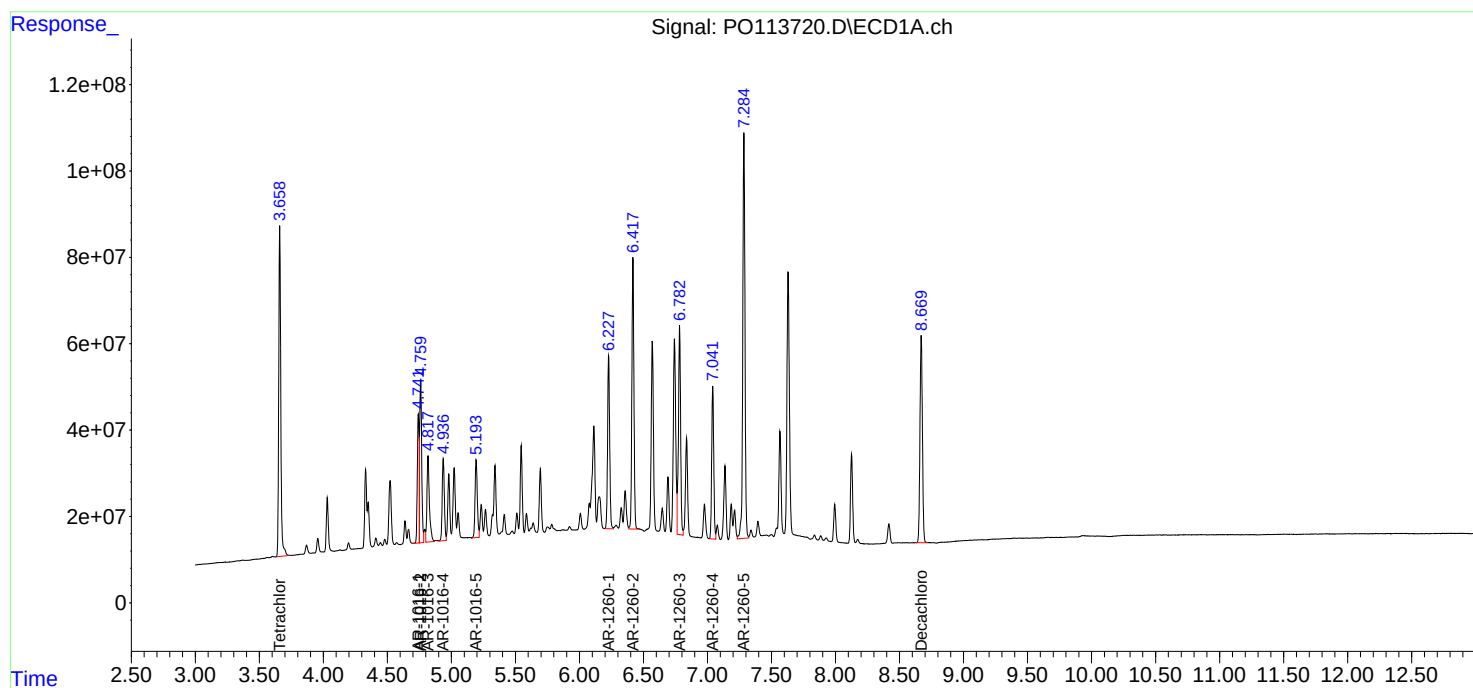

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113721.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 09:53
 Operator : YP/AJ
 Sample : AR1660ICC750
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 11:11:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 15 11:05:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.660	3.651	644.5E6	384.6E6	75.199	75.086
2)	SA Decachlor...	8.670	8.615	475.8E6	149.3E6	74.366	74.549
Target Compounds							
3)	L1 AR-1016-1	4.743	4.723	215.6E6	125.7E6	752.493	752.549
4)	L1 AR-1016-2	4.761	4.740	322.3E6	190.7E6	750.194	744.785
5)	L1 AR-1016-3	4.818	4.915	205.8E6	103.3E6	751.256	748.177
6)	L1 AR-1016-4	4.937	4.958	170.6E6	81899859	747.378	746.392
7)	L1 AR-1016-5	5.193	5.170	172.3E6	103.5E6	747.614	750.414
31)	L7 AR-1260-1	6.229	6.196	353.6E6	171.1E6	759.324	748.187
32)	L7 AR-1260-2	6.418	6.384	547.2E6	221.9E6	754.775	739.877
33)	L7 AR-1260-3	6.783	6.535	455.5E6	187.4E6	751.703	740.783
34)	L7 AR-1260-4	7.042	7.003	301.6E6	130.3E6	746.213	748.147
35)	L7 AR-1260-5	7.286	7.246	822.3E6	286.4E6	740.405	741.349



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113721.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 09:53
Operator : YP/AJ
Sample : AR1660ICC750
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 11:11:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 15 11:05:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

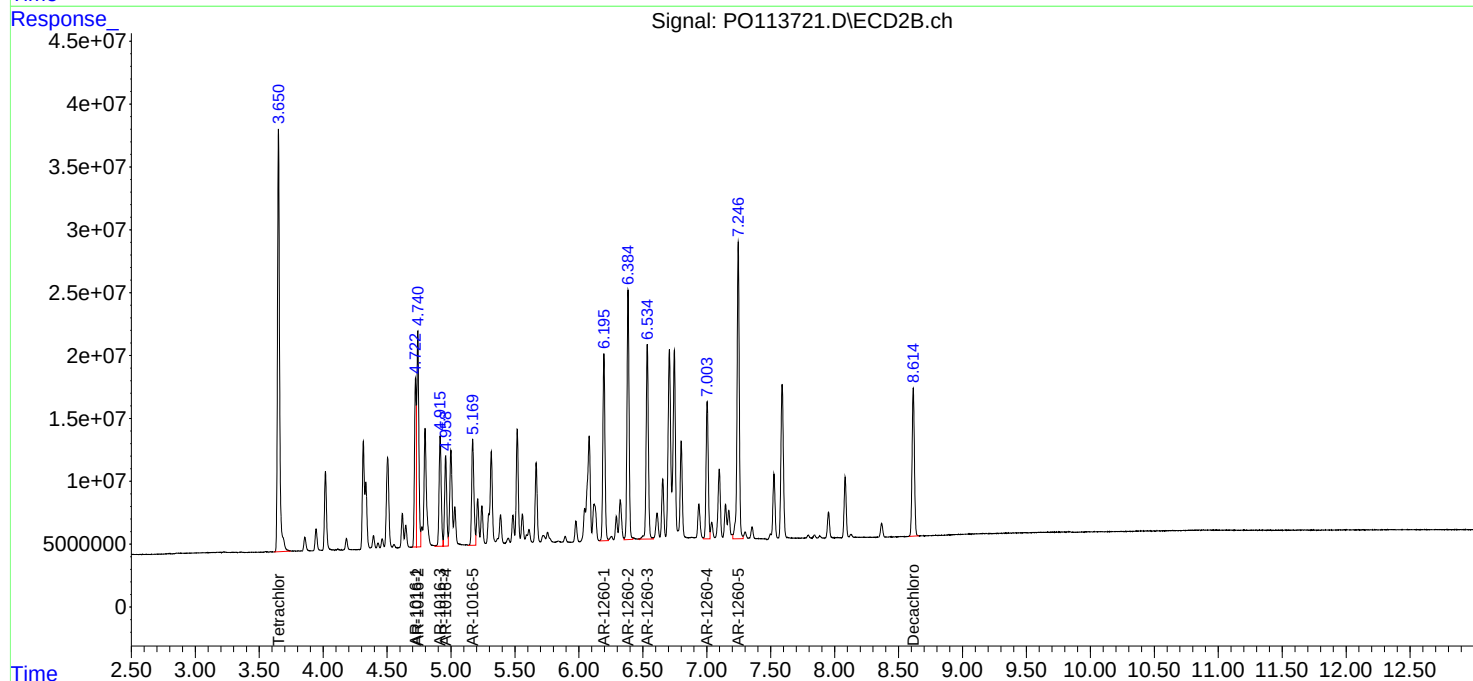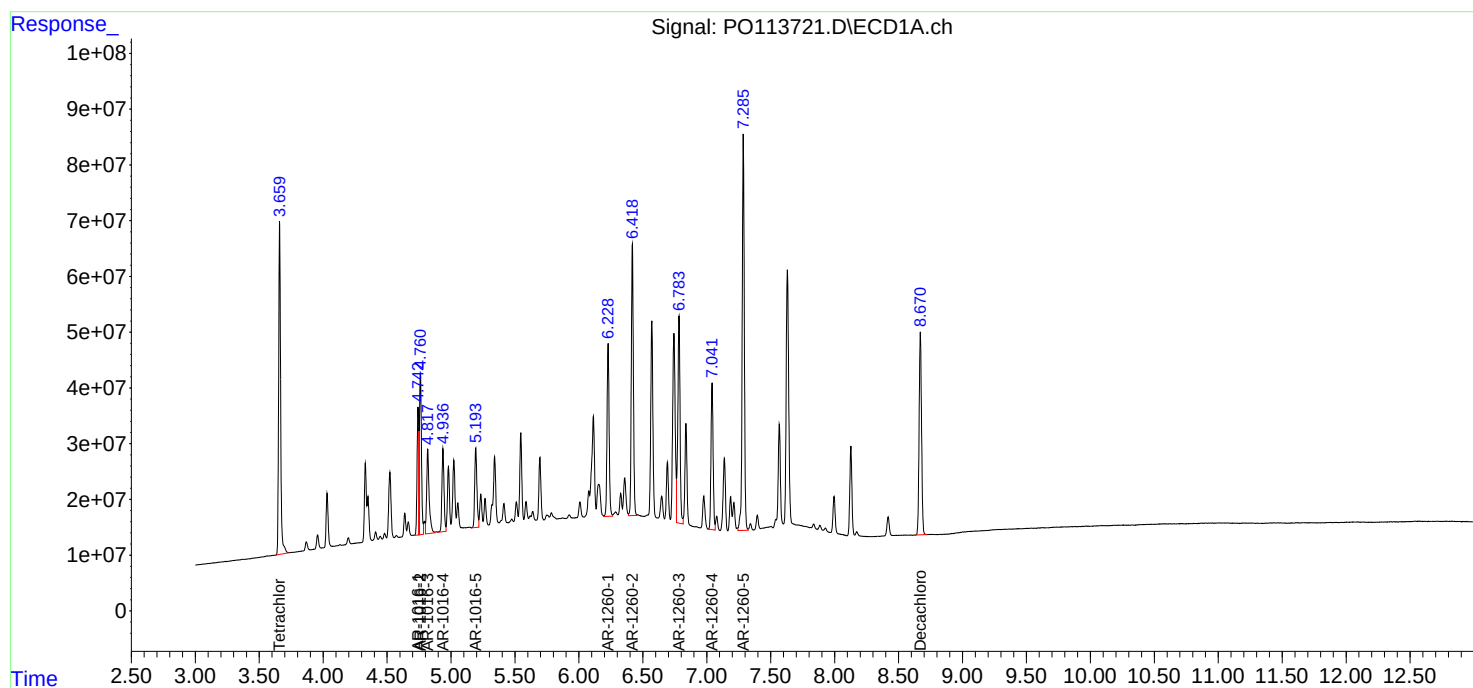

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113722.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 10:11
 Operator : YP/AJ
 Sample : AR1660ICC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 11:05:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 15 11:05:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.660	3.651	435.5E6	260.7E6	50.000	50.000
2) SA Decachlor...	8.670	8.614	326.1E6	102.3E6	50.000	50.000
Target Compounds						
3) L1 AR-1016-1	4.743	4.723	146.1E6	86106618	500.000	500.000
4) L1 AR-1016-2	4.761	4.741	219.8E6	133.1E6	500.000	500.000
5) L1 AR-1016-3	4.818	4.916	141.4E6	72039709	500.000	500.000
6) L1 AR-1016-4	4.937	4.958	118.3E6	57885008	500.000	500.000
7) L1 AR-1016-5	5.193	5.170	120.2E6	72307417	500.000	500.000
31) L7 AR-1260-1	6.229	6.196	237.0E6	118.6E6	500.000	500.000
32) L7 AR-1260-2	6.419	6.384	374.5E6	156.5E6	500.000	500.000
33) L7 AR-1260-3	6.783	6.535	317.7E6	132.9E6	500.000	500.000
34) L7 AR-1260-4	7.041	7.003	208.2E6	91249745	500.000	500.000
35) L7 AR-1260-5	7.285	7.246	555.9E6	200.2E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113722.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 10:11
Operator : YP/AJ
Sample : AR1660ICC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 11:05:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 15 11:05:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

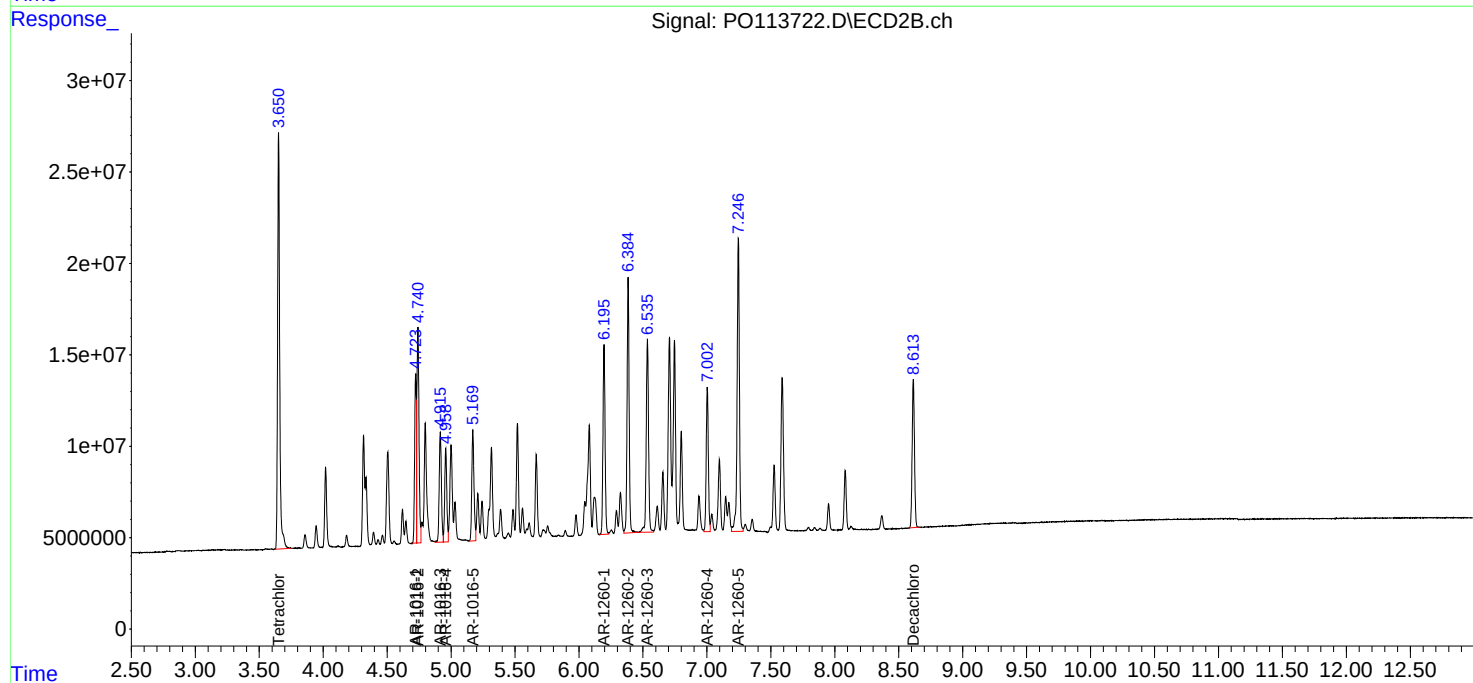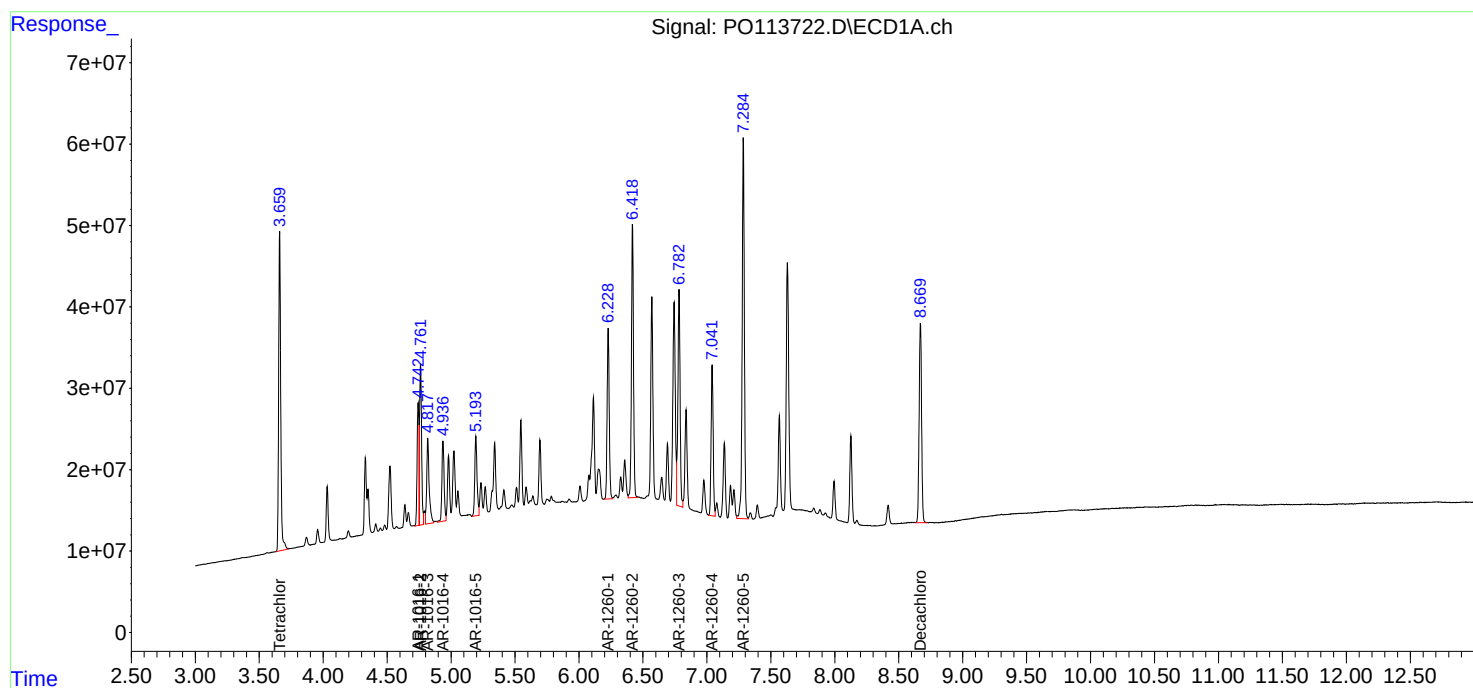

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113723.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 10:30
 Operator : YP/AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC250

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/16/2025
 Supervised By :mohammad ahmed 09/17/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 11:15:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 15 11:05:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.650	234.8E6	141.2E6	26.755	26.884
2) SA Decachlor...	8.671	8.615	176.7E6	56266448	26.911	27.250
Target Compounds						
3) L1 AR-1016-1	4.742	4.723	83067158	49485896	278.789	283.219
4) L1 AR-1016-2	4.761	4.740	123.2E6	73863126	276.594	277.828
5) L1 AR-1016-3	4.818	4.915	83791663	39670595	291.989	276.833m
6) L1 AR-1016-4	4.936	4.957	62801990	32386865	269.840m	283.635m
7) L1 AR-1016-5	5.193	5.168	64527220	41323076	262.680m	285.632m
31) L7 AR-1260-1	6.228	6.195	126.9E6	67517304	266.571	282.415
32) L7 AR-1260-2	6.418	6.384	203.4E6	88290231	272.205	281.873
33) L7 AR-1260-3	6.783	6.535	180.9E6	77229605	284.722	289.274
34) L7 AR-1260-4	7.042	7.003	115.1E6	52427799	275.162	286.353
35) L7 AR-1260-5	7.286	7.246	298.4E6	112.5E6	263.742	279.694

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113723.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 10:30
Operator : YP/AJ
Sample : AR1660ICC250
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/16/2025
Supervised By :mohammad ahmed 09/17/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 11:15:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 15 11:05:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

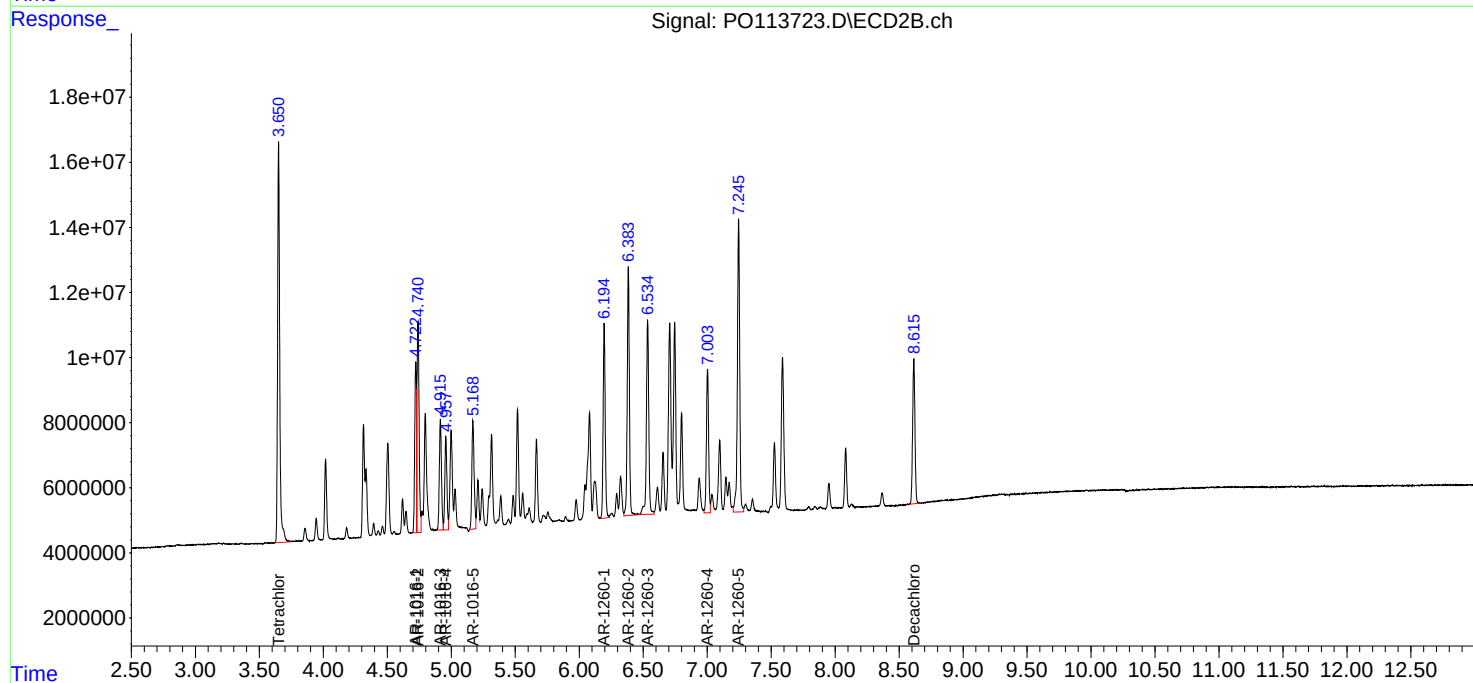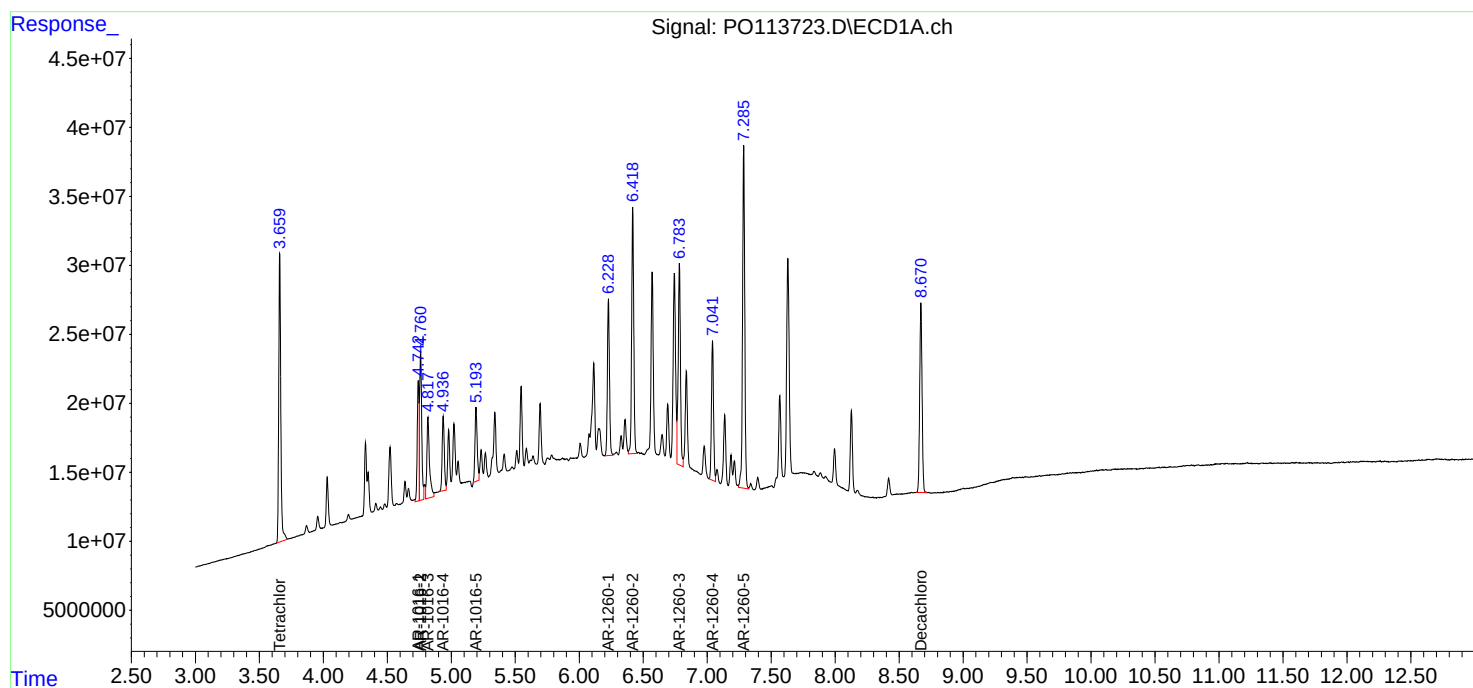

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0091525\
 Data File : P0113724.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 10:48
 Operator : YP/AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1660ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/16/2025
 Supervised By :mohammad ahmed 09/17/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 11:19:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 15 11:05:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.660	3.650	44978188	28453222	5.100	5.327
2) SA Decachlor...	8.670	8.615	35936460	10897672	5.371	5.220
Target Compounds						
3) L1 AR-1016-1	4.744	4.722	16286949	10615009	53.661	58.247
4) L1 AR-1016-2	4.762	4.740	24671155	16039442	54.215	57.936
5) L1 AR-1016-3	4.819	4.914	16959086	8685099	56.680	58.442m
6) L1 AR-1016-4	4.937	4.957	13300047	7240813	55.637m	60.429m
7) L1 AR-1016-5	5.193	5.169	12550255	8566818	52.077m	56.328m
31) L7 AR-1260-1	6.228	6.196	27305815	15008040	55.703	59.724
32) L7 AR-1260-2	6.419	6.384	42049271	20006498	54.906	60.514
33) L7 AR-1260-3	6.783	6.534	41141892	16693888	61.149	59.545
34) L7 AR-1260-4	7.041	7.003	24542000	11185219	56.714	58.380m
35) L7 AR-1260-5	7.286	7.245	56933192	25965493	50.259	62.242

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113724.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 10:48
Operator : YP/AJ
Sample : AR1660ICC050
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/16/2025
Supervised By :mohammad ahmed 09/17/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 11:19:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 15 11:05:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

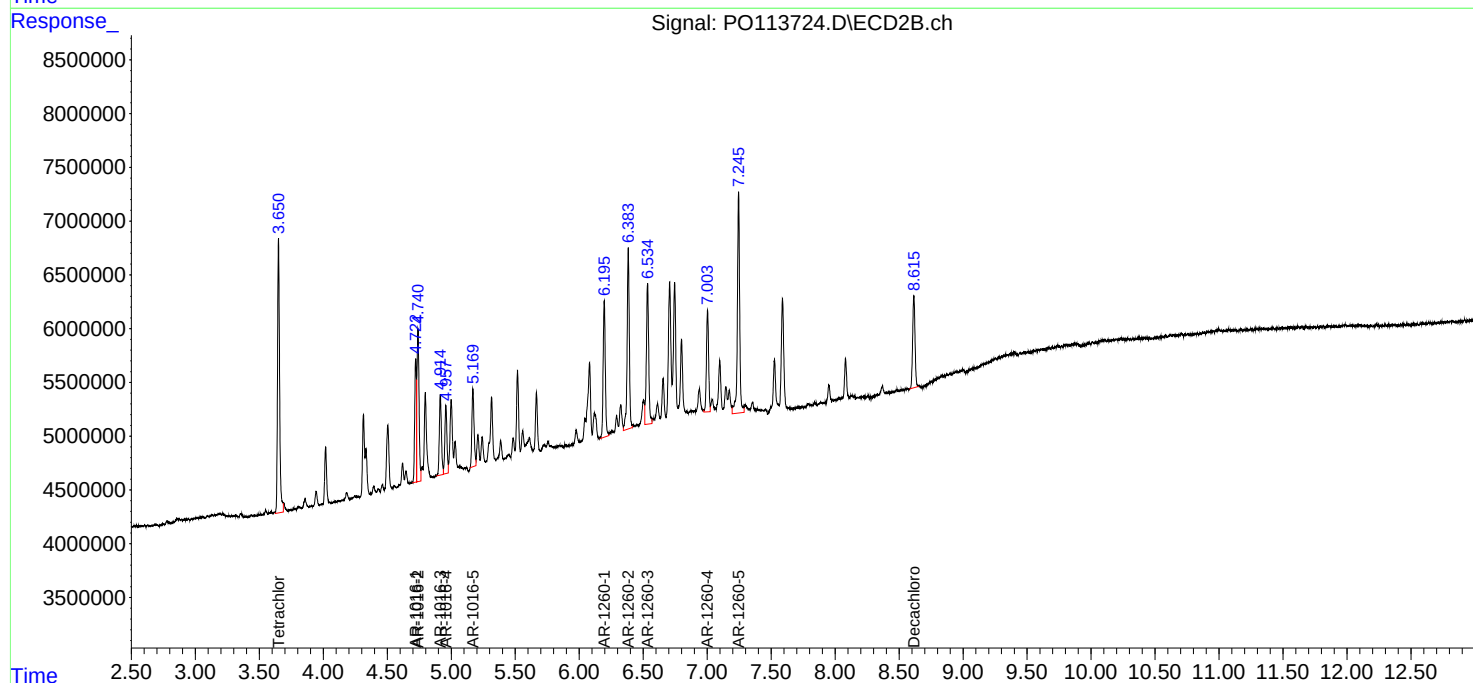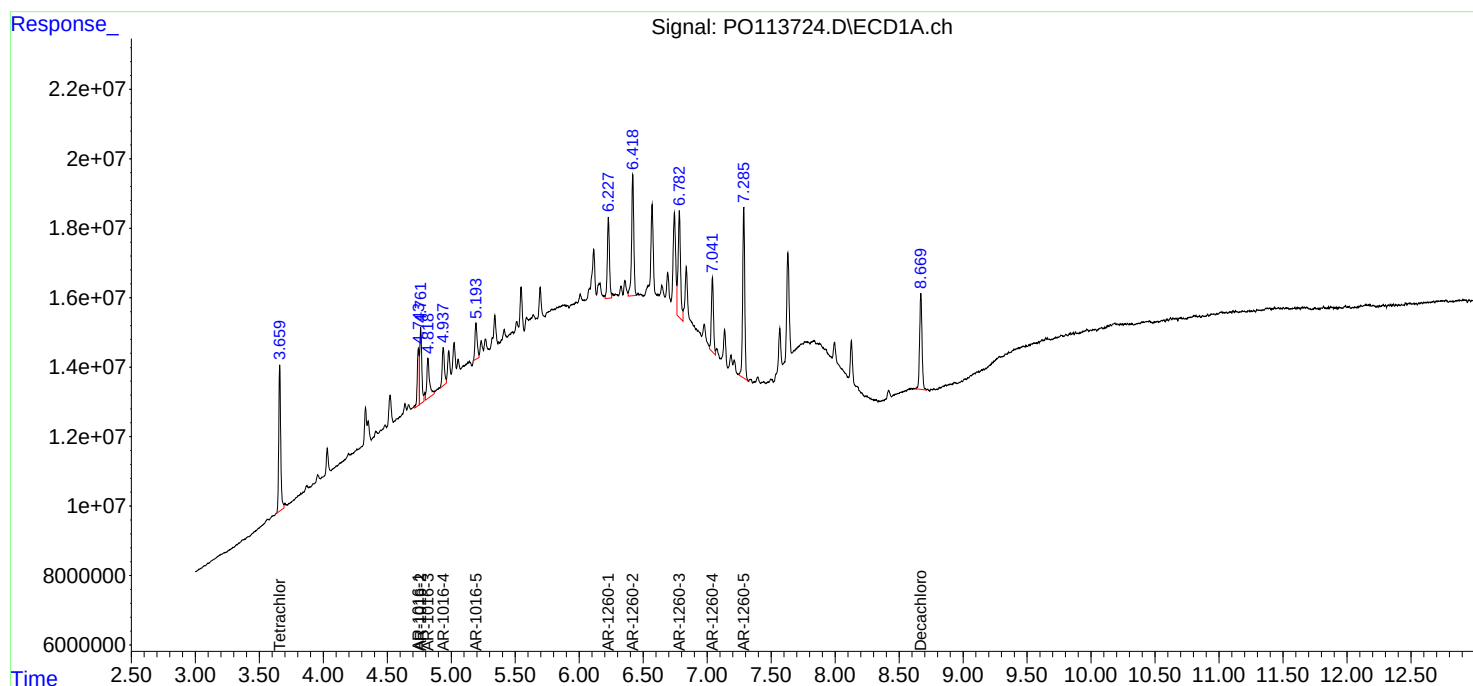

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0091525\
 Data File : P0113725.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 11:06
 Operator : YP/AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 11:46:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 15 11:45:58 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.651	435.5E6	262.7E6	50.000	50.000
2) SA Decachlor...	8.669	8.614	324.6E6	101.5E6	50.000	50.000
Target Compounds						
8) L2 AR-1221-1	3.870	3.858	48427821	33839498	500.000	500.000
9) L2 AR-1221-2	3.956	3.944	35948096	25481100	500.000	500.000
10) L2 AR-1221-3	4.031	4.018	118.4E6	78298360	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113725.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 11:06
Operator : YP/AJ
Sample : AR1221ICC500
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 11:46:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 15 11:45:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

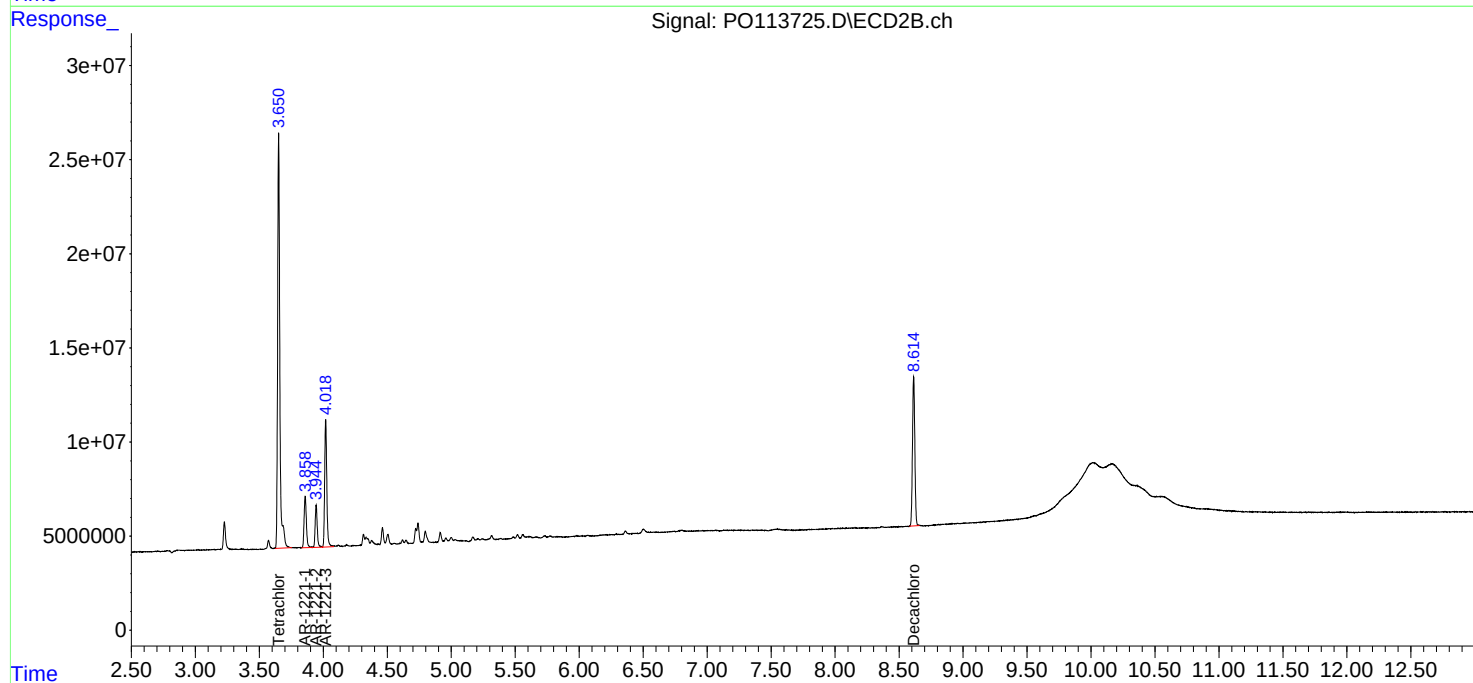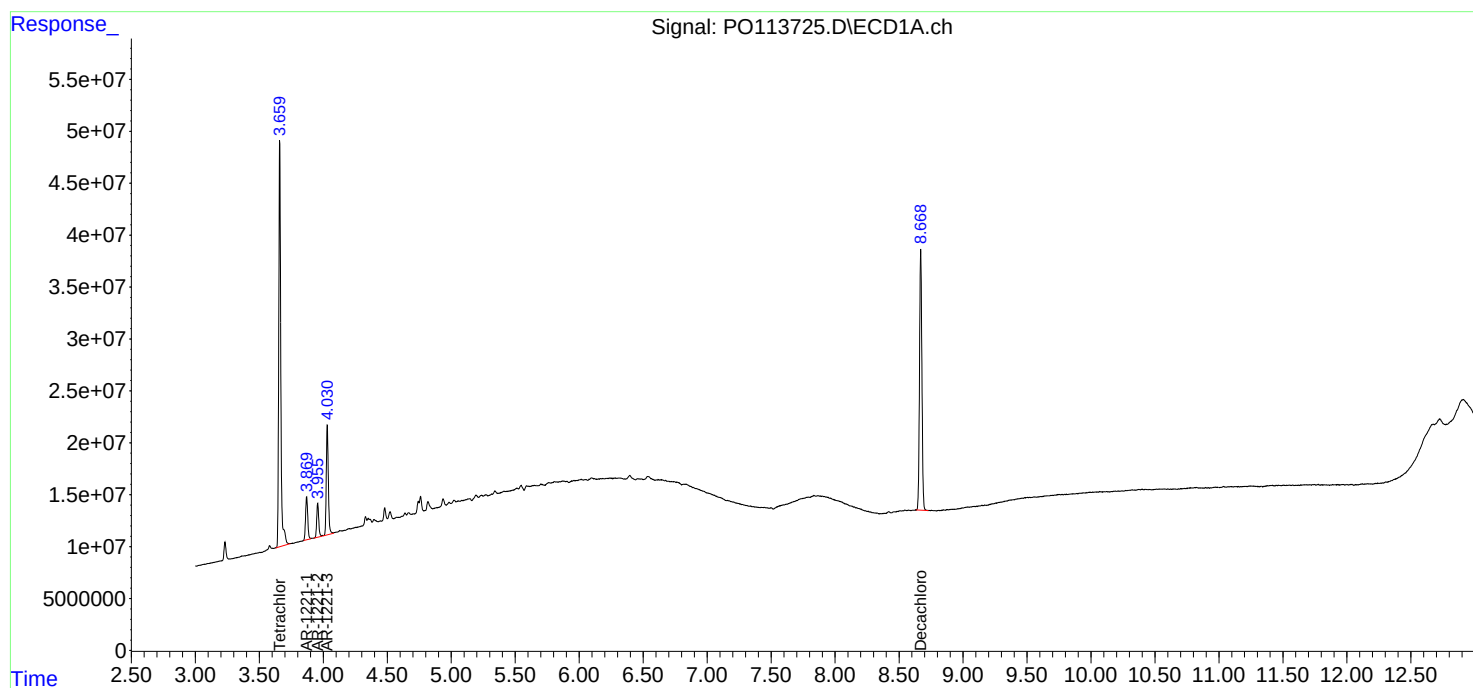

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0091525\
 Data File : P0113726.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 11:25
 Operator : YP/AJ
 Sample : AR1232ICC500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1232ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 11:52:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 15 11:52:36 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.650	429.5E6	257.8E6	50.000	50.000
2) SA Decachlor...	8.671	8.616	334.7E6	103.1E6	50.000	50.000
Target Compounds						
11) L3 AR-1232-1	4.031	4.018	87537440	59200862	500.000	500.000
12) L3 AR-1232-2	4.521	4.740	47976450	61415553	500.000	500.000
13) L3 AR-1232-3	4.760	4.914	98512468	33272859	500.000	500.000
14) L3 AR-1232-4	4.937	4.999	49367482	29320487	500.000	500.000
15) L3 AR-1232-5	4.980	5.169	32629799	30767257	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113726.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 11:25
Operator : YP/AJ
Sample : AR1232ICC500
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1232ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 11:52:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 15 11:52:36 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

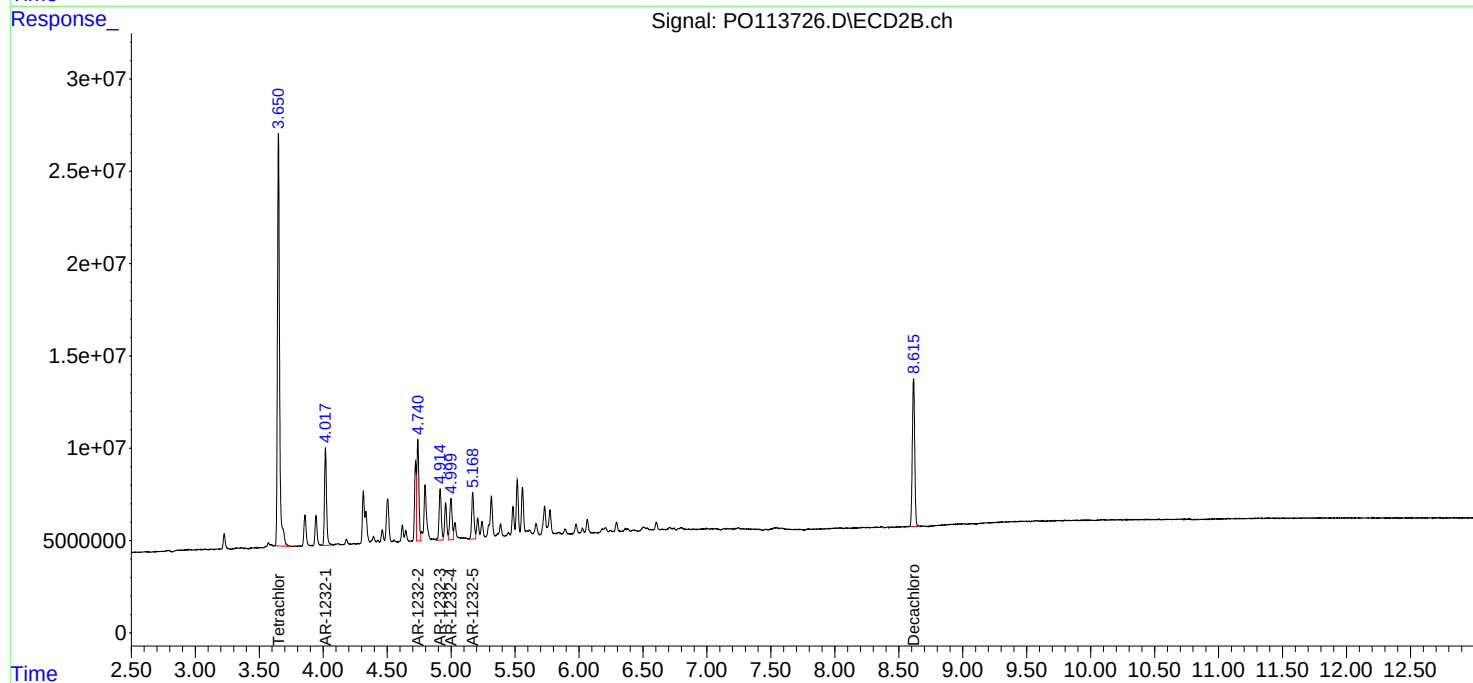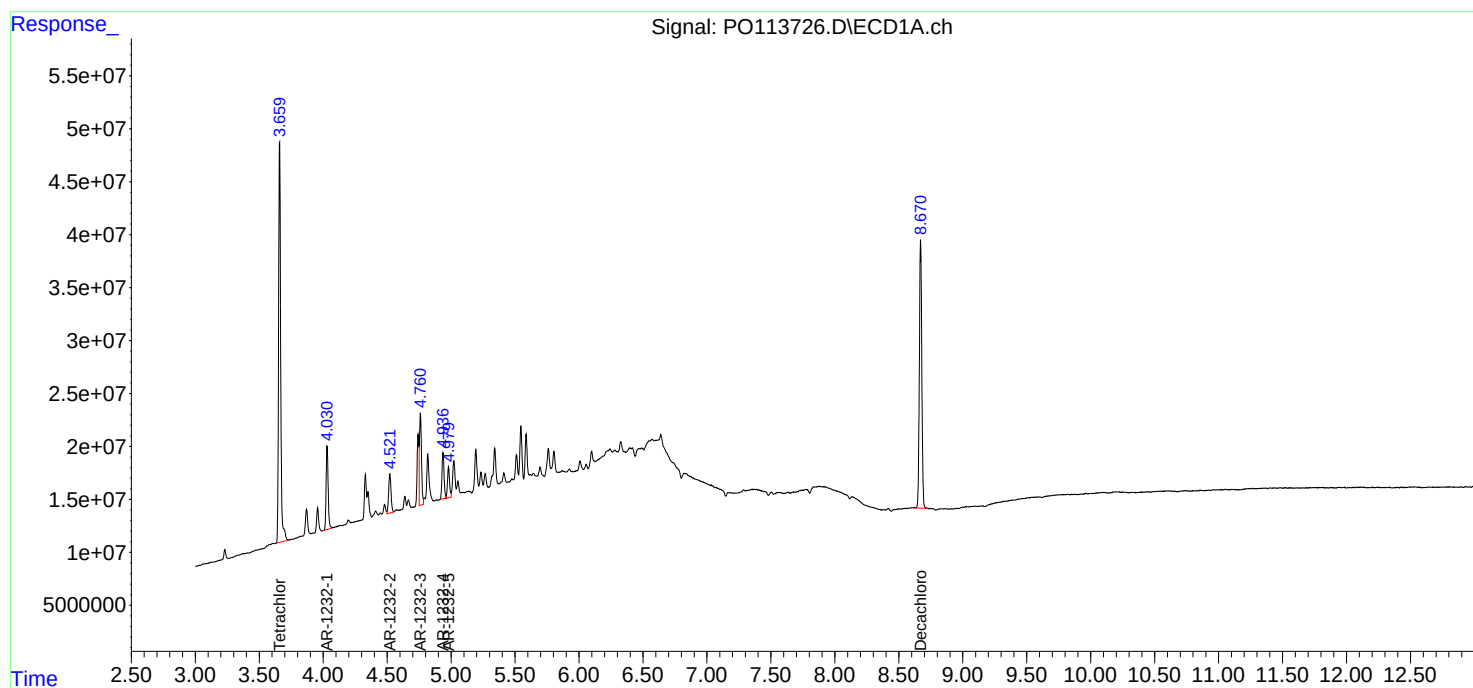

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113727.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 11:43
 Operator : YP/AJ
 Sample : AR1242ICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 12:49:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 15 12:48:41 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.651	856.9E6	508.2E6	103.413	102.682
2) SA Decachlor...	8.671	8.615	662.5E6	201.3E6	98.781	98.964
Target Compounds						
16) L4 AR-1242-1	4.743	4.723	238.6E6	140.1E6	1022.174	1007.884
17) L4 AR-1242-2	4.761	4.740	362.6E6	212.5E6	1028.745	1006.582
18) L4 AR-1242-3	4.818	4.915	227.9E6	114.4E6	1023.990	992.567
19) L4 AR-1242-4	4.937	4.999	185.7E6	109.0E6	1025.254	988.497
20) L4 AR-1242-5	5.587	5.518	203.8E6	137.2E6	1022.117	984.036



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113727.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 11:43
Operator : YP/AJ
Sample : AR1242ICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 12:49:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 15 12:48:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

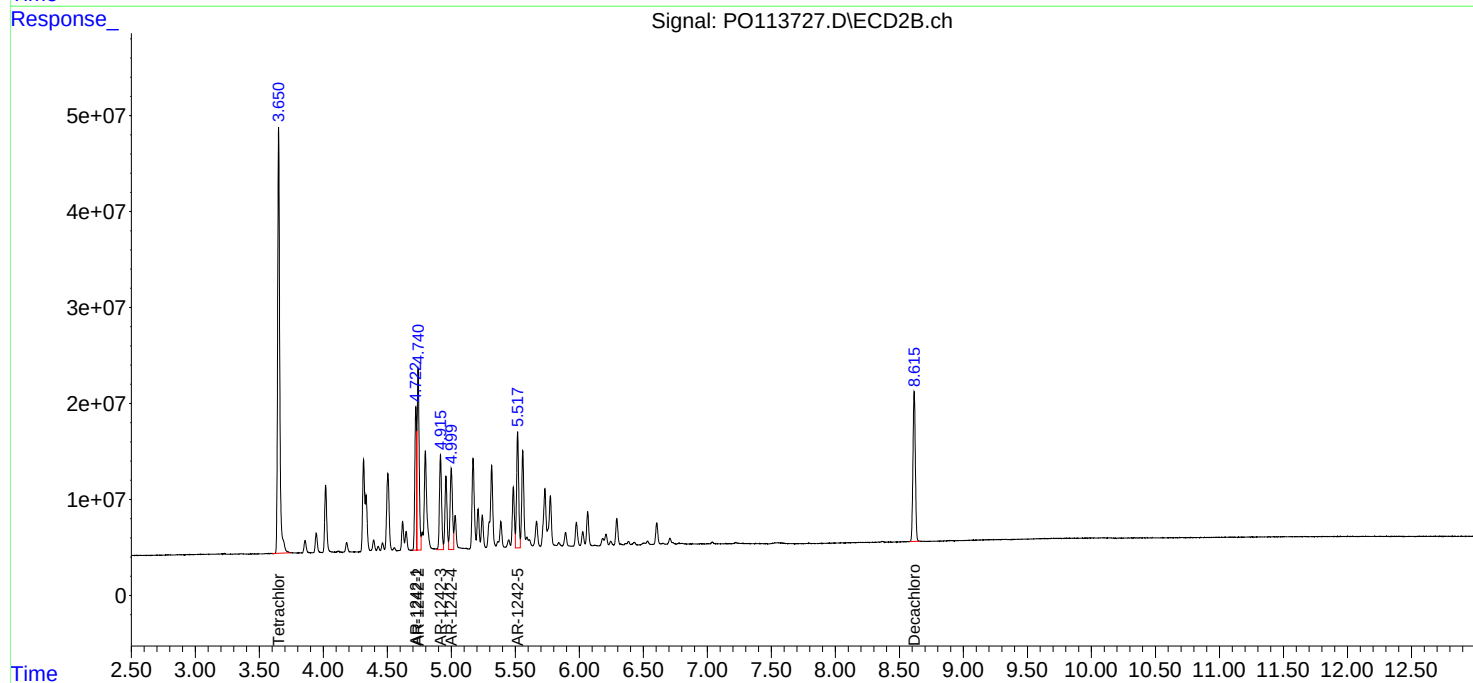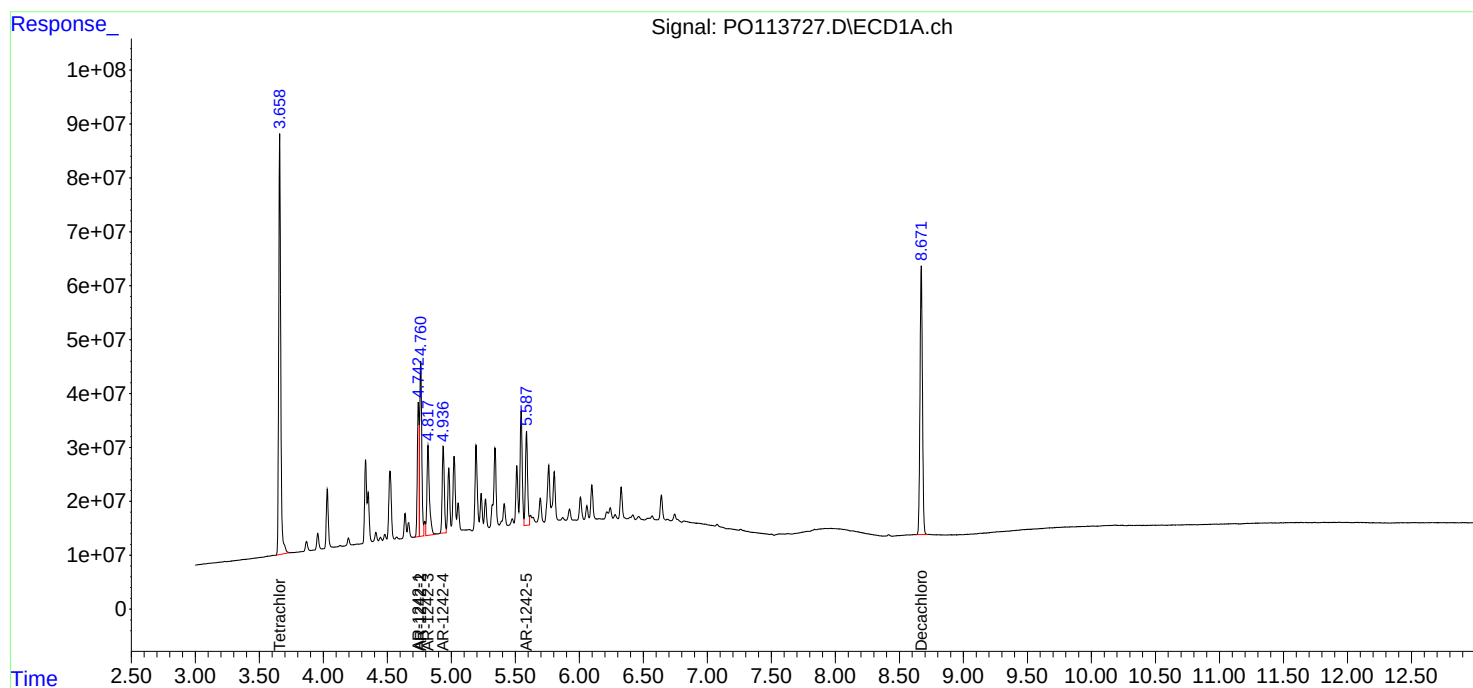

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0091525\
 Data File : P0113728.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 12:02
 Operator : YP/AJ
 Sample : AR1242ICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1242ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 12:53:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 15 12:52:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.651	637.8E6	380.3E6	76.303	76.216
2) SA Decachlor...	8.671	8.615	500.6E6	152.8E6	74.760	75.061
Target Compounds						
16) L4 AR-1242-1	4.742	4.722	180.5E6	106.0E6	765.468	758.656
17) L4 AR-1242-2	4.761	4.740	270.5E6	162.2E6	761.594	762.181
18) L4 AR-1242-3	4.818	4.915	171.0E6	87325225	762.136	755.272
19) L4 AR-1242-4	4.936	5.000	139.6E6	82992496	763.702	751.982
20) L4 AR-1242-5	5.586	5.518	154.3E6	105.2E6	765.978	752.843



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113728.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 12:02
Operator : YP/AJ
Sample : AR1242ICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 12:53:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 15 12:52:59 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

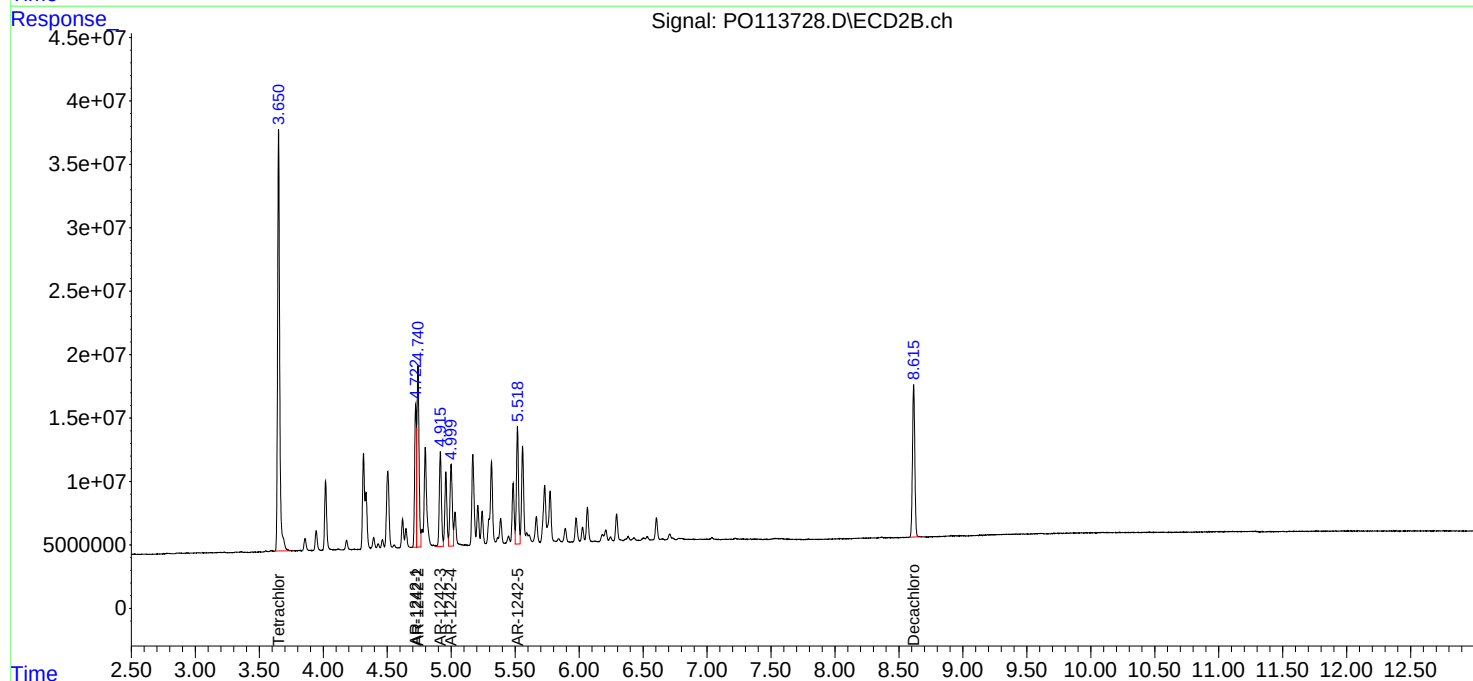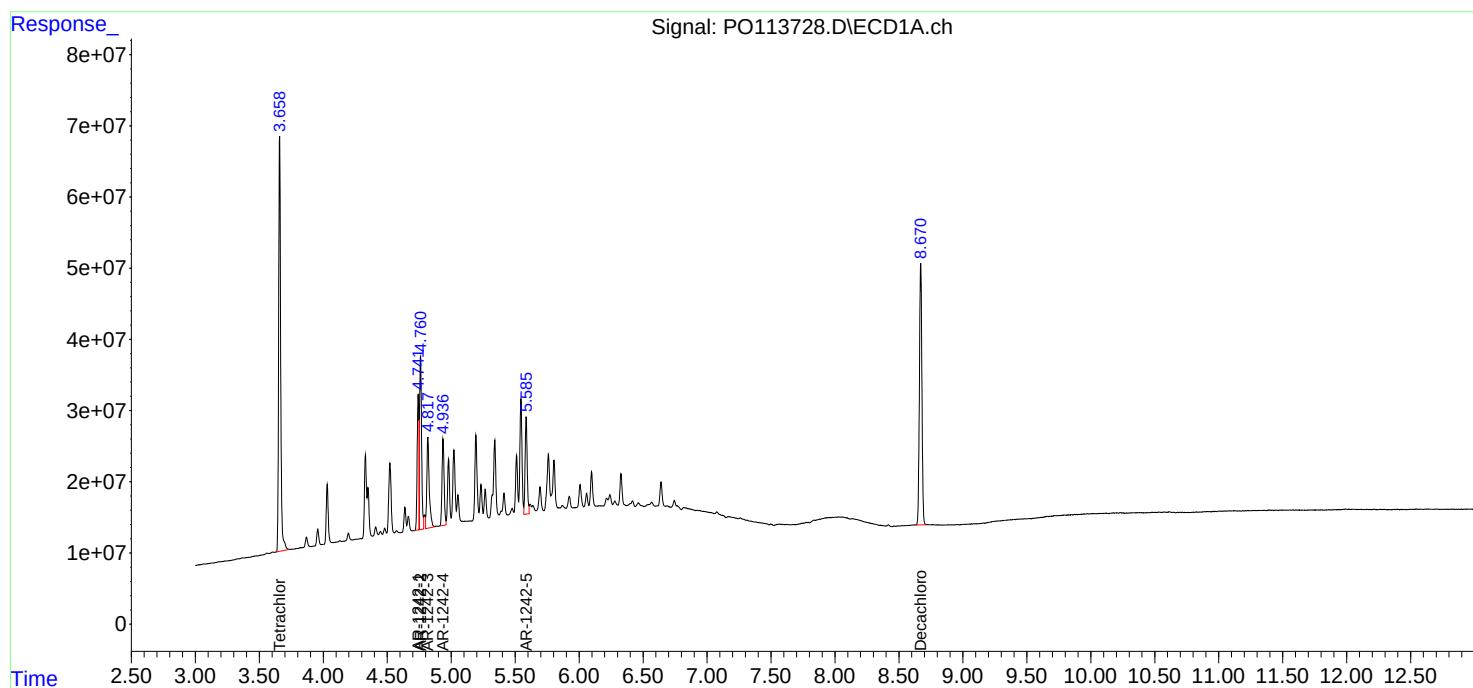

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113729.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 12:20
 Operator : YP/AJ
 Sample : AR1242ICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 12:44:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 15 12:44:08 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.650	400.2E6	240.8E6	50.000	50.000
2) SA Decachlor...	8.671	8.615	339.4E6	102.8E6	50.000	50.000
Target Compounds						
16) L4 AR-1242-1	4.743	4.723	114.1E6	68939510	500.000	500.000
17) L4 AR-1242-2	4.761	4.740	171.2E6	104.9E6	500.000	500.000
18) L4 AR-1242-3	4.818	4.915	108.6E6	58035506	500.000	500.000
19) L4 AR-1242-4	4.937	5.000	88265119	55743459	500.000	500.000
20) L4 AR-1242-5	5.587	5.518	97466339	70828355	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113729.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 12:20
Operator : YP/AJ
Sample : AR1242ICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 12:44:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 15 12:44:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

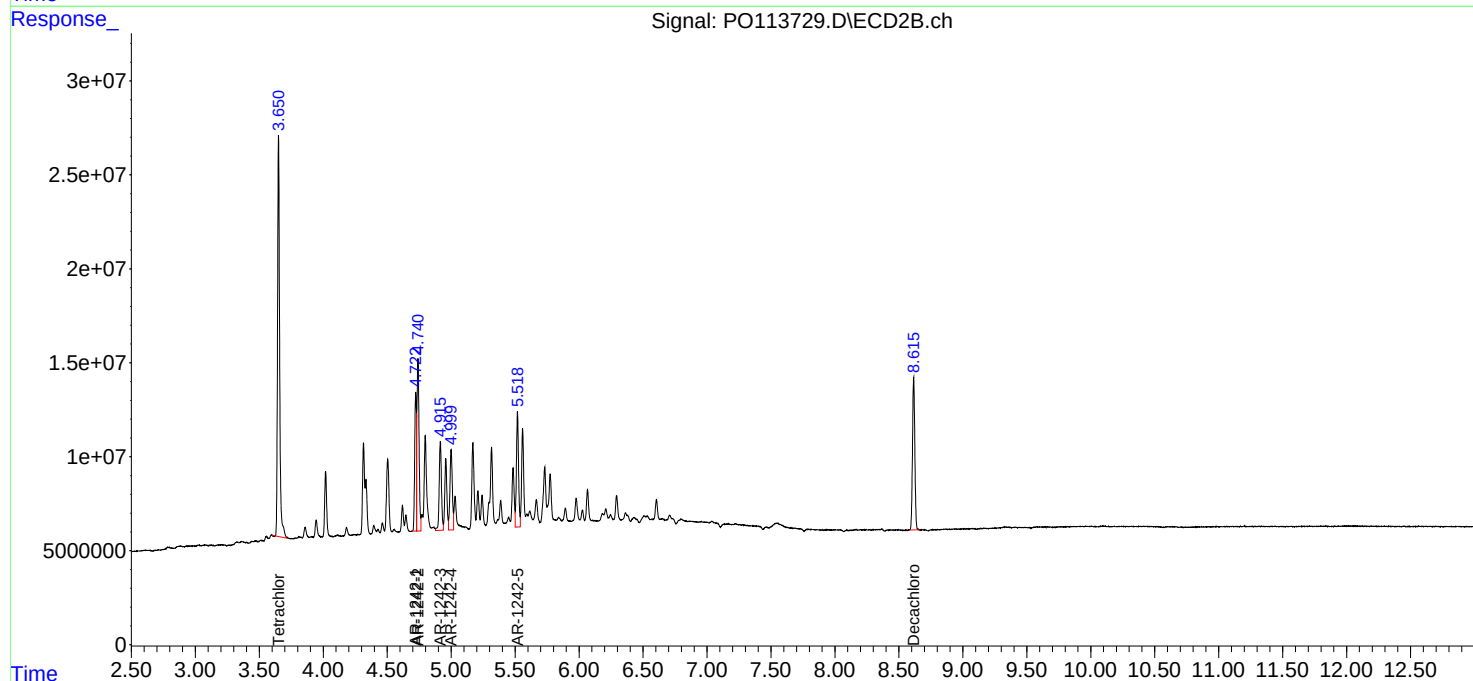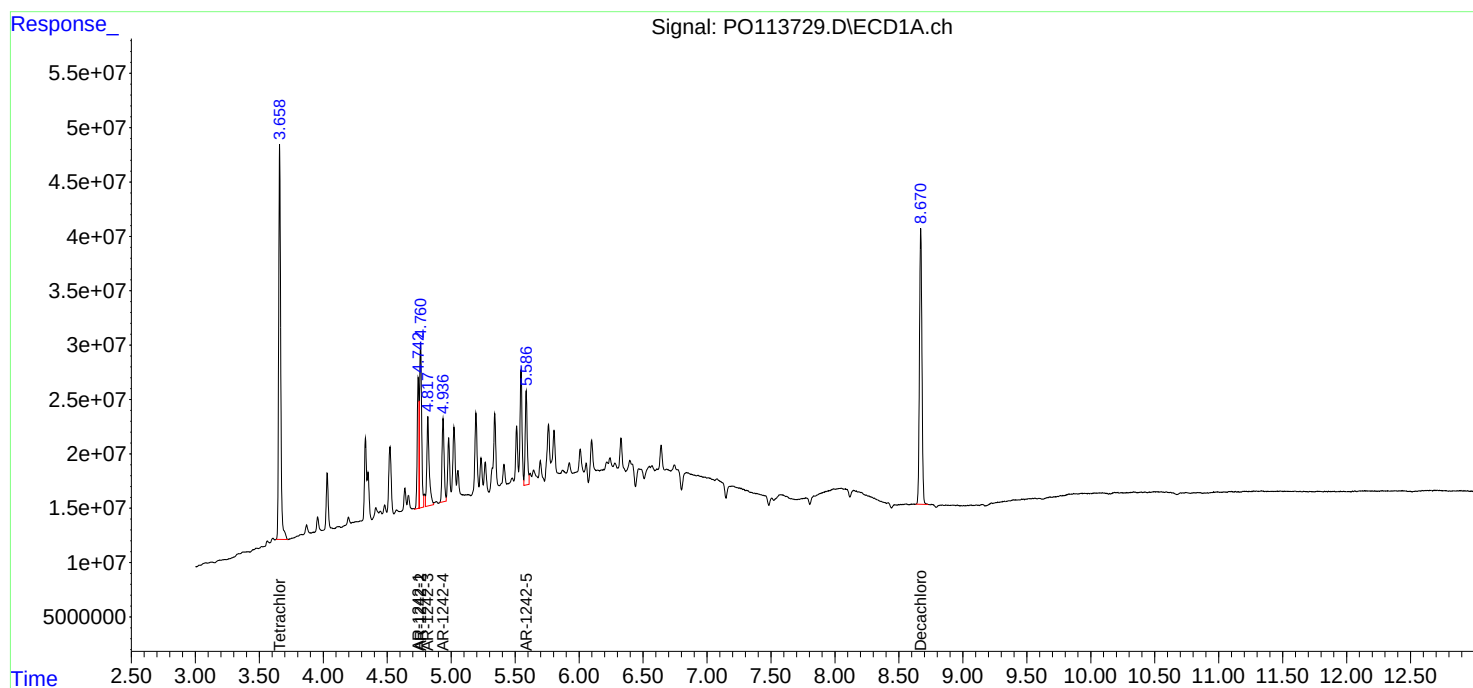

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113730.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 12:38
 Operator : YP/AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 12:58:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 15 12:58:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.650	227.2E6	137.2E6	26.605	26.824
2) SA Decachlor...	8.670	8.615	179.3E6	54699761	26.313	26.382
Target Compounds						
16) L4 AR-1242-1	4.743	4.722	64289772	40282392	266.562	277.583
17) L4 AR-1242-2	4.761	4.740	98374124	60995385	269.668	276.460
18) L4 AR-1242-3	4.818	4.915	61891602	33632533	268.898	279.460
19) L4 AR-1242-4	4.937	4.999	50545262	32527588	269.395	282.109
20) L4 AR-1242-5	5.587	5.518	58614341	41036519	279.475	281.442



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113730.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 12:38
Operator : YP/AJ
Sample : AR1242ICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 12:58:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 15 12:58:17 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

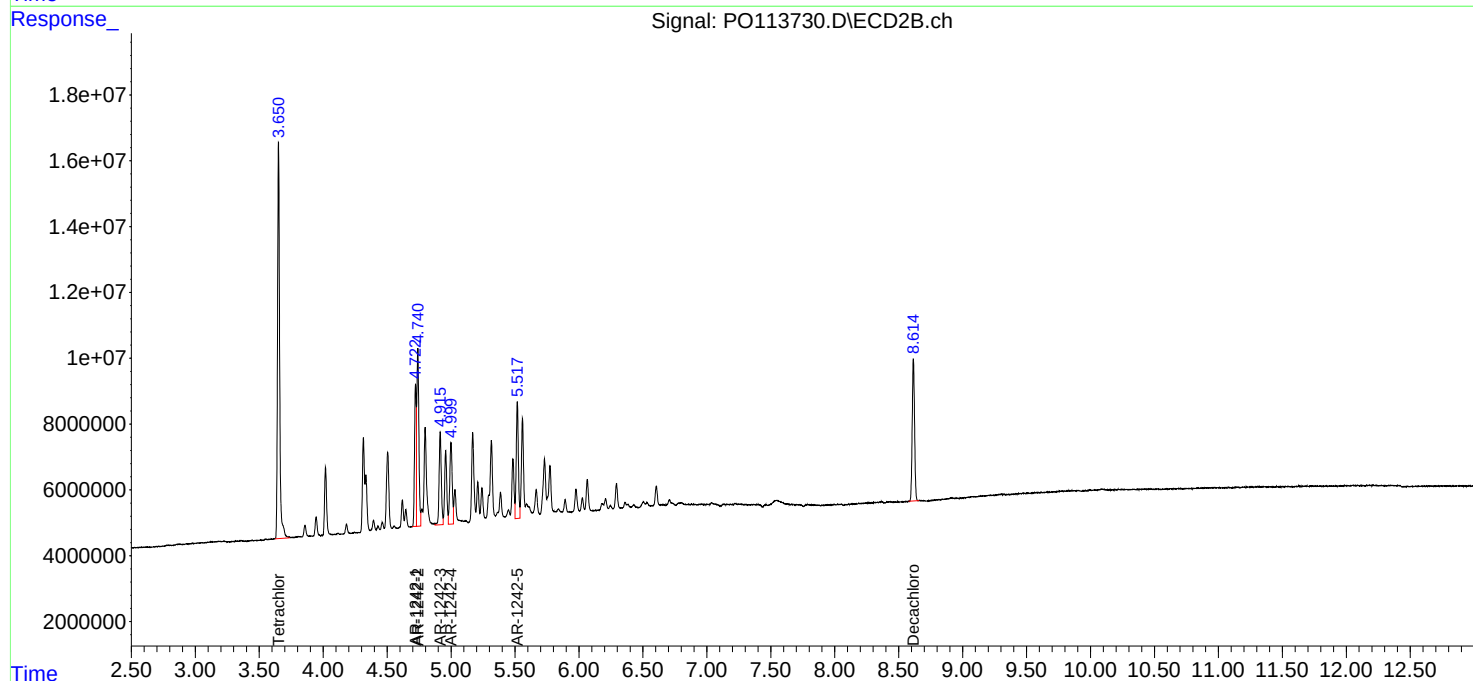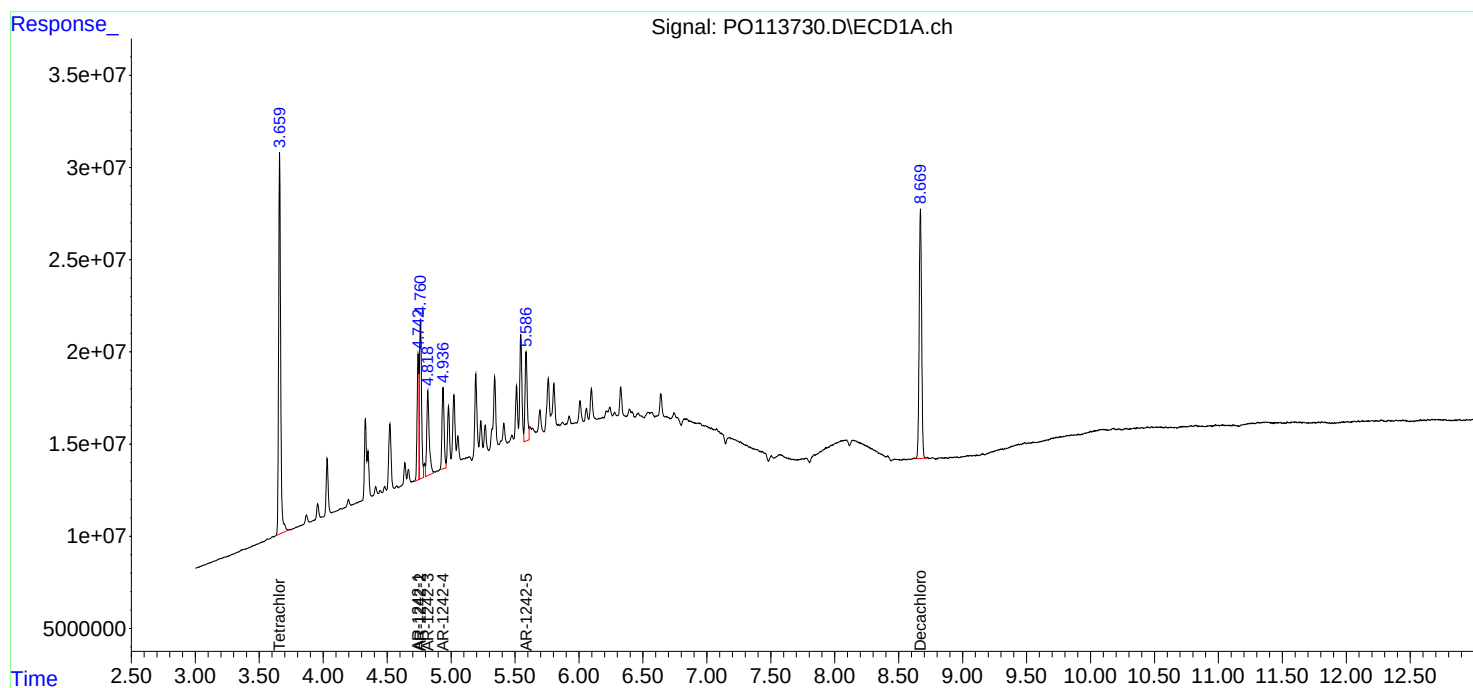

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113731.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 13:34
 Operator : YP/AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/16/2025
 Supervised By :mohammad ahmed 09/17/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 13:53:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 15 13:52:46 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.658	3.650	26418636	15800639	3.352m	3.352m
2)	SA Decachlor...	8.671	8.616	21938075	6851127	3.466	3.545
Target Compounds							
16)	L4 AR-1242-1	4.741	4.723	7313533	5086915	32.420m	37.283
17)	L4 AR-1242-2	4.760	4.741	11071458	7687318	32.781m	37.091
18)	L4 AR-1242-3	4.818	4.914	7714426	4933227	35.882	41.724m
19)	L4 AR-1242-4	4.938	4.997	6204472	5689058	35.471	48.409m#
20)	L4 AR-1242-5	5.588	5.517	10397803	6300322	50.944	45.312m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113731.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 13:34
Operator : YP/AJ
Sample : AR1242ICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/16/2025
Supervised By :mohammad ahmed 09/17/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 13:53:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 15 13:52:46 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

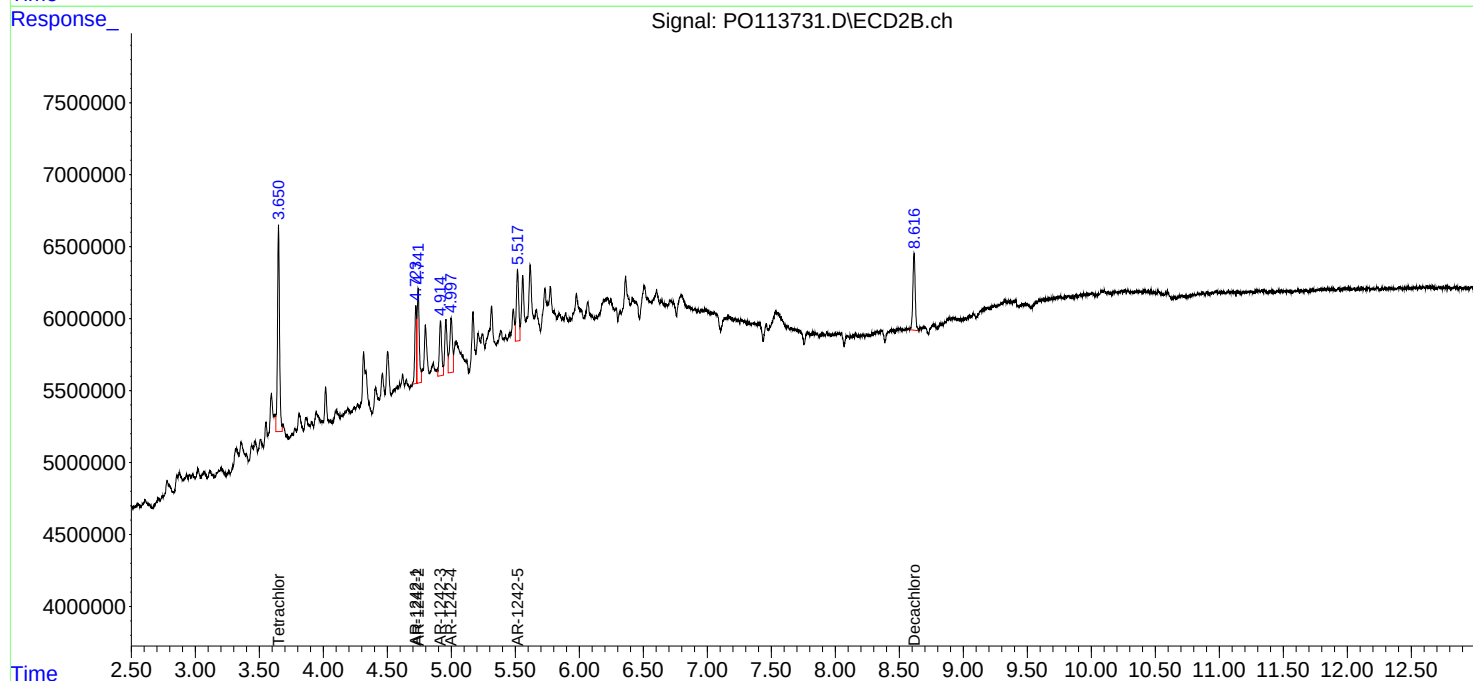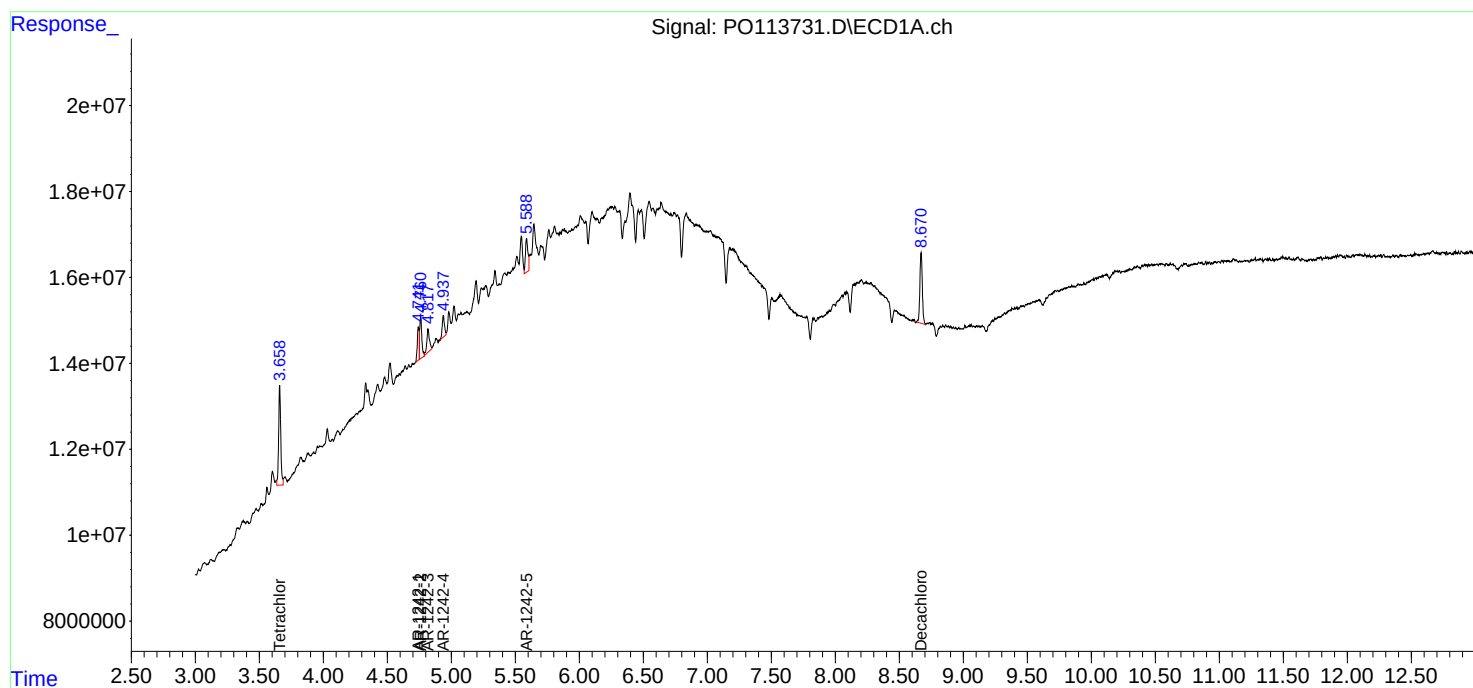

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113732.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 13:54
 Operator : YP/AJ
 Sample : AR1248ICC1000
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 15:00:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 15 14:57:41 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.661	3.651	828.2E6	491.8E6	99.140	98.907
2) SA Decachlor...	8.673	8.616	690.7E6	203.2E6	98.049	97.877
Target Compounds						
21) L5 AR-1248-1	4.745	4.722	176.0E6	104.7E6	974.524	963.707
22) L5 AR-1248-2	4.982	4.958	241.2E6	146.4E6	981.274	960.088
23) L5 AR-1248-3	5.196	4.999	312.0E6	155.1E6	978.325	961.488
24) L5 AR-1248-4	5.548	5.170	478.8E6	182.0E6	979.615	965.593
25) L5 AR-1248-5	5.589	5.559	326.3E6	185.6E6	978.067	964.077



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113732.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 13:54
Operator : YP/AJ
Sample : AR1248ICC1000
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 15:00:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 15 14:57:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

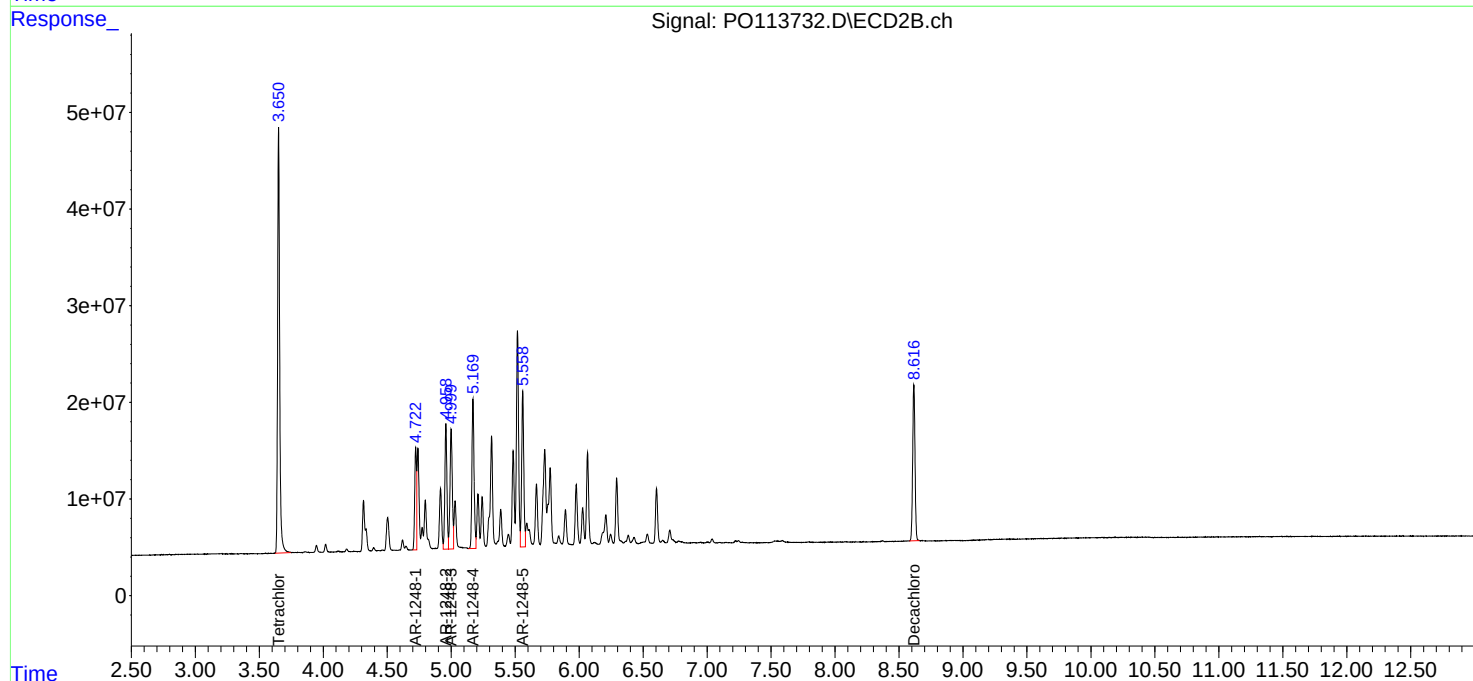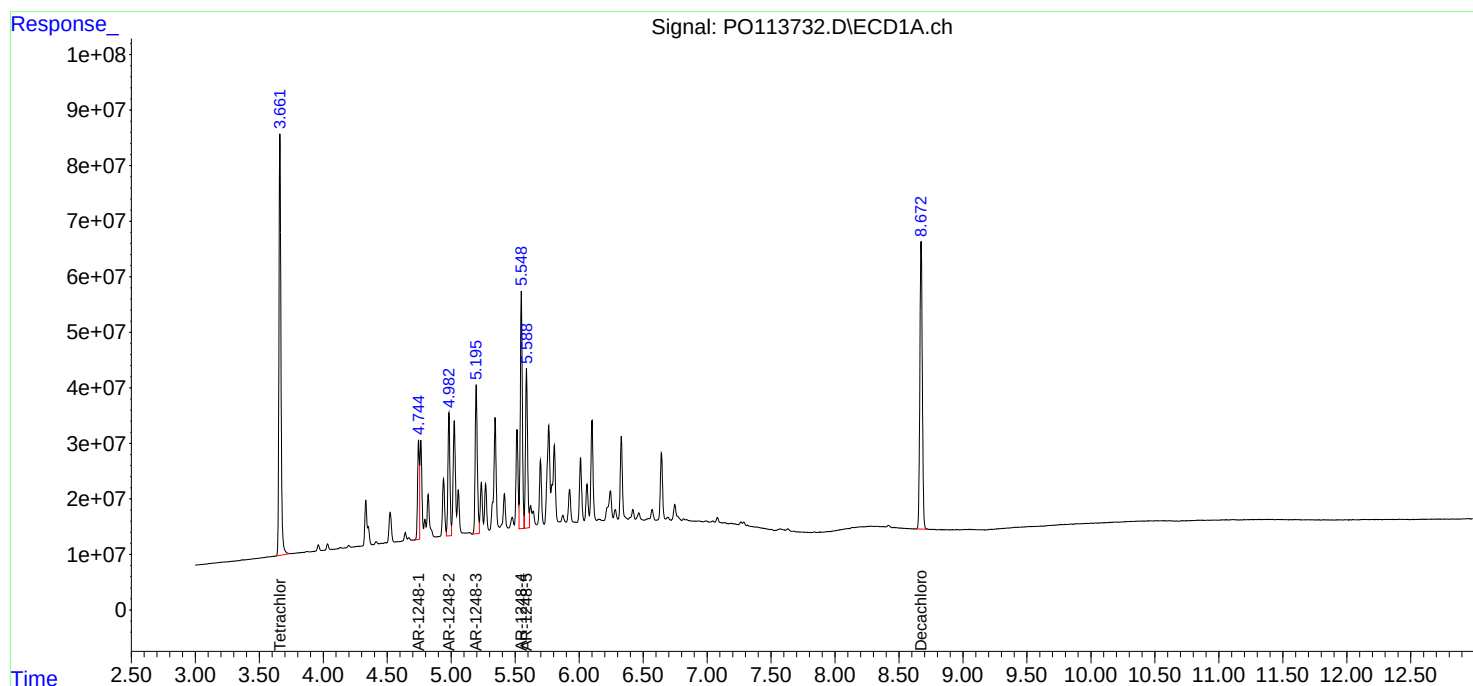

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113733.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 14:13
 Operator : YP/AJ
 Sample : AR1248ICC750
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 15:02:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 15 14:57:41 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.650	634.9E6	375.4E6	75.668	75.333
2) SA Decachlor...	8.670	8.615	524.4E6	155.6E6	74.627	74.969
Target Compounds						
21) L5 AR-1248-1	4.743	4.722	135.7E6	81830538	751.102	752.341
22) L5 AR-1248-2	4.980	4.958	186.3E6	114.2E6	755.166	749.329
23) L5 AR-1248-3	5.193	4.999	239.8E6	120.5E6	751.242	747.815
24) L5 AR-1248-4	5.546	5.169	368.9E6	141.0E6	753.153	748.773
25) L5 AR-1248-5	5.586	5.558	253.3E6	143.1E6	756.086	745.429



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113733.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 14:13
Operator : YP/AJ
Sample : AR1248ICC750
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 15:02:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 15 14:57:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

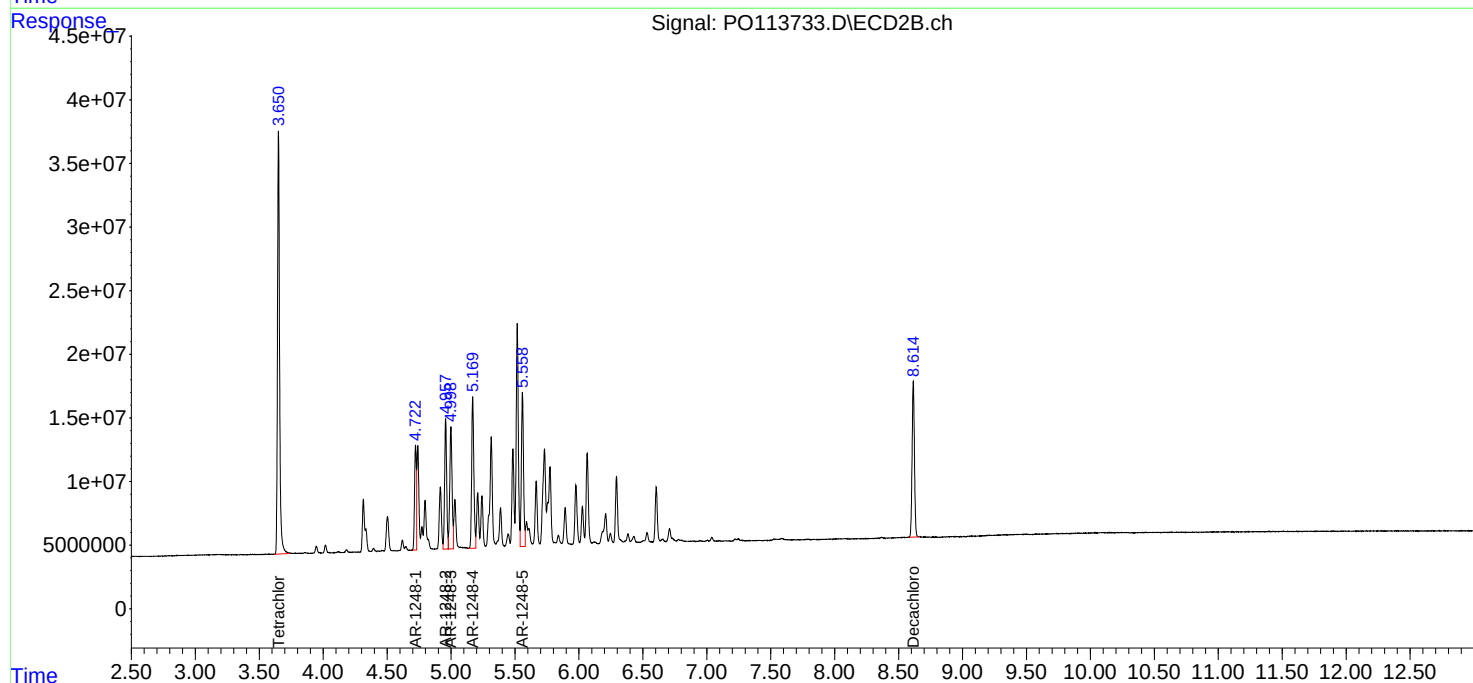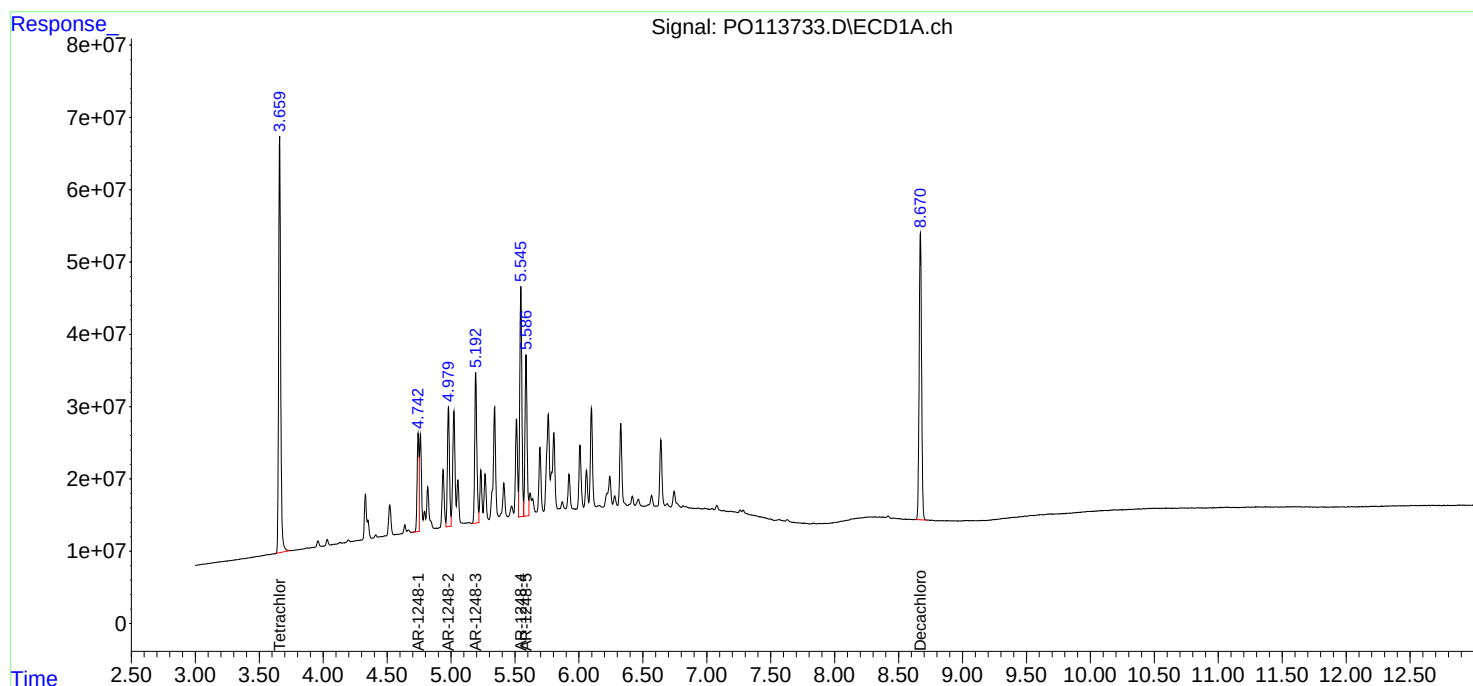

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113734.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 14:31
 Operator : YP/AJ
 Sample : AR1248ICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 14:57:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 15 14:57:41 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.649	421.3E6	251.3E6	50.000	50.000
2) SA Decachlor...	8.670	8.614	359.1E6	106.0E6	50.000	50.000
Target Compounds						
21) L5 AR-1248-1	4.742	4.721	92575652	56269703	500.000	500.000
22) L5 AR-1248-2	4.979	4.957	125.2E6	79271682	500.000	500.000
23) L5 AR-1248-3	5.193	4.998	162.9E6	83768269	500.000	500.000
24) L5 AR-1248-4	5.545	5.168	249.4E6	97489532	500.000	500.000
25) L5 AR-1248-5	5.586	5.557	170.5E6	99711270	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113734.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 14:31
Operator : YP/AJ
Sample : AR1248ICC500
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 14:57:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 15 14:57:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

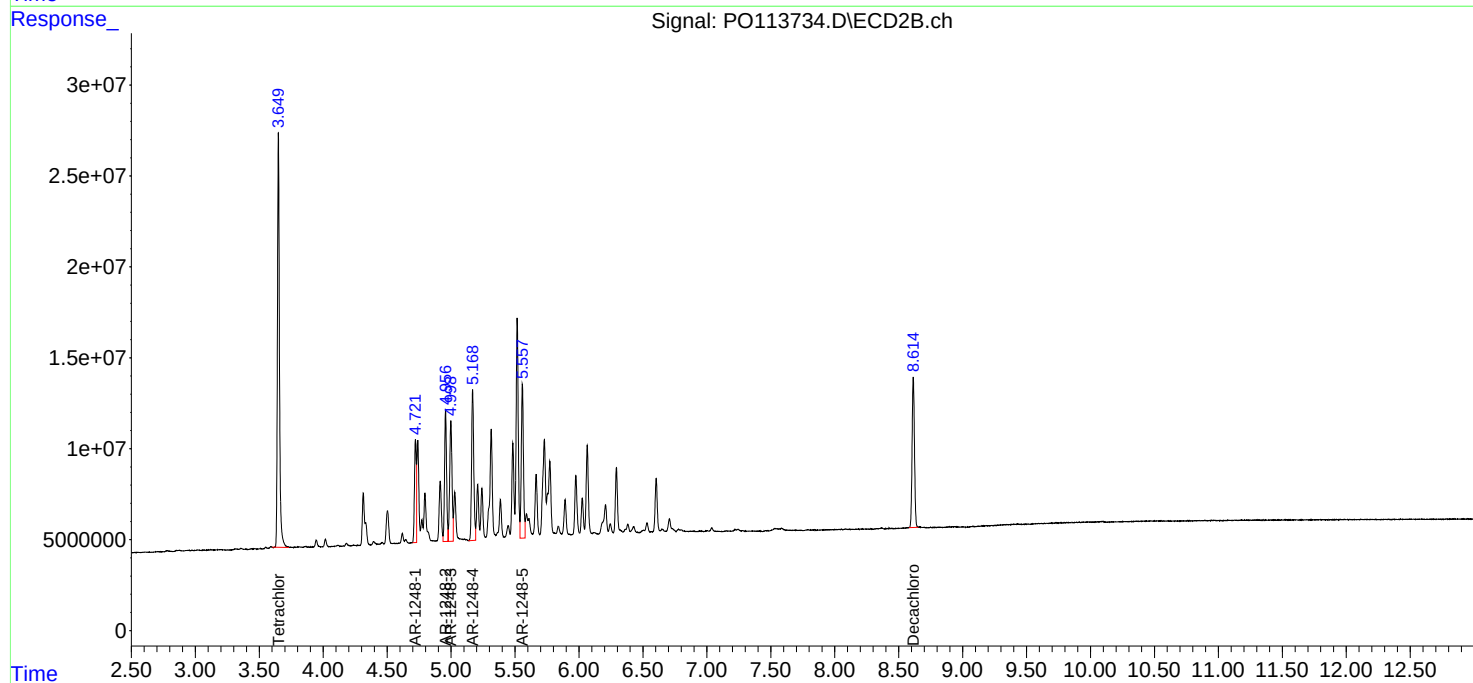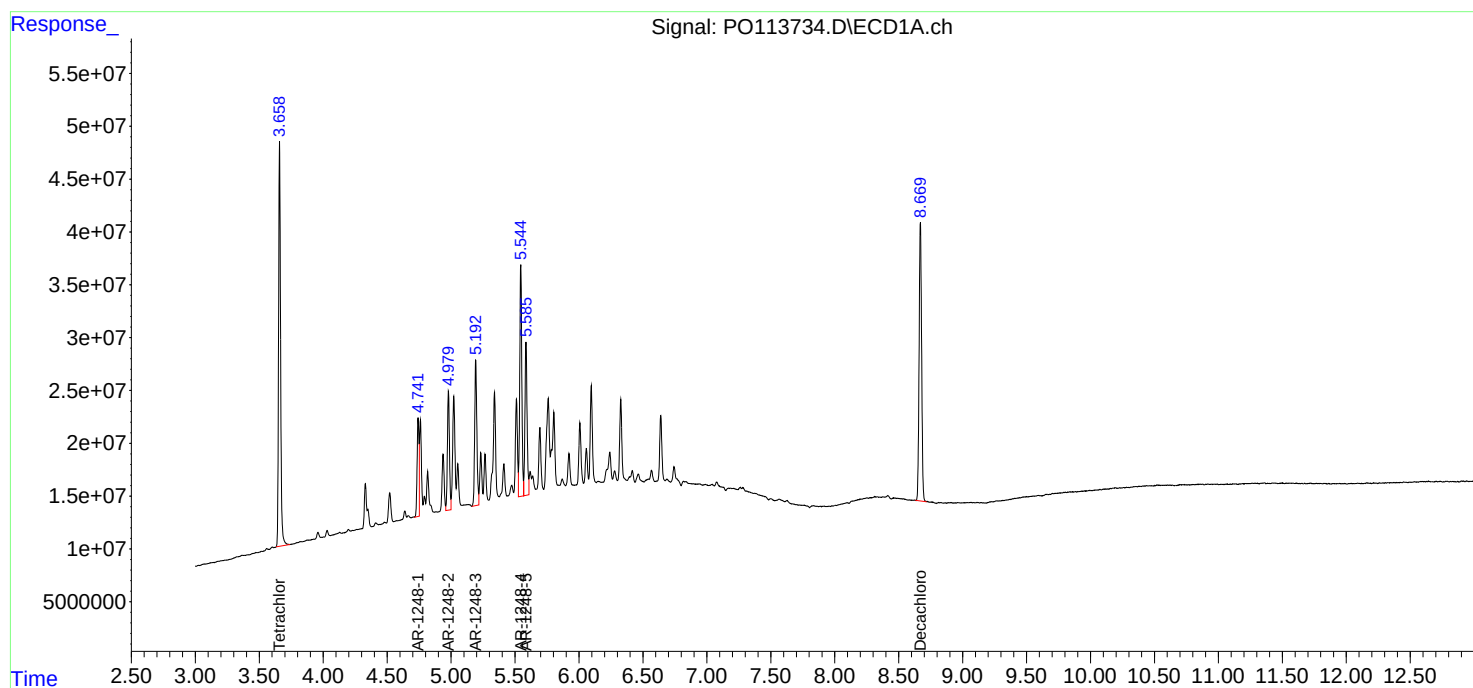

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113735.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 14:49
 Operator : YP/AJ
 Sample : AR1248ICC250
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC250

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/16/2025
 Supervised By :mohammad ahmed 09/17/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 15:05:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 15 14:57:41 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.650	218.3E6	136.0E6	25.864m	26.676
2) SA Decachlor...	8.671	8.615	190.3E6	56024890	26.532	26.467
Target Compounds						
21) L5 AR-1248-1	4.743	4.722	46836022	30431626	256.848	271.693
22) L5 AR-1248-2	4.980	4.958	66055658	43924160	263.119	277.620
23) L5 AR-1248-3	5.194	4.999	87559252	46565053	267.831	278.197
24) L5 AR-1248-4	5.546	5.169	134.2E6	53811343	267.565	275.862
25) L5 AR-1248-5	5.587	5.559	91796490	55645015	267.580	278.801

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113735.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 14:49
Operator : YP/AJ
Sample : AR1248ICC250
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1248ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/16/2025
Supervised By :mohammad ahmed 09/17/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 15:05:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 15 14:57:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

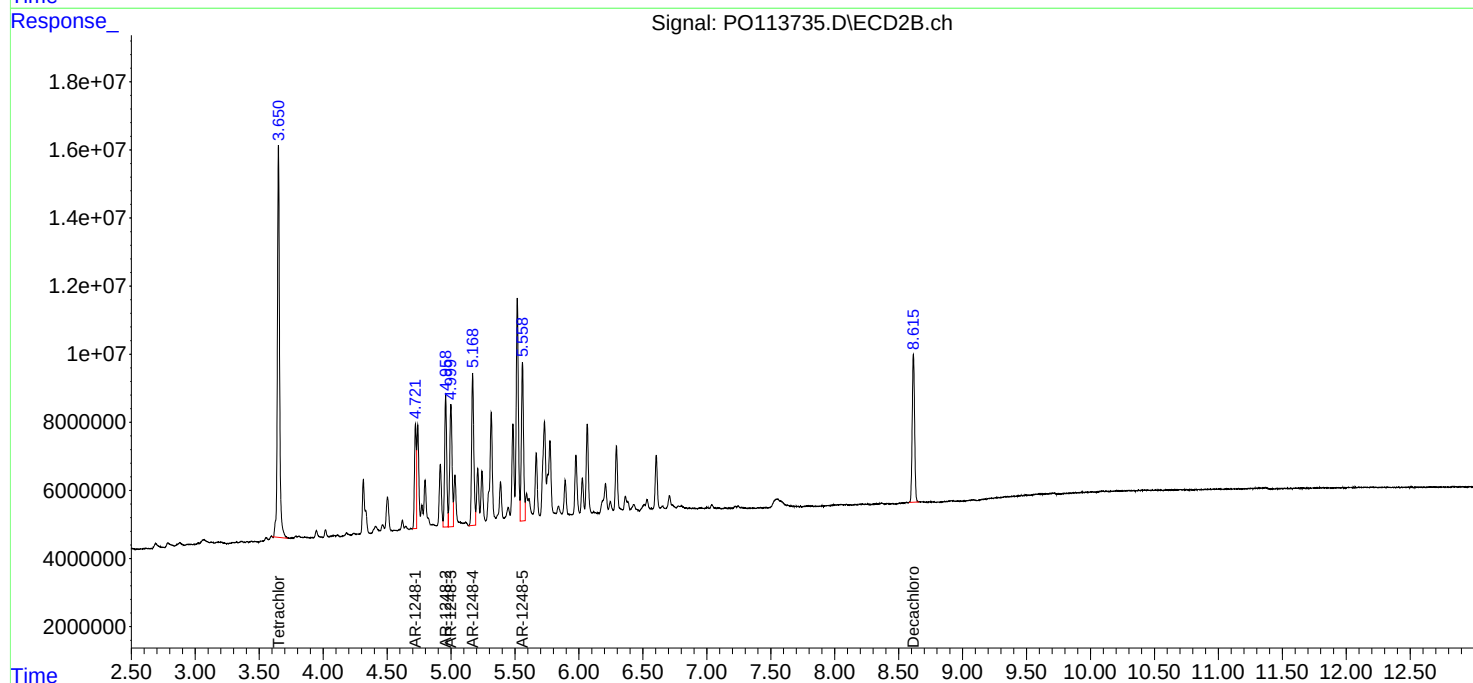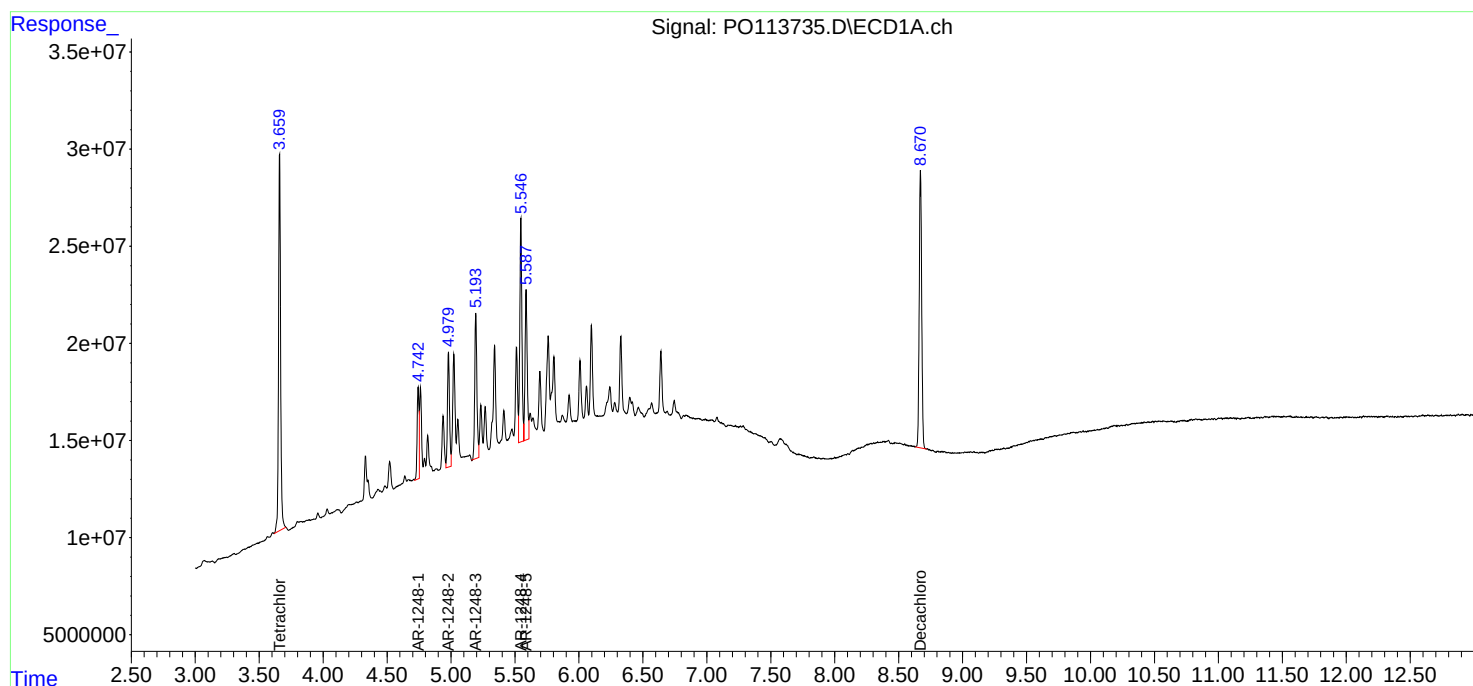

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113736.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 15:26
 Operator : YP/AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 15:45:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 15 15:45:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.660	3.650	32089373	20534701	3.979	4.192
2) SA Decachlor...	8.671	8.615	28408639	8300377	4.132	4.098
Target Compounds						
21) L5 AR-1248-1	4.744	4.722	8597711	4929969	47.693	45.094
22) L5 AR-1248-2	4.981	4.957	10595062	7750399	43.562	49.185
23) L5 AR-1248-3	5.193	4.999	15737208	8252286	48.499	49.440
24) L5 AR-1248-4	5.546	5.169	24775522	9558331	49.519	49.197
25) L5 AR-1248-5	5.588	5.558	15935750	10777751	47.120	53.150



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113736.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 15:26
Operator : YP/AJ
Sample : AR1248ICC050
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 15:45:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 15 15:45:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

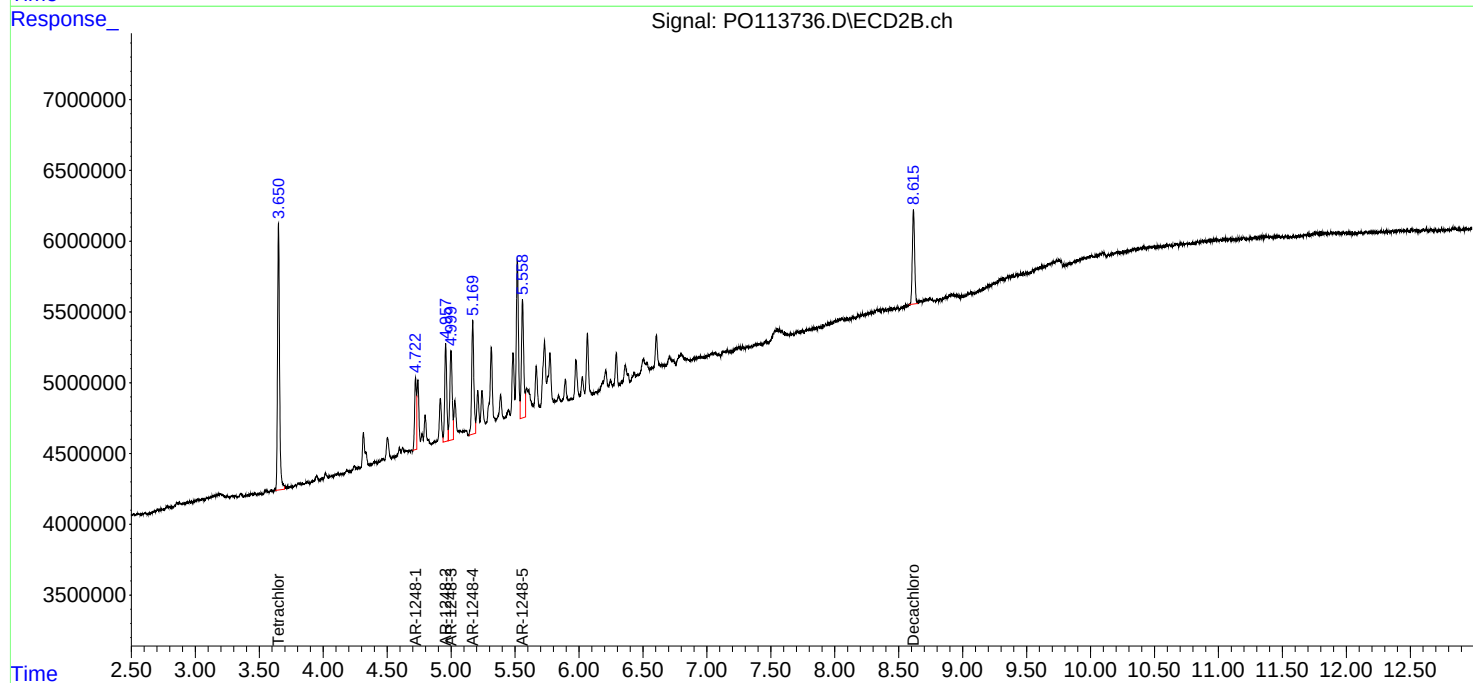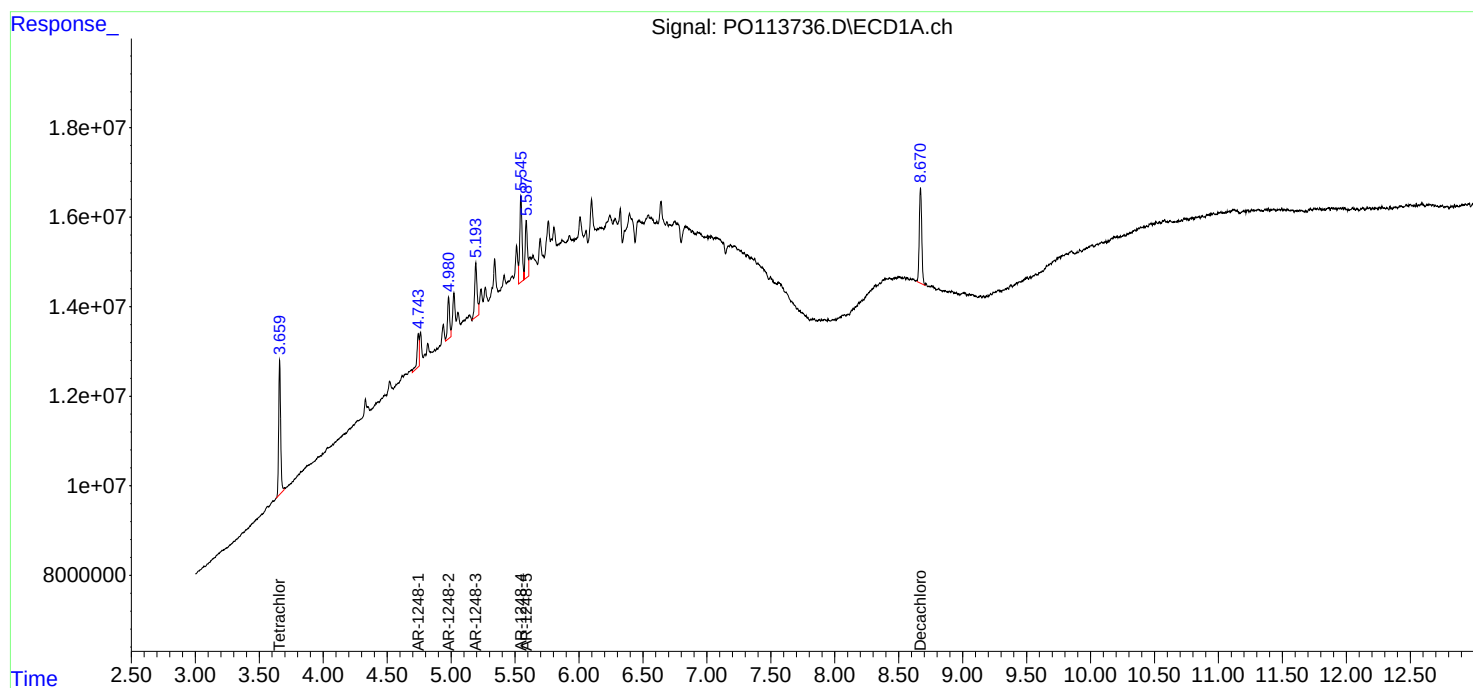

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113737.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 15:45
 Operator : YP/AJ
 Sample : AR1254ICC1000
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 16:39:18 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 15 16:36:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.660	3.651	832.6E6	490.7E6	98.269	98.049
2) SA Decachlor...	8.670	8.616	720.4E6	202.3E6	97.290	96.875
Target Compounds						
26) L6 AR-1254-1	5.546	5.519	525.3E6	279.6E6	964.321	957.531
27) L6 AR-1254-2	5.695	5.667	478.2E6	241.2E6	958.454	953.589
28) L6 AR-1254-3	6.098	6.066	746.6E6	370.6E6	965.121	968.115
29) L6 AR-1254-4	6.328	6.294	555.0E6	235.6E6	971.115	964.300
30) L6 AR-1254-5	6.745	6.709	718.1E6	290.2E6	971.401	964.075



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113737.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 15:45
Operator : YP/AJ
Sample : AR1254ICC1000
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 16:39:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 15 16:36:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

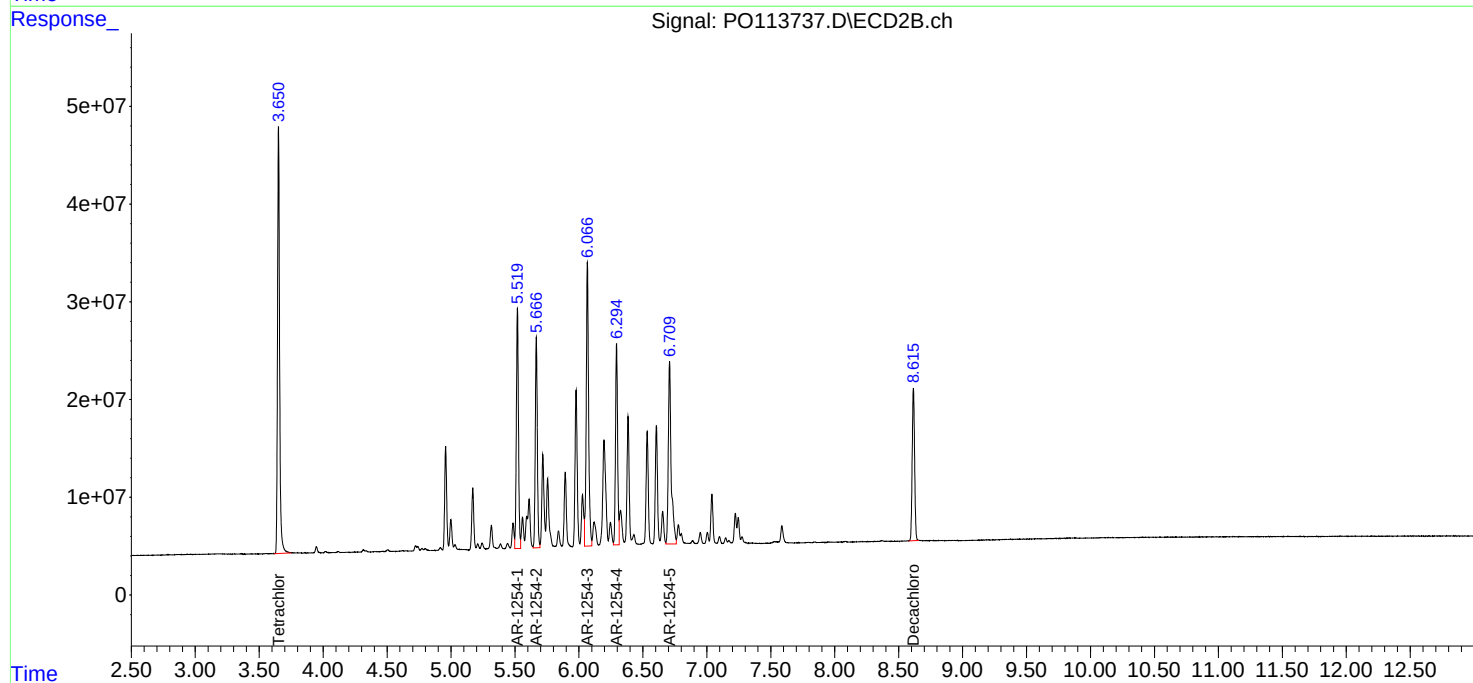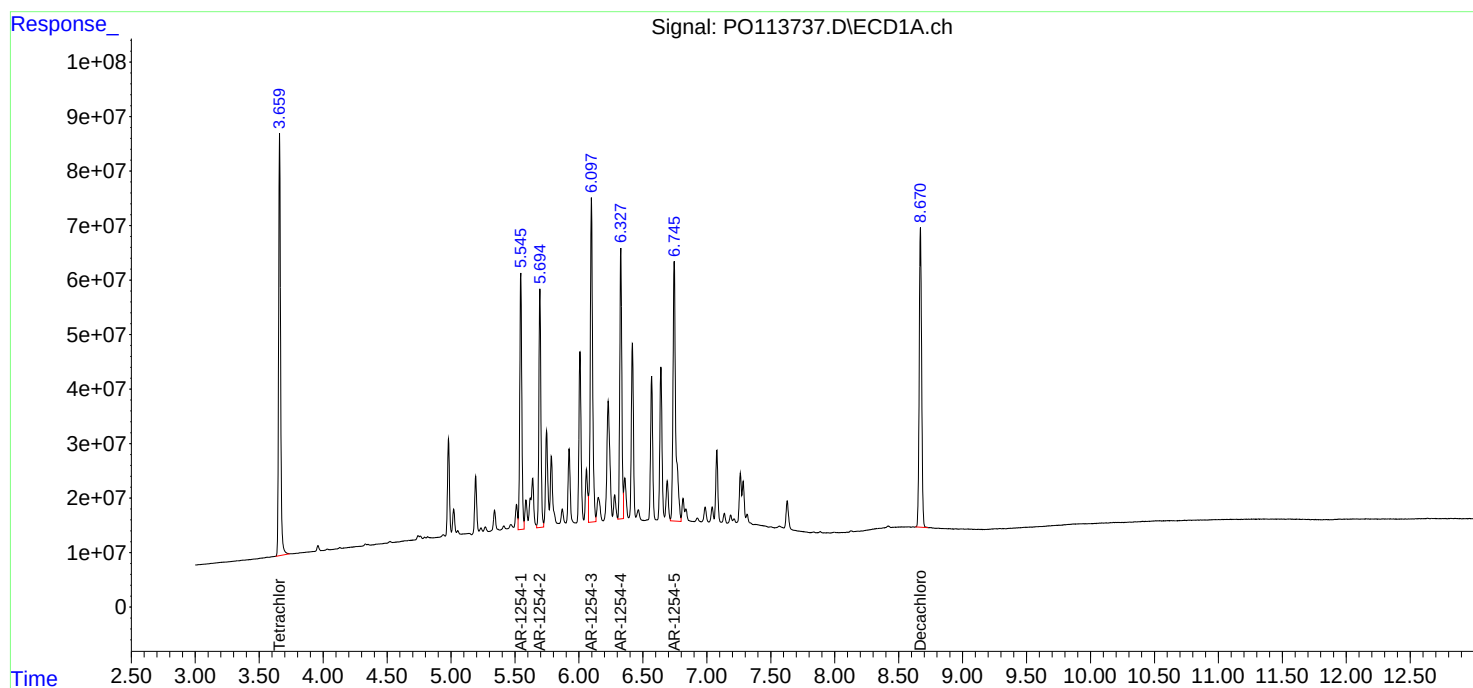

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113738.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 16:02
 Operator : YP/AJ
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 16:42:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 15 16:36:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.658	3.651	636.3E6	374.3E6	75.068	74.866
2) SA Decachlor...	8.668	8.613	552.3E6	155.6E6	74.727	74.646
Target Compounds						
26) L6 AR-1254-1	5.544	5.518	402.1E6	217.0E6	742.146	745.382
27) L6 AR-1254-2	5.693	5.666	366.4E6	188.0E6	739.478	745.446
28) L6 AR-1254-3	6.096	6.065	570.3E6	285.2E6	741.389	746.594
29) L6 AR-1254-4	6.326	6.293	424.0E6	181.9E6	744.553	746.305
30) L6 AR-1254-5	6.743	6.708	550.0E6	223.6E6	745.976	745.051



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113738.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 16:02
Operator : YP/AJ
Sample : AR1254ICC750
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 16:42:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 15 16:36:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

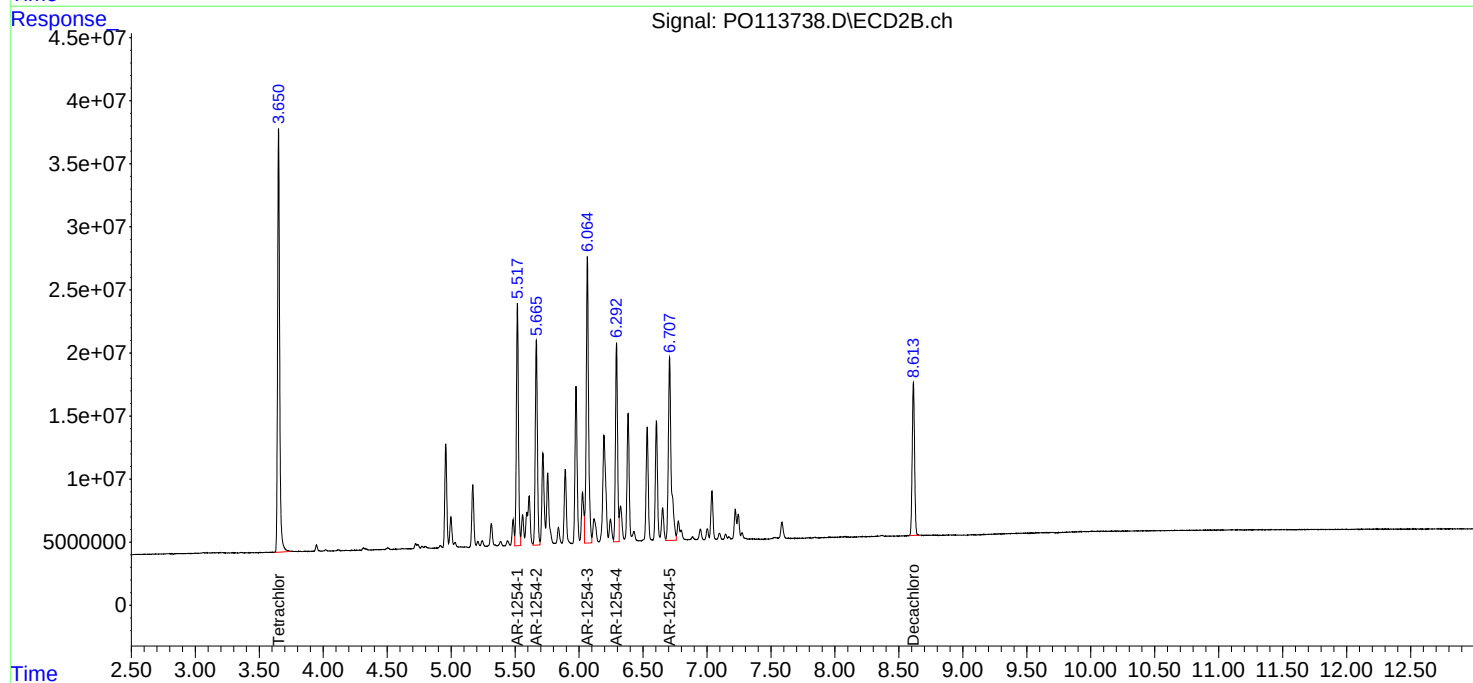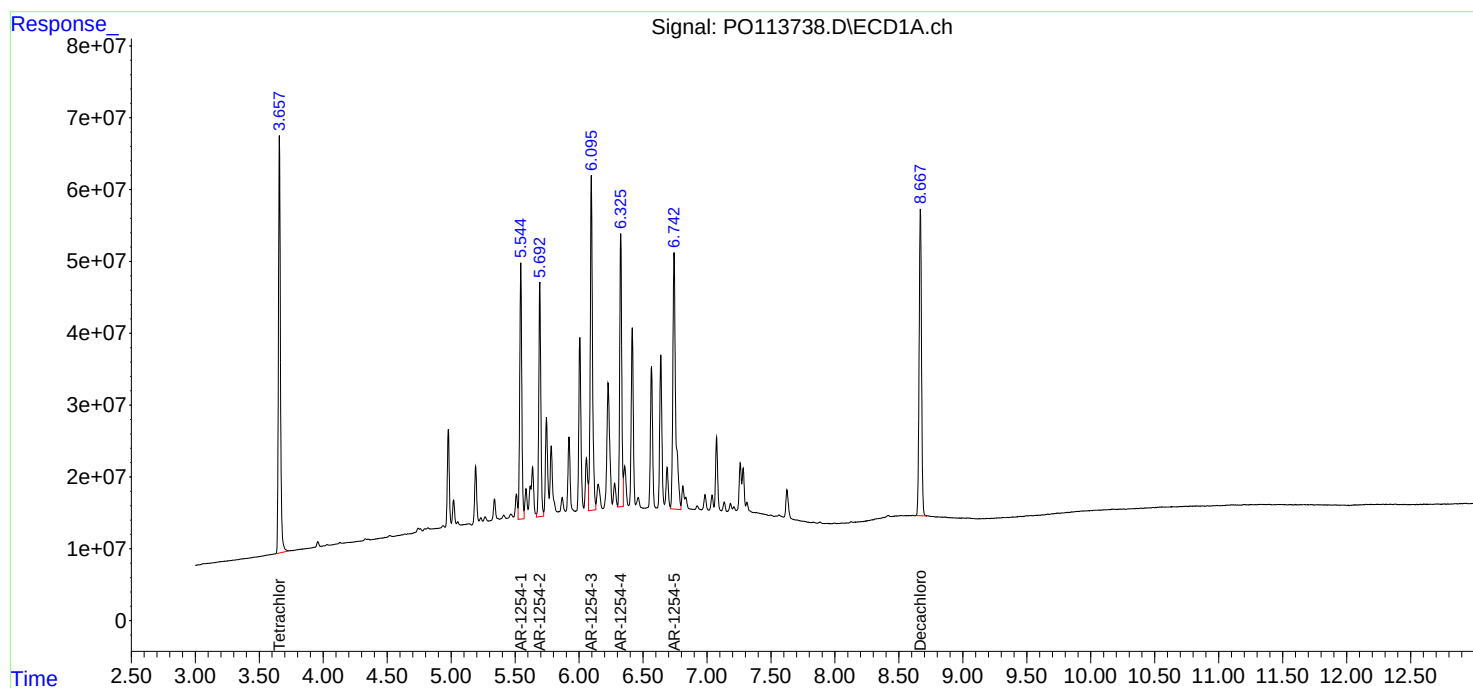

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113739.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 16:20
 Operator : YP/AJ
 Sample : AR1254ICC500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 16:36:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 15 16:36:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.651	431.0E6	255.1E6	50.000	50.000
2) SA Decachlor...	8.671	8.615	380.3E6	107.7E6	50.000	50.000
Target Compounds						
26) L6 AR-1254-1	5.546	5.519	282.1E6	152.2E6	500.000	500.000
27) L6 AR-1254-2	5.695	5.667	259.8E6	132.4E6	500.000	500.000
28) L6 AR-1254-3	6.098	6.066	400.3E6	197.5E6	500.000	500.000
29) L6 AR-1254-4	6.327	6.294	294.0E6	126.5E6	500.000	500.000
30) L6 AR-1254-5	6.745	6.708	380.2E6	155.9E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113739.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 16:20
Operator : YP/AJ
Sample : AR1254ICC500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 16:36:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 15 16:36:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

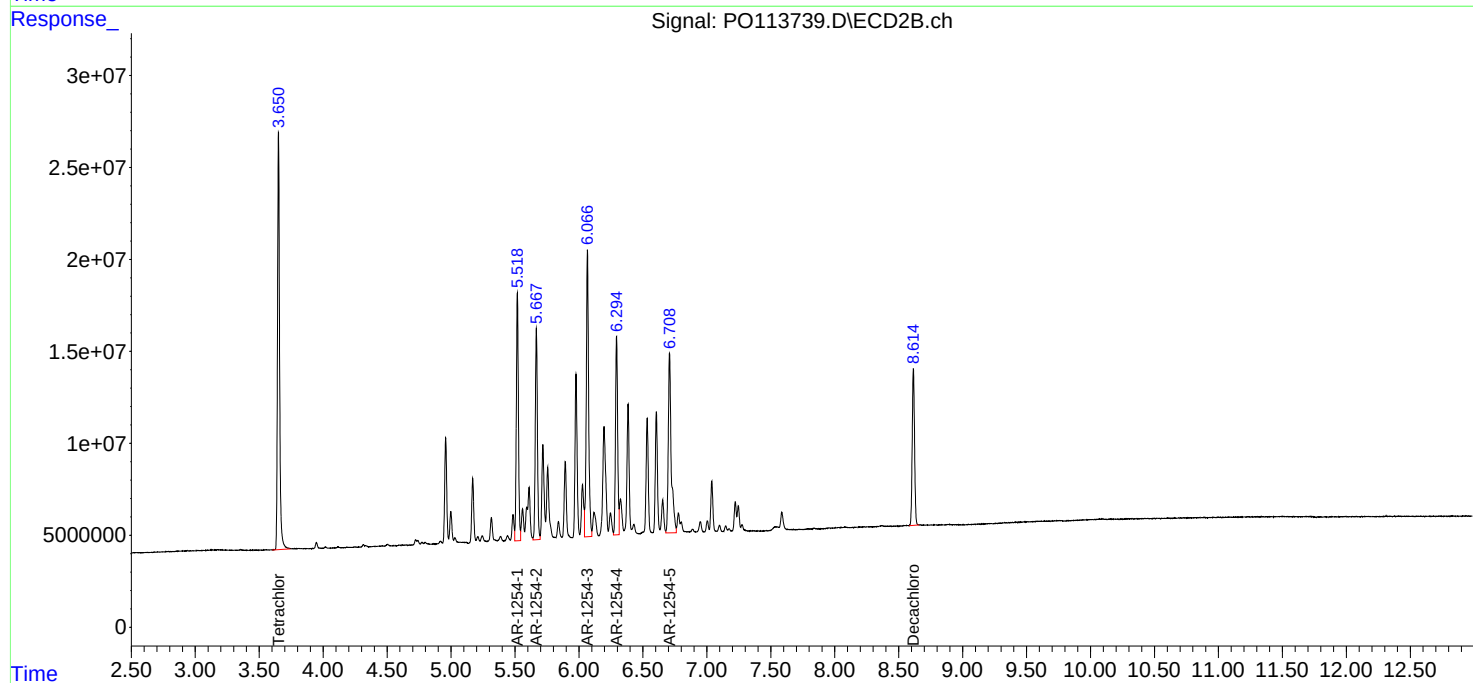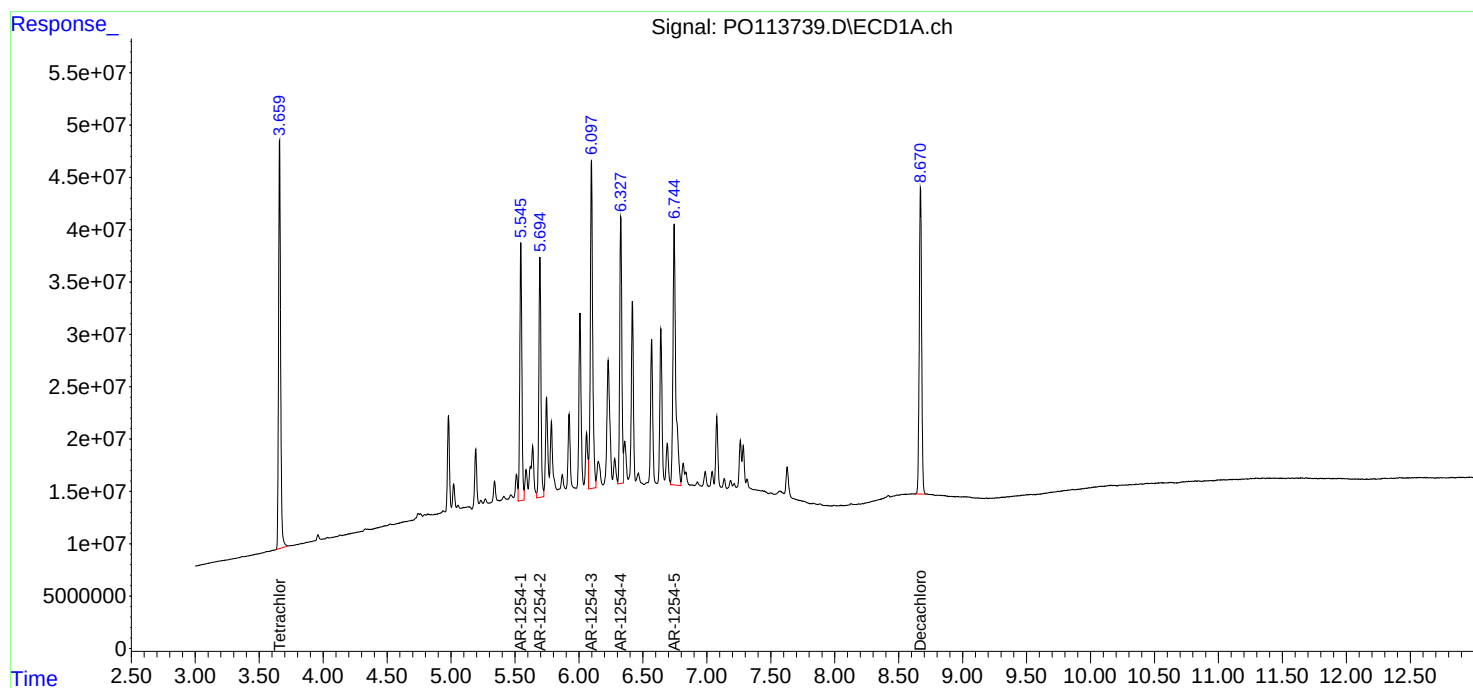

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113740.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 16:38
 Operator : YP/AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 16:53:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 15 16:52:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.658	3.650	227.0E6	135.8E6	26.310	26.589
2) SA Decachlor...	8.667	8.614	201.4E6	57331341	26.654	26.838
Target Compounds						
26) L6 AR-1254-1	5.545	5.518	155.3E6	84783533	276.504	279.737
27) L6 AR-1254-2	5.693	5.667	145.8E6	73758590	281.747	280.535
28) L6 AR-1254-3	6.096	6.066	222.6E6	108.3E6	278.402	274.343
29) L6 AR-1254-4	6.326	6.294	161.6E6	69525562	274.556	275.529
30) L6 AR-1254-5	6.743	6.708	198.8E6	85059150	264.465	274.289



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113740.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 16:38
Operator : YP/AJ
Sample : AR1254ICC250
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 16:53:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 15 16:52:59 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

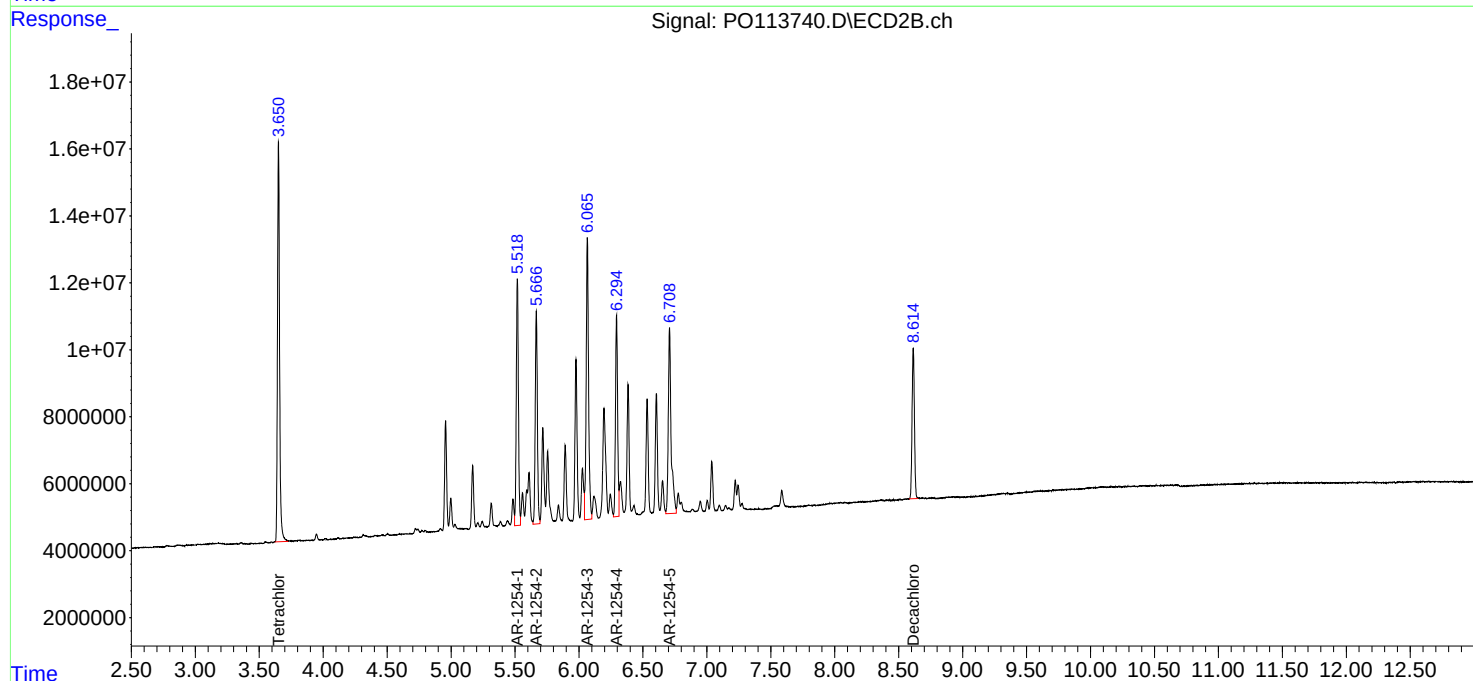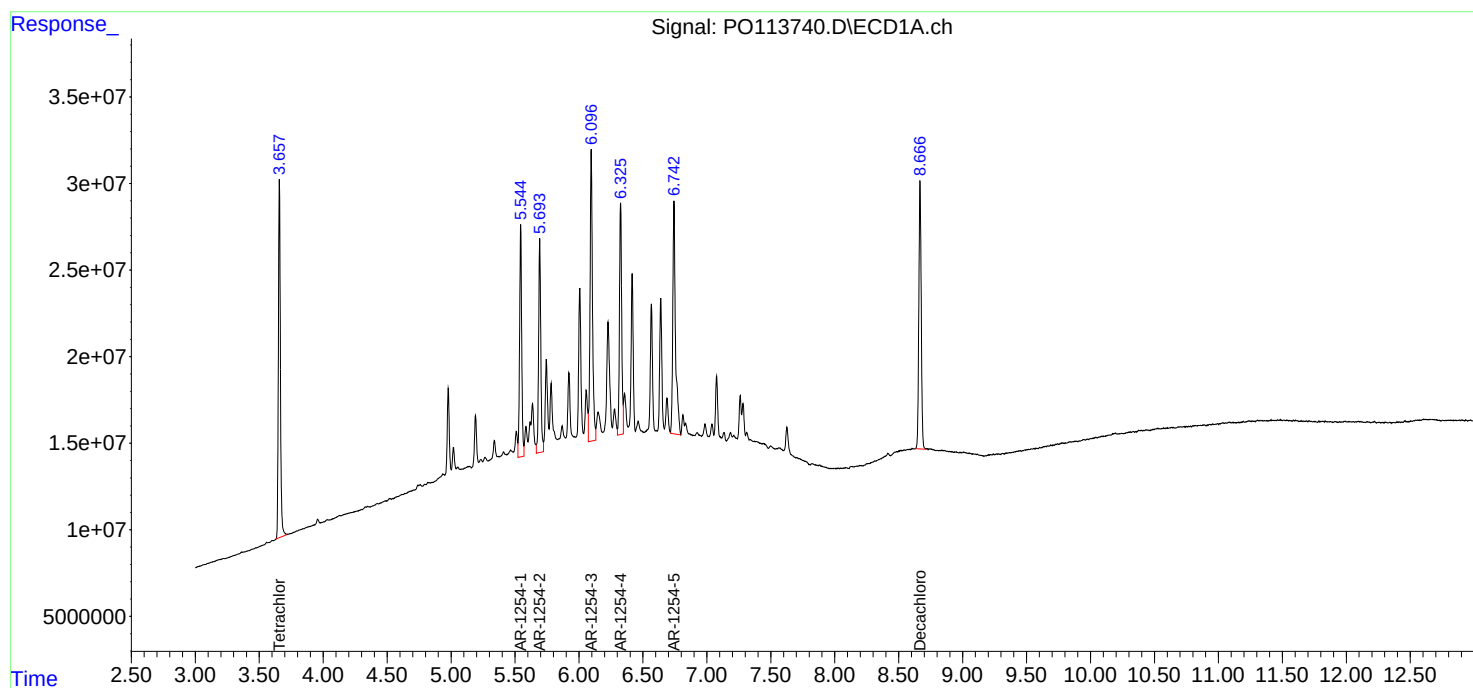

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0091525\
 Data File : P0113741.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 17:14
 Operator : YP/AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/16/2025
 Supervised By :mohammad ahmed 09/17/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 19:39:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 15 19:39:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.660	3.651	32604883	21214123	3.973	4.299
2) SA Decachlor...	8.671	8.615	30383689	8729895	4.184	4.242
Target Compounds						
26) L6 AR-1254-1	5.546	5.518	23962057	14982815	43.722m	49.547
27) L6 AR-1254-2	5.696	5.666	23644186	13435529	47.101m	50.877
28) L6 AR-1254-3	6.098	6.066	35630196	17869805	45.808m	46.137
29) L6 AR-1254-4	6.326	6.293	18974714	8881039	34.957m	37.411
30) L6 AR-1254-5	6.746	6.709	35724526	14721584	47.995	47.957

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO091525\
Data File : PO113741.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 17:14
Operator : YP/AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 49 Sample Multiplier: 1



Instrument :
ECD_0
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/16/2025
Supervised By :mohammad ahmed 09/17/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 19:39:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 15 19:39:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

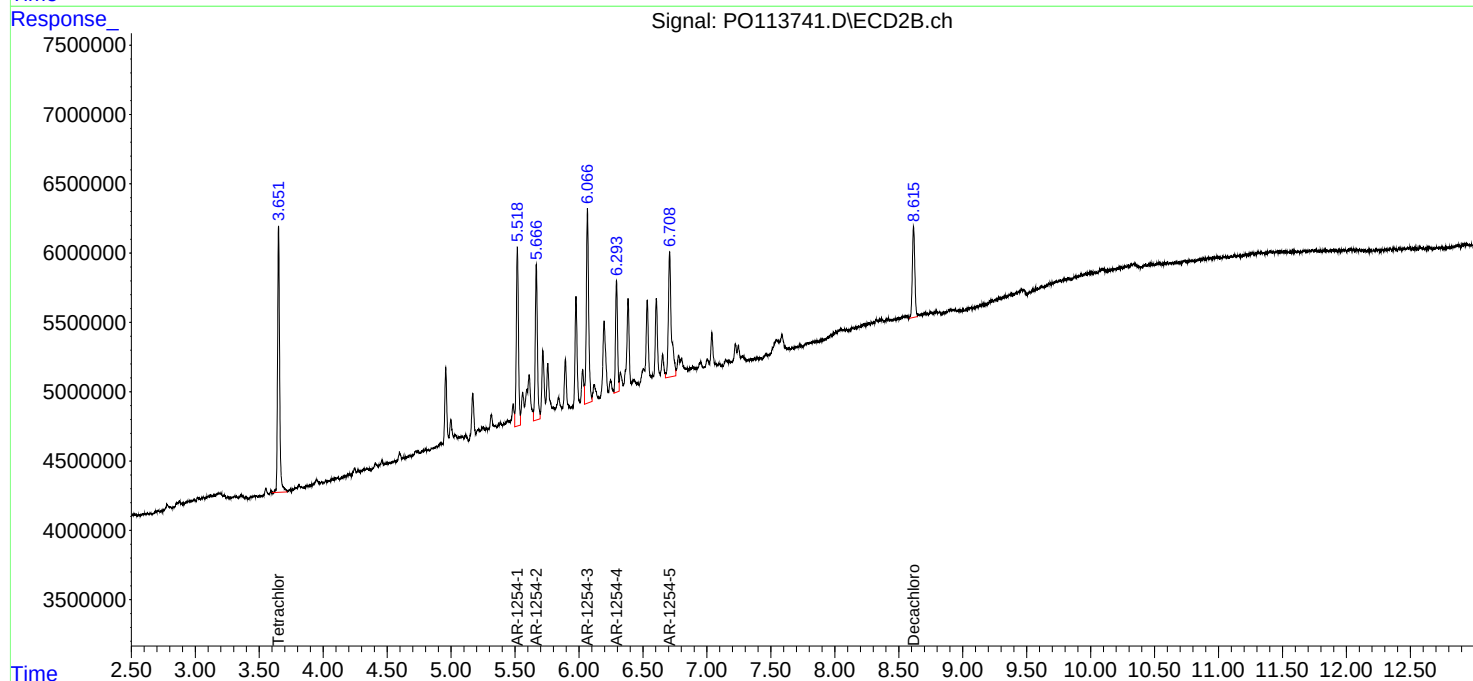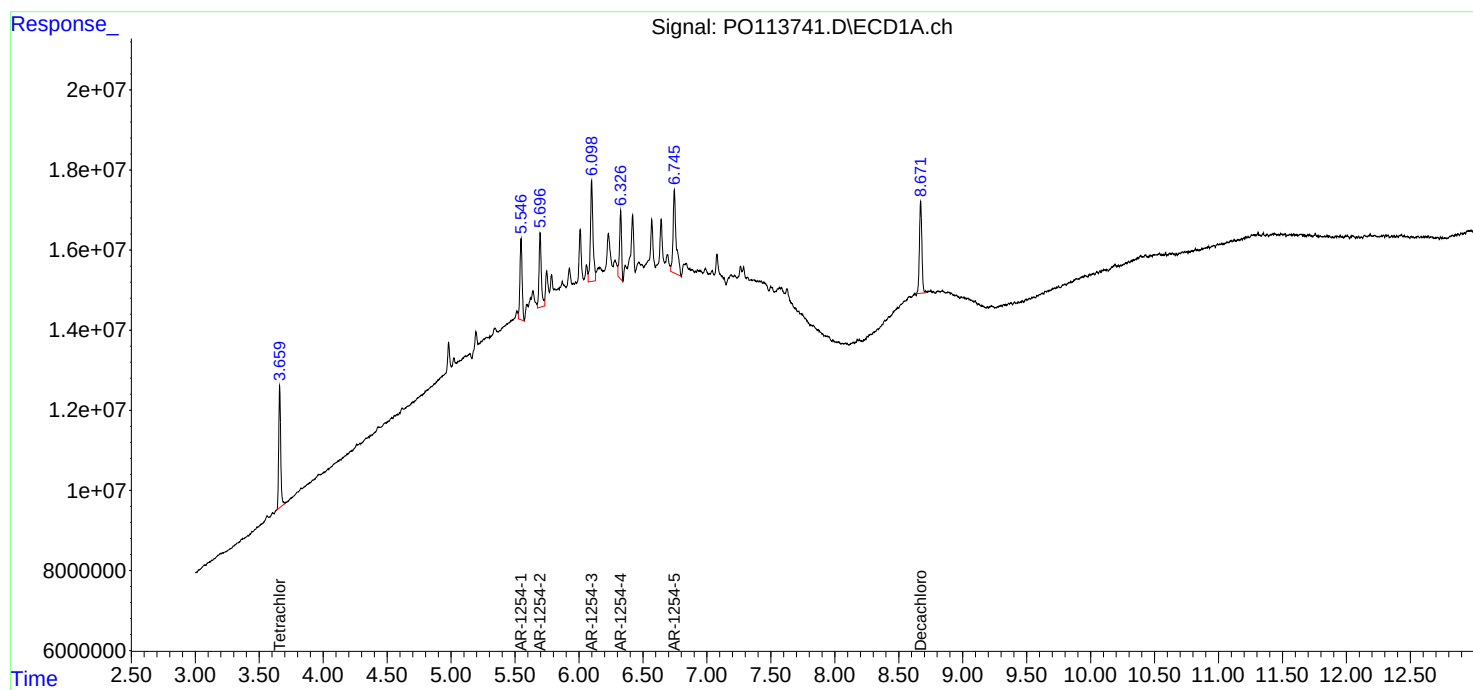

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113742.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 17:33
 Operator : YP/AJ
 Sample : AR1262ICC500
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1262ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 01:50:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 01:47:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.650	426.8E6	253.6E6	50.000	50.000
2) SA Decachlor...	8.669	8.615	383.5E6	108.0E6	50.000	50.000
Target Compounds						
36) L8 AR-1262-1	6.783	6.747	496.2E6	183.1E6	500.000	500.000
37) L8 AR-1262-2	7.286	7.246	792.1E6	228.3E6	500.000	500.000
38) L8 AR-1262-3	7.567	7.526	279.6E6	87099423	500.000	500.000
39) L8 AR-1262-4	7.632	7.591	500.1E6	139.0E6	500.000	500.000
40) L8 AR-1262-5	8.127	8.082	199.6E6	56842713	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113742.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 17:33
Operator : YP/AJ
Sample : AR1262ICC500
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1262ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 01:50:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 01:47:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

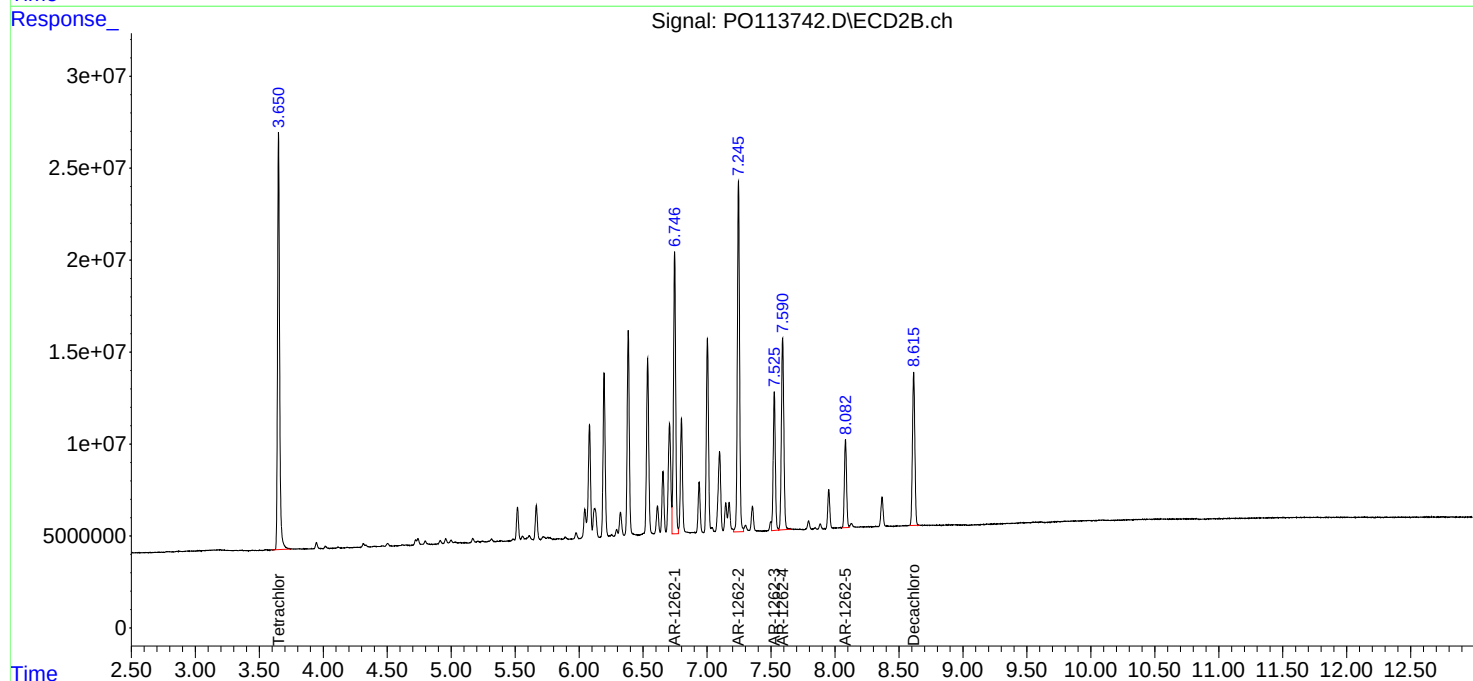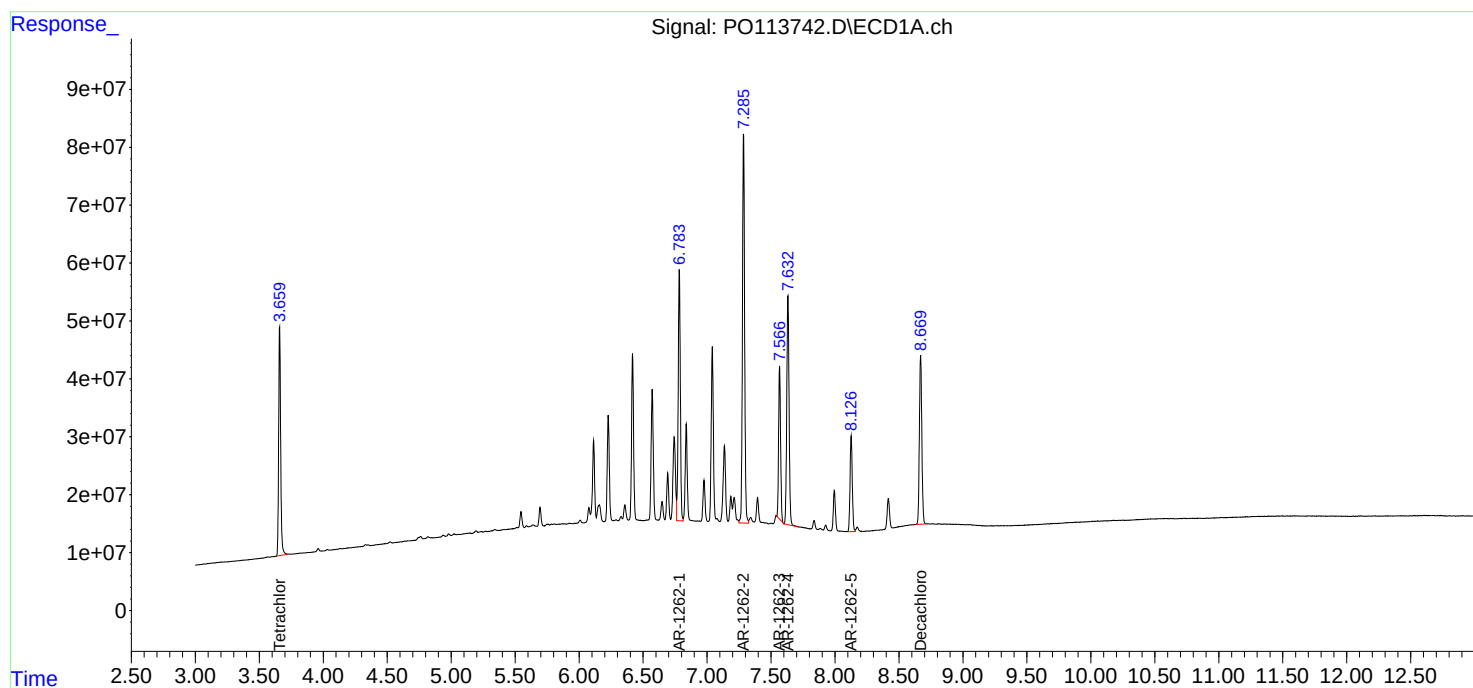

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113743.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 17:51
 Operator : YP/AJ
 Sample : AR1268ICC1000
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 02:03:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:01:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.660	3.651	865.0E6	509.2E6	99.055	98.843
2) SA Decachlor...	8.670	8.616	1381.3E6	381.2E6	99.482	97.437
Target Compounds						
41) L9 AR-1268-1	7.568	7.528	1758.9E6	463.8E6	984.979	956.606
42) L9 AR-1268-2	7.634	7.593	1483.0E6	382.6E6	983.516	955.801
43) L9 AR-1268-3	7.837	7.796	1211.4E6	309.5E6	976.404	960.140
44) L9 AR-1268-4	8.127	8.084	446.3E6	126.2E6	970.520	979.192
45) L9 AR-1268-5	8.419	8.369	3223.0E6	880.6E6	1011.065	983.971



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113743.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 17:51
Operator : YP/AJ
Sample : AR1268ICC1000
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 02:03:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:01:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

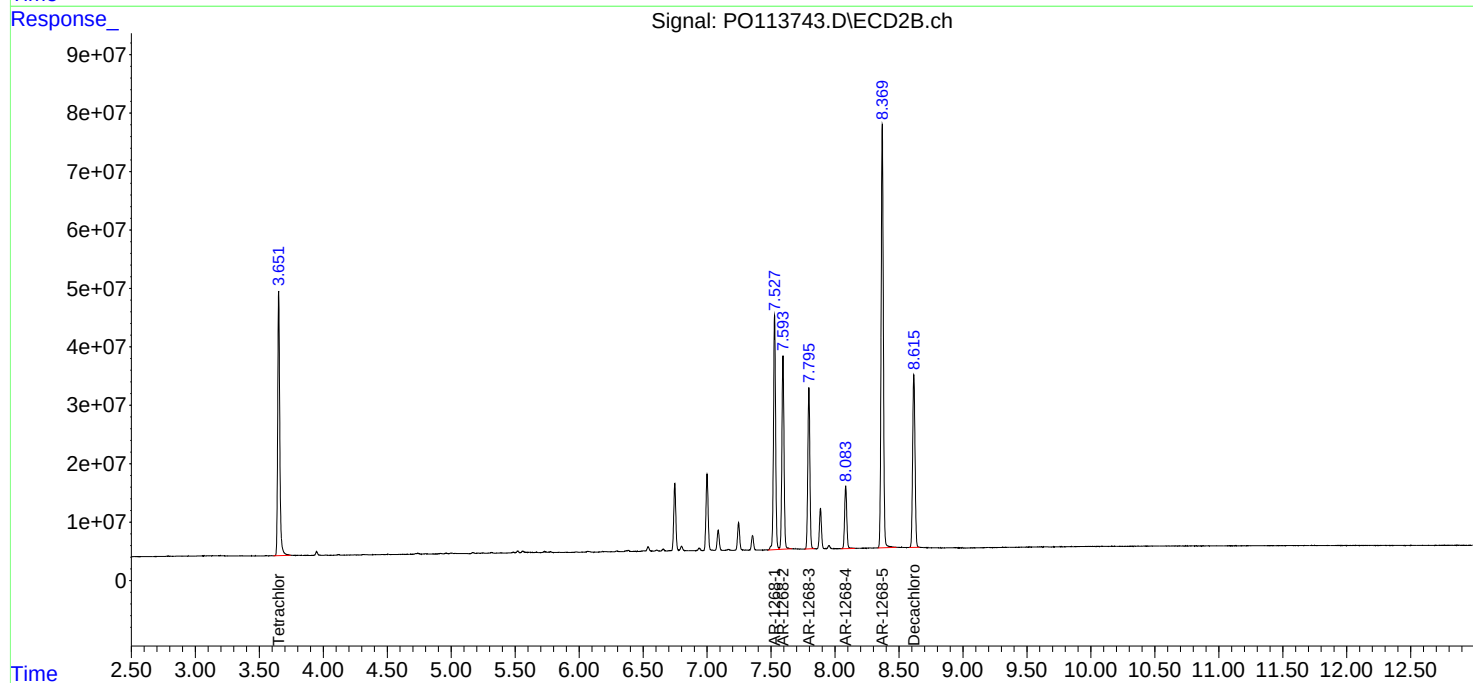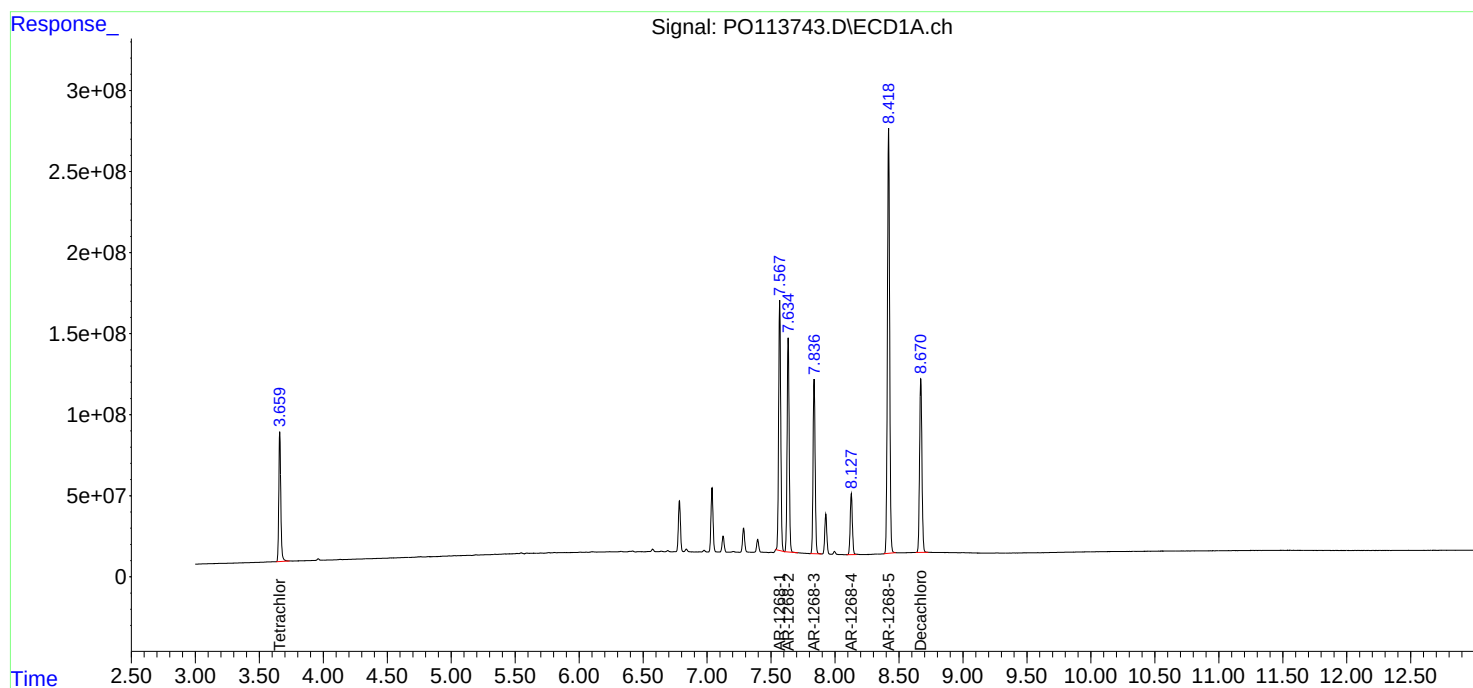

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113744.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 18:10
 Operator : YP/AJ
 Sample : AR1268ICC750
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 02:03:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:01:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.660	3.651	631.3E6	372.8E6	72.285	72.363
2) SA Decachlor...	8.669	8.614	1006.0E6	280.2E6	72.451	71.610
Target Compounds						
41) L9 AR-1268-1	7.566	7.525	1282.4E6	345.8E6	718.100	713.212
42) L9 AR-1268-2	7.633	7.591	1087.7E6	286.0E6	721.344	714.685
43) L9 AR-1268-3	7.836	7.794	893.2E6	230.7E6	719.893	715.611
44) L9 AR-1268-4	8.126	8.082	329.5E6	91925617	716.601	713.429
45) L9 AR-1268-5	8.417	8.368	2320.8E6	642.3E6	728.041	717.663


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113744.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 18:10
Operator : YP/AJ
Sample : AR1268ICC750
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 02:03:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:01:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

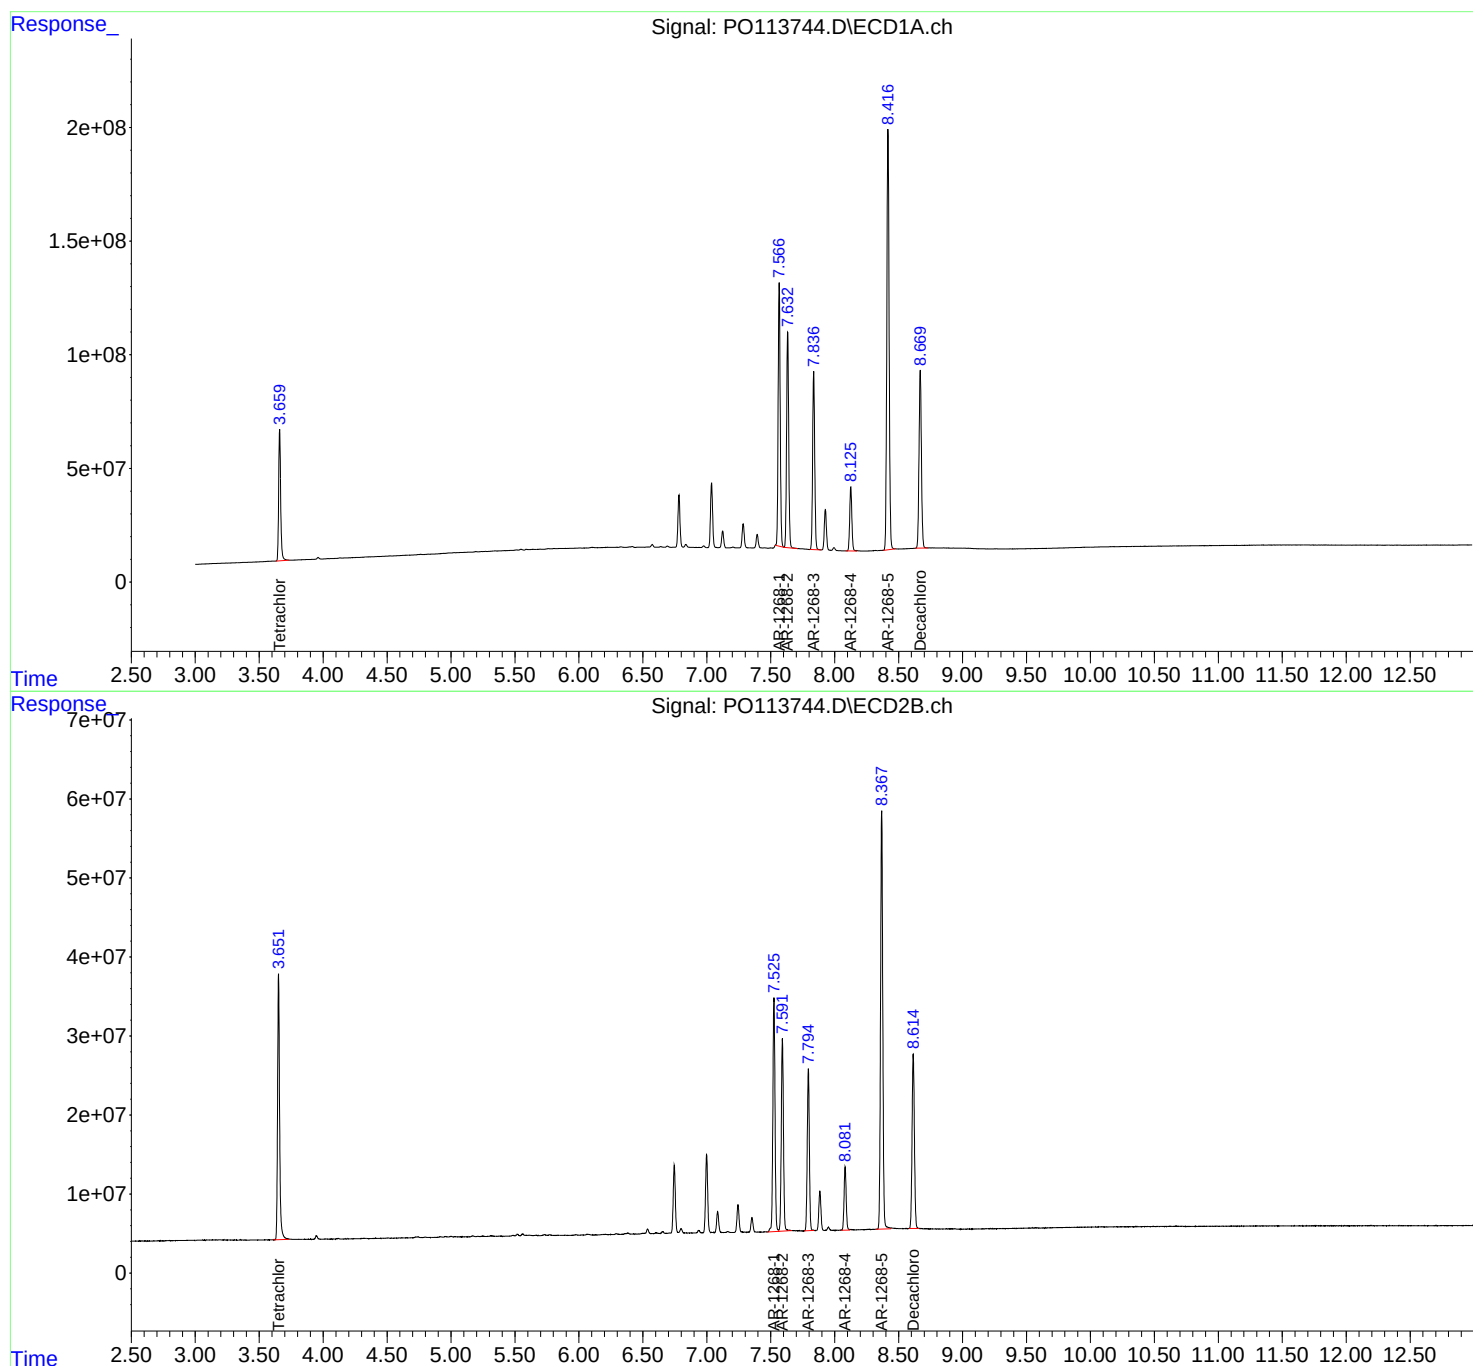

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0091525\
 Data File : P0113745.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 18:27
 Operator : YP/AJ
 Sample : AR1268ICC500
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1268ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 02:03:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:01:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.658	3.651	436.7E6	257.6E6	50.000	50.000
2) SA Decachlor...	8.669	8.614	694.3E6	195.6E6	50.000	50.000
Target Compounds						
41) L9 AR-1268-1	7.567	7.526	892.9E6	242.4E6	500.000	500.000
42) L9 AR-1268-2	7.632	7.592	753.9E6	200.1E6	500.000	500.000
43) L9 AR-1268-3	7.836	7.794	620.4E6	161.2E6	500.000	500.000
44) L9 AR-1268-4	8.125	8.082	229.9E6	64425183	500.000	500.000
45) L9 AR-1268-5	8.417	8.368	1593.8E6	447.5E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113745.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 18:27
Operator : YP/AJ
Sample : AR1268ICC500
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 02:03:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:01:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

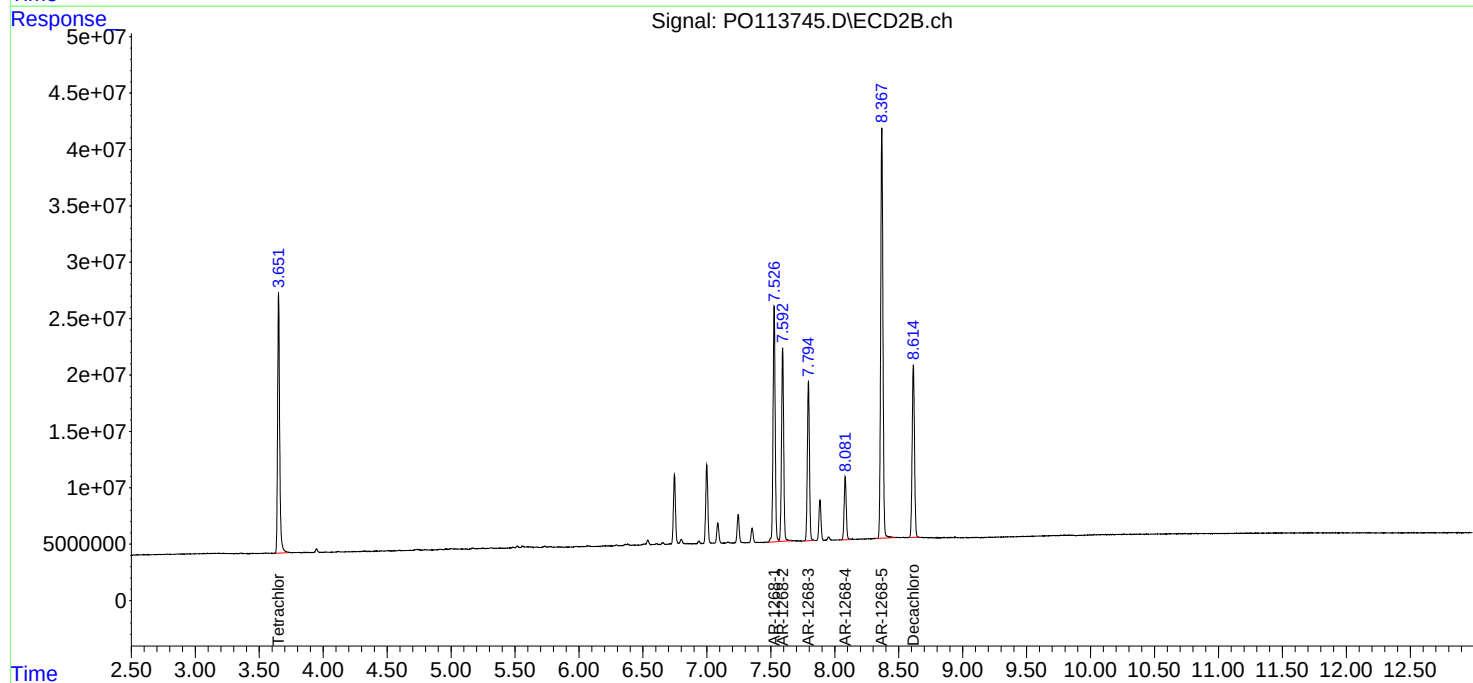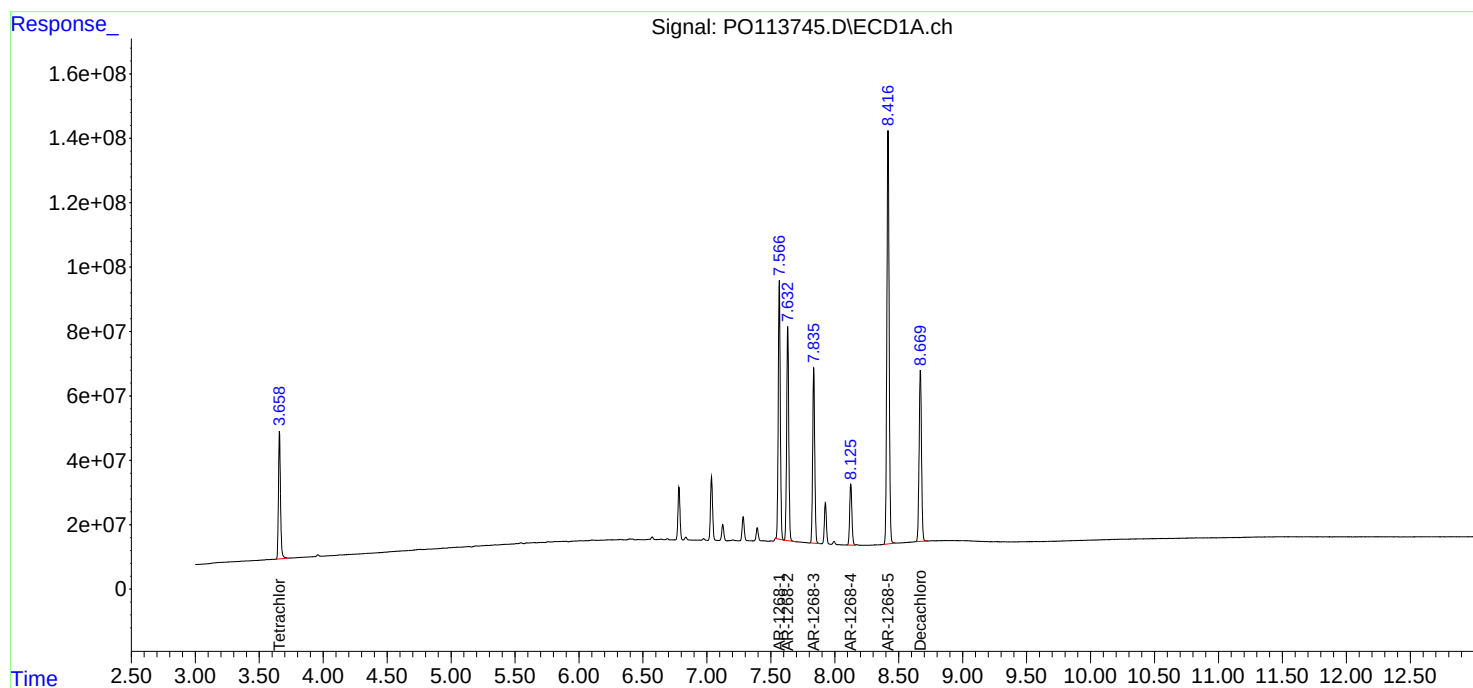

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0091525\
 Data File : P0113746.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 18:45
 Operator : YP/AJ
 Sample : AR1268ICC250
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1268ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 02:04:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:01:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.651	237.7E6	142.4E6	27.220	27.635
2) SA Decachlor...	8.670	8.615	376.2E6	108.7E6	27.093	27.779
Target Compounds						
41) L9 AR-1268-1	7.567	7.526	486.3E6	138.1E6	272.310	284.836
42) L9 AR-1268-2	7.633	7.592	409.7E6	112.7E6	271.717	281.690
43) L9 AR-1268-3	7.837	7.794	338.7E6	90329232	272.965	280.208
44) L9 AR-1268-4	8.126	8.082	124.8E6	35449635	271.479	275.123
45) L9 AR-1268-5	8.418	8.368	854.3E6	245.3E6	267.989	274.088



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO091525\
Data File : PO113746.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 18:45
Operator : YP/AJ
Sample : AR1268ICC250
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_0
ClientSampleId :
AR1268ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 02:04:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:01:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

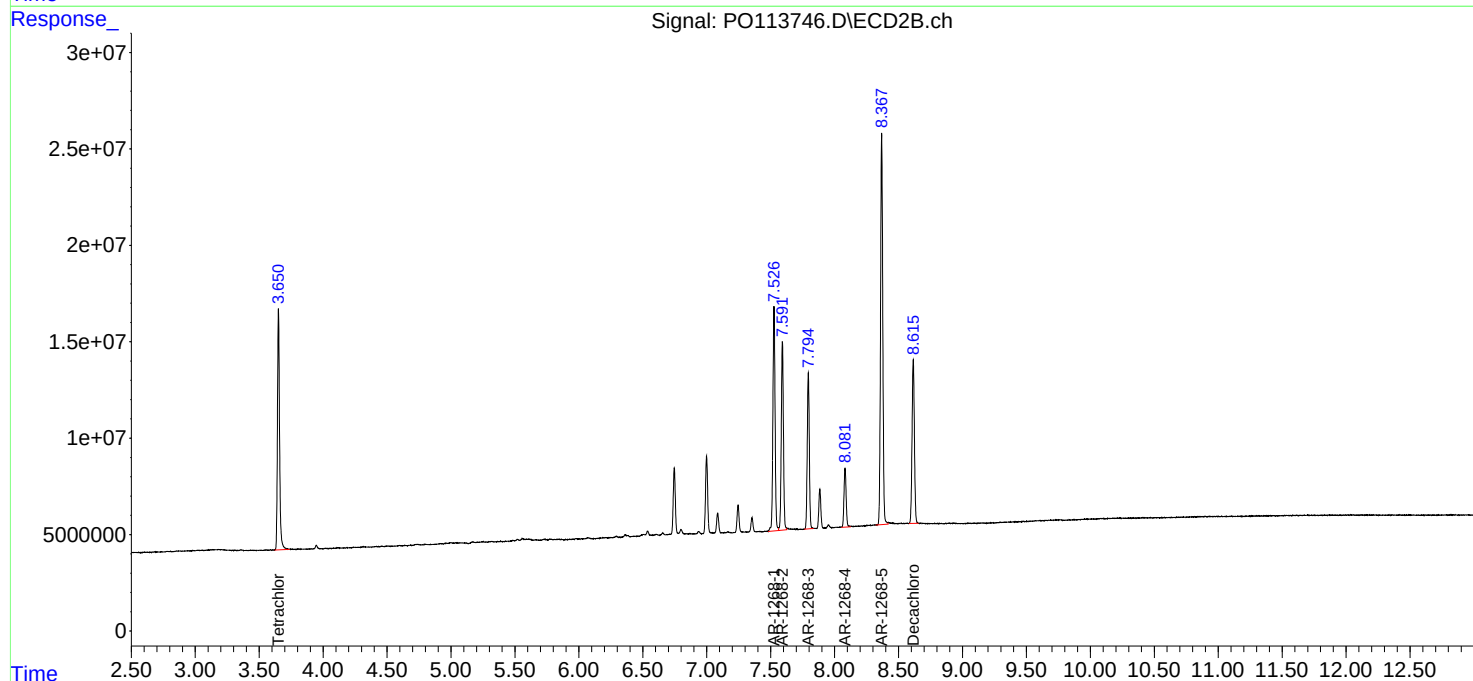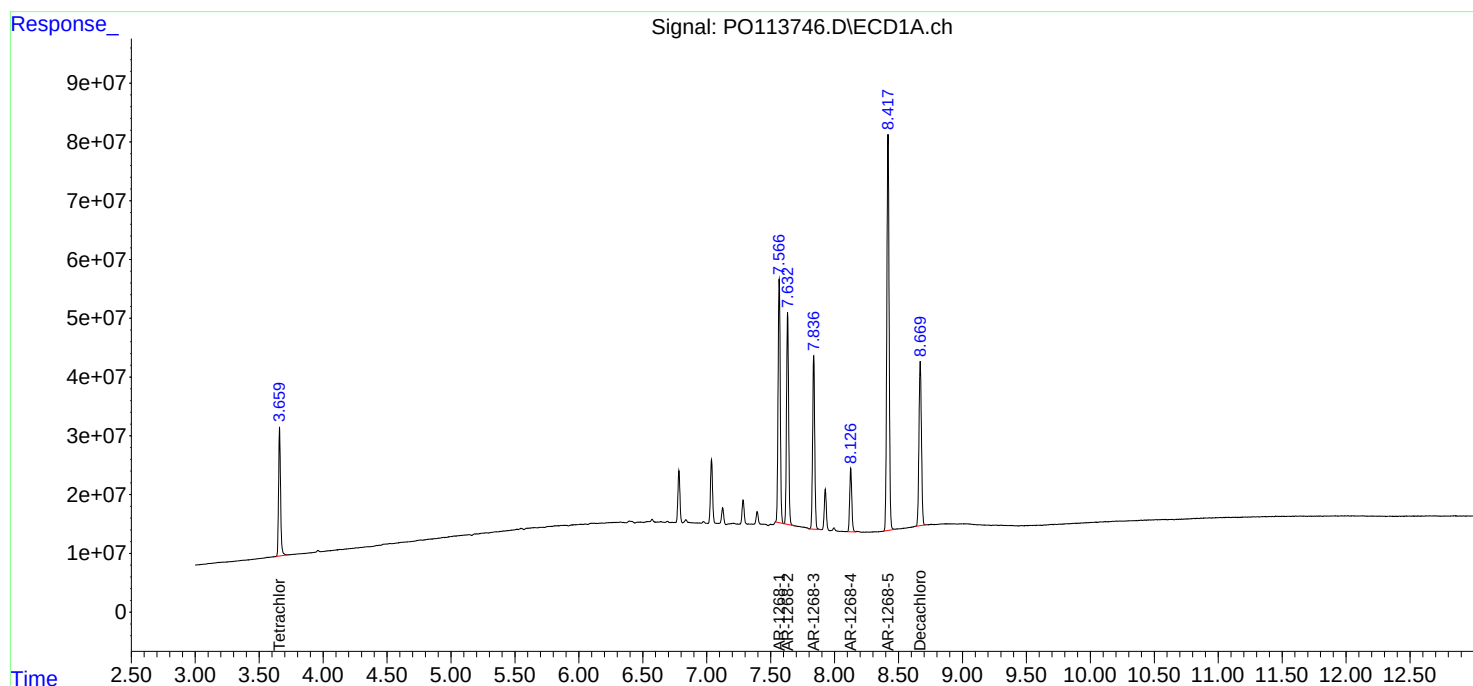

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0091525\
 Data File : P0113747.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 19:21
 Operator : YP/AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1268ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/16/2025
 Supervised By :mohammad ahmed 09/17/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 02:19:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:01:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.650	33720326	21028789	3.567m	3.698m
2) SA Decachlor...	8.669	8.614	59999796	17591430	3.987	4.109
Target Compounds						
41) L9 AR-1268-1	7.567	7.525	82715552	23926524	42.364	43.669m
42) L9 AR-1268-2	7.633	7.591	68138068	18835061	41.307	41.950m
43) L9 AR-1268-3	7.835	7.794	55807392	16548138	41.472m	46.525m
44) L9 AR-1268-4	8.127	8.082	21450005	5726150	43.328	40.814
45) L9 AR-1268-5	8.418	8.368	134.1E6	39149700	38.910	39.977

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO091525\
Data File : PO113747.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 19:21
Operator : YP/AJ
Sample : AR1268ICC050
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_0
ClientSampleId :
AR1268ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/16/2025
Supervised By :mohammad ahmed 09/17/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 02:19:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:01:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

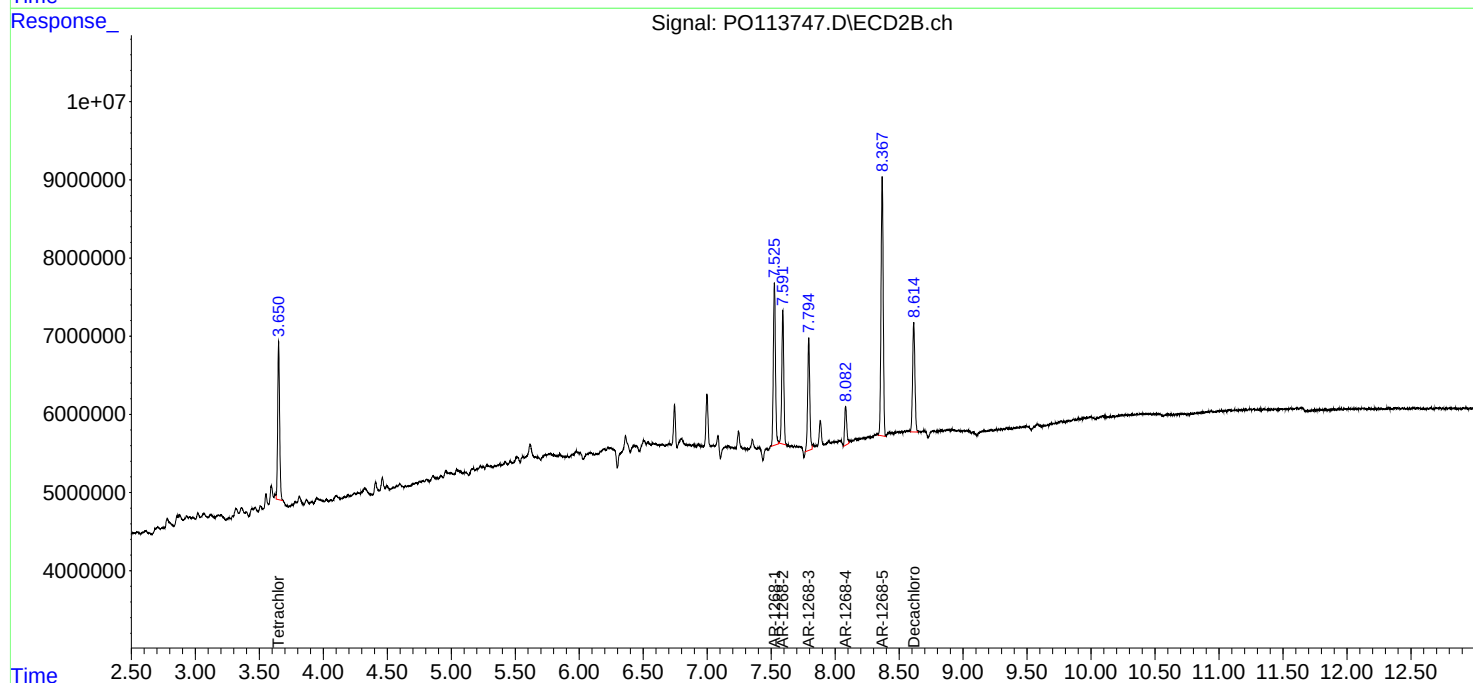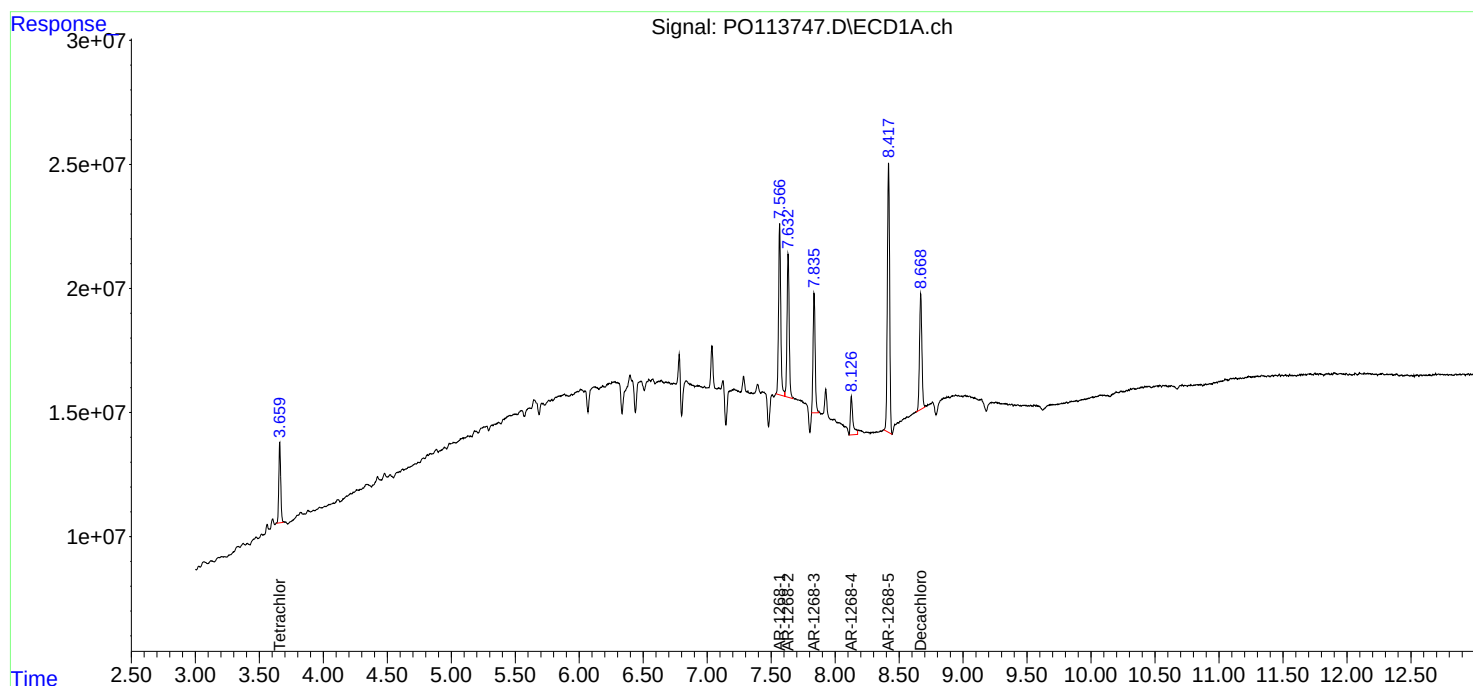

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0091525\
 Data File : P0113748.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 19:40
 Operator : YP/AJ
 Sample : P0091525ICV500
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 ICVPO091525

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/16/2025
 Supervised By :mohammad ahmed 09/17/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:17:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:49:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.660	3.651	421.1E6	252.3E6	47.750	47.245
2) SA Decachlor...	8.670	8.615	368.7E6	107.8E6	55.107	51.617
Target Compounds						
3) L1 AR-1016-1	4.743	4.723	139.9E6	84089553	460.962	461.418
4) L1 AR-1016-2	4.761	4.740	212.9E6	126.5E6	467.739	456.868
5) L1 AR-1016-3	4.818	4.916	135.0E6	68594551	451.043	459.307
6) L1 AR-1016-4	4.938	4.958	109.1E6	55712186	453.898	461.540
7) L1 AR-1016-5	5.194	5.169	122.7E6	71059159	511.019	473.519
31) L7 AR-1260-1	6.229	6.196	241.9E6	115.4E6	493.521	459.332
32) L7 AR-1260-2	6.419	6.384	365.4E6	150.9E6	477.120	456.489
33) L7 AR-1260-3	6.783	6.535	329.0E6	123.7E6	488.937	441.186
34) L7 AR-1260-4	7.042	7.003	241.8E6	88225295	558.825	461.402
35) L7 AR-1260-5	7.285	7.246	634.2E6	195.2E6	559.829m	458.660

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113748.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 19:40
Operator : YP/AJ
Sample : PO091525ICV500
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ICVPO091525

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/16/2025
Supervised By :mohammad ahmed 09/17/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:17:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

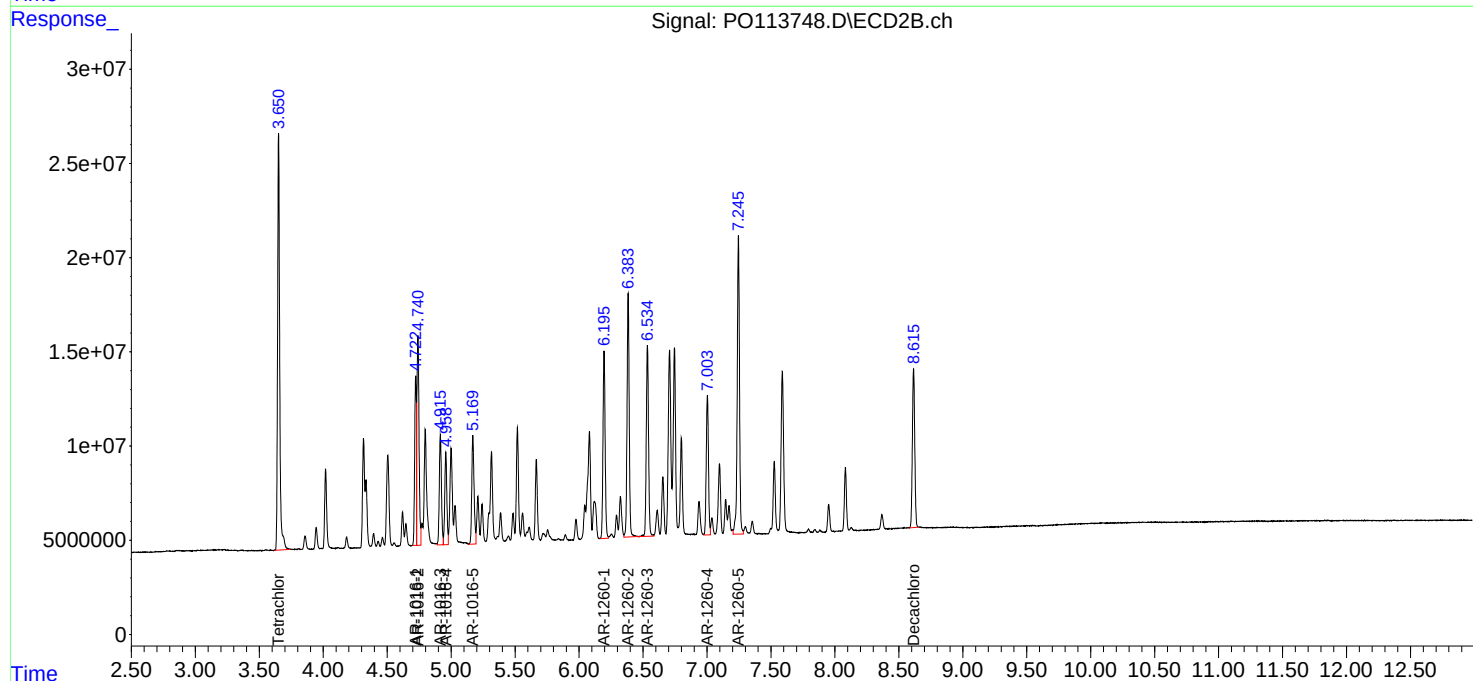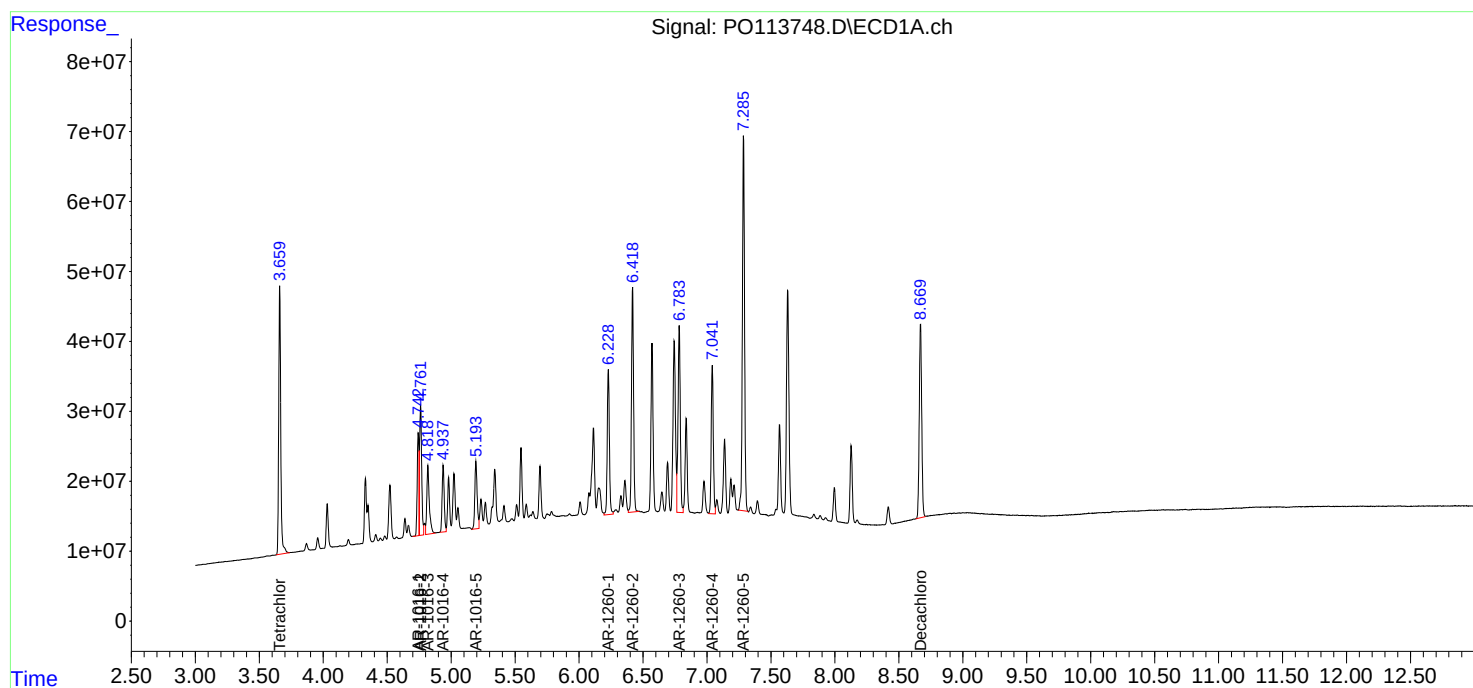

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113749.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 20:16
 Operator : YP/AJ
 Sample : AR1242ICV500
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO091525AR1242

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:17:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:49:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.657	3.650	441.4E6	263.1E6	50.044	49.252
2) SA Decachlor...	8.668	8.614	381.6E6	113.9E6	57.032	54.539
Target Compounds						
16) L4 AR-1242-1	4.740	4.722	123.8E6	74583010	557.090	546.627
17) L4 AR-1242-2	4.758	4.740	191.7E6	114.6E6	570.198	552.993
18) L4 AR-1242-3	4.816	4.915	121.2E6	61579269	563.714	530.803
19) L4 AR-1242-4	4.935	4.999	96419332	59974944	551.225	521.534
20) L4 AR-1242-5	5.585	5.517	115.6E6	74740078	552.190	526.903



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113749.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 20:16
Operator : YP/AJ
Sample : AR1242ICV500
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO091525AR1242

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:17:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

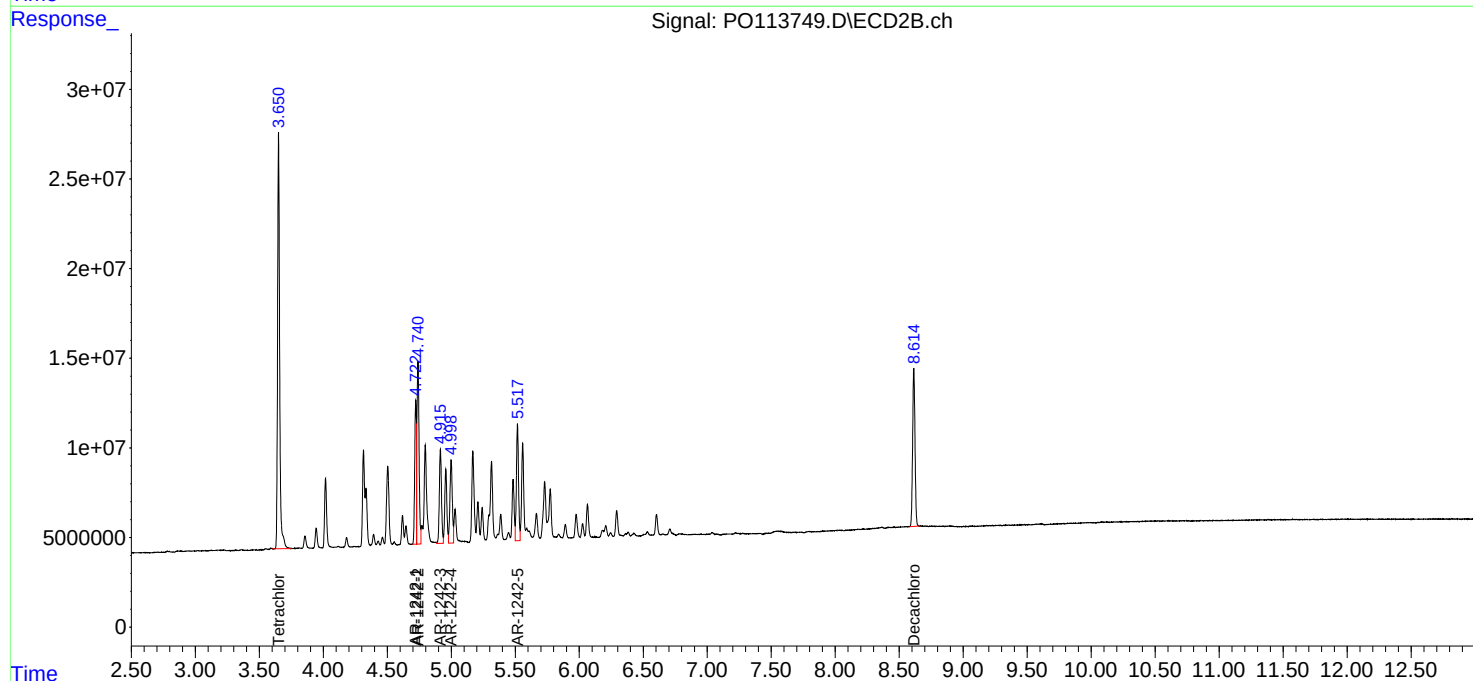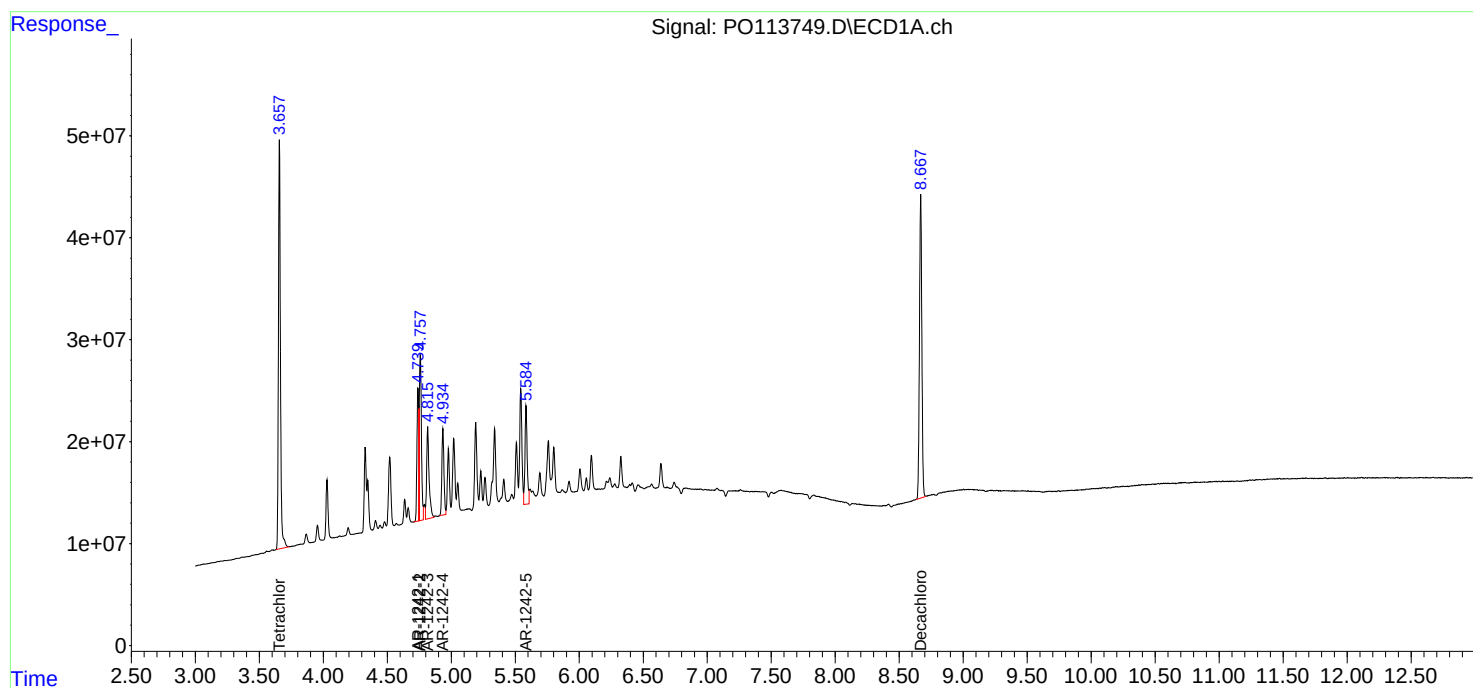

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113750.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 21:11
 Operator : YP/AJ
 Sample : AR1248ICV500
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO091525AR1248

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:17:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:49:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.650	438.0E6	259.4E6	49.663	48.576
2) SA Decachlor...	8.670	8.614	383.1E6	115.5E6	57.257	55.337
Target Compounds						
21) L5 AR-1248-1	4.742	4.722	94445285	58206014	523.909	532.408
22) L5 AR-1248-2	4.980	4.958	129.9E6	82371105	534.029	522.742
23) L5 AR-1248-3	5.193	4.999	171.2E6	86721195	527.568	519.554
24) L5 AR-1248-4	5.545	5.169	270.3E6	100.9E6	540.341	519.466
25) L5 AR-1248-5	5.587	5.558	189.4E6	102.3E6	560.046	504.416



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113750.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 21:11
Operator : YP/AJ
Sample : AR1248ICV500
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO091525AR1248

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:17:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

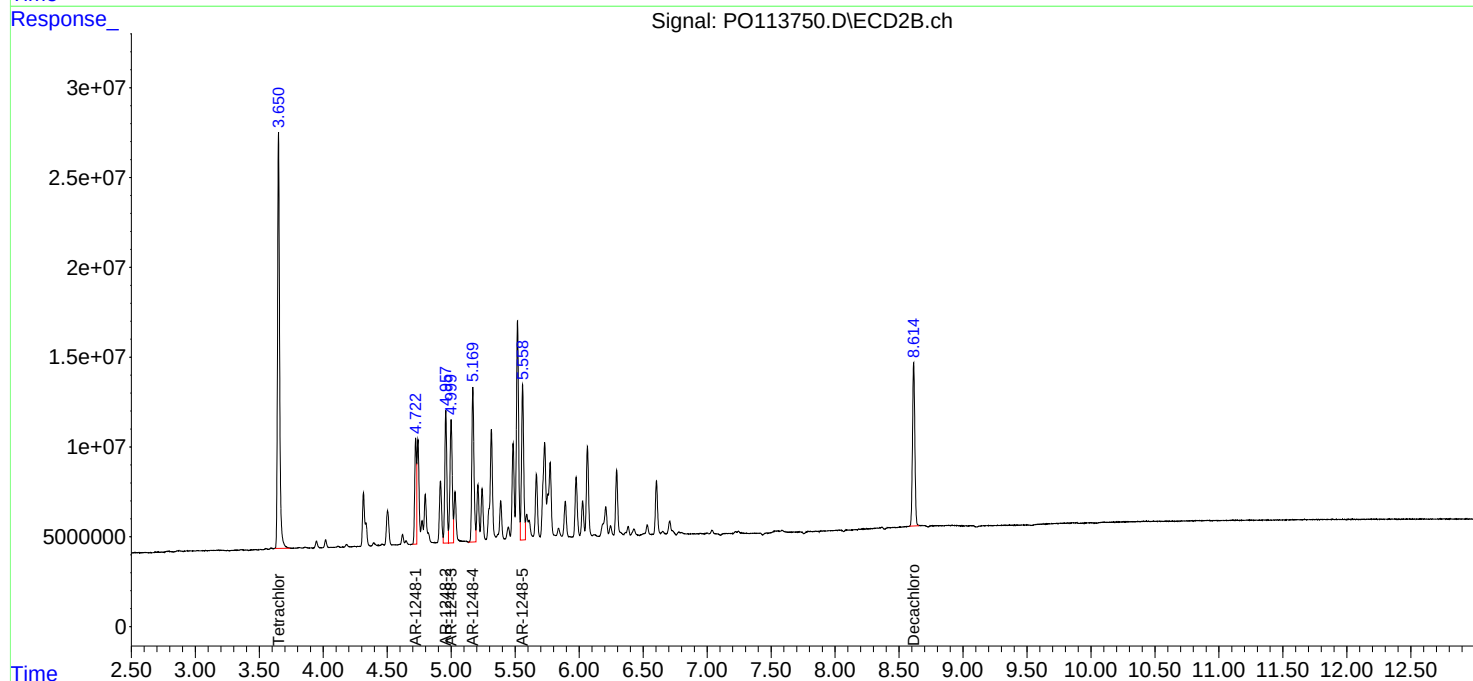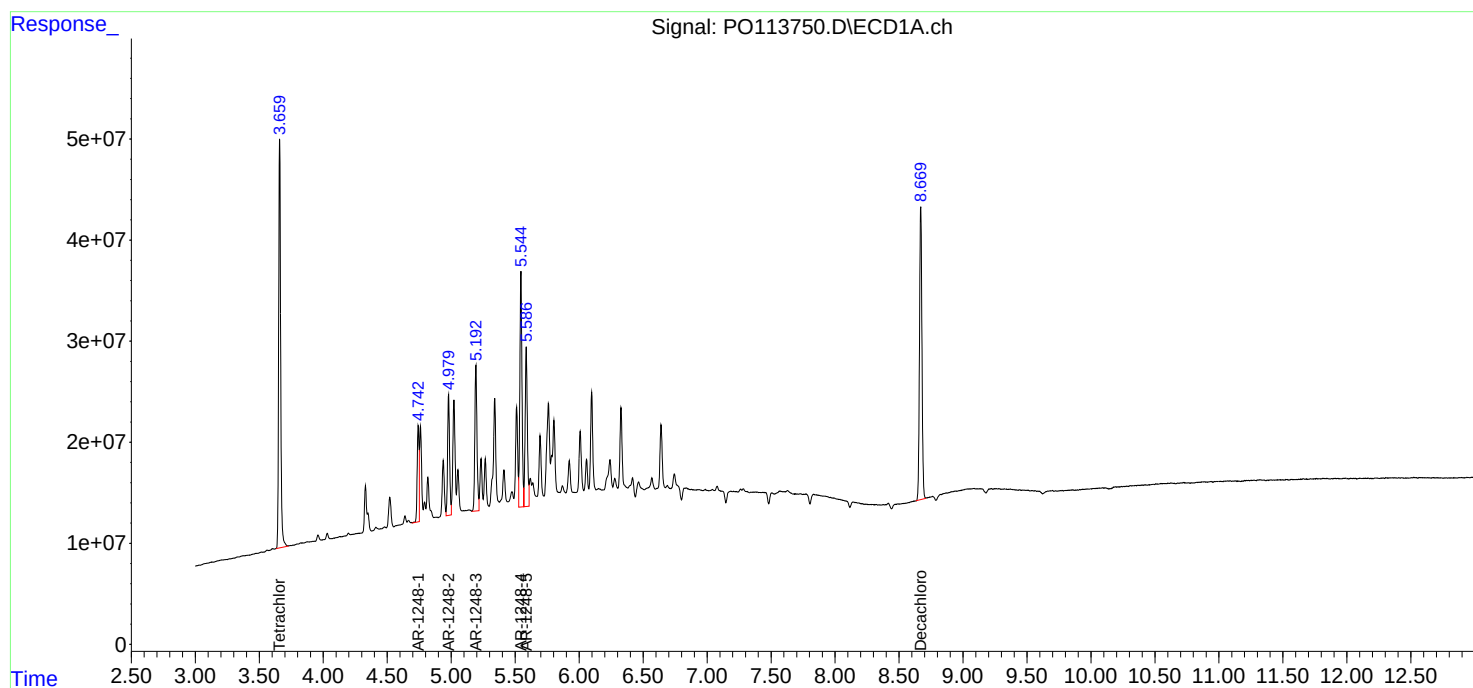

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113751.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 22:05
 Operator : YP/AJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO091525AR1254

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:31:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:49:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.660	3.651	440.3E6	259.3E6	49.924	48.556
2) SA Decachlor...	8.670	8.614	371.3E6	112.9E6	55.506	54.082
Target Compounds						
26) L6 AR-1254-1	5.546	5.518	282.3E6	154.3E6	517.827	510.406
27) L6 AR-1254-2	5.695	5.666	257.8E6	134.1E6	507.105	507.836
28) L6 AR-1254-3	6.098	6.065	403.2E6	201.1E6	515.520	519.138
29) L6 AR-1254-4	6.327	6.293	292.8E6	127.5E6	535.416	537.239
30) L6 AR-1254-5	6.745	6.708	386.2E6	158.2E6	518.905	515.275



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113751.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 22:05
Operator : YP/AJ
Sample : AR1254ICV500
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO091525AR1254

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:31:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

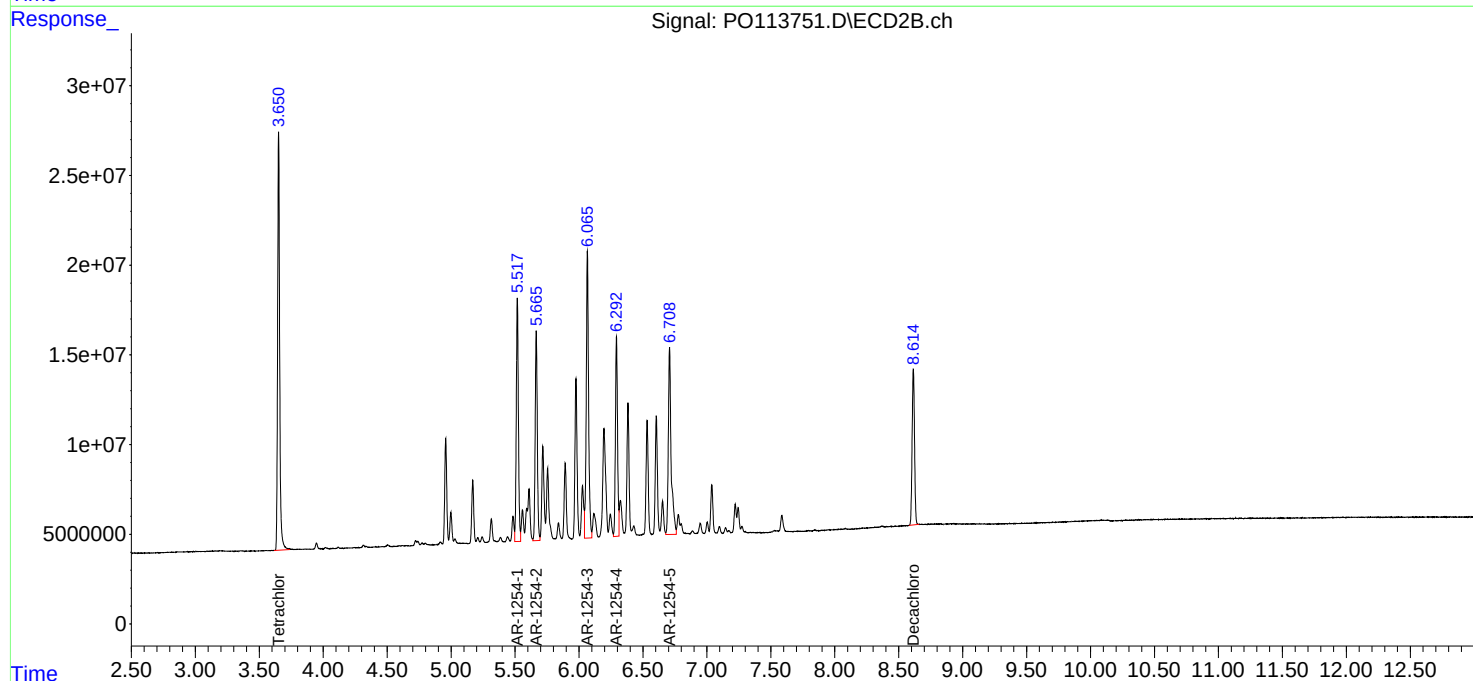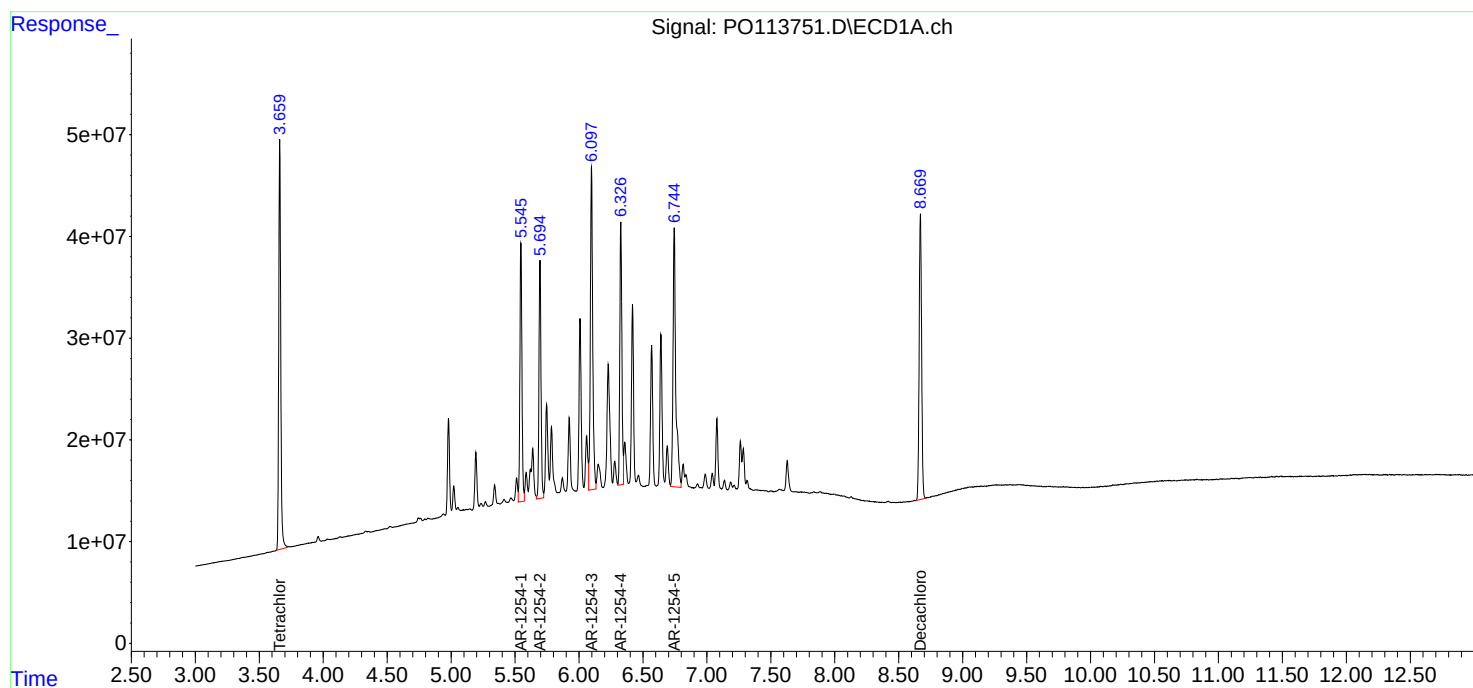

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
 Data File : P0113752.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 23:00
 Operator : YP/AJ
 Sample : AR1268ICV500
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO091525AR1268

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 02:27:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:01:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.650	448.2E6	264.5E6	53.295	52.666
2) SA Decachlor...	8.669	8.614	672.1E6	202.9E6	49.301	52.494
Target Compounds						
41) L9 AR-1268-1	7.567	7.526	923.5E6	251.0E6	521.490	514.235
42) L9 AR-1268-2	7.633	7.592	782.4E6	205.3E6	525.625	515.394
43) L9 AR-1268-3	7.837	7.794	679.1E6	165.2E6	555.335	506.291
44) L9 AR-1268-4	8.126	8.082	256.4E6	65042500	563.782	513.027
45) L9 AR-1268-5	8.417	8.367	1640.6E6	456.1E6	525.651	518.739



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113752.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 23:00
Operator : YP/AJ
Sample : AR1268ICV500
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO091525AR1268

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 02:27:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:01:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

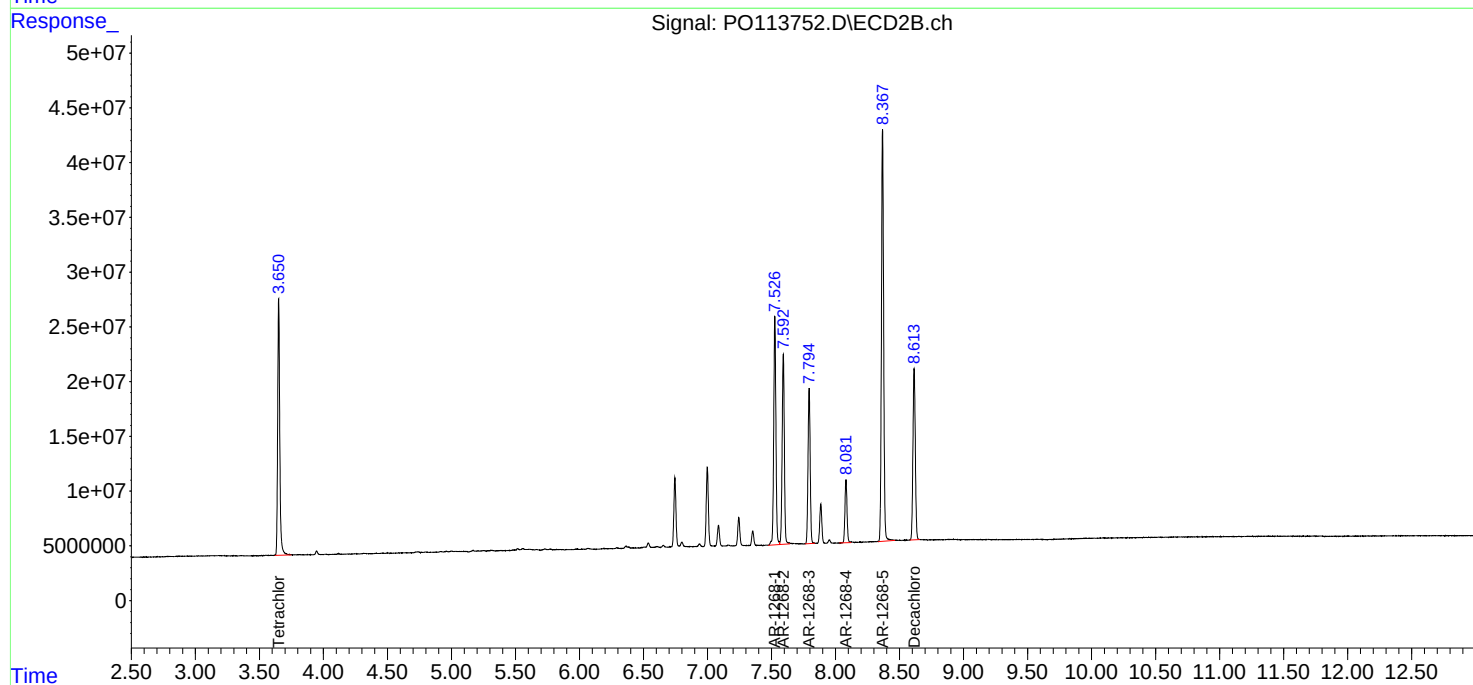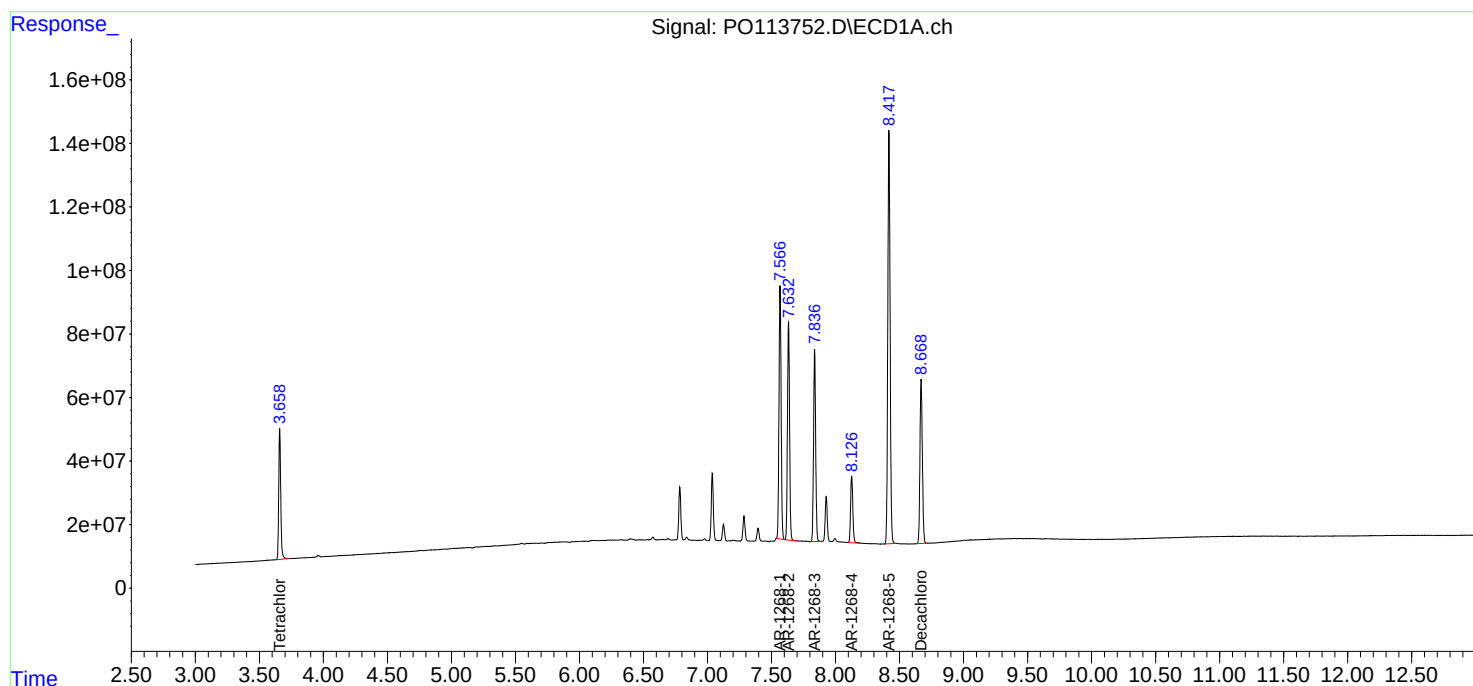



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: GENV01

Lab Code: ACE

SDG NO.: Q3277

Continuing Calib Date: 10/06/2025

Initial Calibration Date(s): 09/15/2025 09/15/2025

Continuing Calib Time: 09:49

Initial Calibration Time(s): 09:34 19:21

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.74	4.74	4.64	4.84	0.00
Aroclor-1016-2	(2)	4.76	4.76	4.66	4.86	0.00
Aroclor-1016-3	(3)	4.81	4.82	4.72	4.92	0.01
Aroclor-1016-4	(4)	4.93	4.94	4.84	5.04	0.01
Aroclor-1016-5	(5)	5.19	5.19	5.09	5.29	0.00
Aroclor-1260-1	(1)	6.22	6.23	6.13	6.33	0.01
Aroclor-1260-2	(2)	6.41	6.42	6.32	6.52	0.01
Aroclor-1260-3	(3)	6.78	6.78	6.68	6.88	0.00
Aroclor-1260-4	(4)	7.03	7.04	6.94	7.14	0.01
Aroclor-1260-5	(5)	7.28	7.29	7.19	7.39	0.01
Tetrachloro-m-xylene		3.66	3.66	3.56	3.76	0.00
Decachlorobiphenyl		8.66	8.67	8.57	8.77	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: GENV01

Lab Code: ACE

SDG NO.: Q3277

Continuing Calib Date: 10/06/2025

Initial Calibration Date(s): 09/15/2025

09/15/2025

Continuing Calib Time: 09:49

Initial Calibration Time(s): 09:34

19:21

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.72	4.72	4.62	4.82	0.00
Aroclor-1016-2	(2)	4.73	4.74	4.64	4.84	0.01
Aroclor-1016-3	(3)	4.91	4.92	4.82	5.02	0.01
Aroclor-1016-4	(4)	4.95	4.96	4.86	5.06	0.01
Aroclor-1016-5	(5)	5.16	5.17	5.07	5.27	0.01
Aroclor-1260-1	(1)	6.19	6.20	6.10	6.30	0.01
Aroclor-1260-2	(2)	6.38	6.38	6.28	6.48	0.00
Aroclor-1260-3	(3)	6.53	6.54	6.44	6.64	0.01
Aroclor-1260-4	(4)	6.99	7.00	6.90	7.10	0.01
Aroclor-1260-5	(5)	7.24	7.25	7.15	7.35	0.01
Tetrachloro-m-xylene		3.65	3.65	3.55	3.75	0.01
Decachlorobiphenyl		8.60	8.61	8.51	8.71	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance **Contract:** GENV01
Lab Code: ACE **SDG NO.:** Q3277
GC Column: ZB-MR1 **ID:** 0.32 (mm) **Initi. Calib. Date(s):** 09/15/2025 09/15/2025

Client Sample No.: CCAL01 **Date Analyzed:** 10/06/2025
Lab Sample No.: AR1660CCC500 **Data File :** PO114249.D **Time Analyzed:** 09:49

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.737	4.643	4.843	589.600	500.000	17.9
Aroclor-1016-2	4.756	4.661	4.861	602.320	500.000	20.5
Aroclor-1016-3	4.813	4.718	4.918	593.270	500.000	18.7
Aroclor-1016-4	4.932	4.837	5.037	577.950	500.000	15.6
Aroclor-1016-5	5.188	5.093	5.293	611.650	500.000	22.3
Aroclor-1260-1	6.222	6.129	6.329	580.830	500.000	16.2
Aroclor-1260-2	6.412	6.319	6.519	569.840	500.000	14.0
Aroclor-1260-3	6.776	6.683	6.883	549.700	500.000	9.9
Aroclor-1260-4	7.034	6.941	7.141	644.310	500.000	28.9
Aroclor-1260-5	7.278	7.185	7.385	661.270	500.000	32.3
Decachlorobiphenyl	8.660	8.570	8.770	45.840	50.000	-8.3
Tetrachloro-m-xylene	3.657	3.560	3.760	51.480	50.000	3.0



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance **Contract:** GENV01
Lab Code: ACE **SDG NO.:** Q3277
GC Column: ZB-MR2 **ID:** 0.32 (mm) **Initi. Calib. Date(s):** 09/15/2025 09/15/2025

Client Sample No.: CCAL01 **Date Analyzed:** 10/06/2025
Lab Sample No.: AR1660CCC500 **Data File :** PO114249.D **Time Analyzed:** 09:49

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.715	4.623	4.823	552.550	500.000	10.5
Aroclor-1016-2	4.733	4.641	4.841	560.670	500.000	12.1
Aroclor-1016-3	4.908	4.816	5.016	555.290	500.000	11.1
Aroclor-1016-4	4.950	4.858	5.058	561.850	500.000	12.4
Aroclor-1016-5	5.162	5.070	5.270	571.080	500.000	14.2
Aroclor-1260-1	6.187	6.096	6.296	532.050	500.000	6.4
Aroclor-1260-2	6.375	6.284	6.484	496.720	500.000	-0.7
Aroclor-1260-3	6.526	6.435	6.635	487.810	500.000	-2.4
Aroclor-1260-4	6.994	6.903	7.103	484.920	500.000	-3.0
Aroclor-1260-5	7.236	7.146	7.346	480.440	500.000	-3.9
Decachlorobiphenyl	8.603	8.514	8.714	45.990	50.000	-8.0
Tetrachloro-m-xylene	3.645	3.551	3.751	47.970	50.000	-4.1

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100625\
 Data File : PO114249.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2025 09:49
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/06/2025
 Supervised By :mohammad ahmed 10/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 11:40:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:49:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.657	3.645	454.1E6	256.2E6	51.482	47.974
2) SA Decachlor...	8.660	8.603	306.7E6	96020047	45.844	45.992
Target Compounds						
3) L1 AR-1016-1	4.737	4.715	179.0E6	100.7E6	589.600m	552.549m
4) L1 AR-1016-2	4.756	4.733	274.1E6	155.2E6	602.320m	560.670m
5) L1 AR-1016-3	4.813	4.908	177.5E6	82928356	593.266	555.285
6) L1 AR-1016-4	4.932	4.950	138.9E6	67820196	577.951	561.847
7) L1 AR-1016-5	5.188	5.162	146.9E6	85700284	611.650	571.084
31) L7 AR-1260-1	6.222	6.187	284.7E6	133.7E6	580.832m	532.050
32) L7 AR-1260-2	6.412	6.375	436.4E6	164.2E6	569.844	496.716
33) L7 AR-1260-3	6.776	6.526	369.8E6	136.8E6	549.697	487.807
34) L7 AR-1260-4	7.034	6.994	278.8E6	92723078	644.305m	484.925
35) L7 AR-1260-5	7.278	7.236	749.1E6	204.5E6	661.275m	480.435 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100625\
Data File : PO114249.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2025 09:49
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/06/2025
Supervised By :mohammad ahmed 10/08/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 11:40:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

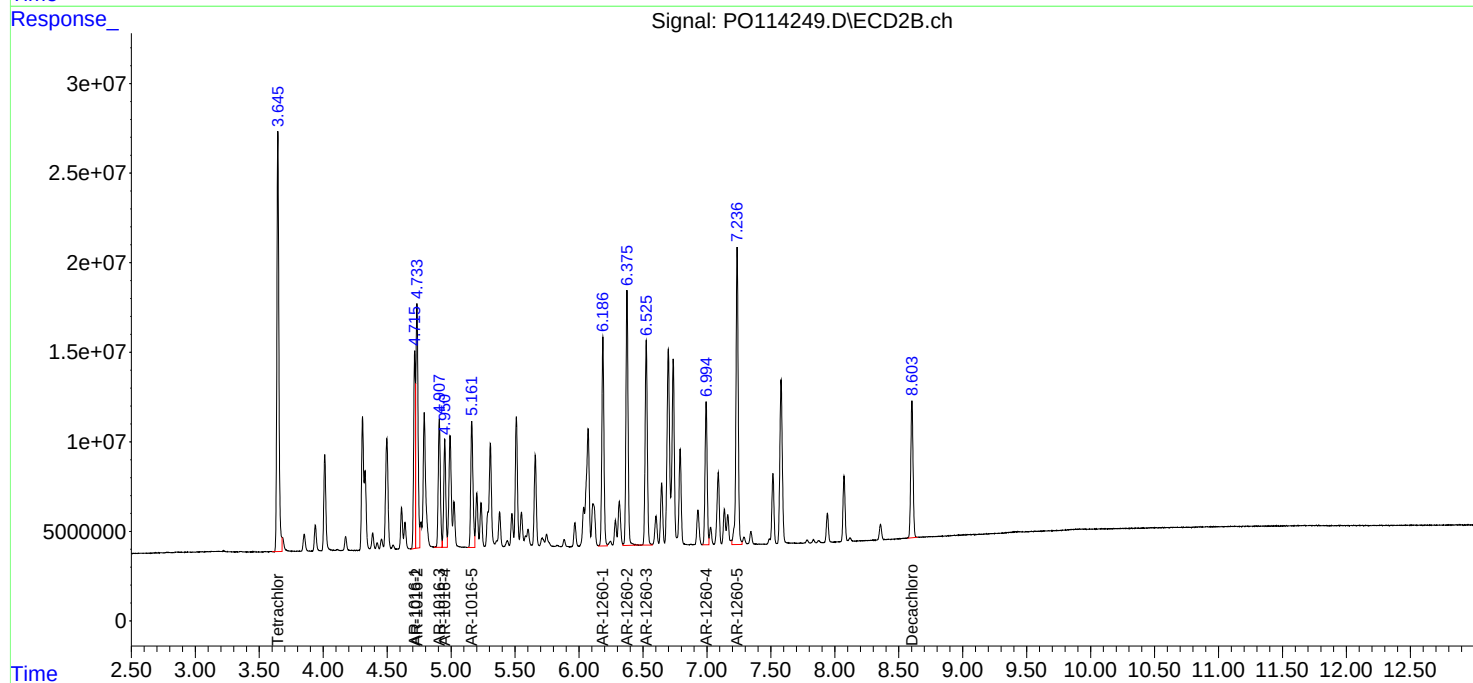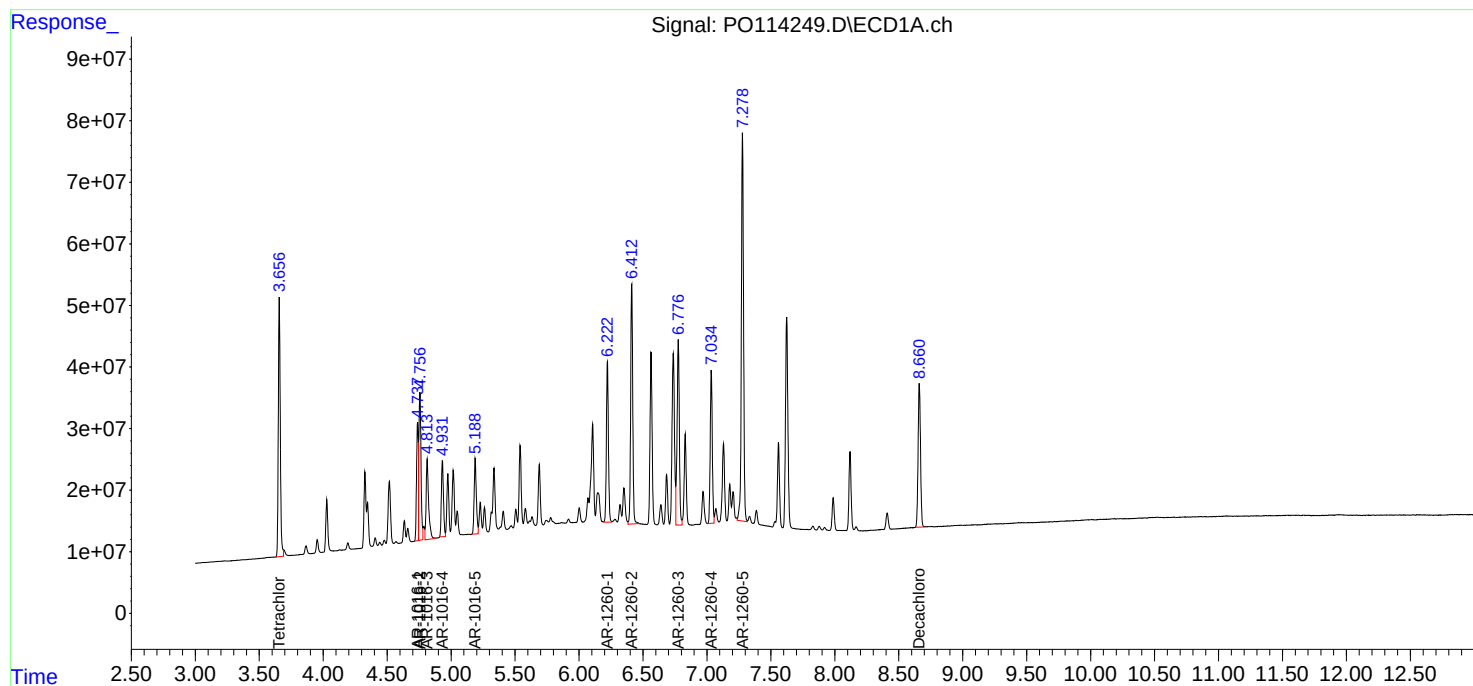



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: GENV01

Lab Code: ACE

SDG NO.: Q3277

Continuing Calib Date: 10/06/2025

Initial Calibration Date(s): 09/15/2025 09/15/2025

Continuing Calib Time: 15:55

Initial Calibration Time(s): 09:34 19:21

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.74	4.74	4.64	4.84	0.00
Aroclor-1016-2	(2)	4.76	4.76	4.66	4.86	0.00
Aroclor-1016-3	(3)	4.81	4.82	4.72	4.92	0.01
Aroclor-1016-4	(4)	4.93	4.94	4.84	5.04	0.01
Aroclor-1016-5	(5)	5.19	5.19	5.09	5.29	0.00
Aroclor-1260-1	(1)	6.22	6.23	6.13	6.33	0.01
Aroclor-1260-2	(2)	6.41	6.42	6.32	6.52	0.01
Aroclor-1260-3	(3)	6.78	6.78	6.68	6.88	0.00
Aroclor-1260-4	(4)	7.04	7.04	6.94	7.14	0.01
Aroclor-1260-5	(5)	7.28	7.29	7.19	7.39	0.01
Tetrachloro-m-xylene		3.66	3.66	3.56	3.76	0.00
Decachlorobiphenyl		8.66	8.67	8.57	8.77	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: GENV01

Lab Code: ACE

SDG NO.: Q3277

Continuing Calib Date: 10/06/2025

Initial Calibration Date(s): 09/15/2025 09/15/2025

Continuing Calib Time: 15:55

Initial Calibration Time(s): 09:34 19:21

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.72	4.72	4.62	4.82	0.00
Aroclor-1016-2	(2)	4.74	4.74	4.64	4.84	0.00
Aroclor-1016-3	(3)	4.91	4.92	4.82	5.02	0.01
Aroclor-1016-4	(4)	4.95	4.96	4.86	5.06	0.01
Aroclor-1016-5	(5)	5.16	5.17	5.07	5.27	0.01
Aroclor-1260-1	(1)	6.19	6.20	6.10	6.30	0.01
Aroclor-1260-2	(2)	6.38	6.38	6.28	6.48	0.00
Aroclor-1260-3	(3)	6.53	6.54	6.44	6.64	0.01
Aroclor-1260-4	(4)	7.00	7.00	6.90	7.10	0.00
Aroclor-1260-5	(5)	7.24	7.25	7.15	7.35	0.01
Tetrachloro-m-xylene		3.65	3.65	3.55	3.75	0.00
Decachlorobiphenyl		8.61	8.61	8.51	8.71	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance **Contract:** GENV01
Lab Code: ACE **SDG NO.:** Q3277
GC Column: ZB-MR1 **ID:** 0.32 (mm) **Initi. Calib. Date(s):** 09/15/2025 09/15/2025

Client Sample No.: CCAL02 **Date Analyzed:** 10/06/2025
Lab Sample No.: AR1660CCC500 **Data File :** PO114264.D **Time Analyzed:** 15:55

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.738	4.643	4.843	582.670	500.000	16.5
Aroclor-1016-2	4.756	4.661	4.861	595.070	500.000	19.0
Aroclor-1016-3	4.813	4.718	4.918	569.650	500.000	13.9
Aroclor-1016-4	4.932	4.837	5.037	559.330	500.000	11.9
Aroclor-1016-5	5.187	5.093	5.293	586.500	500.000	17.3
Aroclor-1260-1	6.222	6.129	6.329	550.580	500.000	10.1
Aroclor-1260-2	6.412	6.319	6.519	535.800	500.000	7.2
Aroclor-1260-3	6.777	6.683	6.883	472.020	500.000	-5.6
Aroclor-1260-4	7.035	6.941	7.141	505.610	500.000	1.1
Aroclor-1260-5	7.279	7.185	7.385	509.360	500.000	1.9
Decachlorobiphenyl	8.661	8.570	8.770	37.070	50.000	-25.9
Tetrachloro-m-xylene	3.657	3.560	3.760	50.160	50.000	0.3



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance **Contract:** GENV01
Lab Code: ACE **SDG NO.:** Q3277
GC Column: ZB-MR2 **ID:** 0.32 (mm) **Initi. Calib. Date(s):** 09/15/2025 09/15/2025

Client Sample No.: CCAL02 **Date Analyzed:** 10/06/2025
Lab Sample No.: AR1660CCC500 **Data File :** PO114264.D **Time Analyzed:** 15:55

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.716	4.623	4.823	529.080	500.000	5.8
Aroclor-1016-2	4.735	4.641	4.841	554.850	500.000	11.0
Aroclor-1016-3	4.909	4.816	5.016	558.280	500.000	11.7
Aroclor-1016-4	4.952	4.858	5.058	560.240	500.000	12.0
Aroclor-1016-5	5.163	5.070	5.270	581.980	500.000	16.4
Aroclor-1260-1	6.189	6.096	6.296	488.920	500.000	-2.2
Aroclor-1260-2	6.377	6.284	6.484	458.970	500.000	-8.2
Aroclor-1260-3	6.528	6.435	6.635	445.750	500.000	-10.9
Aroclor-1260-4	6.996	6.903	7.103	443.550	500.000	-11.3
Aroclor-1260-5	7.239	7.146	7.346	436.000	500.000	-12.8
Decachlorobiphenyl	8.605	8.514	8.714	40.720	50.000	-18.6
Tetrachloro-m-xylene	3.647	3.551	3.751	49.050	50.000	-1.9

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100625\
 Data File : PO114264.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2025 15:55
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/07/2025
 Supervised By :mohammad ahmed 10/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 02:11:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:49:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.657	3.647	442.4E6	262.0E6	50.157	49.048
2) SA Decachlor...	8.661	8.605	248.0E6	85005363	37.066	40.716
Target Compounds						
3) L1 AR-1016-1	4.738	4.716	176.8E6	96420788	582.667	529.083m
4) L1 AR-1016-2	4.756	4.735	270.8E6	153.6E6	595.070	554.853
5) L1 AR-1016-3	4.813	4.909	170.4E6	83374837	569.651	558.275
6) L1 AR-1016-4	4.932	4.952	134.5E6	67626616	559.326	560.243
7) L1 AR-1016-5	5.187	5.163	140.8E6	87335352	586.499m	581.979
31) L7 AR-1260-1	6.222	6.189	269.9E6	122.9E6	550.585	488.918
32) L7 AR-1260-2	6.412	6.377	410.3E6	151.7E6	535.804	458.974
33) L7 AR-1260-3	6.777	6.528	317.6E6	125.0E6	472.023	445.754
34) L7 AR-1260-4	7.035	6.996	218.8E6	84811903	505.606	443.551
35) L7 AR-1260-5	7.279	7.239	577.0E6	185.6E6	509.362	435.996

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100625\
Data File : PO114264.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2025 15:55
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/07/2025
Supervised By :mohammad ahmed 10/08/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 02:11:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

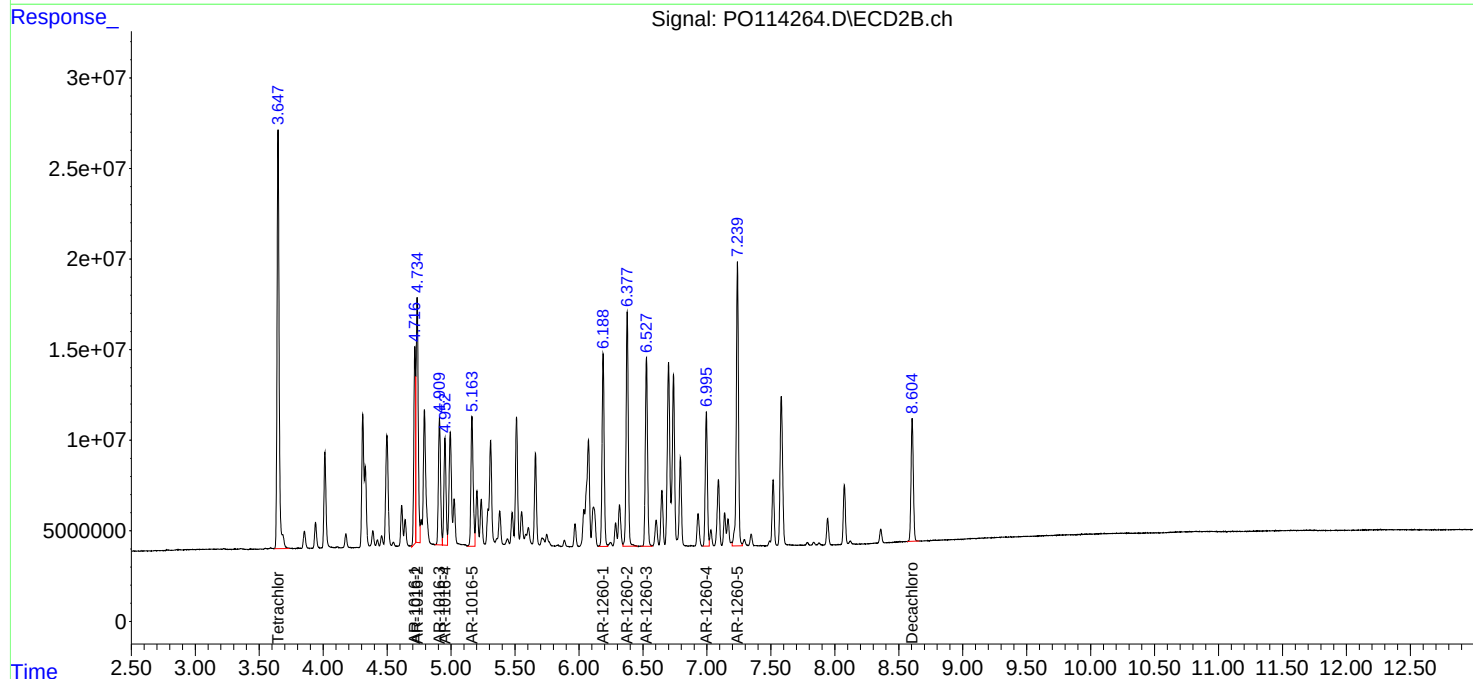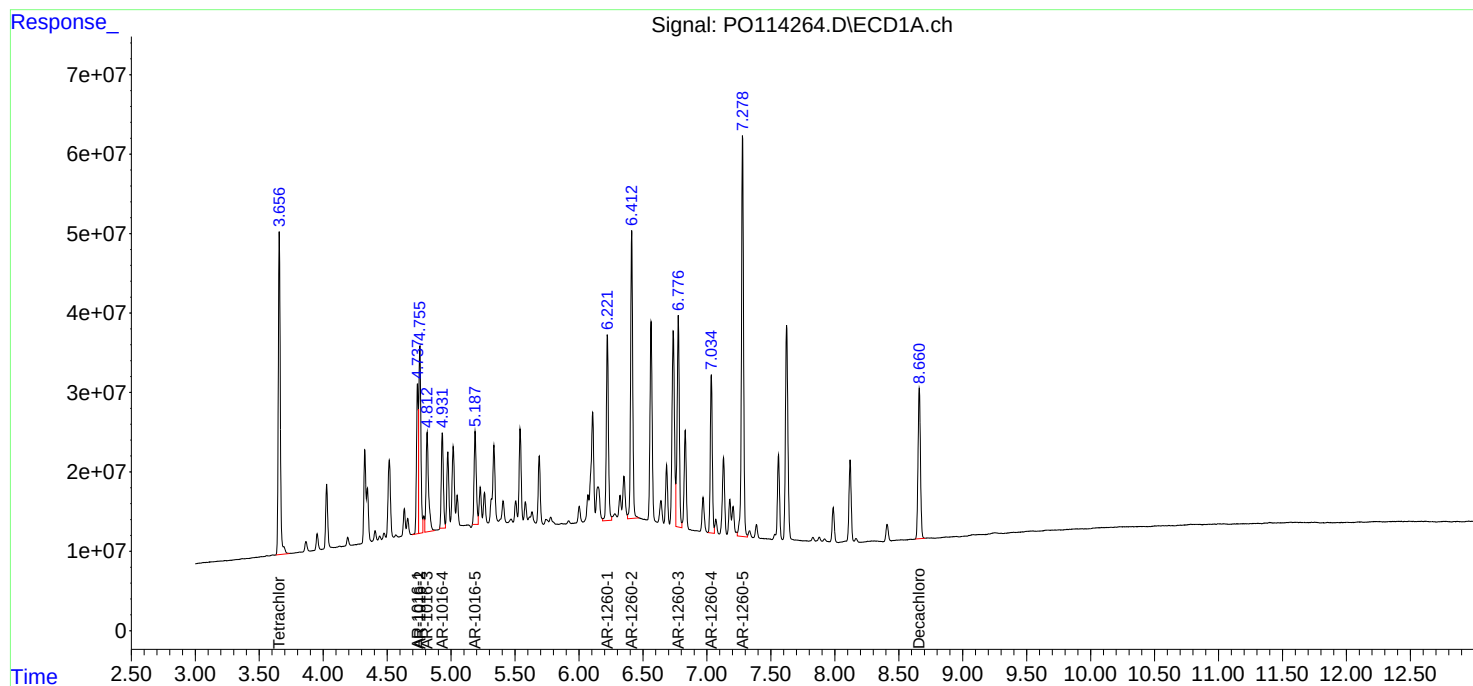

Analytical Sequence

Client: G Environmental

SDG No.: Q3277

Project: Newport

Instrument ID: ECD_O

GC Column: ZB-MR1

ID: 0.32 (mm)

Inst. Calib. Date(s): 09/15/2025 09/15/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

CLIENT ID	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
IBLK	IBLK	09/15/2025	09:16	PO113719.D	8.67	3.66
AR1660ICC1000	AR1660ICC1000	09/15/2025	09:34	PO113720.D	8.67	3.66
AR1660ICC750	AR1660ICC750	09/15/2025	09:53	PO113721.D	8.67	3.66
AR1660ICC500	AR1660ICC500	09/15/2025	10:11	PO113722.D	8.67	3.66
AR1660ICC250	AR1660ICC250	09/15/2025	10:30	PO113723.D	8.67	3.66
AR1660ICC050	AR1660ICC050	09/15/2025	10:48	PO113724.D	8.67	3.66
AR1221ICC500	AR1221ICC500	09/15/2025	11:06	PO113725.D	8.67	3.66
AR1232ICC500	AR1232ICC500	09/15/2025	11:25	PO113726.D	8.67	3.66
AR1242ICC1000	AR1242ICC1000	09/15/2025	11:43	PO113727.D	8.67	3.66
AR1242ICC750	AR1242ICC750	09/15/2025	12:02	PO113728.D	8.67	3.66
AR1242ICC500	AR1242ICC500	09/15/2025	12:20	PO113729.D	8.67	3.66
AR1242ICC250	AR1242ICC250	09/15/2025	12:38	PO113730.D	8.67	3.66
AR1242ICC050	AR1242ICC050	09/15/2025	13:34	PO113731.D	8.67	3.66
AR1248ICC1000	AR1248ICC1000	09/15/2025	13:54	PO113732.D	8.67	3.66
AR1248ICC750	AR1248ICC750	09/15/2025	14:13	PO113733.D	8.67	3.66
AR1248ICC500	AR1248ICC500	09/15/2025	14:31	PO113734.D	8.67	3.66
AR1248ICC250	AR1248ICC250	09/15/2025	14:49	PO113735.D	8.67	3.66
AR1248ICC050	AR1248ICC050	09/15/2025	15:26	PO113736.D	8.67	3.66
AR1254ICC1000	AR1254ICC1000	09/15/2025	15:45	PO113737.D	8.67	3.66
AR1254ICC750	AR1254ICC750	09/15/2025	16:02	PO113738.D	8.67	3.66
AR1254ICC500	AR1254ICC500	09/15/2025	16:20	PO113739.D	8.67	3.66
AR1254ICC250	AR1254ICC250	09/15/2025	16:38	PO113740.D	8.67	3.66
AR1254ICC050	AR1254ICC050	09/15/2025	17:14	PO113741.D	8.67	3.66
AR1262ICC500	AR1262ICC500	09/15/2025	17:33	PO113742.D	8.67	3.66
AR1268ICC1000	AR1268ICC1000	09/15/2025	17:51	PO113743.D	8.67	3.66
AR1268ICC750	AR1268ICC750	09/15/2025	18:10	PO113744.D	8.67	3.66
AR1268ICC500	AR1268ICC500	09/15/2025	18:27	PO113745.D	8.67	3.66
AR1268ICC250	AR1268ICC250	09/15/2025	18:45	PO113746.D	8.67	3.66
AR1268ICC050	AR1268ICC050	09/15/2025	19:21	PO113747.D	8.67	3.66
AR1660CCC500	AR1660CCC500	10/06/2025	09:49	PO114249.D	8.66	3.66
IBLK	IBLK	10/06/2025	11:02	PO114253.D	8.66	3.66
PB169987BL	PB169987BL	10/06/2025	12:10	PO114254.D	8.67	3.66
PB169987BS	PB169987BS	10/06/2025	12:28	PO114255.D	8.66	3.66
WC1	Q3277-01	10/06/2025	13:05	PO114257.D	8.66	3.66
TR-01-100325MS	Q3288-01MS	10/06/2025	13:41	PO114259.D	8.66	3.66
TR-01-100325MSD	Q3288-01MSD	10/06/2025	13:59	PO114260.D	8.66	3.66
AR1660CCC500	AR1660CCC500	10/06/2025	15:55	PO114264.D	8.66	3.66
IBLK	IBLK	10/06/2025	17:08	PO114268.D	8.66	3.65

Analytical Sequence

Client: G Environmental

SDG No.: Q3277

Project: Newport

Instrument ID: ECD_O

GC Column: ZB-MR2

ID: 0.32 (mm)

Inst. Calib. Date(s): 09/15/2025 09/15/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

CLIENT ID	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
IBLK	IBLK	09/15/2025	09:16	PO113719.D	8.62	3.65
AR1660ICC1000	AR1660ICC1000	09/15/2025	09:34	PO113720.D	8.61	3.65
AR1660ICC750	AR1660ICC750	09/15/2025	09:53	PO113721.D	8.62	3.65
AR1660ICC500	AR1660ICC500	09/15/2025	10:11	PO113722.D	8.61	3.65
AR1660ICC250	AR1660ICC250	09/15/2025	10:30	PO113723.D	8.62	3.65
AR1660ICC050	AR1660ICC050	09/15/2025	10:48	PO113724.D	8.62	3.65
AR1221ICC500	AR1221ICC500	09/15/2025	11:06	PO113725.D	8.61	3.65
AR1232ICC500	AR1232ICC500	09/15/2025	11:25	PO113726.D	8.62	3.65
AR1242ICC1000	AR1242ICC1000	09/15/2025	11:43	PO113727.D	8.62	3.65
AR1242ICC750	AR1242ICC750	09/15/2025	12:02	PO113728.D	8.62	3.65
AR1242ICC500	AR1242ICC500	09/15/2025	12:20	PO113729.D	8.62	3.65
AR1242ICC250	AR1242ICC250	09/15/2025	12:38	PO113730.D	8.62	3.65
AR1242ICC050	AR1242ICC050	09/15/2025	13:34	PO113731.D	8.62	3.65
AR1248ICC1000	AR1248ICC1000	09/15/2025	13:54	PO113732.D	8.62	3.65
AR1248ICC750	AR1248ICC750	09/15/2025	14:13	PO113733.D	8.62	3.65
AR1248ICC500	AR1248ICC500	09/15/2025	14:31	PO113734.D	8.61	3.65
AR1248ICC250	AR1248ICC250	09/15/2025	14:49	PO113735.D	8.62	3.65
AR1248ICC050	AR1248ICC050	09/15/2025	15:26	PO113736.D	8.62	3.65
AR1254ICC1000	AR1254ICC1000	09/15/2025	15:45	PO113737.D	8.62	3.65
AR1254ICC750	AR1254ICC750	09/15/2025	16:02	PO113738.D	8.61	3.65
AR1254ICC500	AR1254ICC500	09/15/2025	16:20	PO113739.D	8.62	3.65
AR1254ICC250	AR1254ICC250	09/15/2025	16:38	PO113740.D	8.61	3.65
AR1254ICC050	AR1254ICC050	09/15/2025	17:14	PO113741.D	8.62	3.65
AR1262ICC500	AR1262ICC500	09/15/2025	17:33	PO113742.D	8.62	3.65
AR1268ICC1000	AR1268ICC1000	09/15/2025	17:51	PO113743.D	8.62	3.65
AR1268ICC750	AR1268ICC750	09/15/2025	18:10	PO113744.D	8.61	3.65
AR1268ICC500	AR1268ICC500	09/15/2025	18:27	PO113745.D	8.61	3.65
AR1268ICC250	AR1268ICC250	09/15/2025	18:45	PO113746.D	8.62	3.65
AR1268ICC050	AR1268ICC050	09/15/2025	19:21	PO113747.D	8.61	3.65
AR1660CCC500	AR1660CCC500	10/06/2025	09:49	PO114249.D	8.60	3.65
IBLK	IBLK	10/06/2025	11:02	PO114253.D	8.60	3.65
PB169987BL	PB169987BL	10/06/2025	12:10	PO114254.D	8.61	3.64
PB169987BS	PB169987BS	10/06/2025	12:28	PO114255.D	8.60	3.64
WC1	Q3277-01	10/06/2025	13:05	PO114257.D	8.60	3.65
TR-01-100325MS	Q3288-01MS	10/06/2025	13:41	PO114259.D	8.60	3.65
TR-01-100325MSD	Q3288-01MSD	10/06/2025	13:59	PO114260.D	8.60	3.65
AR1660CCC500	AR1660CCC500	10/06/2025	15:55	PO114264.D	8.61	3.65
IBLK	IBLK	10/06/2025	17:08	PO114268.D	8.60	3.65

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

PB169987BS

Lab Name: Alliance

Contract: GENV01

Lab Code: ACE

SDG NO.: Q3277

Lab Sample ID: PB169987BS

Date(s) Analyzed: 10/06/2025 10/06/2025

Instrument ID (1): ECD_O

Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm)

GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO114255.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	4.737	4.687	4.787	181	180	7.49
COLUMN 1	2	4.755	4.705	4.805	186		
	3	4.812	4.762	4.862	178		
	4	4.931	4.881	4.981	173		
	5	5.187	5.137	5.237	182		
COLUMN 2	1	4.713	4.663	4.763	171	167	
	2	4.731	4.681	4.781	169		
	3	4.907	4.857	4.957	165		
	4	4.949	4.899	4.999	164		
	5	5.16	5.11	5.21	167		
Aroclor-1260	1	6.221	6.171	6.271	203	182	19.94
COLUMN 1	2	6.411	6.361	6.461	190		
	3	6.776	6.726	6.826	160		
	4	7.034	6.984	7.084	176		
	5	7.278	7.228	7.328	180		
COLUMN 2	1	6.186	6.136	6.236	166	149	
	2	6.374	6.324	6.424	155		
	3	6.524	6.474	6.574	155		
	4	6.992	6.942	7.042	135		
	5	7.235	7.185	7.285	134		

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

TR-01-100325MS

Lab Name: Alliance

Contract: GENV01

Lab Code: ACE

SDG NO.: Q3277

Lab Sample ID: Q3288-01MS

Date(s) Analyzed: 10/06/2025 10/06/2025

Instrument ID (1): ECD_O

Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm)

GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO114259.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	4.736	4.686	4.786	138	143	11.22
COLUMN 1	2	4.754	4.704	4.804	146		
	3	4.812	4.762	4.862	142		
	4	4.93	4.88	4.98	136		
	5	5.187	5.137	5.237	155		
	1	4.715	4.665	4.765	153		
COLUMN 2	2	4.733	4.683	4.783	165	160	
	3	4.908	4.858	4.958	160		
	4	4.951	4.901	5.001	161		
	5	5.162	5.112	5.212	162		
Aroclor-1260	1	6.221	6.171	6.271	140	137	2.88
COLUMN 1	2	6.411	6.361	6.461	140		
	3	6.775	6.725	6.825	121		
	4	7.033	6.983	7.083	136		
	5	7.276	7.226	7.326	147		
	1	6.187	6.137	6.237	159		
COLUMN 2	2	6.375	6.325	6.425	145	141	
	3	6.525	6.475	6.575	142		
	4	6.994	6.944	7.044	127		
	5	7.237	7.187	7.287	130		

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

TR-01-100325MSD

Lab Name: Alliance

Contract: GENV01

Lab Code: ACE

SDG NO.: Q3277

Lab Sample ID: Q3288-01MSD

Date(s) Analyzed: 10/06/2025 10/06/2025

Instrument ID (1): ECD_O

Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm)

GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO114260.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	4.738	4.688	4.788	147	150	5.19
COLUMN 1	2	4.755	4.705	4.805	151		
	3	4.812	4.762	4.862	151		
	4	4.931	4.881	4.981	142		
	5	5.188	5.138	5.238	158		
	1	4.716	4.666	4.766	161		
COLUMN 2	2	4.734	4.684	4.784	159	158	
	3	4.909	4.859	4.959	158		
	4	4.952	4.902	5.002	157		
	5	5.162	5.112	5.212	156		
Aroclor-1260	1	6.222	6.172	6.272	138	130	3.77
COLUMN 1	2	6.411	6.361	6.461	134		
	3	6.776	6.726	6.826	114		
	4	7.034	6.984	7.084	125		
	5	7.278	7.228	7.328	137		
	1	6.187	6.137	6.237	155	135	
COLUMN 2	2	6.376	6.326	6.426	140		
	3	6.526	6.476	6.576	133		
	4	6.995	6.945	7.045	120		
	5	7.237	7.187	7.287	124		



QC SAMPLE DATA

Report of Analysis

Client:	G Environmental	Date Collected:	
Project:	Newport	Date Received:	
Client Sample ID:	PB169987BL	SDG No.:	Q3277
Lab Sample ID:	PB169987BL	Matrix:	SOIL
Analytical Method:	8082A	% Solid:	100
Sample Wt/Vol:	30.01	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	Injection Volume :	
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO114254.D	1	10/06/25 08:43	10/06/25 12:10	PB169987

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	3.90	U	3.90	17.0	ug/kg
11104-28-2	Aroclor-1221	4.00	U	4.00	17.0	ug/kg
11141-16-5	Aroclor-1232	3.70	U	3.70	17.0	ug/kg
53469-21-9	Aroclor-1242	4.00	U	4.00	17.0	ug/kg
12672-29-6	Aroclor-1248	5.90	U	5.90	17.0	ug/kg
11097-69-1	Aroclor-1254	3.20	U	3.20	17.0	ug/kg
37324-23-5	Aroclor-1262	5.00	U	5.00	17.0	ug/kg
11100-14-4	Aroclor-1268	3.60	U	3.60	17.0	ug/kg
11096-82-5	Aroclor-1260	3.20	U	3.20	17.0	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	20.5		32 - 144	102%	SPK: 20
2051-24-3	Decachlorobiphenyl	20.3		32 - 175	102%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100625\
Data File : PO114254.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2025 12:10
Operator : YP/AJ
Sample : PB169987BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB169987BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 13:04:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.660	3.644	180.4E6	103.6E6	20.459	19.398
2) SA Decachlor...	8.669	8.605	135.8E6	40938195	20.303	19.609

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100625\
Data File : PO114254.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2025 12:10
Operator : YP/AJ
Sample : PB169987BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB169987BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 13:04:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

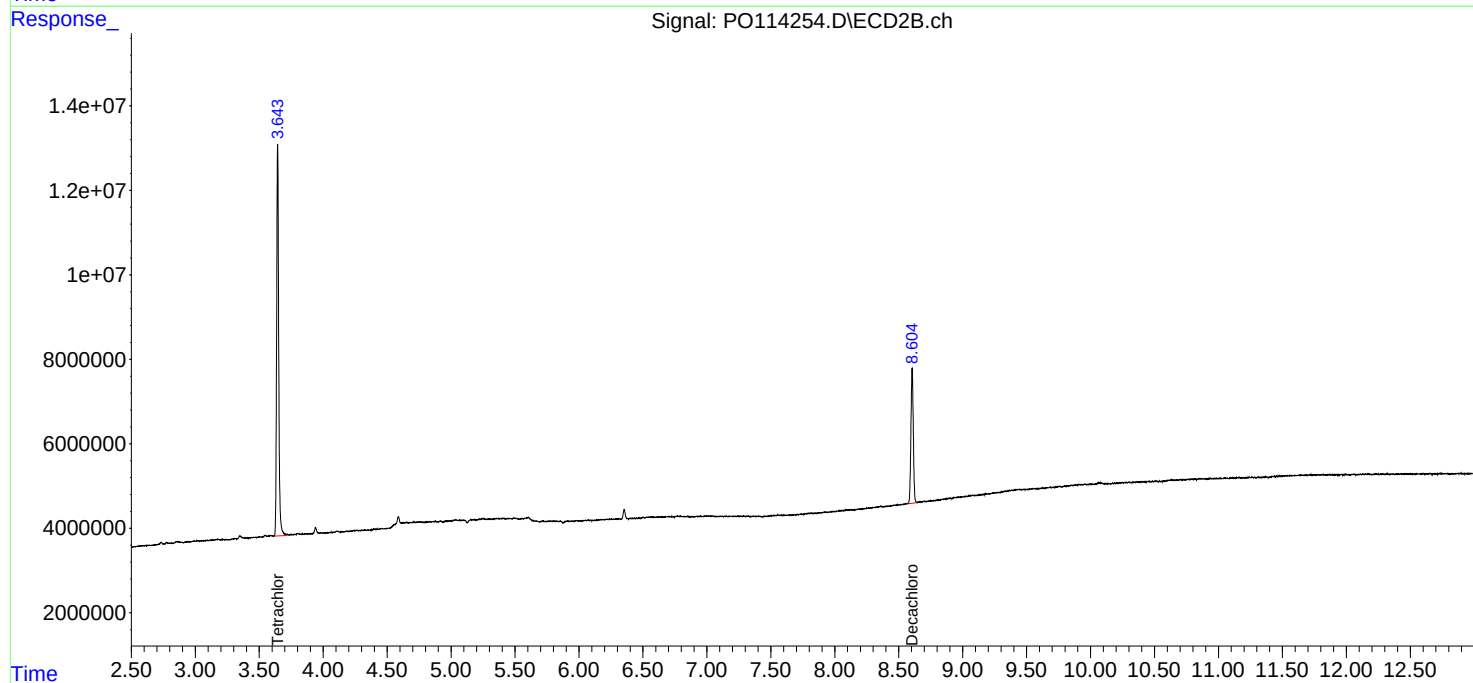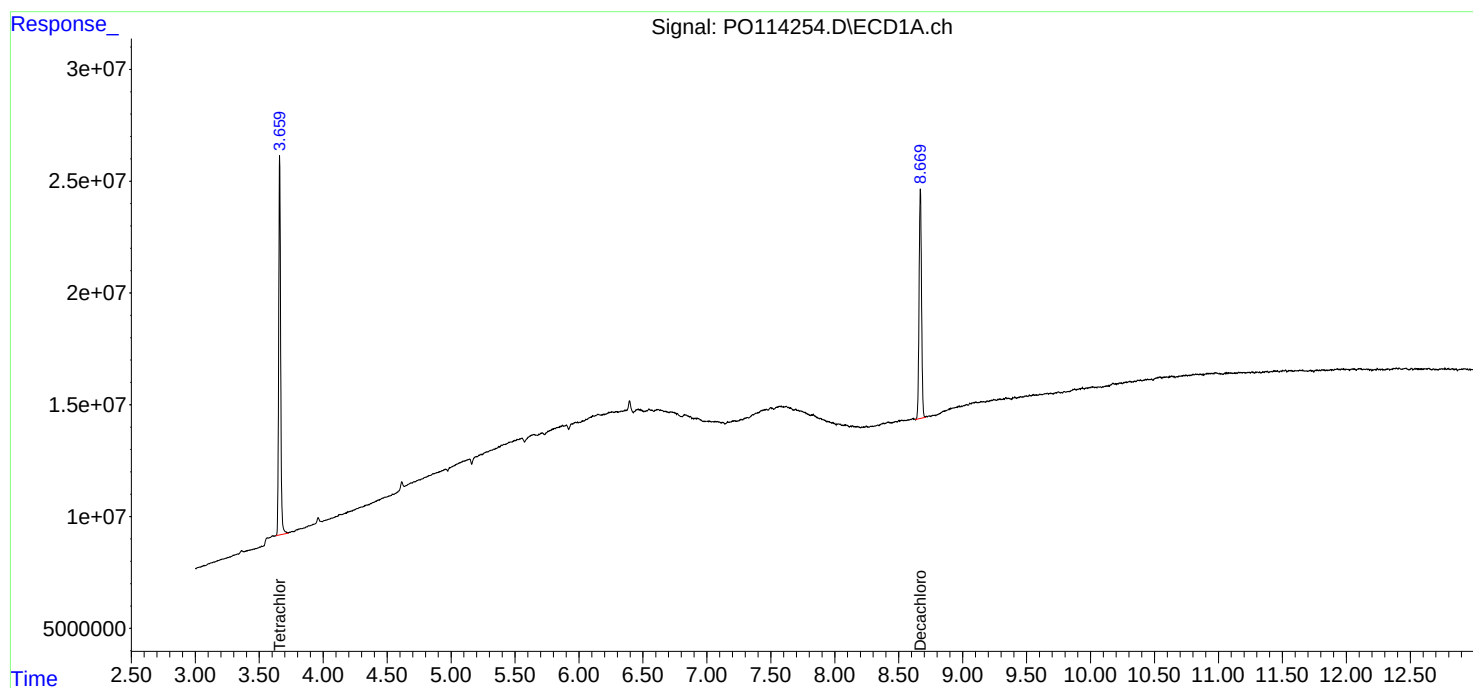


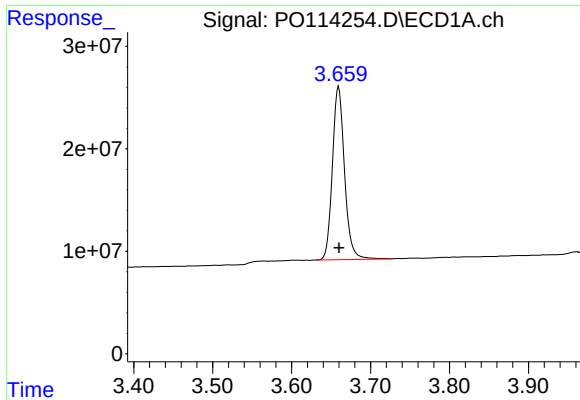

#1 Tetrachloro-m-xylene


R.T.: 3.660 min
Delta R.T.: 0.000 min
Response: 180443519
Conc: 20.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB169987BL

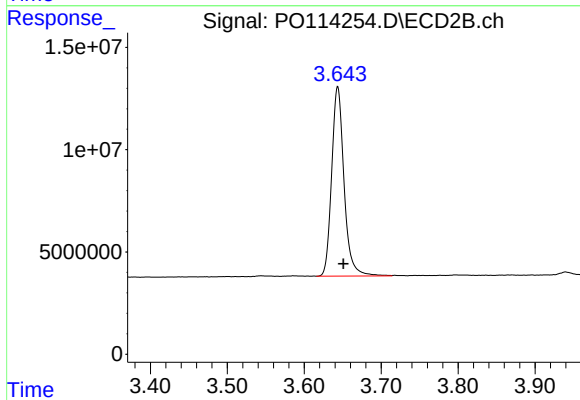


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: -0.007 min
Response: 103605417
Conc: 19.40 ng/ml

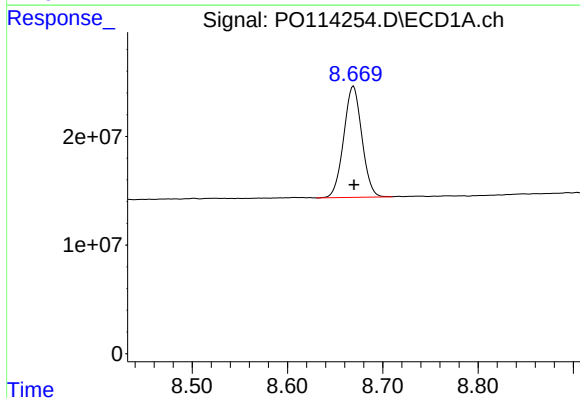

#2 Decachlorobiphenyl

R.T.: 8.669 min
Delta R.T.: 0.000 min
Response: 135833327
Conc: 20.30 ng/ml

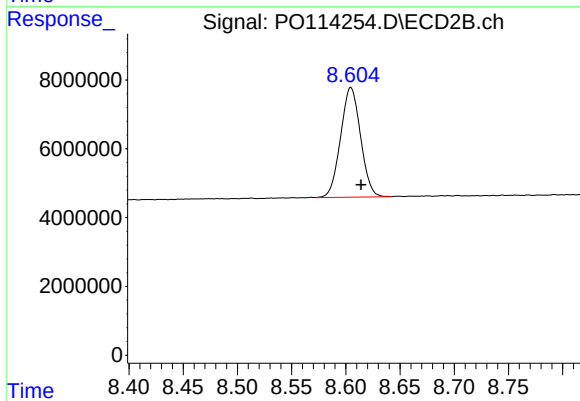

#2 Decachlorobiphenyl

R.T.: 8.605 min
Delta R.T.: -0.009 min
Response: 40938195
Conc: 19.61 ng/ml

Report of Analysis

Client:	G Environmental	Date Collected:	09/15/25
Project:	Newport	Date Received:	09/15/25
Client Sample ID:	PIBLK-PO113719.D	SDG No.:	Q3277
Lab Sample ID:	I.BLK-PO113719.D	Matrix:	WATER
Analytical Method:	8082A	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	5030	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO113719.D	1		09/15/25	po091525

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	17.0		60 - 140	85%	SPK: 20
2051-24-3	Decachlorobiphenyl	17.3		60 - 140	86%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091525\
Data File : PO113719.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 09:16
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:17:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.650	149.9E6	90826369	16.992	17.005
2) SA Decachlor...	8.670	8.615	115.6E6	37797688	17.280	18.105

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091525\
Data File : PO113719.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 09:16
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:17:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

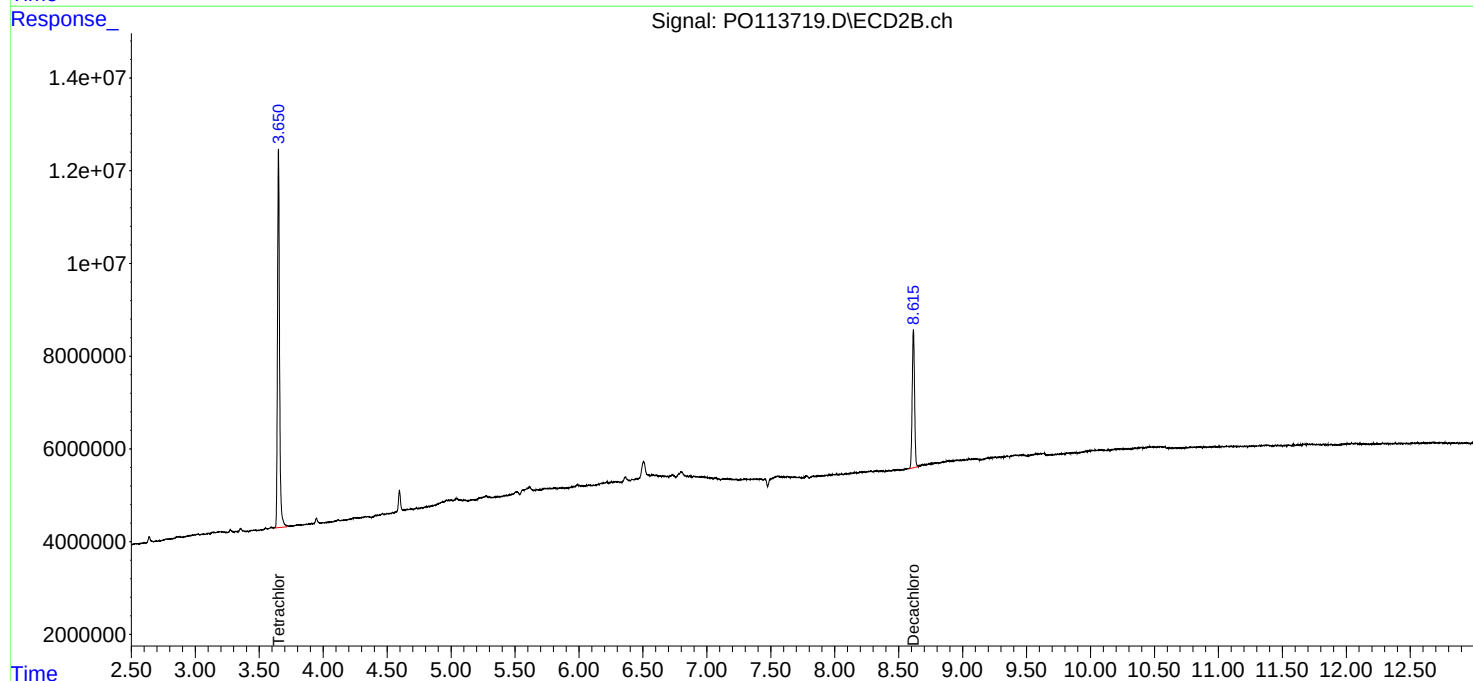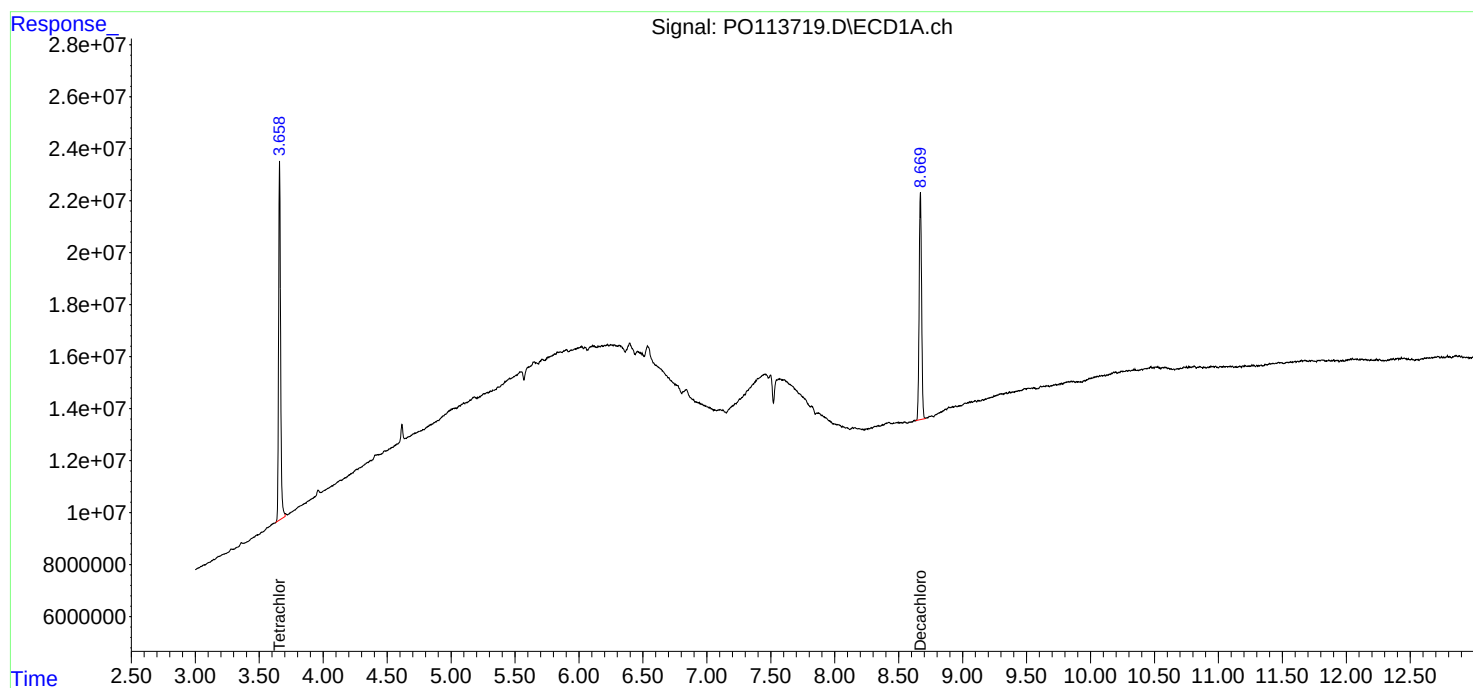


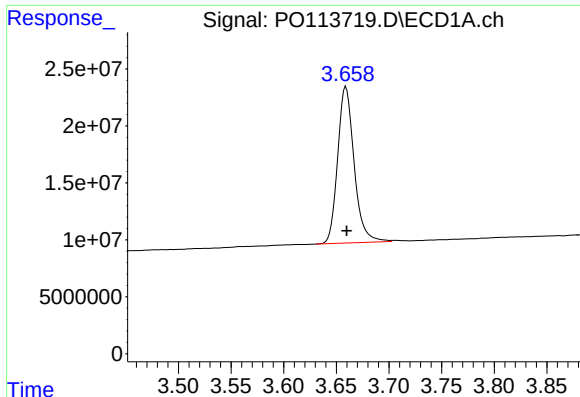

#1 Tetrachloro-m-xylene


R.T.: 3.659 min
Delta R.T.: 0.000 min
Response: 149864244
Conc: 16.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

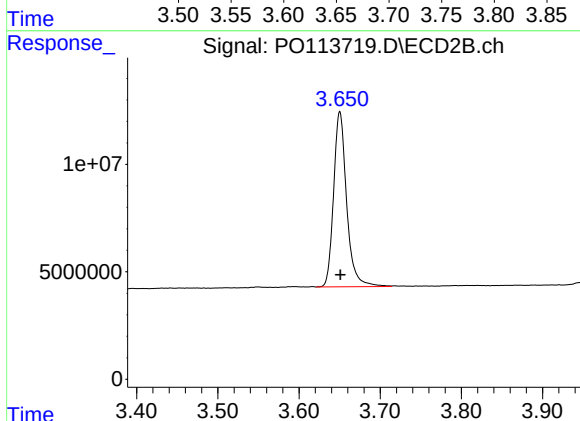


#1 Tetrachloro-m-xylene

R.T.: 3.650 min
Delta R.T.: 0.000 min
Response: 90826369
Conc: 17.01 ng/ml

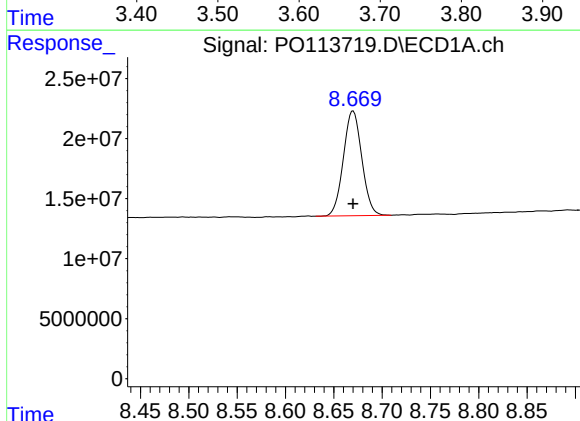

#2 Decachlorobiphenyl

R.T.: 8.670 min
Delta R.T.: 0.000 min
Response: 115604769
Conc: 17.28 ng/ml

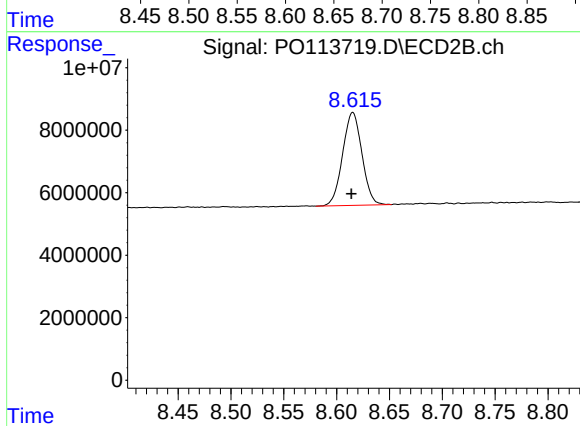

#2 Decachlorobiphenyl

R.T.: 8.615 min
Delta R.T.: 0.001 min
Response: 37797688
Conc: 18.10 ng/ml

Report of Analysis

Client:	G Environmental	Date Collected:	10/06/25
Project:	Newport	Date Received:	10/06/25
Client Sample ID:	PIBLK-PO114253.D	SDG No.:	Q3277
Lab Sample ID:	I.BLK-PO114253.D	Matrix:	WATER
Analytical Method:	8082A	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	5030	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO114253.D	1		10/06/25	PO100625

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	17.7		60 - 140	89%	SPK: 20
2051-24-3	Decachlorobiphenyl	17.6		60 - 140	88%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100625\
Data File : PO114253.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2025 11:02
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 11:43:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.656	3.646	160.6E6	94587815	18.211	17.710
2) SA Decachlor...	8.659	8.602	117.7E6	37830684	17.595	18.120

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100625\
Data File : PO114253.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2025 11:02
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 11:43:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

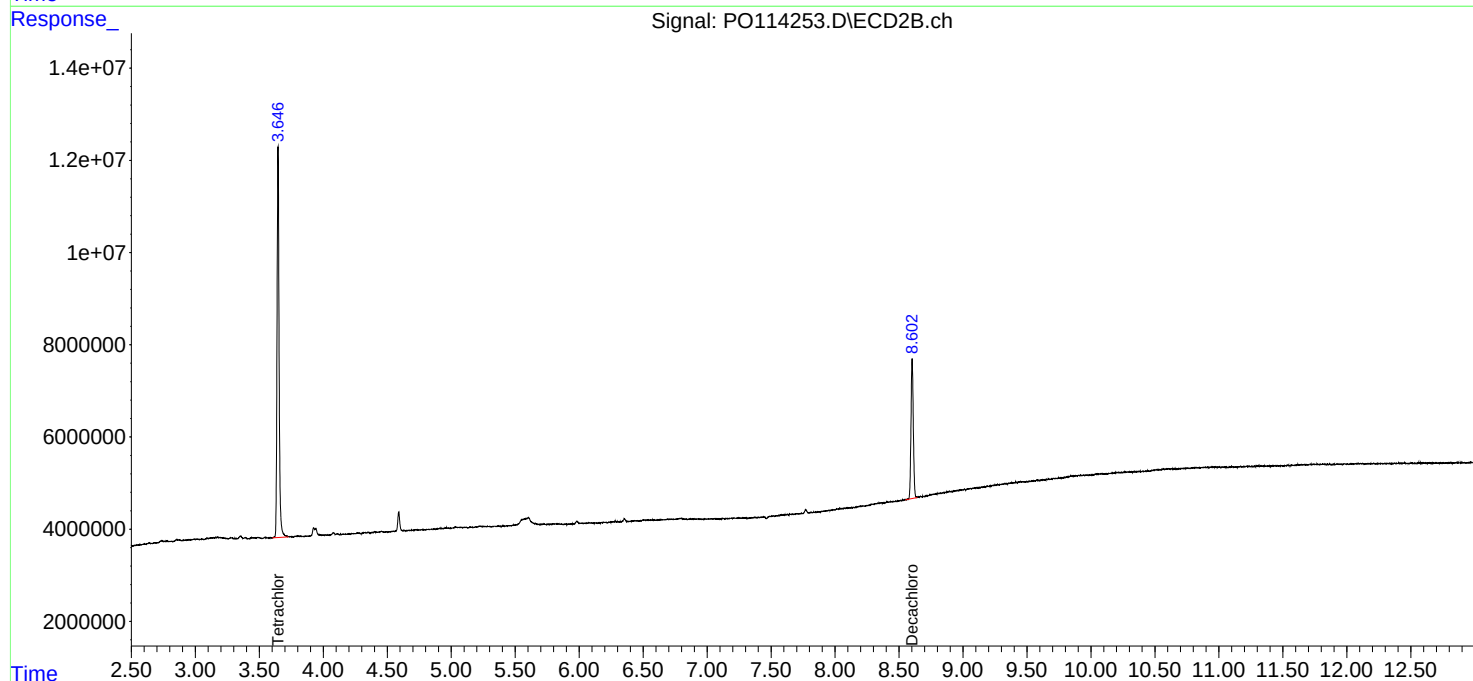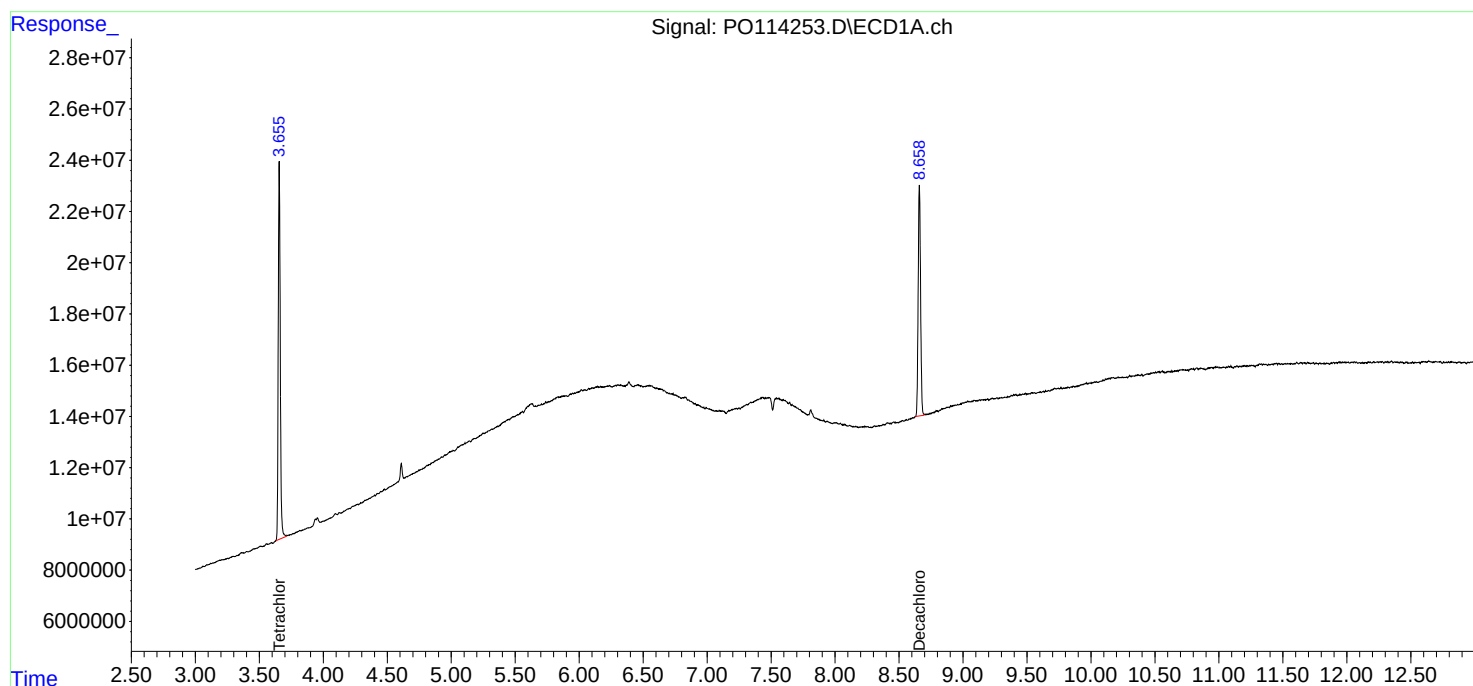


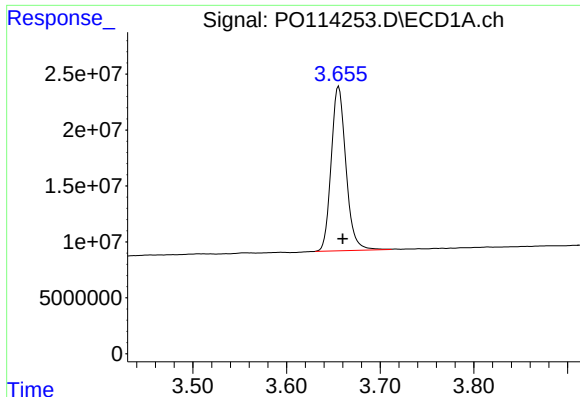

#1 Tetrachloro-m-xylene


R.T.: 3.656 min
Delta R.T.: -0.004 min
Response: 160618446
Conc: 18.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

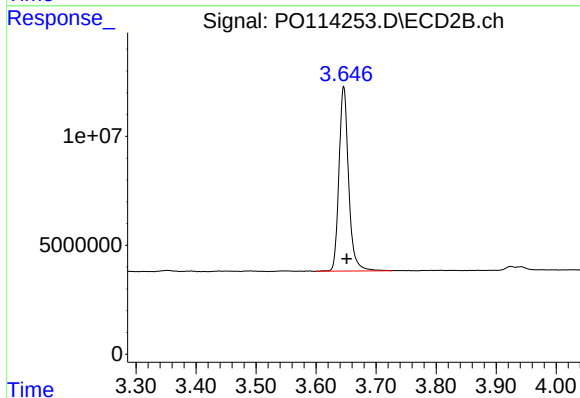


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: -0.005 min
Response: 94587815
Conc: 17.71 ng/ml

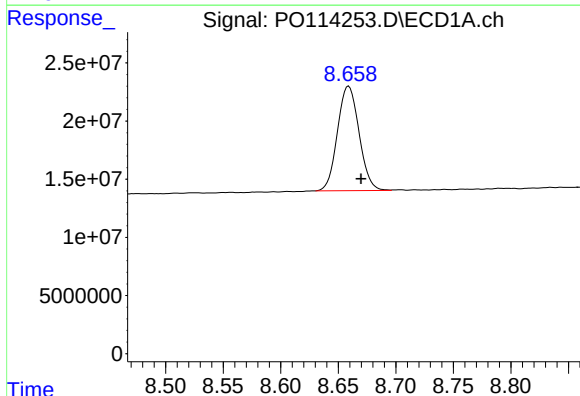

#2 Decachlorobiphenyl

R.T.: 8.659 min
Delta R.T.: -0.011 min
Response: 117712375
Conc: 17.59 ng/ml

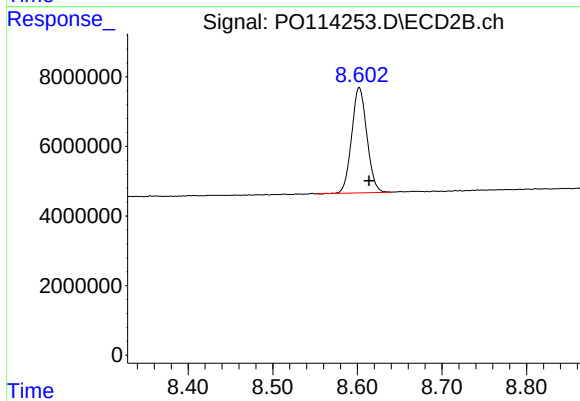

#2 Decachlorobiphenyl

R.T.: 8.602 min
Delta R.T.: -0.012 min
Response: 37830684
Conc: 18.12 ng/ml

Report of Analysis

Client:	G Environmental		Date Collected:	10/06/25	
Project:	Newport		Date Received:	10/06/25	
Client Sample ID:	PIBLK-PO114268.D		SDG No.:	Q3277	
Lab Sample ID:	I.BLK-PO114268.D		Matrix:	WATER	
Analytical Method:	8082A		% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units: mL	Final Vol:	10000	uL
Soil Aliquot Vol:		uL	Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	5030				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO114268.D	1		10/06/25	Po100625

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	17.5		60 - 140	87%	SPK: 20
2051-24-3	Decachlorobiphenyl	14.6		60 - 140	73%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100625\
 Data File : PO114268.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2025 17:08
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 02:12:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:49:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.654	3.646	155.8E6	93249179	17.660	17.459
2) SA Decachlor...	8.659	8.604	97842789	33630944	14.625	16.109

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100625\
Data File : PO114268.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2025 17:08
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 02:12:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

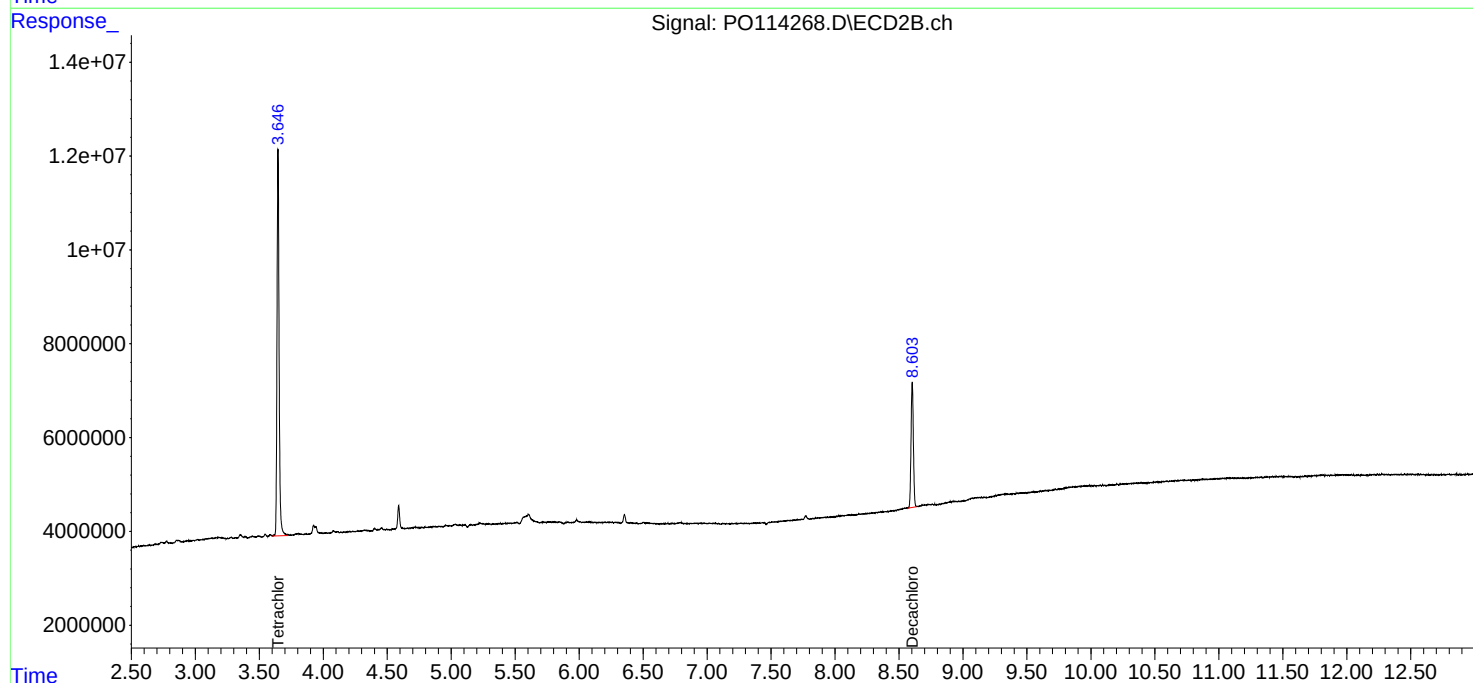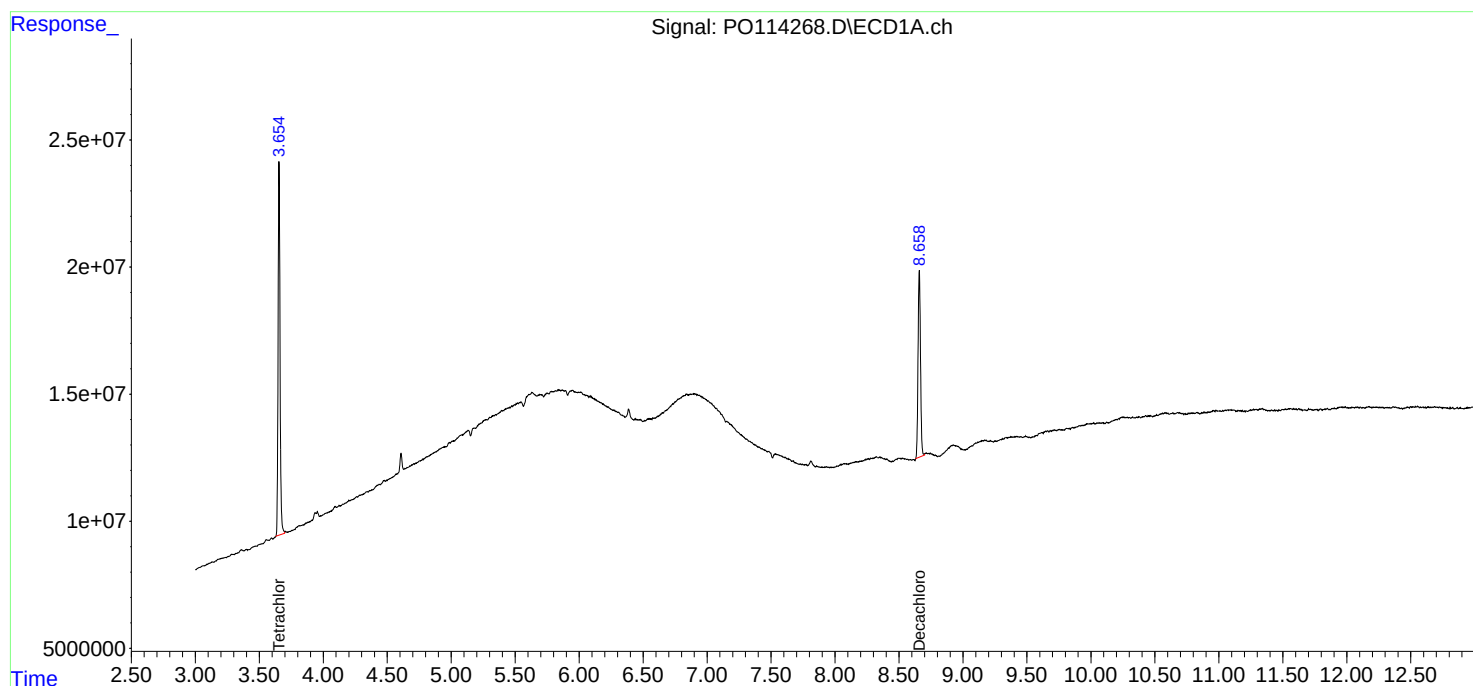


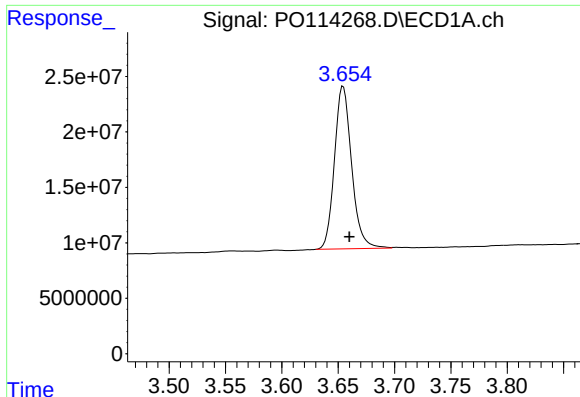

#1 Tetrachloro-m-xylene


R.T.: 3.654 min
Delta R.T.: -0.006 min
Response: 155752192
Conc: 17.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

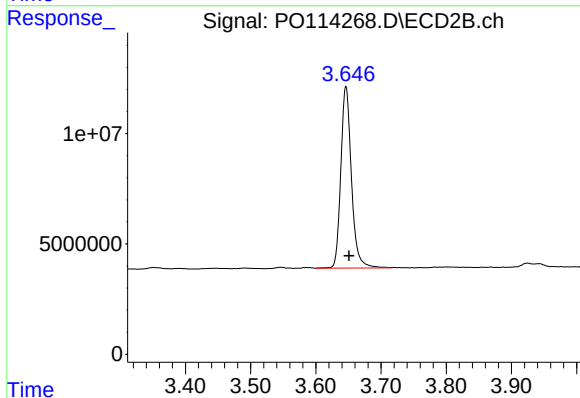


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: -0.005 min
Response: 93249179
Conc: 17.46 ng/ml

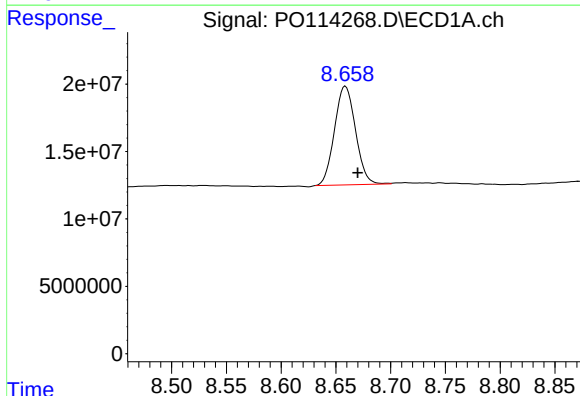

#2 Decachlorobiphenyl

R.T.: 8.659 min
Delta R.T.: -0.011 min
Response: 97842789
Conc: 14.62 ng/ml

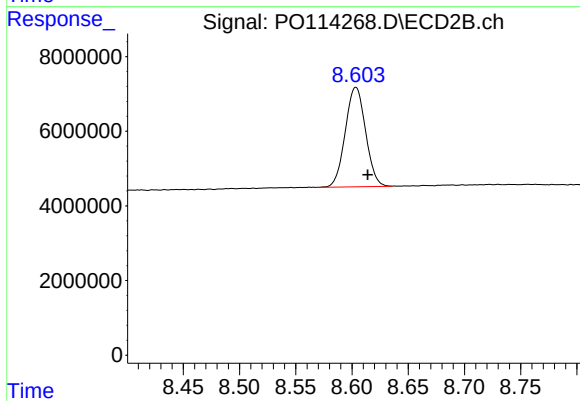

#2 Decachlorobiphenyl

R.T.: 8.604 min
Delta R.T.: -0.010 min
Response: 33630944
Conc: 16.11 ng/ml

Report of Analysis

Client:	G Environmental	Date Collected:	
Project:	Newport	Date Received:	
Client Sample ID:	PB169987BS	SDG No.:	Q3277
Lab Sample ID:	PB169987BS	Matrix:	SOIL
Analytical Method:	8082A	% Solid:	100
Sample Wt/Vol:	30.03	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	Injection Volume :	
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO114255.D	1	10/06/25 08:43	10/06/25 12:28	PB169987

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	180		3.90	17.0	ug/kg
11104-28-2	Aroclor-1221	4.00	U	4.00	17.0	ug/kg
11141-16-5	Aroclor-1232	3.70	U	3.70	17.0	ug/kg
53469-21-9	Aroclor-1242	4.00	U	4.00	17.0	ug/kg
12672-29-6	Aroclor-1248	5.90	U	5.90	17.0	ug/kg
11097-69-1	Aroclor-1254	3.20	U	3.20	17.0	ug/kg
37324-23-5	Aroclor-1262	5.00	U	5.00	17.0	ug/kg
11100-14-4	Aroclor-1268	3.60	U	3.60	17.0	ug/kg
11096-82-5	Aroclor-1260	182		3.20	17.0	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	19.7		32 - 144	99%	SPK: 20
2051-24-3	Decachlorobiphenyl	20.1		32 - 175	101%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100625\
 Data File : PO114255.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2025 12:28
 Operator : YP/AJ
 Sample : PB169987BS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB169987BS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/06/2025
 Supervised By :mohammad ahmed 10/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 13:05:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:49:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.655	3.644	173.7E6	98652255	19.696	18.471
2) SA Decachlor...	8.660	8.602	134.8E6	41571821	20.144	19.912
Target Compounds						
3) L1 AR-1016-1	4.737	4.713	165.1E6	93726775	543.809	514.300m
4) L1 AR-1016-2	4.755	4.731	254.3E6	140.5E6	558.743	507.367m
5) L1 AR-1016-3	4.812	4.907	159.9E6	74103468	534.297	496.194
6) L1 AR-1016-4	4.931	4.949	125.2E6	59400382	520.983	492.094
7) L1 AR-1016-5	5.187	5.160	131.5E6	75075732	547.788	500.284
31) L7 AR-1260-1	6.221	6.186	298.2E6	125.6E6	608.233	499.938
32) L7 AR-1260-2	6.411	6.374	438.1E6	154.3E6	572.002	466.822
33) L7 AR-1260-3	6.776	6.524	322.8E6	130.3E6	479.798	464.664
34) L7 AR-1260-4	7.034	6.992	228.7E6	77643553	528.423	406.062
35) L7 AR-1260-5	7.278	7.235	611.4E6	171.3E6	539.683	402.348 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100625\
Data File : PO114255.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2025 12:28
Operator : YP/AJ
Sample : PB169987BS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

PB169987BS

Manual Integrations



APPROVED

Reviewed By :Yogesh Patel 10/06/2025

Supervised By :mohammad ahmed 10/08/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 13:05:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

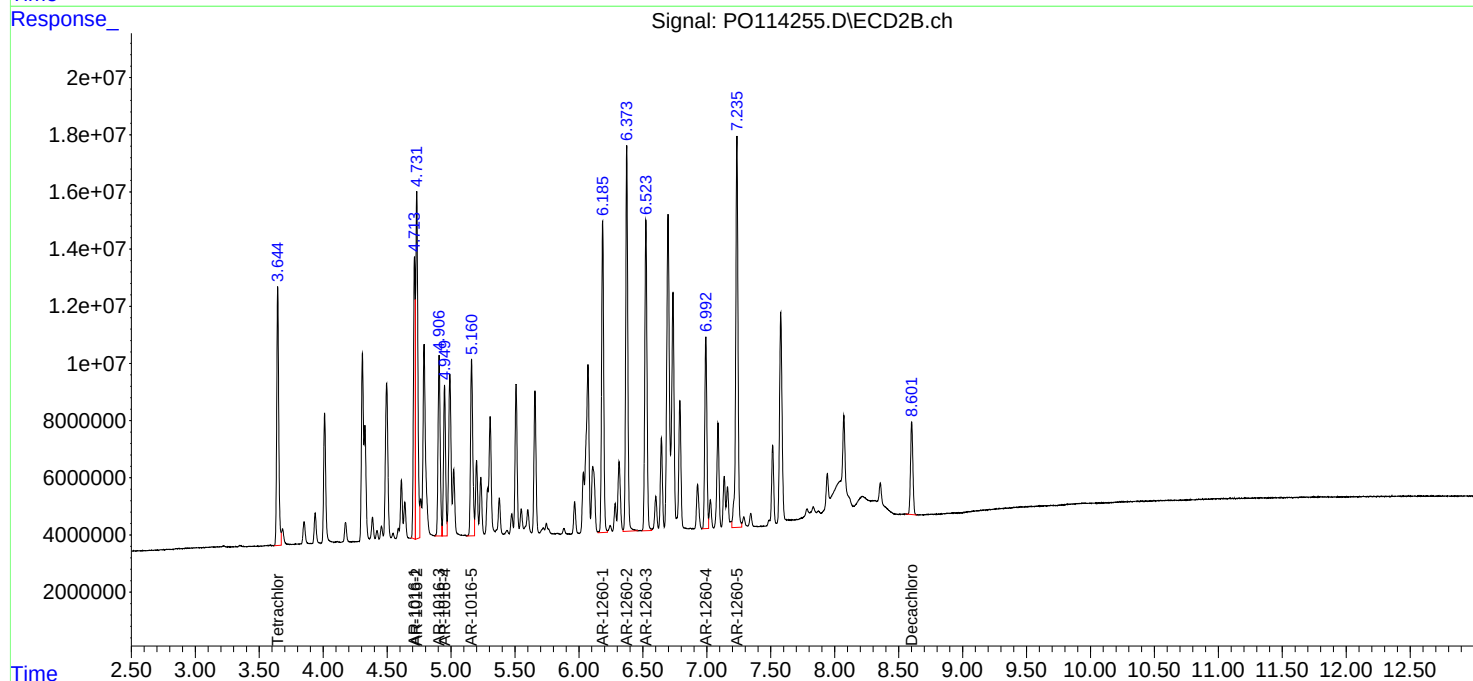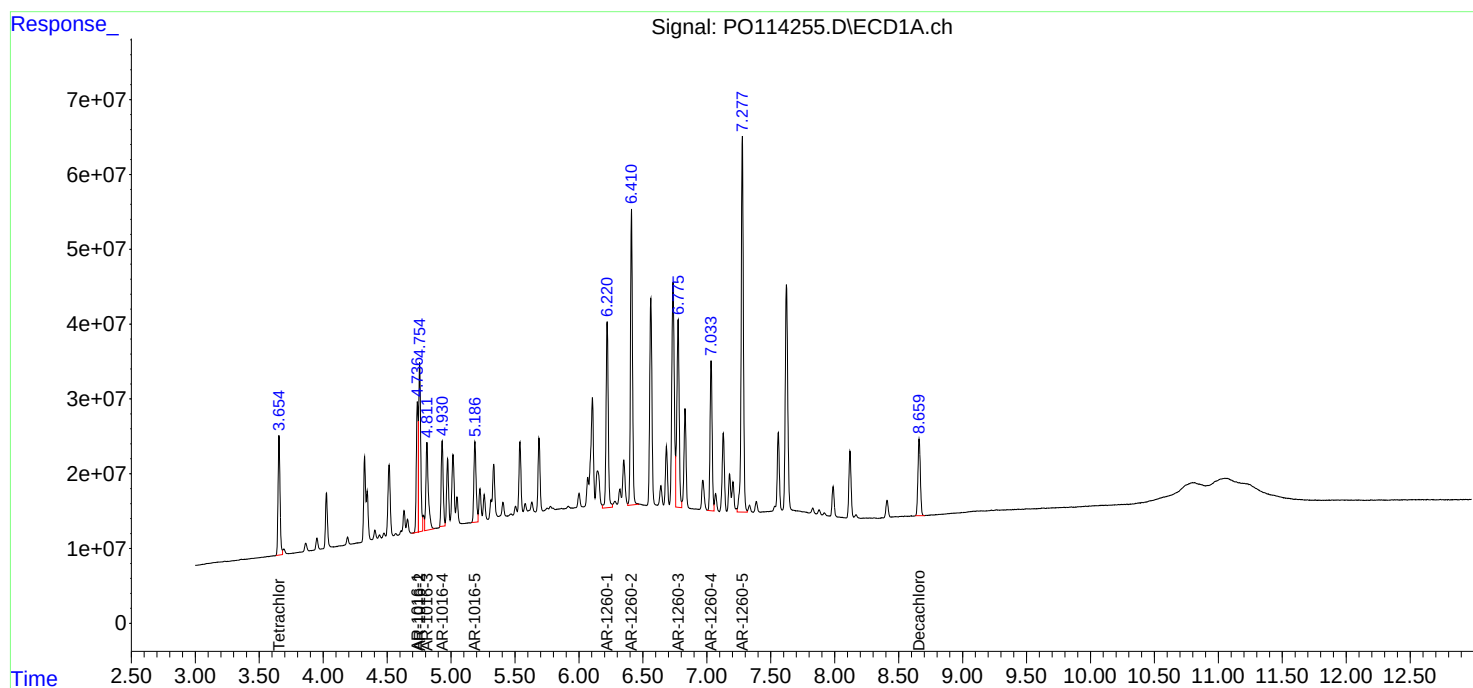

Report of Analysis

Client:	G Environmental	Date Collected:	10/03/25
Project:	Newport	Date Received:	10/03/25
Client Sample ID:	TR-01-100325MS	SDG No.:	Q3277
Lab Sample ID:	Q3288-01MS	Matrix:	SOIL
Analytical Method:	8082A	% Solid:	92.9
Sample Wt/Vol:	30.03	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	Injection Volume :	
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO114259.D	1	10/06/25 08:43	10/06/25 13:41	PB169987

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	160		4.20	18.3	ug/kg
11104-28-2	Aroclor-1221	4.30	U	4.30	18.3	ug/kg
11141-16-5	Aroclor-1232	4.00	U	4.00	18.3	ug/kg
53469-21-9	Aroclor-1242	4.30	U	4.30	18.3	ug/kg
12672-29-6	Aroclor-1248	6.40	U	6.40	18.3	ug/kg
11097-69-1	Aroclor-1254	3.50	U	3.50	18.3	ug/kg
37324-23-5	Aroclor-1262	5.40	U	5.40	18.3	ug/kg
11100-14-4	Aroclor-1268	3.90	U	3.90	18.3	ug/kg
11096-82-5	Aroclor-1260	141		3.50	18.3	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	13.6		32 - 144	68%	SPK: 20
2051-24-3	Decachlorobiphenyl	14.6		32 - 175	73%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100625\
 Data File : PO114259.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2025 13:41
 Operator : YP/AJ
 Sample : Q3288-01MS
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TR-01-100325MS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/06/2025
 Supervised By :mohammad ahmed 10/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 15:04:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:49:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.656	3.646	113.9E6	72472222	12.919	13.569
2) SA Decachlor...	8.660	8.604	92194845	30375967	13.780	14.550
Target Compounds						
3) L1 AR-1016-1	4.736	4.715	116.6E6	77690323	384.081	426.304m
4) L1 AR-1016-2	4.754	4.733	185.2E6	127.2E6	406.875	459.376m
5) L1 AR-1016-3	4.812	4.908	118.2E6	66659798	395.137	446.352
6) L1 AR-1016-4	4.930	4.951	91479661	54362746	380.565	450.361
7) L1 AR-1016-5	5.187	5.162	103.8E6	67799459	432.521	451.797
31) L7 AR-1260-1	6.221	6.187	191.4E6	111.3E6	390.440	442.985
32) L7 AR-1260-2	6.411	6.375	299.6E6	133.8E6	391.254	404.808
33) L7 AR-1260-3	6.775	6.525	227.4E6	111.3E6	337.952	397.038
34) L7 AR-1260-4	7.033	6.994	163.6E6	67728253	378.059	354.206
35) L7 AR-1260-5	7.276	7.237	464.8E6	154.5E6	410.317	362.883

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100625\
Data File : PO114259.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2025 13:41
Operator : YP/AJ
Sample : Q3288-01MS
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

TR-01-100325MS

Manual Integrations



APPROVED

Reviewed By :Yogesh Patel 10/06/2025

Supervised By :mohammad ahmed 10/08/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 15:04:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

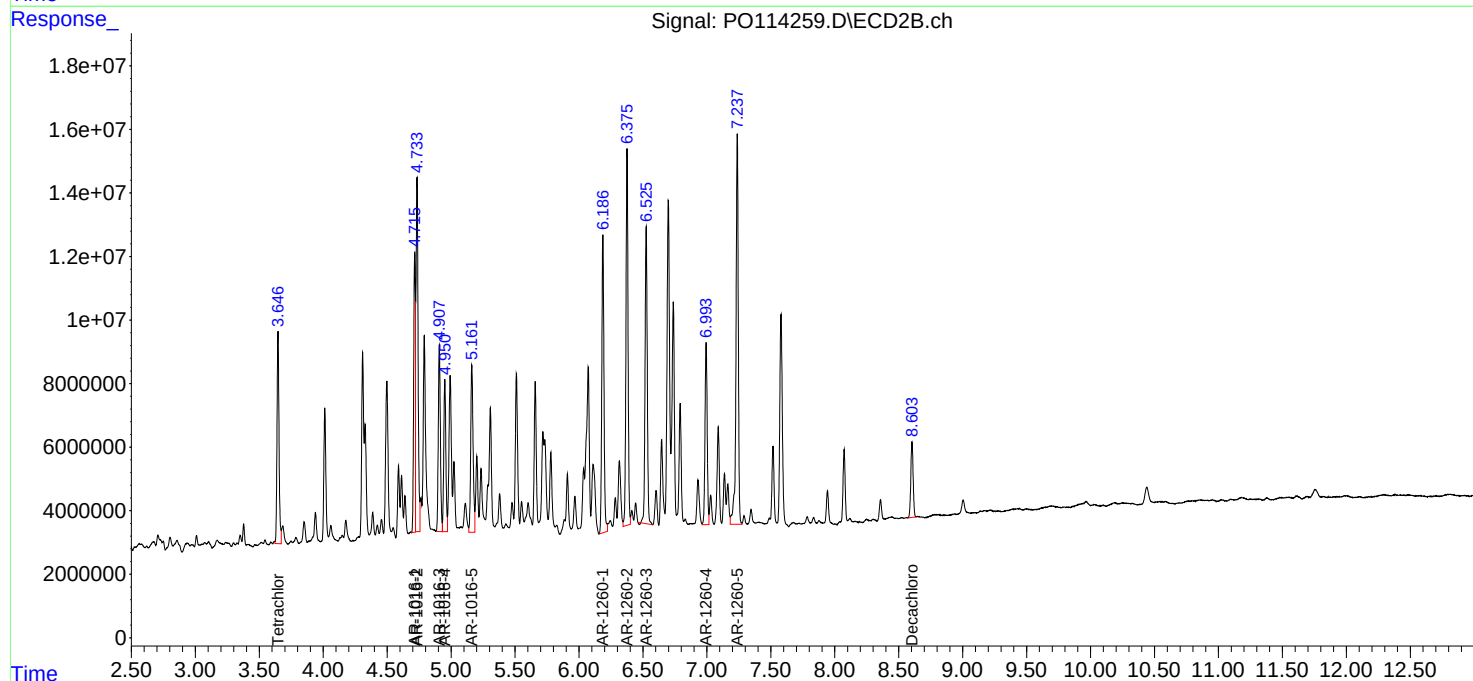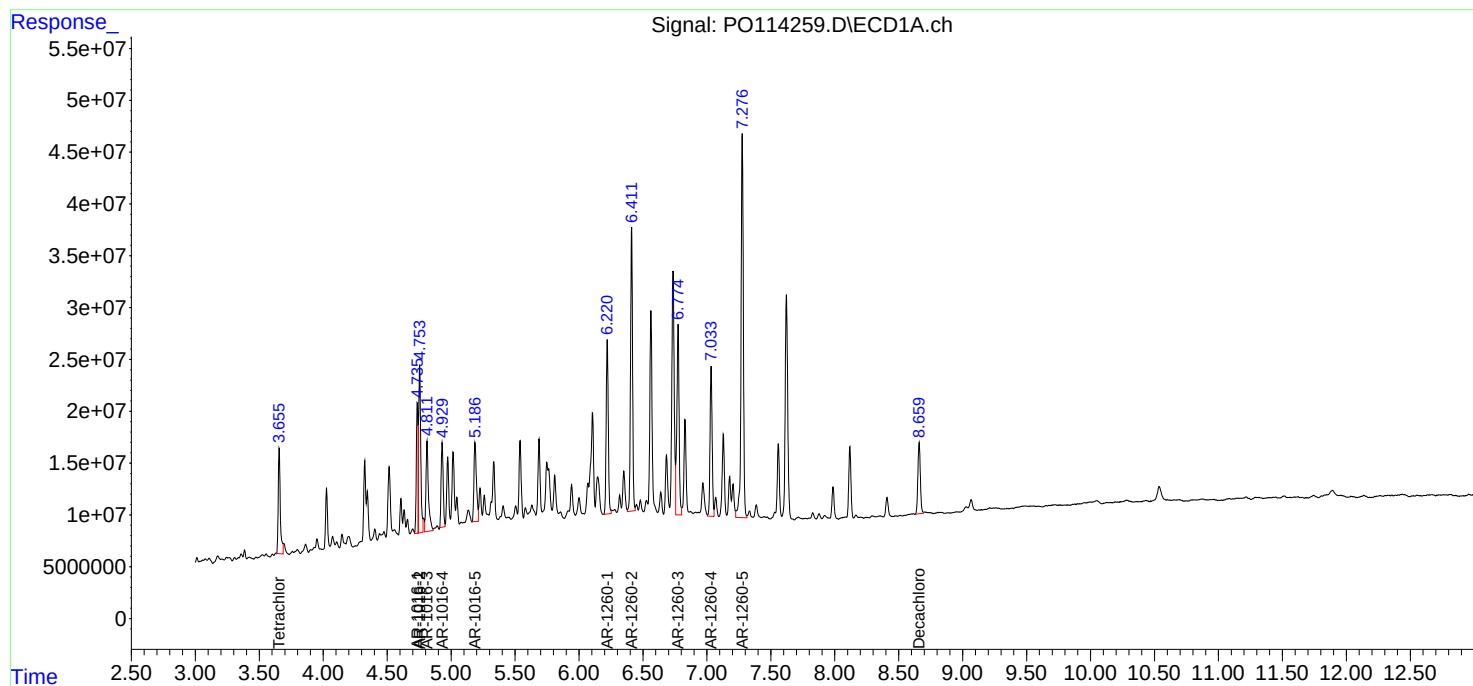

Report of Analysis

Client:	G Environmental		Date Collected:	10/03/25	
Project:	Newport		Date Received:	10/03/25	
Client Sample ID:	TR-01-100325MSD		SDG No.:	Q3277	
Lab Sample ID:	Q3288-01MSD		Matrix:	SOIL	
Analytical Method:	8082A		% Solid:	92.9	Decanted:
Sample Wt/Vol:	30.08	Units: g	Final Vol:	10000	uL
Soil Aliquot Vol:		uL	Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	SW3541B				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO114260.D	1	10/06/25 08:43	10/06/25 13:59	PB169987

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	158		4.20	18.3	ug/kg
11104-28-2	Aroclor-1221	4.30	U	4.30	18.3	ug/kg
11141-16-5	Aroclor-1232	4.00	U	4.00	18.3	ug/kg
53469-21-9	Aroclor-1242	4.30	U	4.30	18.3	ug/kg
12672-29-6	Aroclor-1248	6.40	U	6.40	18.3	ug/kg
11097-69-1	Aroclor-1254	3.40	U	3.40	18.3	ug/kg
37324-23-5	Aroclor-1262	5.40	U	5.40	18.3	ug/kg
11100-14-4	Aroclor-1268	3.90	U	3.90	18.3	ug/kg
11096-82-5	Aroclor-1260	135		3.50	18.3	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	14.1		32 - 144	70%	SPK: 20
2051-24-3	Decachlorobiphenyl	14.1		32 - 175	70%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100625\
 Data File : PO114260.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2025 13:59
 Operator : YP/AJ
 Sample : Q3288-01MSD
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TR-01-100325MSD

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/06/2025
 Supervised By :mohammad ahmed 10/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 15:05:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:49:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.656	3.647	117.5E6	75032203	13.322	14.048
2) SA Decachlor...	8.660	8.604	85135376	29322549	12.725	14.045
Target Compounds						
3) L1 AR-1016-1	4.738	4.716	124.9E6	82031247	411.435	450.124m
4) L1 AR-1016-2	4.755	4.734	192.2E6	122.8E6	422.386	443.614m
5) L1 AR-1016-3	4.812	4.909	126.0E6	65916980	421.245	441.378
6) L1 AR-1016-4	4.931	4.952	95083999	52828723	395.560	437.652
7) L1 AR-1016-5	5.188	5.162	105.8E6	65592580	440.446	437.091
31) L7 AR-1260-1	6.222	6.187	189.3E6	109.2E6	386.150	434.392
32) L7 AR-1260-2	6.411	6.376	286.5E6	129.6E6	374.057	391.991
33) L7 AR-1260-3	6.776	6.526	213.9E6	104.3E6	317.858	372.075
34) L7 AR-1260-4	7.034	6.995	151.1E6	64144928	349.122	335.466
35) L7 AR-1260-5	7.278	7.237	433.6E6	147.8E6	382.763	347.121

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100625\
Data File : PO114260.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2025 13:59
Operator : YP/AJ
Sample : Q3288-01MSD
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TR-01-100325MSD

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/06/2025
Supervised By :mohammad ahmed 10/08/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 15:05:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

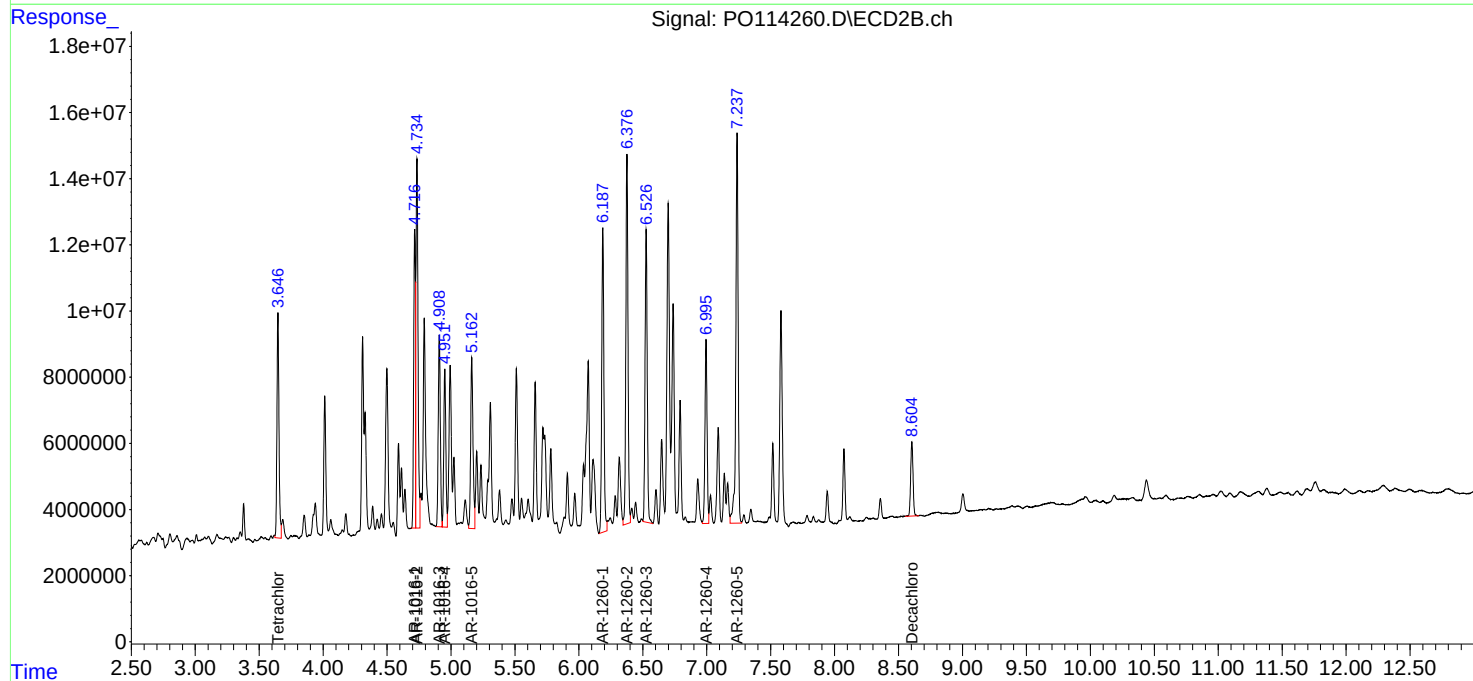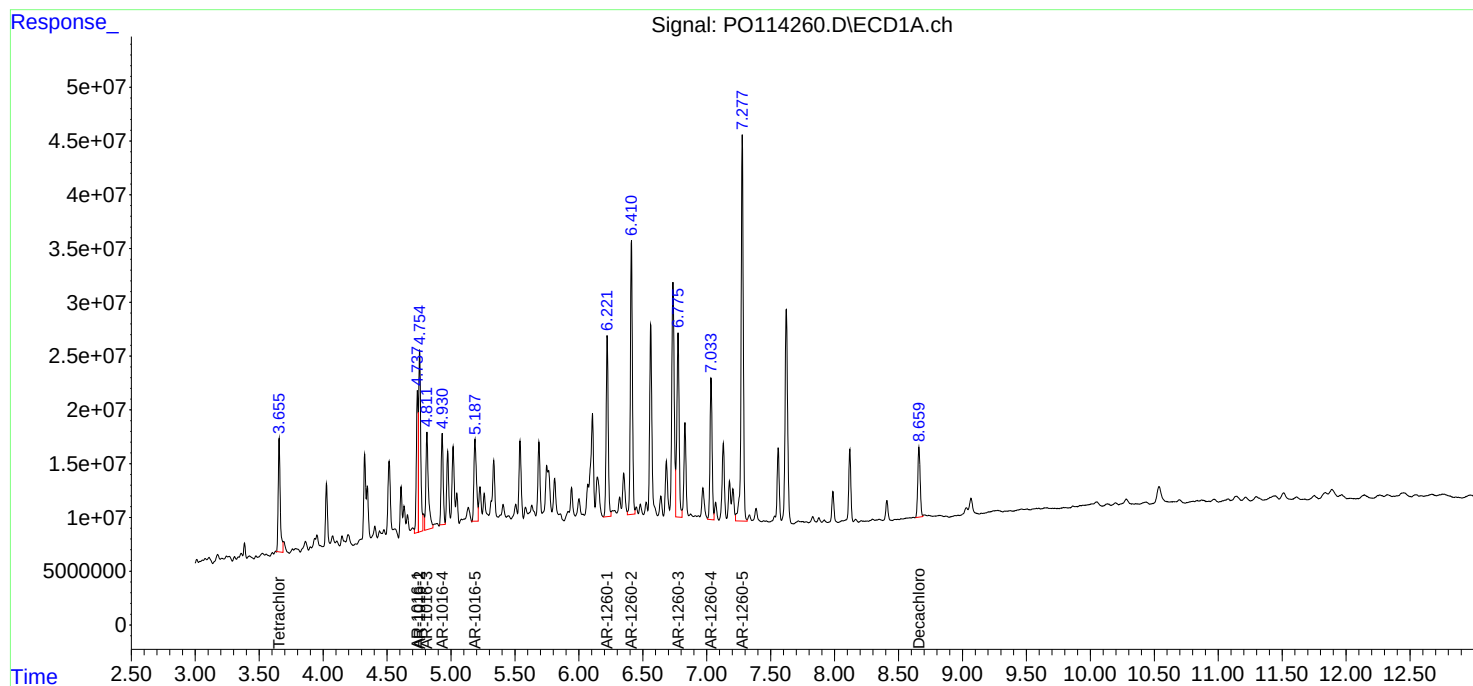

Manual Integration Report

Sequence:	po091525	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660ICC250	PO113723.D	AR-1016-3 #2	yogesh	9/16/2025 8:17:06 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1660ICC250	PO113723.D	AR-1016-4	yogesh	9/16/2025 8:17:06 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1660ICC250	PO113723.D	AR-1016-4 #2	yogesh	9/16/2025 8:17:06 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1660ICC250	PO113723.D	AR-1016-5	yogesh	9/16/2025 8:17:06 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1660ICC250	PO113723.D	AR-1016-5 #2	yogesh	9/16/2025 8:17:06 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1660ICC050	PO113724.D	AR-1016-3 #2	yogesh	9/16/2025 8:17:08 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1660ICC050	PO113724.D	AR-1016-4	yogesh	9/16/2025 8:17:08 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1660ICC050	PO113724.D	AR-1016-4 #2	yogesh	9/16/2025 8:17:08 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1660ICC050	PO113724.D	AR-1016-5	yogesh	9/16/2025 8:17:08 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1660ICC050	PO113724.D	AR-1016-5 #2	yogesh	9/16/2025 8:17:08 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1660ICC050	PO113724.D	AR-1260-4 #2	yogesh	9/16/2025 8:17:08 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1242ICC050	PO113731.D	AR-1242-1	yogesh	9/16/2025 8:17:09 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1242ICC050	PO113731.D	AR-1242-2	yogesh	9/16/2025 8:17:09 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software

Manual Integration Report

Sequence:	po091525	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1242ICC050	PO113731.D	AR-1242-3 #2	yogesh	9/16/2025 8:17:09 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1242ICC050	PO113731.D	AR-1242-4 #2	yogesh	9/16/2025 8:17:09 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1242ICC050	PO113731.D	AR-1242-5 #2	yogesh	9/16/2025 8:17:09 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1242ICC050	PO113731.D	Tetrachloro-m-xylene	yogesh	9/16/2025 8:17:09 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1242ICC050	PO113731.D	Tetrachloro-m-xylene #2	yogesh	9/16/2025 8:17:09 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1248ICC250	PO113735.D	Tetrachloro-m-xylene	yogesh	9/16/2025 8:17:11 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1254ICC050	PO113741.D	AR-1254-1	yogesh	9/16/2025 8:17:15 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1254ICC050	PO113741.D	AR-1254-2	yogesh	9/16/2025 8:17:15 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1254ICC050	PO113741.D	AR-1254-3	yogesh	9/16/2025 8:17:15 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1254ICC050	PO113741.D	AR-1254-4	yogesh	9/16/2025 8:17:15 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1268ICC050	PO113747.D	AR-1268-1 #2	yogesh	9/16/2025 8:17:16 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1268ICC050	PO113747.D	AR-1268-2 #2	yogesh	9/16/2025 8:17:16 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1268ICC050	PO113747.D	AR-1268-3	yogesh	9/16/2025 8:17:16 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software

Manual Integration Report

Sequence:

po091525

Instrument

ECD_o

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1268ICC050	PO113747.D	AR-1268-3 #2	yogesh	9/16/2025 8:17:16 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1268ICC050	PO113747.D	Tetrachloro-m-xylene	yogesh	9/16/2025 8:17:16 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
AR1268ICC050	PO113747.D	Tetrachloro-m-xylene #2	yogesh	9/16/2025 8:17:16 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software
PO091525ICV500	PO113748.D	AR-1260-5	yogesh	9/16/2025 8:45:08 AM	mohammad	9/17/2025 2:07:54	Peak Integrated by Software

Manual Integration Report

Sequence:	PO100625	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660CCC500	PO114249.D	AR-1016-1	yogesh	10/6/2025 1:33:43 PM	mohammad	10/8/2025 3:34:35	Peak Integrated by Software
AR1660CCC500	PO114249.D	AR-1016-1 #2	yogesh	10/6/2025 1:33:43 PM	mohammad	10/8/2025 3:34:35	Peak Integrated by Software
AR1660CCC500	PO114249.D	AR-1016-2	yogesh	10/6/2025 1:33:43 PM	mohammad	10/8/2025 3:34:35	Peak Integrated by Software
AR1660CCC500	PO114249.D	AR-1016-2 #2	yogesh	10/6/2025 1:33:43 PM	mohammad	10/8/2025 3:34:35	Peak Integrated by Software
AR1660CCC500	PO114249.D	AR-1260-1	yogesh	10/6/2025 1:33:43 PM	mohammad	10/8/2025 3:34:35	Peak Integrated by Software
AR1660CCC500	PO114249.D	AR-1260-4	yogesh	10/6/2025 1:33:43 PM	mohammad	10/8/2025 3:34:35	Peak Integrated by Software
AR1660CCC500	PO114249.D	AR-1260-5	yogesh	10/6/2025 1:33:43 PM	mohammad	10/8/2025 3:34:35	Peak Integrated by Software
AR1242CCC500	PO114250.D	AR-1242-1 #2	yogesh	10/6/2025 1:33:45 PM	mohammad	10/8/2025 3:34:35	Peak Integrated by Software
AR1242CCC500	PO114250.D	AR-1242-2 #2	yogesh	10/6/2025 1:33:45 PM	mohammad	10/8/2025 3:34:35	Peak Integrated by Software
AR1242CCC500	PO114250.D	AR-1242-4	yogesh	10/6/2025 1:33:45 PM	mohammad	10/8/2025 3:34:35	Peak Integrated by Software
AR1248CCC500	PO114251.D	AR-1248-1 #2	yogesh	10/6/2025 1:33:47 PM	mohammad	10/8/2025 3:34:35	Peak Integrated by Software
PB169987BS	PO114255.D	AR-1016-2 #2	yogesh	10/6/2025 1:33:49 PM	mohammad	10/8/2025 3:34:35	Peak Integrated by Software
Q3288-01MS	PO114259.D	AR-1016-1 #2	yogesh	10/6/2025 3:59:34 PM	mohammad	10/8/2025 3:34:35	Peak Integrated by Software

Manual Integration Report

Sequence:	PO100625	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
Q3288-01MS	PO114259.D	AR-1016-2 #2	yogesh	10/6/2025 3:59:34 PM	mohammad	10/8/2025 3:34:35	Peak Integrated by Software
Q3288-01MSD	PO114260.D	AR-1016-1 #2	yogesh	10/6/2025 3:59:35 PM	mohammad	10/8/2025 3:34:35	Peak Integrated by Software
Q3288-01MSD	PO114260.D	AR-1016-2 #2	yogesh	10/6/2025 3:59:35 PM	mohammad	10/8/2025 3:34:35	Peak Integrated by Software
AR1660CCC500	PO114264.D	AR-1016-1 #2	yogesh	10/7/2025 10:33:40 AM	mohammad	10/8/2025 3:34:35	Peak Integrated by Software
AR1660CCC500	PO114264.D	AR-1016-5	yogesh	10/7/2025 10:33:40 AM	mohammad	10/8/2025 3:34:35	Peak Integrated by Software
AR1248CCC500	PO114266.D	AR-1248-4	yogesh	10/7/2025 10:33:42 AM	mohammad	10/8/2025 3:34:35	Peak Integrated by Software
AR1248CCC500	PO114266.D	AR-1248-5	yogesh	10/7/2025 10:33:42 AM	mohammad	10/8/2025 3:34:35	Peak Integrated by Software

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO091525

Review By	yogesh	Review On	9/15/2025 12:11:18 PM
Supervise By	mohammad	Supervise On	9/17/2025 2:07:54 AM
SubDirectory	PO091525	HP Acquire Method	HP Processing Method PO091525
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,PP24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854 PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862		

Sr#	Sampleld	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO113718.D	15 Sep 2025 08:58	YP/AJ	Ok
2	I.BLK	PO113719.D	15 Sep 2025 09:16	YP/AJ	Ok
3	AR1660ICC1000	PO113720.D	15 Sep 2025 09:34	YP/AJ	Ok
4	AR1660ICC750	PO113721.D	15 Sep 2025 09:53	YP/AJ	Ok
5	AR1660ICC500	PO113722.D	15 Sep 2025 10:11	YP/AJ	Ok
6	AR1660ICC250	PO113723.D	15 Sep 2025 10:30	YP/AJ	Ok,M
7	AR1660ICC050	PO113724.D	15 Sep 2025 10:48	YP/AJ	Ok,M
8	AR1221ICC500	PO113725.D	15 Sep 2025 11:06	YP/AJ	Ok
9	AR1232ICC500	PO113726.D	15 Sep 2025 11:25	YP/AJ	Ok
10	AR1242ICC1000	PO113727.D	15 Sep 2025 11:43	YP/AJ	Ok
11	AR1242ICC750	PO113728.D	15 Sep 2025 12:02	YP/AJ	Ok
12	AR1242ICC500	PO113729.D	15 Sep 2025 12:20	YP/AJ	Ok
13	AR1242ICC250	PO113730.D	15 Sep 2025 12:38	YP/AJ	Ok
14	AR1242ICC050	PO113731.D	15 Sep 2025 13:34	YP/AJ	Ok,M
15	AR1248ICC1000	PO113732.D	15 Sep 2025 13:54	YP/AJ	Ok
16	AR1248ICC750	PO113733.D	15 Sep 2025 14:13	YP/AJ	Ok
17	AR1248ICC500	PO113734.D	15 Sep 2025 14:31	YP/AJ	Ok
18	AR1248ICC250	PO113735.D	15 Sep 2025 14:49	YP/AJ	Ok,M
19	AR1248ICC050	PO113736.D	15 Sep 2025 15:26	YP/AJ	Ok
20	AR1254ICC1000	PO113737.D	15 Sep 2025 15:45	YP/AJ	Ok
21	AR1254ICC750	PO113738.D	15 Sep 2025 16:02	YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO091525

Review By	yogesh	Review On	9/15/2025 12:11:18 PM
Supervise By	mohammad	Supervise On	9/17/2025 2:07:54 AM
SubDirectory	PO091525	HP Acquire Method	HP Processing Method PO091525
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,PP24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854		
CCC			
Internal Standard/PEM			
ICV/I.BLK	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	AR1254ICC500	PO113739.D	15 Sep 2025 16:20	YP/AJ	Ok
23	AR1254ICC250	PO113740.D	15 Sep 2025 16:38	YP/AJ	Ok
24	AR1254ICC050	PO113741.D	15 Sep 2025 17:14	YP/AJ	Ok,M
25	AR1262ICC500	PO113742.D	15 Sep 2025 17:33	YP/AJ	Ok
26	AR1268ICC1000	PO113743.D	15 Sep 2025 17:51	YP/AJ	Ok
27	AR1268ICC750	PO113744.D	15 Sep 2025 18:10	YP/AJ	Ok
28	AR1268ICC500	PO113745.D	15 Sep 2025 18:27	YP/AJ	Ok
29	AR1268ICC250	PO113746.D	15 Sep 2025 18:45	YP/AJ	Ok
30	AR1268ICC050	PO113747.D	15 Sep 2025 19:21	YP/AJ	Ok,M
31	PO091525ICV500	PO113748.D	15 Sep 2025 19:40	YP/AJ	Ok,M
32	AR1242ICV500	PO113749.D	15 Sep 2025 20:16	YP/AJ	Ok
33	AR1248ICV500	PO113750.D	15 Sep 2025 21:11	YP/AJ	Ok
34	AR1254ICV500	PO113751.D	15 Sep 2025 22:05	YP/AJ	Ok
35	AR1268ICV500	PO113752.D	15 Sep 2025 23:00	YP/AJ	Ok
36	DDT ANALOG	PO113753.D	15 Sep 2025 23:37	YP/AJ	Ok,M

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO100625

Review By	yogesh	Review On	10/6/2025 12:37:59 PM
Supervise By	mohammad	Supervise On	10/8/2025 3:34:35 AM
SubDirectory	PO100625	HP Acquire Method	HP Processing Method PO091925
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,PP24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854		
CCC	PP24824,PP24828,PP24832,PP24836,PP24840,PP24844,PP24852		
Internal Standard/PEM			
ICV/I.BLK	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO114248.D	06 Oct 2025 09:10	YP/AJ	Ok
2	AR1660CCC500	PO114249.D	06 Oct 2025 09:49	YP/AJ	Ok,M
3	AR1242CCC500	PO114250.D	06 Oct 2025 10:07	YP/AJ	Not Ok
4	AR1248CCC500	PO114251.D	06 Oct 2025 10:25	YP/AJ	Ok,M
5	AR1254CCC500	PO114252.D	06 Oct 2025 10:44	YP/AJ	Ok
6	I.BLK	PO114253.D	06 Oct 2025 11:02	YP/AJ	Ok
7	PB169987BL	PO114254.D	06 Oct 2025 12:10	YP/AJ	Ok
8	PB169987BS	PO114255.D	06 Oct 2025 12:28	YP/AJ	Ok,M
9	Q3249-11	PO114256.D	06 Oct 2025 12:46	YP/AJ	Ok
10	Q3277-01	PO114257.D	06 Oct 2025 13:05	YP/AJ	Ok
11	Q3288-01	PO114258.D	06 Oct 2025 13:22	YP/AJ	Ok
12	Q3288-01MS	PO114259.D	06 Oct 2025 13:41	YP/AJ	Ok,M
13	Q3288-01MSD	PO114260.D	06 Oct 2025 13:59	YP/AJ	Ok,M
14	Q3289-01	PO114261.D	06 Oct 2025 14:17	YP/AJ	Ok
15	Q3289-03	PO114262.D	06 Oct 2025 14:36	YP/AJ	Ok,M
16	Q3289-05	PO114263.D	06 Oct 2025 14:54	YP/AJ	Ok
17	AR1660CCC500	PO114264.D	06 Oct 2025 15:55	YP/AJ	Ok,M
18	AR1242CCC500	PO114265.D	06 Oct 2025 16:14	YP/AJ	Ok
19	AR1248CCC500	PO114266.D	06 Oct 2025 16:32	YP/AJ	Ok,M
20	AR1254CCC500	PO114267.D	06 Oct 2025 16:51	YP/AJ	Ok
21	I.BLK	PO114268.D	06 Oct 2025 17:08	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO091525

Review By	yogesh	Review On	9/15/2025 12:11:18 PM
Supervise By	mohammad	Supervise On	9/17/2025 2:07:54 AM
SubDirectory	PO091525	HP Acquire Method	HP Processing Method PO091525

STD. NAME	STD REF.#
Tune/Reschk	
Initial Calibration Stds	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,PP24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854
CCC	
Internal Standard/PEM	
ICV/I.BLK	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleID	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO113718.D	15 Sep 2025 08:58		YP/AJ	Ok
2	I.BLK	I.BLK	PO113719.D	15 Sep 2025 09:16		YP/AJ	Ok
3	AR1660ICC1000	AR1660ICC1000	PO113720.D	15 Sep 2025 09:34		YP/AJ	Ok
4	AR1660ICC750	AR1660ICC750	PO113721.D	15 Sep 2025 09:53		YP/AJ	Ok
5	AR1660ICC500	AR1660ICC500	PO113722.D	15 Sep 2025 10:11		YP/AJ	Ok
6	AR1660ICC250	AR1660ICC250	PO113723.D	15 Sep 2025 10:30		YP/AJ	Ok,M
7	AR1660ICC050	AR1660ICC050	PO113724.D	15 Sep 2025 10:48		YP/AJ	Ok,M
8	AR1221ICC500	AR1221ICC500	PO113725.D	15 Sep 2025 11:06		YP/AJ	Ok
9	AR1232ICC500	AR1232ICC500	PO113726.D	15 Sep 2025 11:25		YP/AJ	Ok
10	AR1242ICC1000	AR1242ICC1000	PO113727.D	15 Sep 2025 11:43		YP/AJ	Ok
11	AR1242ICC750	AR1242ICC750	PO113728.D	15 Sep 2025 12:02		YP/AJ	Ok
12	AR1242ICC500	AR1242ICC500	PO113729.D	15 Sep 2025 12:20		YP/AJ	Ok
13	AR1242ICC250	AR1242ICC250	PO113730.D	15 Sep 2025 12:38		YP/AJ	Ok
14	AR1242ICC050	AR1242ICC050	PO113731.D	15 Sep 2025 13:34		YP/AJ	Ok,M
15	AR1248ICC1000	AR1248ICC1000	PO113732.D	15 Sep 2025 13:54		YP/AJ	Ok
16	AR1248ICC750	AR1248ICC750	PO113733.D	15 Sep 2025 14:13		YP/AJ	Ok
17	AR1248ICC500	AR1248ICC500	PO113734.D	15 Sep 2025 14:31		YP/AJ	Ok
18	AR1248ICC250	AR1248ICC250	PO113735.D	15 Sep 2025 14:49		YP/AJ	Ok,M

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO091525

Review By	yogesh	Review On	9/15/2025 12:11:18 PM
Supervise By	mohammad	Supervise On	9/17/2025 2:07:54 AM
SubDirectory	PO091525	HP Acquire Method	HP Processing Method PO091525
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,PP24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854 PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862		

19	AR1248ICC050	AR1248ICC050	PO113736.D	15 Sep 2025 15:26		YP/AJ	Ok
20	AR1254ICC1000	AR1254ICC1000	PO113737.D	15 Sep 2025 15:45		YP/AJ	Ok
21	AR1254ICC750	AR1254ICC750	PO113738.D	15 Sep 2025 16:02		YP/AJ	Ok
22	AR1254ICC500	AR1254ICC500	PO113739.D	15 Sep 2025 16:20		YP/AJ	Ok
23	AR1254ICC250	AR1254ICC250	PO113740.D	15 Sep 2025 16:38		YP/AJ	Ok
24	AR1254ICC050	AR1254ICC050	PO113741.D	15 Sep 2025 17:14		YP/AJ	Ok,M
25	AR1262ICC500	AR1262ICC500	PO113742.D	15 Sep 2025 17:33		YP/AJ	Ok
26	AR1268ICC1000	AR1268ICC1000	PO113743.D	15 Sep 2025 17:51		YP/AJ	Ok
27	AR1268ICC750	AR1268ICC750	PO113744.D	15 Sep 2025 18:10		YP/AJ	Ok
28	AR1268ICC500	AR1268ICC500	PO113745.D	15 Sep 2025 18:27		YP/AJ	Ok
29	AR1268ICC250	AR1268ICC250	PO113746.D	15 Sep 2025 18:45		YP/AJ	Ok
30	AR1268ICC050	AR1268ICC050	PO113747.D	15 Sep 2025 19:21		YP/AJ	Ok,M
31	PO091525ICV500	ICVPO091525	PO113748.D	15 Sep 2025 19:40		YP/AJ	Ok,M
32	AR1242ICV500	ICVPO091525AR1242	PO113749.D	15 Sep 2025 20:16		YP/AJ	Ok
33	AR1248ICV500	ICVPO091525AR1248	PO113750.D	15 Sep 2025 21:11		YP/AJ	Ok
34	AR1254ICV500	ICVPO091525AR1254	PO113751.D	15 Sep 2025 22:05		YP/AJ	Ok
35	AR1268ICV500	ICVPO091525AR1268	PO113752.D	15 Sep 2025 23:00		YP/AJ	Ok
36	DDT ANALOG	DDT ANALOG	PO113753.D	15 Sep 2025 23:37		YP/AJ	Ok,M

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO100625

Review By	yogesh	Review On	10/6/2025 12:37:59 PM
Supervise By	mohammad	Supervise On	10/8/2025 3:34:35 AM
SubDirectory	PO100625	HP Acquire Method	HP Processing Method PO091925

STD. NAME	STD REF.#
Tune/Reschk	
Initial Calibration Stds	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,PP24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854
CCC	PP24824,PP24828,PP24832,PP24836,PP24840,PP24844,PP24852
Internal Standard/PEM	
ICV/I.BLK	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO114248.D	06 Oct 2025 09:10		YP/AJ	Ok
2	AR1660CCC500	AR1660CCC500	PO114249.D	06 Oct 2025 09:49		YP/AJ	Ok,M
3	AR1242CCC500	AR1242CCC500	PO114250.D	06 Oct 2025 10:07	CCC FAIL 1st column	YP/AJ	Not Ok
4	AR1248CCC500	AR1248CCC500	PO114251.D	06 Oct 2025 10:25		YP/AJ	Ok,M
5	AR1254CCC500	AR1254CCC500	PO114252.D	06 Oct 2025 10:44		YP/AJ	Ok
6	I.BLK	I.BLK	PO114253.D	06 Oct 2025 11:02		YP/AJ	Ok
7	PB169987BL	PB169987BL	PO114254.D	06 Oct 2025 12:10		YP/AJ	Ok
8	PB169987BS	PB169987BS	PO114255.D	06 Oct 2025 12:28		YP/AJ	Ok,M
9	Q3249-11	S-9(4-4.5)	PO114256.D	06 Oct 2025 12:46		YP/AJ	Ok
10	Q3277-01	WC1	PO114257.D	06 Oct 2025 13:05		YP/AJ	Ok
11	Q3288-01	TR-01-100325	PO114258.D	06 Oct 2025 13:22		YP/AJ	Ok
12	Q3288-01MS	TR-01-100325MS	PO114259.D	06 Oct 2025 13:41		YP/AJ	Ok,M
13	Q3288-01MSD	TR-01-100325MSD	PO114260.D	06 Oct 2025 13:59		YP/AJ	Ok,M
14	Q3289-01	VNJ-240	PO114261.D	06 Oct 2025 14:17		YP/AJ	Ok
15	Q3289-03	VNJ-261	PO114262.D	06 Oct 2025 14:36		YP/AJ	Ok,M
16	Q3289-05	72-11966	PO114263.D	06 Oct 2025 14:54		YP/AJ	Ok
17	AR1660CCC500	AR1660CCC500	PO114264.D	06 Oct 2025 15:55		YP/AJ	Ok,M
18	AR1242CCC500	AR1242CCC500	PO114265.D	06 Oct 2025 16:14		YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO100625

Review By	yogesh	Review On	10/6/2025 12:37:59 PM
Supervise By	mohammad	Supervise On	10/8/2025 3:34:35 AM
SubDirectory	PO100625	HP Acquire Method	HP Processing Method PO091925
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,P P24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP 24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854		
CCC	PP24824,PP24828,PP24832,PP24836,PP24840,PP24844,PP24852		
Internal Standard/PEM			
ICV/I.BLK	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

19	AR1248CCC500	AR1248CCC500	PO114266.D	06 Oct 2025 16:32		YP/AJ	Ok,M
20	AR1254CCC500	AR1254CCC500	PO114267.D	06 Oct 2025 16:51		YP/AJ	Ok
21	I.BLK	I.BLK	PO114268.D	06 Oct 2025 17:08		YP/AJ	Ok

M : Manual Integration



PERCENT SOLID

Supervisor: Iwona
Analyst: jignesh
Date: 10/3/2025

OVENTEMP IN Celsius(°C): 107
Time IN: 17:30
In Date: 10/02/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 104
Time OUT: 08:40
Out Date: 10/03/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % solids-oven

QC:LB137394

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
Q2409-05	COP-SOIL-PILE	12	1.18	10.58	11.76	11.38	96.4	
Q3249-03	S-3 (4-4.5)	1	1.11	10.45	11.56	9.51	80.4	
Q3249-08	S-8 (4.5-5)	2	1.19	10.75	11.94	10.38	85.5	
Q3249-16	S-14 (4-4.5)	3	1.13	10.32	11.45	9.34	79.6	
Q3249-19	S-18 (4.5-5)	4	1.18	10.64	11.82	10.8	90.4	
Q3249-22	S-20 (4-4.5)	5	1.18	10.47	11.65	10.64	90.4	
Q3249-24	S-22 (4.5-5)	6	1.19	10.11	11.3	10.33	90.4	
Q3249-27	S-24 (4.5-5)	7	1.15	11.05	12.2	9.82	78.5	
Q3269-01	EG1-TP1	8	1.18	10.78	11.96	10.97	90.8	
Q3269-02	EG1-TP1-E2	9	1.13	10.63	11.76	10.8	91.0	
Q3269-04	EG1-TP2	10	1.13	10.85	11.98	10.97	90.7	
Q3269-05	EG1-TP2-E2	11	1.11	10.77	11.88	11.13	93.0	
Q3270-01	SG-1-TEST-PIT	16	1.18	10.73	11.91	10.77	89.4	
Q3270-02	SG-1-TEST-PIT	17	1.19	10.32	11.51	10.79	93.0	
Q3271-01	72-11929	18	1.13	9.61	10.74	9.79	90.1	
Q3271-02	72-11929-E2	19	1.19	10.47	11.66	10.57	89.6	
Q3272-01	VNJ-235	20	1.19	10.68	11.87	10.15	83.9	
Q3272-02	VNJ-235-E2	21	1.13	10.47	11.6	10.15	86.2	
Q3272-03	R7	22	1.12	10.85	11.97	7.78	61.4	
Q3272-04	R7-E2	23	1.18	10.67	11.85	8.98	73.1	
Q3272-06	RT5417-CONCRETE	24	1.00	1.00	2.00	2.00	100.0	Concreate sample
Q3276-01	SB2	13	1.14	10.92	12.06	10.6	86.6	
Q3276-02	SB2A	14	1.15	10.38	11.53	10.6	91.0	
Q3277-01	WC1	15	1.18	10.41	11.59	11.34	97.6	

$$\% \text{ Solid} = \frac{(C-A) * 100}{(B-A)}$$

WORKLIST(Hardcopy Internal Chain)

137394

WorkList Name : %1-100225 WorkList ID : 192236 Department : Wet-Chemistry Date : 10-02-2025 09:10:00

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q2409-05	COP-SOIL-PILE	Solid	Percent Solids	Cool 4 deg C	COPP02	D51	06/24/2025	Chemtech -SO
Q3249-03	S-3(4-4.5)	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	09/29/2025	Chemtech -SO
Q3249-08	S-8(4.5-5)	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	09/29/2025	Chemtech -SO
Q3249-16	S-14(4-4.5)	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	09/29/2025	Chemtech -SO
Q3249-19	S-18(4.5-5)	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	09/29/2025	Chemtech -SO
Q3249-22	S-20(4-4.5)	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	09/29/2025	Chemtech -SO
Q3249-24	S-22(4.5-5)	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	09/29/2025	Chemtech -SO
Q3249-27	S-24(4.5-5)	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	09/29/2025	Chemtech -SO
Q3269-01	EG1-TP1	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	09/29/2025	Chemtech -SO
Q3269-02	EG1-TP1-E2	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/02/2025	Chemtech -SO
Q3269-04	EG1-TP2	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/02/2025	Chemtech -SO
Q3269-05	EG1-TP2-E2	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/02/2025	Chemtech -SO
Q3270-01	SG-1-TEST-PIT	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/02/2025	Chemtech -SO
Q3270-02	SG-1-TEST-PIT	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/02/2025	Chemtech -SO
Q3271-01	72-11929	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/02/2025	Chemtech -SO
Q3271-02	72-11929-E2	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/02/2025	Chemtech -SO
Q3272-01	VNJ-235	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/02/2025	Chemtech -SO
Q3272-02	VNJ-235-E2	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/02/2025	Chemtech -SO
Q3272-03	R7	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/02/2025	Chemtech -SO
Q3272-04	R7-E2	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/02/2025	Chemtech -SO
Q3272-06	RT5417-CONCRETE	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/02/2025	Chemtech -SO

Date/Time 10/02/25 16:00
 Raw Sample Received by: SO WCI
 Raw Sample Relinquished by: CP S
 Date/Time 10/02/25 17:40
 Raw Sample Received by: CP S
 Raw Sample Relinquished by: SO WCI

WORKLIST(Hardcopy Internal Chain)

8137394

WorkList Name : %1-100225

WorkList ID : 192236

Department : Wet-Chemistry

Date : 10-02-2025 09:10:00

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q3276-01	SB2	Solid	Percent Solids	Cool 4 deg C	GENV01	D31	10/01/2025	Chemtech -SO
Q3276-02	SB2A	Solid	Percent Solids	Cool 4 deg C	GENV01	D31	10/01/2025	Chemtech -SO
Q3277-01	WC1	Solid	Percent Solids	Cool 4 deg C	GENV01	D31	09/30/2025	Chemtech -SO

Date/Time 10/02/25 16:00
 Raw Sample Received by: SP
 Raw Sample Relinquished by: CP

Date/Time 10/02/25 17:40
 Raw Sample Received by: CP
 Raw Sample Relinquished by: SP

SOP ID: M3541-ASE Extraction-15

Clean Up SOP #: Acid Cleanup

Extraction Start Date : 10/06/2025

Matrix : Solid

Extraction Start Time : 08:43

Weigh By: EH

Extraction By: RJ

Extraction End Date : 10/06/2025

Balance check: EH

Filter By: RJ

Extraction End Time : 12:00

Balance ID: EX-SC-2

pH Meter ID: N/A

Concentration By: EH

pH Strip Lot#: N/A

Hood ID: 3,7

Supervisor By : ritesh

Extraction Method: ☐ Separatory Funnel

☐ Continuous Liquid/Liquid

☐ Sonication

☐ Waste Dilution

☒ Soxhlet

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	5000 PPB	PP24930
Surrogate	1.0ML	200 PPB	PP24663
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Hexane/Acetone/1:1	N/A	EP2643
Baked Na2SO4	N/A	EP2646
Hexane	N/A	E3974
H2SO4 1:1	N/A	EP2610
Sand	N/A	E3951
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

40ML Vial Lot # 03-40BTS721.Q3287-01 used Limited Volume as Sample is Oil.

KD Bath ID: N/A

Envap ID: NEVAP-02

KD Bath Temperature: N/A


Envap Temperature: 40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
10/06/25	RJ LEL-106)	R. P. (KBL)
12:05	Preparation Group	Analysis Group

Analytical Method: M3541-ASE Extraction-15

Concentration Date: 10/06/2025

Sample ID	Client Sample ID	Test	g/ mL	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB169987BL	ABLK987	PCB	30.01	N/A	ritesh	Evelyn	10			U2-1
PB169987BS	ALCS987	PCB	30.03	N/A	ritesh	Evelyn	10			2
Q3249-11	S-9(4-4.5)	PCB	30.06	N/A	ritesh	Evelyn	10			3
Q3277-01	WC1	PCB	30.09	N/A	ritesh	Evelyn	10	B		4
Q3287-01	TSS-25-0001-0002	PCB	1.02	N/A	ritesh	Evelyn	10	B	Oil	
Q3288-01	TR-01-100325	PCB	30.04	N/A	ritesh	Evelyn	10	E		5
Q3288-01MS	TR-01-100325MS	PCB	30.03	N/A	ritesh	Evelyn	10	E		6
Q3288-01MS D	TR-01-100325MSD	PCB	30.08	N/A	ritesh	Evelyn	10	E		U3-1
Q3289-01	VNJ-240	PCB	30.05	N/A	ritesh	Evelyn	10	E		2
Q3289-03	VNJ-261	PCB	30.07	N/A	ritesh	Evelyn	10	E		3
Q3289-05	72-11966	PCB	30.03	N/A	ritesh	Evelyn	10	E		4
Q3290-01	CL-02-100325	PCB	30.06	N/A	ritesh	Evelyn	10	D		5

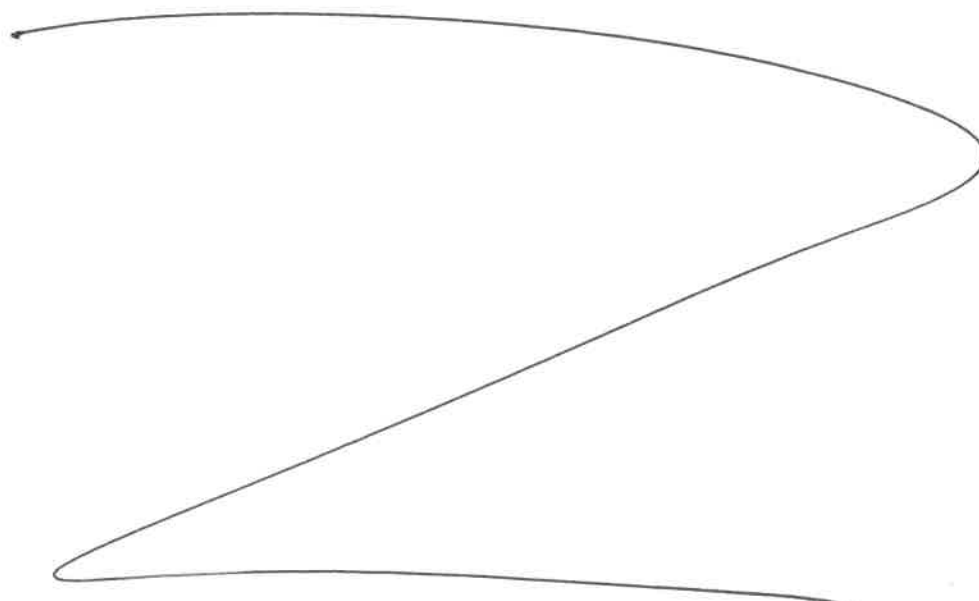

RJ
10/06

16467
8:43

WORKLIST(Hardcopy Internal Chain)

WorkList Name : Q3287

WorkList ID : 192288

Department : Extraction

Date : 10-06-2025 08:38:01

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q3249-11	S-9(4.4.5)	Solid	PCB	Cool 4 deg C	PSEG03	D31	09/29/2025	8082A
Q3277-01	WC1	Solid	PCB	Cool 4 deg C	GENV01	D31	09/30/2025	8082A
Q3287-01	TSS-25-0001-0002	Solid	PCB	Cool 4 deg C	PSEG03	D31	10/03/2025	8082A
Q3288-01	TR-01-100325	Solid	PCB	Cool 4 deg C	PSEG05	D31	10/03/2025	8082A
Q3289-01	VNJ-240	Solid	PCB	Cool 4 deg C	PSEG03	D31	10/03/2025	8082A
Q3289-03	VNJ-261	Solid	PCB	Cool 4 deg C	PSEG03	D31	10/03/2025	8082A
Q3289-05	72-11966	Solid	PCB	Cool 4 deg C	PSEG03	D31	10/03/2025	8082A
Q3290-01	CL-02-100325	Solid	PCB	Cool 4 deg C	PSEG05	D31	10/03/2025	8082A

Date/Time 10/06/25 8:38
Raw Sample Received by: RS CP
Raw Sample Relinquished by: CP

Date/Time 10/06/25 8:55
Raw Sample Received by: CP
Raw Sample Relinquished by: RS LC

Prep Standard - Chemical Standard Summary

Order ID : Q3277

Test : PCB

Prepbatch ID : PB169987,

Sequence ID/Qc Batch ID: PO100625,

Standard ID :

EP2610,EP2643,EP2646,PP24329,PP24330,PP24381,PP24663,PP24805,PP24806,PP24807,PP24808,PP24809,PP24810,PP24811,PP24812,PP24814,PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,PP24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862,PP24930,

Chemical ID :

E3804,E3875,E3944,E3951,E3962,E3963,E3971,E3972,E3974,M6157,P11522,P11592,P12700,P12703,P12952,P12953,P12957,P13356,P13373,P13375,P13590,P13592,P13695,P13697,P13706,P13786,P13789,P13833,P13879,P13881,P13885,W3112,W3177,W3234,



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
314	1.1 H2SO4 SOLN	EP2610	05/07/2025	11/07/2025	RUPESHKUMAR SHAH	Extraction_SCALE_2 (EX-SC-2)	None	Riteshkumar Patel 05/07/2025
<u>FROM</u>	1000.00000ml of M6157 + 1000.00000ml of W3112 = Final Quantity: 2000.000 ml							

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
230	1:1ACETONE/HEXANE	EP2643	09/16/2025	03/16/2026	Evelyn Huang	None	None	Riteshkumar Patel
09/16/2025								

<u>FROM</u>	4000.00000ml of E3971 + 4000.00000ml of E3972 = Final Quantity: 8000.000 ml
--------------------	---



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	EP2646	09/26/2025	01/28/2026	Evelyn Huang	Extraction_SC ALE_2 (EX-SC-2)	None	Riteshkumar Patel 09/26/2025
<u>FROM</u> 4000.00000gram of E3875 = Final Quantity: 4000.000 gram								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
84	Pest/PCB Surrogate Stock 20 PPM	PP24329	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025
<u>FROM</u> 1.00000ml of P13356 + 9.00000ml of W3177 = Final Quantity: 10.000 ml								

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
202	AR1660 1000/100 ppb working solution 1st source	PP24330	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.10000ml of P13697 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1893	AR1254 1000 PPB Working Sol. 2nd Source	PP24381	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 1.00000ml of P12957 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
465	200 PPB Pest/PCB Surrogate Spike	PP24663	06/24/2025	12/24/2025	Abdul Mirza	None	None	Yogesh Patel
								07/21/2025

FROM 1.00000ml of P13786 + 999.00000ml of E3944 = Final Quantity: 1000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
84	Pest/PCB Surrogate Stock 20 PPM	PP24805	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 1.00000ml of P13789 + 9.00000ml of E3962 = Final Quantity: 10.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
213	AR1221 1000 PPB WORKING SOLUTION	PP24806	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.10000ml of P13375 + 99.40000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
214	AR1232 1000 PPB WORKING SOLUTION	PP24807	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.10000ml of P13879 + 99.40000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
215	AR1242 1000 PPB WORKING STD	PP24808	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.10000ml of P13706 + 99.40000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
216	AR1248 1000 PPB WORKING STD	PP24809	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.10000ml of P13695 + 99.40000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
217	AR1254 1000 PPB WORKING STD	PP24810	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.10000ml of P11592 + 99.40000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1529	AR1262 1000 PPB Working Solution	PP24811	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.10000ml of P13881 + 99.40000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1532	AR1268 1000 PPB Working Solution	PP24812	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.10000ml of P13885 + 99.40000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
404	AR1660 100 PPM Stock Solution 2nd Source	PP24814	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 1.00000ml of P12952 + 9.00000ml of E3804 = Final Quantity: 10.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
405	AR1660 1000/100 PPB ICV STD	PP24815	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 98.50000ml of E3962 + 0.50000ml of PP24805 + 1.00000ml of PP24814 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3789	AR1221 1000 PPB WORKING SOL.2ND SOURCE(AGILENT)	PP24816	08/18/2025	02/15/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 1.00000ml of P13373 + 98.50000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1887	AR1232 1000 PPB Working Sol. 2nd Source	PP24817	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 1.00000ml of P12700 + 98.50000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1889	AR1242 1000 PPB Working Sol. 2nd Source	PP24818	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 1.00000ml of P13590 + 98.50000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1890	AR1248 1000 PPB Working Sol. 2nd Source	PP24819	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 1.00000ml of P13592 + 98.50000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2193	AR1254 100 PPM STOCK SOLUTION	PP24820	08/18/2025	02/15/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 1.00000ml of P13833 + 9.00000ml of E3963 = Final Quantity: 10.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3757	AR1262 1000 PPB Working Solution second source	PP24821	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 1.00000ml of P12703 + 98.50000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3817	AR1268 1000 ppb Working Soln. 2nd source	PP24822	08/18/2025	02/15/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 1.00000ml of P11522 + 98.50000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
203	AR1660 750 PPB STD	PP24823	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.25000ml of W3234 + 0.75000ml of PP24330 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
204	AR1660 500 PPB STD	PP24824	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24330 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
205	AR1660 250 PPB STD	PP24825	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.75000ml of W3234 + 0.25000ml of PP24330 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
206	AR1660 50 PPB STD	PP24826	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.90000ml of W3234 + 0.10000ml of PP24824 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1079	AR1221 750 PPB STD	PP24827	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.25000ml of W3234 + 0.75000ml of PP24806 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
222	AR1221 500 PPB STD	PP24828	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24806 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1080	AR1221 250 PPB STD	PP24829	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.75000ml of W3234 + 0.25000ml of PP24806 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1081	AR1221 50 PPB STD	PP24830	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.90000ml of W3234 + 0.10000ml of PP24828 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1063	AR1232 750 PPB STD	PP24831	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.25000ml of W3234 + 0.75000ml of PP24807 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
223	AR1232 500 PPB STD	PP24832	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24807 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1064	AR1232 250 PPB STD	PP24833	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.75000ml of W3234 + 0.25000ml of PP24807 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1065	AR1232 50 PPB STD	PP24834	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.90000ml of W3234 + 0.10000ml of PP24832 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1067	AR1242 750 PPB STD	PP24835	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.25000ml of W3234 + 0.75000ml of PP24808 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
224	AR1242 500 PPB STD	PP24836	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24808 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1068	AR1242 250 PPB STD	PP24837	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.75000ml of W3234 + 0.25000ml of PP24808 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1069	AR1242 50 PPB STD	PP24838	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.90000ml of W3234 + 0.10000ml of PP24836 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1075	AR1248 750 PPB STD	PP24839	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.25000ml of W3234 + 0.75000ml of PP24809 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
225	AR1248 500 PPB STD	PP24840	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24809 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1076	AR1248 250 PPB STD	PP24841	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.75000ml of W3234 + 0.25000ml of PP24809 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1077	AR1248 50 PPB STD	PP24842	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.90000ml of W3234 + 0.10000ml of PP24840 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1071	AR1254 750 PPB STD	PP24843	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
08/19/2025								

FROM 0.25000ml of W3234 + 0.75000ml of PP24810 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
226	AR1254 500 PPB STD	PP24844	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
08/19/2025								

FROM 0.50000ml of W3234 + 0.50000ml of PP24810 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1072	AR1254 250 PPB STD	PP24845	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.75000ml of W3234 + 0.25000ml of PP24810 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1073	AR1254 50 PPB STD	PP24846	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.90000ml of W3234 + 0.10000ml of PP24844 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3753	AR1262 750 PPB STD	PP24847	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.25000ml of W3234 + 0.75000ml of PP24811 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1530	AR1262 500 PPB STD	PP24848	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24811 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3754	AR1262 250 PPB STD	PP24849	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.75000ml of W3234 + 0.25000ml of PP24811 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3755	AR1262 50 PPB STD	PP24850	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.90000ml of W3234 + 0.10000ml of PP24848 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3820	AR1268 750 PPB STD	PP24851	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.25000ml of W3234 + 0.75000ml of PP24812 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1533	AR1268 500 PPB STD	PP24852	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24812 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3821	AR1268 250 PPB STD	PP24853	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.75000ml of W3234 + 0.25000ml of PP24812 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3822	AR1268 50 PPB STD	PP24854	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.90000ml of W3234 + 0.10000ml of PP24852 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
406	AR1660 500 PPB ICV	PP24855	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24815 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3790	AR1221 500 PPB ICV(AGILENT)	PP24856	08/18/2025	02/15/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24816 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1888	AR1232 500 PPB ICV	PP24857	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24817 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1891	AR1242 500 PPB ICV	PP24858	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24818 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1892	AR1248 500 PPB ICV	PP24859	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24819 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1894	AR1254 500 PPB ICV	PP24860	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24381 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3758	AR1262 500 PPB STD ICV	PP24861	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24821 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3823	AR1268 500 PPB STD ICV	PP24862	08/18/2025	02/15/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24822 = Final Quantity: 1.000 ml



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3857	5000 PPB PCB SPIKE SOLUTION 2ND SOURCE	PP24930	09/18/2025	03/18/2026	Abdul Mirza	None	None	Yogesh Patel 09/19/2025
<u>FROM</u> 0.50000ml of P12953 + 99.50000ml of E3972 = Final Quantity: 100.000 ml								

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	9005-05 / Acetone Ultra (cs/4x4L)	24E0761004	02/18/2026	10/01/2024 / Rajesh	09/25/2024 / Rajesh	E3804

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	417203	01/28/2026	07/28/2025 / RUPESH	01/29/2025 / Rajesh	E3875

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H1462005	05/24/2027	06/20/2025 / RUPESH	05/14/2025 / RUPESH	E3944

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-3382-05 / Sand, Purified (cs/4x2.5kg)	25A2756718	12/31/2028	07/09/2025 / RUPESH	04/28/2020 / RUPESH	E3951

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	25C0362005	04/30/2026	08/05/2025 / RUPESH	07/30/2025 / RUPESH	E3962

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H2762008	02/15/2026	08/15/2025 / RUPESH	08/07/2025 / RUPESH	E3963

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	25C0362005	04/30/2026	09/15/2025 / Evelyn	09/04/2025 / Riteshkumar	E3971

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H1462005	05/24/2027	09/16/2025 / Evelyn	09/04/2025 / Riteshkumar	E3972

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	25C0362006	04/10/2027	09/26/2025 / Riteshkumar	09/26/2025 / Riteshkumar	E3974

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	24i1262013	11/07/2025	05/07/2025 / RUPESH	02/18/2025 / Mohan	M6157

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-382-1 / Aroclor 1268	0006587800	09/18/2025	03/18/2025 / yogesh	02/21/2022 / Ankita	P11522

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32011 / PCB Mix, Aroclor 1254, 1000ug/mL, Hexane, 1mL/ampul	A0175403	02/18/2026	08/18/2025 / yogesh	03/18/2022 / Abdul	P11592

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc	91867 / Aroclor 1232 100 ug/mL	020823	02/18/2026	08/18/2025 / yogesh	08/07/2023 / Ankita	P12700

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc	x9166 / Aroclor 1262 100 ug/mL	060523	02/18/2026	08/18/2025 / yogesh	08/07/2023 / Ankita	P12703

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	20064 / Aroclor 1016/1260	022023	02/18/2026	08/18/2025 / yogesh	12/20/2023 / Yogesh	P12952

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	20064 / Aroclor 1016/1260	022023	03/18/2026	09/18/2025 / Abdul	12/20/2023 / Yogesh	P12953

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ Arochlor 1254	121823	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P12957

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	09/18/2025	03/18/2025 / yogesh	04/22/2024 / Abdul	P13356

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-292-1 / Aroclor 1221	0006783205	09/18/2025	03/18/2025 / yogesh	05/02/2024 / Ankita	P13373

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32007 / PCB Mix, Aroclor 1221, 1000ug/mL, Hexane, 1mL/ampul	A0207511	02/18/2026	08/18/2025 / yogesh	05/03/2024 / Abdul	P13375

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-312-1 / Aroclor 1242	0006665550	02/18/2026	08/18/2025 / yogesh	10/14/2024 / Ankita	P13590

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-342-1 / Aroclor 1248	0006726317	02/18/2026	08/18/2025 / yogesh	10/14/2024 / Ankita	P13592

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32010 / PCB Mix, Aroclor 1248, 1000ug/mL, Hexane, 1mL/ampul	A0214733	02/18/2026	08/18/2025 / yogesh	10/17/2024 / yogesh	P13695

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32039 / PCB Mix, Aroclor 1016/1260, 1000ug/mL, hexane, 1mL/ampul	A0210629	09/18/2025	03/18/2025 / yogesh	10/17/2024 / yogesh	P13697

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32009 / PCB Mix, Aroclor 1242, 1000ug/mL, Hexane, 1mL/ampul	A0210232	02/18/2026	08/18/2025 / yogesh	10/17/2024 / yogesh	P13706

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0214495	12/24/2025	06/24/2025 / Abdul	11/19/2024 / Ankita	P13786

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0214495	02/18/2026	08/18/2025 / yogesh	11/19/2024 / Ankita	P13789

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32011 / PCB Mix, Aroclor 1254, 1000ug/mL, Hexane, 1mL/ampul	a0217391	02/18/2026	08/18/2025 / yogesh	12/09/2024 / Ankita	P13833

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32008 / PCB Mix, Aroclor 1232, 1000ug/mL, Hexane, 1mL/ampul	A0219655	02/18/2026	08/18/2025 / yogesh	01/23/2025 / Ankita	P13879

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32409 / PCB Stock Solution, Aroclor 1262 Std, 1mL, Hexane	A0217041	02/18/2026	08/18/2025 / yogesh	01/23/2025 / Ankita	P13881

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32410 / PCB Stock Solution, Aroclor 1268 Std, 1mL, Hexane	A0217264	02/18/2026	08/18/2025 / yogesh	01/23/2025 / Ankita	P13885

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / Iwona	07/03/2024 / Iwona	W3112

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24G1962003	08/22/2025	02/03/2025 / jignesh	01/31/2025 / jignesh	W3177

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	25C0362005	04/30/2026	07/28/2025 / jignesh	07/25/2025 / jignesh	W3234

Material No.: 9005-05
Batch No.: 24E0761004
Manufactured Date: 2024-05-02
Retest Date: 2029-05-01
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.5 %	99.8 %
Color (APHA)	≤ 10	< 5
Residue after Evaporation	≤ 5 ppm	< 1 ppm
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.5	0.1
Water (H ₂ O)	≤ 0.5 %	0.1 %
Solubility in H ₂ O	Passes Test	Passes Test
Chloride (Cl)	≤ 0.2 ppm	< 0.2 ppm
Phosphate (PO ₄)	≤ 0.05 ppm	< 0.05 ppm
Trace Impurities – Aluminum (Al)	≤ 50.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 5.0 ppb
Trace Impurities – Barium (Ba)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Beryllium (Be)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Bismuth (Bi)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Calcium (Ca)	≤ 25.0 ppb	3.6 ppb
Trace Impurities – Chromium (Cr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Cobalt (Co)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Copper (Cu)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Gallium (Ga)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Germanium (Ge)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Gold (Au)	≤ 20 ppb	< 5 ppb
Trace Impurities – Iron (Fe)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Lead (Pb)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Lithium (Li)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Magnesium (Mg)	≤ 20 ppb	< 1 ppb
Trace Impurities – Manganese (Mn)	≤ 10.0 ppb	< 1.0 ppb

Recd by RP on 9/25/24

E 3804

>>> Continued on page 2 >>>

Acetone
CMOS

 **avantor™**



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
Trace Impurities – Molybdenum (Mo)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Nickel (Ni)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Niobium (Nb)	≤ 50.0 ppb	< 1.0 ppb
Trace Impurities – Potassium (K)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Silicon (Si)	≤ 50 ppb	< 10 ppb
Trace Impurities – Silver (Ag)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Sodium (Na)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Strontium (Sr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Tantalum (Ta)	≤ 50.0 ppb	< 5.0 ppb
Trace Impurities – Thallium (Tl)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Tin (Sn)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Titanium (Ti)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Vanadium (V)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Zinc (Zn)	≤ 20.0 ppb	7.9 ppb
Trace Impurities – Zirconium (Zr)	≤ 10.0 ppb	< 1.0 ppb
Particle Count – 0.5 µm and greater (Rion KS42AF)	≤ 100 par/ml	8 par/ml
Particle Count – 1.0 µm and greater (Rion KS42AF)	≤ 8 par/ml	2 par/ml

>>> Continued on page 3 >>>

Acetone
CMOS

 **avantor™**



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
------	---------------	--------

For Microelectronic Use

Country of Origin: USA
Packaging Site: Paris Mfg Ctr & DC



Michelle Bales
Sr. Manager, Quality Assurance

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03

Batch No.: 25C0362006

Manufactured Date: 2025-01-29

Expiration Date: 2026-04-30

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	6
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	4
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	100.0 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	100 %
Color (APHA)	≤ 10	10
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	$< 0.01 \%$

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E 3974

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC



**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MÉXICO
CP 64070
TEL +52 81 13 52 67 67
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na ₂ SO ₄
SPECIFICATION NUMBER:	6399	RELEASE DATE:	MAY/23/2024
LOT NUMBER :	417203		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na ₂ SO ₄)	Min. 99.0%	99.8 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.2
Insoluble matter	Max. 0.01%	0.001 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO ₄)	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.001 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.001 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.2 %
Retained on US Standard No. 60 sieve	Min. 94%	96.2 %
Through US Standard No. 60 sieve	Max. 5%	3.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

RE-02-01, Ed. 3

E 3875

Acetone
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

Avantor™



Material No.: 9254-03

Batch No.: 24H1462005

Manufactured Date: 2024-05-24

Expiration Date: 2027-05-24

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	99.8 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (μeq/g)	<= 0.3	0.2
Titration Base (μeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	0.2 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	<1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

E3944

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC



Material	BDH9274-2.5KG
Material Description	BDH SAND STDD OTTAWA W+I 2.5KG
Grade	NOT APPLICABLE
Batch	25A2756718
Reassay Date	12/31/2028
CAS Number	14808-60-7
Molecular Formula	SiO ₂
Molecular Mass	60.09
Date of Manufacture	12/05/2024
Storage	Room Temperature

Characteristics	Specifications	Measured Values
Appearance	Beige granules.	Beige granules.
Moisture	<= 0.1 %	0.1 %
Particle Size 30-40 mesh	>= 80 %	99 %
CUSTOMER PART # BDH9274-2.5KG		

Received on 1/12/25.

E3951

Internal ID #: 793

Signature	Additional Information
We certify that this batch conforms to the specifications listed above. This document has been electronically produced and is valid without a signature. Leona Edwardson, Quality Control Sr. Manager - Solon VWR Chemicals, LLC. 28600 Fountain Parkway, Solon OH 44139 USA	Analysis may have been rounded to significant digits in specification limits Product meets analytical specifications of the grades listed.

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 25C0362005
Manufactured Date: 2025-01-29
Expiration Date: 2026-04-30
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	≤ 10	6
ECD-Sensitive Impurities (as EthyleneDibromide) - Single Impurity Peak (ng/mL)	≤ 5	5
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	100.0 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	100 %
Color (APHA)	≤ 10	10
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	$< 0.01 \%$

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

Received on 7/30/25

E3962

Jamie Croak
Director Quality Operations, Bioscience Production

Acetone.
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

Avantor™



Material No.: 9254-03
Batch No.: 24H2762008
Manufactured Date: 2024-04-18
Expiration Date: 2027-04-18
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	100.0 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.0 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (μeq/g)	<= 0.3	0.2
Titration Base (μeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	<0.1 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

Received on 8/6/25

E 3963

J. Croak

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA, 19087, U.S.A. Phone 610.386.1700

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 25C0362005
Manufactured Date: 2025-01-29
Expiration Date: 2026-04-30
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	≤ 10	6
ECD-Sensitive Impurities (as EthyleneDibromide) - Single Impurity Peak (ng/mL)	≤ 5	5
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	100.0 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	100 %
Color (APHA)	≤ 10	10
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	$< 0.01 \%$

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

E3971

Jamie Croak
Director Quality Operations, Bioscience Production

Acetone
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

avantor™



Material No.: 9254-03

Batch No.: 24H1462005

Manufactured Date: 2024-05-24

Expiration Date: 2027-05-24

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	99.8 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (µeq/g)	<= 0.3	0.2
Titration Base (µeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	0.2 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	<1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

E3972

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

Sulfuric Acid
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis
Low Selenium

avantor™



MG157
MS

Material No.: 9673-33

Batch No.: 24I1262013

Manufactured Date: 2024-08-07

Retest Date: 2029-08-06

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
ACS – Assay (H ₂ SO ₄)	95.0 – 98.0 %	96.2 %
Appearance	Passes Test	Passes Test
ACS – Color (APHA)	<= 10	5
ACS – Residue after Ignition	<= 3 ppm	<1 ppm
ACS – Substances Reducing Permanganate(as SO ₂)	<= 2 ppm	<2 ppm
Ammonium (NH ₄)	<= 1 ppm	<1 ppm
Chloride (Cl)	<= 0.1 ppm	<0.1 ppm
Nitrate (NO ₃)	<= 0.2 ppm	0.1 ppm
Phosphate (PO ₄)	<= 0.5 ppm	<0.1 ppm
Trace Impurities – Aluminum (Al)	<= 30.0 ppb	<5.0 ppb
Arsenic & Antimony (as As)	<= 4.0 ppb	<2.0 ppb
Trace Impurities – Boron (B)	<= 10.0 ppb	<5.0 ppb
Trace Impurities – Cadmium (Cd)	<= 2.0 ppb	<1.0 ppb
Trace Impurities – Chromium (Cr)	<= 6.0 ppb	<1.0 ppb
Trace Impurities – Cobalt (Co)	<= 0.5 ppb	<0.3 ppb
Trace Impurities – Copper (Cu)	<= 1.0 ppb	<1.0 ppb
Trace Impurities – Gold (Au)	<= 10.0 ppb	<5.0 ppb
Heavy Metals (as Pb)	<= 500.0 ppb	<100.0 ppb
Trace Impurities – Iron (Fe)	<= 50.0 ppb	<1.0 ppb
Trace Impurities – Lead (Pb)	<= 0.5 ppb	<0.5 ppb
Trace Impurities – Magnesium (Mg)	<= 7.0 ppb	<1.0 ppb
Trace Impurities – Manganese (Mn)	<= 1.0 ppb	<1.0 ppb
Trace Impurities – Mercury (Hg)	<= 0.5 ppb	<0.1 ppb
Trace Impurities – Nickel (Ni)	<= 2.0 ppb	<0.3 ppb
Trace Impurities – Potassium (K)	<= 500.0 ppb	<10.0 ppb
Trace Impurities – Selenium (Se)	<= 50.0 ppb	7.2 ppb
Trace Impurities – Silicon (Si)	<= 100.0 ppb	12.8 ppb
Trace Impurities – Silver (Ag)	<= 1.0 ppb	<1.0 ppb

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

Sulfuric Acid

BAKER INSTRA-ANALYZED® Reagent

For Trace Metal Analysis

Low Selenium

 **avantor**™



Material No.: 9673-33

Batch No.: 2411262013

Test	Specification	Result
Trace Impurities – Sodium (Na)	≤ 500.0 ppb	< 5.0 ppb
Trace Impurities – Strontium (Sr)	≤ 5.0 ppb	< 1.0 ppb
Trace Impurities – Tin (Sn)	≤ 5.0 ppb	1.1 ppb
Trace Impurities – Zinc (Zn)	≤ 5.0 ppb	< 1.0 ppb

For Laboratory, Research, or Manufacturing Use

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC



Jamie Croak

Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC



Certificate of Analysis

P11518
↓
P11522
AJ
02/21/22

Product Name: Aroclor 1268 Standard

Product Number: PP-382-1

Lot Issue Date: 09-Feb-2021

Lot Number: 0006587800

Expiration Date: 31-Mar-2029

Description:

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

Analyte	CAS#	Analyte Lot	Concentration ± Uncertainty
Aroclor 1268	011100-14-4	RM00937	100.0 ± 0.5 µg/mL

Matrix: isooctane (2,2,4-trimethylpentane)

Storage Conditions: Store at Room Temperature (15° to 30°C).

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Hazards:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this RM.


Expiration of Certification:

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:


Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026
Page: 1 of 1

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32011 **Lot No.:** A0175403

Description : Aroclor® 1254 Standard

Aroclor® 1254 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : November 30, 2027 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1254	1,000.7 µg/mL	+/- 5.9437 µg/mL Gravimetric
	CAS # 11097-69-1 (Lot 124-191-B)		+/- 31.7284 µg/mL Unstressed
	Purity ----%		+/- 41.4406 µg/mL Stressed

Solvent: Hexane

CAS # 110-54-3

Purity 99%

P11588
↓
P11592 / (S)

AR
04/30/2022

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

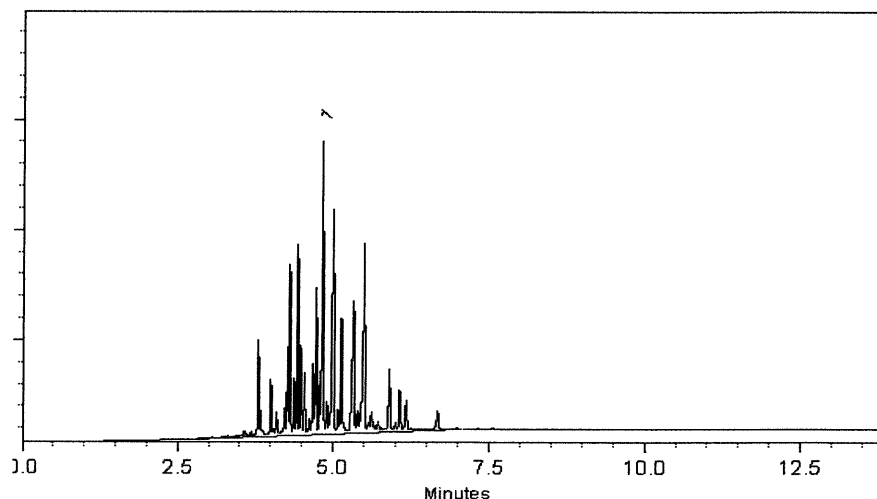

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Cathleen Soltis

Cathleen Soltis - Mix Technician

Date Mixed: 15-Aug-2021

Balance: 1128360905

Alexis Shelow

Alexis Shelow - Operations Tech I

Date Passed: 17-Aug-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11588
↓
P11592 / (5)

AR
04/30/22



CERTIFIED WEIGHT REPORT

Part Number: **91867**
 Lot Number: **020823**
 Description: **WP 037 - Aroclor 1232**
PCB Technical Mixture
 Expiration Date: **020833**
 Recommended Storage: **Ambient (20 °C)**
 Nominal Concentration (µg/mL): **100**
 NIST Test ID#: **6UTB**

Solvent(
Aceton


Weight(s) shown below were combined and diluted to (mL): **100.0**
 5E-05 Balance Uncertainty
 0.057 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (g)
1. Aroclor 1232	17	45-6A	100	100	0.5	0.01000

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measure Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments

GC3-M1 Analysis by Melissa Stonier
 Column ID SPB-608 30 meter X 0.53mm X 5µm film thickness
 Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
 Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
 Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)
 Rate = 8°C/min, Total run time = 35 min
 Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1
 Standard injection = 1.5µL, Range=3

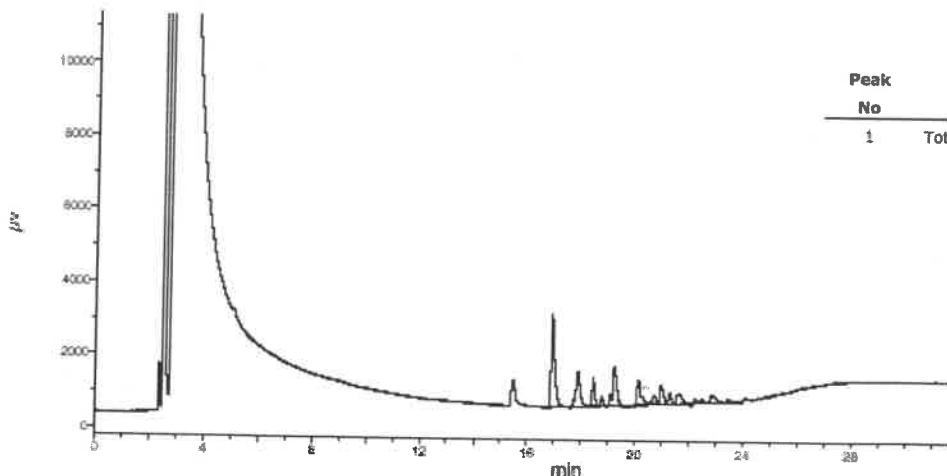




CERTIFIED WEIGHT REPORT

Part Number: X9166
Lot Number: 060523
Description: Aroclor 1262
Appendix IX Compound
Expiration Date: 060533
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 100
NIST Test ID#: 6UTB
5E-05 Balance Uncertainty
Volume(s) shown below were combined and diluted to (mL): 20.0 0.002 Flask Uncertainty

Compound	Part Number	Lot Number	Dil. Factor	Initial Vol. (mL)	Uncertainty Pipette (mL)	Co
1. Aroclor 1262	70444	080322	0.10	2.00	0.017	

Method GC7MSD-7.M: Column:(30m X 0.25mm ID X 0.25µm film thickn min.), Rate = 8°C/min., Injector B= 200°C, Detector B = 290°C.

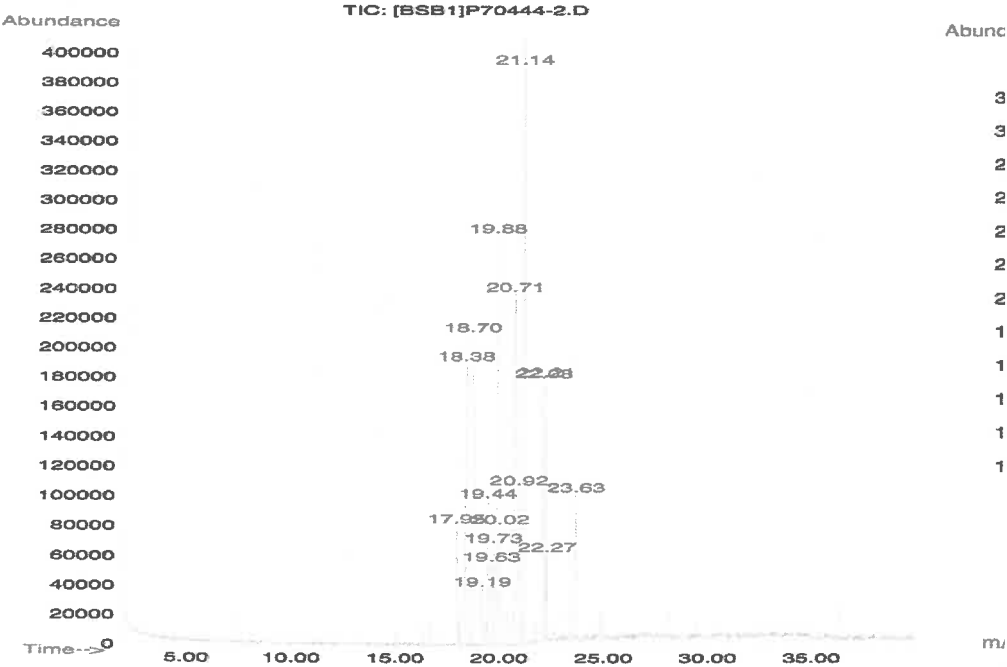

- The certified value is the concentration calculated from gravimetric and volumetric me
- Standards are prepared gravimetrically using balances that are calibrated with weight
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appro
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Certified Reference Material CRM

CERTIFIED WEIGHT REPORT

Part Number:
20064

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE
022023

DATE
022023

Weight(s) shown below were combined and diluted to (mL):
200.0

5E-05 Balance Uncertainty
0.010 Flask Uncertainty

Part Number:
20064

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE
022023

DATE
022023


Weight(s) shown below were combined and diluted to (mL):
200.0

5E-05 Balance Uncertainty
0.010 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. Aroclor 1016	15	020491JC	1000	100	0.2	0.20004	0.20060	1002.8	4.0	12674-11-2	N/A	N/A
2. Aroclor 1260	21	020491JC	1000	100	0.2	0.20004	0.20081	1003.9	4.0	11086-82-5	0.5mg/m3	orl-rat 1315mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stortier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 280°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C, FID Signal = Etdaq Channel 1
Standard Injection = 1.5µL, Range=3

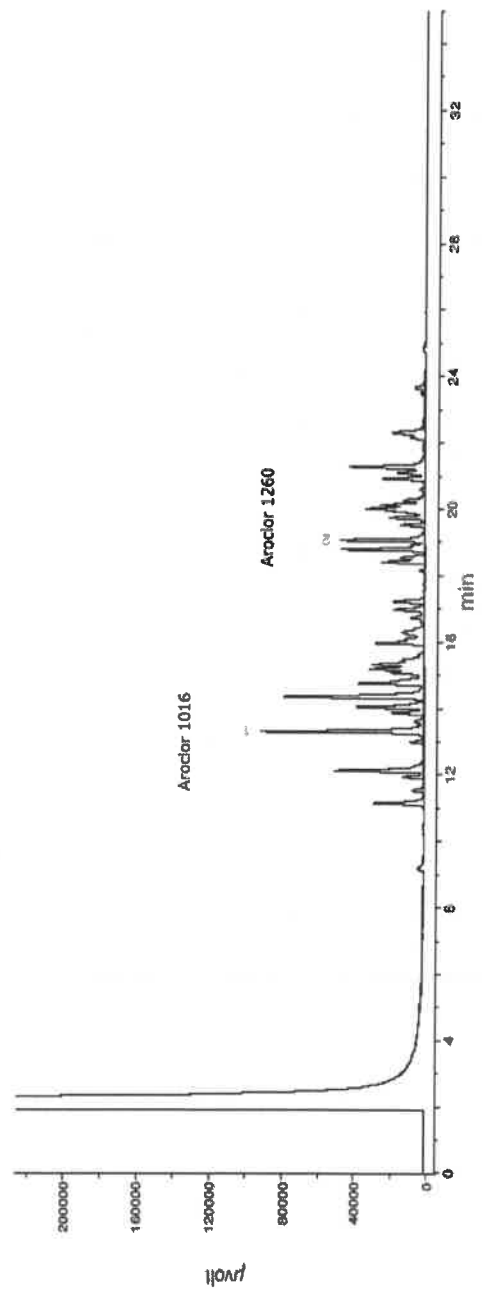



Certified Reference Material CRM

CERTIFIED WEIGHT REPORT

Part Number:
20084

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE
022023

DATE
022023

5E-05 Balance Uncertainty
0.010 Flask Uncertainty

Nominal Conc (µg/mL):
200.0

Weight(s) shown below were combined and diluted to (mL):

Part Number:
20084

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE
022023

DATE
022023

5E-05 Balance Uncertainty
0.010 Flask Uncertainty


Nominal Conc (µg/mL):
200.0

Weight(s) shown below were combined and diluted to (mL):

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. Aroclor 1016	15	020491JC	1000	100	0.2	0.20004	0.20060	1002.8	4.0	12674-11-2	N/A	N/A
2. Aroclor 1260	21	020491JC	1000	100	0.2	0.20004	0.20081	1003.9	4.0	11086-82-5	0.5mg/m3	orl-rat 1315mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stortier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 280°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C, FID Signal = Etdaq Channel 1
Standard Injection = 1.5µL, Range=3

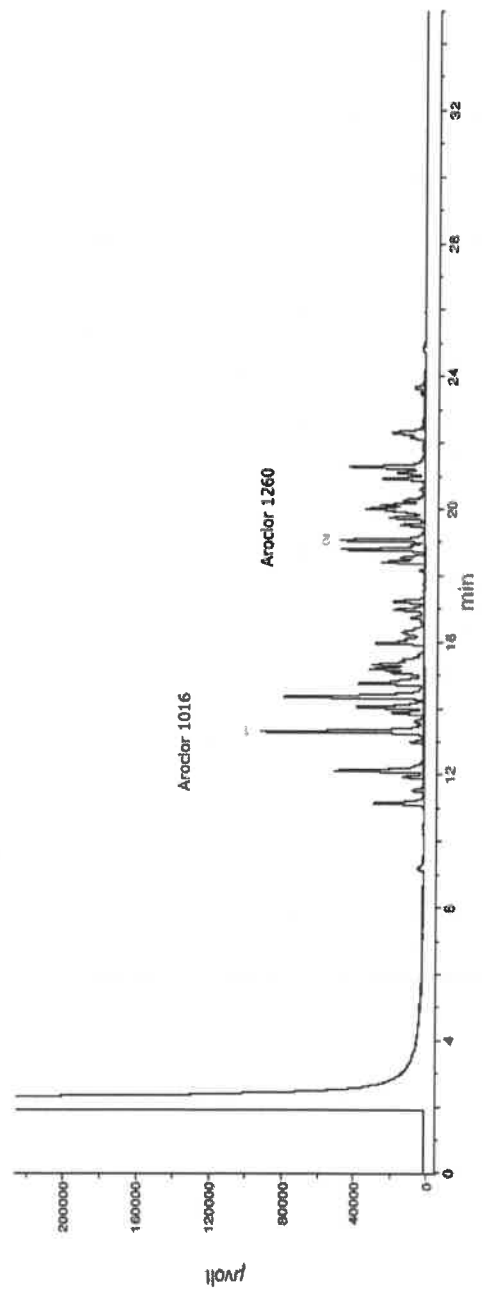



CERTIFIED WEIGHT REPORT

Part Number: 99139
Lot Number: 121823
Description: Aroclor 1254

Expiration Date: 121833
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 100
NIST Test ID#: 6UTB

Volume(s) shown below were combined and diluted to (mL): 20.0
Note: Aroclor 1254 is a mix of isomers.

Solvent(s): Iso-octane
Lot#: 82227

Formulated By: Anthony Mahoney	121823	DATE
Reviewed By: Pedro L. Rentas	121823	DATE


P12956 / Y.P.
12/18/23
P12957

Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Initial Uncertainty	Pipette (mL)	Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information		
											(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA) LD50
1. Aroclor 1254	79100	121823	0.10	2.00	0.017	0.017	1003.3	100.1	11097-69-1	1.8	0.5mg/m3 (skin)		or-rat 1295mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stonier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150 °C (Time 1 = 4 min), Temp 2 = 280 °C (Time 2 = 13.5 min)
Rate = 8 °C/min, Total run time = 35 min
Injector temp. = 200 °C, FID Temp. = 300 °C, FID Signal = EDAQ Channel 1
Standard injection = 1.5µL, Range=3

Peak No.	Name	FID RT (min.)
1	Total Aroclor 1254	18.12

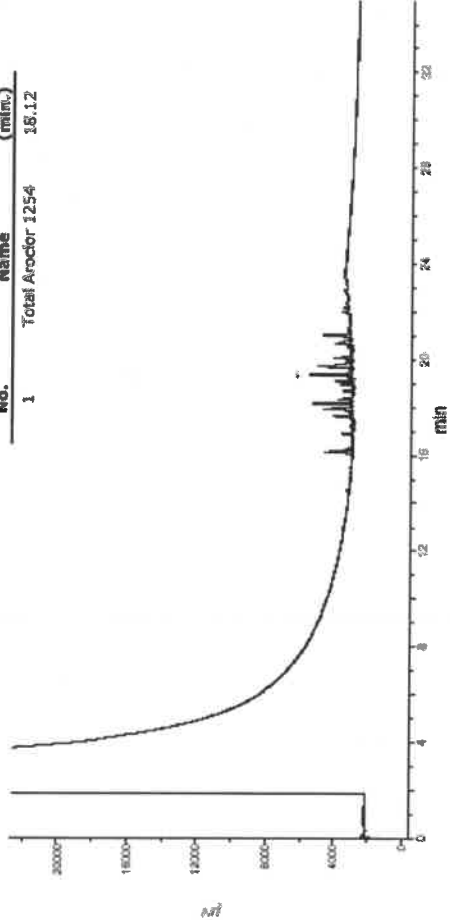



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0206810

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13348
↓
P13357
10
DAUF
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

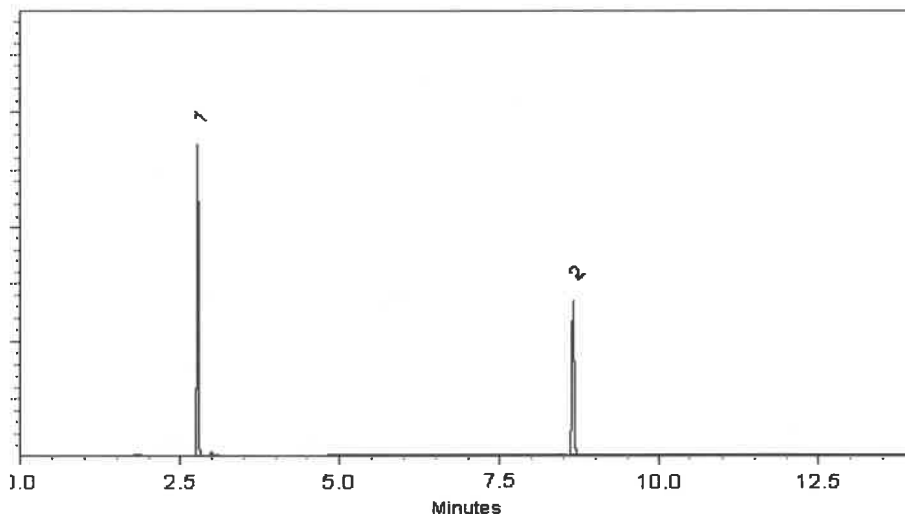


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024

Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
SAUF
04/25/2025



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32007 **Lot No.:** A0207511

Description : Aroclor® 1221 Standard

Aroclor® 1221 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : May 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1221	11104-28-2	13192500	----%	1,002.7 µg/mL	+/- 55.6424

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 13374
↓
P 13375
/

[Signature]
05/6/2024

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

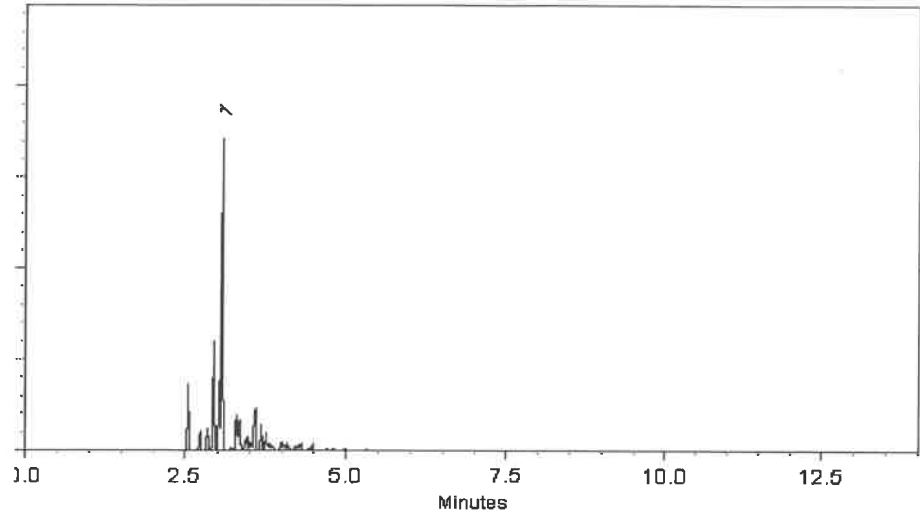

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 06-Feb-2024

Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC


Date Passed: 08-Feb-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13374 } ②
↓
P 13375 }


05/6/2024

ISO 17034



Agilent

Trusted Answers

Reference Material Certificate

Product Name: Aroclor 1242 Standard

Lot Number: 0006665550

Product Number: PP-312-1

Lot Issue Date: 08-Feb-2022

Storage Conditions: Store at Room Temperature (15° to 30°C).

Expiration Date: 31-Jan-2027

Component Name	CERTIFIED VALUES		CAS#	Analyte Lot
	Concentration	Expanded Uncertainty		
Aroclor 1242	100.4	± 0.5 µg/mL	053469-21-9	NT01020

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P13589
↓
P13590AJ
10/14/24

ISO 17034



Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015
Quality Management System. Cert# 95T215321

Page: 2 of 2

www.agilent.com/quality/

CSD-QA-015.1



ISO 17025
Cert No. AT-

Reference Material Certificate
Product Information Sheet**Product Name:** Aroclor 1248 Standard**Lot Number:** 0006726317**Product Number:** PP-342-1**Lot Issue Date:** 27-Jan-2023**Storage Conditions:** Store at Room Temperature (15° to 30°C).**Expiration Date:** 28-Feb-2031

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
Aroclor 1248	100.3 ±	0.5 µg/mL	012672-29-6	NT01582

Matrix: isooctane (2,2,4-trimethylpentane)**Description:**

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material (RM) standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above. Purity values are taken from approved vendor raw material certificates.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference (RM) standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference (RM) standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard (RM) is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P13591
↓
P13592AJ
10/14/2024



Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO
9001:2015 Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/

CSD-QA-015.1

ISO 17025



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32010 **Lot No.:** A0214733

Description : Aroclor® 1248 Standard

Aroclor® 1248 Standard 1,000µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : November 30, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

P13695 } Y.P.
P13696 } 10/17/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1248	12672-29-6	15242800	----%	1,005.0 µg/mL	+/- 55.7700

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2µl

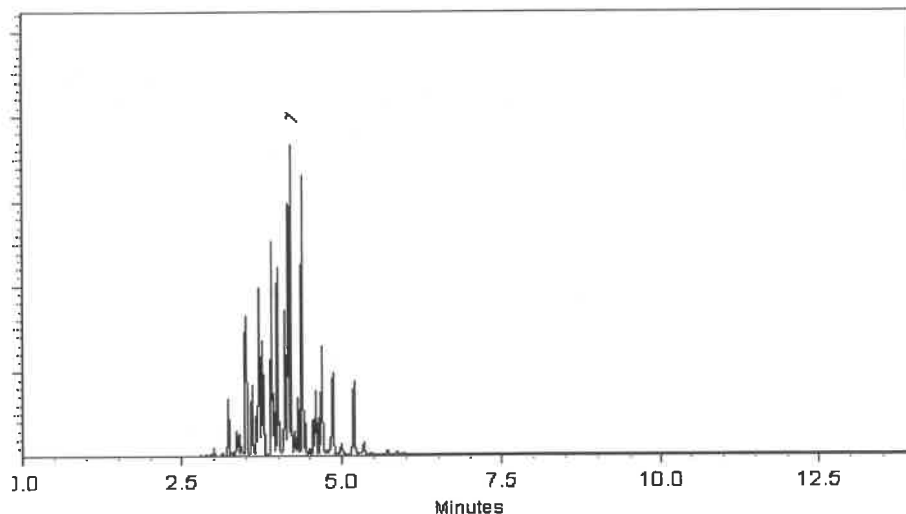

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Rebecca Gingerich - Operations Tech II

Date Mixed: 02-Aug-2024

Balance Serial # C322230531

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 13-Aug-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32039 **Lot No.:** A0210629

Description : Aroclor® 1016/1260 Mix
Aroclor® 1016/1260 Mix 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : July 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

P13697
↓
P13701 } Y.P.
10/19/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1016	12674-11-2	07	----%	1,005.3 µg/mL	+/- 55.7809
2	Aroclor 1260	11096-82-5	1320657	----%	1,000.0 µg/mL	+/- 55.4850

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

0.2µl

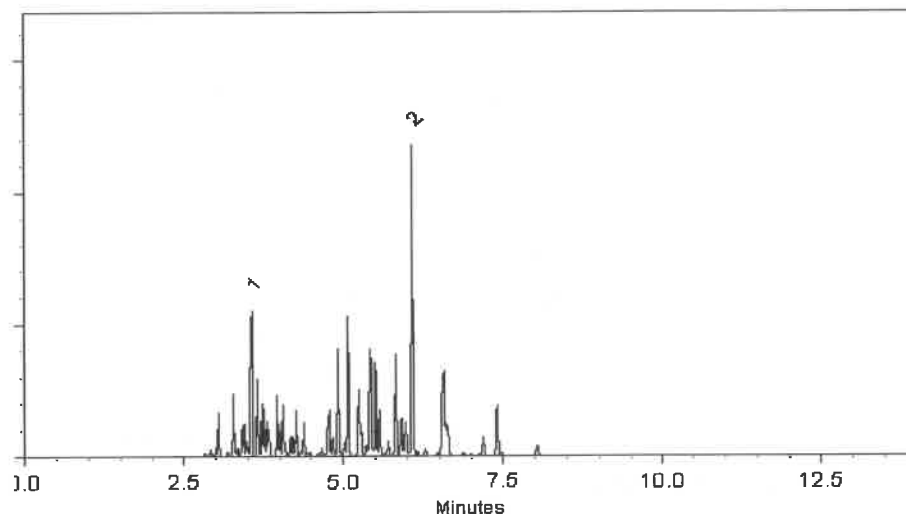


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Apr-2024

Balance Serial # B442140311


Dillan Murphy - Operations Technician I

Date Passed: 24-Apr-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32009 **Lot No.:** A0210232
Description : Aroclor® 1242 Standard
Aroclor® 1242 Standard 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : July 31, 2030 **Storage:** 25°C nominal
Handling: This product contains PCBs. **Ship:** Ambient

P13706 } y.p.
P13707 } 10/17/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1242	53469-21-9	01141	----%	1,000.7 µg/mL	+/- 55.5295

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2µl

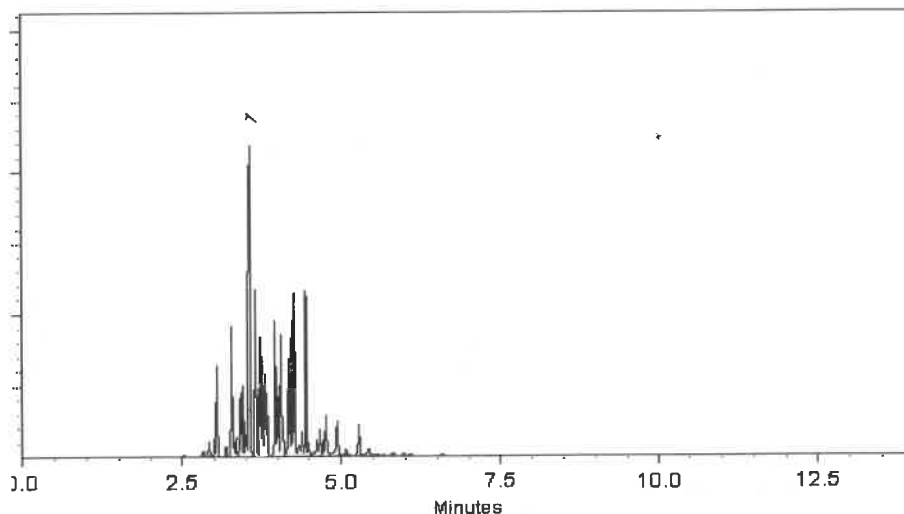

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Amanda Miller - Operations Tech III - ARM QC

Date Mixed: 11-Apr-2024

Balance Serial # B442140311


Christie Mills - Operations Lead Tech - ARM QC

Date Passed: 17-Apr-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0214495

Description : Pesticide Surrogate Mix

Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : October 31, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P19785
AJ
11/19/24
P19789

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.2 µg/mL	+/- 11.1087
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30679	99%	201.4 µg/mL	+/- 11.1753

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:
30m x 25mm x 2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD

Split Vent:
10 ml/min.

Inj. Vol
1µl

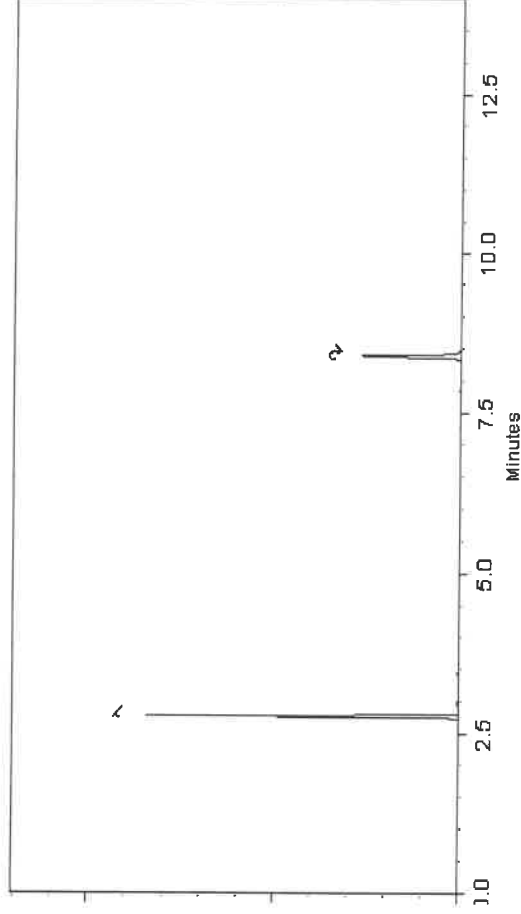

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

A. O. P.
Aaron Enyart - Operations Tech I

Date Mixed: 29-Jul-2024 **Balance Serial #** B345965662

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 01-Aug-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0214495

Description : Pesticide Surrogate Mix

Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : October 31, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P19785
AJ
11/19/24
P19789

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.2 µg/mL	+/- 11.1087
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30679	99%	201.4 µg/mL	+/- 11.1753

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:
30m x 25mm x 2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD

Split Vent:
10 ml/min.

Inj. Vol
1µl

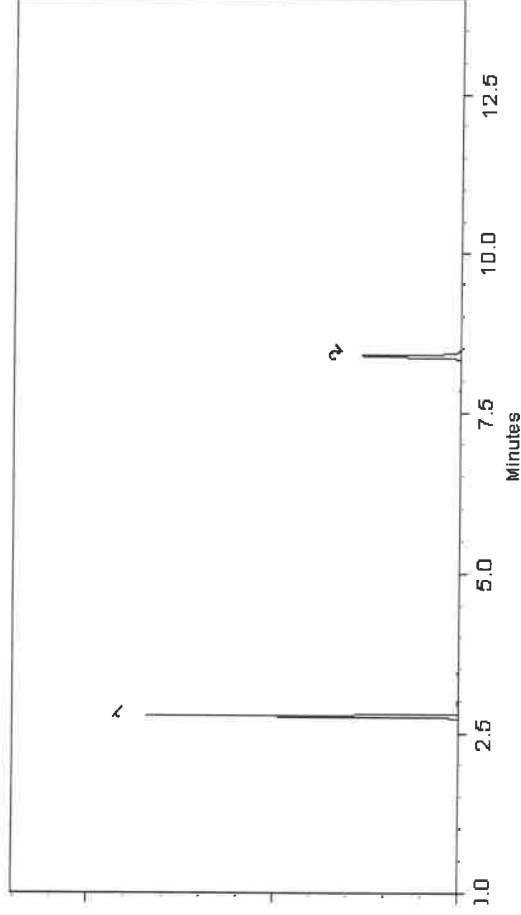

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

A. O. P.
Aaron Enyart - Operations Tech I

Date Mixed: 29-Jul-2024 **Balance Serial #** B345965662

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 01-Aug-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32011 **Lot No.:** A0217391

Description : Aroclor® 1254 Standard

Aroclor® 1254 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : January 31, 2031 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1254	11097-69-1	124-191-B	----%	1,004.7 µg/mL	+/- 55.7515

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P13830
↓
P13832
↓
P13834
AJ
12/09/24

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

300 ml/min.

Inj. Vol

1µl

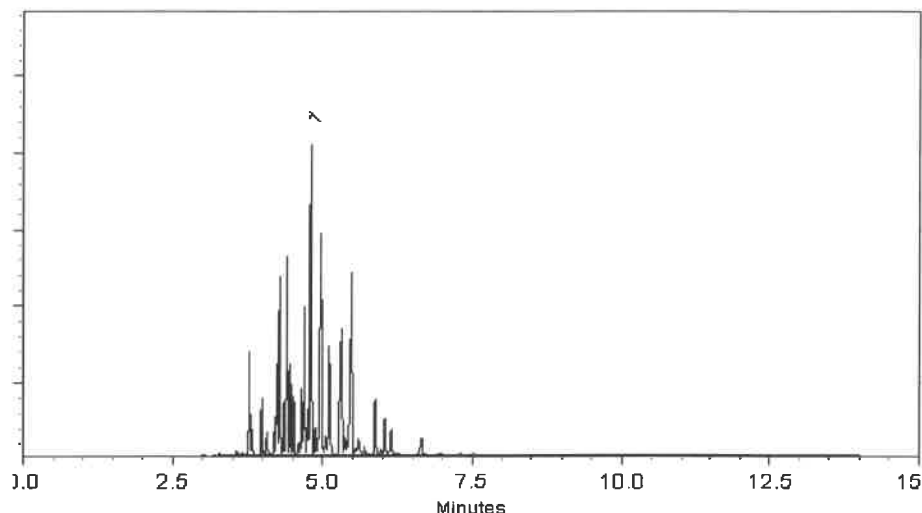

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Michael Maye
Michael Maye - Operations Tech I

Date Mixed: 02-Oct-2024

Balance Serial # C322230531

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 07-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32008

Lot No.: A0219655

Description : Aroclor® 1232 Standard

Aroclor® 1232 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : March 31, 2031

Storage: 25°C nominal

Handling:

This product contains PCBs.

Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1232	11141-16-5	15665-01	---%	1,007.0 µg/mL	+/- 55.8810

Solvent: Hexane

CAS # 110-54-3

Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

P13878



AJ
01/28/25

P13880

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

1µl

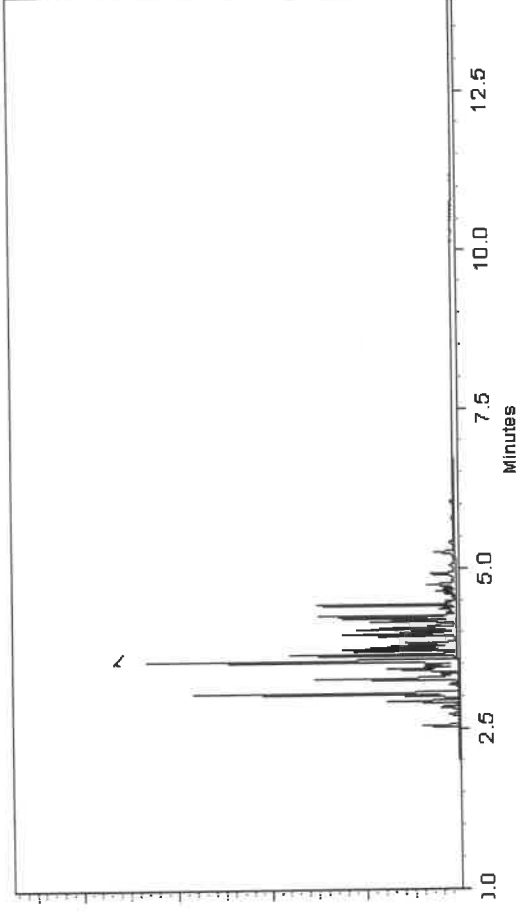

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Michael Maye
Michael Maye - Operations Tech I

Date Mixed: 02-Dec-2024

Balance Serial #

C322230531

Brittany Federhik
Brittany Federhiko - Operations Tech I

Date Passed: 05-Dec-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com



Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32409 **Lot No.:** A0217041

Description : Aroclor® 1262 Standard

Aroclor® 1262 Standard 1,000 µg/mL, 1mL/ampul, Hexane

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : December 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1262	37324-23-5	10849100	----%	1,000.0 µg/mL	+/- 55.4925

Solvent: Hexane
CAS # 110-54-3
Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

P13881
AJ
01128125

Quality Confirmation Test

Column:
30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD

Split Vent:
300 ml/min.

Inj. Vol
0.2µl

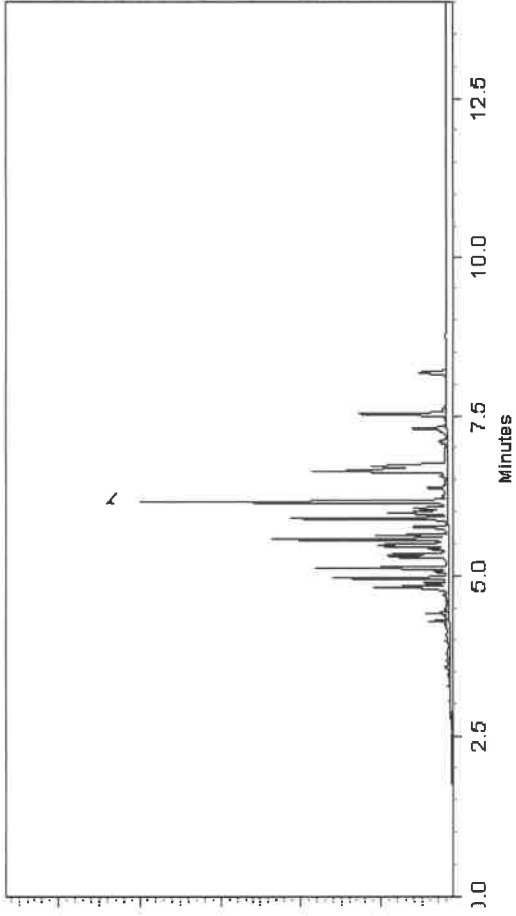

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Rebecca Gingerich - Operations Tech II


Jennifer Pollino - Operations Tech III - ARM QC

Date Mixed: 25-Sep-2024 Balance Serial # C322230531

Date Passed: 30-Sep-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32410

Lot No.: A0217264

Description : Aroclor® 1268 Standard

Aroclor® 1268 Standard 1,000 µg/mL, 1mL/ampul, Hexane

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : January 31, 2031

Storage: 25°C nominal

Handling:

This product contains PCBs.

Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1268	11100-14-4	12353400	----%	1,009.8 µg/mL	+/- 56.0364

Solvent: Hexane

CAS # 110-54-3

Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

P13884

+

AJ
01/28/25

P13886

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

Split ratio 500:1

Inj. Vol

0.2µl

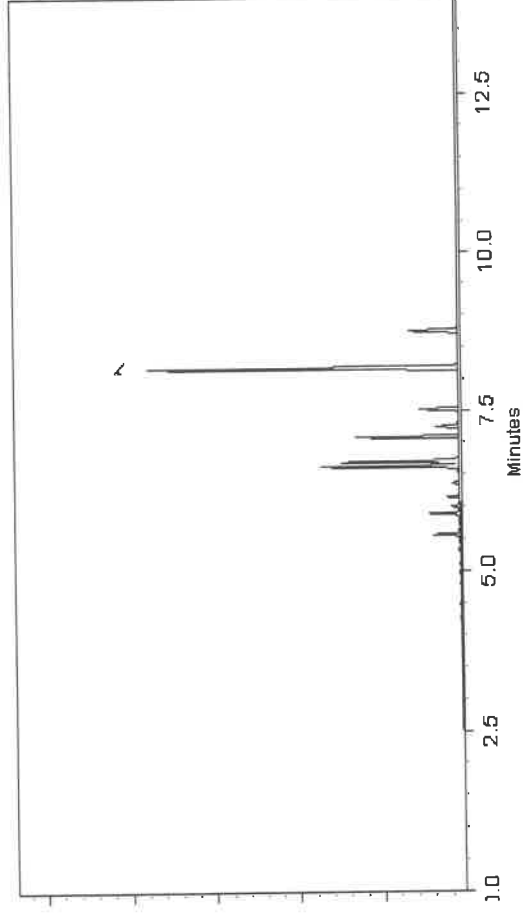

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Stacey Wanner - Operations Technician I

Balance Serial # 1128360905

Date Mixed: 01-Oct-2024

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 02-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 24G1962003
Manufactured Date: 2024-05-23
Expiration Date: 2025-08-22
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Croak
Director Quality Operations, Bioscience Production

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis

avantor™



Material No.: 9262-03

Batch No.: 25C0362005

Manufactured Date: 2025-01-29

Expiration Date: 2026-04-30

Revision No.: 0

W3234 JB
OP4421. 07/28/2025

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	<= 10	6
ECD-Sensitive Impurities (as EthyleneDibromide) - Single Impurity Peak (ng/mL)	<= 5	5
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	>= 99.5 %	100.0 %
Assay (as n-Hexane) (by GC, corrected for water)	>= 95 %	100 %
Color (APHA)	<= 10	10
Residue after Evaporation	<= 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	<= 0.05 %	<0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC



SHIPPING DOCUMENTS

CLIENT INFORMATION

REPORT TO BE SENT TO:

COMPANY: Gen Environmental
ADDRESS: B Carriado
CITY: Succasunna STATE: NJ ZIP:
ATTENTION:
PHONE: FAX:

CLIENT PROJECT INFORMATION

PROJECT NAME: Newport
PROJECT NO.: LOCATION:
PROJECT MANAGER:
e-mail:
PHONE: FAX:

CLIENT BILLING INFORMATION

BILL TO: G Environmental PO#:
ADDRESS: B Carriado
CITY: Succasunna STATE: NJ ZIP:
ATTENTION: PHONE:

ANALYSIS

DATA TURNAROUND INFORMATION

FAX (RUSH) DAYS*
HARDCOPY (DATA PACKAGE) DAYS*
EDD: DAYS*
*TO BE APPROVED BY CHEMTECH
STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS

DATA DELIVERABLE INFORMATION

☐ Level 1 (Results Only) ☐ Level 4 (QC + Full Raw Data)
☐ Level 2 (Results + QC) ☒ NJ Reduced ☐ US EPA CLP
☐ Level 3 (Results + QC) ☐ NYS ASP A ☐ NYS ASP B
+ Raw Data ☐ Other
☒ EDD FORMAT edd, has site

EPH VOC GRD THAL Metals PCBS ICUP Metals ICUP Metals ICUP Metals ICUP Metals ICUP Metals

ALLIANCE SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# OF BOTTLES	PRESERVATIVES									COMMENTS
			COMP	GRAB	DATE	TIME		1	2	3	4	5	6	7	8	9	
1.	<u>WC1</u>	<u>9/30/15</u> <u>5011</u>	<u>X</u>	<u> </u>	<u>9/30/15</u>	<u>1600</u>	<u>3</u>	<u>*</u>									
2.																	
3.																	
4.																	
5.																	
6.																	
7.																	
8.																	
9.																	
10.																	

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER: 1. <u> </u>	DATE/TIME: <u>1540</u> <u>10/2/25</u>	RECEIVED BY: 1. <u> </u>	Conditions of bottles or coolers at receipt: ☐ COMPLIANT ☐ NON COMPLIANT ☐ COOLER TEMP <u>2.1</u> °C
RELINQUISHED BY SAMPLER: 2. <u> </u>	DATE/TIME: <u> </u>	RECEIVED BY: 2. <u> </u>	Comments: <u>Waste Class</u>
RELINQUISHED BY SAMPLER: 3. <u> </u>	DATE/TIME: <u> </u>	RECEIVED BY: 3. <u> </u>	Page <u> </u> of <u> </u> CLIENT: ☐ Hand Delivered ☐ Other <u> </u> Shipment Complete ☐ YES ☐ NO

Laboratory Certification

Certified By	License No.
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255425
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	TX-C25-00189
Virginia	460312

LOGIN REPORT/SAMPLE TRANSFER

Order ID : Q3277 GENV01

Order Date : 10/2/2025 3:50:00 PM

Project Mgr :

Client Name : G Environmental

Project Name : ~~Lexington~~ **Newport**

Report Type : NJ Reduced

Client Contact : Gary Landis

Receive DateTime : 10/2/2025 3:40:00 PM

EDD Type : NJ HAZSITE

Invoice Name : G Environmental

Purchase Order :

Hard Copy Date :

Invoice Contact : Gary Landis

Date Signoff :

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DUE DATES
Q3277-01	WC1	Solid	09/30/2025	16:00	VOC-TCLVOA-10		8260D		10 Bus. Days

Relinquished By : 

Date / Time : 10/2/25 1620

Received By : 

Date / Time : 10/03/25

Storage Area : VOA Refridgerator Room