
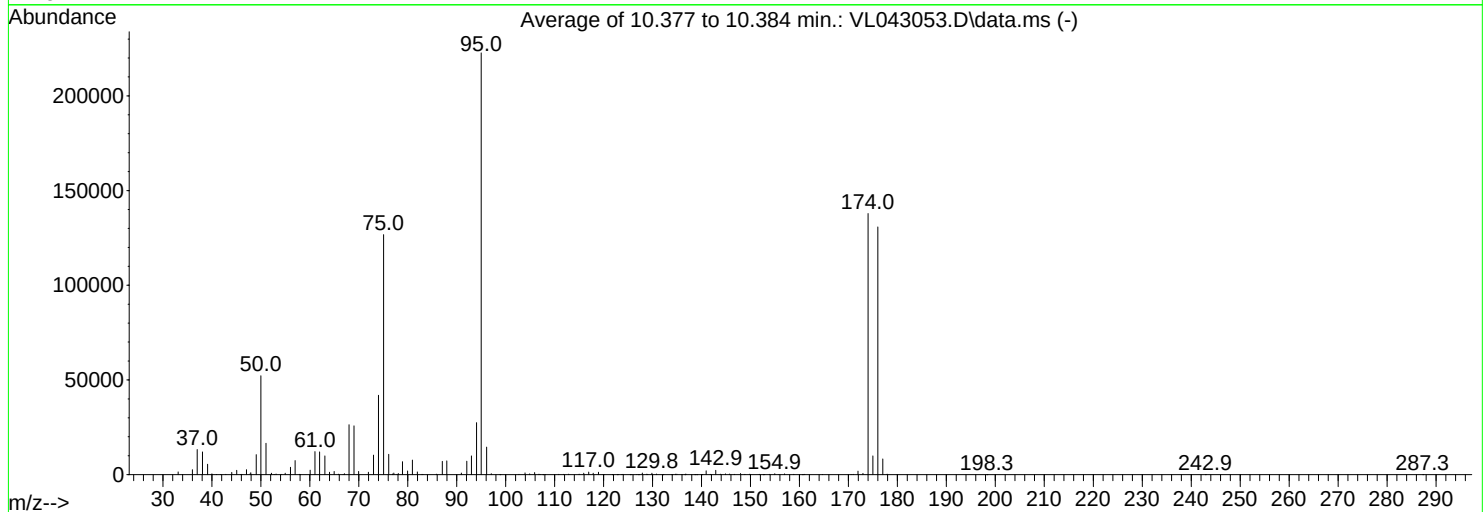


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100825\
Data File : VL043053.D
Acq On : 08 Oct 2025 08:00
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL100225AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Oct 03 08:23:34 2025

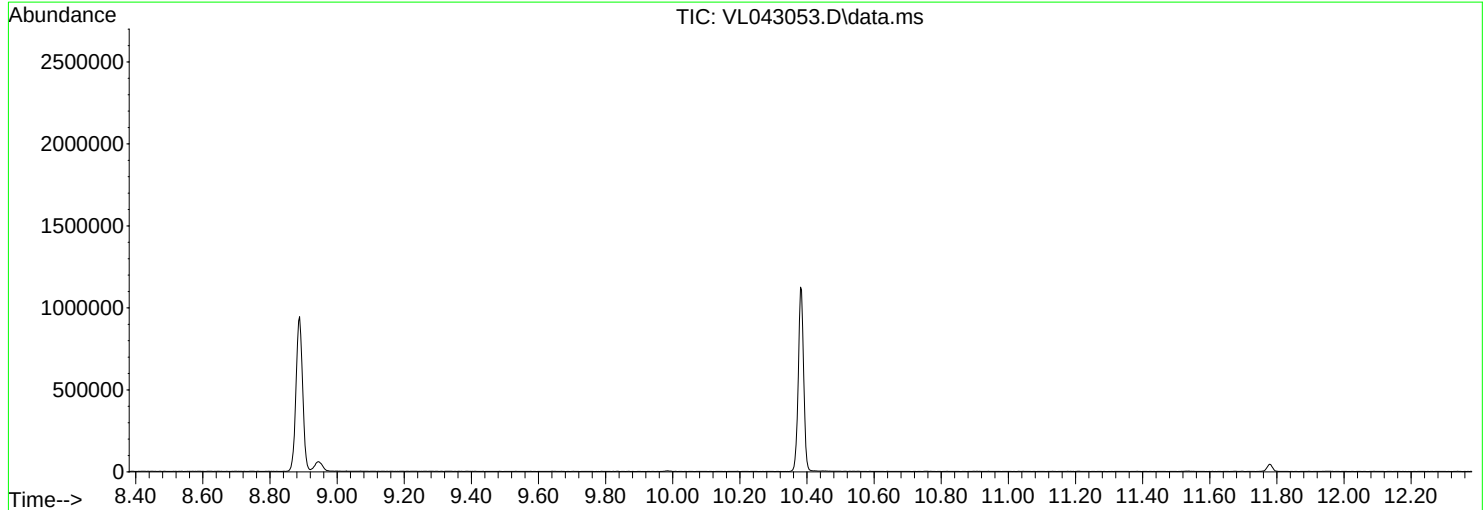

AutoFind: Scans 3179, 3180, 3181; Background Corrected with Scan 3165

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	23.5	52232	PASS
75	95	30	66	56.9	126765	PASS
95	95	100	100	100.0	222720	PASS
96	95	5	9	6.5	14516	PASS
173	174	0.00	2	0.5	727	PASS
174	95	50	120	61.9	137885	PASS
175	174	4	9	7.2	9912	PASS
176	174	93	101	94.8	130755	PASS
177	176	5	9	6.3	8273	PASS

Average of 10.377 to 10.384 min.: VL043053.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	1449	45.05	2301	53.10	357	64.00	1231
34.00	51	45.90	80	54.10	140	64.95	1663
36.00	2590	46.10	180	54.95	759	65.85	231
37.00	13307	47.05	2613	56.05	3851	66.80	101
38.05	12032	47.80	436	57.00	7464	67.05	510
39.10	5459	47.95	997	57.90	146	68.00	26405
40.00	430	49.05	10569	58.10	56	69.00	25795
40.95	81	50.00	52232	60.05	2388	69.95	1723
41.80	71	51.05	16602	61.05	12159	71.95	1245
42.85	177	52.15	766	62.00	11965	73.00	10332
44.05	1185	52.70	91	63.05	9906	74.00	41931

Average of 10.377 to 10.384 min.: VL043053.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.05	126765	83.10	68	98.80	36	111.85	213
76.10	10728	85.85	274	102.70	139	112.85	292
76.90	339	87.05	7042	103.95	956	115.00	241
77.15	885	87.95	7242	104.90	399	115.95	756
77.80	199	90.95	821	105.90	1086	116.95	1387
78.05	566	92.05	7105	106.80	264	117.85	806
78.90	6811	93.00	9919	107.00	49	118.95	1306
79.95	1964	94.05	27456	107.60	21	119.90	17
80.95	7672	95.00	222720	108.10	53	121.80	18
81.95	1414	96.10	14516	110.00	87	122.80	36
82.90	150	97.05	480	110.85	142	123.70	52

Average of 10.377 to 10.384 min.: VL043053.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
123.95	167	134.70	229	143.85	221	154.95	472
125.45	43	134.95	252	144.90	469	155.80	72
126.80	50	136.00	50	145.75	320	156.95	428
127.10	40	136.60	46	146.70	166	158.85	181
127.90	818	136.80	355	147.95	582	160.60	39
128.80	267	138.60	22	148.85	156	161.05	155
129.00	190	139.00	21	149.85	276	164.70	53
129.85	766	140.00	46	151.80	147	170.55	71
130.80	308	140.95	2009	152.60	22	170.95	212
132.10	24	141.80	198	152.90	87	171.95	1901
133.90	41	142.90	2301	153.85	175	172.95	727

Average of 10.377 to 10.384 min.: VL043053.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
174.00	137885						
175.00	9912						
176.00	130755						
177.00	8273						
177.90	254						
198.30	26						
242.90	24						
287.30	26						