

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100825\
 Data File : VL043062.D
 Acq On : 08 Oct 2025 13:58
 Operator : SY/MD
 Sample : Q3306-01DUP
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 IA1DUP


Quant Time: Oct 09 01:18:08 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL100225AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Oct 03 08:23:34 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.793	49	183624	10.000	ppbv	0.02
33) 1,4-Difluorobenzene	3.965	114	501713	10.000	ppbv	0.03
55) Chlorobenzene-d5	8.888	117	398502	10.000	ppbv	0.03
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.380	95	292656	10.194	ppbv	0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	101.900%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.502	85	14182	0.458	ppbv	98
3) Chlorodifluoromethane	1.852	51	1064	0.036	ppbv	97
4) Chloromethane	1.534	50	5451	0.482	ppbv	94
9) Propene	1.489	41	12777	1.058	ppbv	86
10) Heptane	4.985	43	1096	0.037	ppbv #	61
11) Trichlorofluoromethane	1.881	101	7500	0.236	ppbv	95
12) 1,1,2-Trichlorotrifluo...	2.146	101	1659	0.066	ppbv	97
13) Ethanol	1.725	45	49077	110.920	ppbv	90
15) Acetone	1.839	43	173289	6.740	ppbv	98
16) 1,3-Butadiene	1.625	39	10677	1.007	ppbv #	11
17) tert-Butyl alcohol	2.046	59	3568	0.131	ppbv #	87
19) Isopropyl Alcohol	1.890	45	15415	1.251	ppbv #	1
20) Methylene Chloride	2.065	84	264125	23.536	ppbv	95
21) Allyl Chloride	2.065	41	9278	0.563	ppbv #	29
23) Vinyl Acetate	2.457	43	11937	2.187	ppbv #	88
25) Ethyl Acetate	2.832	43	237047	3.675	ppbv #	77
26) Hexane	2.832	57	339260	13.674	ppbv #	34
29) Chloroform	2.855	83	2279	0.054	ppbv	91
34) 2-Butanone	2.564	43	12032	0.353	ppbv	100
35) Carbon Tetrachloride	3.771	117	1761	0.043	ppbv #	93
36) Benzene	3.661	78	7995	0.167	ppbv #	92
39) 1,2-Dichloropropane	3.965	63	124928	7.031	ppbv #	22
41) Tetrahydrofuran	2.832	42	132513	7.532	ppbv #	49
44) 2,2,4-Trimethylpentane	4.645	57	5833	0.076	ppbv #	23
53) Toluene	6.940	91	14257	0.295	ppbv	97
58) Ethyl Benzene	9.357	91	2678	0.043	ppbv	90
60) o-Xylene	9.969	91	4126	0.080	ppbv	98
66) Benzyl Chloride	11.642	91	98	0.036	ppbv #	65
73) 1,3,5-Trimethylbenzene	11.205	105	2155	0.040	ppbv	92
74) 1,2,4-Trimethylbenzene	11.539	105	6164	0.102	ppbv #	60
75) 1,3-Dichlorobenzene	11.675	146	1650	0.042	ppbv #	81
76) 1,4-Dichlorobenzene	11.675	146	1650	0.044	ppbv #	81
79) Naphthalene	13.539	128	61	0.235	ppbv #	59
80) Naphthalene,2-methyl-	14.465	142	1513	0.721	ppbv #	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Oct 09 01:18:08 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL100225AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug 26 06:05:16 2022
QLast Update : Fri Oct 03 08:23:34 2025
Response via : Initial Calibration




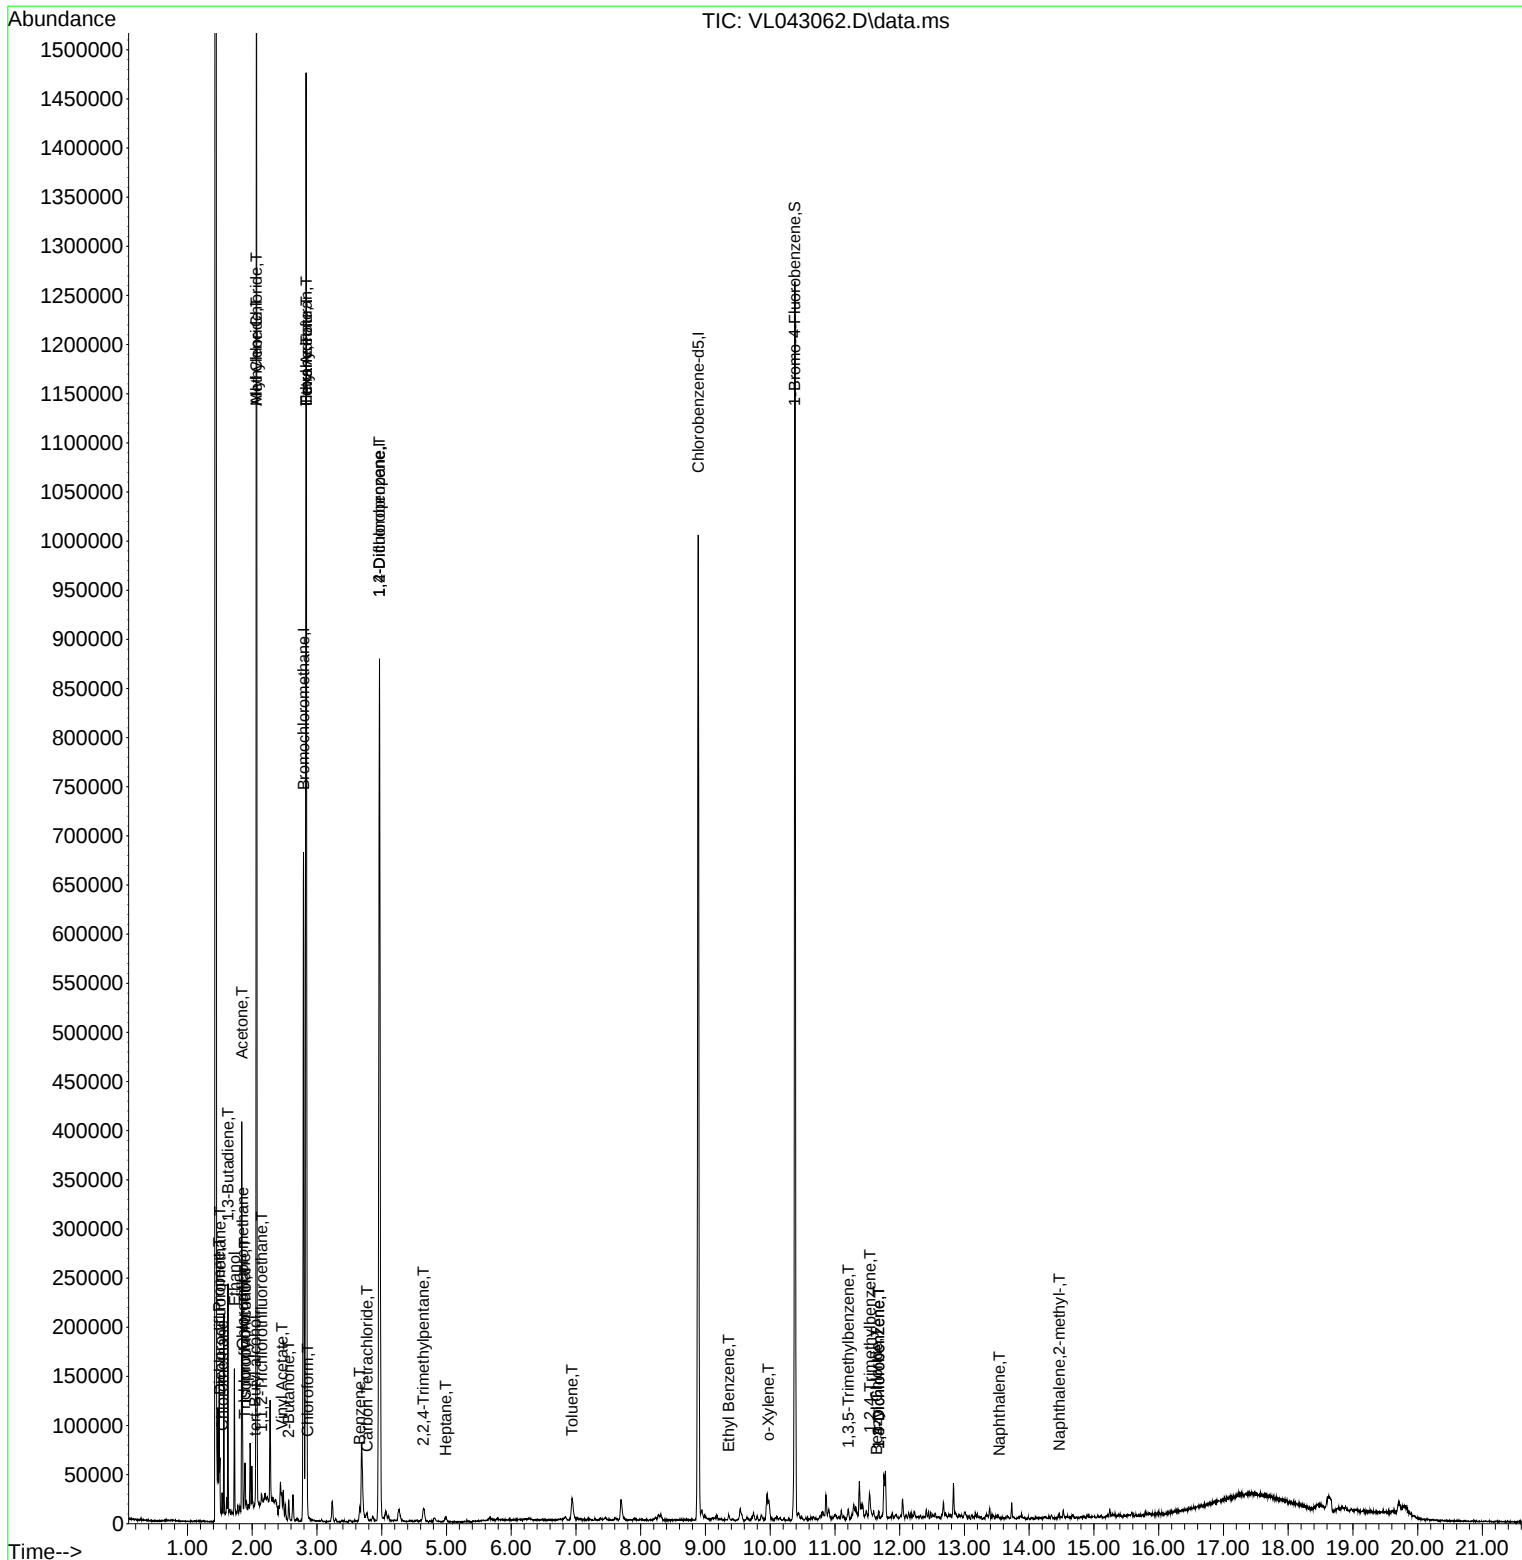




#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 2.793 min Scan# 81
Delta R.T. 0.019 min
Lab File: VL043062.D
Acq: 08 Oct 2025 13:58




Instrument :
MSVOA_L
ClientSampleId :
IA1DUP


Tgt Ion: 49 Resp: 183624
Ion Ratio Lower Upper
49 100
128 48.7 24.1 72.2
130 61.0 31.4 94.3

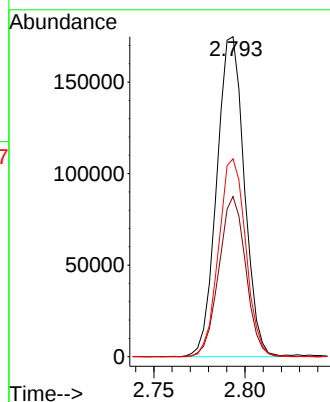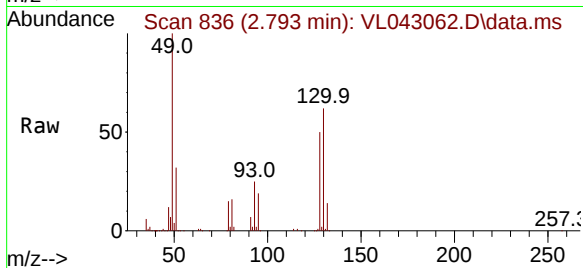

#2
Dichlorodifluoromethane
Concen: 0.458 ppbv
RT: 1.502 min Scan# 437
Delta R.T. 0.006 min
Lab File: VL043062.D
Acq: 08 Oct 2025 13:58

Tgt Ion: 85 Resp: 14182
Ion Ratio Lower Upper
85 100
87 31.3 25.8 38.6



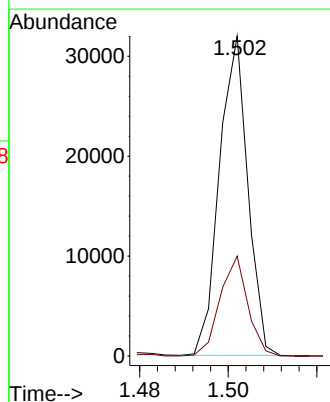
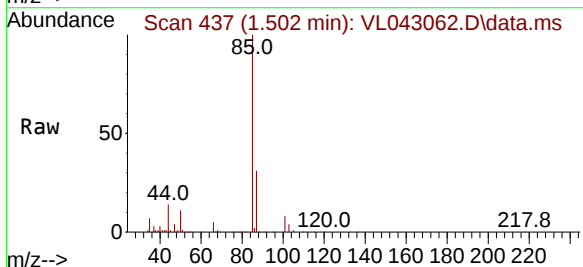




#3
Chlorodifluoromethane
Concen: 0.036 ppbv
RT: 1.852 min Scan# 54
Delta R.T. 0.379 min
Lab File: VL043062.D
Acq: 08 Oct 2025 13:58




Instrument :
MSVOA_L
ClientSampleId :
IA1DUP


Tgt Ion: 51 Resp: 1064
Ion Ratio Lower Upper
51 100
67 17.5 15.1 22.7



#4
Chloromethane
Concen: 0.482 ppbv
RT: 1.534 min Scan# 447
Delta R.T. 0.006 min
Lab File: VL043062.D
Acq: 08 Oct 2025 13:58

Tgt Ion: 50 Resp: 5451
Ion Ratio Lower Upper
50 100
52 36.0 26.2 39.2




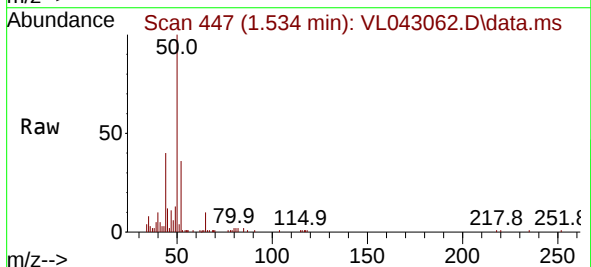




#9
Propene
Concen: 1.058 ppbv
RT: 1.489 min Scan# 41
Delta R.T. 0.010 min
Lab File: VL043062.D
Acq: 08 Oct 2025 13:58




Instrument :
MSVOA_L
ClientSampleId :
IA1DUP


Tgt Ion: 41 Resp: 12777
Ion Ratio Lower Upper
41 100
42 55.7 53.3 79.9



#10
Heptane
Concen: 0.037 ppbv
RT: 4.985 min Scan# 1513
Delta R.T. 0.029 min
Lab File: VL043062.D
Acq: 08 Oct 2025 13:58

Tgt Ion: 43 Resp: 1096
Ion Ratio Lower Upper
43 100
57 77.4 40.3 60.5#





#11

Trichlorofluoromethane

Concen: 0.236 ppbv

RT: 1.881 min Scan# 511

Delta R.T. 0.010 min

Lab File: VL043062.D

Acq: 08 Oct 2025 13:58

Instrument :

MSVOA_L

ClientSampleId :





IA1DUP

Tgt Ion:101 Resp: 7500

Ion Ratio Lower Upper

101 100

103 67.9 51.1 76.7

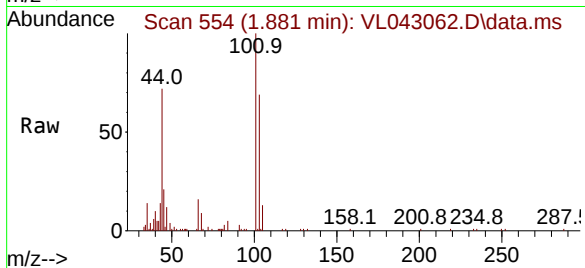

#12

1,1,2-Trichlorotrifluoroethane

Concen: 0.066 ppbv

RT: 2.146 min Scan# 636

Delta R.T. 0.016 min

Lab File: VL043062.D




Acq: 08 Oct 2025 13:58


Tgt Ion:101 Resp: 1659

Ion Ratio Lower Upper

101 100

151 69.7 58.1 87.1




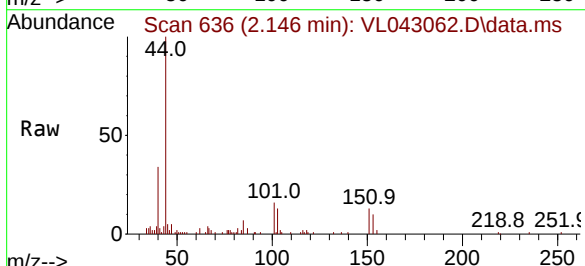




#13
 Ethanol
 Concen: 110.920 ppbv
 RT: 1.725 min Scan# 503
 Delta R.T. 0.009 min
 Lab File: VL043062.D
 Acq: 08 Oct 2025 13:58




Instrument :
 MSVOA_1
 ClientSampleId :
 IA1DUP


Tgt Ion: 45 Resp: 49077
 Ion Ratio Lower Upper
 45 100
 46 38.2 17.8 71.4



#15
 Acetone
 Concen: 6.740 ppbv
 RT: 1.839 min Scan# 541
 Delta R.T. 0.010 min
 Lab File: VL043062.D
 Acq: 08 Oct 2025 13:58

Tgt Ion: 43 Resp: 173289
 Ion Ratio Lower Upper
 43 100
 58 26.6 22.2 33.4




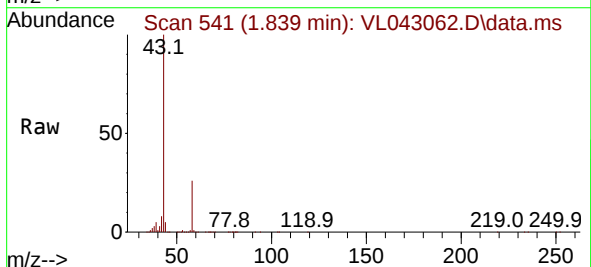




#16
1,3-Butadiene
Concen: 1.007 ppbv
RT: 1.625 min Scan# 41
Delta R.T. 0.019 min
Lab File: VL043062.D
Acq: 08 Oct 2025 13:58




Instrument :
MSVOA_L
ClientSampleId :
IA1DUP


Tgt Ion: 39 Resp: 10677
Ion Ratio Lower Upper
39 100
54 0.0 61.4 92.2#

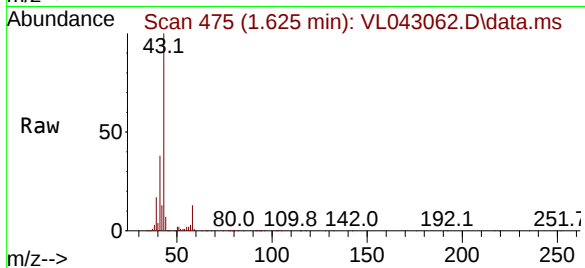

#17
tert-Butyl alcohol
Concen: 0.131 ppbv
RT: 2.046 min Scan# 605
Delta R.T. 0.013 min
Lab File: VL043062.D
Acq: 08 Oct 2025 13:58

Tgt Ion: 59 Resp: 3568
Ion Ratio Lower Upper
59 100
57 15.5 8.5 12.7#


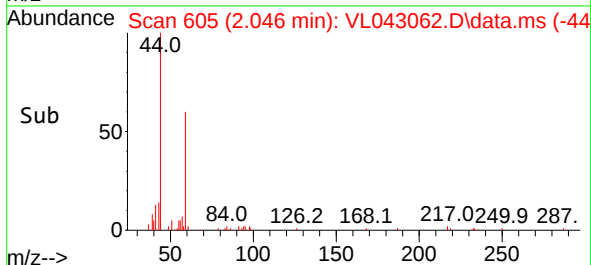

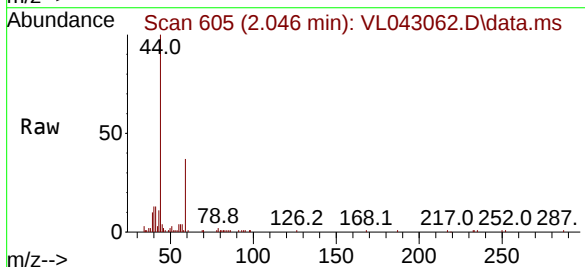




#19
Isopropyl Alcohol
Concen: 1.251 ppbv
RT: 1.890 min Scan# 511
Delta R.T. 0.013 min
Lab File: VL043062.D
Acq: 08 Oct 2025 13:58




Instrument :
MSVOA_L
ClientSampleId :
IA1DUP


Tgt Ion: 45 Resp: 15415
Ion Ratio Lower Upper
45 100
58 299.3 42.3 63.5#

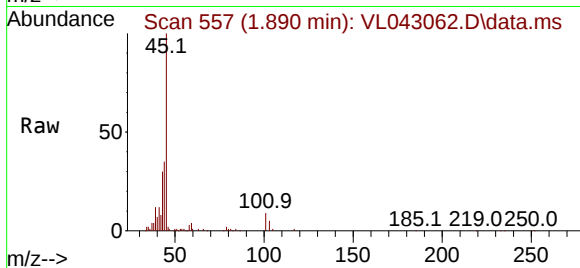

#20
Methylene Chloride
Concen: 23.536 ppbv
RT: 2.065 min Scan# 611
Delta R.T. 0.013 min
Lab File: VL043062.D
Acq: 08 Oct 2025 13:58

Tgt Ion: 84 Resp: 264125
Ion Ratio Lower Upper
84 100
49 146.4 112.5 168.7
51 45.4 34.2 51.2
86 65.9 48.4 72.6


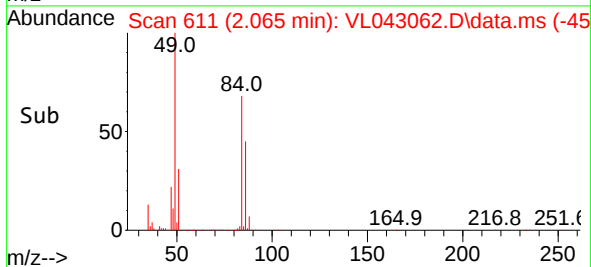

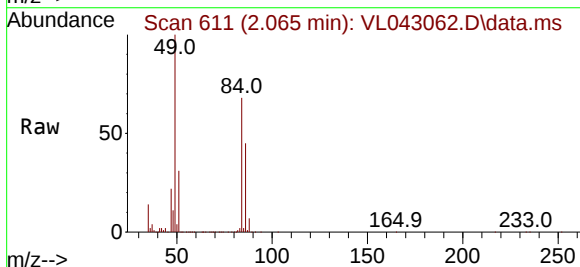




#21
 Allyl Chloride
 Concen: 0.563 ppbv
 RT: 2.065 min Scan# 611
 Delta R.T. -0.023 min
 Lab File: VL043062.D
 Acq: 08 Oct 2025 13:58




Instrument :
 MSVOA_L
 ClientSampleId :
 IA1DUP


Tgt Ion: 41 Resp: 9278
 Ion Ratio Lower Upper
 41 100
 76 0.9 25.9 38.9#
 39 11.8 63.0 94.4#

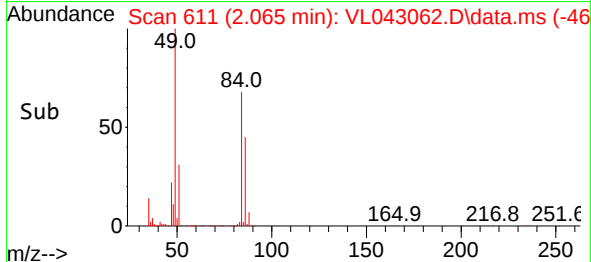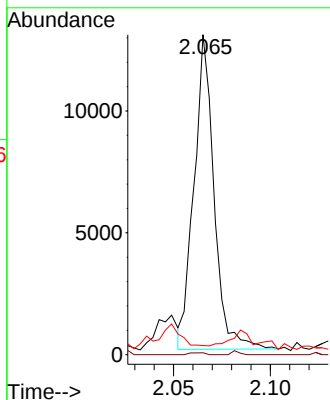

#23
 Vinyl Acetate
 Concen: 2.187 ppbv
 RT: 2.457 min Scan# 732
 Delta R.T. 0.006 min
 Lab File: VL043062.D
 Acq: 08 Oct 2025 13:58

Tgt Ion: 43 Resp: 11937
 Ion Ratio Lower Upper
 43 100
 86 11.3 7.5 11.3#
 42 15.5 8.4 12.6#
 44 3.6 7.8 11.8#


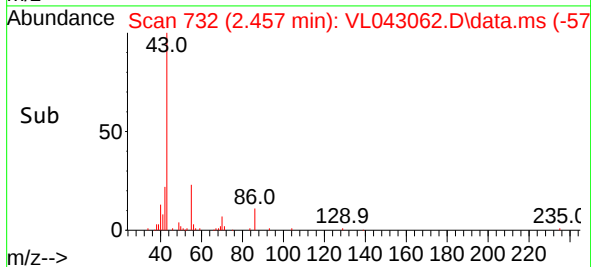
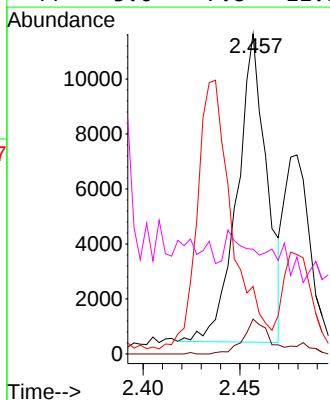
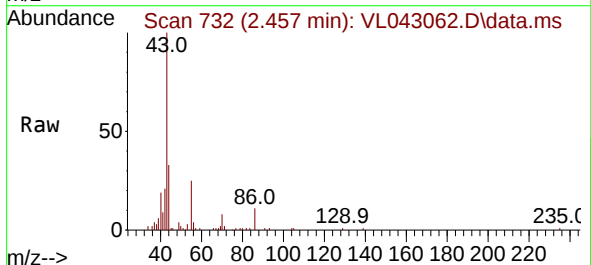




#25
Ethyl Acetate
Concen: 3.675 ppbv
RT: 2.832 min Scan# 848
Delta R.T. 0.013 min
Lab File: VL043062.D
Acq: 08 Oct 2025 13:58




Instrument :
MSVOA_1
ClientSampleId :
IA1DUP


Tgt Ion: 43 Resp: 237047
Ion Ratio Lower Upper
43 100
45 0.8 8.3 12.5#
61 0.4 7.5 11.3#
70 1.7 6.8 10.2#

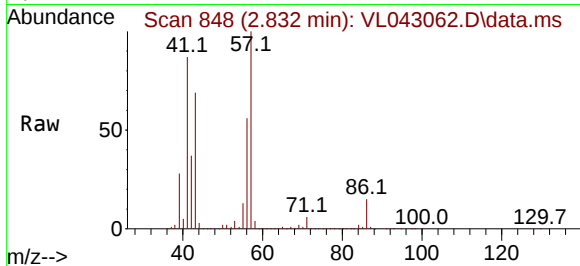

#26
Hexane
Concen: 13.674 ppbv
RT: 2.832 min Scan# 848
Delta R.T. 0.019 min
Lab File: VL043062.D
Acq: 08 Oct 2025 13:58

Tgt Ion: 57 Resp: 339260
Ion Ratio Lower Upper
57 100
41 89.7 76.1 114.1
43 70.0 201.4 302.0#
56 55.3 44.0 66.0

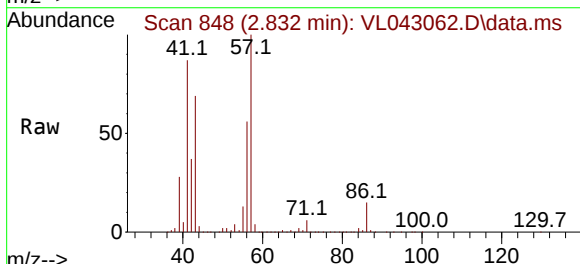



#29

Chloroform

Concen: 0.054 ppbv

RT: 2.855 min Scan# 81

Delta R.T. 0.019 min

Lab File: VL043062.D

Acq: 08 Oct 2025 13:58

Instrument :

MSVOA_L

ClientSampleId :





IA1DUP

Tgt Ion: 83 Resp: 2279

Ion Ratio Lower Upper

83 100

85 71.9 52.0 78.0

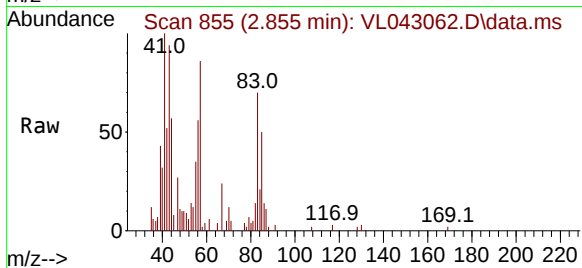

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 3.965 min Scan# 1198

Delta R.T. 0.026 min

Lab File: VL043062.D

Acq: 08 Oct 2025 13:58




Tgt Ion: 114 Resp: 501713


Ion Ratio Lower Upper

114 100

63 25.0 19.4 29.2

88 17.5 13.9 20.9


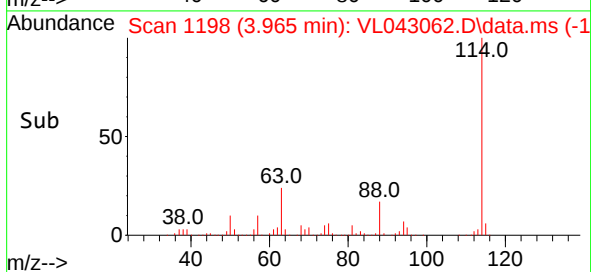

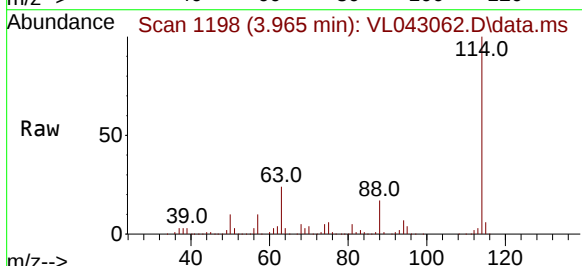




#34
2-Butanone
Concen: 0.353 ppbv
RT: 2.564 min Scan# 71
Delta R.T. 0.019 min
Lab File: VL043062.D
Acq: 08 Oct 2025 13:58




Instrument :
MSVOA_L
ClientSampleId :
IA1DUP


Tgt Ion: 43 Resp: 12032
Ion Ratio Lower Upper
43 100
72 23.2 18.4 27.6

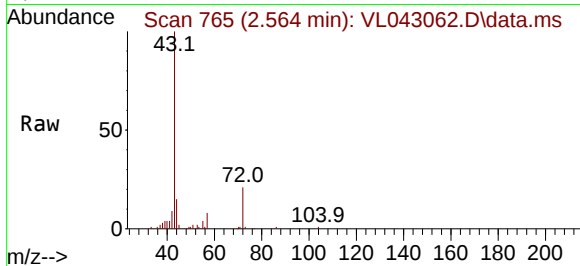

#35
Carbon Tetrachloride
Concen: 0.043 ppbv
RT: 3.771 min Scan# 1138
Delta R.T. 0.026 min
Lab File: VL043062.D
Acq: 08 Oct 2025 13:58

Tgt Ion: 117 Resp: 1761
Ion Ratio Lower Upper
117 100
119 96.7 78.2 117.4
121 16.8 24.8 37.2#

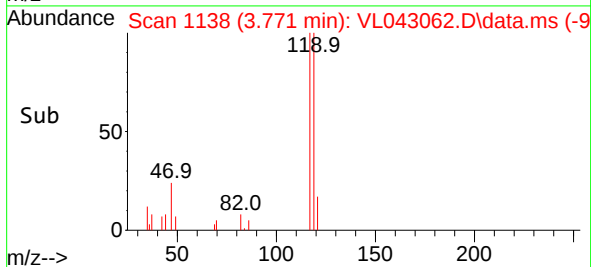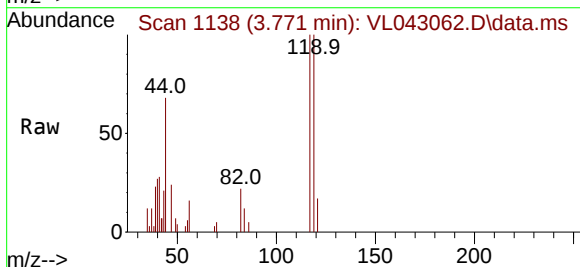



#36

Benzene

Concen: 0.167 ppbv

RT: 3.661 min Scan# 1104

Delta R.T. 0.023 min

Lab File: VL043062.D

Acq: 08 Oct 2025 13:58

Instrument :

MSVOA_L

ClientSampleId :

IA1DUP





Tgt Ion: 78 Resp: 7995

Ion Ratio Lower Upper

78 100

77 29.9 19.2 28.8#

50 19.5 14.9 22.3

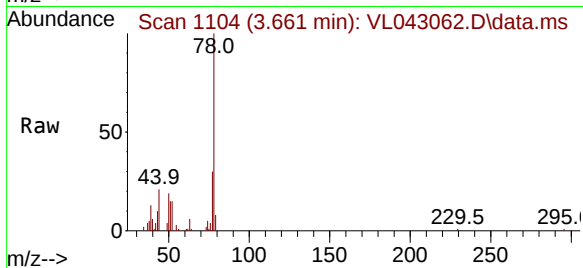

#39

1,2-Dichloropropane

Concen: 7.031 ppbv

RT: 3.965 min Scan# 1198

Delta R.T. -0.327 min

Lab File: VL043062.D

Acq: 08 Oct 2025 13:58




Tgt Ion: 63 Resp: 124928


Ion Ratio Lower Upper

63 100

41 0.1 61.6 92.4#

62 16.6 58.1 87.1#

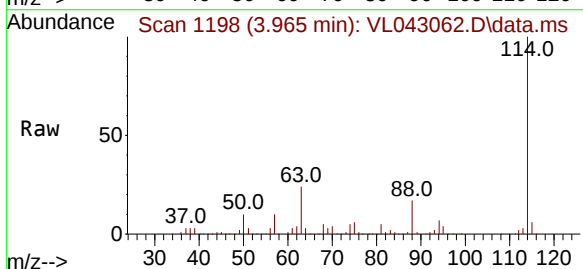



#41

Tetrahydrofuran

Concen: 7.532 ppbv

RT: 2.832 min Scan# 84

Delta R.T. -0.204 min

Lab File: VL043062.D

Acq: 08 Oct 2025 13:58

Instrument :

MSVOA_L

ClientSampleId :

IA1DUP





Tgt Ion: 42 Resp: 132513

Ion Ratio Lower Upper

42 100

72 0.8 31.0 46.6#

71 14.3 29.8 44.6#

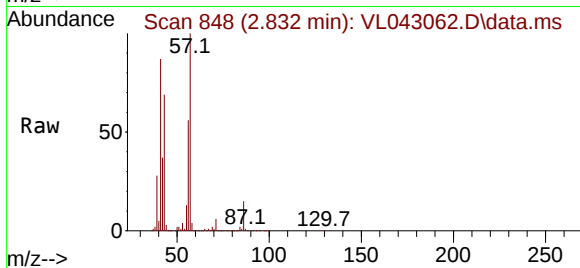

#44

2,2,4-Trimethylpentane

Concen: 0.076 ppbv

RT: 4.645 min Scan# 1408

Delta R.T. 0.029 min

Lab File: VL043062.D

Acq: 08 Oct 2025 13:58




Tgt Ion: 57 Resp: 5833


Ion Ratio Lower Upper

57 100

41 87.6 27.0 40.4#

56 0.0 26.0 39.0#


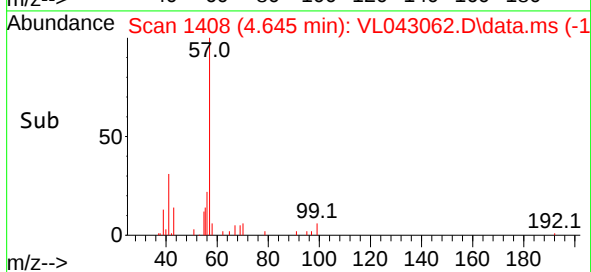

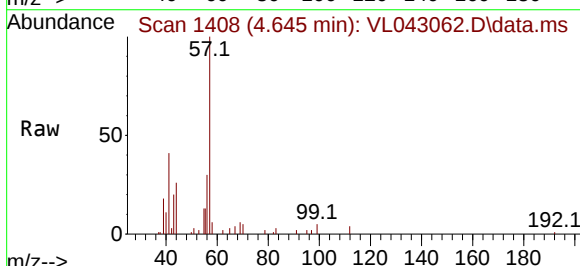




#53
Toluene
Concen: 0.295 ppbv
RT: 6.940 min Scan# 2107
Delta R.T. 0.032 min
Lab File: VL043062.D
Acq: 08 Oct 2025 13:58




Instrument :
MSVOA_L
ClientSampleId :
IA1DUP


Tgt Ion: 91 Resp: 14257
Ion Ratio Lower Upper
91 100
92 61.8 47.8 71.6



#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 8.888 min Scan# 2719
Delta R.T. 0.026 min
Lab File: VL043062.D
Acq: 08 Oct 2025 13:58

Tgt Ion: 117 Resp: 398502
Ion Ratio Lower Upper
117 100
82 64.0 53.0 79.6
119 31.9 25.4 38.2

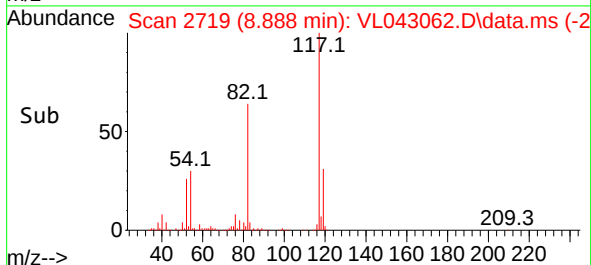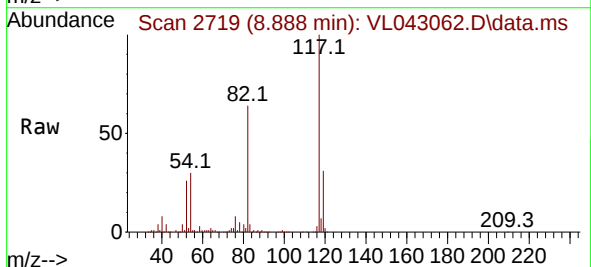



#58

Ethyl Benzene

Concen: 0.043 ppbv

RT: 9.357 min Scan# 21

Delta R.T. 0.019 min

Lab File: VL043062.D

Acq: 08 Oct 2025 13:58

Instrument :

MSVOA_L

ClientSampleId :





IA1DUP

Tgt Ion: 91 Resp: 2678

Ion Ratio Lower Upper

91 100

106 24.5 24.1 36.1

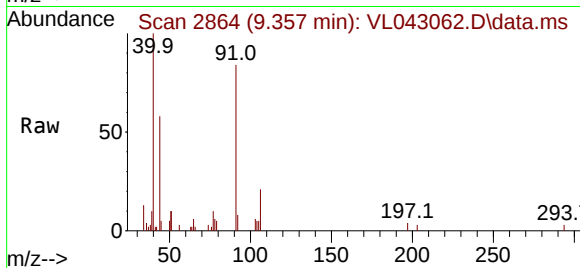

#60

o-Xylene

Concen: 0.080 ppbv

RT: 9.969 min Scan# 3053

Delta R.T. 0.023 min

Lab File: VL043062.D




Acq: 08 Oct 2025 13:58


Tgt Ion: 91 Resp: 4126

Ion Ratio Lower Upper

91 100

106 42.3 21.9 65.5




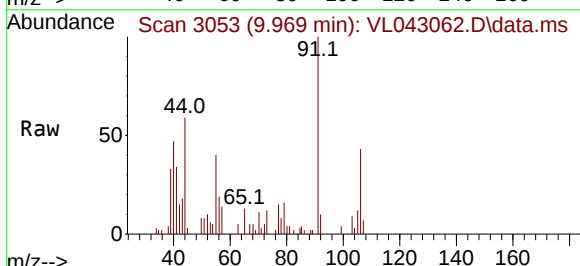




#66
Benzyl Chloride
Concen: 0.036 ppbv
RT: 11.642 min Scan# 3180
Delta R.T. 0.039 min
Lab File: VL043062.D
Acq: 08 Oct 2025 13:58




Instrument :
MSVOA_L
ClientSampleId :
IA1DUP


Tgt Ion: 91 Resp: 98
Ion Ratio Lower Upper
91 100
126 0.0 14.2 21.4#
128 0.0 4.8 7.2#

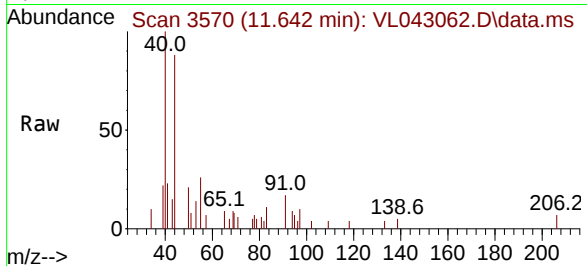

#68
1-Bromo-4-Fluorobenzene
Concen: 10.194 ppbv
RT: 10.380 min Scan# 3180
Delta R.T. 0.019 min
Lab File: VL043062.D
Acq: 08 Oct 2025 13:58

Tgt Ion: 95 Resp: 292656
Ion Ratio Lower Upper
95 100
174 66.0 52.3 78.5
175 4.9 3.8 5.8

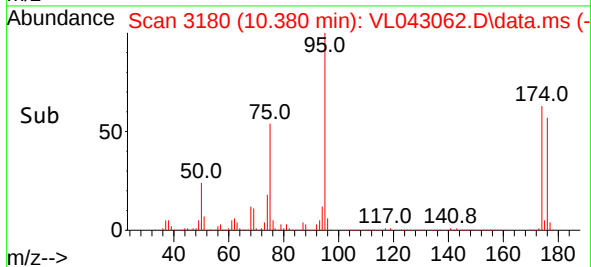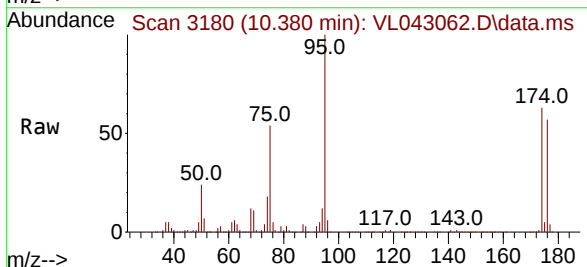



#73

1,3,5-Trimethylbenzene

Concen: 0.040 ppbv

RT: 11.205 min Scan# 3435

Delta R.T. 0.016 min

Lab File: VL043062.D

Acq: 08 Oct 2025 13:58

Instrument :

MSVOA_L

ClientSampleId :





IA1DUP

Tgt Ion:105 Resp: 2155

Ion Ratio Lower Upper

105 100

120 41.8 37.5 56.3

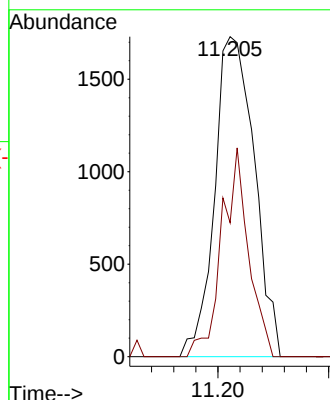

#74

1,2,4-Trimethylbenzene

Concen: 0.102 ppbv

RT: 11.539 min Scan# 3538

Delta R.T. 0.016 min

Lab File: VL043062.D

Acq: 08 Oct 2025 13:58

Tgt Ion:105 Resp: 6164




Ion Ratio Lower Upper


105 100

120 44.6 39.7 59.5

91 12.4 56.5 84.7#

77 15.5 19.9 29.9#

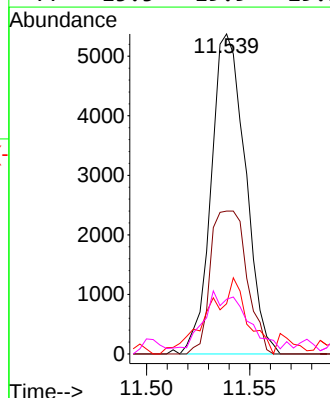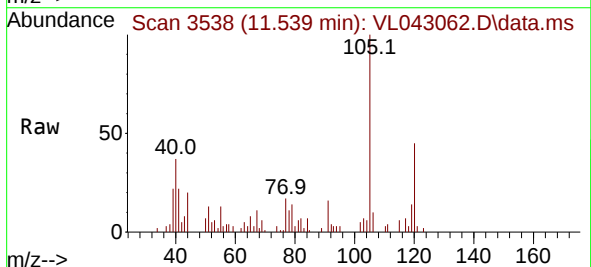



#75

1,3-Dichlorobenzene

Concen: 0.042 ppbv

RT: 11.675 min Scan# 3580

Delta R.T. 0.081 min

Lab File: VL043062.D

Acq: 08 Oct 2025 13:58





Instrument :

MSVOA_L

ClientSampleId :

IA1DUP

Tgt Ion:	146	Resp:	1650
Ion Ratio	Lower	Upper	
146	100		
111	71.1	22.6	67.7#
148	66.6	31.9	95.7

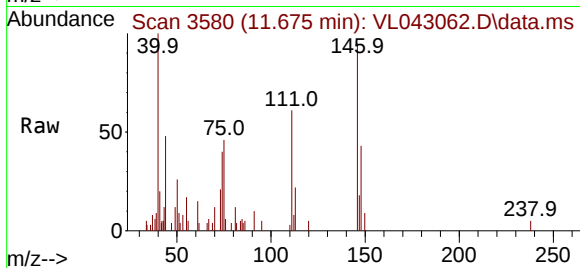

#76

1,4-Dichlorobenzene

Concen: 0.044 ppbv




RT: 11.675 min Scan# 3580


Delta R.T. 0.016 min

Lab File: VL043062.D

Acq: 08 Oct 2025 13:58

Tgt Ion:	146	Resp:	1650
Ion Ratio	Lower	Upper	
146	100		
111	71.1	21.7	65.1#
148	66.6	32.1	96.3





#79

Naphthalene

Concen: 0.235 ppbv

RT: 13.539 min Scan# 4144

Delta R.T. 0.039 min

Lab File: VL043062.D

Acq: 08 Oct 2025 13:58

Instrument :

MSVOA_L

ClientSampleId :

IA1DUP





Tgt Ion:128 Resp: 61

Ion Ratio Lower Upper

128 100

127 0.0 10.6 16.0#

129 30.0 8.8 13.2#

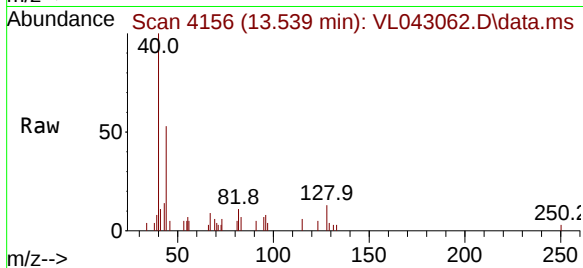

#80

Naphthalene,2-methyl-

Concen: 0.721 ppbv

RT: 14.465 min Scan# 4442

Delta R.T. 0.020 min

Lab File: VL043062.D

Acq: 08 Oct 2025 13:58

Tgt Ion:142 Resp: 1513

Ion Ratio Lower Upper

142 100

141 88.4 66.6 100.0

115 54.8 30.1 45.1#

