


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101025\
Data File : BF143919.D
Acq On : 10 Oct 2025 11:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 06 15:29:47 2025

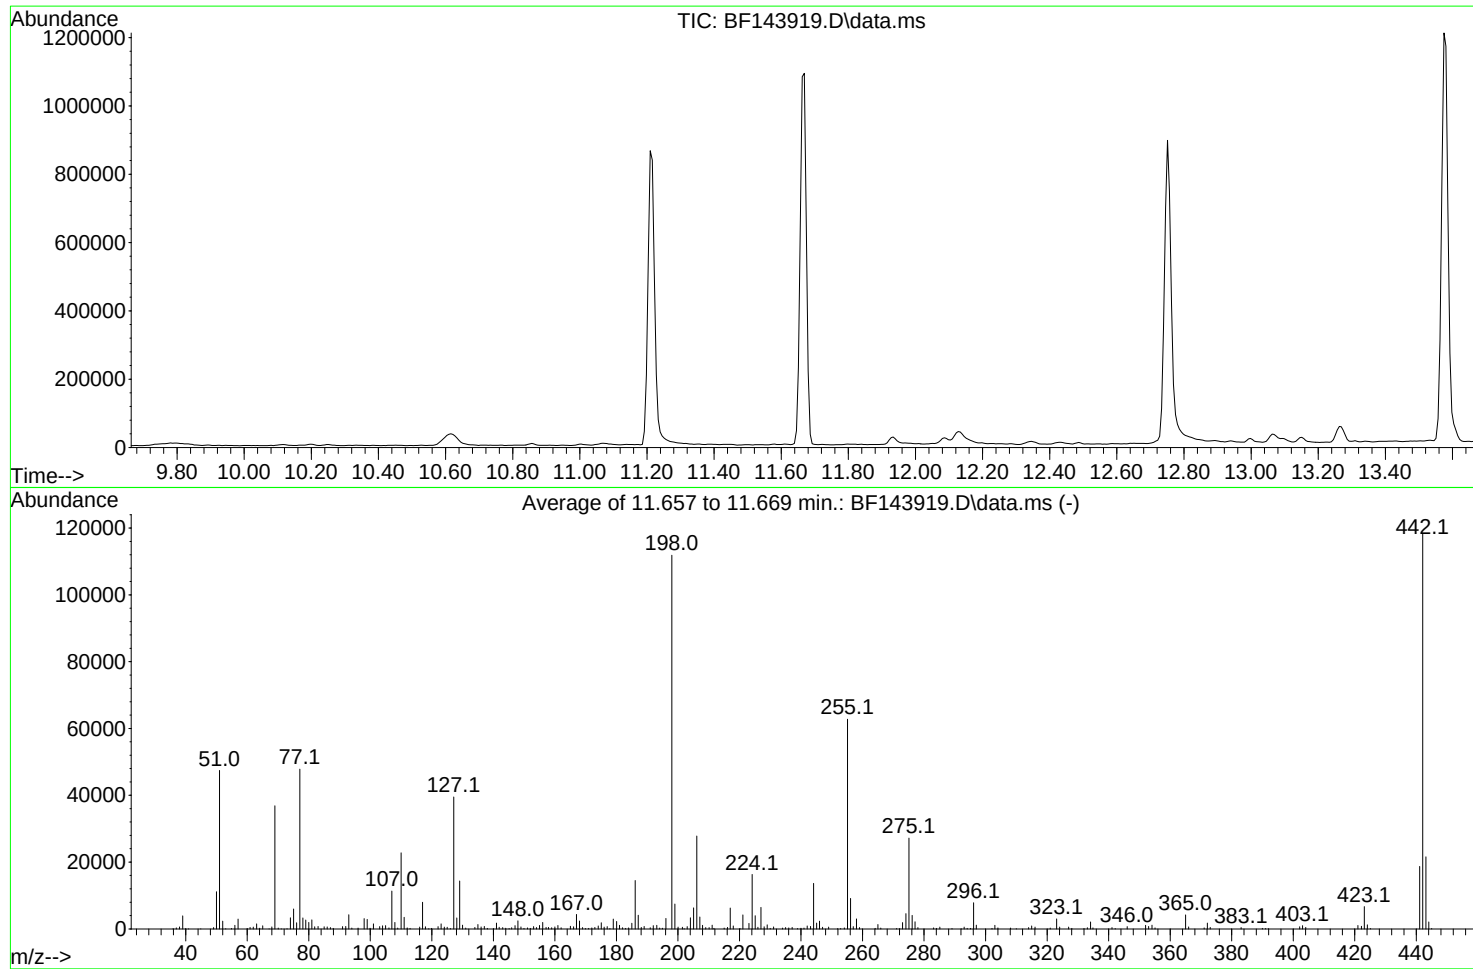




AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.6	596	PASS
69	69	100	100	100.0	36837	PASS
70	69	0.00	2	0.7	249	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	111853	PASS
199	198	5	9	6.7	7452	PASS
365	198	1	100	3.8	4202	PASS
441	443	0.01	150	86.7	18693	PASS
442	442	100	100	100.0	118192	PASS
443	442	15	24	18.2	21559	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101025\
Data File : BF143919.D
Acq On : 10 Oct 2025 11:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 10 13:10:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

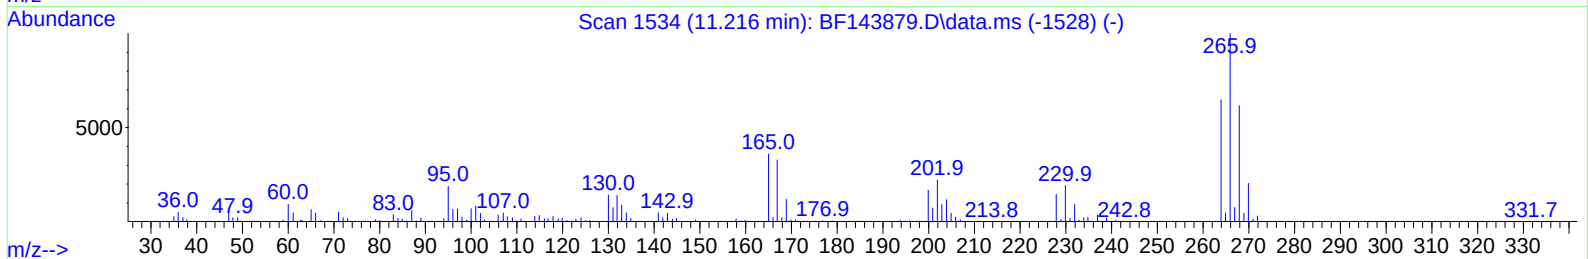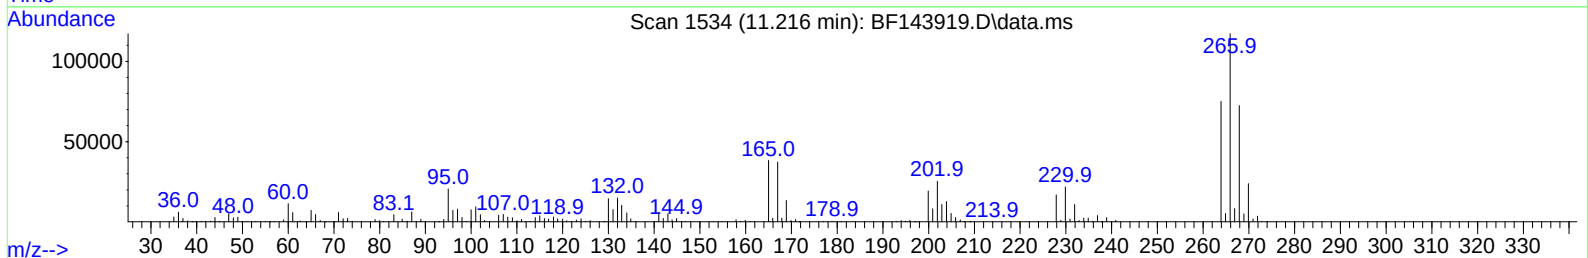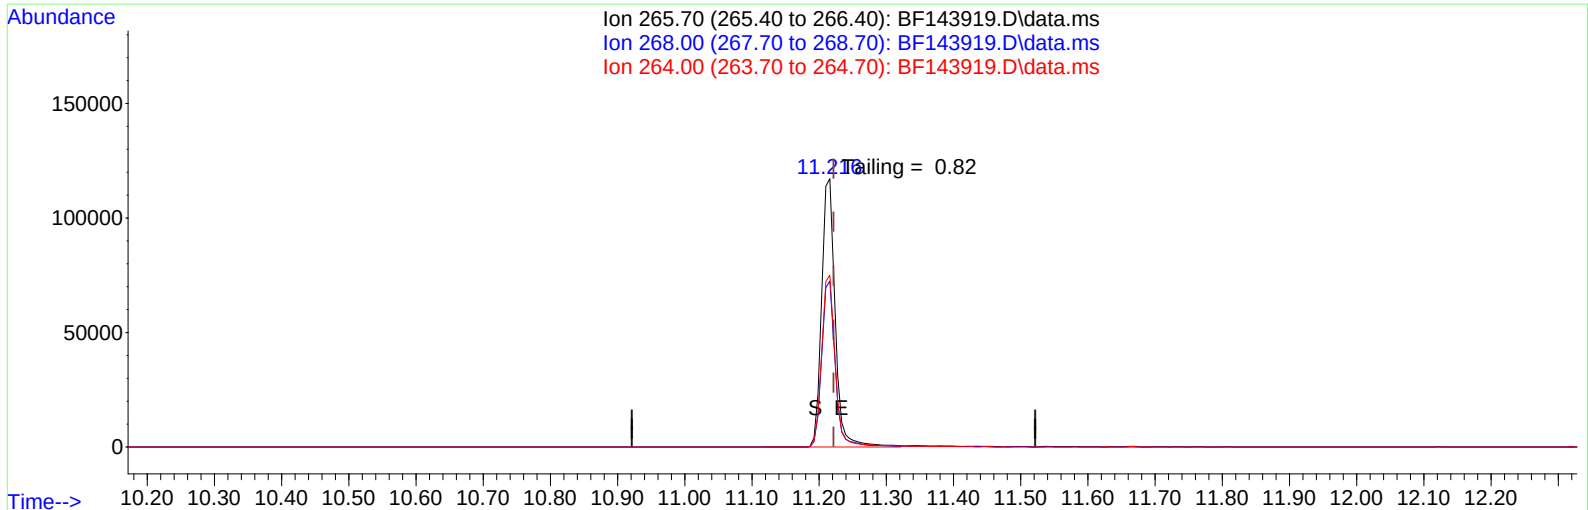

TIC: BF143919.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.006) 39764.54 ng




response 165677

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	61.81
264.00	64.70	64.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101025\
Data File : BF143919.D
Acq On : 10 Oct 2025 11:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 10 13:10:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

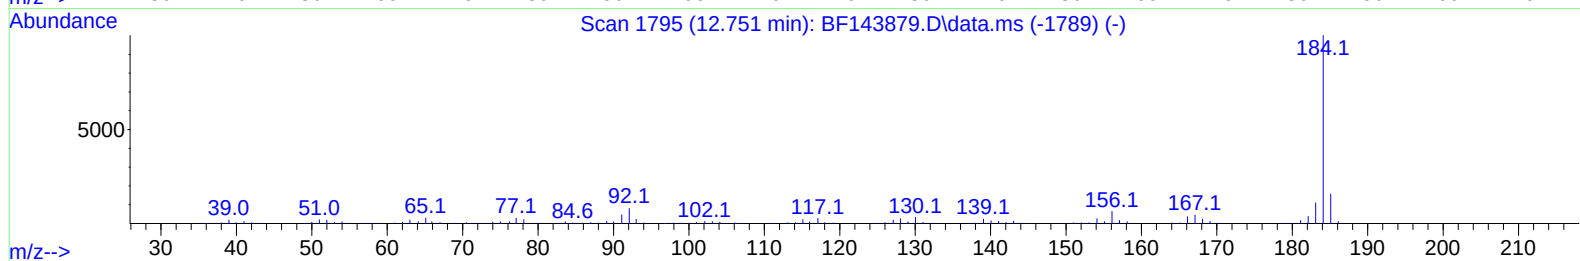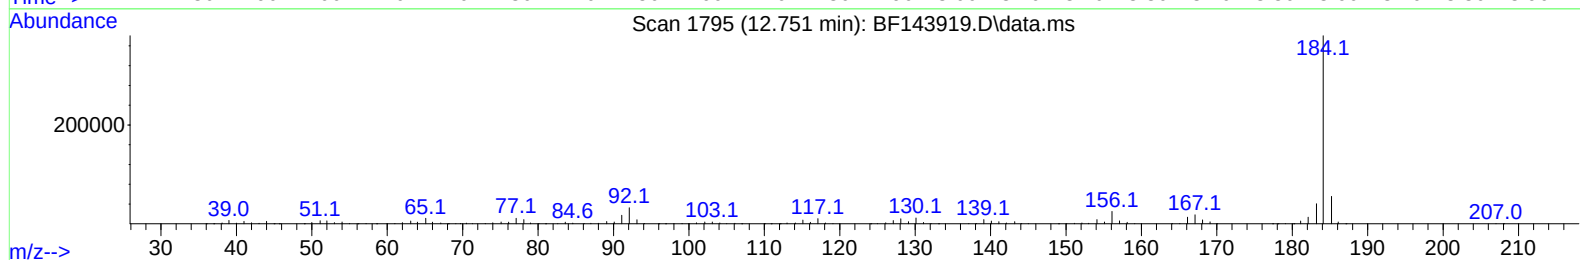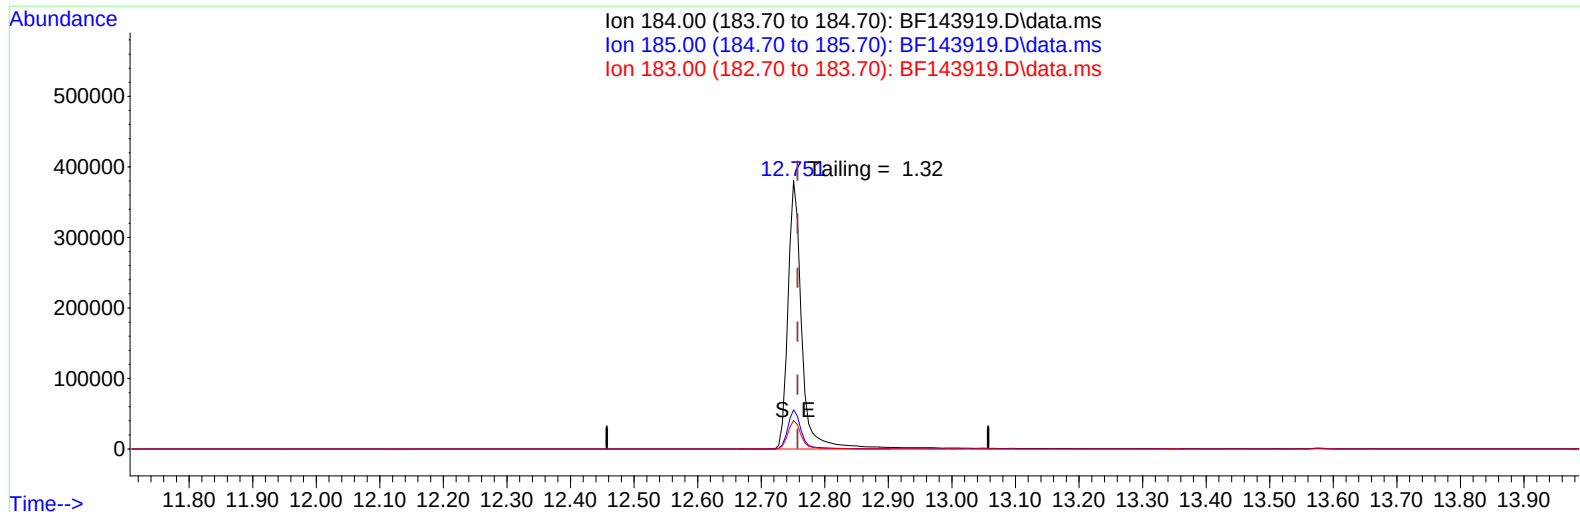

TIC: BF143919.D\data.ms

(77) Benzidine

12.751min (-0.006) 0.00 ng

response 579712

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.63
183.00	11.00	10.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/10/2025	BNA_F	<u>BF143919.D</u>
Compound Name	Response	Retention Time
DDT	326543	13.574
DDD	5283	13.274
DDE	738	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6021	332564	1.81

Instrument :
BNA_F
ClientSampleId :
DFTPP