

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100925\
 Data File : VL043087.D
 Acq On : 09 Oct 2025 14:25
 Operator : SY/MD
 Sample : Q3320-04 10X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SV2


Quant Time: Oct 09 22:15:51 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL100225AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Oct 03 08:23:34 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.777	49	189452	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.943	114	494714	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.862	117	492557	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.361	95	419950	11.835	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	118.400%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.496	85	2308	0.072	ppbv	98
3) Chlorodifluoromethane	1.473	51	2973	0.096	ppbv #	90
4) Chloromethane	1.528	50	526	0.045	ppbv #	50
8) Dichlorotetrafluoroethane	1.496	85	2308	0.088	ppbv #	15
9) Propene	1.483	41	4532	0.364	ppbv	96
10) Heptane	4.962	43	2005	0.065	ppbv #	7
11) Trichlorofluoromethane	1.871	101	38752	1.181	ppbv	98
12) 1,1,2-Trichlorotrifluo...	1.871	101	38752	1.499	ppbv #	13
13) Ethanol	1.428	45	396596	877.460	ppbv	81
15) Acetone	1.829	43	187635	7.073	ppbv	99
16) 1,3-Butadiene	1.615	39	964	0.088	ppbv #	11
17) tert-Butyl alcohol	2.039	59	2248	0.080	ppbv #	66
19) Isopropyl Alcohol	1.428	45	396596	31.205	ppbv #	25
20) Methylene Chloride	2.056	84	3580	0.309	ppbv	93
23) Vinyl Acetate	2.444	43	1305	0.232	ppbv #	1
25) Ethyl Acetate	2.816	43	18245	0.274	ppbv #	77
26) Hexane	2.816	57	24236	0.947	ppbv #	30
27) Carbon Disulfide	2.143	76	4724	0.156	ppbv #	1
29) Chloroform	2.836	83	2116	0.048	ppbv	88
32) 1,1,1-Trichloroethane	3.357	97	3784	0.089	ppbv #	46
34) 2-Butanone	2.548	43	9023	0.269	ppbv	96
36) Benzene	3.642	78	3029	0.064	ppbv #	86
38) Trichloroethene	4.528	130	56644	2.877	ppbv	97
39) 1,2-Dichloropropane	3.939	63	125657	7.172	ppbv #	22
51) 2-Hexanone	7.422	43	4001	0.137	ppbv #	94
52) Tetrachloroethene	8.205	164	568256	32.470	ppbv	99
53) Toluene	6.911	91	15976	0.335	ppbv	97
60) o-Xylene	9.943	91	9090	0.142	ppbv	95
66) Benzyl Chloride	11.610	91	163	0.049	ppbv #	65
71) 2-Chlorotoluene	10.976	91	3802	0.053	ppbv	77
73) 1,3,5-Trimethylbenzene	11.189	105	2577	0.039	ppbv #	83
74) 1,2,4-Trimethylbenzene	11.523	105	3042	0.041	ppbv #	54
79) Naphthalene	13.497	128	238	0.238	ppbv #	69
80) Naphthalene,2-methyl-	14.458	142	595	0.681	ppbv #	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Oct 09 22:15:51 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL100225AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug 26 06:05:16 2022
QLast Update : Fri Oct 03 08:23:34 2025
Response via : Initial Calibration





#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 2.777 min Scan# 830

Delta R.T. 0.003 min

Lab File: VL043087.D

Acq: 09 Oct 2025 14:25

Instrument :

MSVOA_L

ClientSampleId :

SV2





Tgt Ion: 49 Resp: 189452

Ion Ratio Lower Upper

49 100

128 47.3 24.1 72.2

130 60.7 31.4 94.3

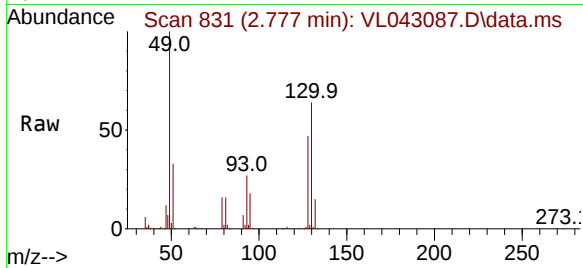

#2

Dichlorodifluoromethane

Concen: 0.072 ppbv

RT: 1.496 min Scan# 435

Delta R.T. 0.000 min

Lab File: VL043087.D




Acq: 09 Oct 2025 14:25


Tgt Ion: 85 Resp: 2308

Ion Ratio Lower Upper

85 100

87 30.9 25.8 38.6

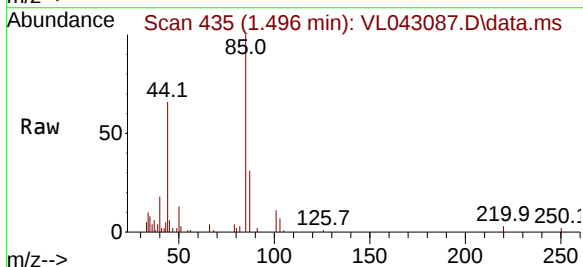



#3

Chlorodifluoromethane

Concen: 0.096 ppbv

RT: 1.473 min Scan# 428

Delta R.T. 0.000 min

Lab File: VL043087.D

Acq: 09 Oct 2025 14:25

Instrument :

MSVOA_L

ClientSampleId :





SV2

Tgt Ion: 51 Resp: 2973

Ion Ratio Lower Upper

51 100

67 14.3 15.1 22.7#

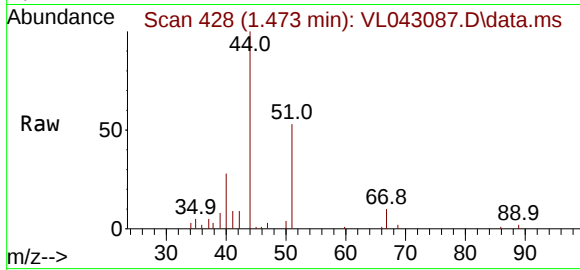

#4

Chloromethane

Concen: 0.045 ppbv

RT: 1.528 min Scan# 445

Delta R.T. 0.000 min

Lab File: VL043087.D




Acq: 09 Oct 2025 14:25


Tgt Ion: 50 Resp: 526

Ion Ratio Lower Upper

50 100

52 60.9 26.2 39.2#


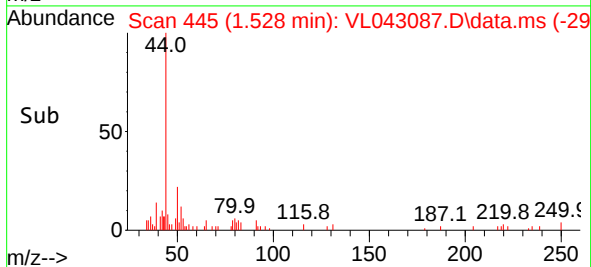

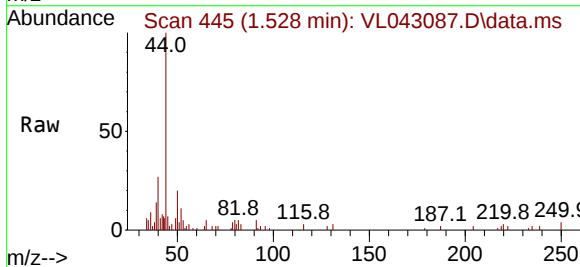




#8
 Dichlorotetrafluoroethane
 Concen: 0.088 ppbv
 RT: 1.496 min Scan# 41
 Delta R.T. -0.055 min
 Lab File: VL043087.D
 Acq: 09 Oct 2025 14:25




Instrument :
 MSVOA_L
 ClientSampleId :
 SV2


Tgt Ion: 85 Resp: 2308
 Ion Ratio Lower Upper
 85 100
 135 0.6 56.3 84.5#

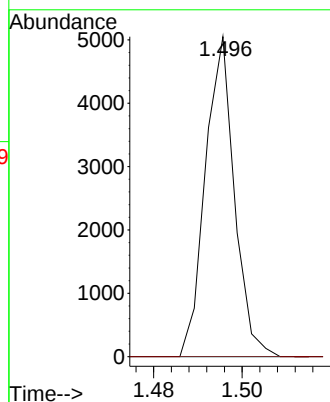

#9
 Propene
 Concen: 0.364 ppbv
 RT: 1.483 min Scan# 431
 Delta R.T. 0.003 min
 Lab File: VL043087.D
 Acq: 09 Oct 2025 14:25

Tgt Ion: 41 Resp: 4532
 Ion Ratio Lower Upper
 41 100
 42 63.6 53.3 79.9





#10

Heptane

Concen: 0.065 ppbv

RT: 4.962 min Scan# 11

Delta R.T. 0.007 min

Lab File: VL043087.D

Acq: 09 Oct 2025 14:25

Instrument :

MSVOA_L

ClientSampleId :





SV2

Tgt Ion: 43 Resp: 2005

Ion Ratio Lower Upper

43 100

57 114.7 40.3 60.5#

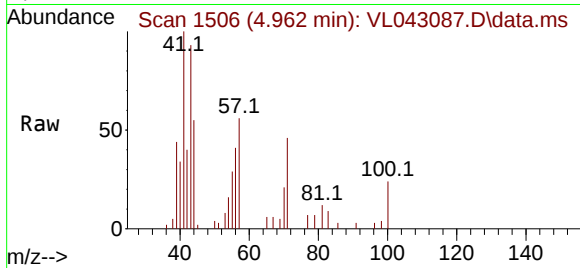

#11

Trichlorofluoromethane

Concen: 1.181 ppbv

RT: 1.871 min Scan# 551

Delta R.T. 0.000 min

Lab File: VL043087.D




Acq: 09 Oct 2025 14:25


Tgt Ion:101 Resp: 38752

Ion Ratio Lower Upper

101 100

103 65.5 51.1 76.7


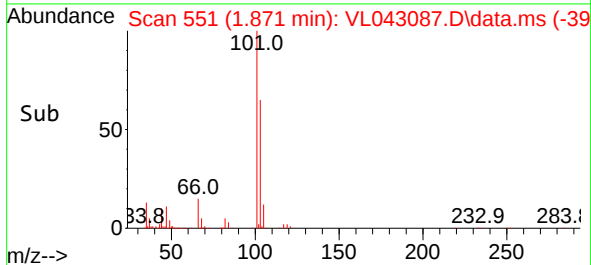

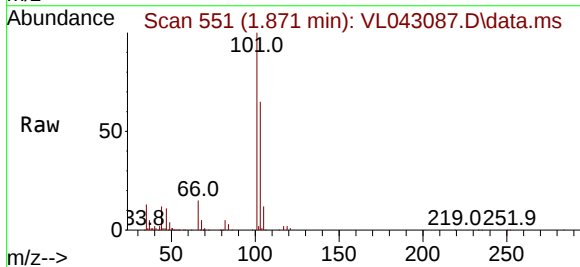




#12
 1,1,2-Trichlorotrifluoroethane
 Concen: 1.499 ppbv
 RT: 1.871 min Scan# 51
 Delta R.T. -0.259 min
 Lab File: VL043087.D
 Acq: 09 Oct 2025 14:25




Instrument :
 MSVOA_L
 ClientSampleId :
 SV2


Tgt Ion:101 Resp: 38752
 Ion Ratio Lower Upper
 101 100
 151 0.0 58.1 87.1#

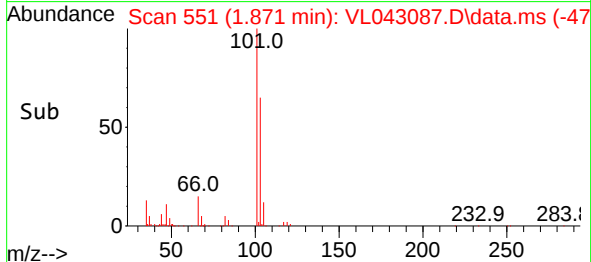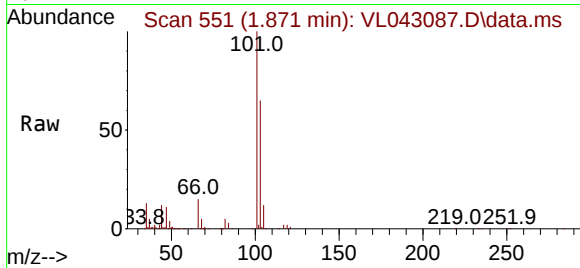

#13
 Ethanol
 Concen: 877.460 ppbv
 RT: 1.428 min Scan# 414
 Delta R.T. -0.288 min
 Lab File: VL043087.D
 Acq: 09 Oct 2025 14:25

Tgt Ion: 45 Resp: 396596
 Ion Ratio Lower Upper
 45 100
 46 32.5 17.8 71.4

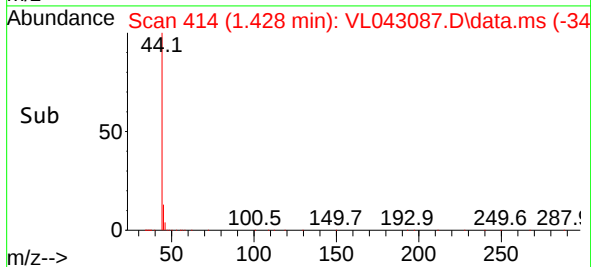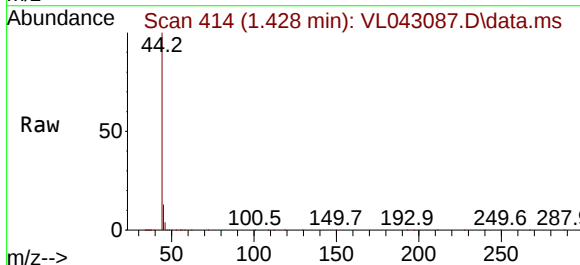



#15

Acetone

Concen: 7.073 ppbv

RT: 1.829 min Scan# 51

Delta R.T. 0.000 min

Lab File: VL043087.D

Acq: 09 Oct 2025 14:25

Instrument :

MSVOA_L

ClientSampleId :





SV2

Tgt Ion: 43 Resp: 187635

Ion Ratio Lower Upper

43 100

58 28.2 22.2 33.4

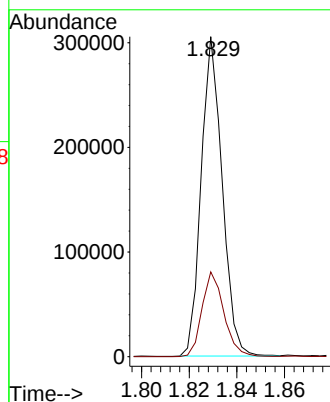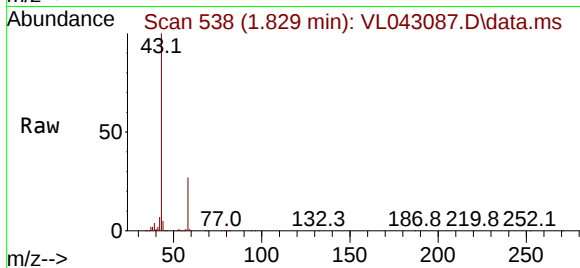

#16

1,3-Butadiene

Concen: 0.088 ppbv

RT: 1.615 min Scan# 472

Delta R.T. 0.010 min

Lab File: VL043087.D




Acq: 09 Oct 2025 14:25


Tgt Ion: 39 Resp: 964

Ion Ratio Lower Upper

39 100

54 0.0 61.4 92.2#




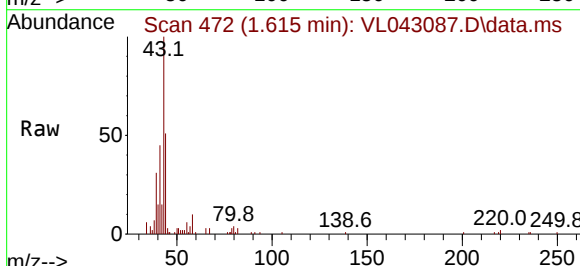




#17
tert-Butyl alcohol
Concen: 0.080 ppbv
RT: 2.039 min Scan# 601
Delta R.T. 0.007 min
Lab File: VL043087.D
Acq: 09 Oct 2025 14:25




Instrument :
MSVOA_L
ClientSampleId :
SV2


Tgt Ion: 59 Resp: 2248
Ion Ratio Lower Upper
59 100
57 23.4 8.5 12.7#

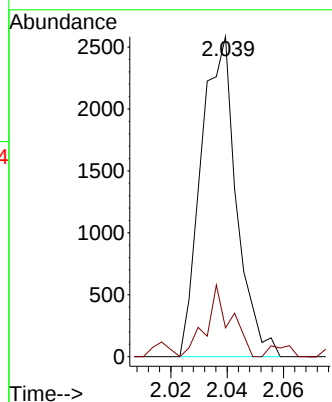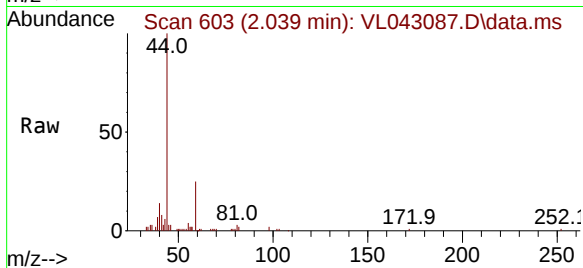

#19
Isopropyl Alcohol
Concen: 31.205 ppbv
RT: 1.428 min Scan# 414
Delta R.T. -0.450 min
Lab File: VL043087.D
Acq: 09 Oct 2025 14:25

Tgt Ion: 45 Resp: 396596
Ion Ratio Lower Upper
45 100
58 0.0 42.3 63.5#

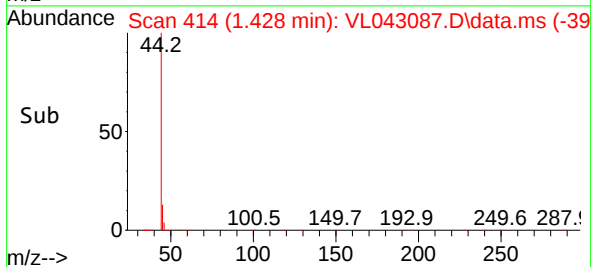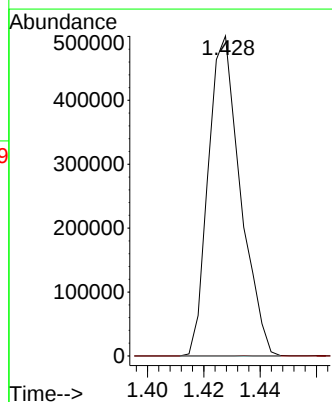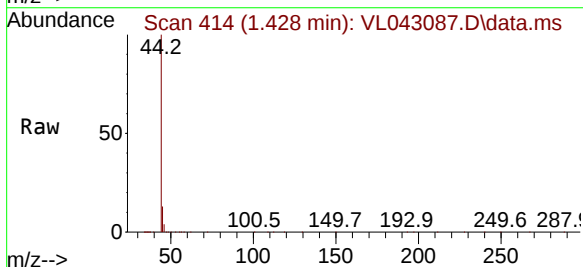







#20
Methylene Chloride
Concen: 0.309 ppbv
RT: 2.056 min Scan# 607
Delta R.T. 0.003 min
Lab File: VL043087.D
Acq: 09 Oct 2025 14:25

Instrument :
MSVOA_L
ClientSampleId :
SV2

Tgt Ion: 84 Resp: 3580




Ion	Ratio	Lower	Upper
84	100		
49	133.4	112.5	168.7
51	37.6	34.2	51.2
86	54.9	48.4	72.6




#23
Vinyl Acetate
Concen: 0.232 ppbv
RT: 2.444 min Scan# 728
Delta R.T. -0.006 min
Lab File: VL043087.D
Acq: 09 Oct 2025 14:25

Tgt Ion: 43 Resp: 1305

Ion	Ratio	Lower	Upper
43	100		
86	23.9	7.5	11.3#
42	0.0	8.4	12.6#
44	197.6	7.8	11.8#

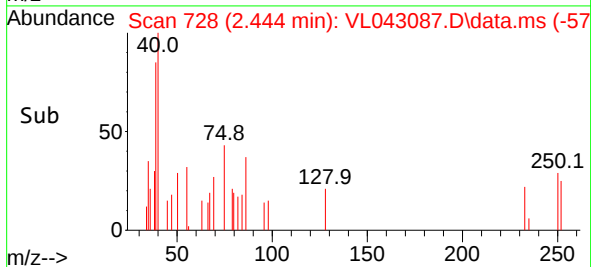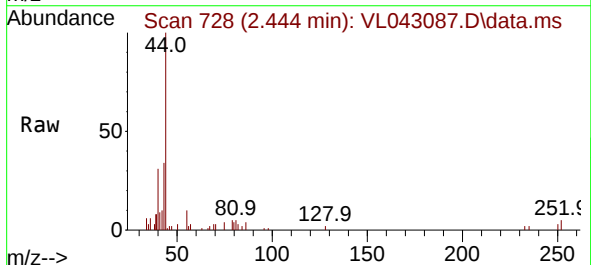



#25

Ethyl Acetate

Concen: 0.274 ppbv

RT: 2.816 min Scan# 844

Delta R.T. -0.003 min

Lab File: VL043087.D

Acq: 09 Oct 2025 14:25

Instrument :

MSVOA_L

ClientSampleId :

SV2

Tgt Ion: 43 Resp: 18245





Ion Ratio Lower Upper

43 100

45 0.9 8.3 12.5#

61 0.8 7.5 11.3#

70 2.1 6.8 10.2#

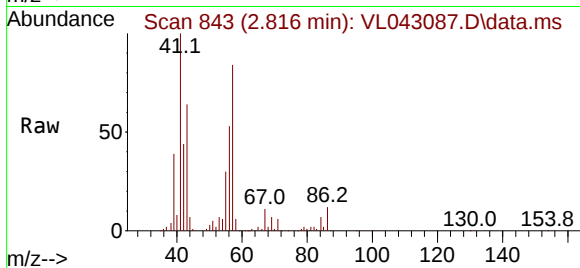

#26

Hexane

Concen: 0.947 ppbv

RT: 2.816 min Scan# 843

Delta R.T. 0.003 min

Lab File: VL043087.D

Acq: 09 Oct 2025 14:25

Tgt Ion: 57 Resp: 24236




Ion Ratio Lower Upper


57 100

41 114.3 76.1 114.1#

43 76.3 201.4 302.0#

56 66.6 44.0 66.0#

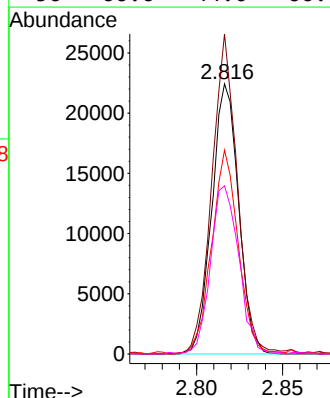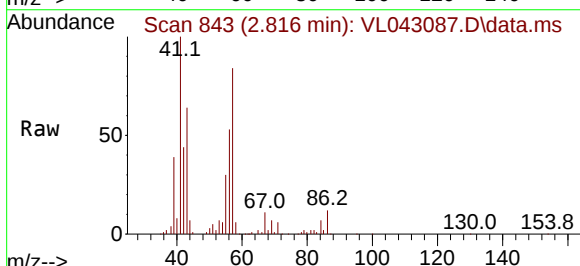



#27

Carbon Disulfide

Concen: 0.156 ppbv

RT: 2.143 min Scan# 61

Delta R.T. 0.000 min

Lab File: VL043087.D

Acq: 09 Oct 2025 14:25

Instrument :

MSVOA_L

ClientSampleId :

SV2





Tgt Ion: 76 Resp: 4724

Ion Ratio Lower Upper

76 100

44 718.2 14.0 21.0#

78 17.2 9.4 14.0#

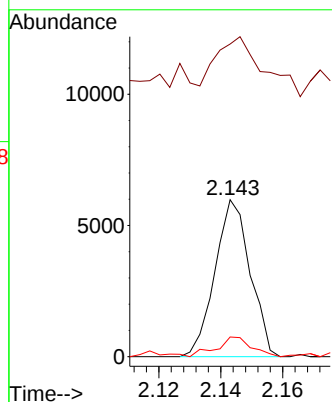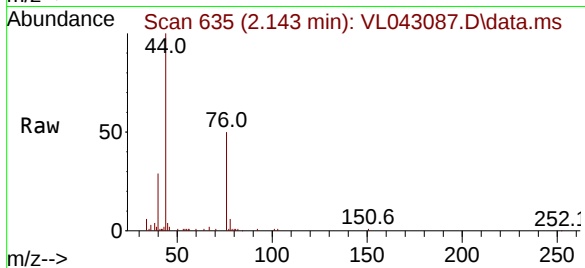

#29

Chloroform

Concen: 0.048 ppbv

RT: 2.836 min Scan# 849

Delta R.T. 0.000 min

Lab File: VL043087.D




Acq: 09 Oct 2025 14:25


Tgt Ion: 83 Resp: 2116

Ion Ratio Lower Upper

83 100

85 55.4 52.0 78.0

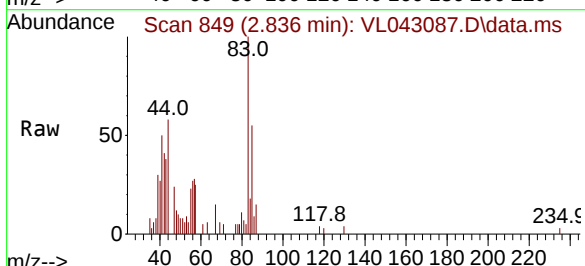



#32

1,1,1-Trichloroethane

Concen: 0.089 ppbv

RT: 3.357 min Scan# 1009

Delta R.T. 0.003 min

Lab File: VL043087.D

Acq: 09 Oct 2025 14:25

Instrument :

MSVOA_L

ClientSampleId :

SV2





Tgt Ion: 97 Resp: 3784

Ion Ratio Lower Upper

97 100

99 102.7 51.2 76.8#

61 91.6 40.1 60.1#

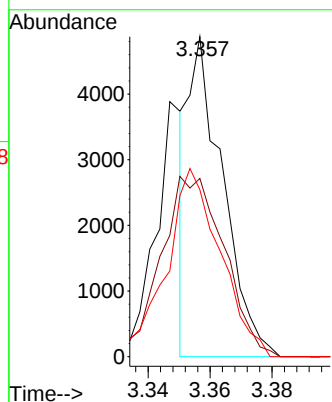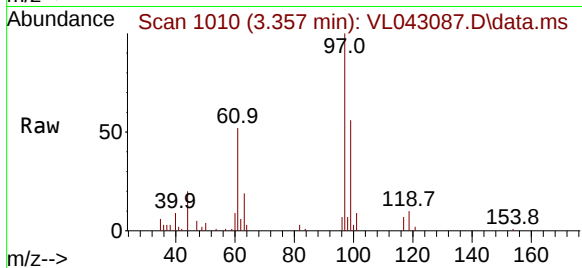

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 3.943 min Scan# 1191

Delta R.T. 0.003 min

Lab File: VL043087.D

Acq: 09 Oct 2025 14:25




Tgt Ion: 114 Resp: 494714


Ion Ratio Lower Upper

114 100

63 25.5 19.4 29.2

88 17.4 13.9 20.9



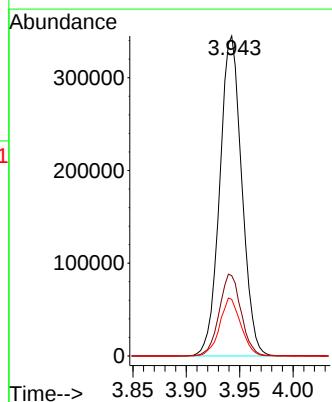
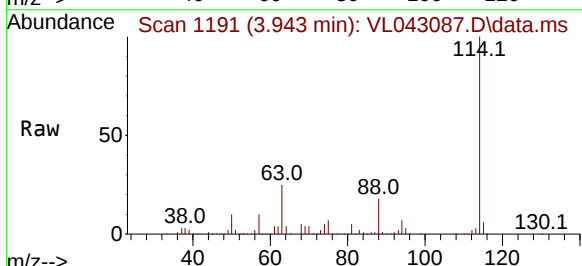




#34
2-Butanone
Concen: 0.269 ppbv
RT: 2.548 min Scan# 70
Delta R.T. 0.003 min
Lab File: VL043087.D
Acq: 09 Oct 2025 14:25




Instrument :
MSVOA_L
ClientSampleId :
SV2


Tgt Ion: 43 Resp: 9023
Ion Ratio Lower Upper
43 100
72 21.0 18.4 27.6



#36
Benzene
Concen: 0.064 ppbv
RT: 3.642 min Scan# 1098
Delta R.T. 0.003 min
Lab File: VL043087.D
Acq: 09 Oct 2025 14:25

Tgt Ion: 78 Resp: 3029
Ion Ratio Lower Upper
78 100
77 29.4 19.2 28.8#
50 11.0 14.9 22.3#

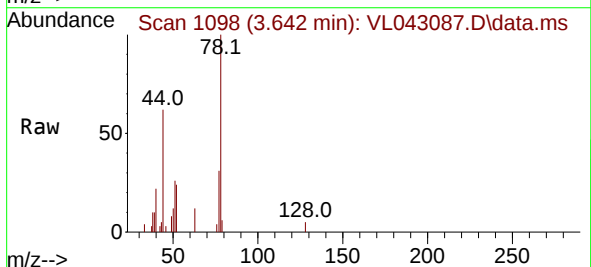



#38

Trichloroethene

Concen: 2.877 ppbv

RT: 4.528 min Scan# 1190

Delta R.T. 0.003 min

Lab File: VL043087.D

Acq: 09 Oct 2025 14:25

Instrument :

MSVOA_L

ClientSampleId :

SV2

Tgt Ion:130 Resp: 56644





Ion Ratio Lower Upper

130 100

95 111.6 86.4 129.6

132 96.1 75.7 113.5

97 67.7 56.9 85.3



#39

1,2-Dichloropropane

Concen: 7.172 ppbv

RT: 3.939 min Scan# 1190

Delta R.T. -0.353 min

Lab File: VL043087.D

Acq: 09 Oct 2025 14:25




Tgt Ion: 63 Resp: 125657


Ion Ratio Lower Upper

63 100

41 0.1 61.6 92.4#

62 17.3 58.1 87.1#









#51
2-Hexanone
Concen: 0.137 ppbv
RT: 7.422 min Scan# 21
Delta R.T. 0.010 min
Lab File: VL043087.D
Acq: 09 Oct 2025 14:25




Instrument :
MSVOA_L
ClientSampleId :
SV2


Tgt Ion: 43 Resp: 4001
Ion Ratio Lower Upper
43 100
58 44.5 39.1 58.7
98 2.4 0.5 0.7#

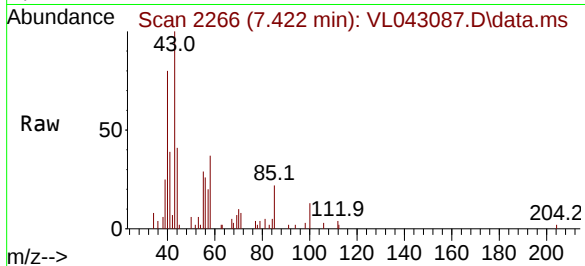

#52
Tetrachloroethene
Concen: 32.470 ppbv
RT: 8.205 min Scan# 2508
Delta R.T. 0.000 min
Lab File: VL043087.D
Acq: 09 Oct 2025 14:25

Tgt Ion: 164 Resp: 568256
Ion Ratio Lower Upper
164 100
166 126.6 101.8 152.8
129 102.8 84.5 126.7
131 100.8 80.9 121.3


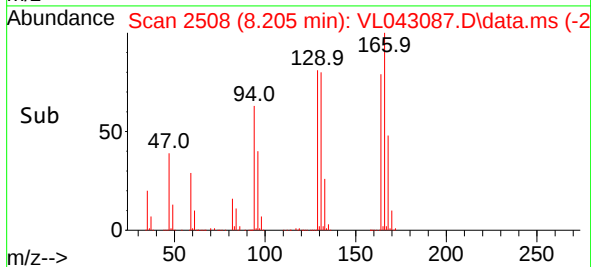

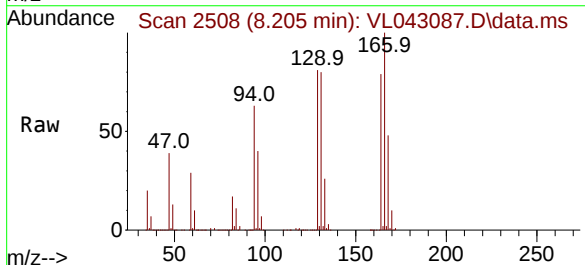




#53
Toluene
Concen: 0.335 ppbv
RT: 6.911 min Scan# 2108
Delta R.T. 0.003 min
Lab File: VL043087.D
Acq: 09 Oct 2025 14:25




Instrument :
MSVOA_L
ClientSampleId :
SV2


Tgt Ion: 91 Resp: 15976
Ion Ratio Lower Upper
91 100
92 57.1 47.8 71.6



#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 8.862 min Scan# 2711
Delta R.T. 0.000 min
Lab File: VL043087.D
Acq: 09 Oct 2025 14:25

Tgt Ion: 117 Resp: 492557
Ion Ratio Lower Upper
117 100
82 64.4 53.0 79.6
119 32.5 25.4 38.2









#60
o-Xylene
Concen: 0.142 ppbv
RT: 9.943 min Scan# 3046
Delta R.T. -0.003 min
Lab File: VL043087.D
Acq: 09 Oct 2025 14:25




Instrument :
MSVOA_L
ClientSampleId :
SV2


Tgt Ion: 91 Resp: 9090
Ion Ratio Lower Upper
91 100
106 40.2 21.9 65.5



#66
Benzyl Chloride
Concen: 0.049 ppbv
RT: 11.610 min Scan# 3560
Delta R.T. 0.007 min
Lab File: VL043087.D
Acq: 09 Oct 2025 14:25

Tgt Ion: 91 Resp: 163
Ion Ratio Lower Upper
91 100
126 0.0 14.2 21.4#
128 0.0 4.8 7.2#

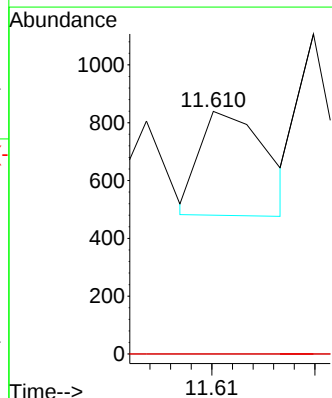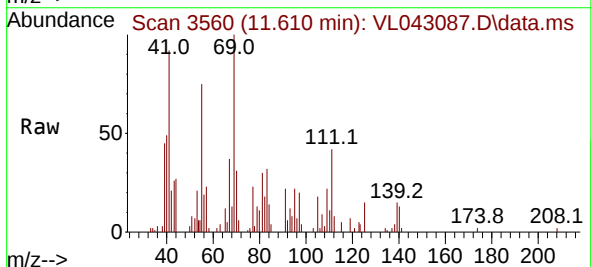



#68

1-Bromo-4-Fluorobenzene

Concen: 11.835 ppbv

RT: 10.361 min Scan# 3174

Delta R.T. 0.000 min

Lab File: VL043087.D

Acq: 09 Oct 2025 14:25

Instrument :

MSVOA_L

ClientSampleId :

SV2





Tgt Ion: 95 Resp: 419950

Ion Ratio Lower Upper

95 100

174 64.2 52.3 78.5

175 4.7 3.8 5.8

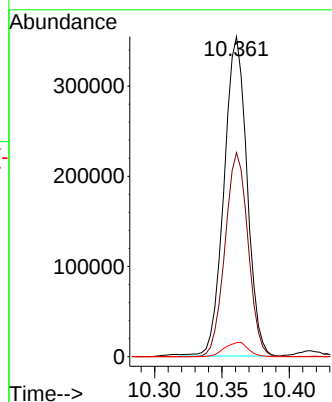

#71

2-Chlorotoluene

Concen: 0.053 ppbv

RT: 10.976 min Scan# 3364

Delta R.T. 0.091 min

Lab File: VL043087.D




Acq: 09 Oct 2025 14:25


Tgt Ion: 91 Resp: 3802

Ion Ratio Lower Upper

91 100

126 17.8 12.2 48.6





#73

1,3,5-Trimethylbenzene

Concen: 0.039 ppbv

RT: 11.189 min Scan# 3430

Delta R.T. 0.000 min

Lab File: VL043087.D

Acq: 09 Oct 2025 14:25

Instrument :

MSVOA_L

ClientSampleId :





SV2

Tgt Ion:105 Resp: 2577

Ion Ratio Lower Upper

105 100

120 35.5 37.5 56.3#



#74

1,2,4-Trimethylbenzene

Concen: 0.041 ppbv

RT: 11.523 min Scan# 3533

Delta R.T. 0.000 min

Lab File: VL043087.D

Acq: 09 Oct 2025 14:25

Tgt Ion:105 Resp: 3042




Ion Ratio Lower Upper


105 100

120 37.5 39.7 59.5#

91 7.8 56.5 84.7#

77 16.2 19.9 29.9#



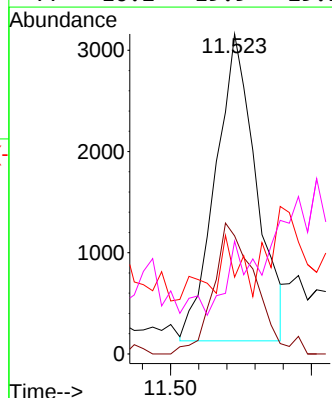



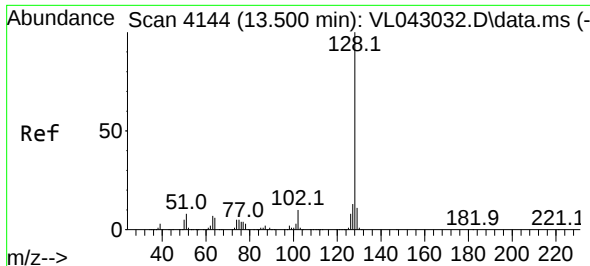

#79
Naphthalene
Concen: 0.238 ppbv
RT: 13.497 min Scan# 4144
Delta R.T. -0.003 min
Lab File: VL043087.D
Acq: 09 Oct 2025 14:25

Instrument :
MSVOA_L
ClientSampleId :
SV2

Tgt Ion:128 Resp: 238
Ion Ratio Lower Upper
128 100
127 0.0 10.6 16.0#
129 0.0 8.8 13.2#

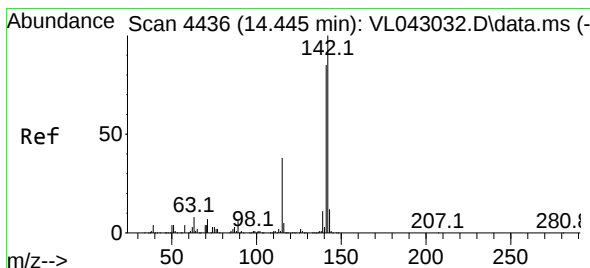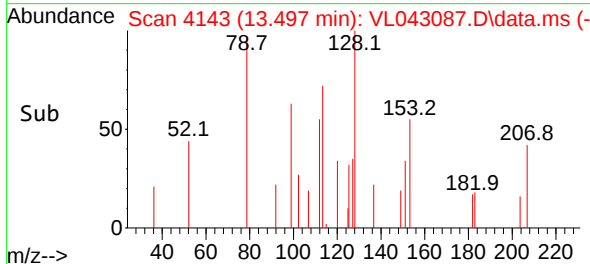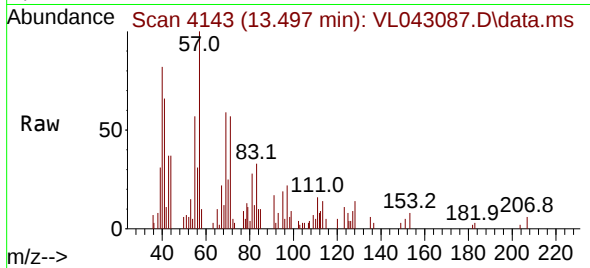

#80
Naphthalene,2-methyl-
Concen: 0.681 ppbv
RT: 14.458 min Scan# 4440
Delta R.T. 0.013 min
Lab File: VL043087.D
Acq: 09 Oct 2025 14:25

Tgt Ion:142 Resp: 595
Ion Ratio Lower Upper
142 100
141 79.5 66.6 100.0
115 76.6 30.1 45.1#

