

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101025\
Data File : BF143921.D
Acq On : 10 Oct 2025 13:24
Operator : RC/JU
Sample : PB170055BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170055BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143921.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.222	3	5	12	rVB	87142	110796	2.26%	0.369%
2	5.134	490	500	508	rBV	44606	78328	1.60%	0.261%
3	5.504	557	563	569	rBV	2764732	4049069	82.60%	13.501%
4	6.504	726	733	739	rBV	2716642	4115650	83.95%	13.723%
5	6.881	792	797	802	rBV	676207	836709	17.07%	2.790%
6	7.440	885	892	898	rBV	1827180	2661511	54.29%	8.874%
7	8.163	1009	1015	1022	rBV	838686	1107641	22.59%	3.693%
8	9.239	1191	1198	1216	rBV	3098045	4427277	90.31%	14.762%
9	9.922	1308	1314	1329	rBV	976175	1258495	25.67%	4.196%
10	10.716	1442	1449	1468	rBV	2114907	3018629	61.58%	10.065%
11	11.410	1562	1567	1574	rBV	996496	1315504	26.83%	4.386%
12	13.004	1829	1838	1844	rBV	3478908	4902311	100.00%	16.346%
13	14.057	2009	2017	2031	rBV	762209	1069108	21.81%	3.565%
14	15.539	2263	2269	2287	rVB	453707	788985	16.09%	2.631%
15	17.262	2553	2562	2585	rVB5	48045	251416	5.13%	0.838%




Sum of corrected areas: 29991429

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101025\
Data File : BF143921.D
Acq On : 10 Oct 2025 13:24
Operator : RC/JU
Sample : PB170055BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170055BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

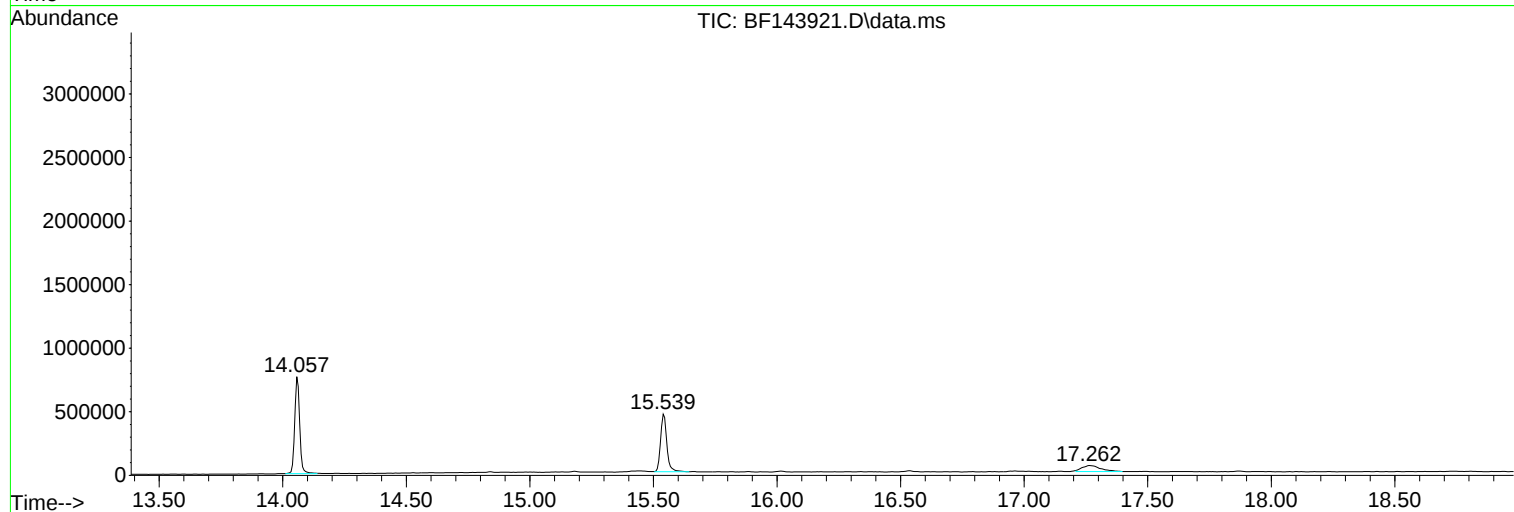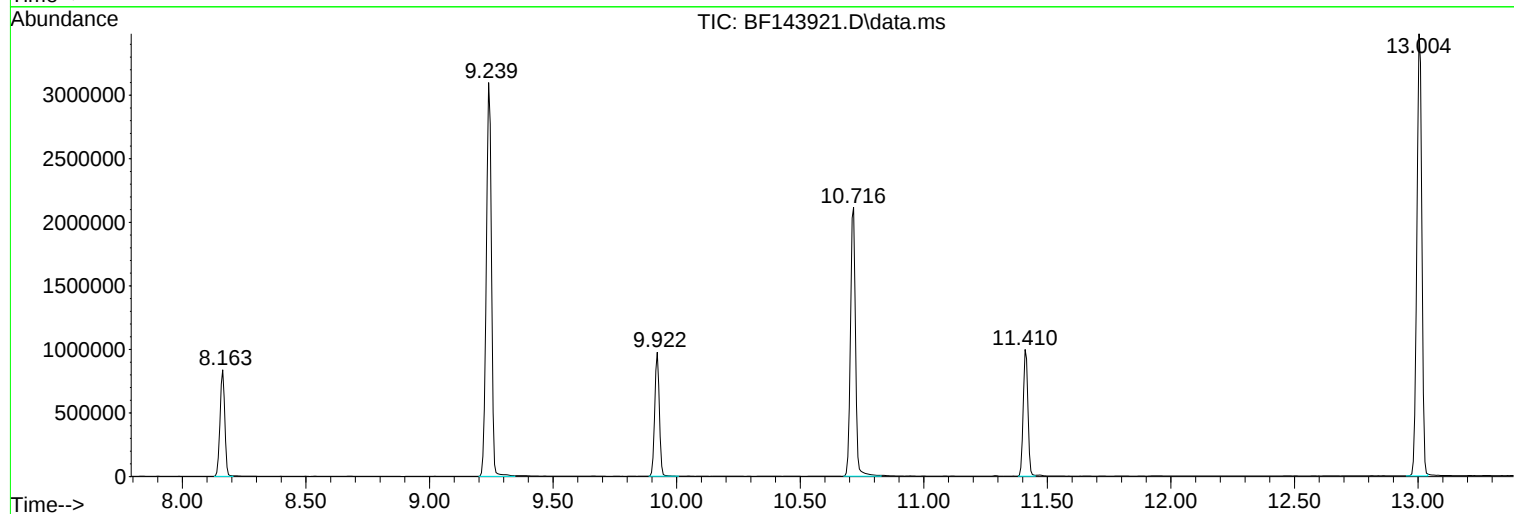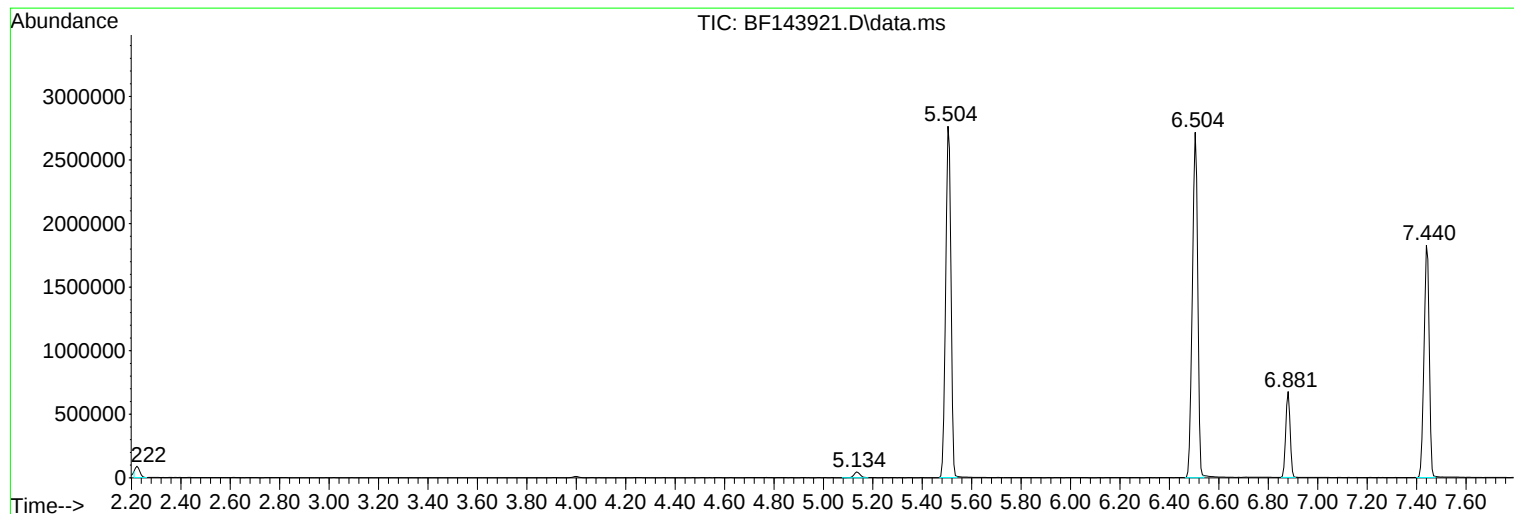

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101025\
Data File : BF143921.D
Acq On : 10 Oct 2025 13:24
Operator : RC/JU
Sample : PB170055BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170055BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101025\
Data File : BF143921.D
Acq On : 10 Oct 2025 13:24
Operator : RC/JU
Sample : PB170055BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170055BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------