


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101425\
Data File : BG064496.D
Acq On : 14 Oct 2025 10:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 02 16:40:42 2025

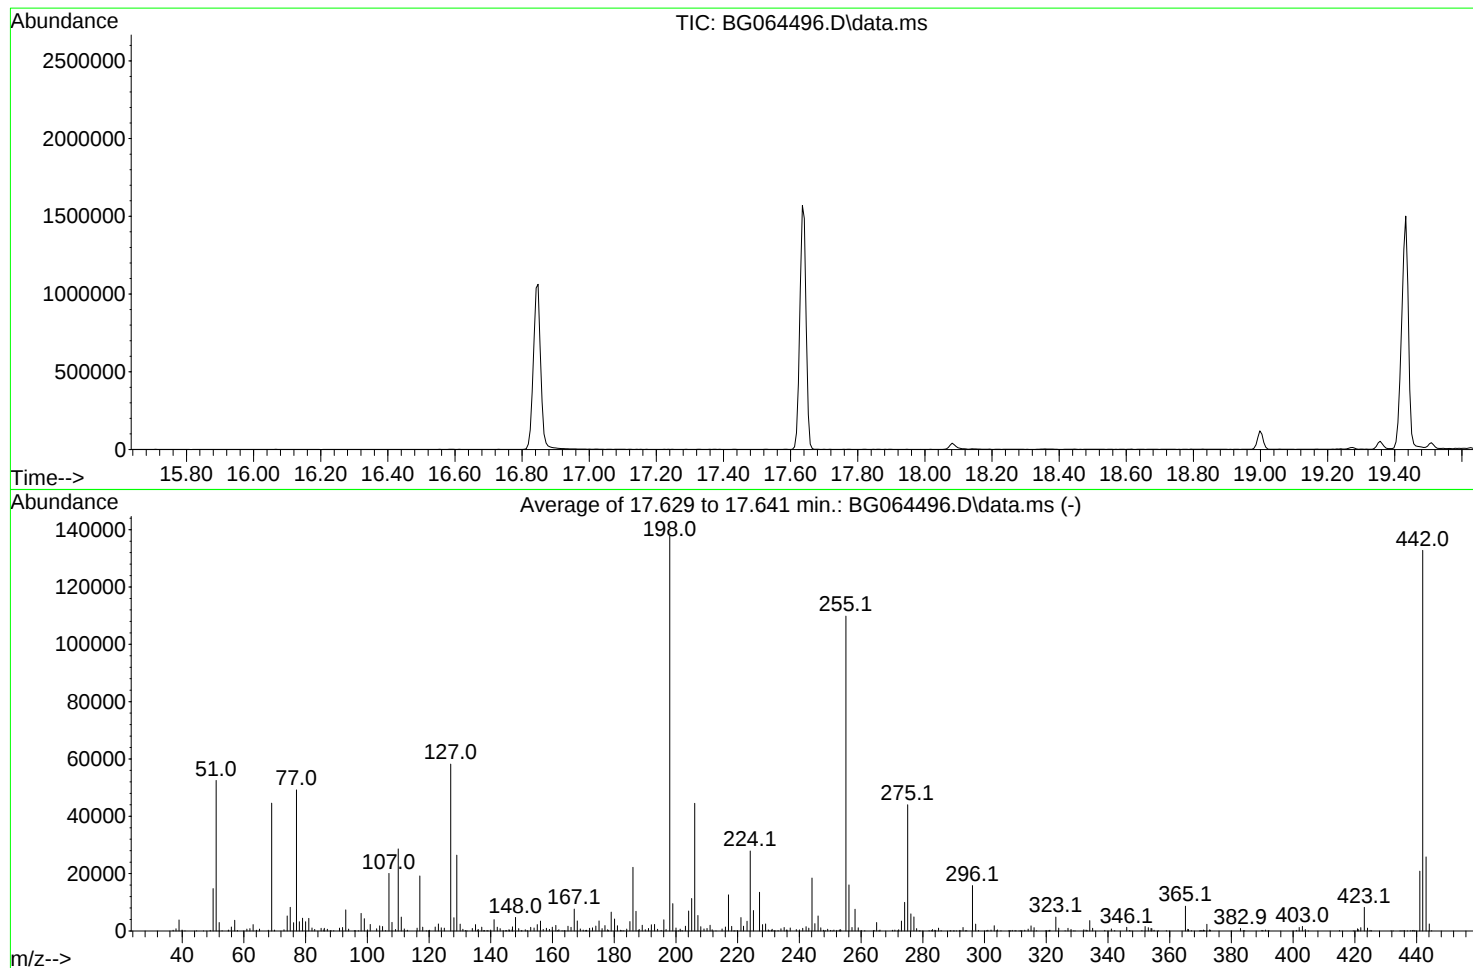




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.6	261	PASS
69	69	100	100	100.0	44592	PASS
70	69	0.00	2	0.7	302	PASS
197	198	0.00	2	0.3	457	PASS
198	198	100	100	100.0	137768	PASS
199	198	5	9	6.9	9513	PASS
365	198	1	100	6.3	8633	PASS
441	443	0.01	150	80.8	20877	PASS
442	442	100	100	100.0	132784	PASS
443	442	15	24	19.4	25823	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101425\
Data File : BG064496.D
Acq On : 14 Oct 2025 10:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 14 11:46:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 02 16:40:42 2025
Response via : Initial Calibration

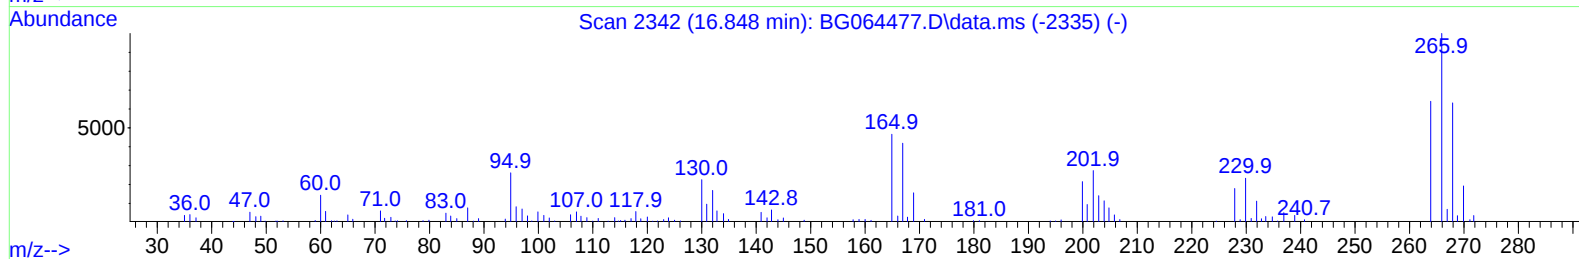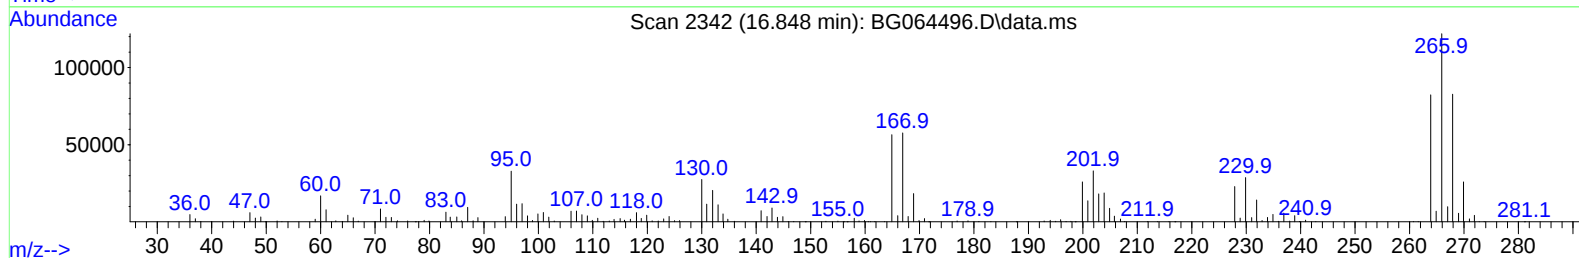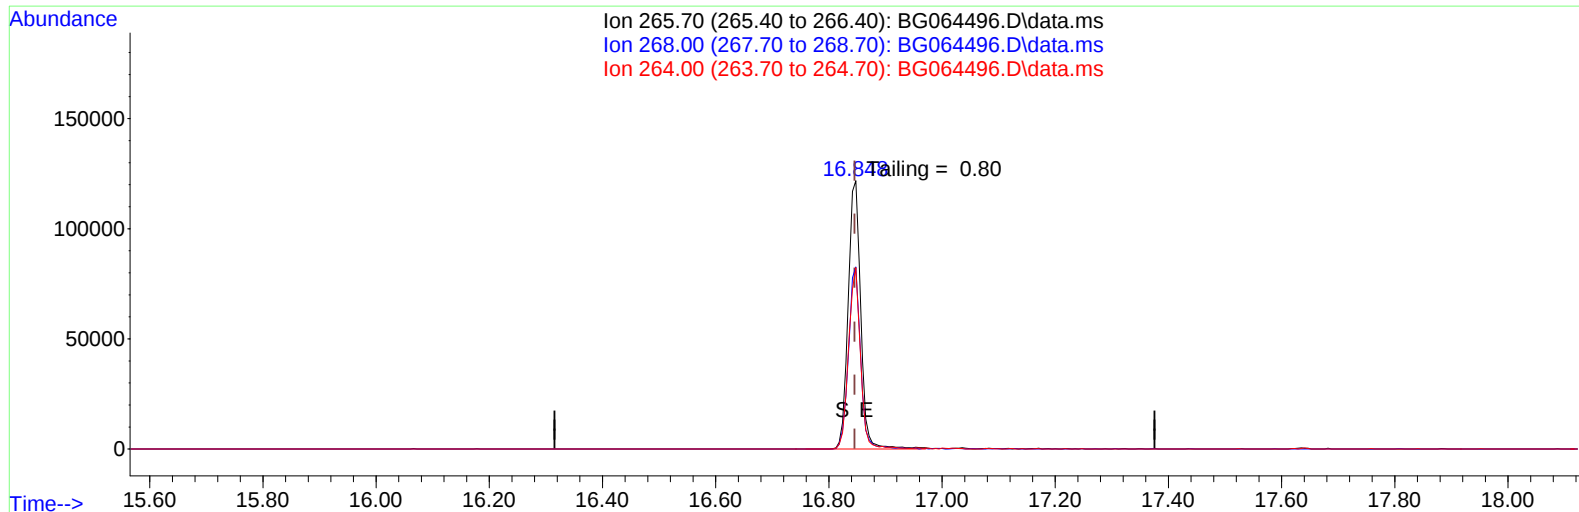

TIC: BG064496.D\data.ms

(70) Pentachlorophenol (C)

16.848min (+ 0.002) 22066.93 ng




response 187984

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	67.84
264.00	64.00	67.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101425\
Data File : BG064496.D
Acq On : 14 Oct 2025 10:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 14 11:46:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 02 16:40:42 2025
Response via : Initial Calibration

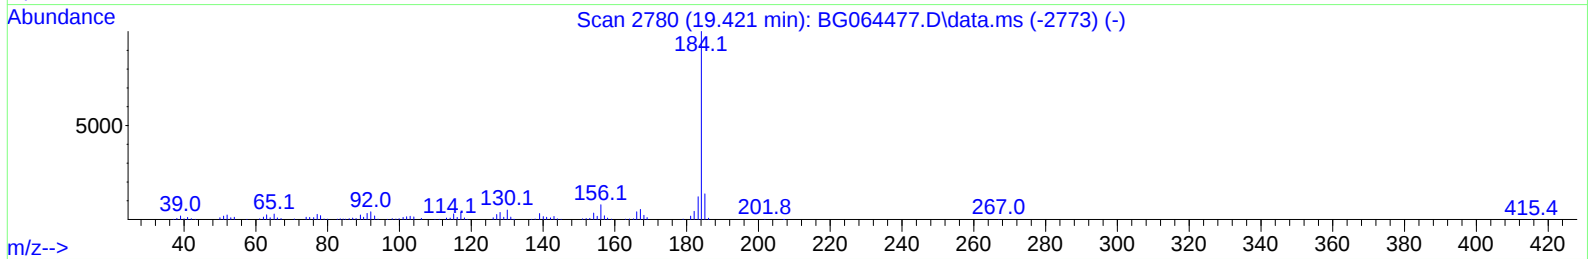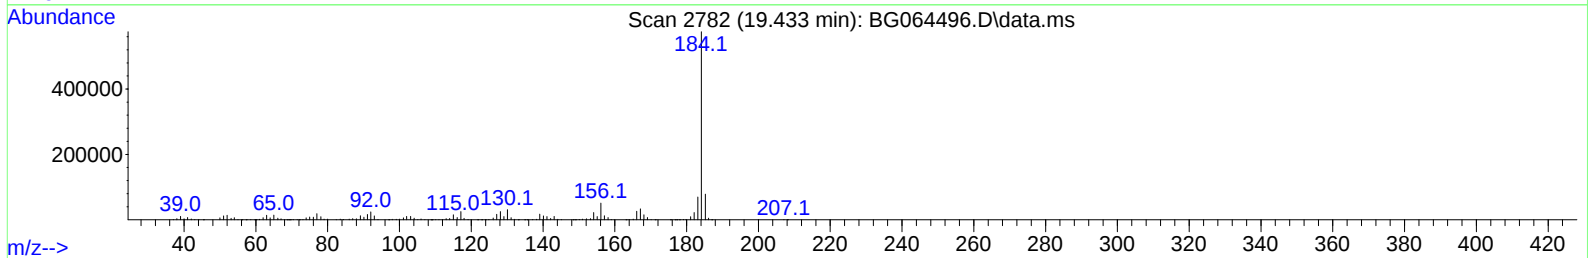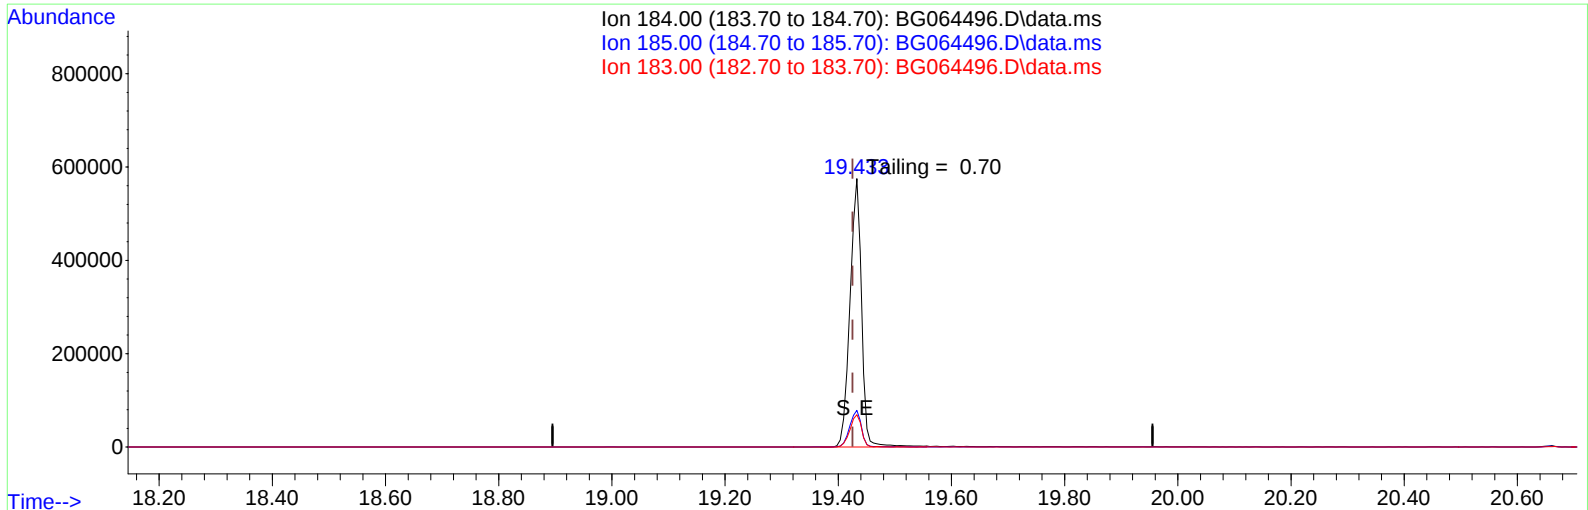

TIC: BG064496.D\data.ms

(77) Benzidine

19.433min (+ 0.008) 0.00 ng

response 816435

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.68
183.00	12.20	12.07
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/14/2025	BNA_G	<u>BG064496.D</u>
Compound Name	Response	Retention Time
DDT	574696	20.661
DDD	4604	20.22
DDE	55	19.803
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4659	579355	0.80

Instrument :
BNA_G
ClientSampleId :
DFTPP