
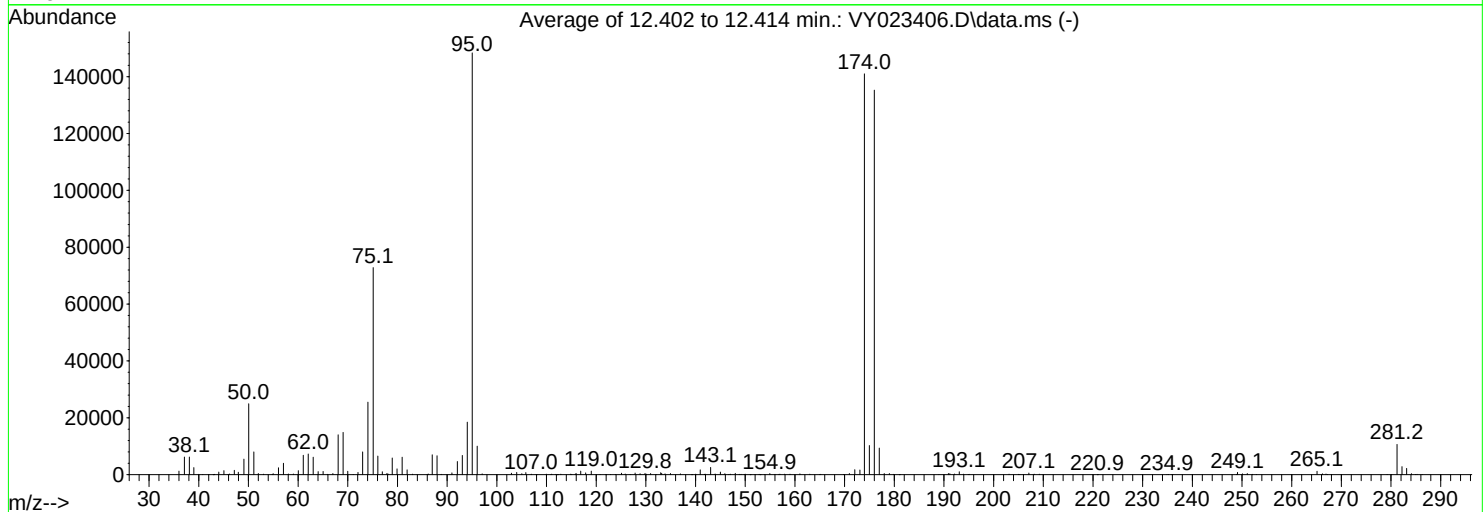


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100925\
Data File : VY023406.D
Acq On : 09 Oct 2025 08:16
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Title : SW846 8260
Last Update : Wed Oct 08 05:12:50 2025

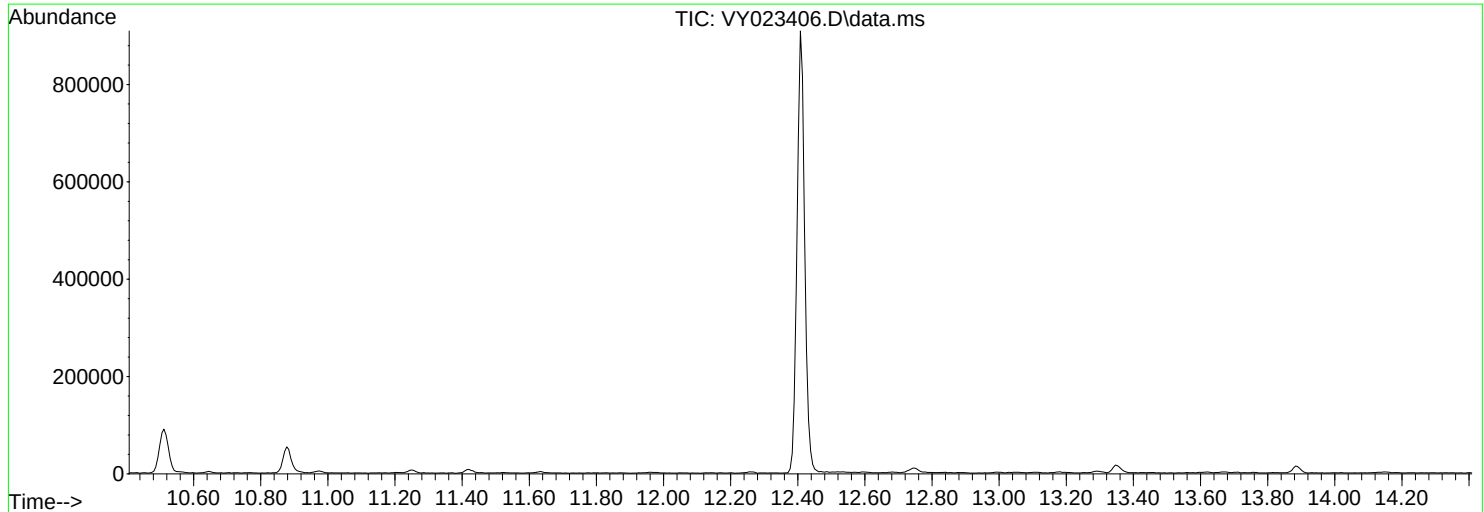

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	24923	PASS
75	95	30	60	49.1	72837	PASS
95	95	100	100	100.0	148373	PASS
96	95	5	9	6.8	10026	PASS
173	174	0.00	2	1.1	1617	PASS
174	95	50	100	95.0	141019	PASS
175	174	5	9	7.3	10229	PASS
176	174	95	101	95.9	135248	PASS
177	176	5	9	6.9	9326	PASS