
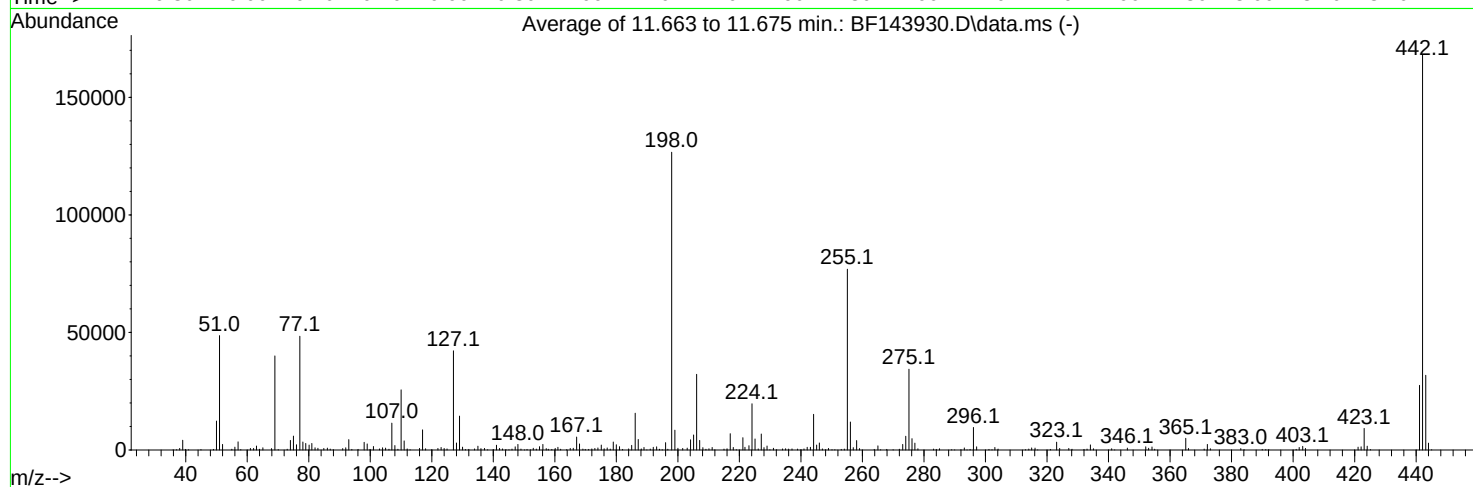


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101325\
Data File : BF143930.D
Acq On : 13 Oct 2025 12:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 06 15:29:47 2025

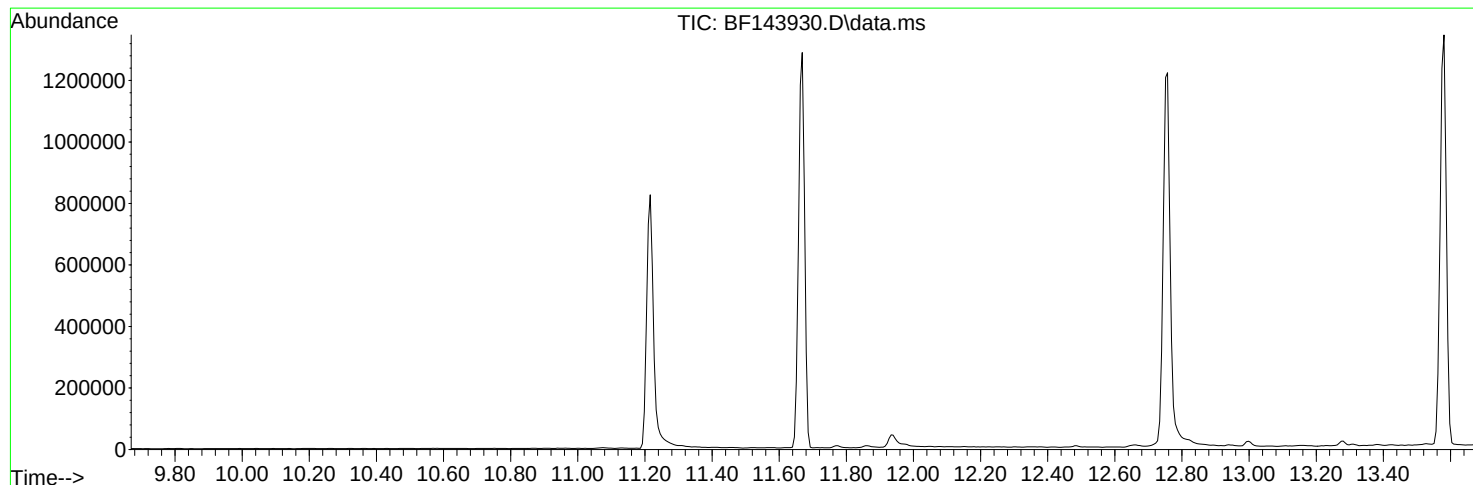




AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.4	574	PASS
69	69	100	100	100.0	40000	PASS
70	69	0.00	2	0.4	167	PASS
197	198	0.00	2	0.2	296	PASS
198	198	100	100	100.0	126685	PASS
199	198	5	9	6.6	8383	PASS
365	198	1	100	3.9	4916	PASS
441	443	0.01	150	86.5	27453	PASS
442	442	100	100	100.0	167979	PASS
443	442	15	24	18.9	31733	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101325\
Data File : BF143930.D
Acq On : 13 Oct 2025 12:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 13 15:22:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

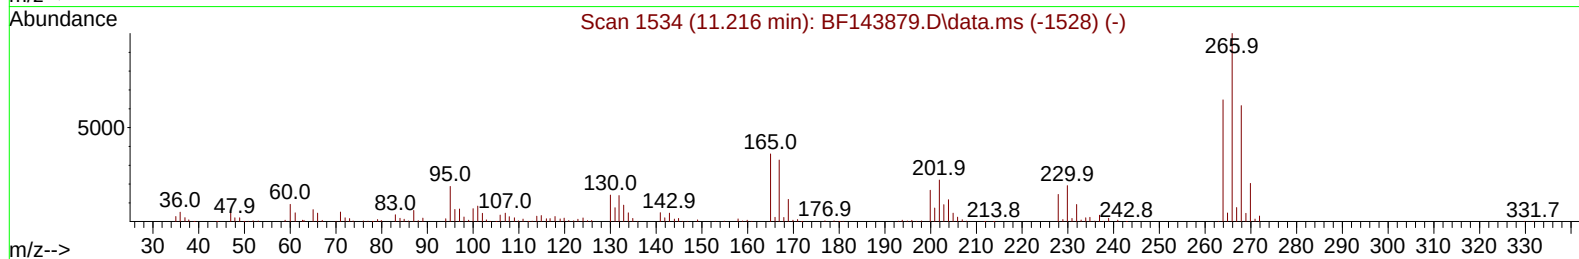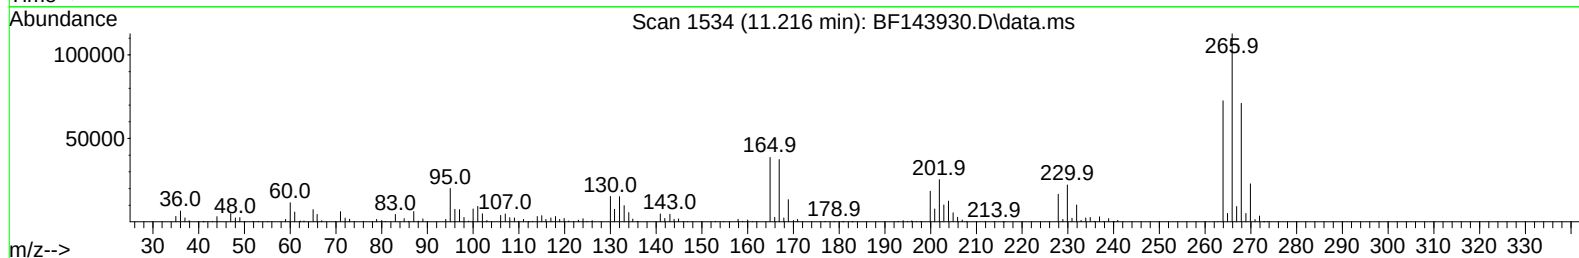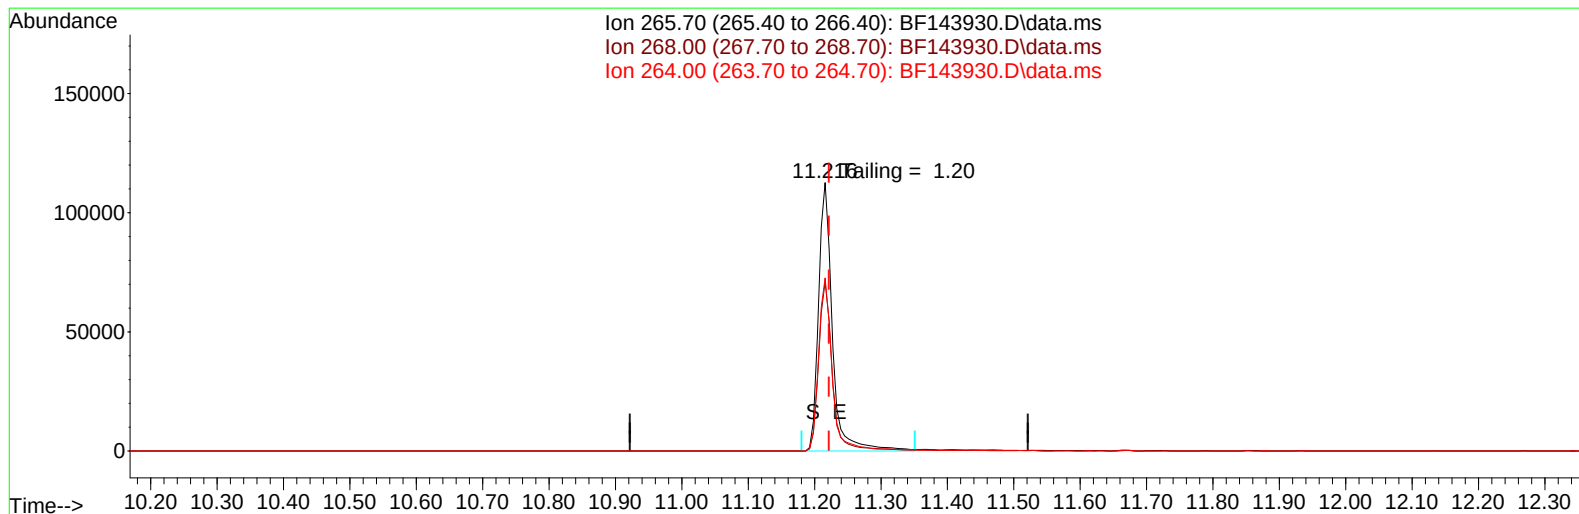

TIC: BF143930.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.006) 38478.14 ng




response 163993

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	63.02
264.00	64.70	64.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101325\
Data File : BF143930.D
Acq On : 13 Oct 2025 12:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 13 15:22:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

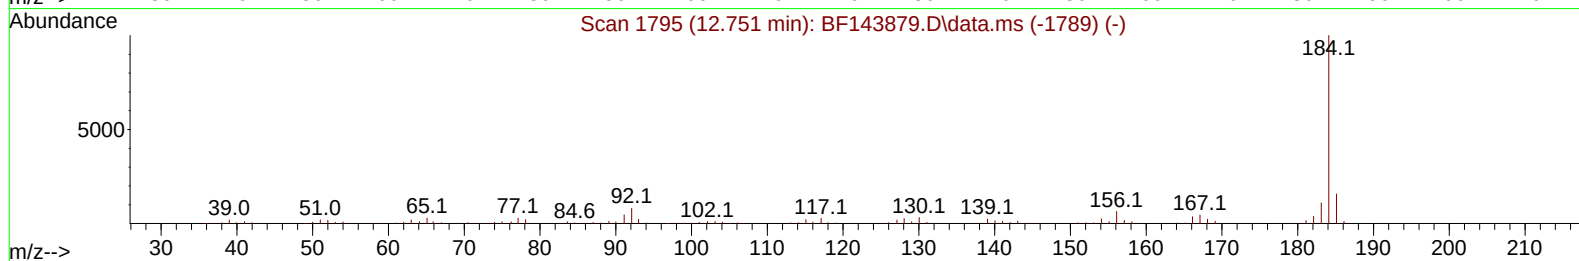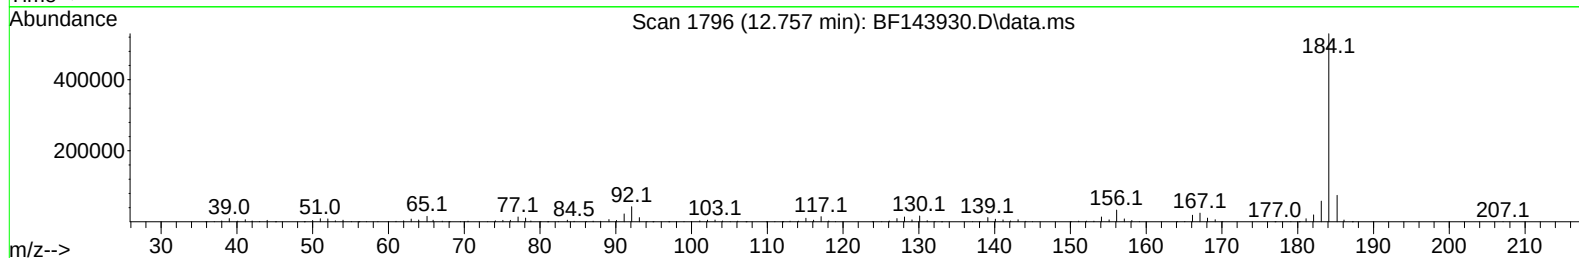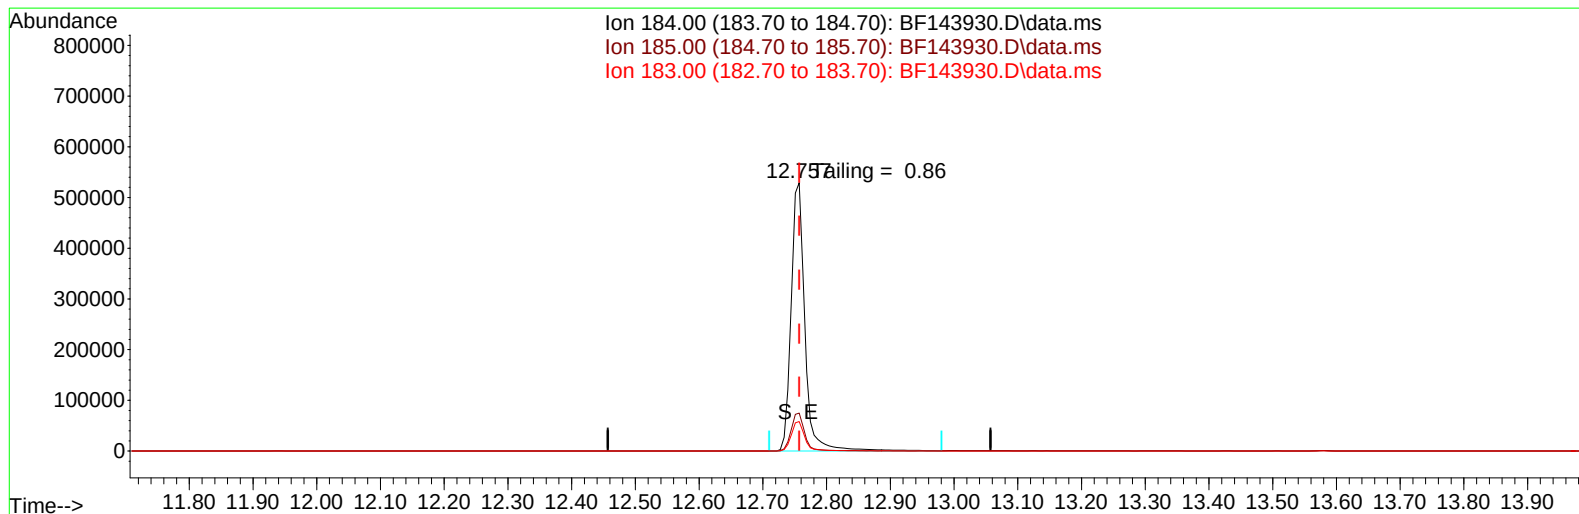

TIC: BF143930.D\data.ms

(77) Benzidine

12.757min (-0.000) 0.00 ng

response 793737

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.12
183.00	11.00	10.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/13/2025	BNA_F	<u>BF143930.D</u>
Compound Name	Response	Retention Time
DDT	361655	13.58
DDD	6906	13.275
DDE	1366	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8272	369927	2.24

Instrument :
BNA_F
ClientSampleId :
DFTPP