


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101325\
Data File : BN038082.D
Acq On : 14 Oct 2025 00:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 24 11:00:01 2025

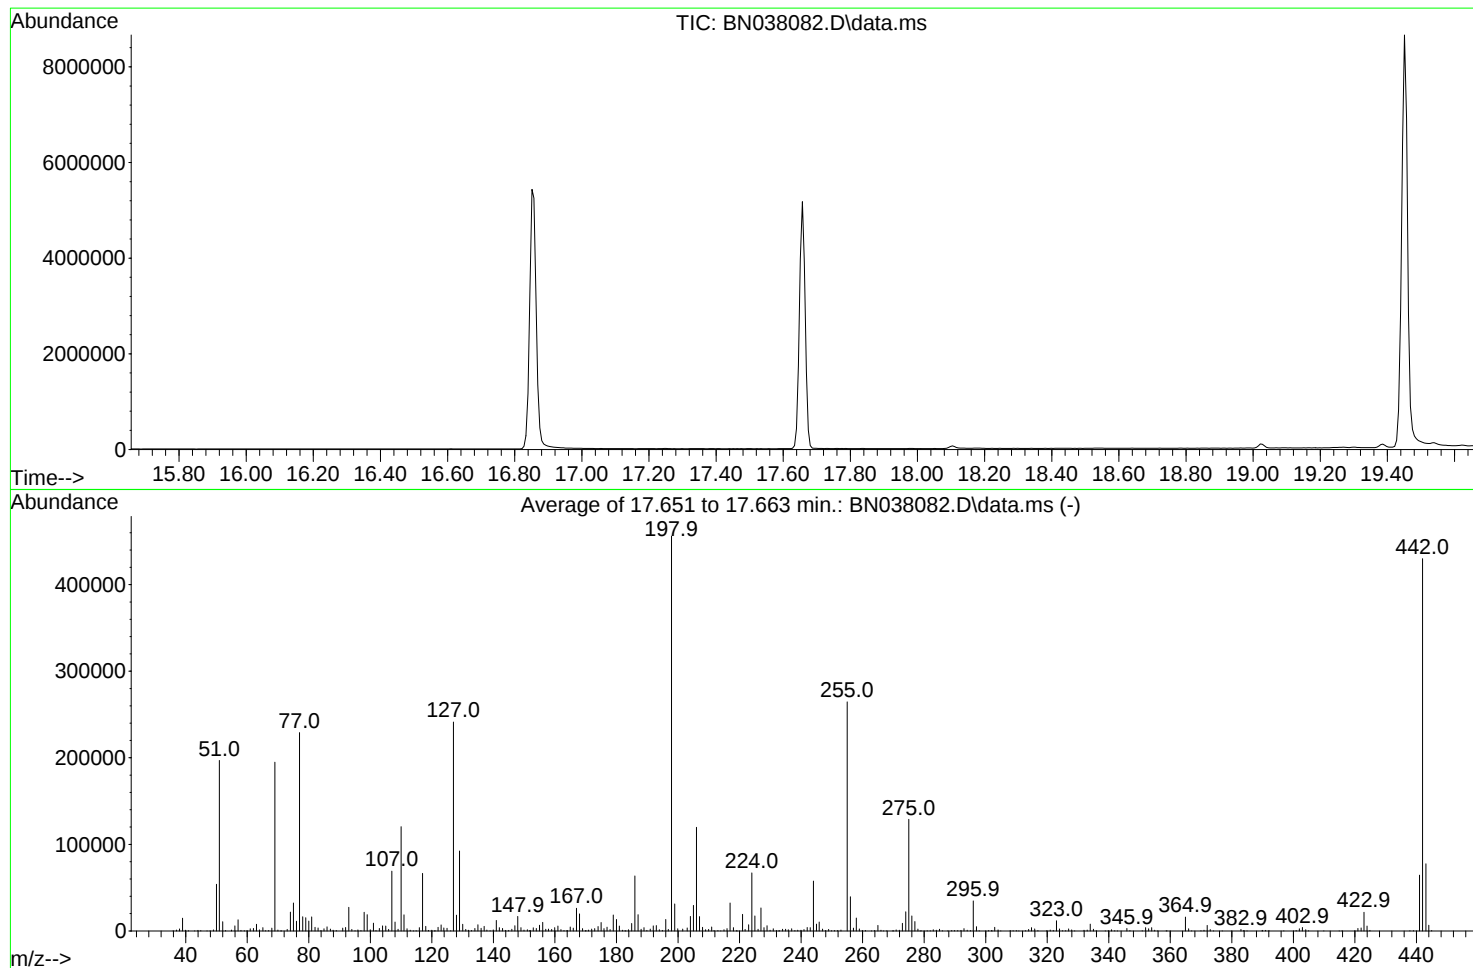




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	3299	PASS
69	69	100	100	100.0	194987	PASS
70	69	0.00	2	0.5	982	PASS
197	198	0.00	2	0.4	1825	PASS
198	198	100	100	100.0	456107	PASS
199	198	5	9	6.8	31077	PASS
365	198	1	100	3.5	16041	PASS
441	443	0.01	150	83.1	64464	PASS
442	442	100	100	100.0	430080	PASS
443	442	15	24	18.0	77528	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101325\
Data File : BN038082.D
Acq On : 14 Oct 2025 00:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 14 04:05:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 13 13:56:00 2025
Response via : Initial Calibration

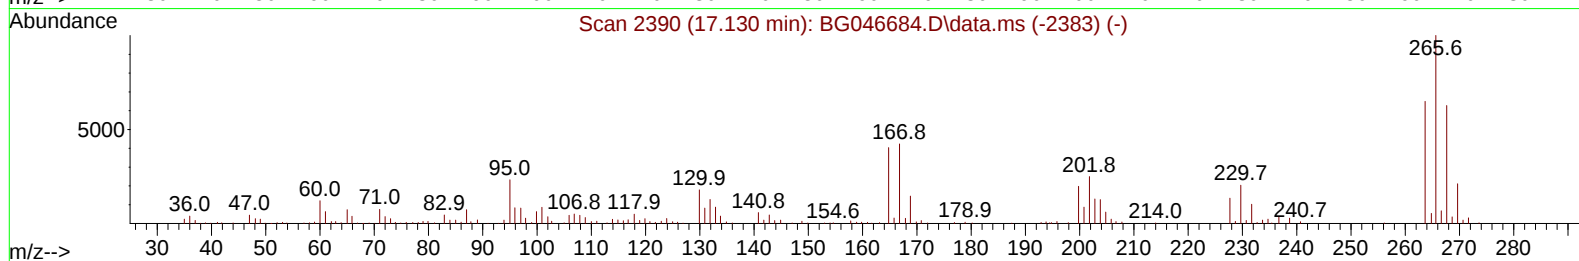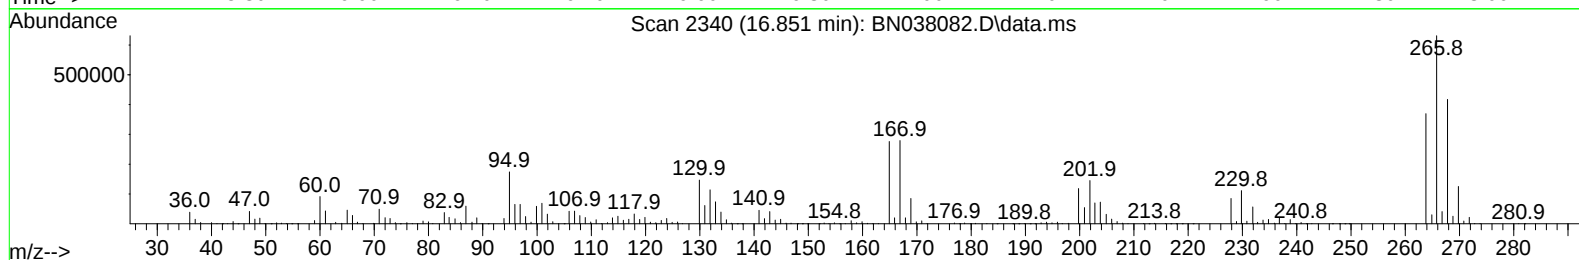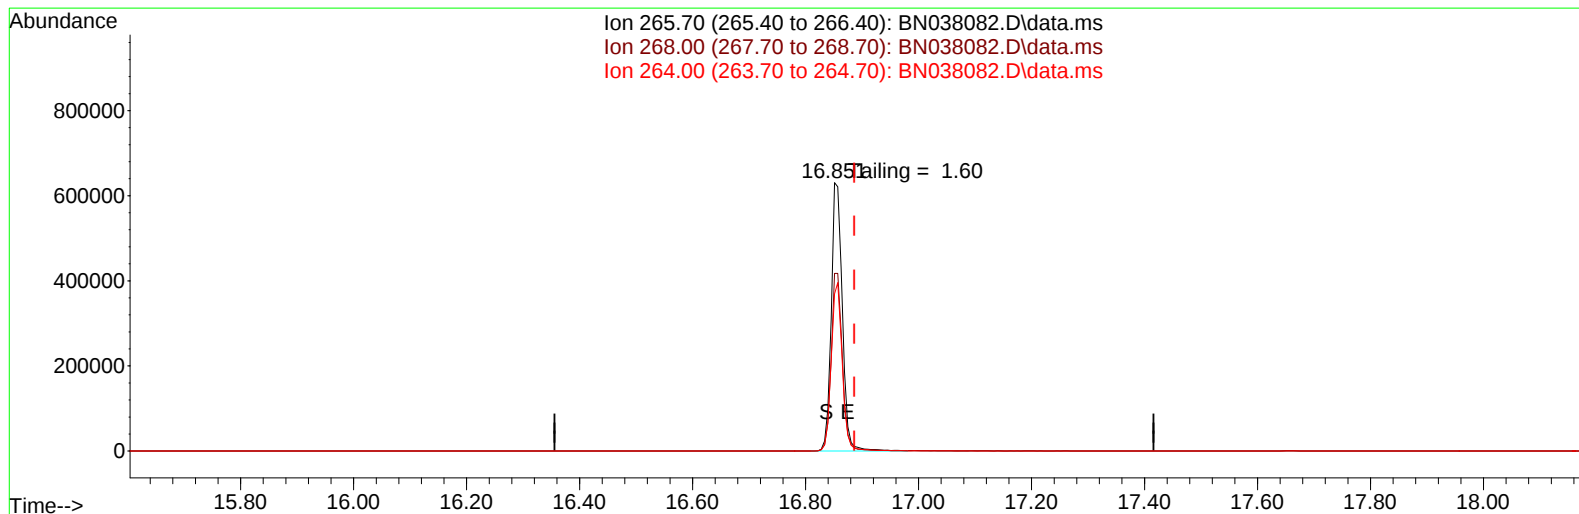

TIC: BN038082.D\data.ms

(70) Pentachlorophenol (C)

16.851min (-0.035) 0.00 ng




response 862228

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.16
264.00	61.60	58.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101325\
Data File : BN038082.D
Acq On : 14 Oct 2025 00:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 14 04:05:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 13 13:56:00 2025
Response via : Initial Calibration

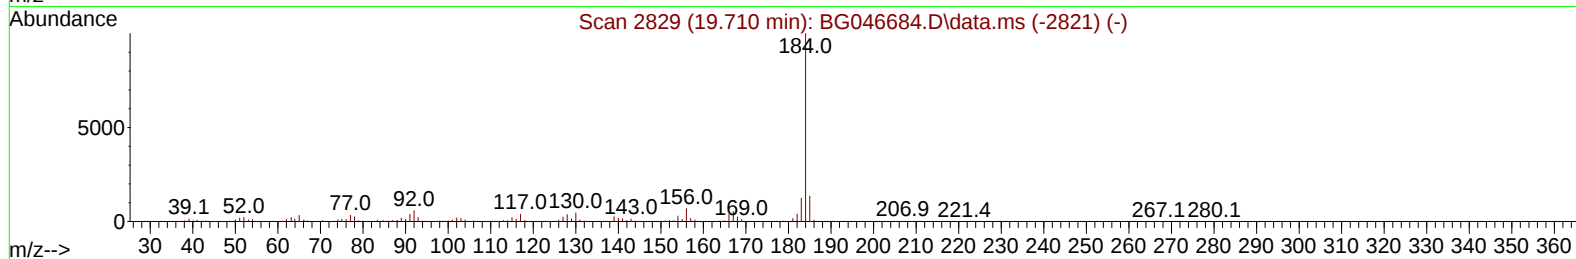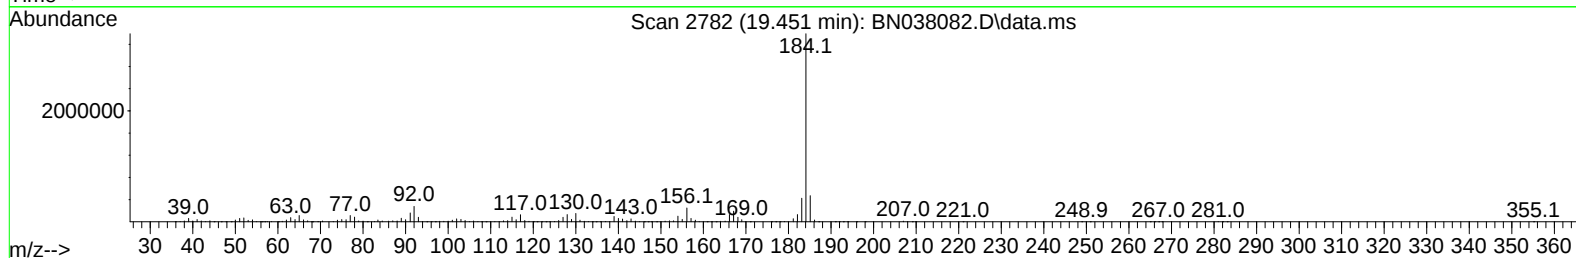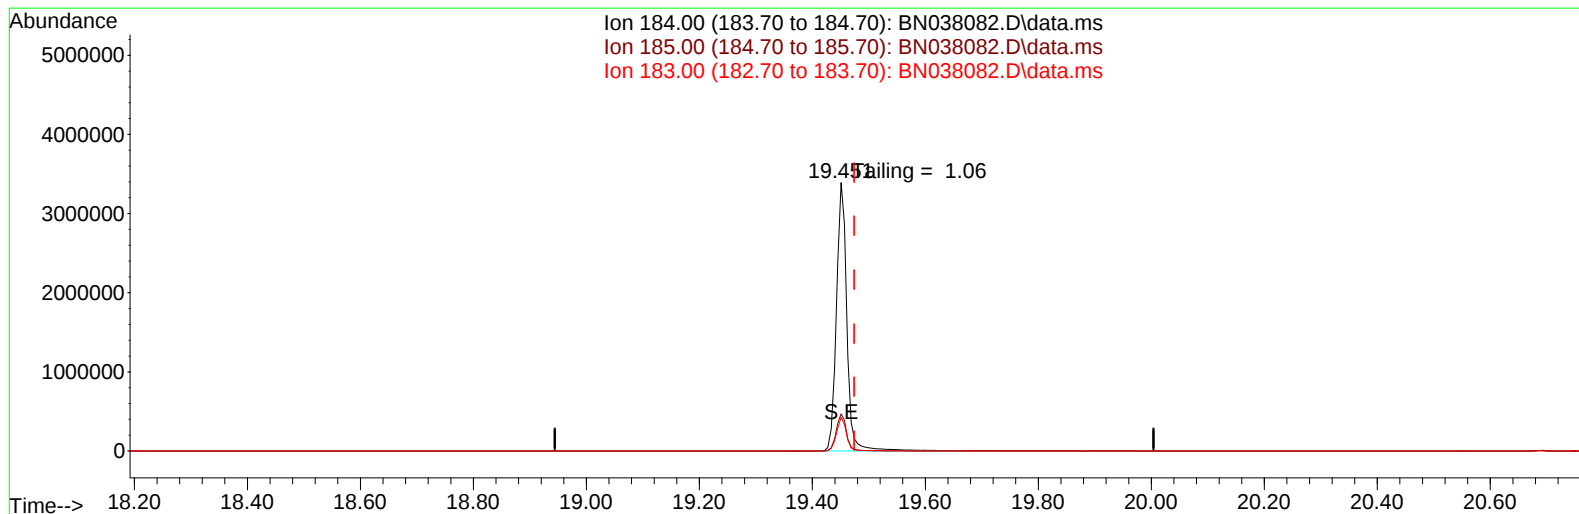

TIC: BN038082.D\data.ms

(77) Benzidine

19.451min (-0.023) 0.00 ng

response 4359890

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.86
183.00	13.20	12.55
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/13/2025	BNA_N	<u>BN038082.D</u>
Compound Name	Response	Retention Time
DDT	1777716	20.692
DDD	13147	20.245
DDE	608	19.745
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13755	1791471	0.77

Instrument :
BNA_N
ClientSampleId :
DFTPP