
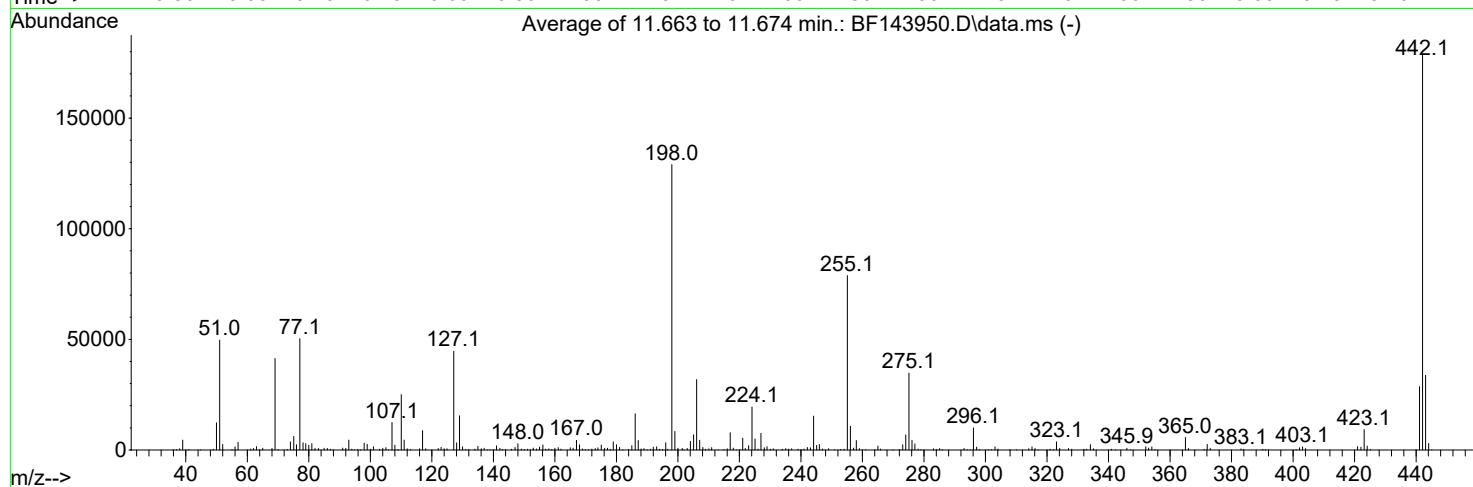


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101525\
Data File : BF143950.D
Acq On : 15 Oct 2025 14:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 06 15:29:47 2025

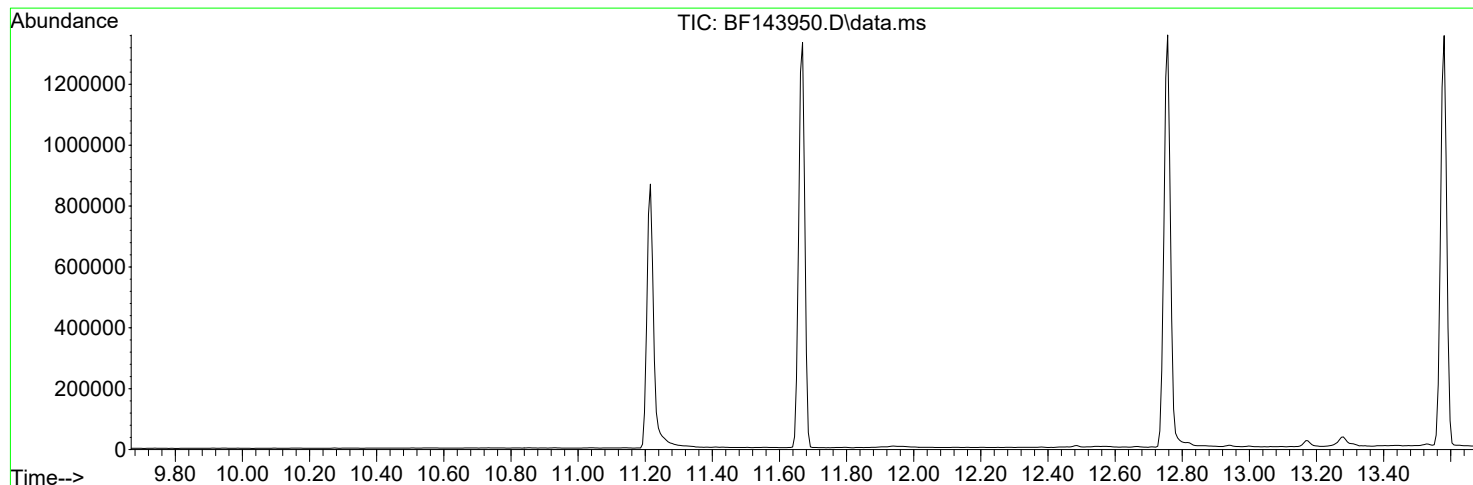

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1603

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	727	PASS
69	69	100	100	100.0	41379	PASS
70	69	0.00	2	0.5	188	PASS
197	198	0.00	2	0.3	335	PASS
198	198	100	100	100.0	129005	PASS
199	198	5	9	6.5	8431	PASS
365	198	1	100	4.4	5634	PASS
441	443	0.01	150	84.8	28643	PASS
442	442	100	100	100.0	178432	PASS
443	442	15	24	18.9	33763	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/15/2025	BNA_F	BF143950.D
Compound Name	Response	Retention Time
DDT	356237	13.58
DDD	6346	13.28
DDE	1775	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8121	364358	2.23

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101525\
Data File : BF143950.D
Acq On : 15 Oct 2025 14:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 16 18:41:55 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

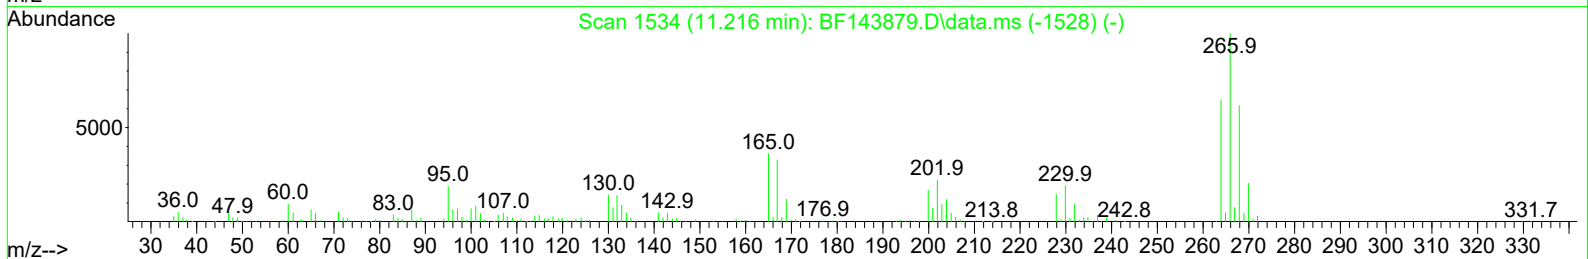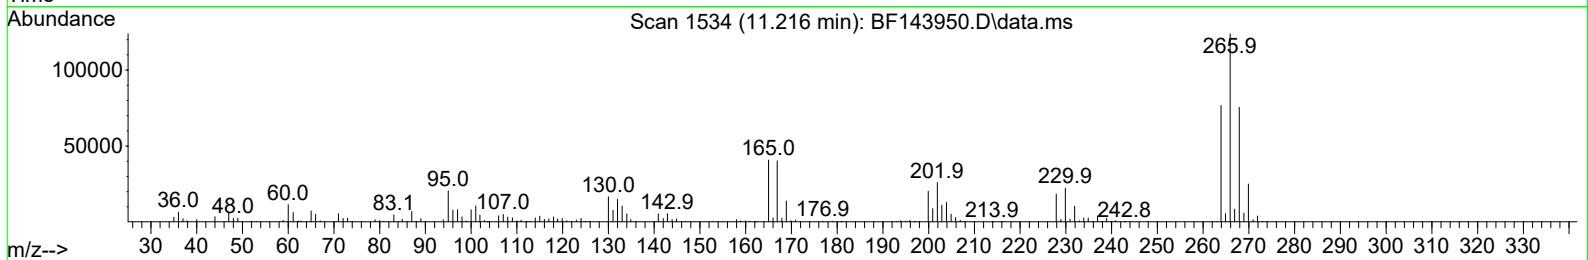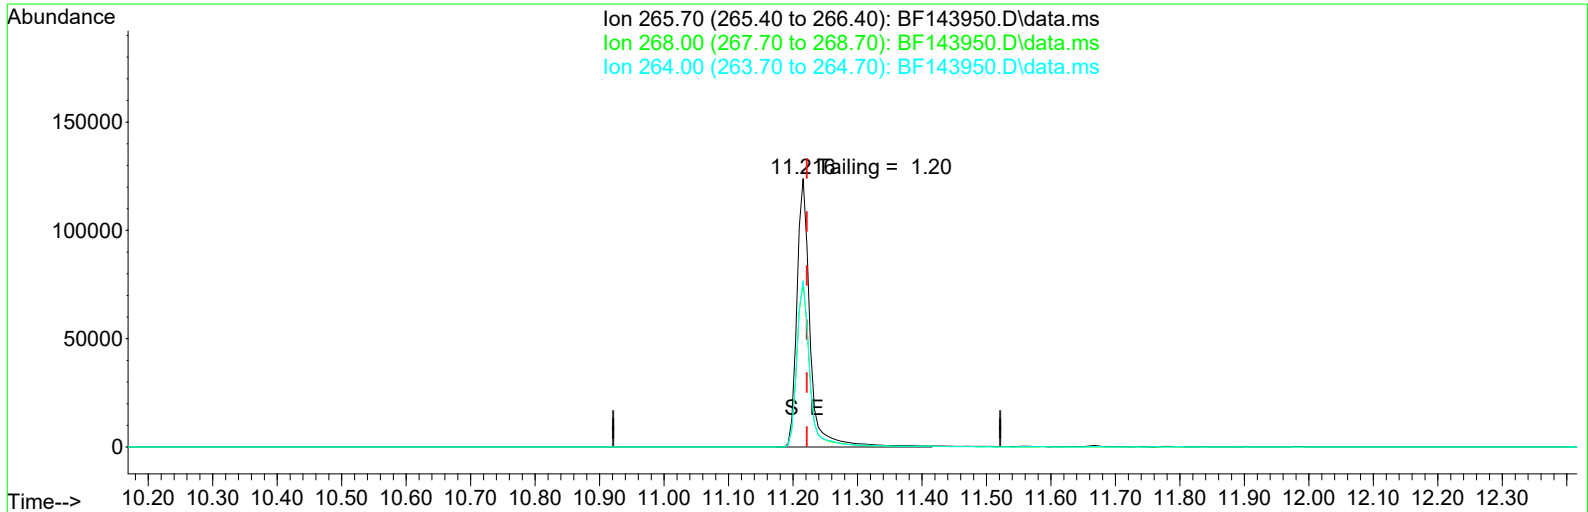

TIC: BF143950.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.006) 30340.06 ng




response 177465

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	60.92
264.00	64.70	61.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101525\
Data File : BF143950.D
Acq On : 15 Oct 2025 14:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 16 18:41:55 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

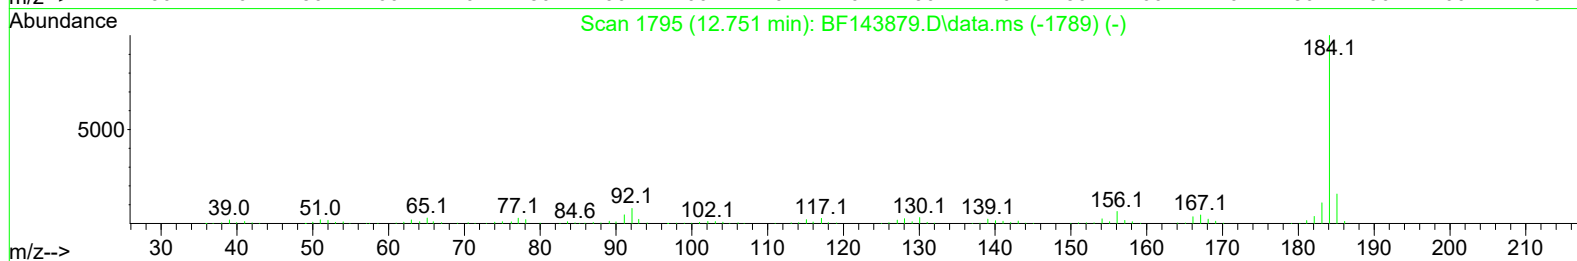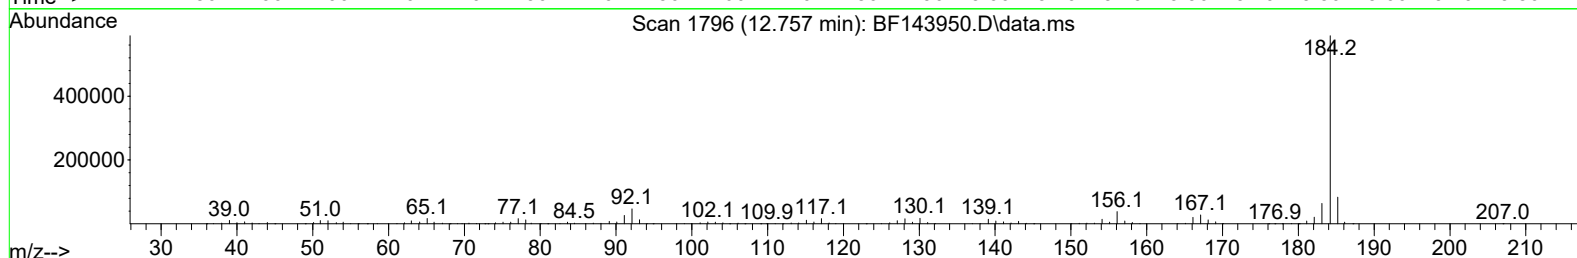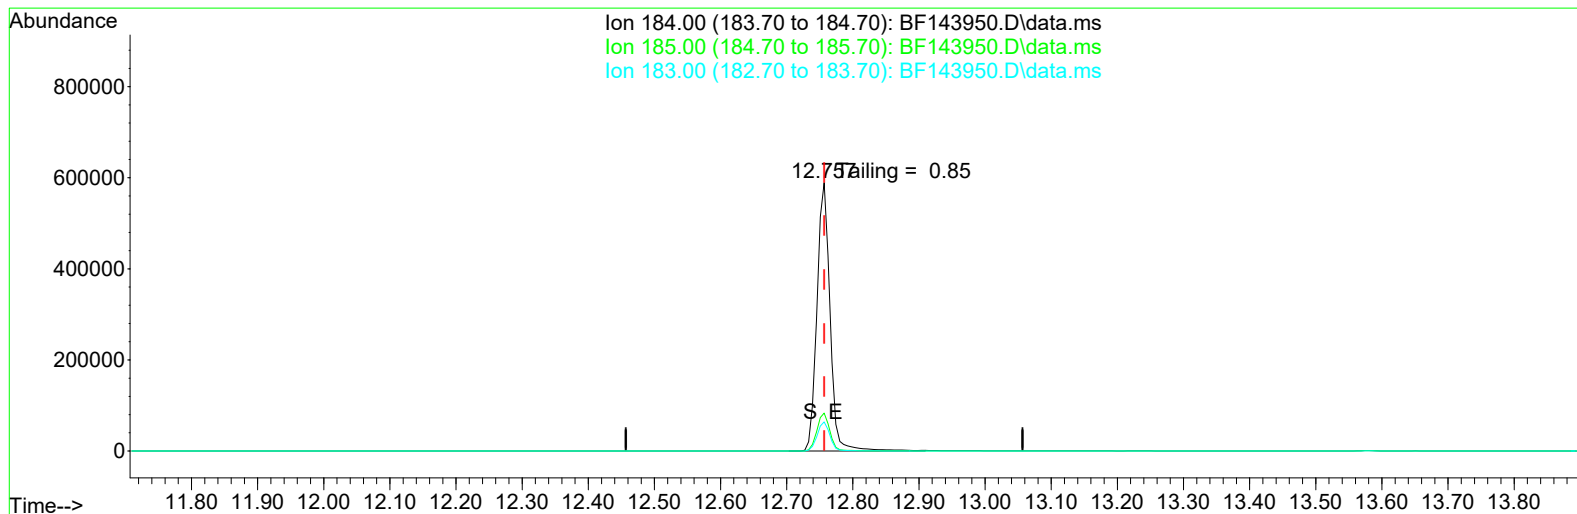

TIC: BF143950.D\data.ms

(77) Benzidine

12.757min (-0.000) 0.00 ng

response 814267

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.15
183.00	11.00	10.88
0.00	0.00	0.00