
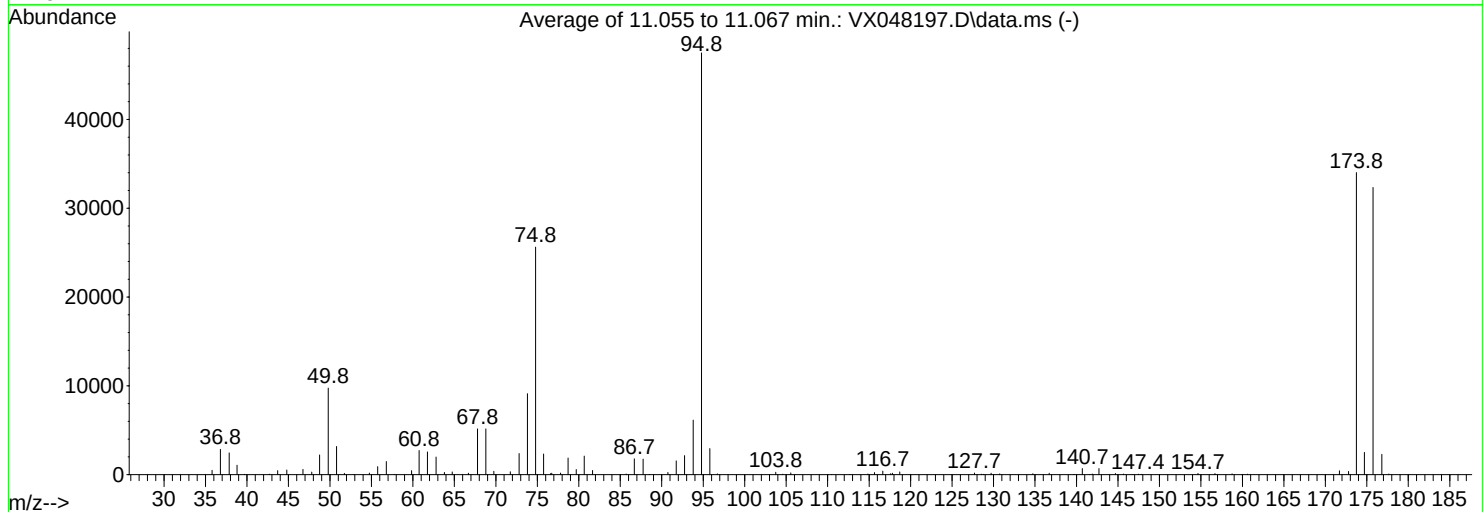


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101725\
Data File : VX048197.D
Acq On : 17 Oct 2025 08:17
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101725W.M
Title : SW846 8260
Last Update : Sat Oct 18 00:06:31 2025

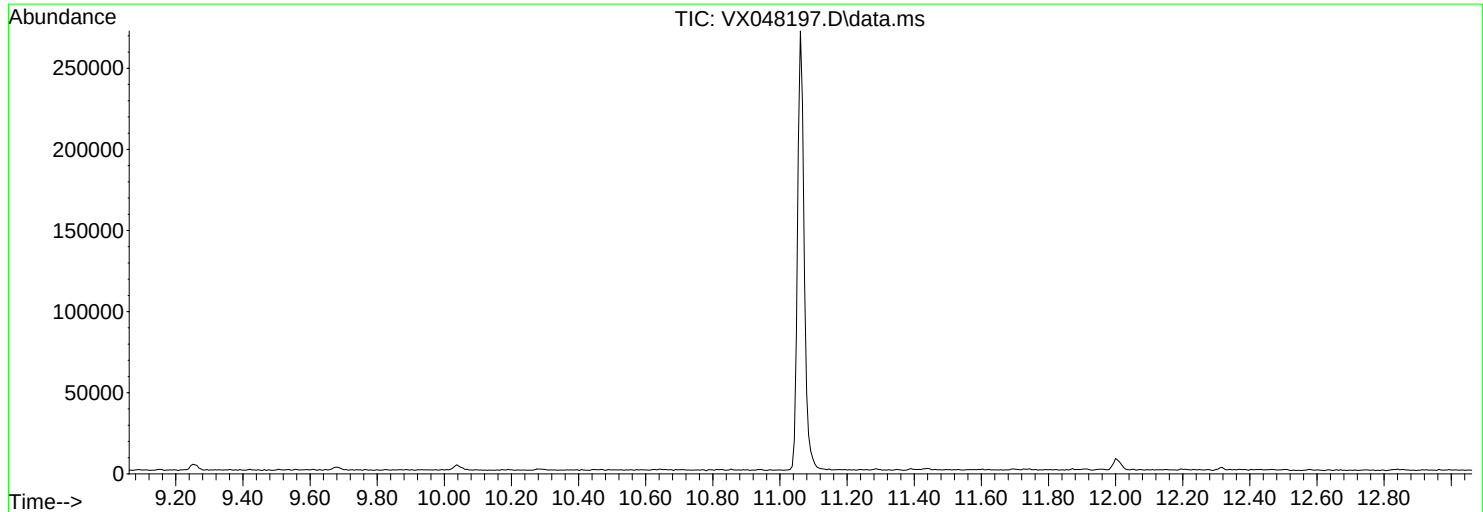

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1629

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.5	9750	PASS
75	95	30	60	53.9	25621	PASS
95	95	100	100	100.0	47507	PASS
96	95	5	9	6.2	2932	PASS
173	174	0.00	2	1.1	366	PASS
174	95	50	100	71.6	34021	PASS
175	174	5	9	7.4	2512	PASS
176	174	95	101	95.1	32341	PASS
177	176	5	9	7.1	2282	PASS