

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101725\
 Data File : PD090657.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2025 13:09
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 13:49:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 17 13:48:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.874	108.8E6	1215.0E6	50.000	50.000
28)	SA Decachlor...	9.066	8.062	167.8E6	1105.6E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.708	3.898	92608674	605.2E6	500.000	500.000
24)	Chlordane-2	5.235	4.479	92865500	631.9E6	500.000	500.000
25)	Chlordane-3	5.941	5.117	379.1E6	1885.9E6	500.000	500.000
26)	Chlordane-4	6.026	5.181	458.8E6	1625.9E6	500.000	500.000
27)	Chlordane-5	6.865	6.081	74238996	730.3E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101725\
Data File : PD090657.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2025 13:09
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 13:49:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
Quant Title : GC Extractables
QLast Update : Fri Oct 17 13:48:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

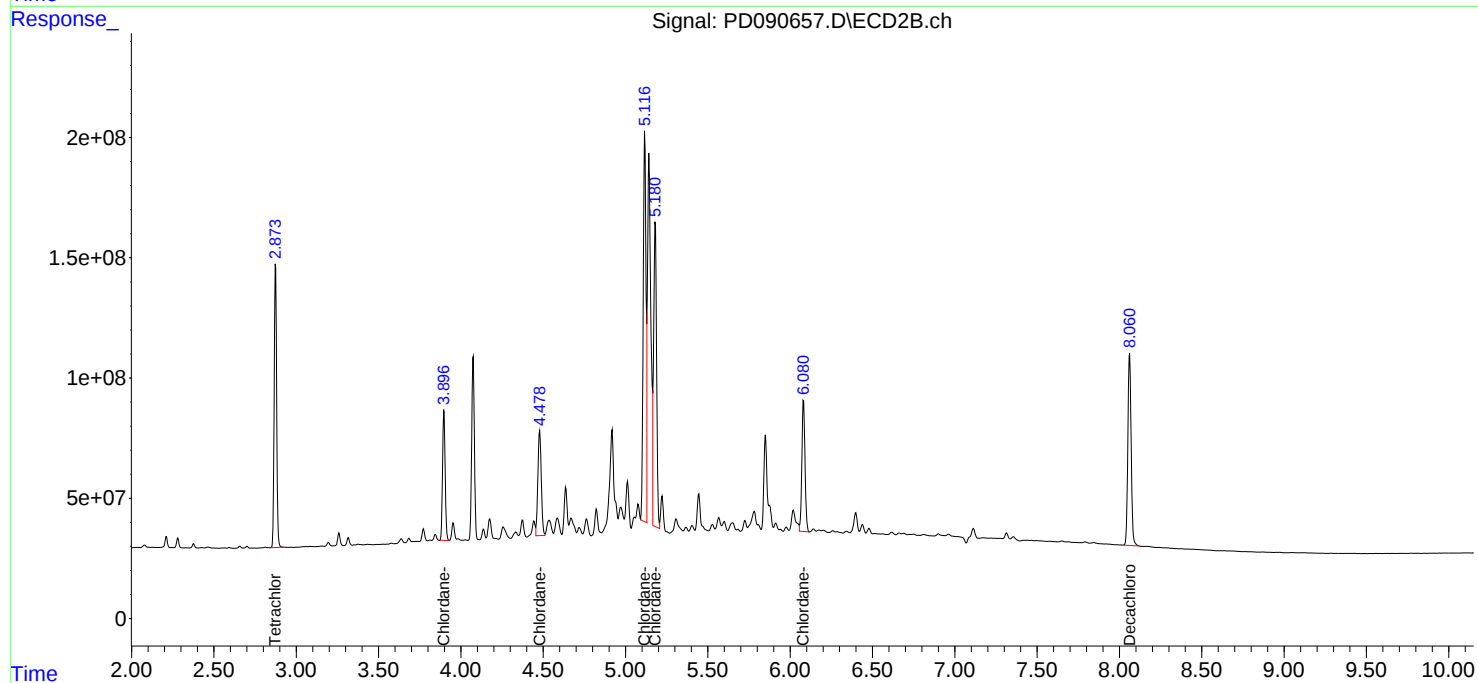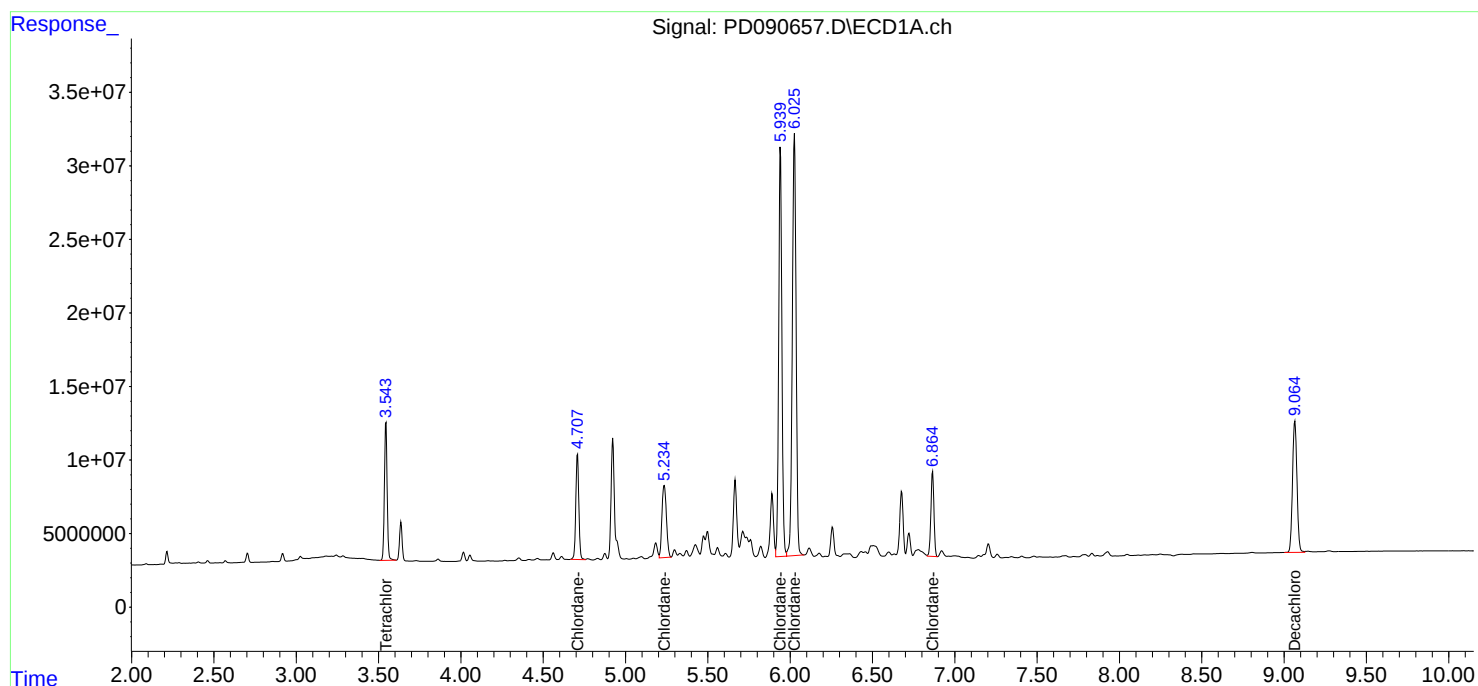


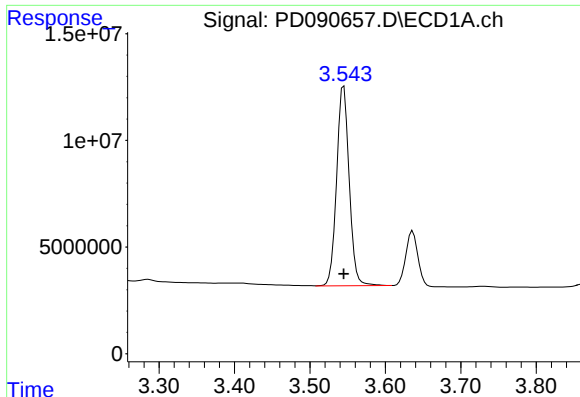

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 108758097
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

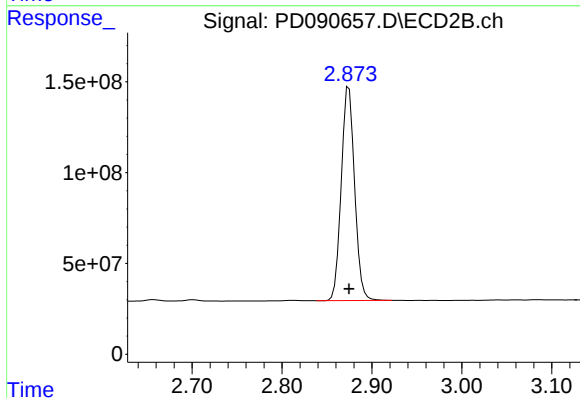


#1 Tetrachloro-m-xylene

R.T.: 2.874 min
Delta R.T.: 0.000 min
Response: 1214996007
Conc: 50.00 ng/ml

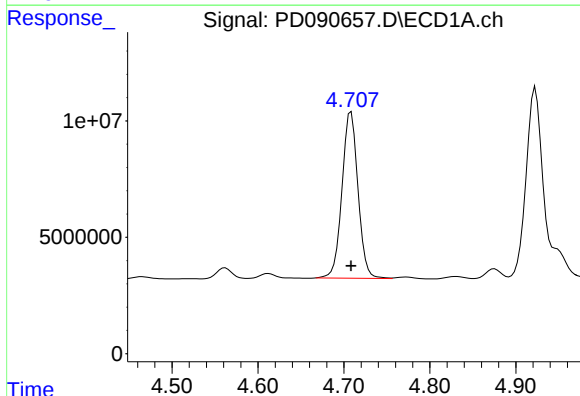


#23 Chlordane-1

R.T.: 4.708 min
Delta R.T.: 0.000 min
Response: 92608674
Conc: 500.00 ng/ml

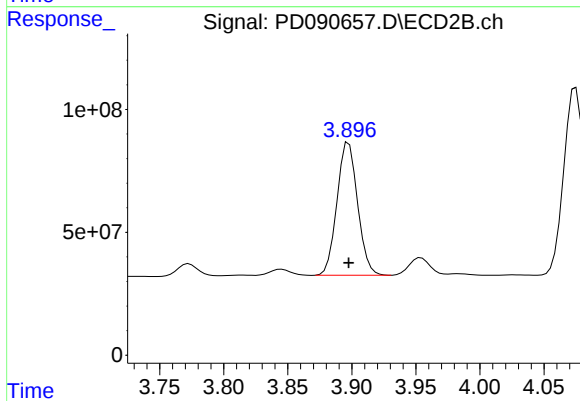

#23 Chlordane-1


R.T.: 3.898 min
Delta R.T.: 0.000 min
Response: 605185458
Conc: 500.00 ng/ml

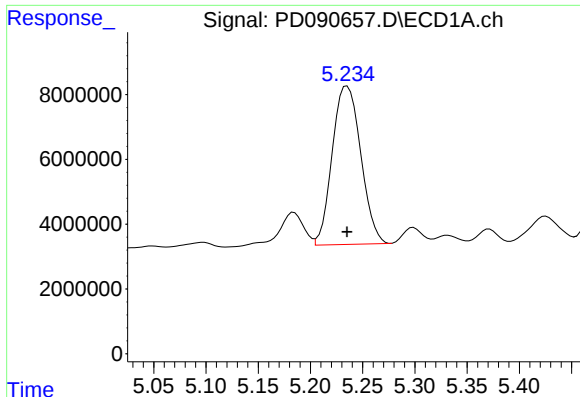

#24 Chlordane-2


R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 92865500
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

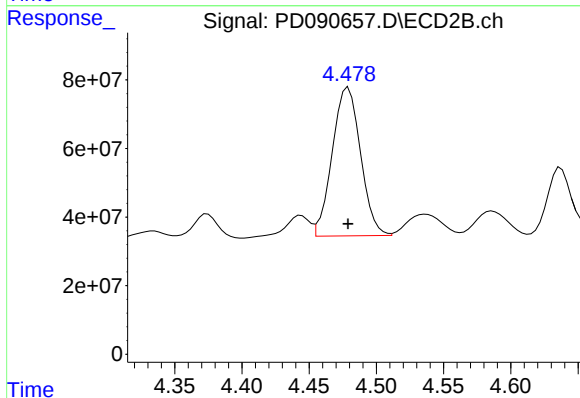


#24 Chlordane-2

R.T.: 4.479 min
Delta R.T.: 0.000 min
Response: 631892083
Conc: 500.00 ng/ml

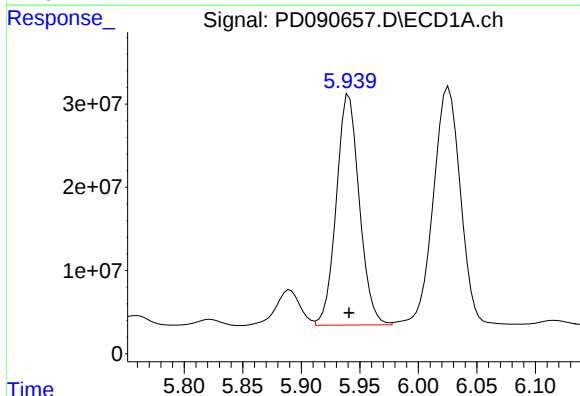


#25 Chlordane-3

R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 379095261
Conc: 500.00 ng/ml

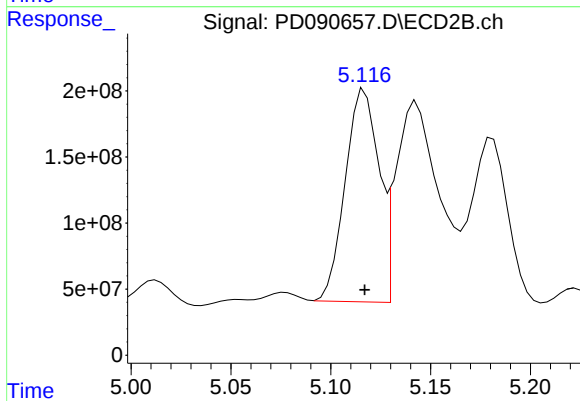

#25 Chlordane-3


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 1885915535
Conc: 500.00 ng/ml

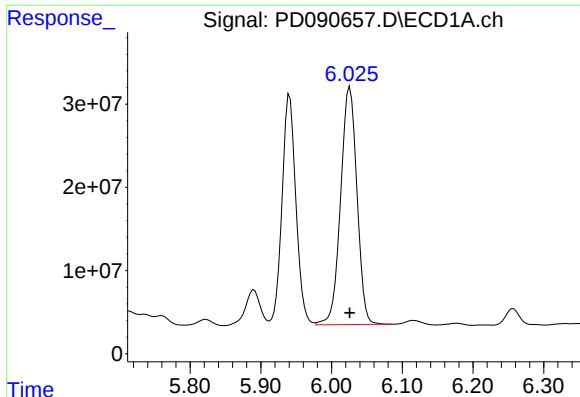

#26 Chlordane-4


R.T.: 6.026 min
Delta R.T.: 0.000 min
Response: 458791566
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

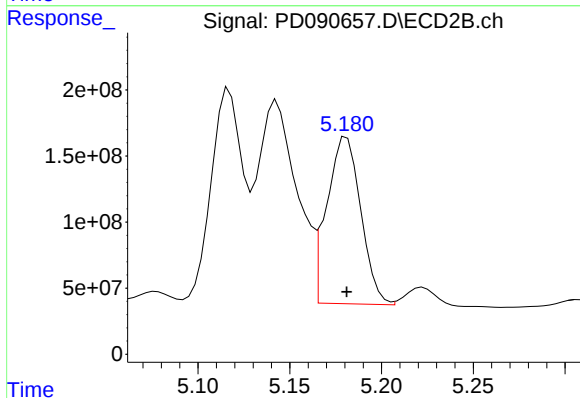


#26 Chlordane-4

R.T.: 5.181 min
Delta R.T.: 0.000 min
Response: 1625937453
Conc: 500.00 ng/ml

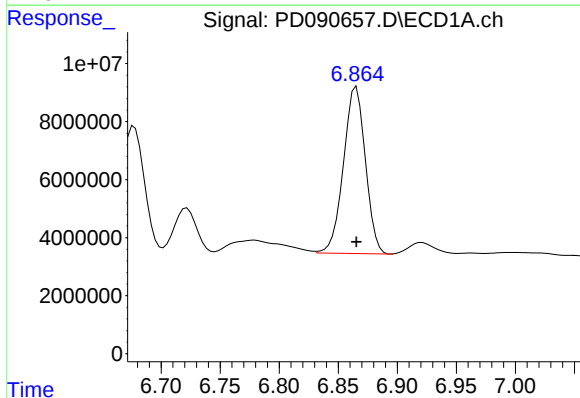


#27 Chlordane-5

R.T.: 6.865 min
Delta R.T.: 0.000 min
Response: 74238996
Conc: 500.00 ng/ml

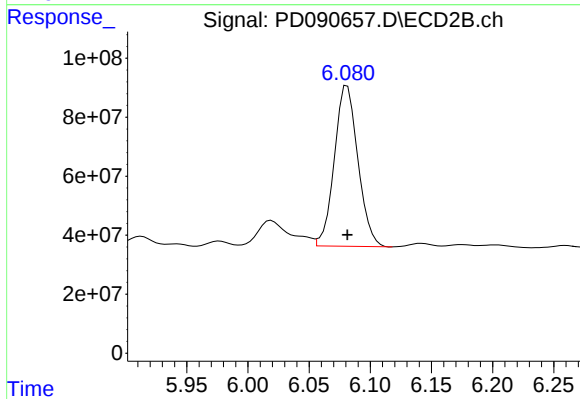

#27 Chlordane-5


R.T.: 6.081 min
Delta R.T.: 0.000 min
Response: 730253582
Conc: 500.00 ng/ml

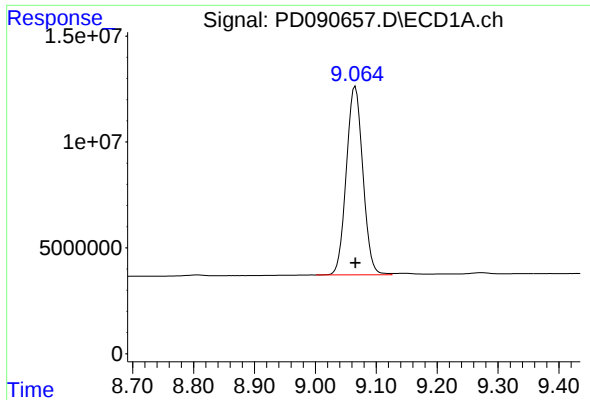

#28 Decachlorobiphenyl

R.T.: 9.066 min
Delta R.T.: 0.000 min
Response: 167755700
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

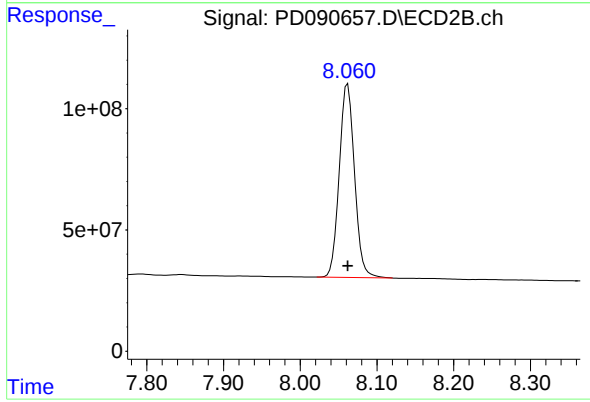

#28 Decachlorobiphenyl

R.T.: 8.062 min
Delta R.T.: 0.000 min
Response: 1105630741
Conc: 50.00 ng/ml