

## Prep Standard - Chemical Standard Summary

**Order ID :** Q3363  
**Test :** Pesticide-TCL  
  
**Prepbatch ID :** PB170142,  
**Sequence ID/Qc Batch ID:** pd101725,

**Standard ID :**

EP2643,EP2652,PP24651,PP24663,PP24738,PP24739,PP24740,PP24741,PP24742,PP24744,PP24745,PP24746,PP24747,PP24748,PP24749,PP24750,PP24751,PP24752,PP24753,PP24754,PP24755,PP24756,PP24757,PP24758,PP24759,PP24760,PP24761,PP24762,PP24763,PP24764,PP24766,PP24942,

**Chemical ID :**

E3875,E3941,E3944,E3951,E3955,E3956,E3971,E3972,E3976,E3978,P12604,P12610,P13038,P13041,P13196,P13246,P13774,P13780,P13786,P13788,P13862,P9053,

## Extractions STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>       | <u>NO.</u>             | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------|------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 230              | 1:1ACETONE/HEXANE | <a href="#">EP2643</a> | 09/16/2025       | 03/16/2026             | Evelyn Huang       | None           | None             | Riteshkumar Patel    |
| 09/16/2025       |                   |                        |                  |                        |                    |                |                  |                      |

**FROM** 4000.00000ml of E3971 + 4000.00000ml of E3972 = Final Quantity: 8000.000 ml

| <u>Recipe ID</u> | <u>NAME</u>          | <u>NO.</u>             | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u>         | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|----------------------|------------------------|------------------|------------------------|--------------------|------------------------|------------------|----------------------|
| 3923             | Baked Sodium Sulfate | <a href="#">EP2652</a> | 10/10/2025       | 01/28/2026             | Evelyn Huang       | Extraction_SC<br>ALE_2 | None             | Riteshkumar Patel    |
| (EX-SC-2)        |                      |                        |                  |                        |                    |                        |                  |                      |

**FROM** 4000.00000gram of E3875 = Final Quantity: 4000.000 gram

## Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>                             | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-----------------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 4027             | Pesticide resolution Check Mixture 8081 | <a href="#">PP24651</a> | 06/16/2025       | 12/11/2025             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                                         |                         |                  |                        |                    |                |                  | 07/22/2025           |

**FROM** 1.00000ml of P13246 + 99.00000ml of E3941 = Final Quantity: 100.000 ml

| <u>Recipe ID</u> | <u>NAME</u>                      | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|----------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 465              | 200 PPB Pest/PCB Surrogate Spike | <a href="#">PP24663</a> | 06/24/2025       | 12/24/2025             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                                  |                         |                  |                        |                    |                |                  | 07/21/2025           |

**FROM** 1.00000ml of P13786 + 999.00000ml of E3944 = Final Quantity: 1000.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>                                   | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-----------------------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 3629             | 20 PPM PEST stock Solution 1st source(RESTEK) | <a href="#">PP24738</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                                               |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 1.00000ml of P13038 + 9.00000ml of E3956 = Final Quantity: 10.000 ml

| <u>Recipe ID</u> | <u>NAME</u>                           | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|---------------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 1472             | 20 PPM Pest Stock Solution 2nd Source | <a href="#">PP24739</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                                       |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 1.00000ml of P13041 + 9.00000ml of E3956 = Final Quantity: 10.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>                         | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 1273             | 20 PPM Mirex Stock (Primary Source) | <a href="#">PP24740</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                                     |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 1.00000ml of P9053 + 9.00000ml of E3956 = Final Quantity: 10.000 ml

| <u>Recipe ID</u> | <u>NAME</u>                               | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 3663             | 20 PPM MIREX Stock STD (Secondary source) | <a href="#">PP24741</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                                           |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 1.00000ml of P13196 + 9.00000ml of E3956 = Final Quantity: 10.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>                     | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|---------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 84               | Pest/PCB Surrogate Stock 20 PPM | <a href="#">PP24742</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                                 |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 1.00000ml of P13788 + 9.00000ml of E3956 = Final Quantity: 10.000 ml

| <u>Recipe ID</u> | <u>NAME</u>                                     | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 3630             | 100/100 PPB PEST Working std.1st Source(RESTEK) | <a href="#">PP24744</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                                                 |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 98.50000ml of E3956 + 0.50000ml of PP24738 + 0.50000ml of PP24740 + 0.50000ml of PP24742 = Final Quantity: 100.000 ml



## Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>                                       | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u>       |
|------------------|---------------------------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------------|
| 80               | 100/100 PPB Pesticide Working Solution 2nd Source | <a href="#">PP24745</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel<br>07/24/2025 |

**FROM** 98.50000ml of E3956 + 0.50000ml of PP24739 + 0.50000ml of PP24741 + 0.50000ml of PP24742 = Final Quantity: 100.000 ml

| <u>Recipe ID</u> | <u>NAME</u>                         | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u>       |
|------------------|-------------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------------|
| 386              | 1000/100 PPB Chlordane STD (Restek) | <a href="#">PP24746</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel<br>07/24/2025 |

**FROM** 0.10000ml of P12604 + 99.40000ml of E3956 + 0.50000ml of PP24742 = Final Quantity: 100.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>                                     | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 3746             | 1000/100 ppb Chlordane<br>STD-RESTEK 2ND SOURCE | <a href="#">PP24747</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                                                 |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 0.10000ml of P12610 + 99.40000ml of E3956 + 0.50000ml of PP24742 = Final Quantity: 100.000 ml

| <u>Recipe ID</u> | <u>NAME</u>                            | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|----------------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 383              | 1000/100 PPB Toxaphene STD<br>(Restek) | <a href="#">PP24748</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                                        |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 0.10000ml of P13774 + 99.40000ml of E3956 + 0.50000ml of PP24742 = Final Quantity: 100.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>                                       | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|---------------------------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 3669             | 1000/100 PPB TOXAPHENE STD<br>2nd source (RESTEK) | <a href="#">PP24749</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                                                   |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 0.10000ml of P13862 + 99.40000ml of E3956 + 0.50000ml of PP24742 = Final Quantity: 100.000 ml

| <u>Recipe ID</u> | <u>NAME</u>                     | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|---------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 3631             | 75 PPB ICAL PEST<br>STD(RESTEK) | <a href="#">PP24750</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                                 |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 0.25000ml of E3956 + 0.75000ml of PP24744 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>                  | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 3632             | 50 PPB ICAL PEST STD(RESTEK) | <a href="#">PP24751</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                              |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 0.50000ml of E3956 + 0.50000ml of PP24744 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u>                  | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 3633             | 25 PPB ICAL PEST STD(RESTEK) | <a href="#">PP24752</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                              |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 0.75000ml of E3956 + 0.25000ml of PP24744 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>                 | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-----------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 3634             | 5 PPB ICAL PEST STD(RESTEK) | <a href="#">PP24753</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                             |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 0.90000ml of E3956 + 0.10000ml of PP24751 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u>                 | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-----------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 3988             | 50 PPB PEST ICV STD(RESTEK) | <a href="#">PP24754</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                             |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 0.50000ml of E3956 + 0.50000ml of PP24745 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>       | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 528              | CHLOR 750 PPB STD | <a href="#">PP24755</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                   |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 0.25000ml of E3956 + 0.75000ml of PP24746 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u>       | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 529              | CHLOR 500 PPB STD | <a href="#">PP24756</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                   |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 0.50000ml of E3956 + 0.50000ml of PP24746 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>       | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 530              | CHLOR 250 PPB STD | <a href="#">PP24757</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                   |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 0.75000ml of E3956 + 0.25000ml of PP24746 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u>      | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 3408             | CHLOR 50 PPB STD | <a href="#">PP24758</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                  |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 0.90000ml of E3956 + 0.10000ml of PP24756 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>           | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-----------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 532              | CHLOR 500 PPB ICV STD | <a href="#">PP24759</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                       |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 0.50000ml of E3956 + 0.50000ml of PP24747 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u>     | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-----------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 533              | TOX 750 PPB STD | <a href="#">PP24760</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                 |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 0.25000ml of E3956 + 0.75000ml of PP24748 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>     | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-----------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 534              | TOX 500 PPB STD | <a href="#">PP24761</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                 |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 0.50000ml of E3956 + 0.50000ml of PP24748 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u>     | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-----------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 535              | TOX 250 PPB STD | <a href="#">PP24762</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                 |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 0.75000ml of E3956 + 0.25000ml of PP24748 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>     | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-----------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 2217             | TOX 100 PPB STD | <a href="#">PP24763</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                 |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 0.90000ml of E3956 + 0.10000ml of PP24748 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u>                   | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 3670             | TOX 500 PPB ICV std ( RESTEK) | <a href="#">PP24764</a> | 07/21/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                               |                         |                  |                        |                    |                |                  | 07/24/2025           |

**FROM** 0.50000ml of PP24749 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>                      | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|----------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 79               | 500 PPB Pesticide Spike Solution | <a href="#">PP24766</a> | 07/28/2025       | 01/21/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                                  |                         |                  |                        |                    |                |                  | 08/19/2025           |

**FROM** 95.00000ml of E3955 + 2.50000ml of PP24739 + 2.50000ml of PP24741 = Final Quantity: 100.000 ml

| <u>Recipe ID</u> | <u>NAME</u>    | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|----------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 758              | PEM Mix w/Surr | <a href="#">PP24942</a> | 09/24/2025       | 03/24/2026             | Abdul Mirza        | None           | None             | Yogesh Patel         |
|                  |                |                         |                  |                        |                    |                |                  | 10/10/2025           |

**FROM** 1.00000ml of P13780 + 99.00000ml of E3971 = Final Quantity: 100.000 ml

## CHEMICAL RECEIPT LOG BOOK

| Supplier                    | ItemCode / ItemName                                    | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|-----------------------------|--------------------------------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| PCI Scientific Supply, Inc. | PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1 | 417203 | 01/28/2026      | 07/28/2025 / RUPESH     | 01/29/2025 / Rajesh         | E3875          |

| Supplier         | ItemCode / ItemName                       | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|-------------------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L) | 243570 | 12/11/2025      | 06/11/2025 / Rajesh     | 06/04/2025 / Rajesh         | E3941          |

| Supplier         | ItemCode / ItemName                        | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|--------------------------------------------|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9254-03 / Acetone, Ultra Resi (cs/4x4L) | 24H1462005 | 05/24/2027      | 06/20/2025 / RUPESH     | 05/14/2025 / RUPESH         | E3944          |

| Supplier         | ItemCode / ItemName                      | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|------------------------------------------|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-3382-05 / Sand, Purified (cs/4x2.5kg) | 25A2756718 | 12/31/2028      | 07/09/2025 / RUPESH     | 04/28/2020 / RUPESH         | E3951          |

| Supplier         | ItemCode / ItemName                        | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|--------------------------------------------|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9254-03 / Acetone, Ultra Resi (cs/4x4L) | 24H2762008 | 04/18/2027      | 07/16/2025 / RUPESH     | 07/16/2025 / RUPESH         | E3955          |

| Supplier         | ItemCode / ItemName                       | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|-------------------------------------------|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L) | 25C0362005 | 04/30/2026      | 07/16/2025 / RUPESH     | 07/16/2025 / RUPESH         | E3956          |

## CHEMICAL RECEIPT LOG BOOK

| Supplier         | ItemCode / ItemName                       | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|-------------------------------------------|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L) | 25C0362005 | 04/30/2026      | 09/15/2025 / Evelyn     | 09/04/2025 / Riteshkumar    | E3971          |

| Supplier         | ItemCode / ItemName                        | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|--------------------------------------------|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9254-03 / Acetone, Ultra Resi (cs/4x4L) | 24H1462005 | 05/24/2027      | 09/16/2025 / Evelyn     | 09/04/2025 / Riteshkumar    | E3972          |

| Supplier                | ItemCode / ItemName                  | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|-------------------------|--------------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Agela Technologies Inc. | FS0006 / Cleanert Florisil cartridge | M07456 | 04/03/2026      | 10/03/2025 / Evelyn     | 10/03/2025 / Evelyn         | E3976          |

| Supplier         | ItemCode / ItemName                       | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|-------------------------------------------|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L) | 25C0362006 | 04/13/2026      | 10/13/2025 / RUPESH     | 10/08/2025 / Riteshkumar    | E3978          |

| Supplier | ItemCode / ItemName    | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 32021 / Chlordane Std. | A0197993 | 01/21/2026      | 07/21/2025 / Abdul      | 07/03/2023 / Abdul          | P12604         |

| Supplier | ItemCode / ItemName    | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 32021 / Chlordane Std. | A0197993 | 01/21/2026      | 07/21/2025 / Abdul      | 07/03/2023 / Abdul          | P12610         |

## CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName                                                                             | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------------------------------------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 32291 / Pesticide Mix, CLP method, organochlorine Std AB#1, 200ug/mL, hexane/toluene, 1mL/ampul | A0200423 | 01/21/2026      | 07/21/2025 / Abdul      | 12/26/2023 / Abdul          | P13038         |

| Supplier | ItemCode / ItemName                                                                             | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------------------------------------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 32291 / Pesticide Mix, CLP method, organochlorine Std AB#1, 200ug/mL, hexane/toluene, 1mL/ampul | A0199099 | 07/21/2026      | 07/21/2025 / Abdul      | 12/26/2023 / Abdul          | P13041         |

| Supplier                 | ItemCode / ItemName       | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|---------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 79136 / Mirex, 1000 ug/ml | 042022 | 01/21/2026      | 07/21/2025 / Abdul      | 01/17/2024 / Abdul          | P13196         |

| Supplier                 | ItemCode / ItemName                             | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|-------------------------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 19161 / 8081 pesticide resolution check mixture | 013124 | 12/17/2025      | 06/17/2025 / Abdul      | 02/09/2024 / Abdul          | P13246         |

| Supplier | ItemCode / ItemName        | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|----------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 32005 / Toxaphene Standard | A0203038 | 01/21/2026      | 07/21/2025 / Abdul      | 05/03/2024 / Ankita         | P13774         |

| Supplier | ItemCode / ItemName                                      | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|----------------------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 32074 / Pesticide Performance Evaluation Mix w/Surrogate | A0213999 | 03/24/2026      | 09/24/2025 / Abdul      | 11/19/2024 / Ankita         | P13780         |

## CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName                                                                | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|------------------------------------------------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL | A0214495 | 12/24/2025      | 06/24/2025 / Abdul      | 11/19/2024 / Ankita         | P13786         |

| Supplier | ItemCode / ItemName                                                                | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|------------------------------------------------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL | A0214495 | 01/21/2026      | 07/21/2025 / Abdul      | 11/19/2024 / Ankita         | P13788         |

| Supplier | ItemCode / ItemName        | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|----------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 32005 / Toxaphene Standard | A0210240 | 01/21/2026      | 07/21/2025 / Abdul      | 12/09/2024 / Abdul          | P13862         |

| Supplier                 | ItemCode / ItemName       | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|---------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 79136 / Mirex, 1000 ug/ml | 112018 | 01/21/2026      | 07/21/2025 / Abdul      | 11/01/2019 / Stephen        | P9053          |



**PRODUCTOS  
QUÍMICOS  
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR  
MONTERREY, N.L. MÉXICO  
CP 64070  
TEL +52 81 13 52 67 67  
www.pqm.com.mx

# CERTIFICATE OF ANALYSIS

|                       |                                   |               |                                 |
|-----------------------|-----------------------------------|---------------|---------------------------------|
| PRODUCT :             | SODIUM SULFATE CRYSTALS ANHYDROUS |               |                                 |
| QUALITY :             | ACS (CODE RMB3375)                | FORMULA :     | Na <sub>2</sub> SO <sub>4</sub> |
| SPECIFICATION NUMBER: | 6399                              | RELEASE DATE: | MAY/23/2024                     |
| LOT NUMBER :          | 417203                            |               |                                 |

| TEST                                     | SPECIFICATIONS | LOT VALUES  |
|------------------------------------------|----------------|-------------|
| Assay (Na <sub>2</sub> SO <sub>4</sub> ) | Min. 99.0%     | 99.8 %      |
| pH of a 5% solution at 25°C              | 5.2 - 9.2      | 6.2         |
| Insoluble matter                         | Max. 0.01%     | 0.001 %     |
| Loss on ignition                         | Max. 0.5%      | 0.1 %       |
| Chloride (Cl)                            | Max. 0.001%    | <0.001 %    |
| Nitrogen compounds (as N)                | Max. 5 ppm     | <5 ppm      |
| Phosphate (PO <sub>4</sub> )             | Max. 0.001%    | <0.001 %    |
| Heavy metals (as Pb)                     | Max. 5 ppm     | <5 ppm      |
| Iron (Fe)                                | Max. 0.001%    | <0.001 %    |
| Calcium (Ca)                             | Max. 0.01%     | 0.001 %     |
| Magnesium (Mg)                           | Max. 0.005%    | 0.001 %     |
| Potassium (K)                            | Max. 0.008%    | 0.001 %     |
| Extraction-concentration suitability     | Passes test    | Passes test |
| Appearance                               | Passes test    | Passes test |
| Identification                           | Passes test    | Passes test |
| Solubility and foreign matter            | Passes test    | Passes test |
| Retained on US Standard No. 10 sieve     | Max. 1%        | 0.2 %       |
| Retained on US Standard No. 60 sieve     | Min. 94%       | 96.2 %      |
| Through US Standard No. 60 sieve         | Max. 5%        | 3.5 %       |
| Through US Standard No. 100 sieve        | Max. 10%       | 0.1 %       |

## COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

RE-02-01, Ed. 3

E 3875

## Certificate of Analysis

1 Reagent Lane  
 Fair Lawn, NJ 07410  
 201.796.7100 tel  
 201.796.1329 fax

Thermo Fisher Scientific's Quality System has been found to conform to Quality Management System  
 Standard ISO9001:2015 by SAI Global Certificate Number CERT – 0120633

This is to certify that units of the lot number below were tested and found to comply with the specifications of the grade listed. Certain data have been supplied by third parties. Thermo Fisher Scientific expressly disclaims all warranties, expressed or implied, including the implied warranties of merchantability and fitness for a particular purpose. Products are for research use or further manufacturing. Not for direct administration to humans or animals. It is the responsibility of the final formulator and end user to determine suitability based upon the intended use of the end product. Products are tested to meet the analytical requirements of the noted grade. The following information is the actual analytical results obtained.

|                   |                                                                                                                                                                                                   |                             |            |
|-------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-----------------------------|------------|
| Catalog Number    | H303                                                                                                                                                                                              | Quality Test / Release Date | 11/07/2024 |
| Lot Number        | 243570                                                                                                                                                                                            |                             |            |
| Description       | HEXANES - OPTIMA                                                                                                                                                                                  |                             |            |
| Country of Origin | United States                                                                                                                                                                                     | Suggested Retest Date       | Nov/2029   |
| Chemical Origin   | Organic - non animal                                                                                                                                                                              |                             |            |
| BSE/TSE Comment   | No animal products are used as starting raw material ingredients, or used in processing, including lubricants, processing aids, or any other material that might migrate to the finished product. |                             |            |

| N/A                         |            |                                 |                         |
|-----------------------------|------------|---------------------------------|-------------------------|
| Result Name                 | Units      | Specifications                  | Test Value              |
| APPEARANCE                  |            | REPORT                          | Clear, colorless liquid |
| ASSAY (N-HEXANE)            | %          | >= 60                           | 69                      |
| ASSAY (SUM C6 HYDROCARBONS) | %          | >= 99.9                         | >99.9                   |
| COLOR                       | APHA       | <= 5                            | <5                      |
| DENSITY AT 25 DEGREES C     | GM/ML      | Inclusive Between 0.653 - 0.673 | 0.669                   |
| EVAPORATION RESIDUE         | ppm        | <= 1                            | <1                      |
| FLUORESCENCE BACKGROUND     | ppb        | <= 1                            | <1                      |
| IDENTIFICATION              | PASS/FAIL  | = PASS TEST                     | PASS TEST               |
| OPTICAL ABS AT 195 NM       | ABS. UNITS | <= 1                            | 0.74                    |
| OPTICAL ABS AT 210 NM       | ABS. UNITS | <= 0.25                         | 0.17                    |
| OPTICAL ABS AT 220 NM       | ABS. UNITS | <= 0.07                         | 0.05                    |
| OPTICAL ABS AT 254 NM       | ABS. UNITS | <= 0.005                        | 0.001                   |
| PESTICIDE RESIDUE ANALYSIS  | NG/L       | <= 10                           | <10                     |
| REFRACTIVE INDEX @ 25 DEG C |            | Inclusive Between 1.375 - 1.385 | 1.379                   |
| SUITABILITY FOR GC/MS       |            | = PASS TEST                     | PASS TEST               |
| SULFUR COMPOUNDS            | %          | <= 0.005                        | <0.005                  |
| THIOPHENE                   | PASS/FAIL  | = PASS TEST                     | PASS TEST               |
| WATER (H2O)                 | %          | <= 0.01                         | <0.01                   |
| WATER-SOLUBLE TITRABLE ACID | MEQ/G      | <= 0.0003                       | 0.0001                  |



Recd. by RI on 6/11/25

E3941

Harout Sahagian - Quality Control Manager - Fair Lawn

Note: The data listed is valid for all package sizes of this lot of this product, expressed as an extension of this catalog number listed above.  
 If there are any questions with this certificate, please call at (800) 227-6701.  
 \*Based on suggested storage condition.

Acetone  
BAKER RESI-ANALYZED® Reagent  
For Organic Residue Analysis

Avantor™



Material No.: 9254-03

Batch No.: 24H1462005

Manufactured Date: 2024-05-24

Expiration Date: 2027-05-24

Revision No.: 0

## Certificate of Analysis

| Test                                                                    | Specification | Result      |
|-------------------------------------------------------------------------|---------------|-------------|
| Assay ((CH <sub>3</sub> ) <sub>2</sub> CO) (by GC, corrected for water) | >= 99.4 %     | 99.8 %      |
| Color (APHA)                                                            | <= 10         | 5           |
| Residue after Evaporation                                               | <= 1.0 ppm    | 0.2 ppm     |
| Substances Reducing Permanganate                                        | Passes Test   | Passes Test |
| Titration Acid (μeq/g)                                                  | <= 0.3        | 0.2         |
| Titration Base (μeq/g)                                                  | <= 0.6        | <0.1        |
| Water (H <sub>2</sub> O)                                                | <= 0.5 %      | 0.2 %       |
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)    | <= 5          | <1          |
| ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)    | <= 10         | 1           |

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States  
Packaging Site: Phillipsburg Mfg Ctr & DC

E3944

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC



|                      |                                |
|----------------------|--------------------------------|
| Material             | BDH9274-2.5KG                  |
| Material Description | BDH SAND STDD OTTAWA W+I 2.5KG |
| Grade                | NOT APPLICABLE                 |
| Batch                | 25A2756718                     |
| Reassay Date         | 12/31/2028                     |
| CAS Number           | 14808-60-7                     |
| Molecular Formula    | SiO <sub>2</sub>               |
| Molecular Mass       | 60.09                          |
| Date of Manufacture  | 12/05/2024                     |
| Storage              | Room Temperature               |

| Characteristics               | Specifications  | Measured Values |
|-------------------------------|-----------------|-----------------|
| Appearance                    | Beige granules. | Beige granules. |
| Moisture                      | <= 0.1 %        | 0.1 %           |
| Particle Size 30-40 mesh      | >= 80 %         | 99 %            |
| CUSTOMER PART # BDH9274-2.5KG |                 |                 |

*Received on 1/12/25.*

**E3951**

Internal ID #: 793

| Signature                                                                                                                                                                                                                                                                                                   | Additional Information                                                                                                                                   |
|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------|
| <p>We certify that this batch conforms to the specifications listed above.</p> <p>This document has been electronically produced and is valid without a signature.</p> <p>Leona Edwardson, Quality Control Sr. Manager - Solon<br/> VWR Chemicals, LLC.<br/> 28600 Fountain Parkway, Solon OH 44139 USA</p> | <p>Analysis may have been rounded to significant digits in specification limits</p> <p>Product meets analytical specifications of the grades listed.</p> |

Acetone  
BAKER RESI-ANALYZED® Reagent  
For Organic Residue Analysis



Material No.: 9254-03  
Batch No.: 24H2762008  
Manufactured Date: 2024-04-18  
Expiration Date: 2027-04-18  
Revision No.: 0

## Certificate of Analysis

| Test                                                                    | Specification | Result      |
|-------------------------------------------------------------------------|---------------|-------------|
| Assay ((CH <sub>3</sub> ) <sub>2</sub> CO) (by GC, corrected for water) | >= 99.4 %     | 100.0 %     |
| Color (APHA)                                                            | <= 10         | 5           |
| Residue after Evaporation                                               | <= 1.0 ppm    | 0.0 ppm     |
| Substances Reducing Permanganate                                        | Passes Test   | Passes Test |
| Titration Acid (µeq/g)                                                  | <= 0.3        | 0.2         |
| Titration Base (µeq/g)                                                  | <= 0.6        | <0.1        |
| Water (H <sub>2</sub> O)                                                | <= 0.5 %      | <0.1 %      |
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)    | <= 5          | 1           |
| ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)    | <= 10         | 1           |

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States  
Packaging Site: Phillipsburg Mfg Ctr & DC

*Received on 7/16/25*

**E 3955**

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA, 19087, U.S.A. Phone 610.386.1700

n-Hexane 95%  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis

 **avantors**<sup>™</sup>



Material No.: 9262-03

Batch No.: 25C0362005

Manufactured Date: 2025-01-29

Expiration Date: 2026-04-30

Revision No.: 0

## Certificate of Analysis

| Test                                                                           | Specification  | Result      |
|--------------------------------------------------------------------------------|----------------|-------------|
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)           | $\leq 5$       | 1           |
| ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)            | $\leq 10$      | 6           |
| ECD-Sensitive Impurities (as EthyleneDibromide) - Single Impurity Peak (ng/mL) | $\leq 5$       | 5           |
| Assay (Total Saturated C <sub>6</sub> Isomers) (by GC, corrected for water)    | $\geq 99.5 \%$ | 100.0 %     |
| Assay (as n-Hexane) (by GC, corrected for water)                               | $\geq 95 \%$   | 100 %       |
| Color (APHA)                                                                   | $\leq 10$      | 10          |
| Residue after Evaporation                                                      | $\leq 1.0$ ppm | 0.1 ppm     |
| Substances Darkened by H <sub>2</sub> SO <sub>4</sub>                          | Passes Test    | Passes Test |
| Water (by KF, coulometric)                                                     | $\leq 0.05 \%$ | $< 0.01 \%$ |

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States  
Packaging Site: Phillipsburg Mfg Ctr & DC

*Received on 7/16/25*

**E3956**



Jamie Croak  
Director Quality Operations, Bioscience Production

n-Hexane 95%  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis



Material No.: 9262-03  
Batch No.: 25C0362005  
Manufactured Date: 2025-01-29  
Expiration Date: 2026-04-30  
Revision No.: 0

## Certificate of Analysis

| Test                                                                           | Specification  | Result      |
|--------------------------------------------------------------------------------|----------------|-------------|
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)           | $\leq 5$       | 1           |
| ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)            | $\leq 10$      | 6           |
| ECD-Sensitive Impurities (as EthyleneDibromide) - Single Impurity Peak (ng/mL) | $\leq 5$       | 5           |
| Assay (Total Saturated C <sub>6</sub> Isomers) (by GC, corrected for water)    | $\geq 99.5 \%$ | 100.0 %     |
| Assay (as n-Hexane) (by GC, corrected for water)                               | $\geq 95 \%$   | 100 %       |
| Color (APHA)                                                                   | $\leq 10$      | 10          |
| Residue after Evaporation                                                      | $\leq 1.0$ ppm | 0.1 ppm     |
| Substances Darkened by H <sub>2</sub> SO <sub>4</sub>                          | Passes Test    | Passes Test |
| Water (by KF, coulometric)                                                     | $\leq 0.05 \%$ | $< 0.01 \%$ |

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States  
Packaging Site: Phillipsburg Mfg Ctr & DC

E3971

Jamie Croak  
Director Quality Operations, Bioscience Production

Acetone  
BAKER RESI-ANALYZED® Reagent  
For Organic Residue Analysis

avantor™



Material No.: 9254-03

Batch No.: 24H1462005

Manufactured Date: 2024-05-24

Expiration Date: 2027-05-24

Revision No.: 0

## Certificate of Analysis

| Test                                                                    | Specification | Result      |
|-------------------------------------------------------------------------|---------------|-------------|
| Assay ((CH <sub>3</sub> ) <sub>2</sub> CO) (by GC, corrected for water) | >= 99.4 %     | 99.8 %      |
| Color (APHA)                                                            | <= 10         | 5           |
| Residue after Evaporation                                               | <= 1.0 ppm    | 0.2 ppm     |
| Substances Reducing Permanganate                                        | Passes Test   | Passes Test |
| Titration Acid (μeq/g)                                                  | <= 0.3        | 0.2         |
| Titration Base (μeq/g)                                                  | <= 0.6        | <0.1        |
| Water (H <sub>2</sub> O)                                                | <= 0.5 %      | 0.2 %       |
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)    | <= 5          | <1          |
| ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)    | <= 10         | 1           |

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States  
Packaging Site: Phillipsburg Mfg Ctr & DC

E3972

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

Cleanert Florisil

1g/6ml 30/pkg

LOT#:M07456

MFG#:G02147

CAT#FS0006



固相萃取产品

Made in China

Agela Technologies

E 3976



n-Hexane 95%  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis

 **avantors<sup>TM</sup>**



Material No.: 9262-03

Batch No.: 25C0362006

Manufactured Date: 2025-01-29

Expiration Date: 2026-04-30

Revision No.: 0

## Certificate of Analysis

| Test                                                                            | Specification  | Result      |
|---------------------------------------------------------------------------------|----------------|-------------|
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)            | $\leq 5$       | 1           |
| ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)            | $\leq 10$      | 6           |
| ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL) | $\leq 5$       | 4           |
| Assay (Total Saturated C <sub>6</sub> Isomers) (by GC, corrected for water)     | $\geq 99.5 \%$ | 100.0 %     |
| Assay (as n-Hexane) (by GC, corrected for water)                                | $\geq 95 \%$   | 100 %       |
| Color (APHA)                                                                    | $\leq 10$      | 10          |
| Residue after Evaporation                                                       | $\leq 1.0$ ppm | 0.2 ppm     |
| Substances Darkened by H <sub>2</sub> SO <sub>4</sub>                           | Passes Test    | Passes Test |
| Water (by KF, coulometric)                                                      | $\leq 0.05 \%$ | $< 0.01 \%$ |

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E 3978



Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32291

Lot No.: A0199099

Description : Organochlorine Pesticide Mix AB #1

Organochlorine Pesticide Mix AB #1 200µg/mL, Hexane/Toluene(50:50), 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : June 30, 2027

Storage: 10°C or colder

Ship: Ambient

P130397 5  
↓  
P13043 1  
✓  
12-26-2023

### CERTIFIED VALUES

| Elution Order | Compound                      | CAS #      | Lot #      | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|-------------------------------|------------|------------|--------|-----------------------------|----------------------------------------|
| 1             | alpha-BHC                     | 319-84-6   | 14434500   | 99%    | 200.0 µg/mL                 | +/- 8.9732                             |
| 2             | gamma-BHC (Lindane)           | 58-89-9    | 14184400   | 98%    | 200.1 µg/mL                 | +/- 8.9762                             |
| 3             | beta-BHC                      | 319-85-7   | BCCC6425   | 99%    | 200.3 µg/mL                 | +/- 8.9844                             |
| 4             | delta-BHC                     | 319-86-8   | 14450800   | 98%    | 200.0 µg/mL                 | +/- 8.9740                             |
| 5             | Heptachlor                    | 76-44-8    | 813251     | 99%    | 200.1 µg/mL                 | +/- 8.9754                             |
| 6             | Aldrin                        | 309-00-2   | 14389400   | 98%    | 200.0 µg/mL                 | +/- 8.9718                             |
| 7             | Heptachlor epoxide (isomer B) | 1024-57-3  | 14448800   | 99%    | 200.1 µg/mL                 | +/- 8.9754                             |
| 8             | trans-Chlordane               | 5103-74-2  | 32943      | 98%    | 199.9 µg/mL                 | +/- 8.9696                             |
| 9             | cis-Chlordane                 | 5103-71-9  | 31766      | 98%    | 200.1 µg/mL                 | +/- 8.9762                             |
| 10            | Endosulfan I                  | 959-98-8   | BCCF4060   | 99%    | 200.1 µg/mL                 | +/- 8.9754                             |
| 11            | 4,4'-DDE                      | 72-55-9    | GHYQG      | 99%    | 200.1 µg/mL                 | +/- 8.9777                             |
| 12            | Dieldrin                      | 60-57-1    | 11129900   | 98%    | 200.0 µg/mL                 | +/- 8.9718                             |
| 13            | Endrin                        | 72-20-8    | 14123200   | 98%    | 199.9 µg/mL                 | +/- 8.9696                             |
| 14            | 4,4'-DDD                      | 72-54-8    | HAN02      | 99%    | 200.1 µg/mL                 | +/- 8.9777                             |
| 15            | Endosulfan II                 | 33213-65-9 | 14374700   | 99%    | 200.0 µg/mL                 | +/- 8.9732                             |
| 16            | 4,4'-DDT                      | 50-29-3    | 230410JLMA | 98%    | 200.0 µg/mL                 | +/- 8.9718                             |

|    |                    |            |            |     |       |       |            |
|----|--------------------|------------|------------|-----|-------|-------|------------|
| 17 | Endrin aldehyde    | 7421-93-4  | 30720      | 98% | 200.1 | µg/mL | +/- 8.9784 |
| 18 | Endosulfan sulfate | 1031-07-8  | BCCH9010   | 99% | 200.0 | µg/mL | +/- 8.9732 |
| 19 | Methoxychlor       | 72-43-5    | 13668200   | 99% | 200.1 | µg/mL | +/- 8.9777 |
| 20 | Endrin ketone      | 53494-70-5 | 1-ABS-16-7 | 98% | 200.0 | µg/mL | +/- 8.9740 |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane/Toluene (50:50)  
**CAS #** 110-54-3/108-88-3  
**Purity** 99%

P13039  
 ↓  
 P13043  
 5  
 1  
 JAW  
 12/26/23

## Quality Confirmation Test

**Column:**  
 30m x .25mm x .2um  
 Rtx-CLP II (cat.# 11323)

**Carrier Gas:**  
 helium-constant pressure 20 psi.

**Temp. Program:**  
 150°C to 300°C  
 @ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
 200°C

**Det. Temp:**  
 300°C

**Det. Type:**  
 ECD

**Split Vent:**  
 Split ratio 50:1

**Inj. Vol**  
 1µl

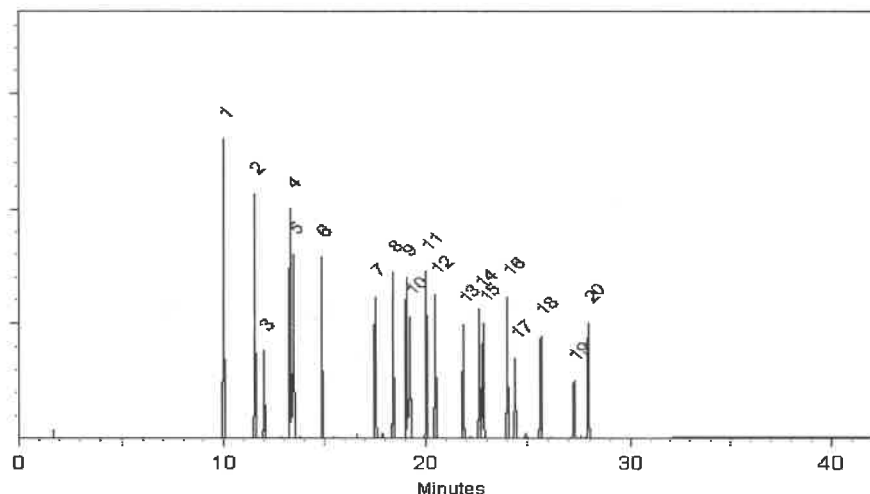

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Josh McCloskey*  
 Josh McCloskey - Operations Technician I

**Date Mixed:** 19-Jun-2023

**Balance Serial #** 1128360905

*Jennifer Pollino*  
 Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 23-Jun-2023

Manufactured under Restek's ISO 9001:2015  
 Registered Quality System  
 Certificate #FM 80397



**CERTIFIED WEIGHT REPORT**

Part Number: **79136**  
Lot Number: **042022**  
Description: **Mirex**

Solvent(s):  
Acetone  
Lot#: 81025

|                         |                  |        |
|-------------------------|------------------|--------|
| <i>Prashant Chauhan</i> |                  | 042022 |
| Formulated By:          | Prashant Chauhan | DATE   |
| <i>Pedro L. Rentas</i>  |                  | 042022 |
| Reviewed By:            | Pedro L. Rentas  | DATE   |

Expiration Date: 042027  
Recommended Storage: Refrigerate (4 °C)  
Nominal Concentration (µg/mL): 1000  
NIST Test ID#: 6UTB



5E-05 Balance Uncertainty  
0.006 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL): 50.0

| Expanded            |                                    |                                        |                      | SDS Information |                   |                   |
|---------------------|------------------------------------|----------------------------------------|----------------------|-----------------|-------------------|-------------------|
| Compound            | RM#                                | Lot Number                             | Nominal Conc (µg/mL) | Purity (%)      | Target Weight (g) | Actual Weight (g) |
| Actual Conc (µg/mL) | Expanded Uncertainty (+/-) (µg/mL) | (Solvent Safety Info. On Attached pg.) |                      |                 |                   |                   |
| CAS#                | OSHA PEL (TWA)                     | LD50                                   |                      |                 |                   |                   |

|          |     |         |      |      |     |         |         |        |      |           |     |                  |
|----------|-----|---------|------|------|-----|---------|---------|--------|------|-----------|-----|------------------|
| 1. Mirex | 437 | 9492400 | 1000 | 99.4 | 0.5 | 0.05034 | 0.05040 | 1001.1 | 10.3 | 2385-85-5 | N/A | ori-rat 306mg/kg |
|----------|-----|---------|------|------|-----|---------|---------|--------|------|-----------|-----|------------------|

Method GC7MSD-1.M: Column: SPB-608 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 150°C (4min.), Temp 2 = 290°C (13.5 min.), Rate = 8°C/min., Injector B= 200°C, Detector B = 290°C. Split Ratio = 100:1, Scan Rate = 2. Analysis performed by Candice Warren.

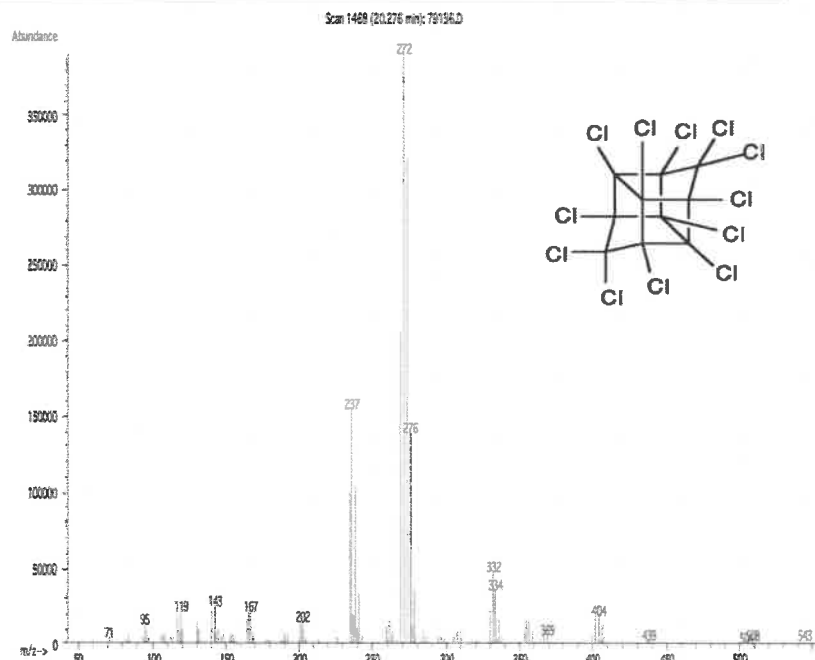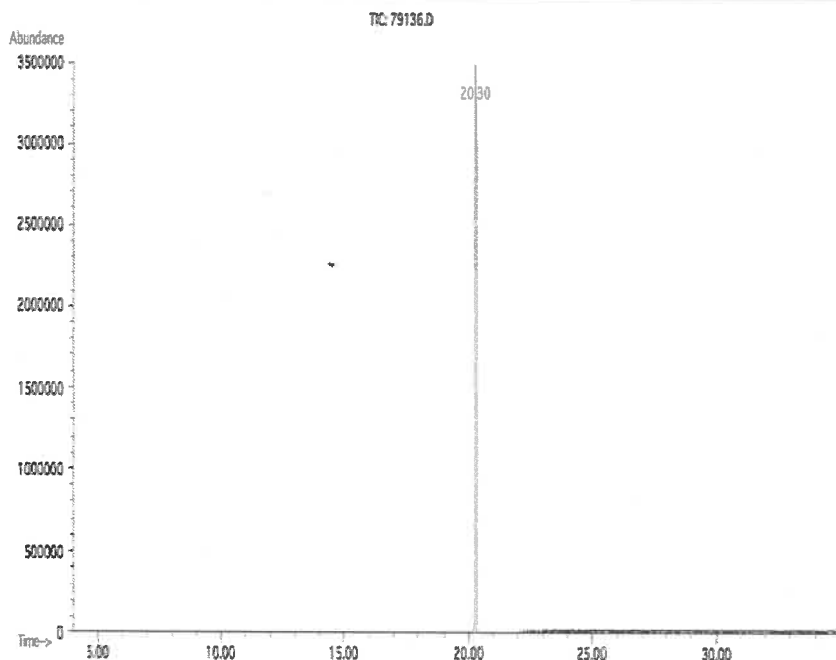

P13195  
↓  
P13199  
↓  
(5)  
↓  
W. H. H. H.  
01/17/2024

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5 % of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

01/17/2024  
JALIN

5



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32021 Lot No.: A0197993  
Description : Chlordane Standard  
Chlordane Standard 1000µg/mL, Hexane, 1mL/ampul  
Container Size : 2 mL Pkg Amt: > 1 mL  
Expiration Date : August 31, 2029 Storage: 10°C or colder  
Ship: Ambient

P 12603  
↓  
P 12605  
3  
Kauf  
7/3/2023

### CERTIFIED VALUES

| Elution Order | Compound                                                              | CAS #   | Lot #  | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|-----------------------------------------------------------------------|---------|--------|--------|-----------------------------|----------------------------------------|
| 1             | Chlordane<br>10% trans-Chlordane; 9% cis-Chlordane; 81% other isomers | 57-74-9 | 978545 | ----%  | 1,005.0 µg/mL               | +/- 55.7700                            |

Solvent: Hexane  
CAS # 110-54-3  
Purity 99%

\* Expanded Uncertainty displayed in same units as Grav. Conc.

### Tech Tips:

CAS #57-74-9 nomenclature is based on EPA method 8081B.

## Quality Confirmation Test

**Column:**

30m x .25mm x .2um  
Rtx-CLP II (cat.# 11323)

**Carrier Gas:**

helium-constant pressure 20 psi.

**Temp. Program:**

200°C to 300°C  
@ 25°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

300°C

**Det. Type:**


ECD

**Split Vent:**

300 ml/min.

**Inj. Vol**

0.2µl

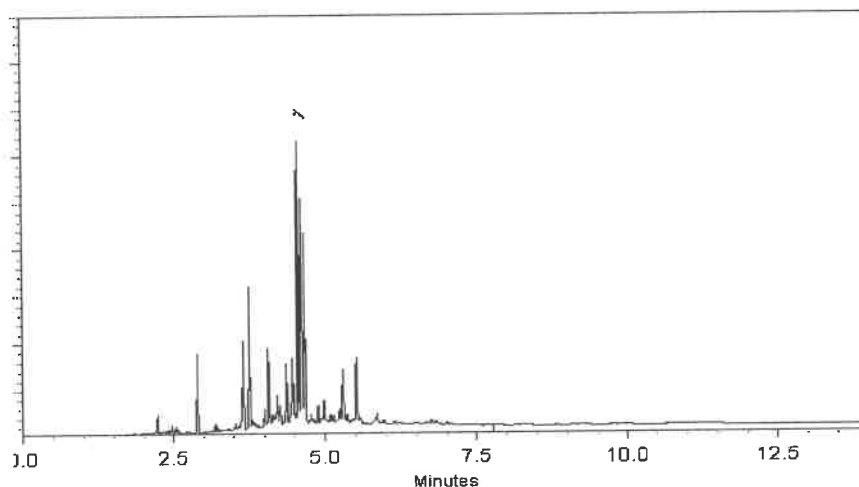

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Morgan Craighead - Mix Technician


Date Mixed: 11-May-2023

Balance Serial # 1128360905

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 16-May-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

P 12603 } (3)  
↓  
P 12605  
  
7/3/2023



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis *chromatographic plus*



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No.: 32021 Lot No.: A0197993  
Description: Chlordane Standard  
Chlordane Standard 1000µg/mL, Hexane, 1mL/ampul  
Container Size: 2 mL Pkg Amt: > 1 mL  
Expiration Date: August 31, 2029 Storage: 10°C or colder  
Ship: Ambient

*Handwritten:* P 12606, P 12610, 5 Five, 7/3/2023

#### CERTIFIED VALUES

| Elution Order | Compound                                                              | CAS #   | Lot #  | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty* (95% C.L.; K=2) |
|---------------|-----------------------------------------------------------------------|---------|--------|--------|-----------------------------|---------------------------------------|
| 1             | Chlordane<br>10% trans-Chlordane; 9% cis-Chlordane; 81% other isomers | 57-74-9 | 978545 | ----   | 1,005.0 µg/mL               | +/- 55.7700                           |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane  
CAS # 110-54-3  
Purity 99%

#### Tech Tips:

CAS #57-74-9 nomenclature is based on EPA method 8081B.

## Quality Confirmation Test

**Column:**

30m x .25mm x .2um  
Rtx-CLP II (cat.# 11323)

**Carrier Gas:**

helium-constant pressure 20 psi.

**Temp. Program:**

200°C to 300°C  
@ 25°C/min. { hold 10 min.}

**Inj. Temp:**

250°C

**Det. Temp:**

300°C

**Det. Type:**


ECD

**Split Vent:**

300 ml/min.

**Inj. Vol**

0.2µl

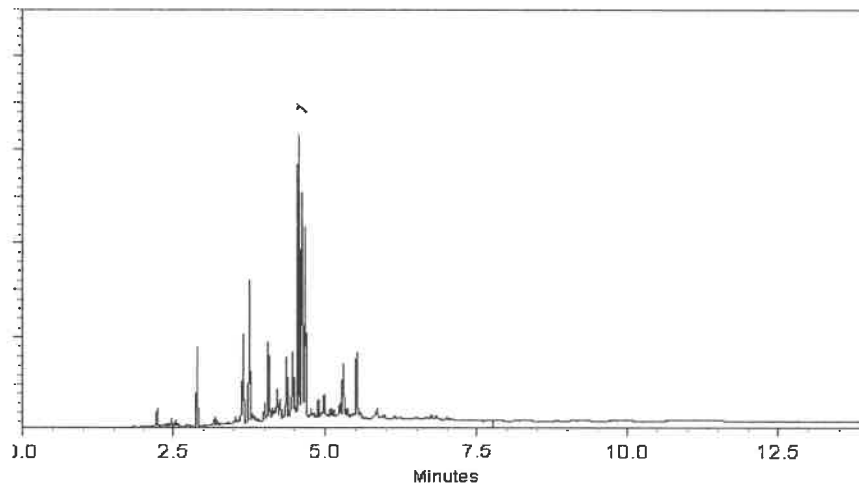

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Morgan Craighead - Mix Technician

Date Mixed: 11-May-2023

Balance Serial # 1128360905

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 16-May-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 32291

Lot No.: A0200423

Description : Organochlorine Pesticide Mix AB #1

Organochlorine Pesticide Mix AB #1 200µg/mL, Hexane/Toluene(50:50), 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : July 31, 2027

Storage: 10°C or colder

Ship: Ambient

P 13034  
↓  
P 13038  
12.26.2023

### CERTIFIED VALUES

| Elution Order | Compound                      | CAS #      | Lot #      | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|-------------------------------|------------|------------|--------|-----------------------------|----------------------------------------|
| 1             | alpha-BHC                     | 319-84-6   | 14434500   | 99%    | 200.5 µg/mL                 | +/- 8.9956                             |
| 2             | gamma-BHC (Lindane)           | 58-89-9    | 14184400   | 98%    | 199.9 µg/mL                 | +/- 8.9696                             |
| 3             | beta-BHC                      | 319-85-7   | BCCC6425   | 99%    | 200.0 µg/mL                 | +/- 8.9732                             |
| 4             | delta-BHC                     | 319-86-8   | 14450800   | 98%    | 199.9 µg/mL                 | +/- 8.9696                             |
| 5             | Heptachlor                    | 76-44-8    | 813251     | 99%    | 202.0 µg/mL                 | +/- 9.0629                             |
| 6             | Aldrin                        | 309-00-2   | 14389400   | 98%    | 200.9 µg/mL                 | +/- 9.0136                             |
| 7             | Heptachlor epoxide (isomer B) | 1024-57-3  | 14448800   | 99%    | 200.0 µg/mL                 | +/- 8.9732                             |
| 8             | trans-Chlordane               | 5103-74-2  | 34616      | 99%    | 200.5 µg/mL                 | +/- 8.9956                             |
| 9             | cis-Chlordane                 | 5103-71-9  | 31766      | 98%    | 201.4 µg/mL                 | +/- 9.0356                             |
| 10            | Endosulfan I                  | 959-98-8   | BCCF4060   | 99%    | 200.0 µg/mL                 | +/- 8.9732                             |
| 11            | 4,4'-DDE                      | 72-55-9    | GHYQG      | 99%    | 201.5 µg/mL                 | +/- 9.0405                             |
| 12            | Dieldrin                      | 60-57-1    | 14515000   | 98%    | 199.9 µg/mL                 | +/- 8.9696                             |
| 13            | Endrin                        | 72-20-8    | 14485300   | 98%    | 200.4 µg/mL                 | +/- 8.9916                             |
| 14            | 4,4'-DDD                      | 72-54-8    | HAN02      | 99%    | 200.5 µg/mL                 | +/- 8.9956                             |
| 15            | Endosulfan II                 | 33213-65-9 | 14374700   | 99%    | 200.0 µg/mL                 | +/- 8.9732                             |
| 16            | 4,4'-DDT                      | 50-29-3    | 230410JLMA | 98%    | 201.9 µg/mL                 | +/- 9.0575                             |

|    |                    |            |          |     |             |            |
|----|--------------------|------------|----------|-----|-------------|------------|
| 17 | Endrin aldehyde    | 7421-93-4  | 30720    | 98% | 201.4 µg/mL | +/- 9.0356 |
| 18 | Endosulfan sulfate | 1031-07-8  | BCCH9010 | 99% | 200.5 µg/mL | +/- 8.9956 |
| 19 | Methoxychlor       | 72-43-5    | 14563200 | 98% | 200.9 µg/mL | +/- 9.0136 |
| 20 | Endrin ketone      | 53494-70-5 | 14537700 | 98% | 199.9 µg/mL | +/- 8.9696 |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane/Toluene (50:50)  
**CAS #** 110-54-3/108-88-3  
**Purity** 99%

P13034  
P13038  
1  
5  
12/26/2023

## Quality Confirmation Test

**Column:**  
30m x .25mm x .2µm  
Rtx-CLP II (cat.# 11323)

**Carrier Gas:**  
helium-constant pressure 20 psi.

**Temp. Program:**  
150°C to 300°C  
@ 4°C/min. ( hold 5 min.)


**Inj. Temp:**  
200°C

**Det. Temp:**  
300°C

**Det. Type:**  
ECD

**Split Vent:**  
Split ratio 50:1

**Inj. Vol**  
1µl

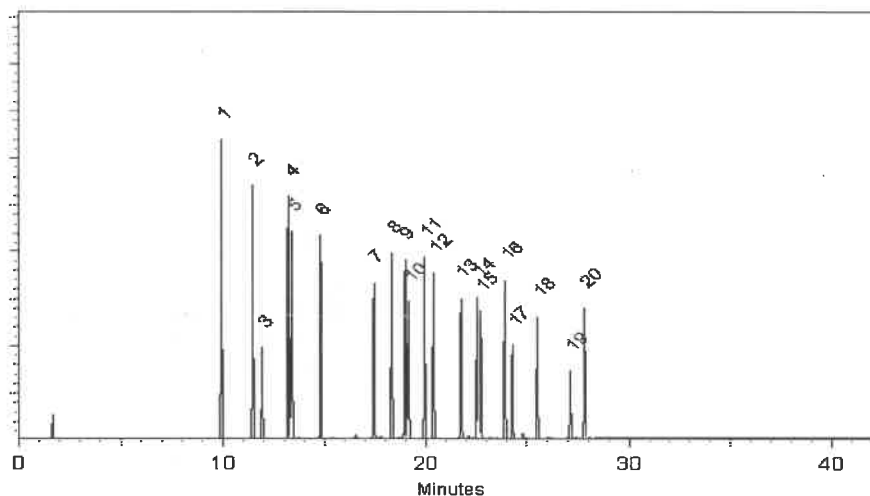

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Sam Moodler*  
Sam Moodler - Operations Tech I

**Date Mixed:** 31-Jul-2023

**Balance Serial #** B442140311

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 03-Aug-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



## CERTIFIED WEIGHT REPORT

Part Number: **19161**  
 Lot Number: **013124**  
 Description: **CLP Pesticides & PCB's Resolution Check Standard**  
 9 components  
 Expiration Date: **013129**  
 Recommended Storage: **Refrigerate (4 °C)**  
 Nominal Concentration (µg/mL): **Varied**  
 NIST Test ID#: **6UTB**

Solvent(s):  
 Hexane 273615 (50%)  
 Toluene 28508 (50%)

Volume(s) shown below were combined and diluted to (mL): 100.0 5E-05 Balance Uncertainty  
 0.021 Flask Uncertainty

|                |                 |        |
|----------------|-----------------|--------|
|                |                 | 013124 |
| Formulated By: | Lawrence Barry  | DATE   |
|                |                 | 013124 |
| Reviewed By:   | Pedro L. Rentas | DATE   |

| Compound                        | Part Number | Lot Number | Dil. Factor | Initial Vol. (mL) | Uncertainty Pipette (mL) | Initial Conc.(ug/mL) | Final Conc.(ug/mL) | Expanded Uncertainty (+/-) µg/mL | SDS Information<br>(Solvent Safety Info. On Attached pg.) |                  |                    |
|---------------------------------|-------------|------------|-------------|-------------------|--------------------------|----------------------|--------------------|----------------------------------|-----------------------------------------------------------|------------------|--------------------|
|                                 |             |            |             |                   |                          |                      |                    |                                  | CAS#                                                      | OSHA PEL (TWA)   | LD50               |
| 1. trans-Chlordane              | 19361       | 013124     | 0.010       | 1.00              | 0.004                    | 101.3                | 1.0                | 0.02                             | 5103-74-2                                                 | 0.5mg/m3 (skin)  | ori-rat 500mg/kg   |
| 2. Endosulfan I                 | 19361       | 013124     | 0.010       | 1.00              | 0.004                    | 101.3                | 1.0                | 0.02                             | 959-98-8                                                  | 0.1mg/m3 (skin)  | ori-rat 18mg/kg    |
| 3. 4,4'-DDE                     | 19361       | 013124     | 0.010       | 1.00              | 0.004                    | 201.6                | 2.0                | 0.03                             | 72-55-9                                                   | N/A              | ori-rat 880mg/kg   |
| 4. Dieldrin                     | 19361       | 013124     | 0.010       | 1.00              | 0.004                    | 202.8                | 2.0                | 0.03                             | 60-57-1                                                   | 0.25mg/m3 (skin) | ori-rat 38300ug/kg |
| 5. Endosulfan sulfate           | 19361       | 013124     | 0.010       | 1.00              | 0.004                    | 204.2                | 2.0                | 0.03                             | 1031-07-8                                                 | N/A              | ori-rat 18mg/kg    |
| 6. Endrin ketone                | 19361       | 013124     | 0.010       | 1.00              | 0.004                    | 202.6                | 2.0                | 0.03                             | 53494-70-5                                                | N/A              | N/A                |
| 7. 4,4'-Methoxychlor            | 19361       | 013124     | 0.010       | 1.00              | 0.004                    | 1000.7               | 10.0               | 0.09                             | 72-43-5                                                   | 10mg/m3          | ori-rat 6000mg/kg  |
| 8. 2,4,5,6-Tetrachloro-m-xylene | 19361       | 013124     | 0.010       | 1.00              | 0.004                    | 202.6                | 2.0                | 0.03                             | 877-09-8                                                  | N/A              | N/A                |
| 9. Decachlorobiphenyl (209)     | 19361       | 013124     | 0.010       | 1.00              | 0.004                    | 202.0                | 2.0                | 0.03                             | 2051-24-3                                                 | N/A              | N/A                |

• The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.  
 • Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).  
 • Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.  
 • All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.  
 • Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

P13243 } (5)  
 ↓  
 P13247 }  
 ↓  
 02/9/2024



110 Benner Circle  
Belleville, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



## FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32005 **Lot No.:** A0203038

**Description :** Toxaphene Standard  
Toxaphene Standard 1000 µg/mL, Hexane, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** January 31, 2028 **Storage:** 10°C or colder

**Ship:** Ambient

## CERTIFIED VALUES

| Elution Order | Compound  | CAS #     | Lot #   | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|-----------|-----------|---------|--------|-----------------------------|----------------------------------------|
| 1             | Toxaphene | 8001-35-2 | 1051817 | —%     | 1,009.0 µg/mL               | +/- 55.9920                            |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

P13773  
↓  
P13779  
AI  
11/19/24

05-06-2024

## Quality Confirmation Test

**Column:**

30m x .25mm x .2um  
Rtx-CLP II (cat.# 11323)

**Carrier Gas:**

helium-constant pressure 20 psi.

**Temp. Program:**

200°C to 300°C  
@ 25°C/min. ( hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

300°C

**Det. Type:**


ECD

**Split Vent:**

300 ml/min.

**Inj. Vol**

0.2µl

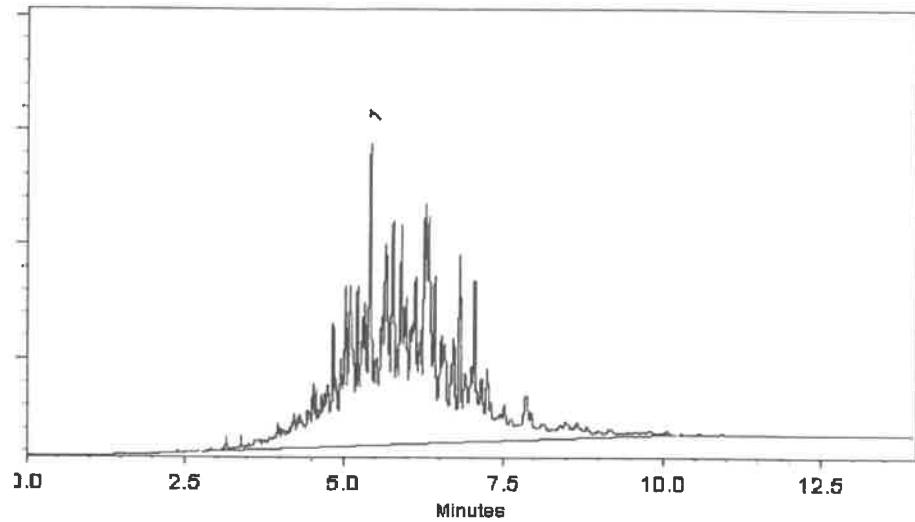

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Dakota Parson - Operations Technician I


Date Mixed: 10-Oct-2023

Balance Serial # 1128353505

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 16-Oct-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

  
P13338  
↓  
P13389  
P13773  
↓  
P13779  
AJ  
11/19/24  
05-06-2024



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32074 **Lot No.:** A0213999

**Description :** Pesticide Performance Eval Mix w/Surrogate

Performance Evaluation Std. 3/90 SOW w/surrogates 1-25µg/mL,  
Hexane, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** July 31, 2028 **Storage:** 10°C or colder

**Handling:** Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13780  
↓  
P13784  
AJ  
11/19/24

## CERTIFIED VALUES

| Elution Order | Compound                     | CAS #     | Lot #     | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------------|-----------|-----------|--------|-----------------------------|----------------------------------------|
| 1             | 2,4,5,6-Tetrachloro-m-xylene | 877-09-8  | RP220407  | 99%    | 2.0 µg/mL                   | +/- 0.1506                             |
| 2             | alpha-BHC                    | 319-84-6  | 15279000  | 99%    | 1.0 µg/mL                   | +/- 0.0749                             |
| 3             | gamma-BHC (Lindane)          | 58-89-9   | 14931300  | 97%    | 1.0 µg/mL                   | +/- 0.0756                             |
| 4             | beta-BHC                     | 319-85-7  | BCCC6425  | 99%    | 1.0 µg/mL                   | +/- 0.0749                             |
| 5             | Endrin                       | 72-20-8   | 15076100  | 98%    | 5.0 µg/mL                   | +/- 0.3769                             |
| 6             | 4,4'-DDT                     | 50-29-3   | 231103JLM | 97%    | 10.0 µg/mL                  | +/- 0.7512                             |
| 7             | Methoxychlor                 | 72-43-5   | 14979500  | 98%    | 24.8 µg/mL                  | +/- 1.8543                             |
| 8             | Decachlorobiphenyl (BZ# 209) | 2051-24-3 | 30638     | 99%    | 2.0 µg/mL                   | +/- 0.1513                             |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

### Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

## Quality Confirmation Test

### Column:

30m x .25mm x .2µm  
Rtx-CLP II (cat.# 11323)

### Carrier Gas:

helium-constant pressure 20 psi.

### Temp. Program:

150°C to 300°C  
@ 4°C/min. (hold 5 min.)

### Inj. Temp:

200°C

### Det. Temp:

300°C

### Det. Type:


ECD

### Split Vent:


Split ratio 50:1

### Inj. Vol

1µl

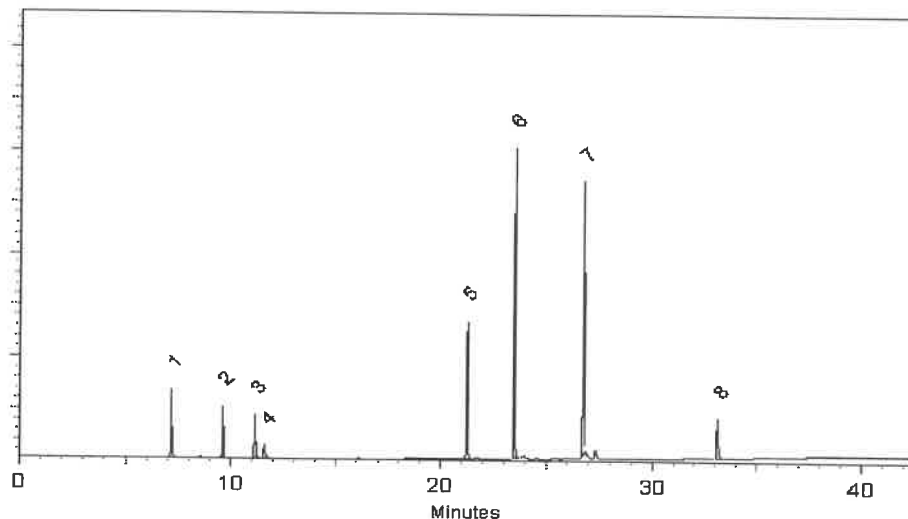

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Malina Homan - Operations Technician I

Date Mixed: 17-Jul-2024

Balance Serial # 1128353505

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 31-Jul-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



## FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32000 **Lot No.:** A0214495

**Description :** Pesticide Surrogate Mix  
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** October 31, 2030 **Storage:** 10°C or colder

**Handling:** Contains PCBs - sonicate prior to use. **Ship:** Ambient

P19785  
↓  
P19789  
AJ  
11/19/24

## CERTIFIED VALUES

| Elution Order | Compound                     | CAS #     | Lot #    | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------------|-----------|----------|--------|-----------------------------|----------------------------------------|
| 1             | 2,4,5,6-Tetrachloro-m-xylene | 877-09-8  | RP220407 | 99%    | 200.2 µg/mL                 | +/- 11.1087                            |
| 2             | Decachlorobiphenyl (BZ# 209) | 2051-24-3 | 30679    | 99%    | 201.4 µg/mL                 | +/- 11.1753                            |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone  
**CAS #** 67-64-1  
**Purity** 99%

### Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

# Quality Confirmation Test

**Column:**

30m x .25mm x .2um  
Rtx-CLP II (cat.# 11323)

**Carrier Gas:**

helium-constant pressure 20 psi.

**Temp. Program:**

200°C to 300°C  
@ 25°C/min. ( hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

300°C

**Det. Type:**


ECD

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

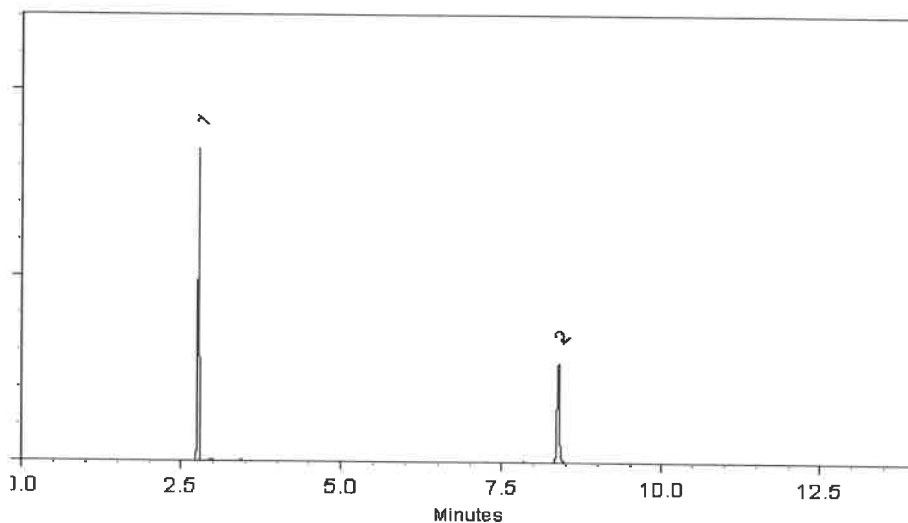

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*A.O.E.*  
Aaron Enyart - Operations Tech I

Date Mixed: 29-Jul-2024

Balance Serial # B345965662

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 01-Aug-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



## FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32000 **Lot No.:** A0214495

**Description :** Pesticide Surrogate Mix  
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** October 31, 2030 **Storage:** 10°C or colder

**Handling:** Contains PCBs - sonicate prior to use. **Ship:** Ambient

P19785  
↓  
P19789  
AJ  
11/19/24

## CERTIFIED VALUES

| Elution Order | Compound                     | CAS #     | Lot #    | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------------|-----------|----------|--------|-----------------------------|----------------------------------------|
| 1             | 2,4,5,6-Tetrachloro-m-xylene | 877-09-8  | RP220407 | 99%    | 200.2 µg/mL                 | +/- 11.1087                            |
| 2             | Decachlorobiphenyl (BZ# 209) | 2051-24-3 | 30679    | 99%    | 201.4 µg/mL                 | +/- 11.1753                            |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone  
**CAS #** 67-64-1  
**Purity** 99%

### Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

# Quality Confirmation Test

**Column:**

30m x .25mm x .2um  
Rtx-CLP II (cat.# 11323)

**Carrier Gas:**

helium-constant pressure 20 psi.

**Temp. Program:**

200°C to 300°C  
@ 25°C/min. ( hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

300°C

**Det. Type:**


ECD

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

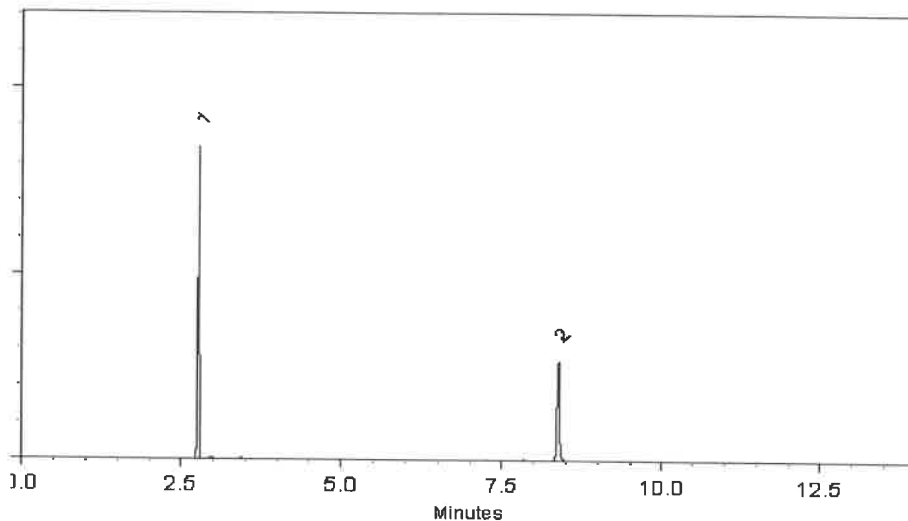

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*A.O.E.*  
Aaron Enyart - Operations Tech I

Date Mixed: 29-Jul-2024

Balance Serial # B345965662

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 01-Aug-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



## FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32005 **Lot No.:** A0210240

**Description :** Toxaphene Standard  
Toxaphene Standard 1000 µg/mL, Hexane, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** July 31, 2028 **Storage:** 10°C or colder

**Ship:** Ambient

## CERTIFIED VALUES

| Elution Order | Compound  | CAS #     | Lot #   | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|-----------|-----------|---------|--------|-----------------------------|----------------------------------------|
| 1             | Toxaphene | 8001-35-2 | 1051817 | ----%  | 1,009.3 µg/mL               | +/- 56.0105                            |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

P13861  
P13862

12/9/2024

## Quality Confirmation Test

**Column:**

30m x .25mm x .2um  
Rtx-CLP II (cat.# 11323)

**Carrier Gas:**

helium-constant pressure 20 psi.

**Temp. Program:**

200°C to 300°C  
@ 25°C/min. ( hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

300°C

**Det. Type:**


ECD

**Split Vent:**

300 ml/min.

**Inj. Vol**

0.2µl

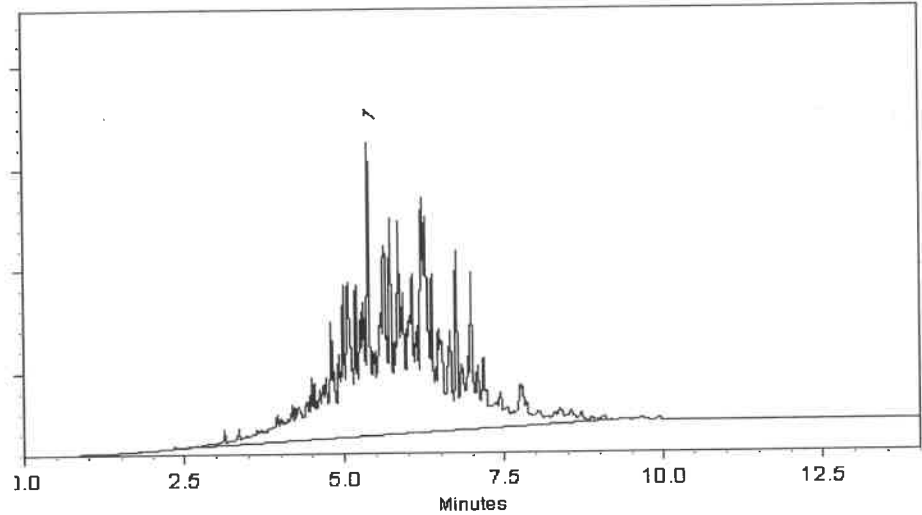

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Amanda Miller - Operations Tech III - ARM QC

Date Mixed: 11-Apr-2024

Balance Serial # B442140311

  
Christie Mills - Operations Lead Tech - ARM QC

Date Passed: 26-Apr-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

P13861 } ②  
P13862 }

  
12/9/2024



**CERTIFIED WEIGHT REPORT**

Part Number: **72072**  
Lot Number: **112018**  
Description: **n-Tetracosane-d50**  
Expiration Date: **112028**  
Recommended Storage: **Ambient (20 °C)**  
Nominal Concentration (µg/mL): **1000**  
NIST Test ID#: **2684186**  
Weight(s) shown below were combined and diluted to (mL): **200.0**

Solvent(s): **Methylene chloride**  
Lot#: **102669**




Received by  
SG on 11/1/19  
P9044 - P9053

5E-05 Balance Uncertainty  
0.058 Flask Uncertainty


|                |                  |        |
|----------------|------------------|--------|
|                |                  | 112018 |
| Formulated By: | Prashant Chauhan | DATE   |
|                |                  | 112018 |
| Reviewed By:   | Pedro Rentas     | DATE   |

| Compound             | RM#  | Lot Number        | Nominal Conc (µg/mL) | Purity (%) | Uncertainty Purity | Target Weight(g) | Actual Weight(g) | Actual Conc (µg/mL) | Expanded Uncertainty (+/-) (µg/mL) | SDS Information (Solvent Safety Info. On Attached pg.) |                |      |
|----------------------|------|-------------------|----------------------|------------|--------------------|------------------|------------------|---------------------|------------------------------------|--------------------------------------------------------|----------------|------|
|                      |      |                   |                      |            |                    |                  |                  |                     |                                    | CAS#                                                   | OSHA PEL (TWA) | LD50 |
| 1. n-Tetracosane-d50 | 2072 | PR-17753/09216TC1 | 1000                 | 98         | 0.2                | 0.20411          | 0.20415          | 1000.2              | 4.2                                | 16416-32-3                                             | N/A            | N/A  |

**Method GC8MSD-3.M:** Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

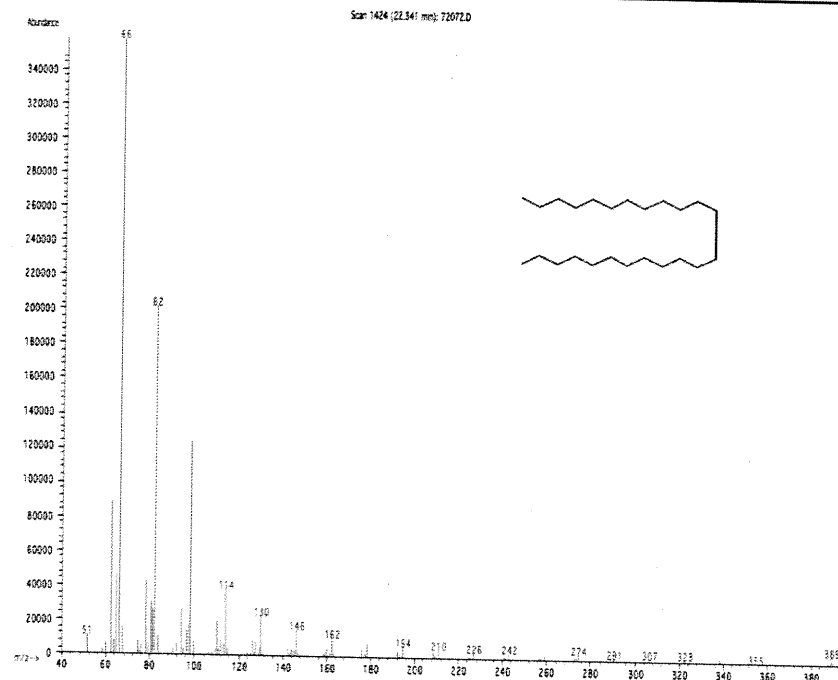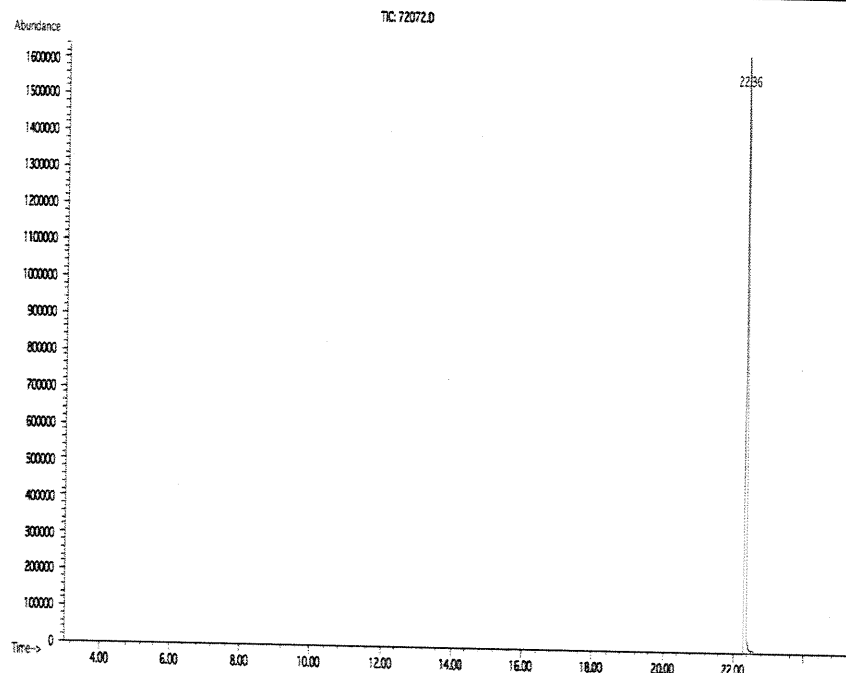

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



## Run 40, "P72072 L112018 [1000µg/mL in MeCl2]"

Run Length: 35.00 min, 20999 points at 10 points/second.

Created: Thu, Nov 22, 2018 at 7:23:18 AM.

Sampled: Sequence "112018-GC4M1", Method "GC4-M1".

Analyzed using Method "GC4-M1".

### Comments

GC4-M1 Analysis by Melissa Stonier

Column ID SPB5 L#60062-01A : 30 meter x 0.53mm x 1.5µm Film Thickness

Flow rates: Total Flow = 300 mL/min, Helium (carrier) = 6.5 mL, Helium (make-up) = 25 mL, Hydrogen (detector) = 30 mL, Air (detector) = 360 mL

Oven Temp 1 = 50°C (1 min), Rate = 10°C/min, Oven Temp 2 = 300°C (9 min), Total Run Time = 35 Minutes.

Injector Temp = 200°C, FID Temp = 300°C, FID Signal = eDag Channel 1.

Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3

