
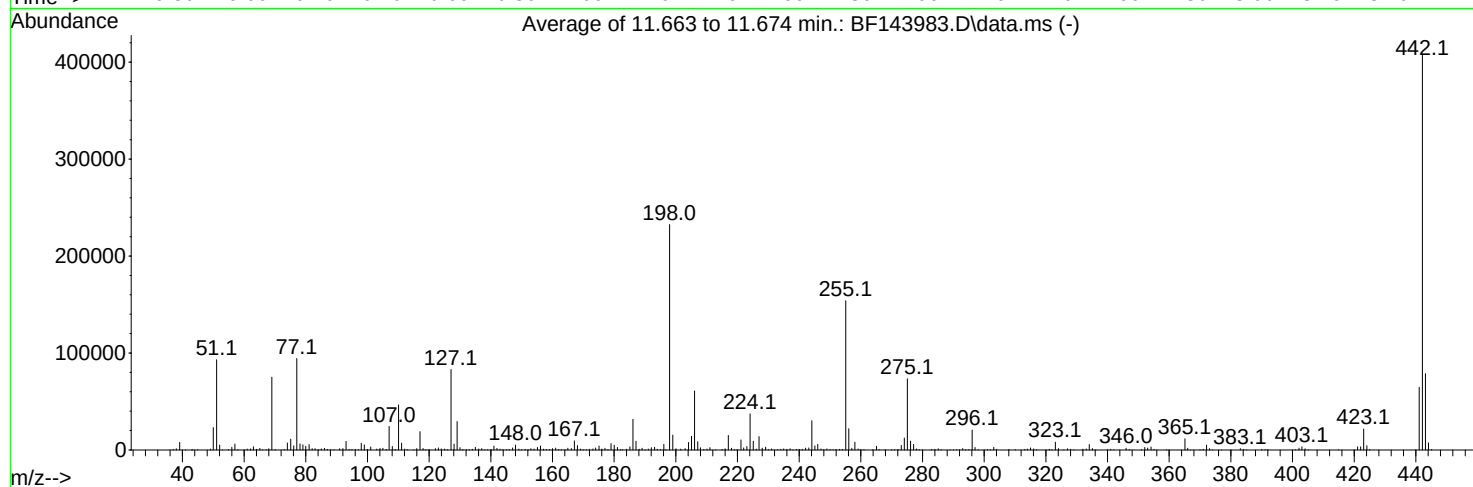


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101725\
Data File : BF143983.D
Acq On : 17 Oct 2025 14:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 06 15:29:47 2025

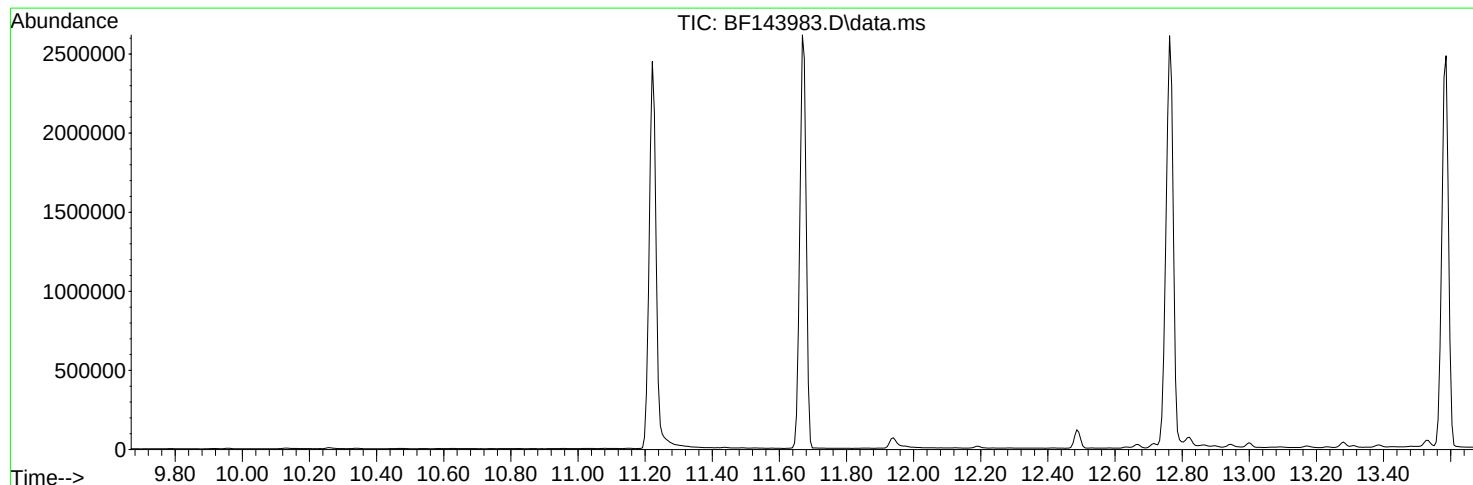




AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.7	1265	PASS
69	69	100	100	100.0	75069	PASS
70	69	0.00	2	0.6	457	PASS
197	198	0.00	2	0.1	330	PASS
198	198	100	100	100.0	232405	PASS
199	198	5	9	6.6	15290	PASS
365	198	1	100	5.0	11551	PASS
441	443	0.01	150	82.2	64648	PASS
442	442	100	100	100.0	407253	PASS
443	442	15	24	19.3	78603	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101725\
Data File : BF143983.D
Acq On : 17 Oct 2025 14:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 17 15:40:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

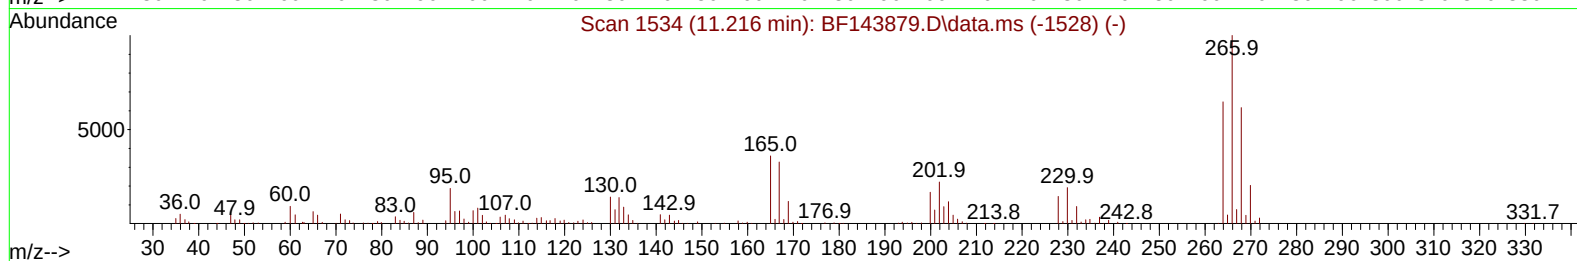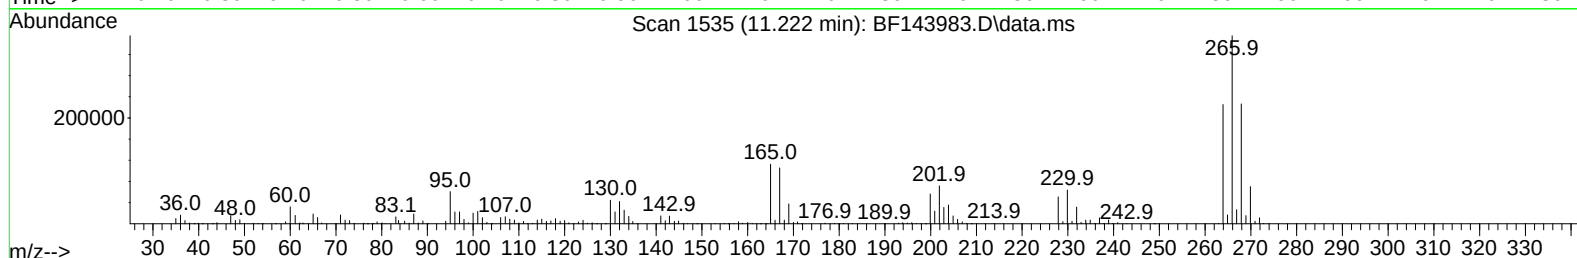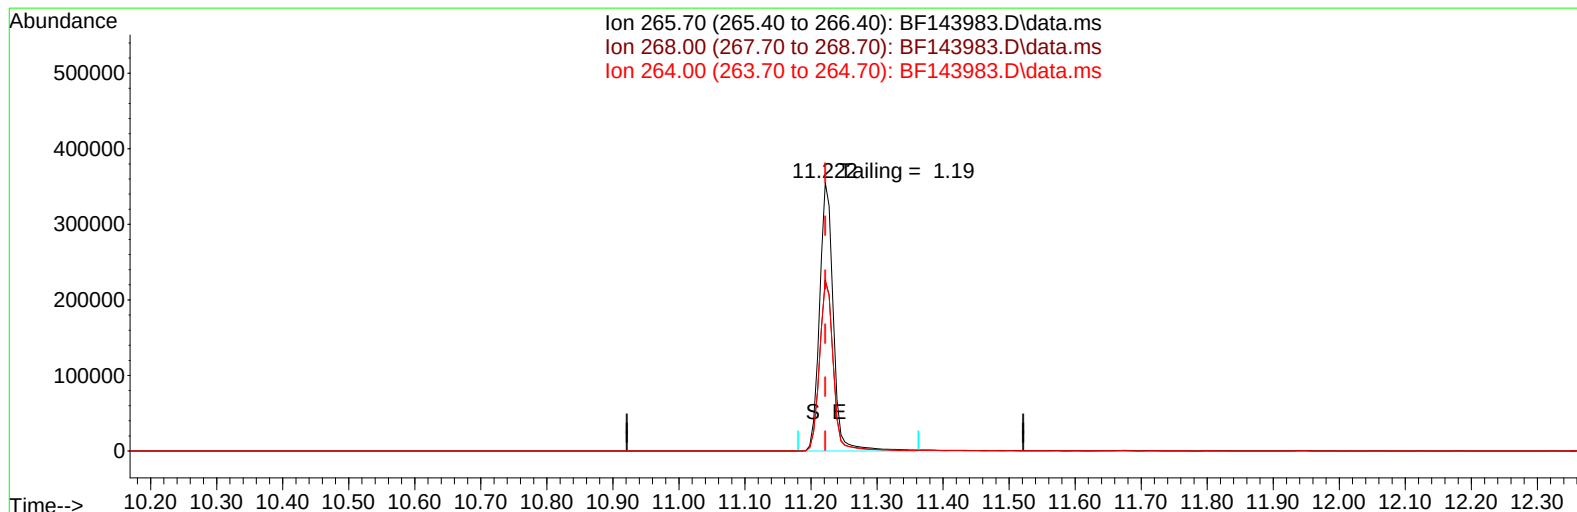

TIC: BF143983.D\data.ms

(70) Pentachlorophenol (C)

11.222min (+ 0.000) 1324535.20 ng




response 515849

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	63.73
264.00	64.70	63.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101725\
Data File : BF143983.D
Acq On : 17 Oct 2025 14:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 17 15:40:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

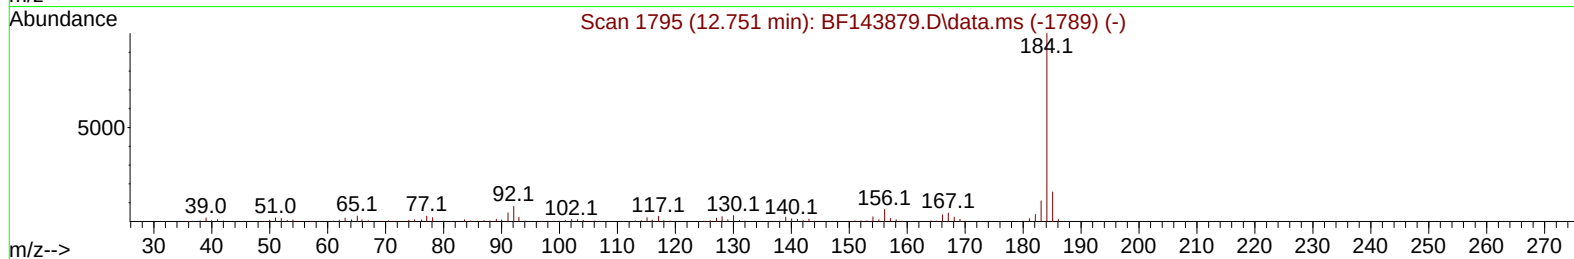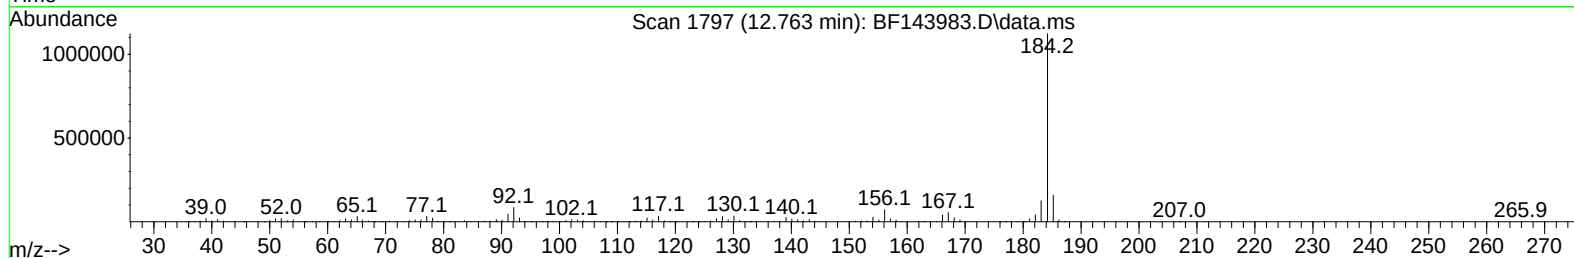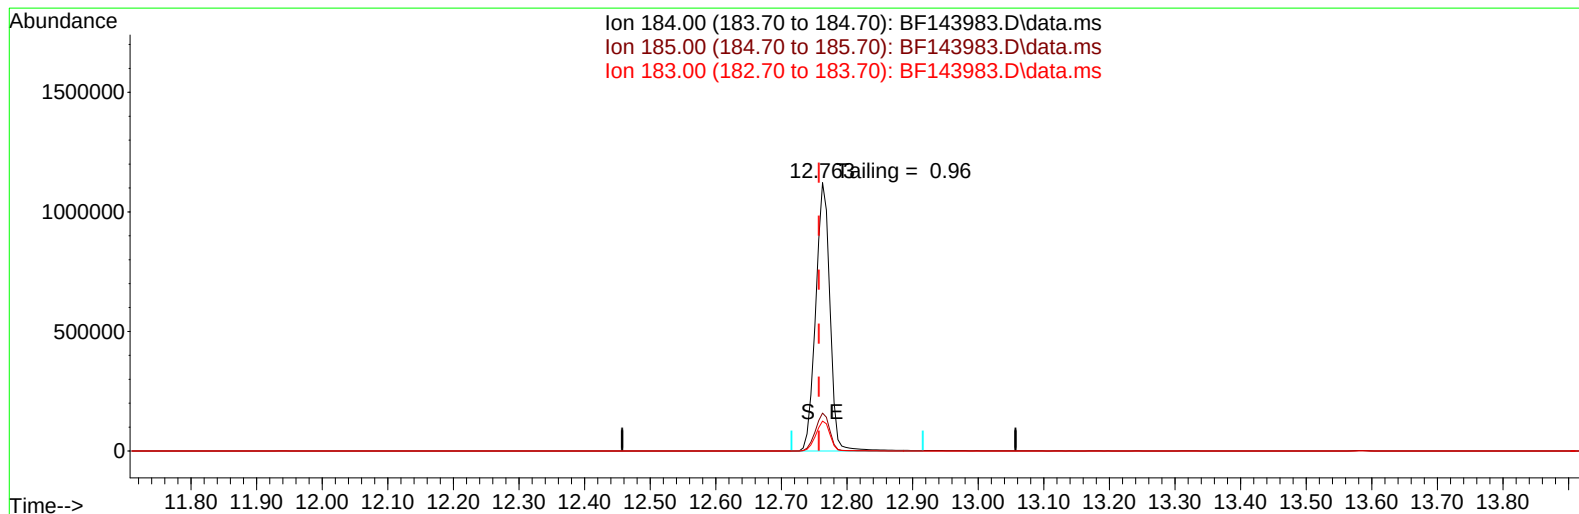

TIC: BF143983.D\data.ms

(77) Benzidine

12.763min (+ 0.006) 0.00 ng

response 1703588

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.18
183.00	11.00	11.18
0.00	0.00	0.00

Instrument :
BNA_F
ClientSampleId :
DFTPP

DDT Breakdown		
Date	Instrument Name	DFTPP Data File
10/17/2025	BNA_F	BF143983.D
Compound Name	Response	Retention Time
DDT	723581	13.586
DDD	14575	13.28
DDE	5521	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20096	743677	2.70