


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101725\
Data File : BG064530.D
Acq On : 17 Oct 2025 10:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 02 16:40:42 2025

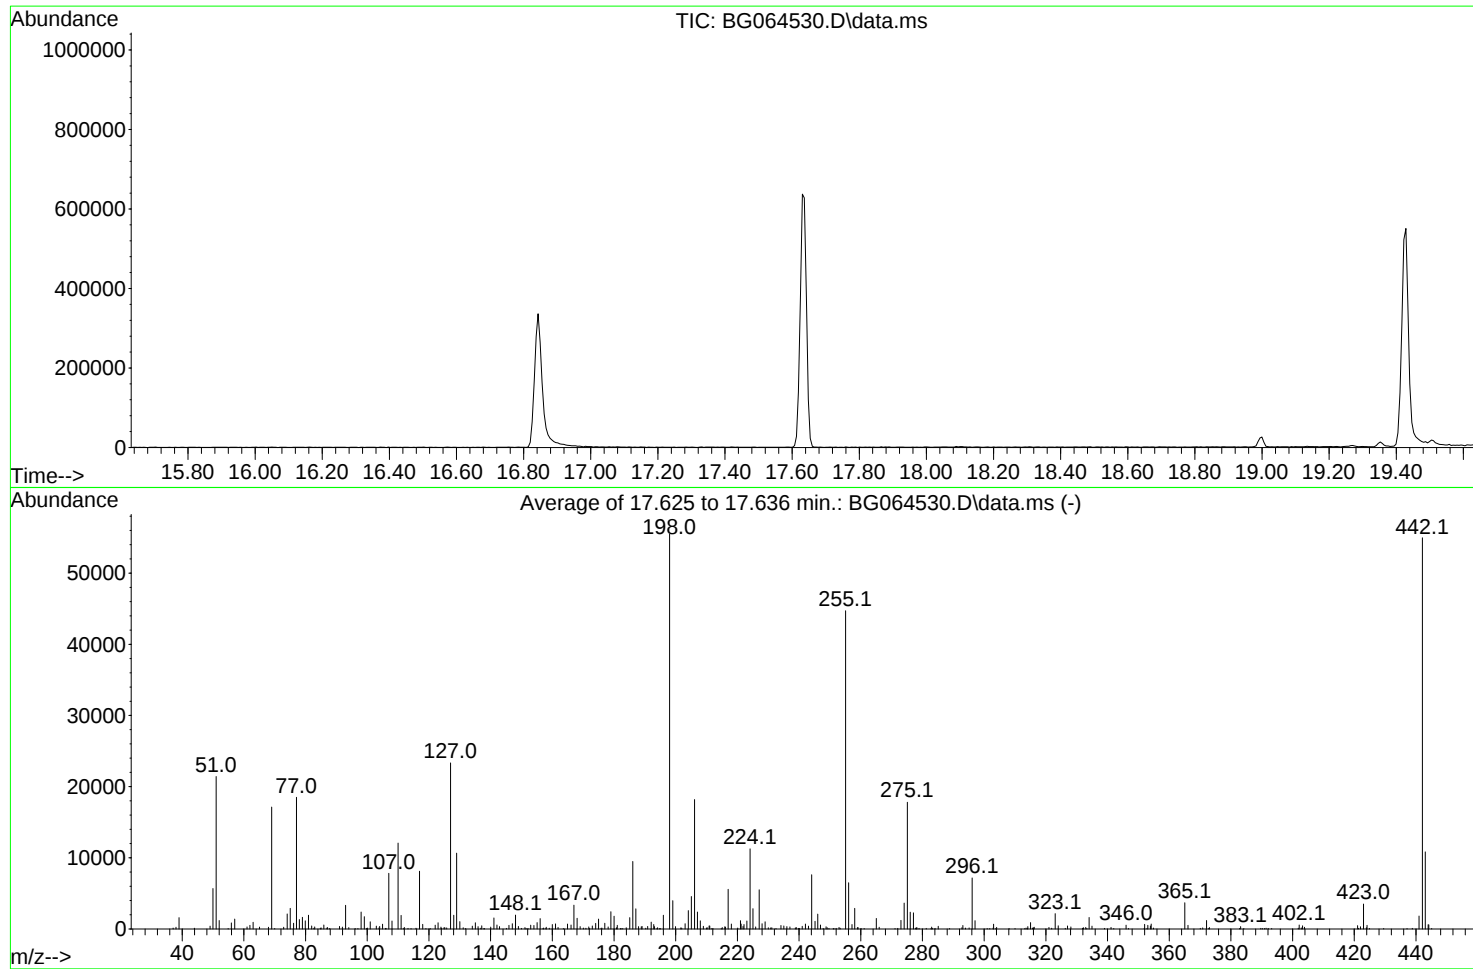




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2468

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.4	234	PASS
69	69	100	100	100.0	17124	PASS
70	69	0.00	2	0.4	68	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55491	PASS
199	198	5	9	7.2	3979	PASS
365	198	1	100	6.6	3684	PASS
441	443	0.01	150	16.7	1803	PASS
442	442	100	100	100.0	54965	PASS
443	442	15	24	19.7	10823	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101725\
Data File : BG064530.D
Acq On : 17 Oct 2025 10:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 17 11:35:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 02 16:40:42 2025
Response via : Initial Calibration

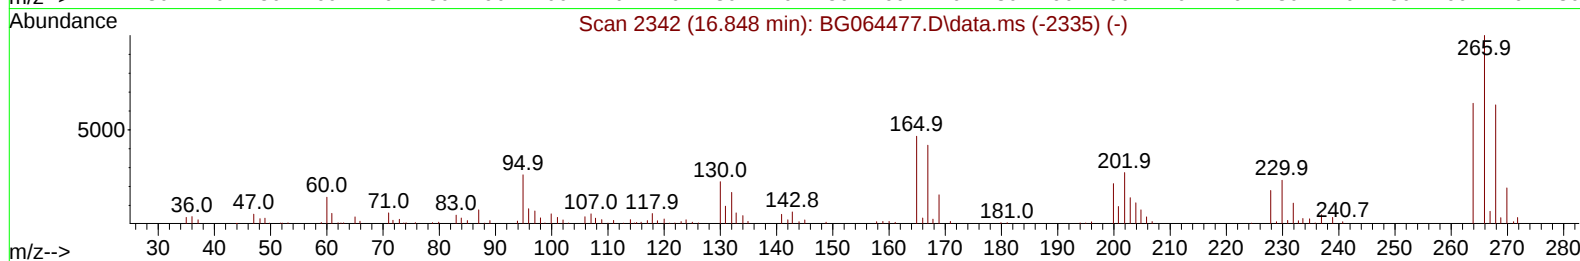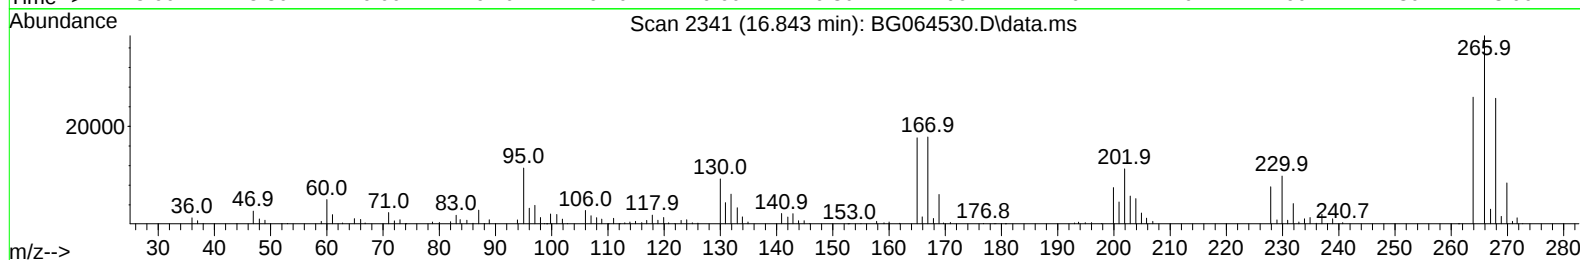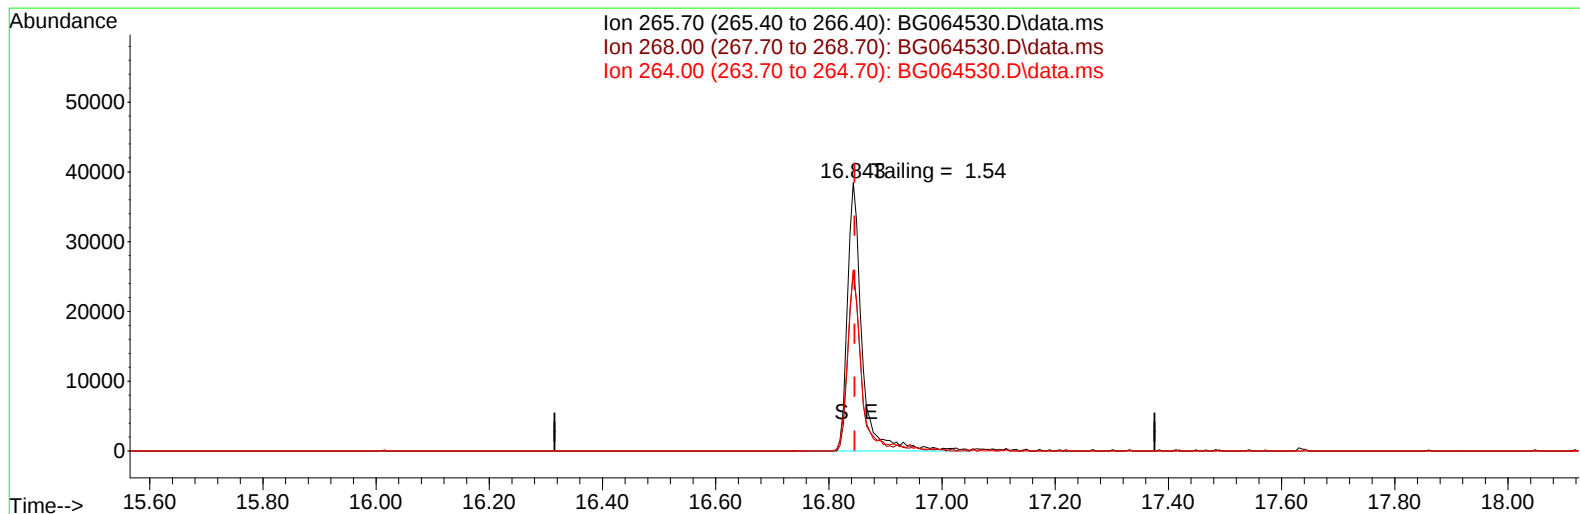

TIC: BG064530.D\data.ms

(70) Pentachlorophenol (C)

16.843min (-0.002) 25263.60 ng




response 67429

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	66.85
264.00	64.00	67.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101725\
Data File : BG064530.D
Acq On : 17 Oct 2025 10:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 17 11:35:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 02 16:40:42 2025
Response via : Initial Calibration

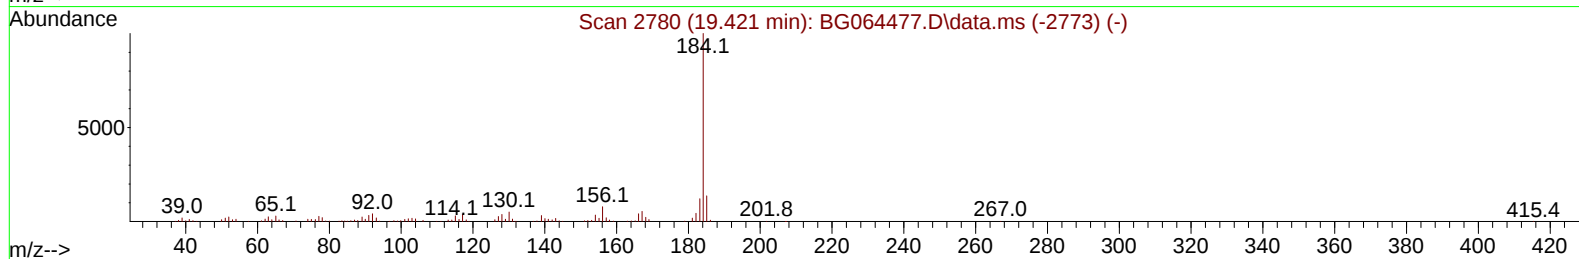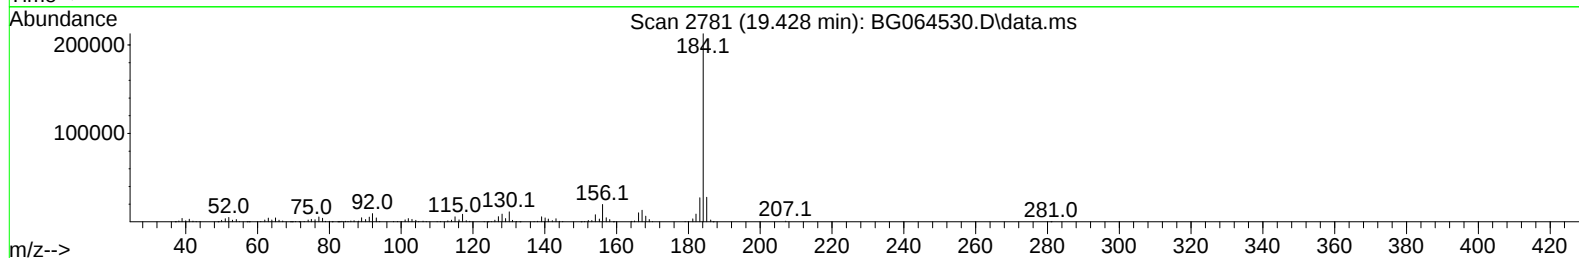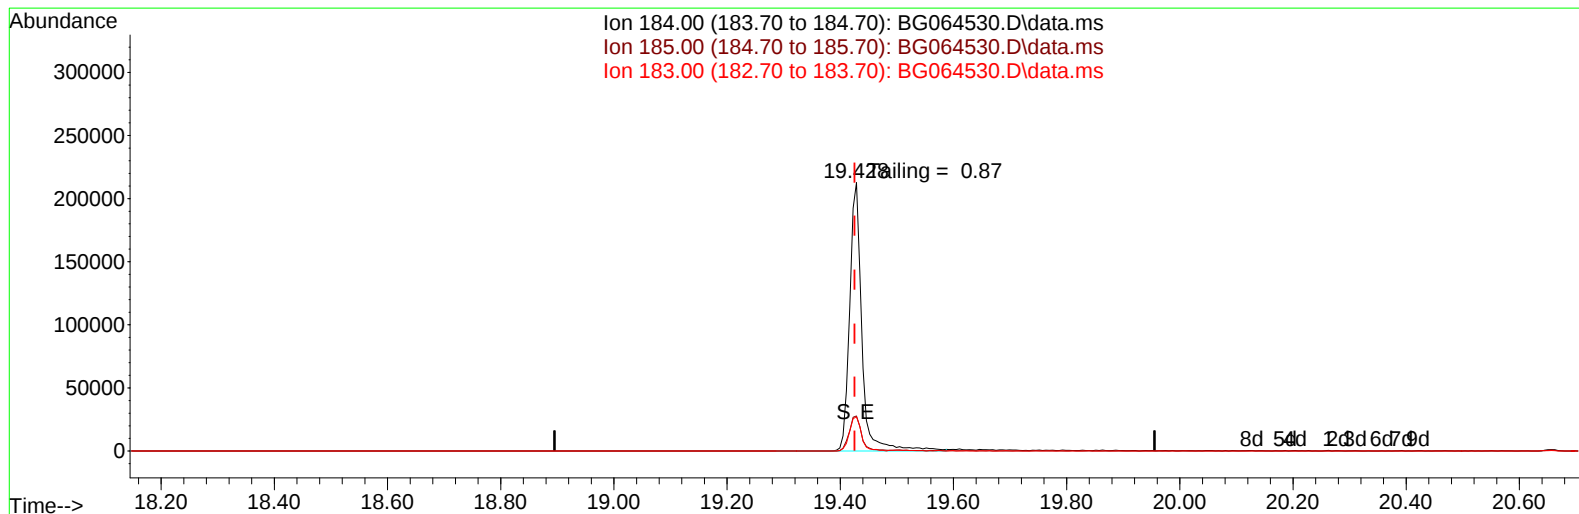

TIC: BG064530.D\data.ms

(77) Benzidine

19.428min (+ 0.003) 197325.20 ng m

response 319160

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.09
183.00	12.20	12.79
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/17/2025	BNA_G	<u>BG064530.D</u>
Compound Name	Response	Retention Time
DDT	235454	20.656
DDD	2620	20.216
DDE	61	19.946
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2681	238135	1.13

Instrument :
BNA_G
ClientSampleId :
DFTPP