


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101525\
Data File : BP025971.D
Acq On : 15 Oct 2025 11:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP101525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 15 23:48:51 2025

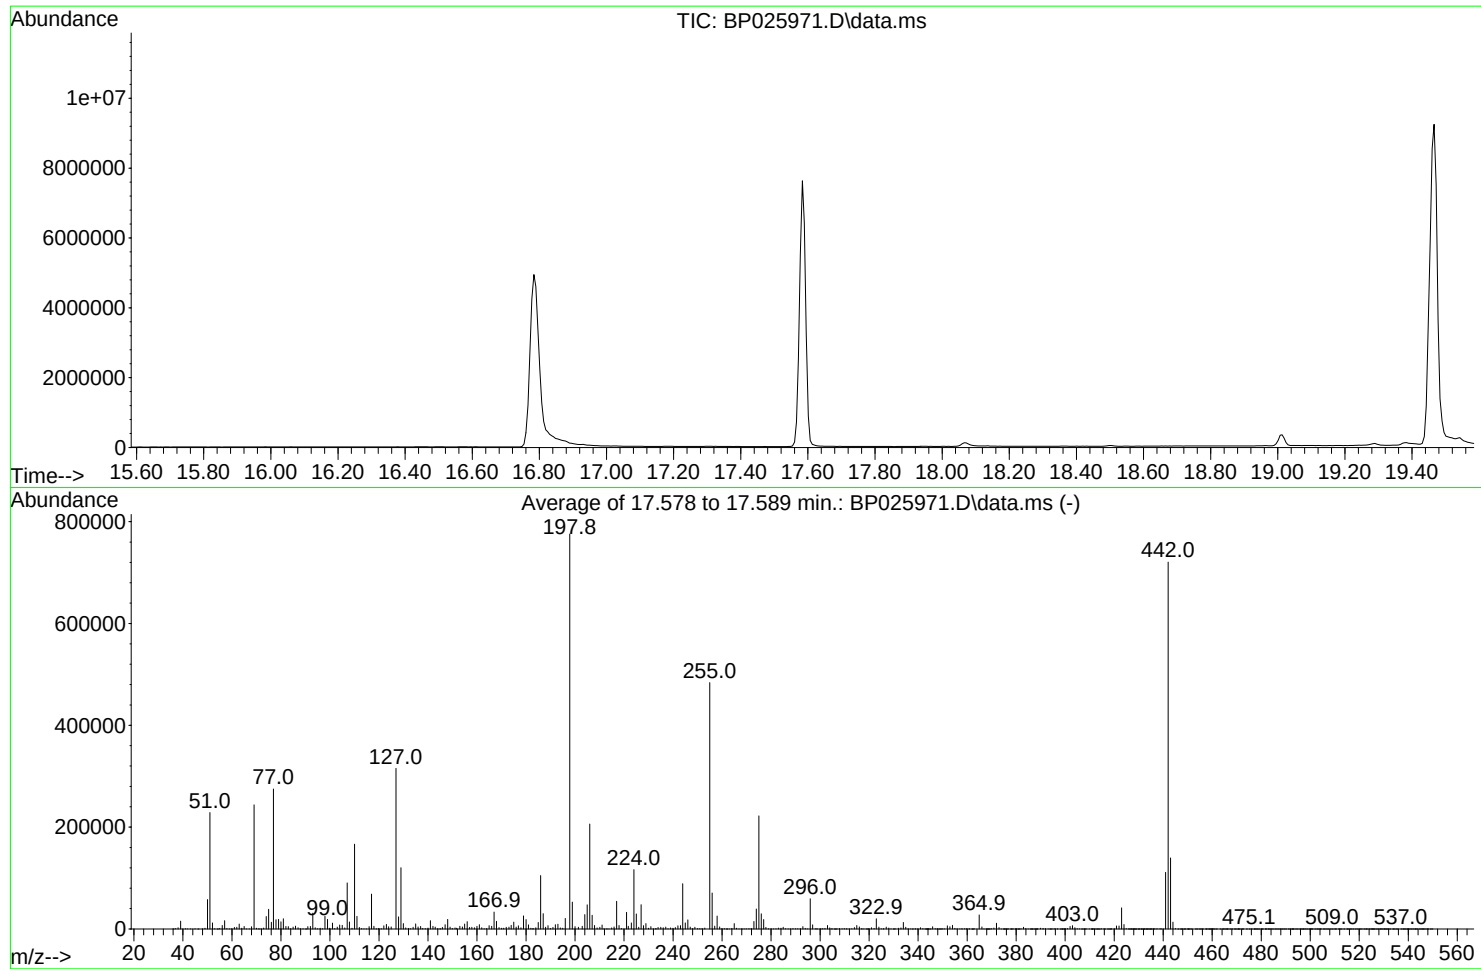

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2480

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	4327	PASS
69	69	100	100	100.0	243851	PASS
70	69	0.00	2	0.6	1362	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	775661	PASS
199	198	5	9	6.8	52652	PASS
365	198	1	100	3.6	27562	PASS
441	443	0.01	150	79.8	111264	PASS
442	442	100	100	100.0	720555	PASS
443	442	15	24	19.3	139424	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/15/2025	BNA_P	<u>BP025971.D</u>
Compound Name	Response	Retention Time
DDT	3045613	20.742
DDD	21056	20.33
DDE	939	19.007
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21995	3067608	0.72

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101525\
Data File : BP025971.D
Acq On : 15 Oct 2025 11:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Oct 17 00:50:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP101525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 15 23:48:51 2025
Response via : Initial Calibration

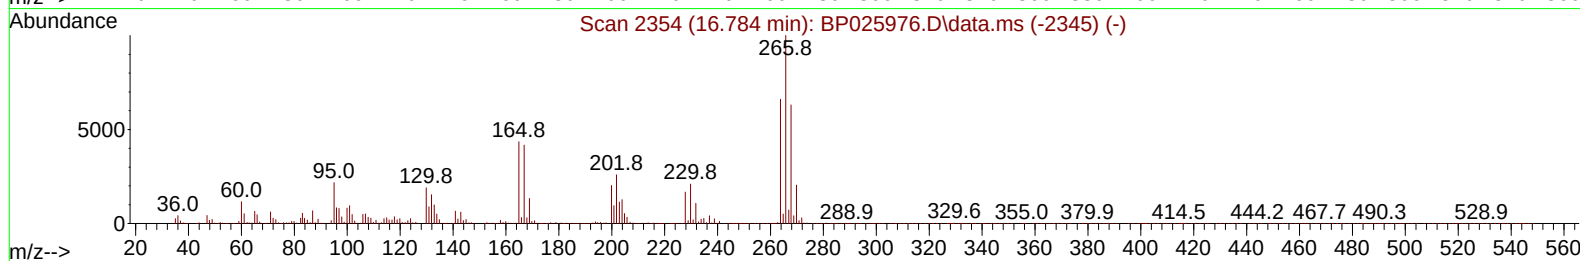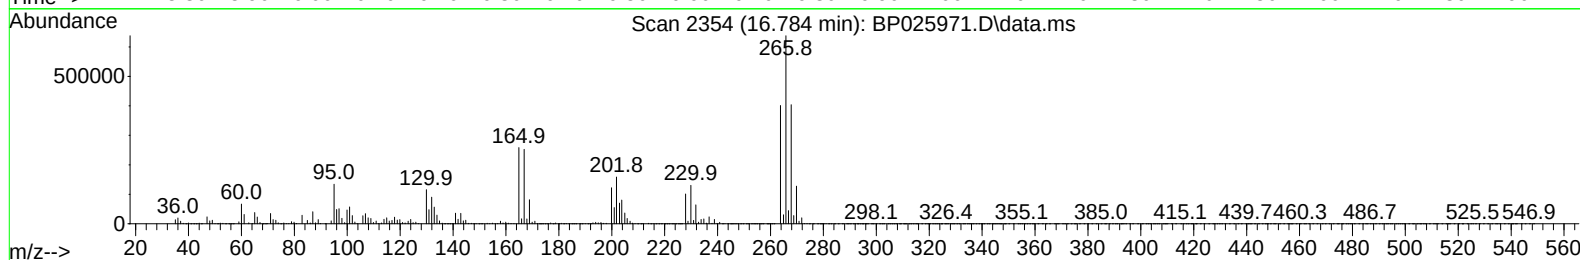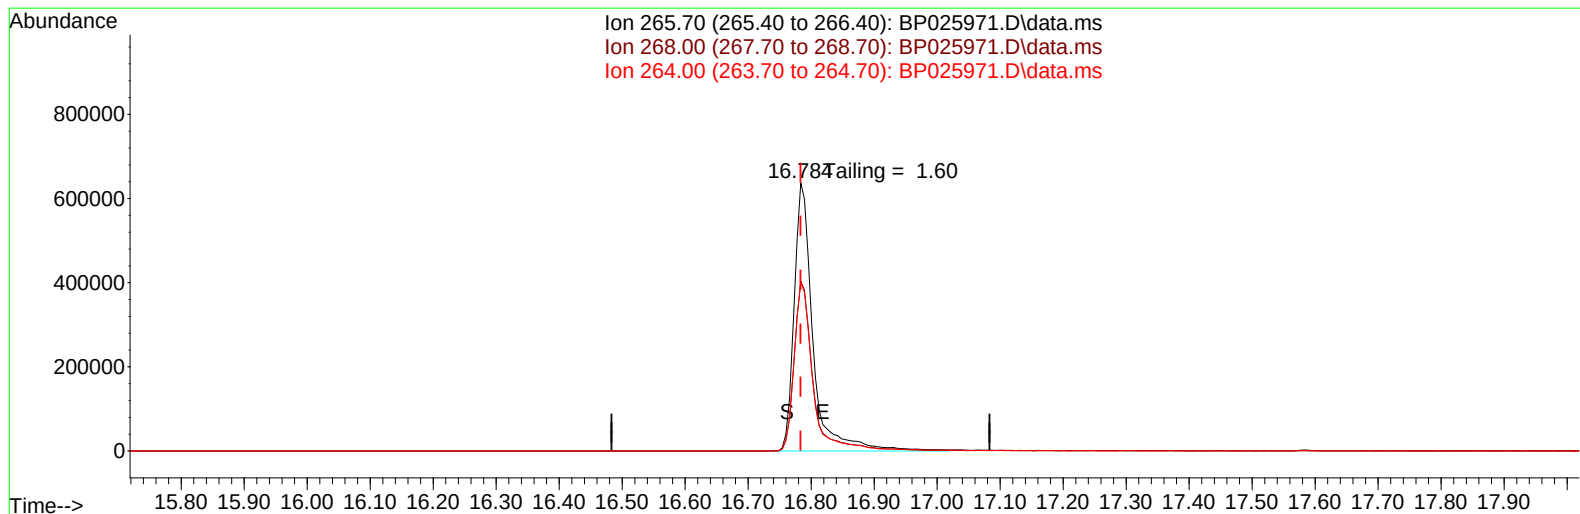

TIC: BP025971.D\data.ms

(70) Pentachlorophenol (C)

16.784min (-0.000) 483538.38 ng

response 1341024

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.29
264.00	66.10	62.92
0.00	0.00	0.00

