


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102225\
Data File : BP026000.D
Acq On : 22 Oct 2025 15:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP101525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 15 23:48:51 2025

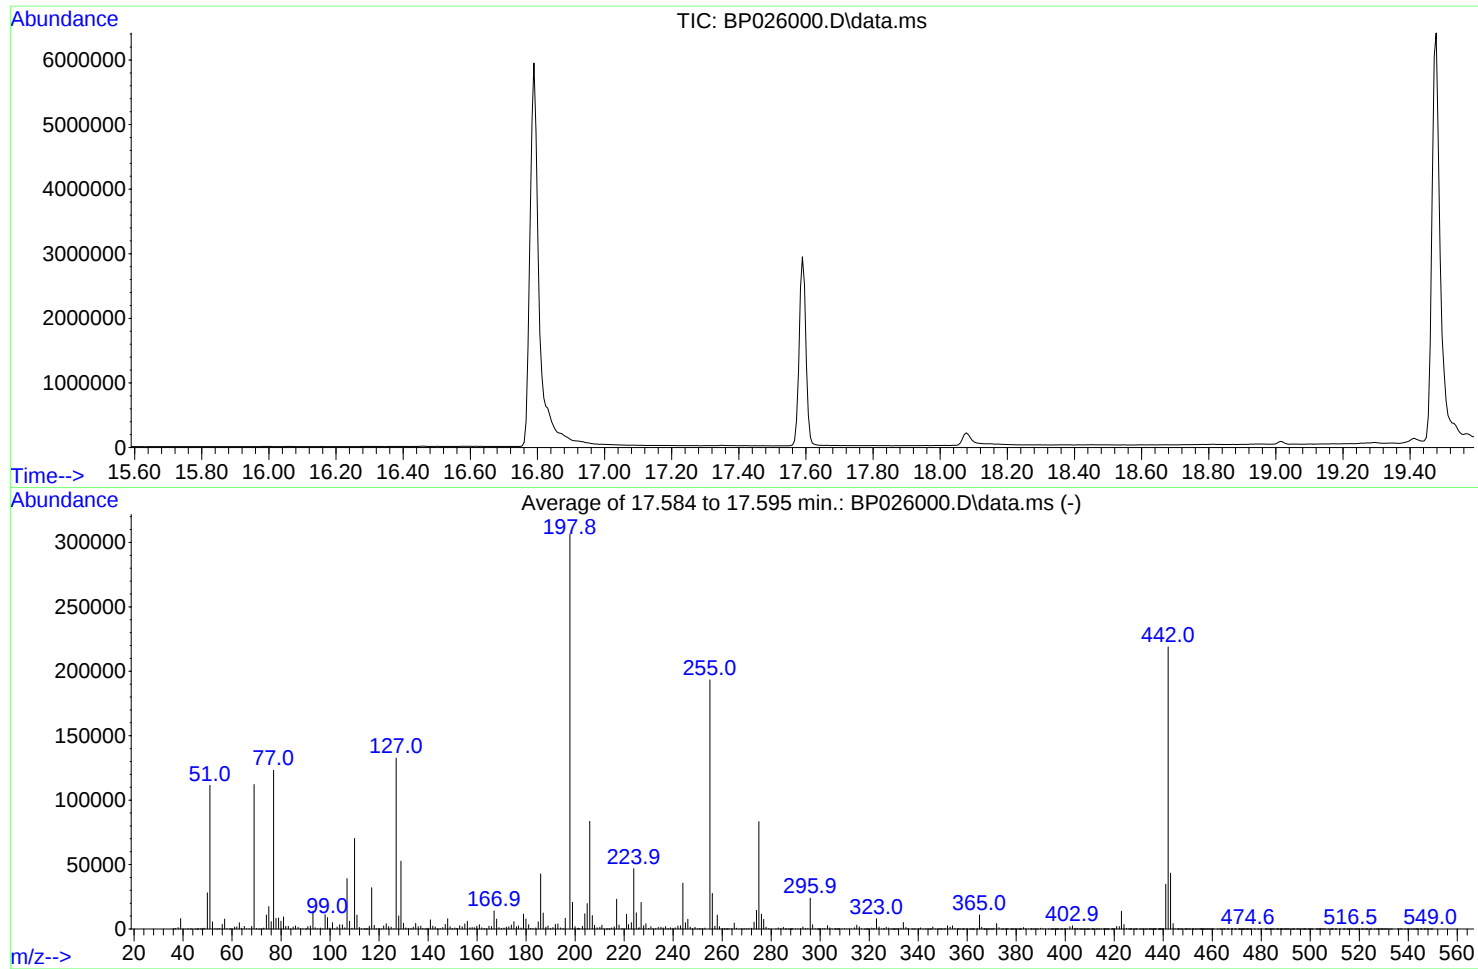

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2480

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	1999	PASS
69	69	100	100	100.0	112155	PASS
70	69	0.00	2	0.5	550	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	306422	PASS
199	198	5	9	6.8	20701	PASS
365	198	1	100	3.6	10940	PASS
441	443	0.01	150	80.2	34763	PASS
442	442	100	100	100.0	218979	PASS
443	442	15	24	19.8	43336	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/22/2025	BNA_P	<u>BP026000.D</u>
Compound Name	Response	Retention Time
DDT	1259216	20.754
DDD	12048	20.307
DDE	246	19.86
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12294	1271510	0.97

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102225\
Data File : BP026000.D
Acq On : 22 Oct 2025 15:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Oct 22 16:39:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP101525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 15 23:48:51 2025
Response via : Initial Calibration

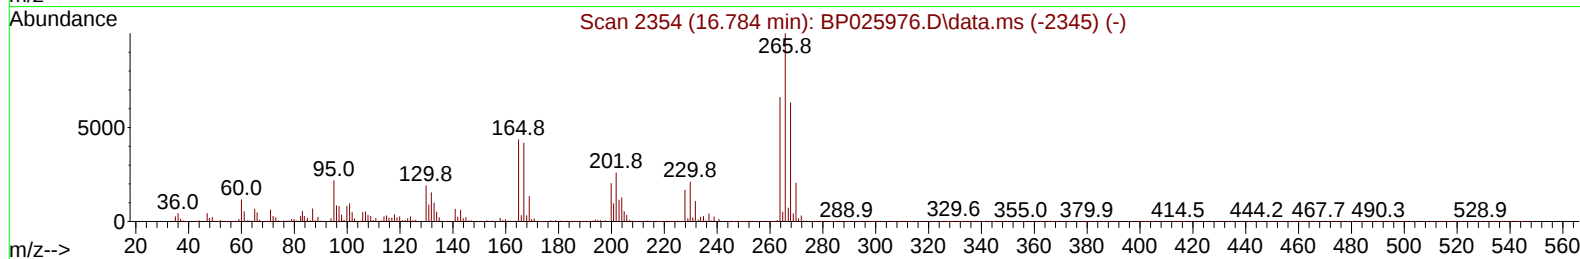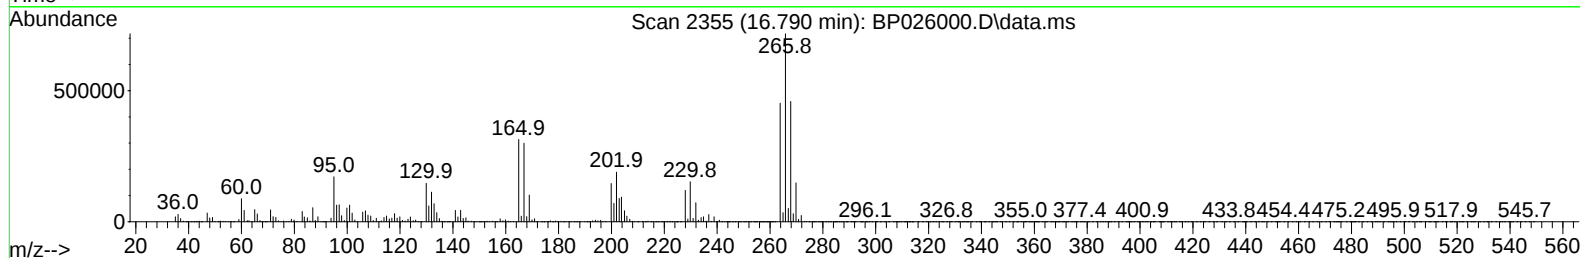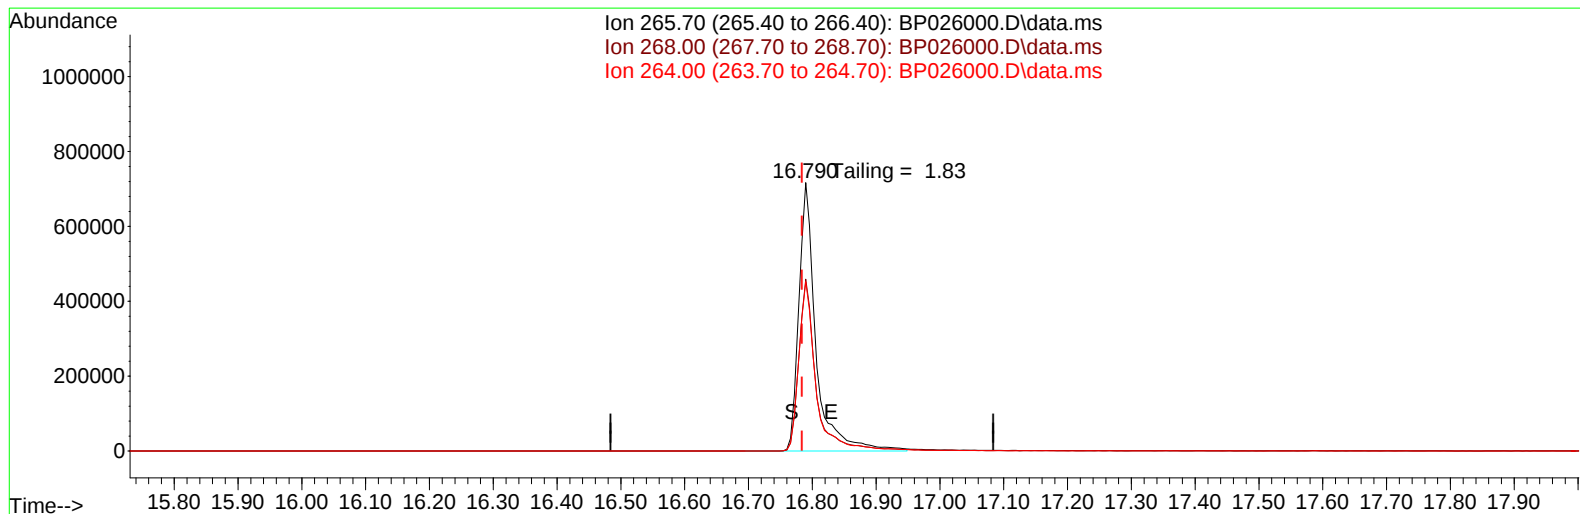

TIC: BP026000.D\data.ms

(70) Pentachlorophenol (C)

16.790min (+ 0.006) 9533301.26 ng




response 1354031

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.01
264.00	66.10	63.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102225\
Data File : BP026000.D
Acq On : 22 Oct 2025 15:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Oct 22 16:39:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP101525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 15 23:48:51 2025
Response via : Initial Calibration

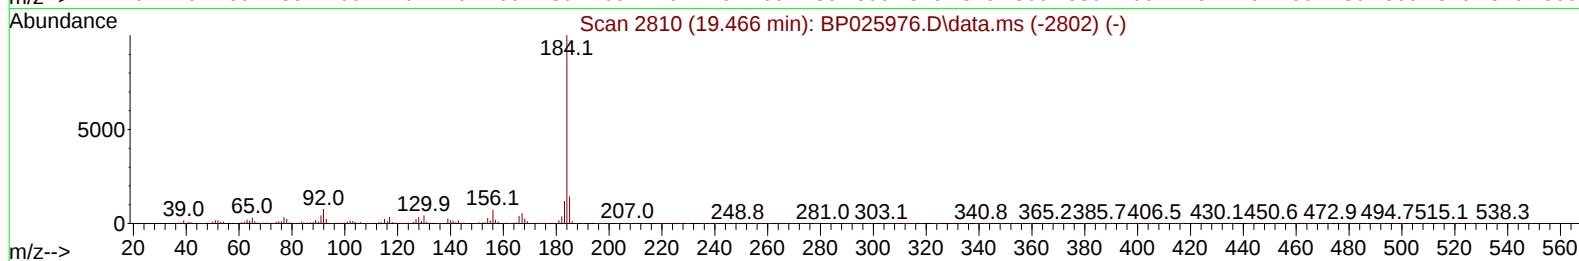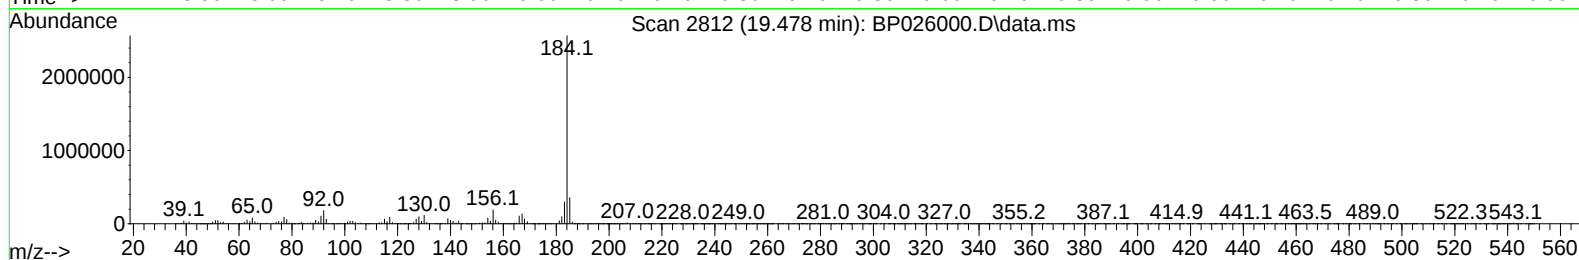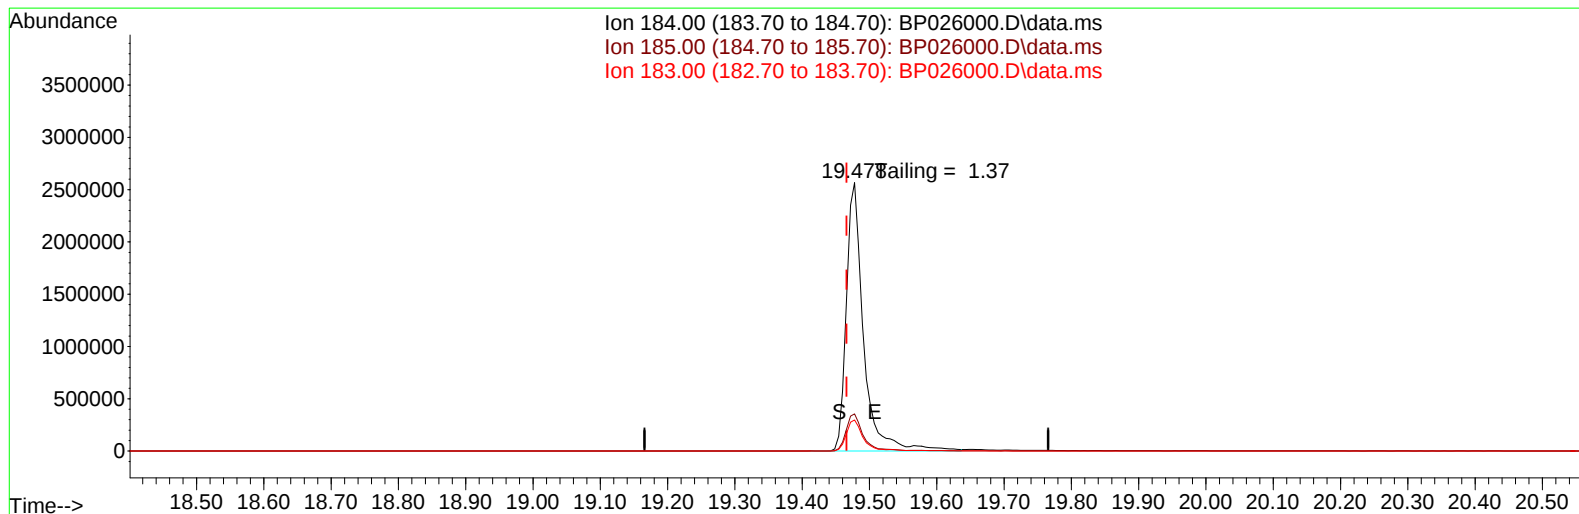

TIC: BP026000.D\data.ms

(77) Benzidine

19.478min (+ 0.012) 2937951.43 ng

response 4424447

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.86
183.00	11.80	11.60
0.00	0.00	0.00