


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102025\
Data File : BN038100.D
Acq On : 20 Oct 2025 16:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 21 02:23:15 2025

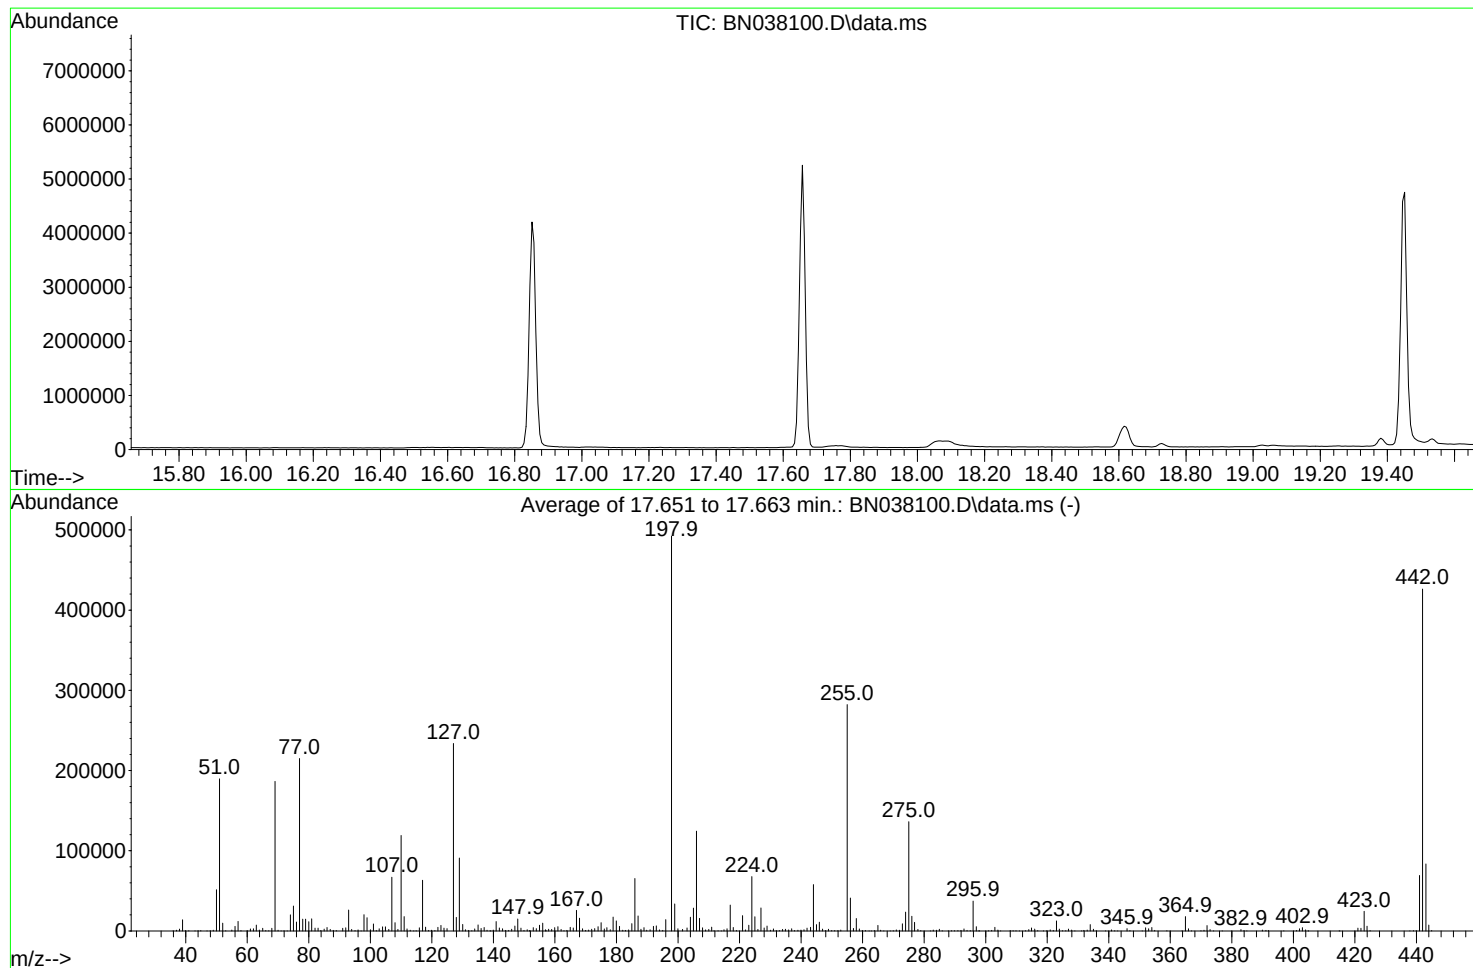




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.8	3346	PASS
69	69	100	100	100.0	186412	PASS
70	69	0.00	2	0.5	886	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	492309	PASS
199	198	5	9	6.8	33669	PASS
365	198	1	100	3.6	17917	PASS
441	443	0.01	150	82.8	69120	PASS
442	442	100	100	100.0	426304	PASS
443	442	15	24	19.6	83453	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102025\
Data File : BN038100.D
Acq On : 20 Oct 2025 16:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 20 18:28:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 20 18:27:35 2025
Response via : Initial Calibration

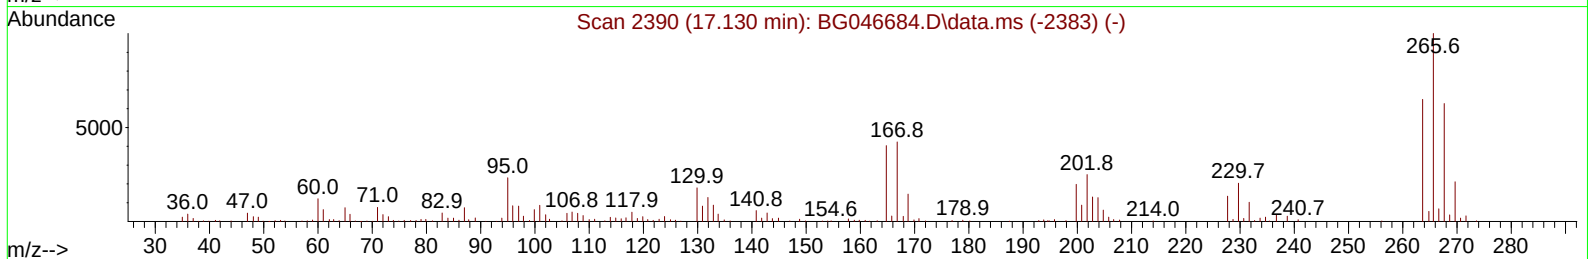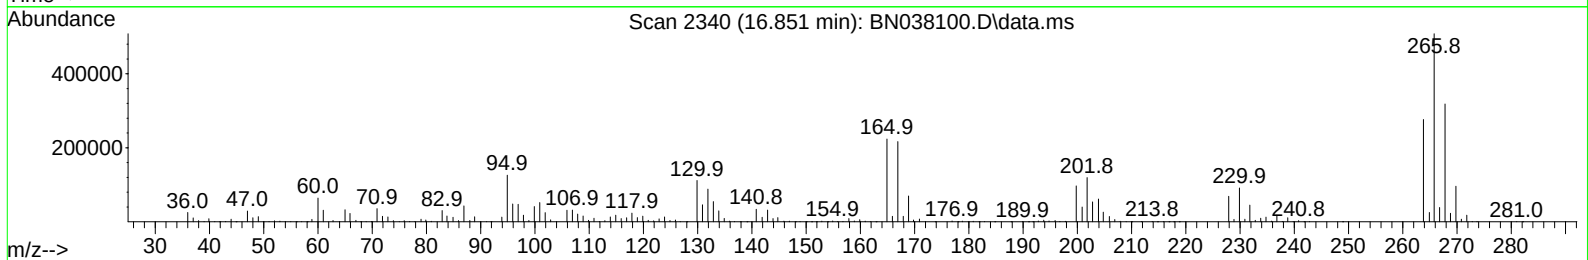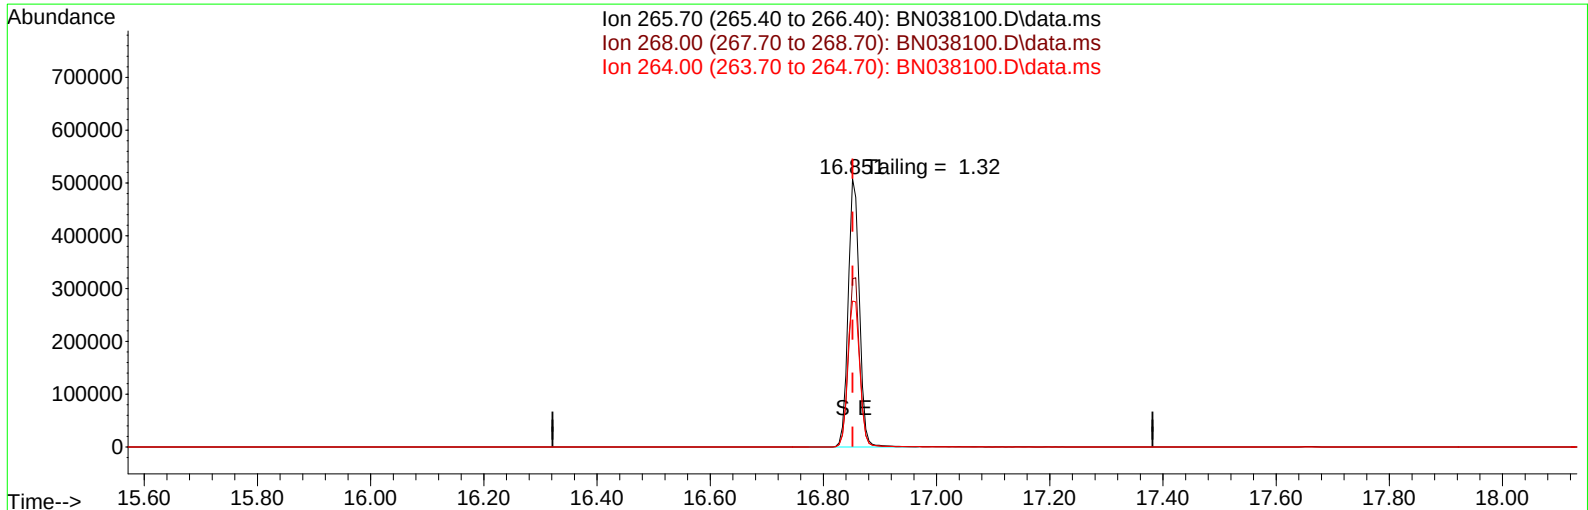

TIC: BN038100.D\data.ms

(70) Pentachlorophenol (C)

16.851min (0.000) 277.76 ng




response 700210

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.64
264.00	61.60	54.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102025\
Data File : BN038100.D
Acq On : 20 Oct 2025 16:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 20 18:28:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 20 18:27:35 2025
Response via : Initial Calibration

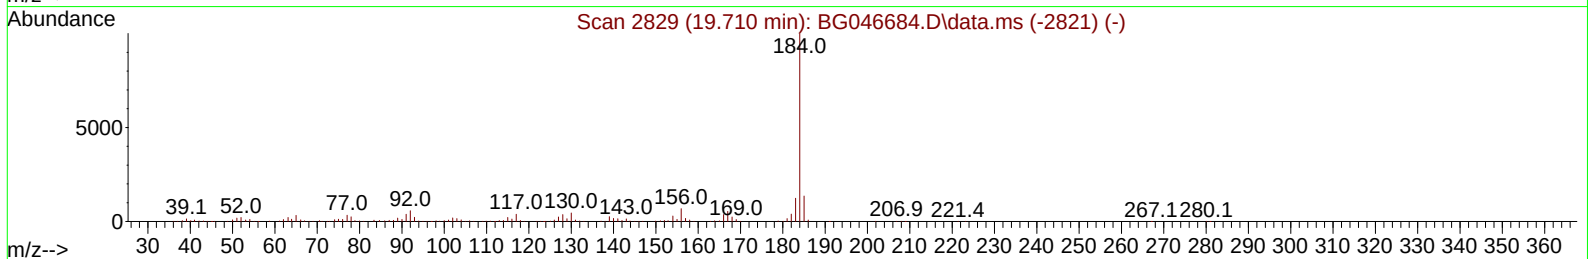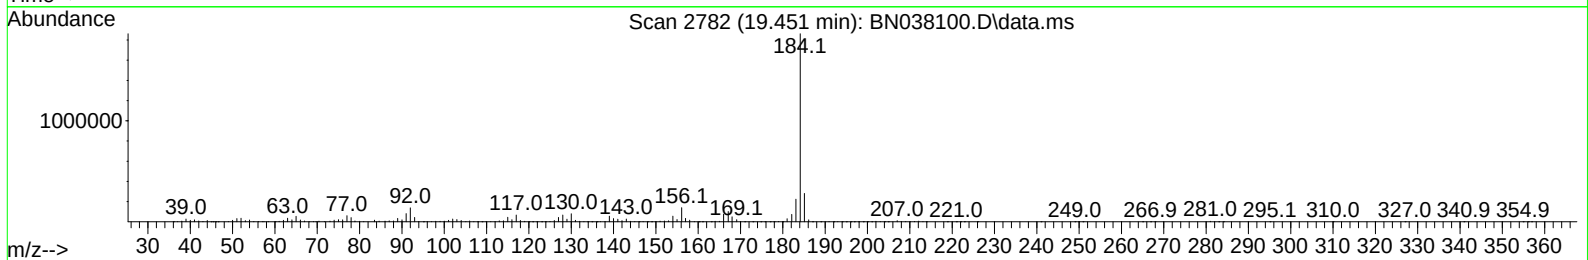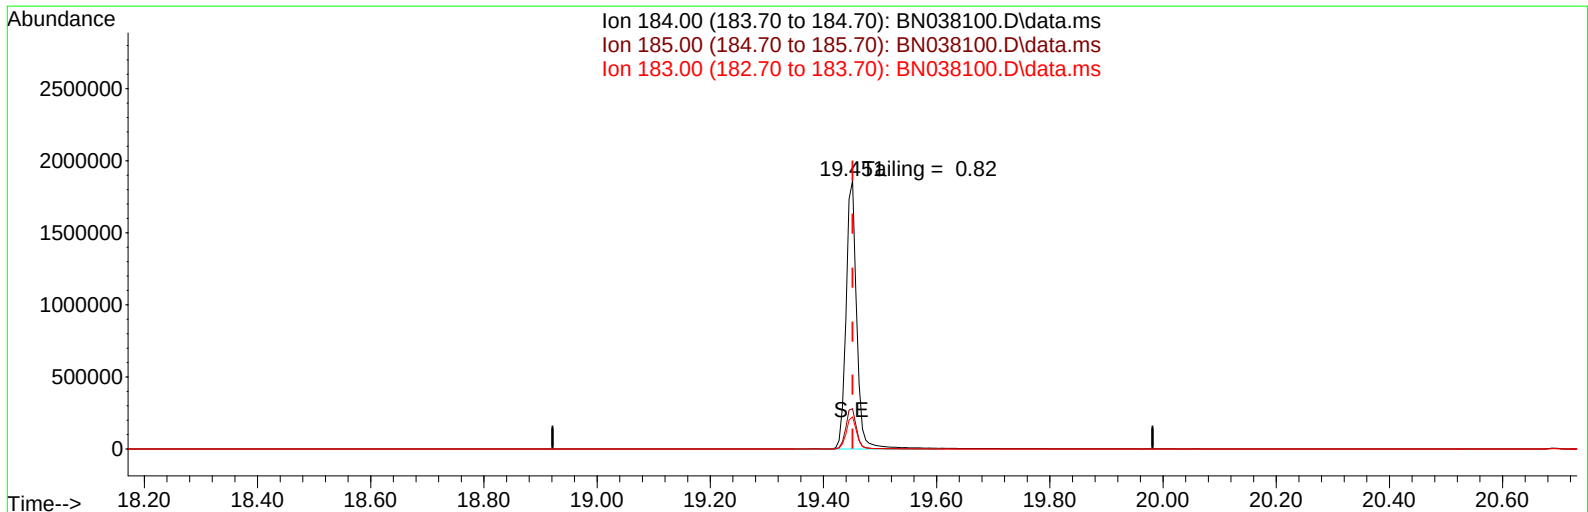

TIC: BN038100.D\data.ms

(77) Benzidine

19.451min (0.000) 0.00 ng

response 2449641

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.05
183.00	13.20	12.03
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/20/2025	BNA_N	<u>BN038100.D</u>
Compound Name	Response	Retention Time
DDT	1547774	20.692
DDD	8872	20.224
DDE	1157	19.745
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10029	1557803	0.64

Instrument :
BNA_N
ClientSampleId :
DFTPP