

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102025\
 Data File : VX048245.D
 Acq On : 20 Oct 2025 17:41
 Operator : JC/MD
 Sample : Q3371-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-184-GW-915-917

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102025W.M
 Title : SW846 8260

Signal : TIC: VX048245.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.154	8	11	22	rVB2	10787	18449	3.40%	0.571%
2	1.459	57	61	72	rVB	19085	24809	4.57%	0.767%
3	2.294	193	198	205	rBV	5668	9942	1.83%	0.307%
4	2.373	205	211	223	rVV	25048	49038	9.03%	1.516%
5	3.331	361	368	379	rVB3	2045	5916	1.09%	0.183%
6	4.233	507	516	530	rVB5	4501	15271	2.81%	0.472%
7	5.373	693	703	719	rBV4	61435	198445	36.55%	6.137%
8	5.544	720	731	748	rVB	101459	316289	58.26%	9.781%
9	5.940	786	796	815	rBV2	67813	203109	37.41%	6.281%
10	6.342	855	862	873	rBV4	2142	6317	1.16%	0.195%
11	6.751	919	929	945	rBV	160941	427254	78.70%	13.213%
12	7.452	1039	1044	1053	rBV3	3326	8731	1.61%	0.270%
13	7.568	1058	1063	1069	rBV3	5234	9929	1.83%	0.307%
14	8.635	1231	1238	1257	rBV	324332	542882	100.00%	16.788%
15	9.019	1297	1301	1308	rVB4	3575	7171	1.32%	0.222%
16	9.512	1376	1382	1392	rBV	5712	10511	1.94%	0.325%
17	10.037	1462	1468	1483	rBV	355730	513627	94.61%	15.884%
18	10.841	1594	1600	1610	rVB3	5102	7930	1.46%	0.245%
19	11.061	1631	1636	1653	rBV	253025	360097	66.33%	11.136%
20	11.463	1697	1702	1711	rVB3	4775	8472	1.56%	0.262%
21	12.006	1785	1791	1800	rBV	359468	483734	89.10%	14.959%
22	12.841	1924	1928	1933	rVB3	4224	5772	1.06%	0.178%




Sum of corrected areas: 3233695

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102025\
Data File : VX048245.D
Acq On : 20 Oct 2025 17:41
Operator : JC/MD
Sample : Q3371-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-184-GW-915-917

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102025W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

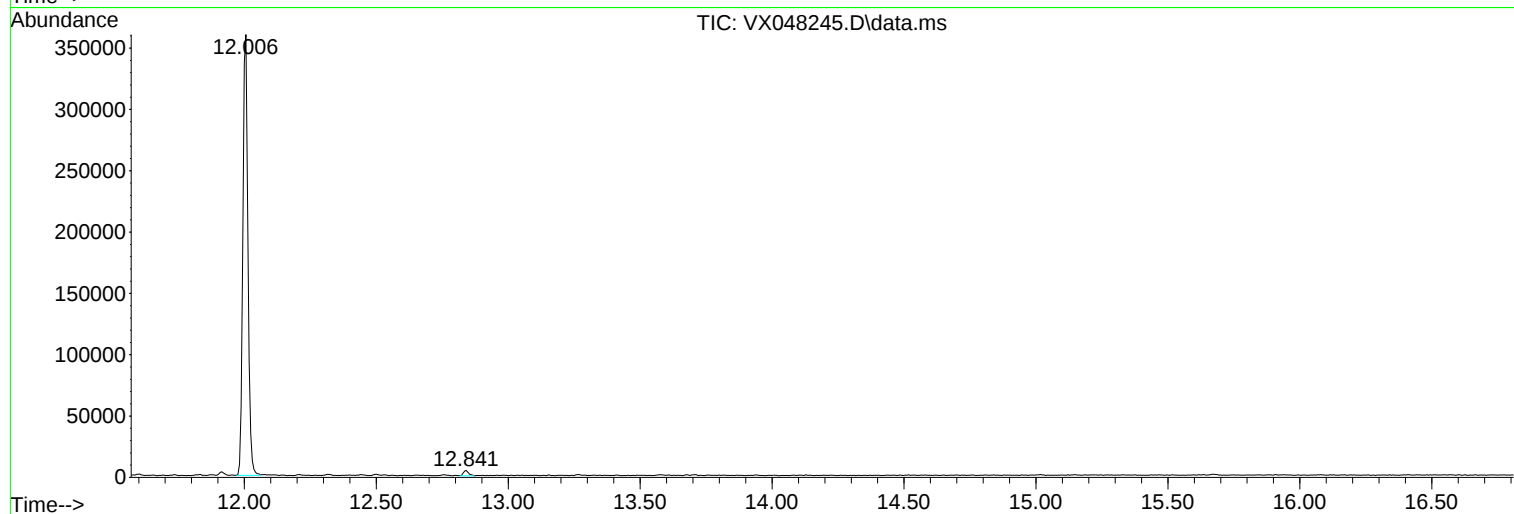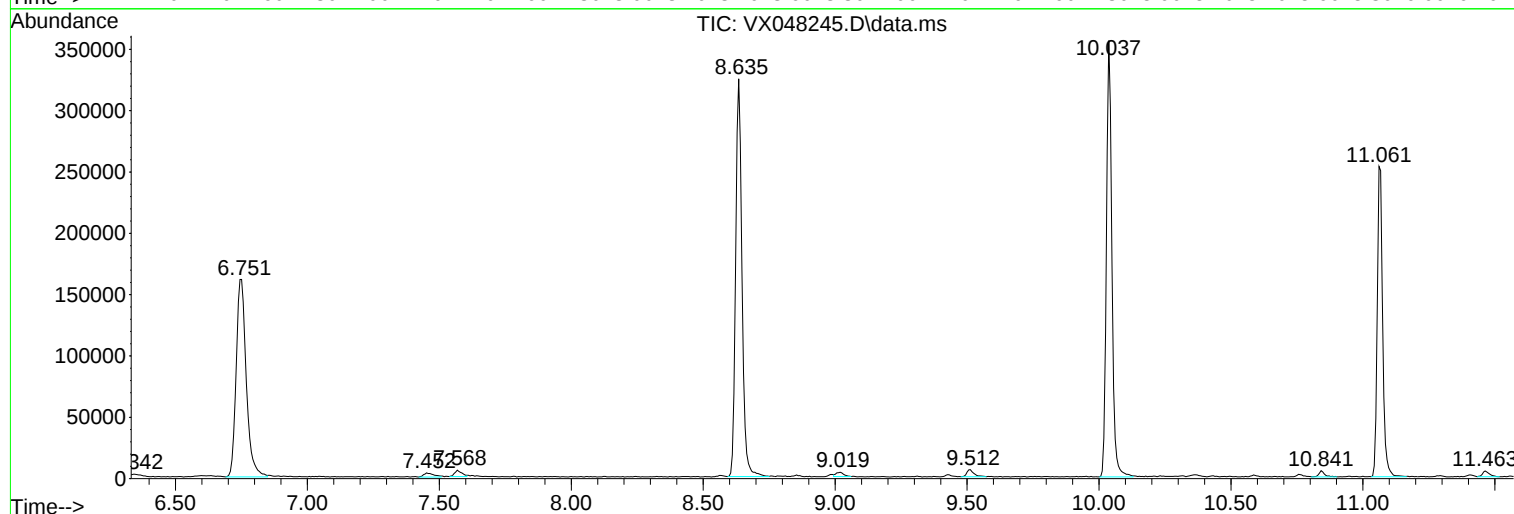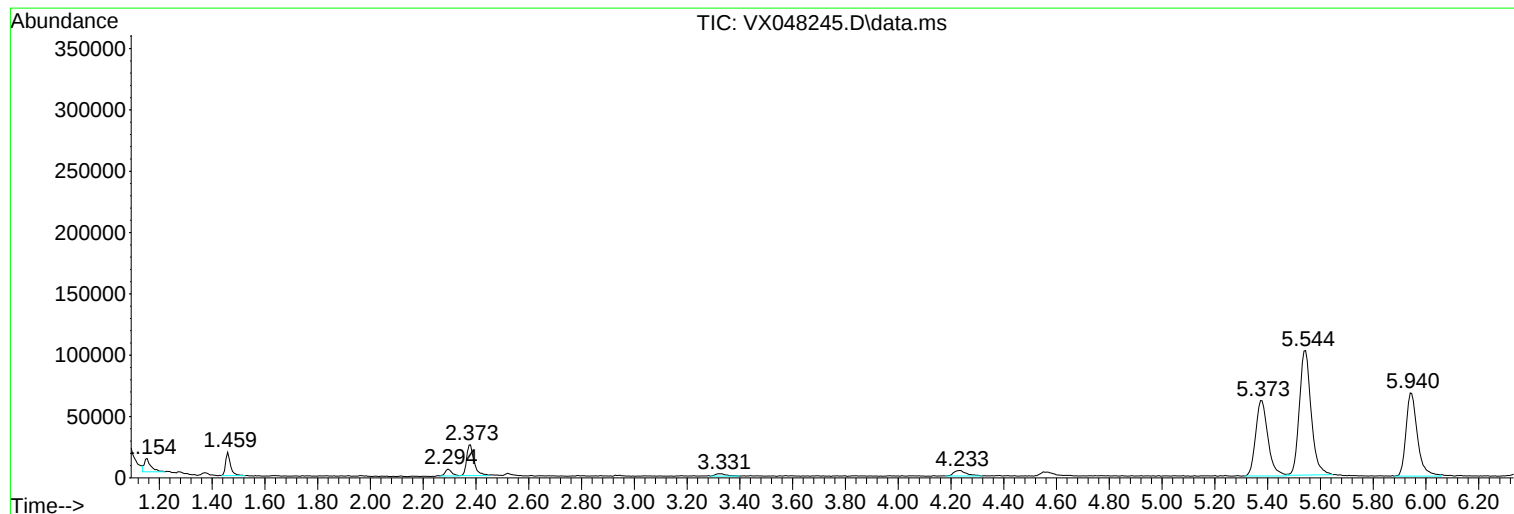

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102025\
Data File : VX048245.D
Acq On : 20 Oct 2025 17:41
Operator : JC/MD
Sample : Q3371-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-184-GW-915-917

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102025W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102025\
Data File : VX048245.D
Acq On : 20 Oct 2025 17:41
Operator : JC/MD
Sample : Q3371-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-184-GW-915-917

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102025W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc