
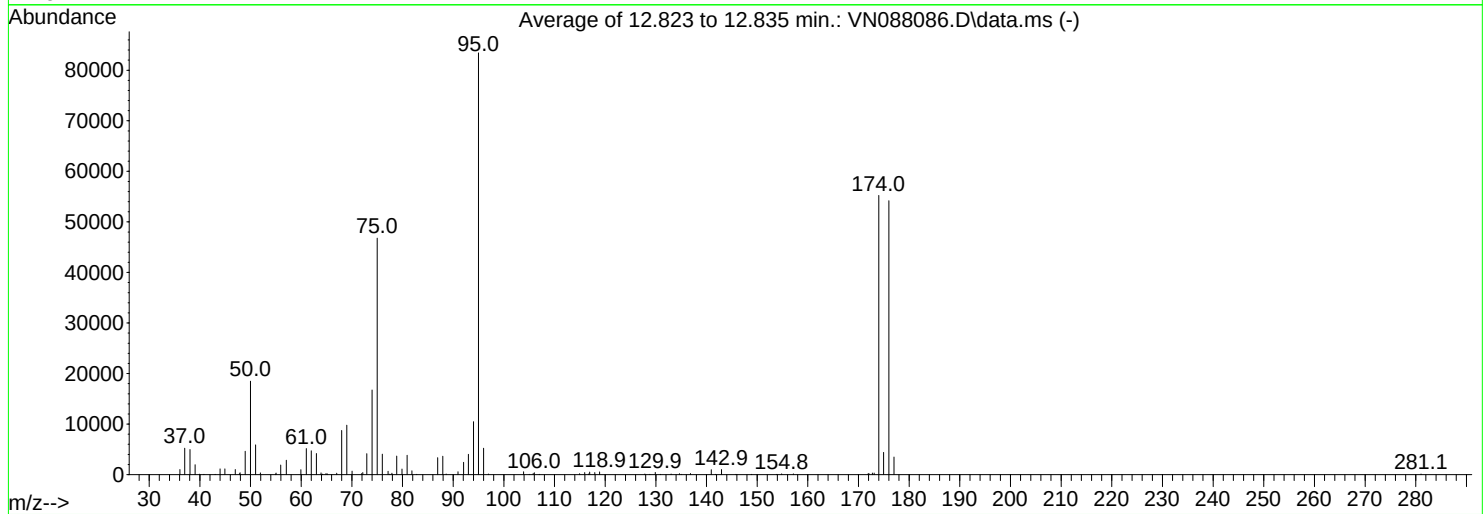


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102425\
Data File : VN088086.D
Acq On : 24 Oct 2025 12:07
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M
Title : SW846 8260
Last Update : Sat Oct 25 00:15:22 2025

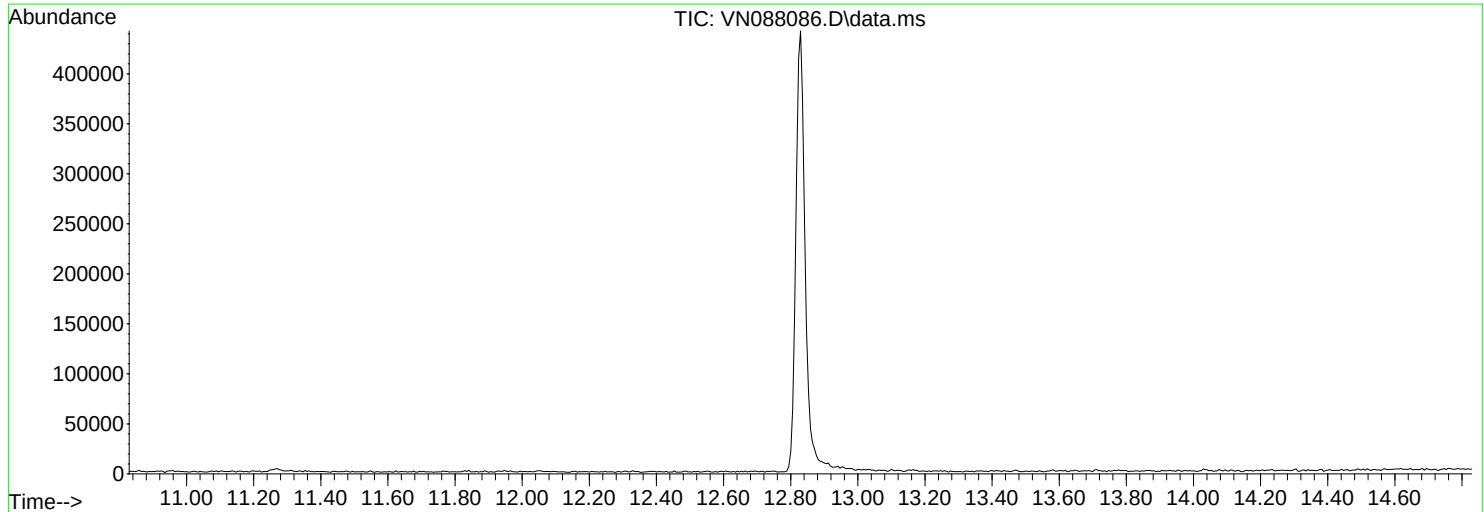

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	18497	PASS
75	95	30	60	56.1	46792	PASS
95	95	100	100	100.0	83443	PASS
96	95	5	9	6.2	5212	PASS
173	174	0.00	2	0.6	333	PASS
174	95	50	100	66.2	55227	PASS
175	174	5	9	8.0	4416	PASS
176	174	95	101	98.1	54195	PASS
177	176	5	9	6.4	3474	PASS

Average of 12.823 to 12.835 min.: VN088086.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	1019	47.95	397	62.00	4725	72.15	421
37.00	5228	48.95	4618	63.00	4179	72.95	415
38.05	4968	50.00	18497	63.90	361	74.00	1674
39.05	1972	51.00	5907	64.20	106	75.00	4679
39.95	84	51.95	353	64.90	211	76.00	4055
40.80	73	54.90	143	65.15	165	77.15	670
43.00	57	55.05	312	67.00	274	77.50	90
44.00	1140	55.95	1905	68.00	8736	77.90	291
44.95	1135	57.05	2857	69.00	9774	78.85	3688
47.00	1026	59.95	982	70.05	688	79.90	1116
47.80	201	61.00	5169	71.90	197	80.90	3847

Average of 12.823 to 12.835 min.: VN088086.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.85	771	96.95	132	118.90	541	142.95	1028
82.80	60	103.90	575	127.85	141	145.80	59
86.95	3369	105.00	59	128.80	69	146.00	50
87.95	3649	105.80	219	129.90	436	148.90	66
88.60	136	106.00	386	130.90	71	153.90	55
90.95	558	107.00	78	133.00	123	154.85	166
92.05	2424	114.95	195	134.65	205	157.15	150
93.00	4025	115.95	424	135.00	52	171.90	167
94.00	10466	116.70	125	136.85	208	172.05	248
95.00	83443	116.95	509	140.95	976	172.75	333
96.00	5212	117.95	428	141.80	64	173.10	326

Average of 12.823 to 12.835 min.: VN088086.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
174.00	55227						
174.95	4416						
176.00	54195						
177.00	3474						
281.05	120						