
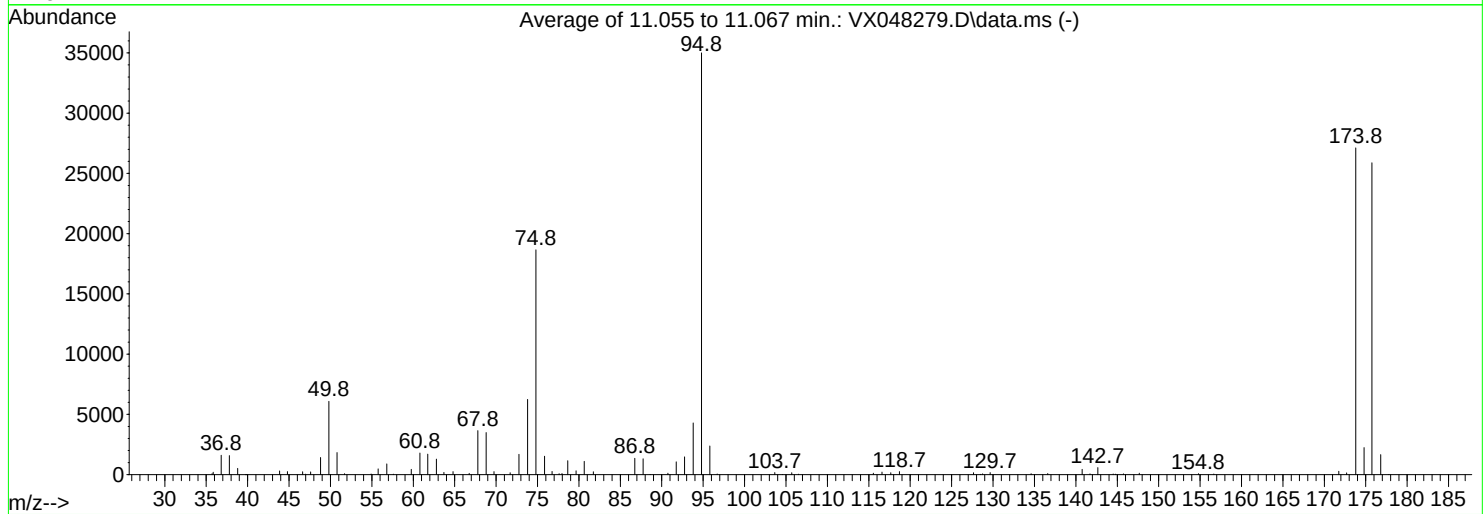


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102225\
Data File : VX048279.D
Acq On : 22 Oct 2025 08:07
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102025W.M
Title : SW846 8260
Last Update : Mon Oct 20 14:13:59 2025

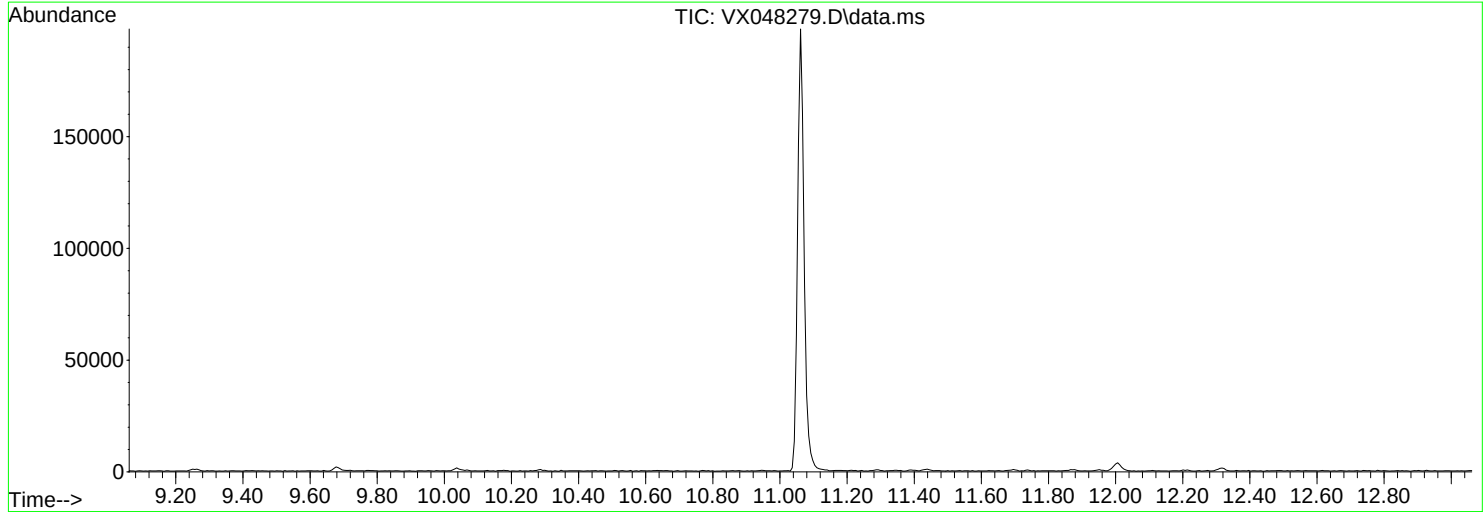

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1629

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.4	6085	PASS
75	95	30	60	53.3	18653	PASS
95	95	100	100	100.0	35005	PASS
96	95	5	9	6.8	2374	PASS
173	174	0.00	2	0.5	144	PASS
174	95	50	100	77.5	27120	PASS
175	174	5	9	8.3	2250	PASS
176	174	95	101	95.4	25885	PASS
177	176	5	9	6.4	1654	PASS