


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100225\
Data File : BG064472.D
Acq On : 2 Oct 2025 8:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 02 16:40:42 2025

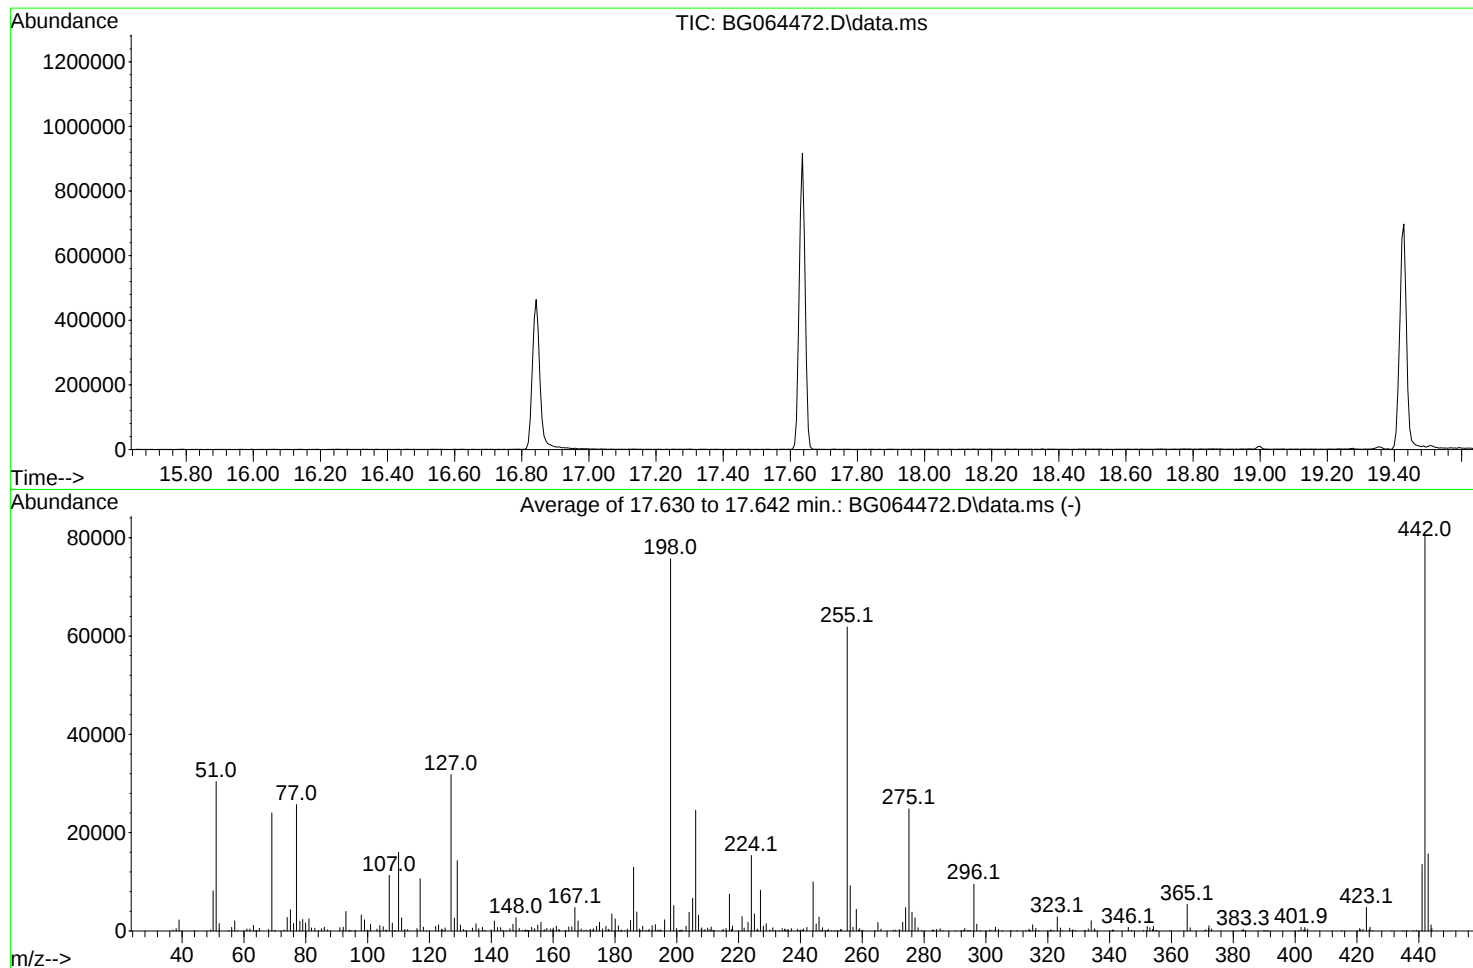




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.1	271	PASS
69	69	100	100	100.0	24008	PASS
70	69	0.00	2	0.4	100	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	75675	PASS
199	198	5	9	6.8	5168	PASS
365	198	1	100	7.1	5406	PASS
441	443	0.01	150	86.2	13521	PASS
442	442	100	100	100.0	80341	PASS
443	442	15	24	19.5	15684	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100225\
Data File : BG064472.D
Acq On : 2 Oct 2025 8:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 02 18:07:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 02 16:40:42 2025
Response via : Initial Calibration

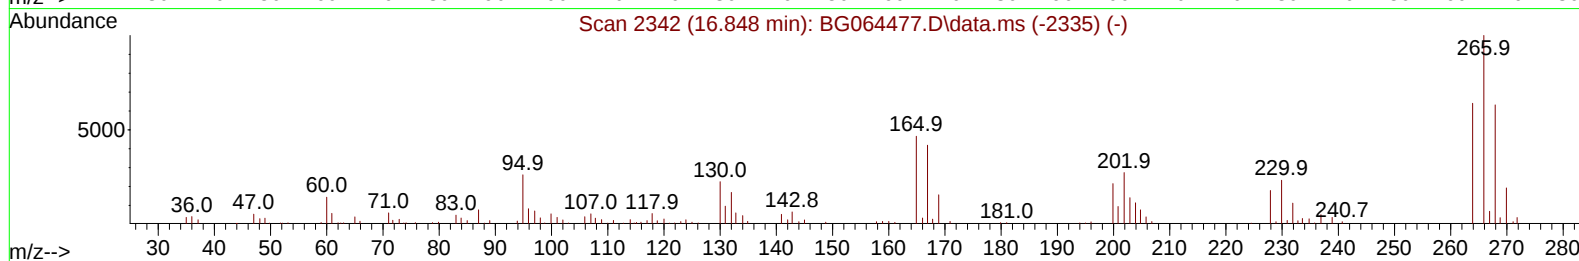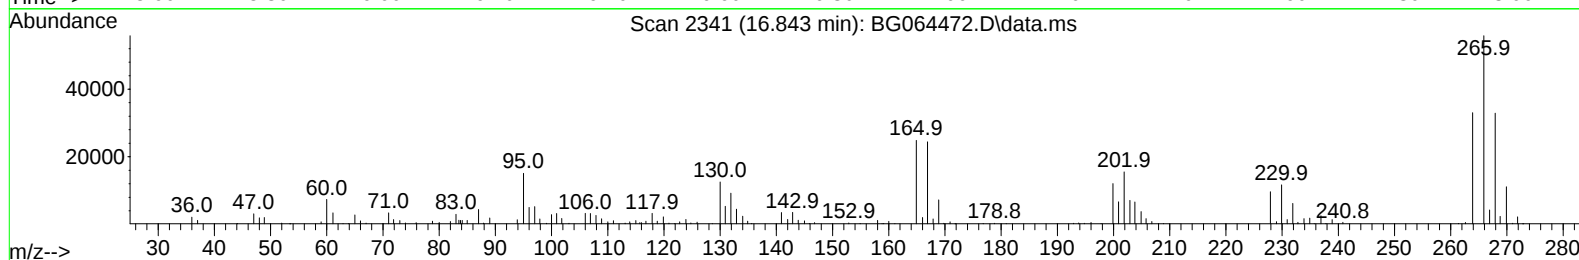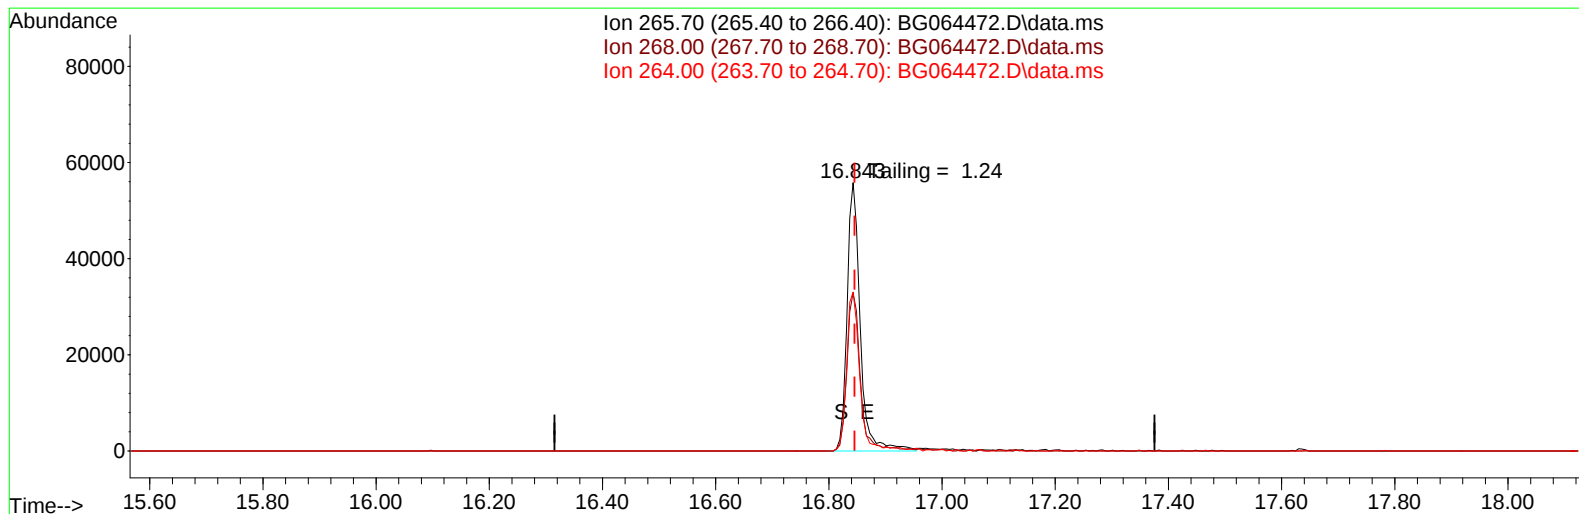

TIC: BG064472.D\data.ms

(70) Pentachlorophenol (C)

16.843min (-0.002) 190750.25 ng




response 90109

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	58.97
264.00	64.00	59.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100225\
Data File : BG064472.D
Acq On : 2 Oct 2025 8:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 02 18:07:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 02 16:40:42 2025
Response via : Initial Calibration

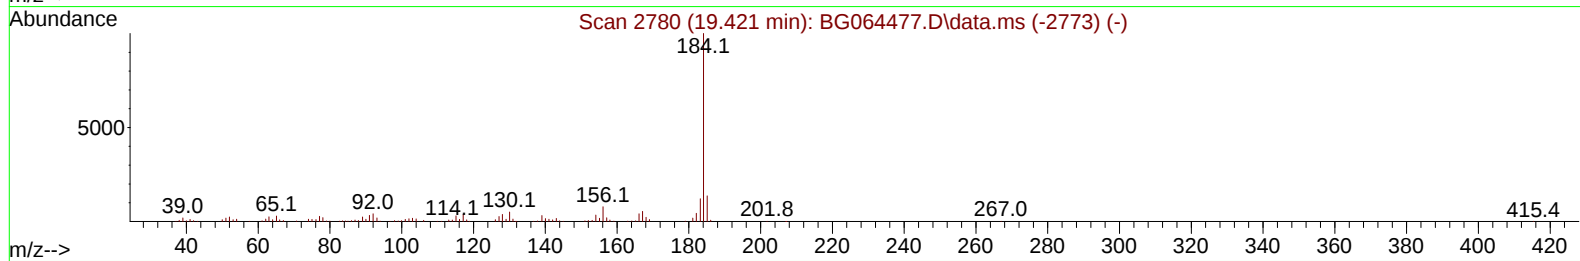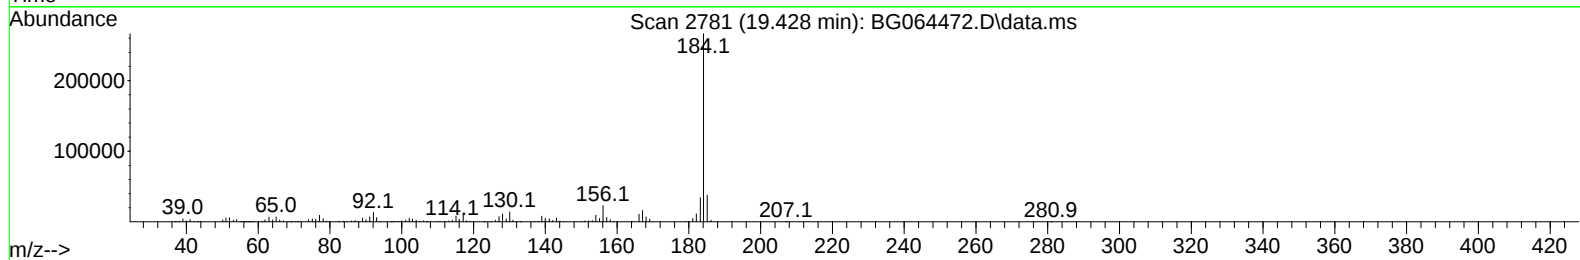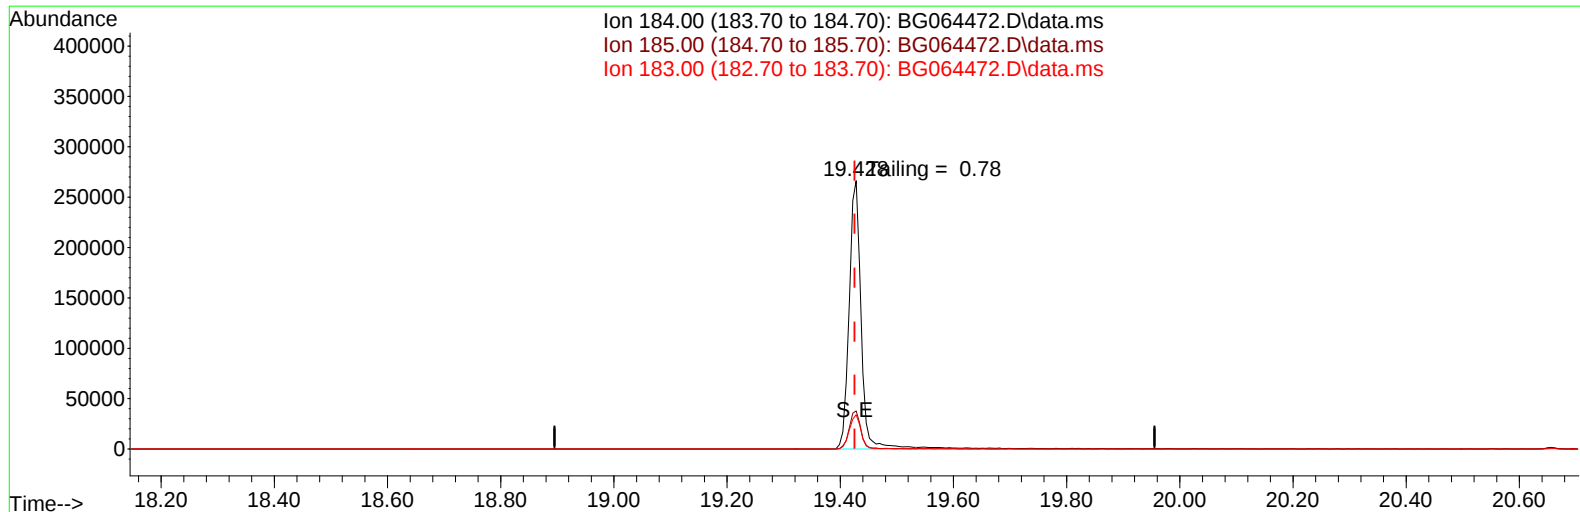

TIC: BG064472.D\data.ms

(77) Benzidine

19.428min (+ 0.003) 15488.27 ng

response 385018

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.19
183.00	12.20	12.79
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/2/2025	BNA_G	<u>BG064472.D</u>
Compound Name	Response	Retention Time
DDT	287203	20.656
DDD	3381	20.221
DDE	0	19.728
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3381	290584	1.16

Instrument :
BNA_G
ClientSampleId :
DFTPP