
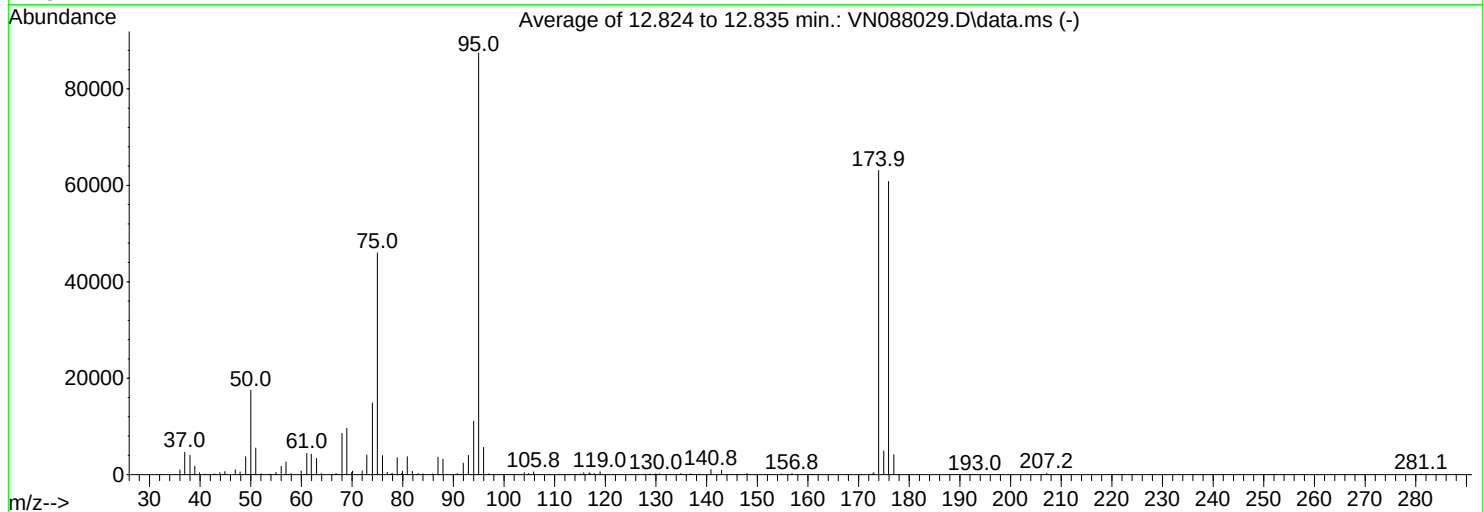


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100825\
Data File : VN088029.D
Acq On : 08 Oct 2025 09:00
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N092325W.M
Title : SW846 8260
Last Update : Wed Sep 24 05:05:30 2025

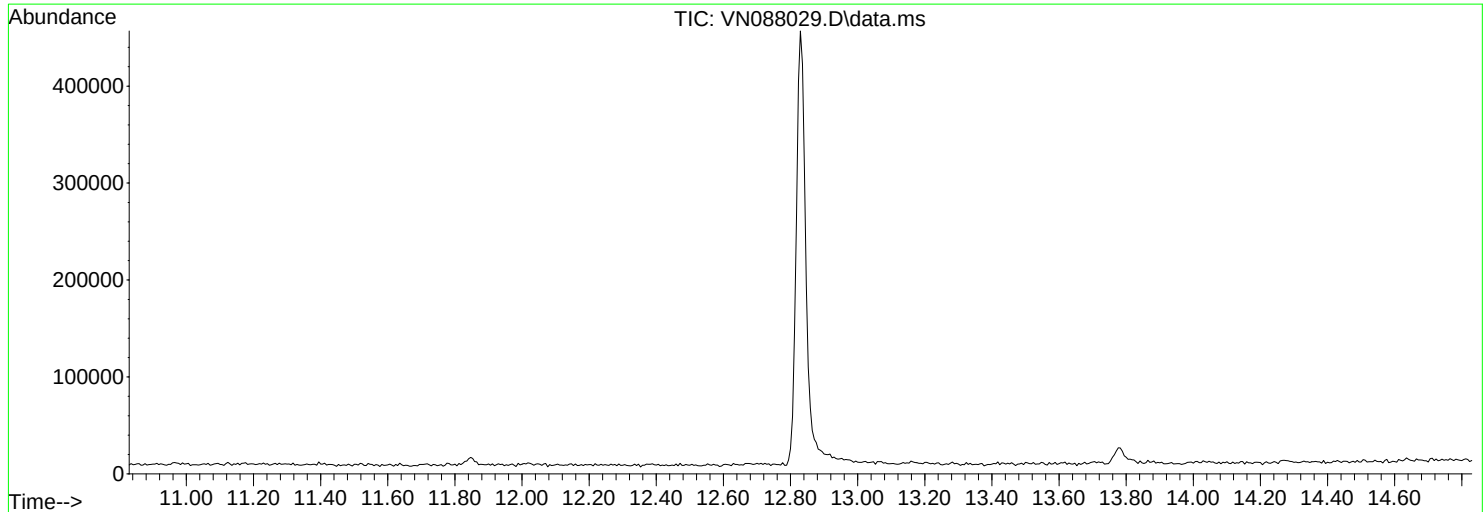

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1838

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.0	17477	PASS
75	95	30	60	52.6	45984	PASS
95	95	100	100	100.0	87474	PASS
96	95	5	9	6.4	5640	PASS
173	174	0.00	2	0.7	447	PASS
174	95	50	100	72.1	63077	PASS
175	174	5	9	7.8	4922	PASS
176	174	95	101	96.4	60787	PASS
177	176	5	9	6.8	4150	PASS

Average of 12.824 to 12.835 min.: VN088029.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	1009	47.90	581	59.95	735	72.00	741
36.95	4647	49.00	3723	61.05	4431	72.90	407
38.00	4004	50.00	17477	61.95	4248	74.00	1487
38.95	1766	51.00	5503	63.00	3349	75.00	4598
39.90	406	51.90	62	63.90	238	76.00	3941
41.05	87	52.05	200	64.20	75	76.95	508
41.90	79	53.80	133	66.85	265	77.75	196
42.90	180	54.95	468	68.00	8577	78.00	198
43.90	433	56.00	1730	68.95	9610	78.90	3521
44.90	634	56.95	2644	69.90	438	79.80	249
46.95	1040	57.95	232	70.10	737	79.95	727

Average of 12.824 to 12.835 min.: VN088029.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.90	3725	92.95	3969	115.05	120	130.00	219
81.90	684	94.00	11096	115.75	389	130.75	204
82.80	75	95.00	87474	116.80	384	132.90	22
83.05	245	95.95	5640	117.00	258	134.90	235
84.00	168	97.00	213	117.80	275	136.80	157
85.85	165	104.00	436	118.20	72	137.10	107
86.95	3617	104.85	244	118.95	606	138.70	63
87.95	3204	105.85	562	127.70	113	140.85	1072
88.70	58	109.00	53	127.95	150	142.95	947
90.80	185	111.00	107	128.85	143	145.00	52
91.95	2395	113.00	79	129.70	105	146.00	66

Average of 12.824 to 12.835 min.: VN088029.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
147.95	241	173.95	63077				
149.80	78	174.95	4922				
150.00	59	175.90	60787				
154.85	151	176.95	4150				
156.85	252	178.00	55				
160.70	56	193.00	52				
160.90	52	207.15	299				
170.60	76	281.05	121				
172.05	128						
172.70	168						
173.00	447						

Instrument :

MSVOA_N

ClientSampleId :

BFB