


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101725\
Data File : VN088054.D
Acq On : 17 Oct 2025 08:56
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N100825W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Oct 09 02:36:32 2025

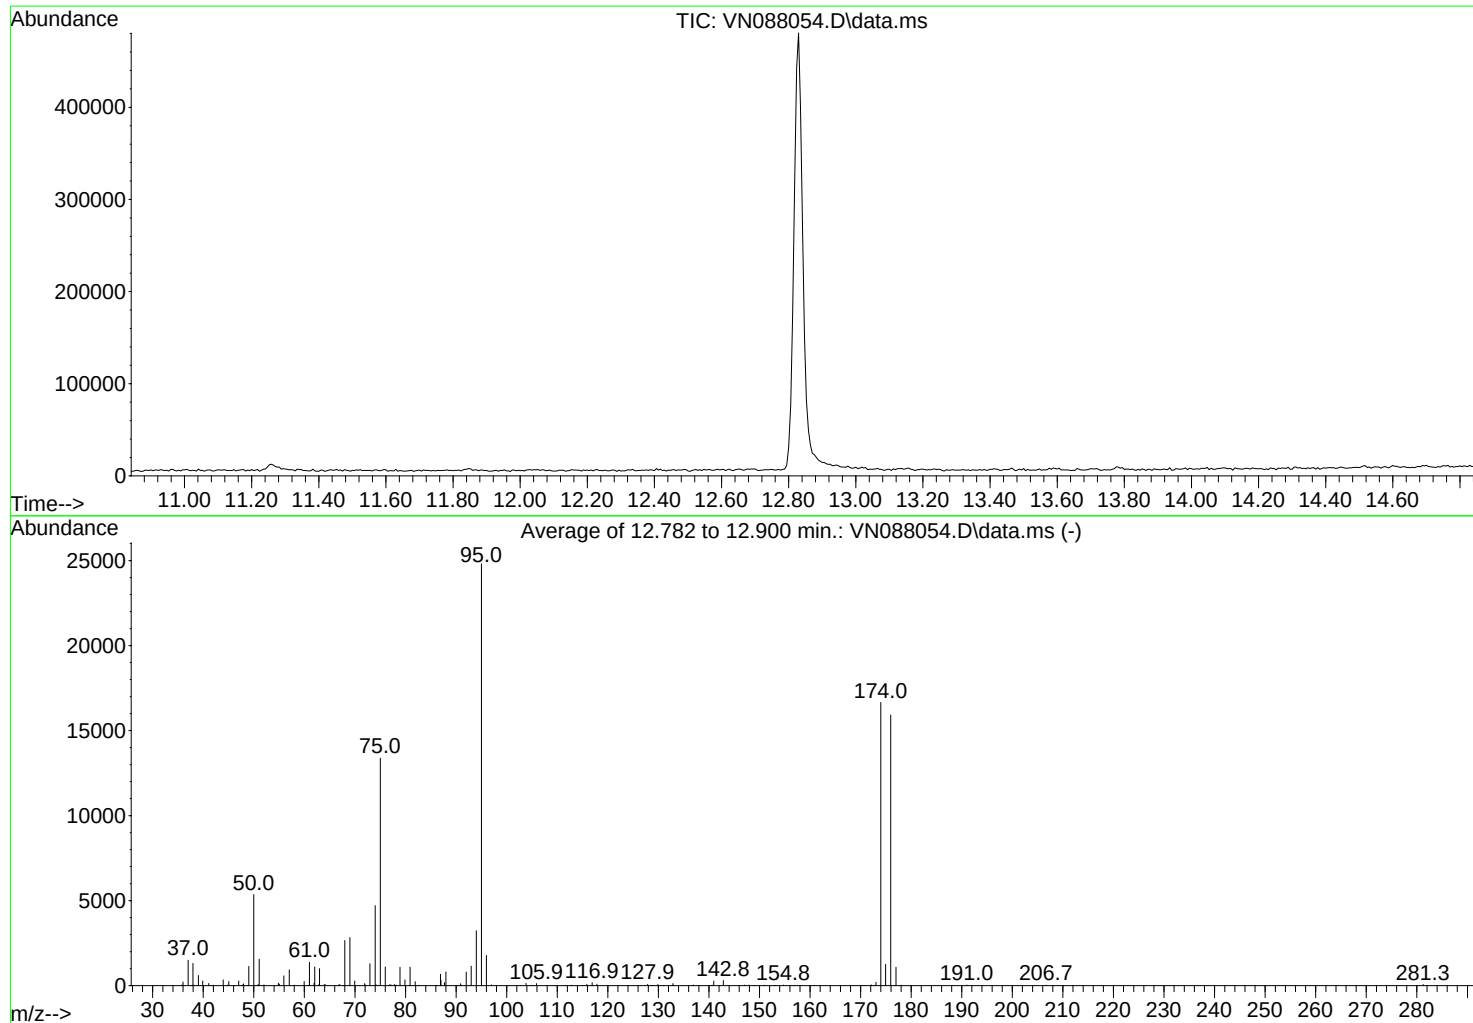

AutoFind: Averaged scan 1841 to 1861; Bkg corrected with scan 1840

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.6	5355	PASS
75	95	30	60	53.9	13380	PASS
95	95	100	100	100.0	24810	PASS
96	95	5	9	7.2	1783	PASS
173	174	0.00	2	1.2	201	PASS
174	95	50	100	67.1	16654	PASS
175	174	5	9	7.5	1251	PASS
176	174	95	101	95.6	15915	PASS
177	176	5	9	6.8	1078	PASS