
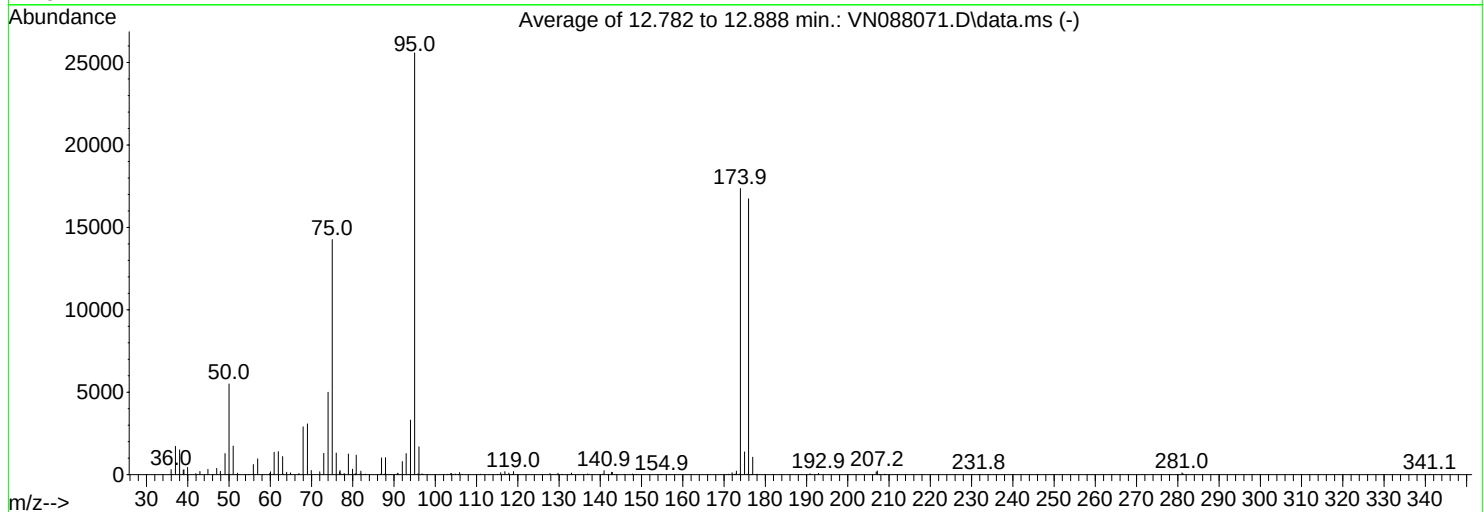


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102025\
Data File : VN088071.D
Acq On : 20 Oct 2025 08:17
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N100825W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Oct 09 02:36:32 2025

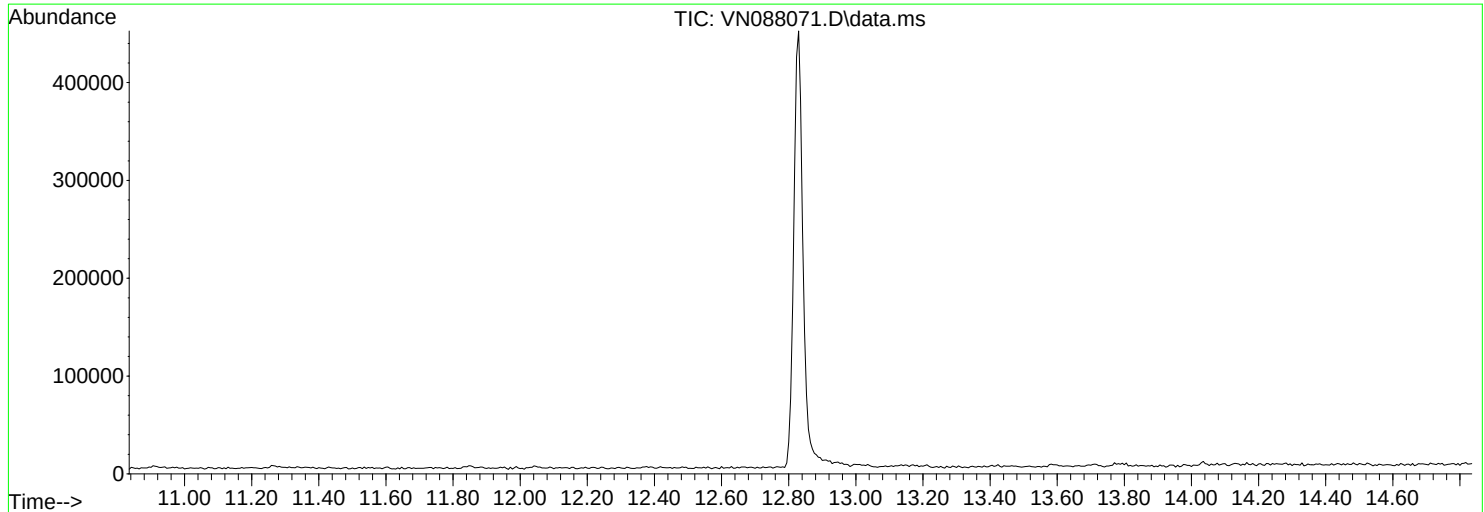

AutoFind: Averaged scan 1841 to 1859; Bkg corrected with scan 1840

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.5	5500	PASS
75	95	30	60	55.7	14257	PASS
95	95	100	100	100.0	25589	PASS
96	95	5	9	6.6	1694	PASS
173	174	0.00	2	1.2	216	PASS
174	95	50	100	67.8	17356	PASS
175	174	5	9	7.9	1374	PASS
176	174	95	101	96.4	16730	PASS
177	176	5	9	6.3	1056	PASS