

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102025\
 Data File : VN088075.D
 Acq On : 20 Oct 2025 10:55
 Operator : JC\MD
 Sample : VN1020WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1020WBL01

Quant Time: Oct 21 05:37:01 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N100825W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Thu Oct 09 02:36:32 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	7.800	128	56116	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	9.083	114	302542	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.847	117	267258	30.000	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.559	65	142234	32.550	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	108.500%
60) 4-Bromofluorobenzene	12.829	95	125221	28.421	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	94.733%
63) Toluene-d8	10.541	98	366105	30.746	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	102.500%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102025\
Data File : VN088075.D
Acq On : 20 Oct 2025 10:55
Operator : JC\MD
Sample : VN1020WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1020WBL01

Quant Time: Oct 21 05:37:01 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N100825W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Thu Oct 09 02:36:32 2025
Response via : Initial Calibration




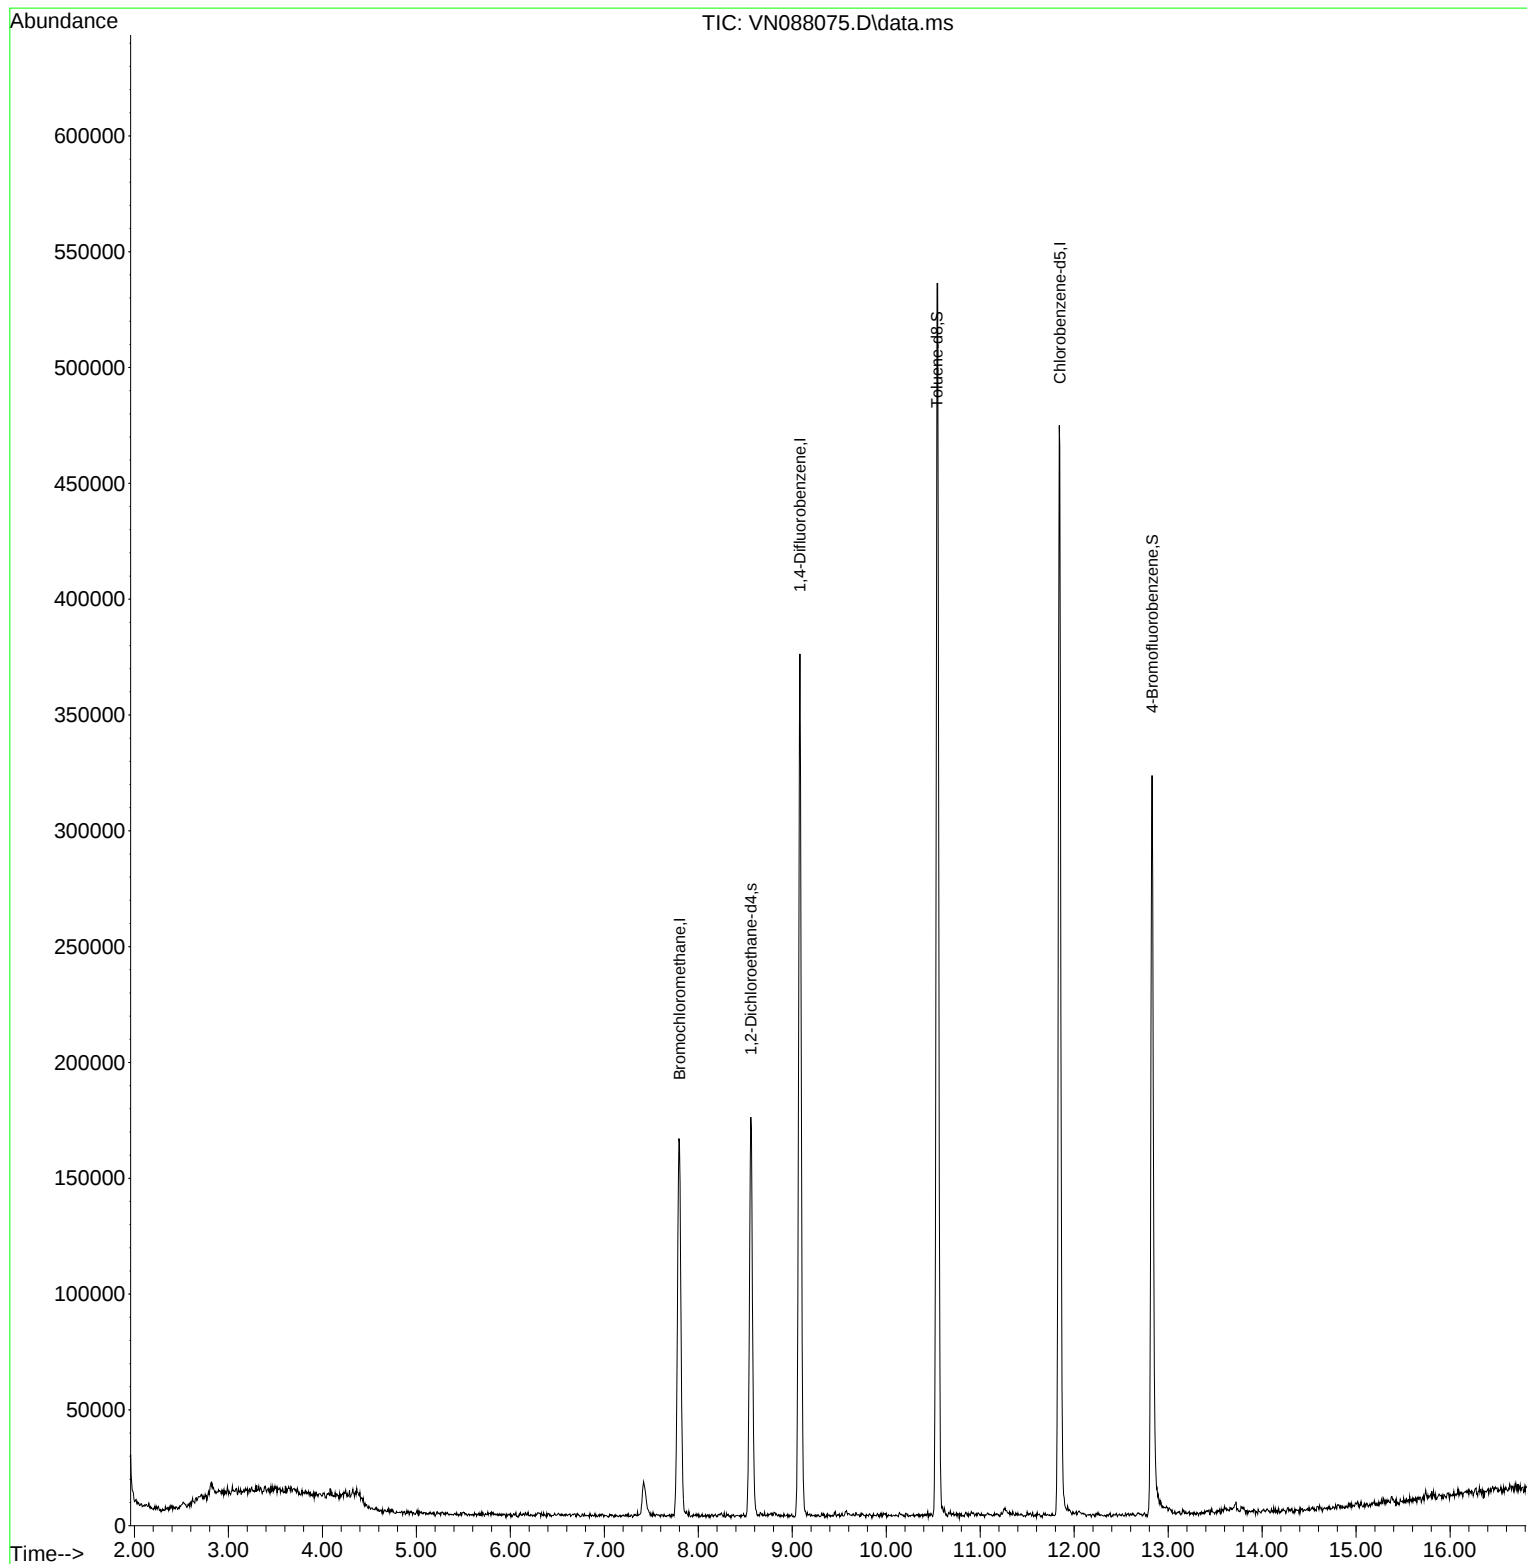


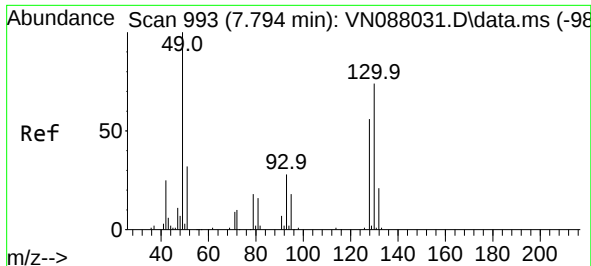

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.800 min Scan# 993
Delta R.T. 0.006 min
Lab File: VN088075.D
Acq: 20 Oct 2025 10:55




Instrument :
MSVOA_N
ClientSampleId :
VN1020WBL01


Tgt Ion:128 Resp: 56116
Ion Ratio Lower Upper
128 100
49 189.1 0.0 439.8
130 125.0 0.0 325.8

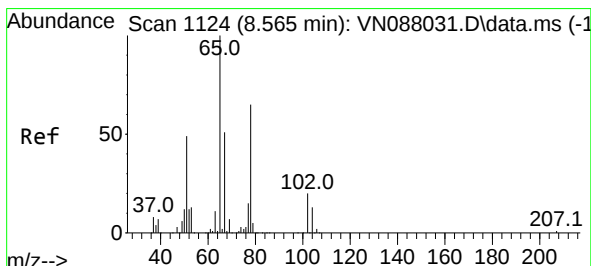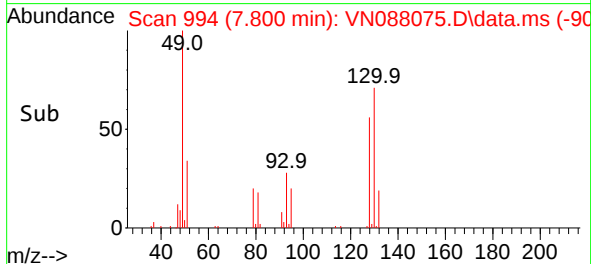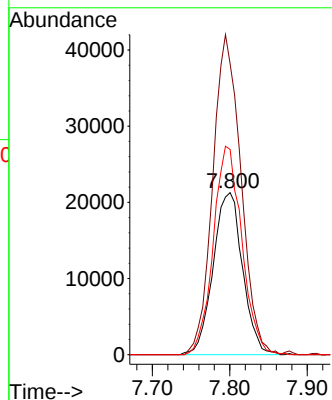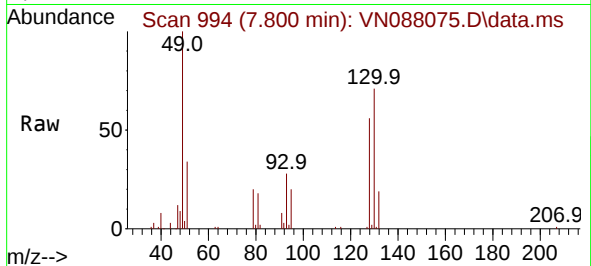

#27
1,2-Dichloroethane-d4
Concen: 32.550 ug/l
RT: 8.559 min Scan# 1123
Delta R.T. -0.006 min
Lab File: VN088075.D
Acq: 20 Oct 2025 10:55

Tgt Ion: 65 Resp: 142234
Ion Ratio Lower Upper
65 100
67 51.4 41.9 62.9

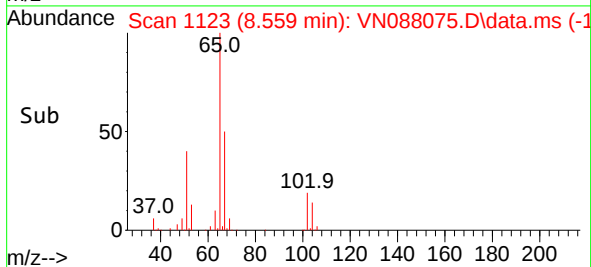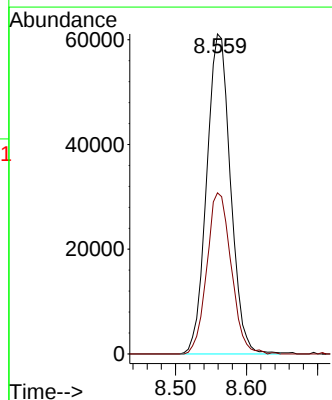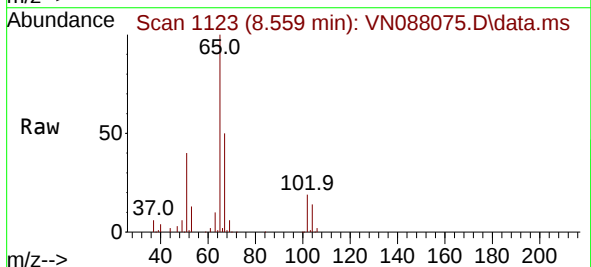

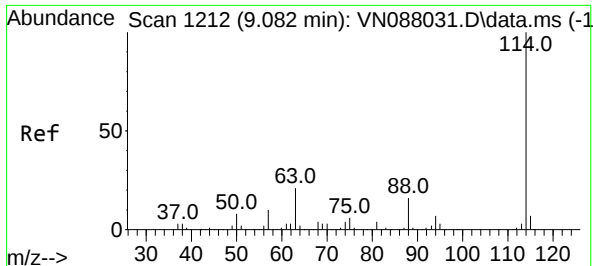

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 9.083 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN088075.D

Acq: 20 Oct 2025 10:55

Instrument :

MSVOA_N

ClientSampleId :

VN1020WBL01





Tgt Ion:114 Resp: 302542

Ion Ratio Lower Upper

114 100

63 22.1 16.6 25.0

88 16.3 12.6 18.8

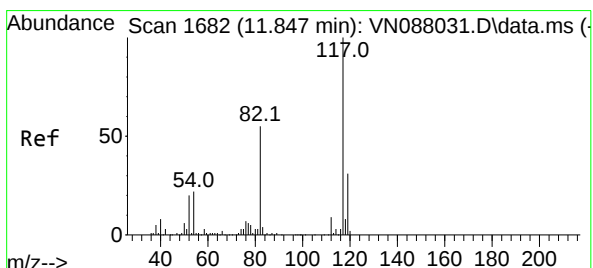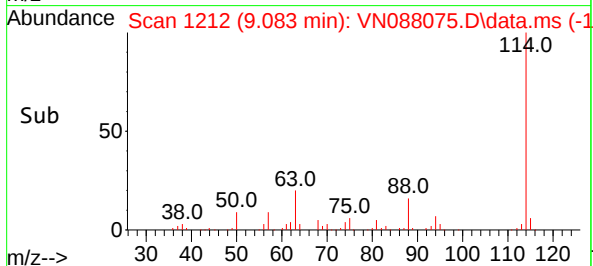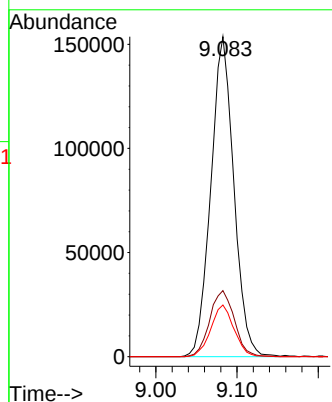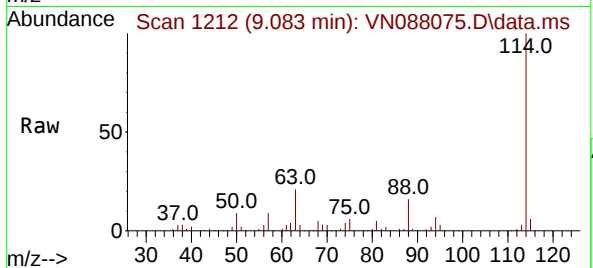

#57

Chlorobenzene-d5

Concen: 30.000 ug/l

RT: 11.847 min Scan# 1682

Delta R.T. 0.000 min

Lab File: VN088075.D

Acq: 20 Oct 2025 10:55




Tgt Ion:117 Resp: 267258


Ion Ratio Lower Upper

117 100

82 58.3 45.2 67.8

119 32.3 25.9 38.9


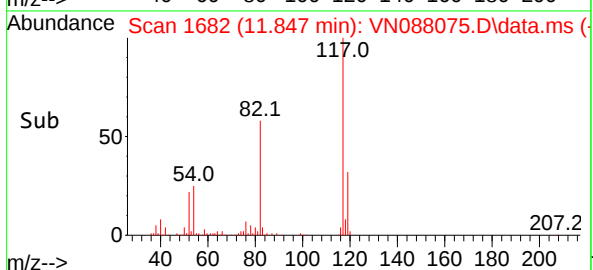
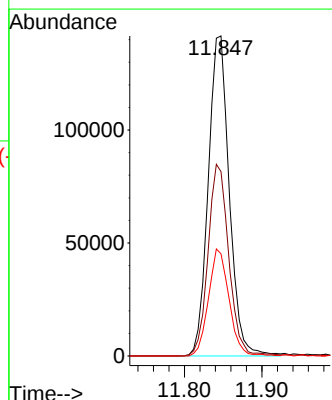
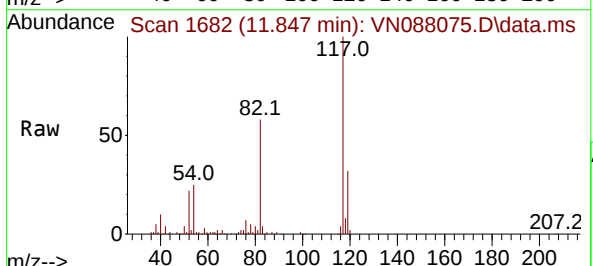


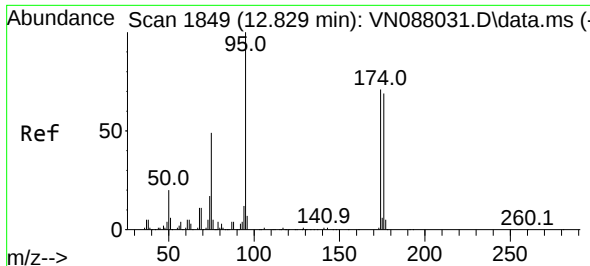

#60
4-Bromofluorobenzene
Concen: 28.421 ug/l
RT: 12.829 min Scan# 1849
Delta R.T. 0.000 min
Lab File: VN088075.D
Acq: 20 Oct 2025 10:55

Instrument :
MSVOA_N
ClientSampleId :
VN1020WBL01

Tgt Ion: 95 Resp: 125221
Ion Ratio Lower Upper
95 100
174 66.2 57.4 86.0
176 64.9 57.0 85.4

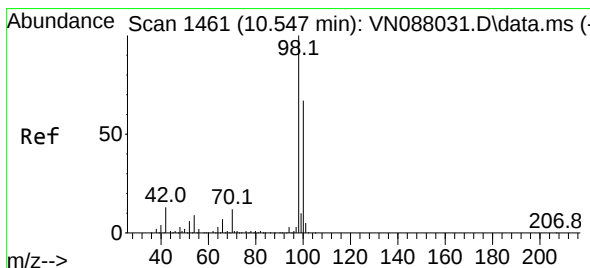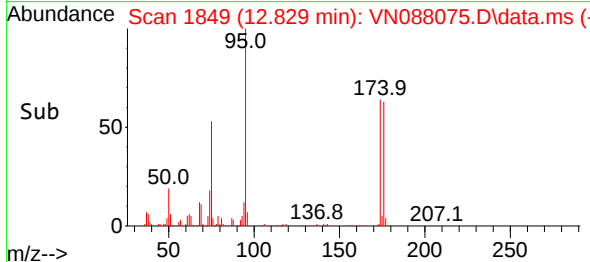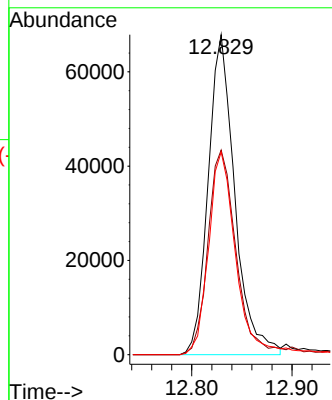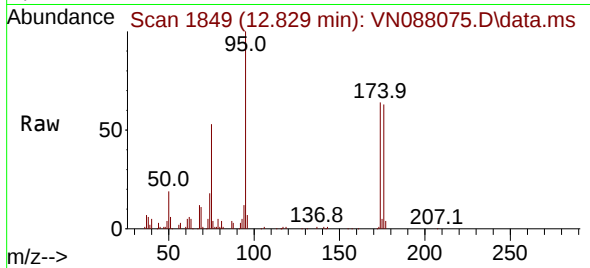

#63
Toluene-d8
Concen: 30.746 ug/l
RT: 10.541 min Scan# 1460
Delta R.T. -0.006 min
Lab File: VN088075.D
Acq: 20 Oct 2025 10:55

Tgt Ion: 98 Resp: 366105
Ion Ratio Lower Upper
98 100
100 65.5 53.1 79.7

