

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102125\
 Data File : P0114562.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2025 22:01
 Operator : YP/AJ
 Sample : Q3393-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PR132-S08-013038-20251017

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/22/2025
 Supervised By :mohammad ahmed 10/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 08:27:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 21 02:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.352	3.656	99334934	91586047	18.297m	22.884 #
2) SA Decachlor...	9.937	8.656	58257634	53177911	16.000	15.954

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102125\
Data File : PO114562.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2025 22:01
Operator : YP/AJ
Sample : Q3393-03
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PR132-S08-013038-20251017


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/22/2025
Supervised By :mohammad ahmed 10/24/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 08:27:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 21 02:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

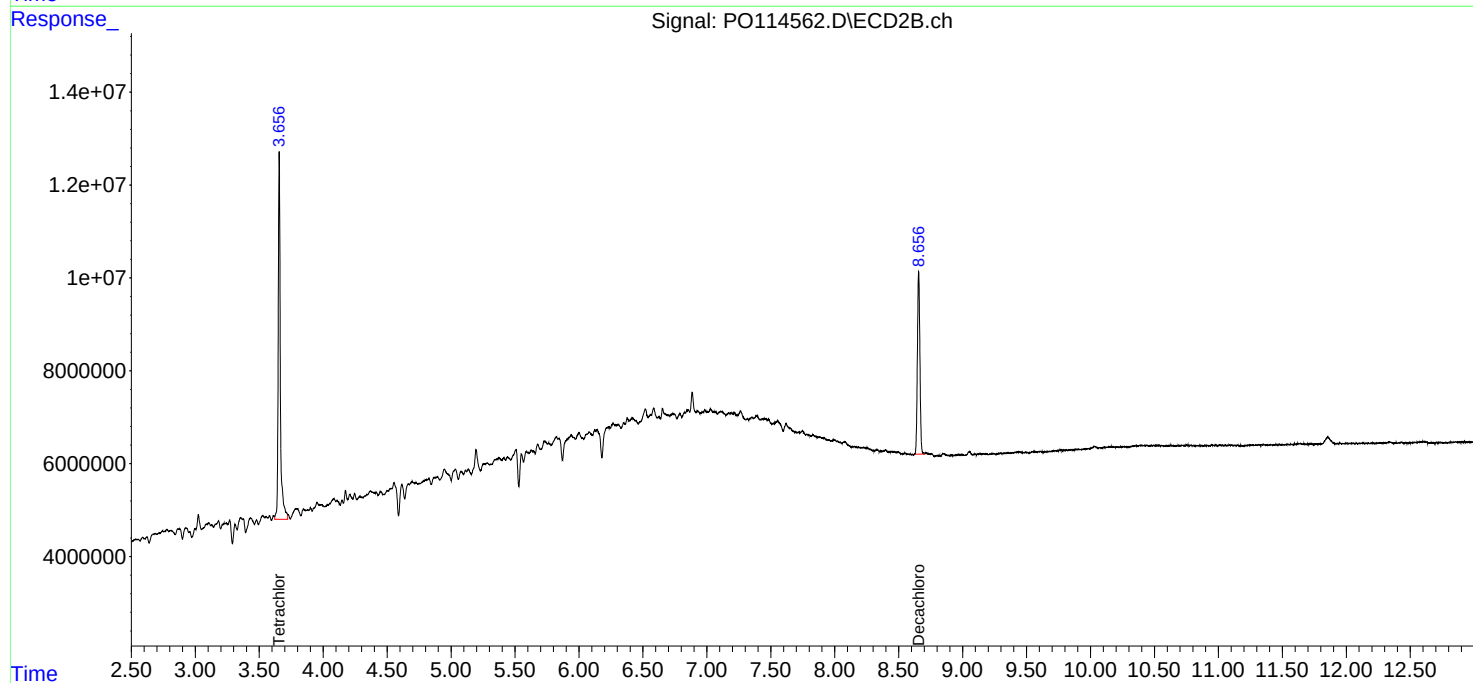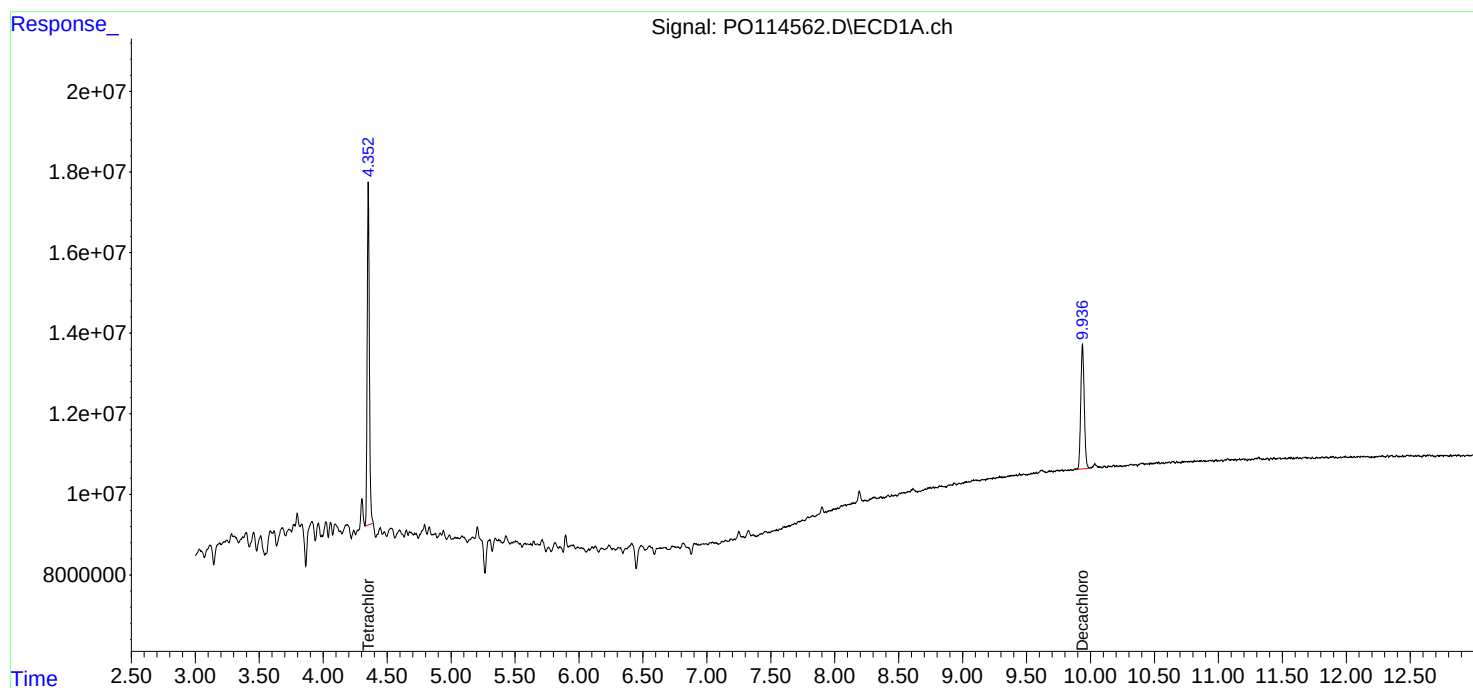

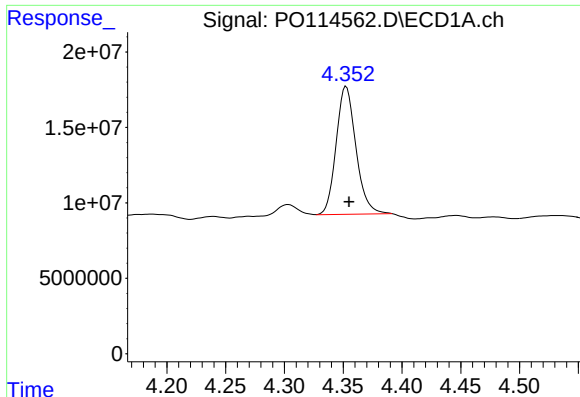


#1 Tetrachloro-m-xylene

R.T.: 4.352 min
Delta R.T.: -0.003 min
Response: 99334934
Conc: 18.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
PR132-S08-013038-20251017


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/22/2025
Supervised By :mohammad ahmed 10/24/2025

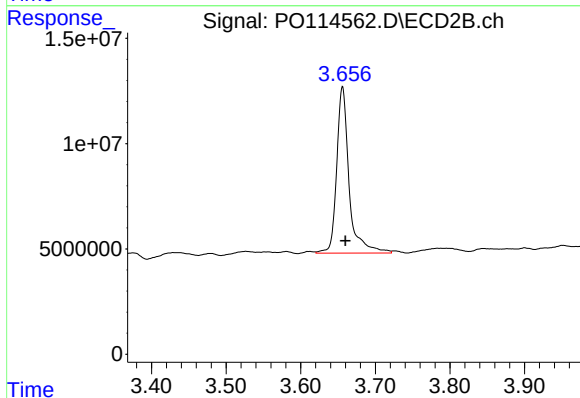


#1 Tetrachloro-m-xylene

R.T.: 3.656 min
Delta R.T.: -0.004 min
Response: 91586047
Conc: 22.88 ng/ml

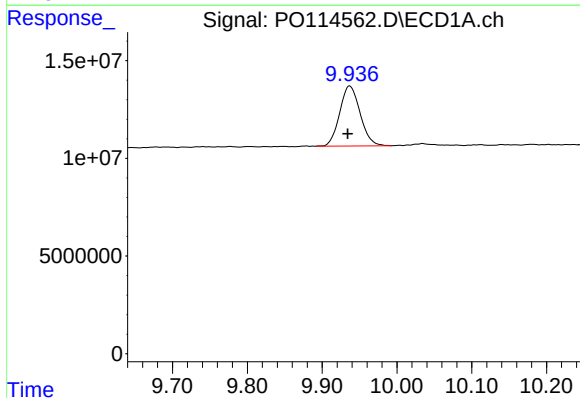

#2 Decachlorobiphenyl

R.T.: 9.937 min
Delta R.T.: 0.002 min
Response: 58257634
Conc: 16.00 ng/ml

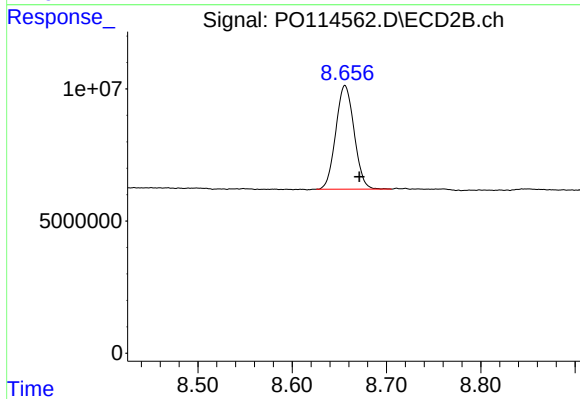

#2 Decachlorobiphenyl

R.T.: 8.656 min
Delta R.T.: -0.015 min
Response: 53177911
Conc: 15.95 ng/ml