

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102125\
 Data File : PO114563.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2025 22:19
 Operator : YP/AJ
 Sample : Q3393-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PR132-S06-000021-20251017

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/22/2025
 Supervised By :mohammad ahmed 10/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 08:28:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 21 02:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.354	3.656	138.6E6	109.9E6	25.537m	27.452
2) SA Decachlor...	9.943	8.658	76114124	70108643	20.904	21.034

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102125\
Data File : PO114563.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2025 22:19
Operator : YP/AJ
Sample : Q3393-04
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PR132-S06-000021-20251017


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/22/2025
Supervised By :mohammad ahmed 10/24/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 08:28:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 21 02:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

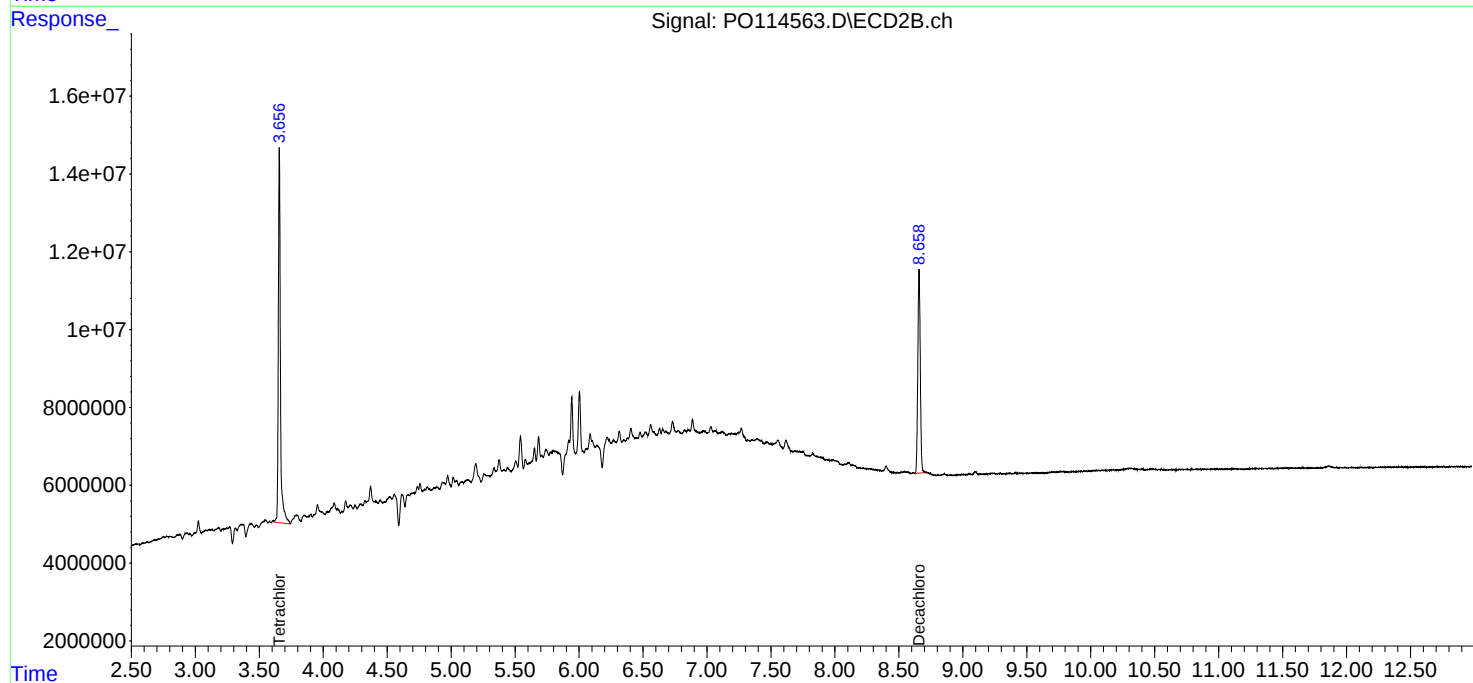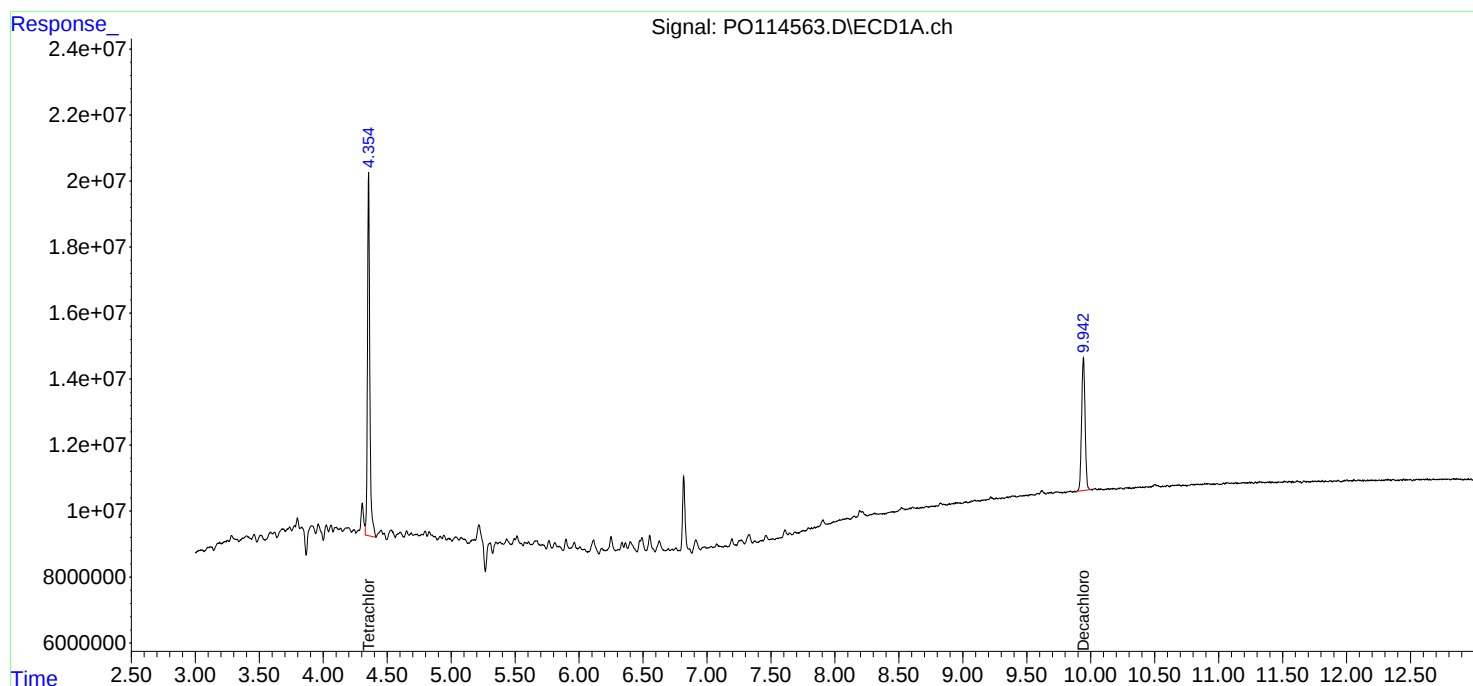

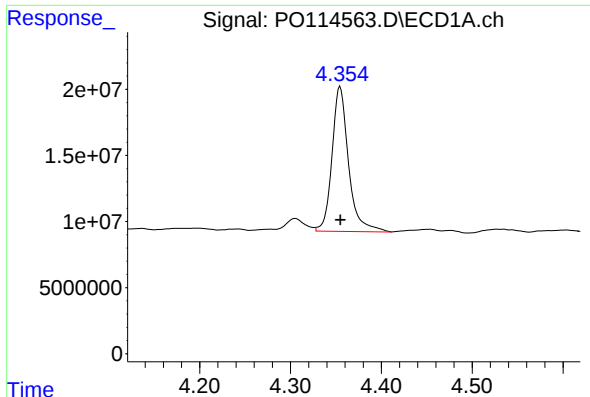


#1 Tetrachloro-m-xylene

R.T.: 4.354 min
Delta R.T.: -0.001 min
Response: 138638354
Conc: 25.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
PR132-S06-000021-20251017


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/22/2025
Supervised By :mohammad ahmed 10/24/2025

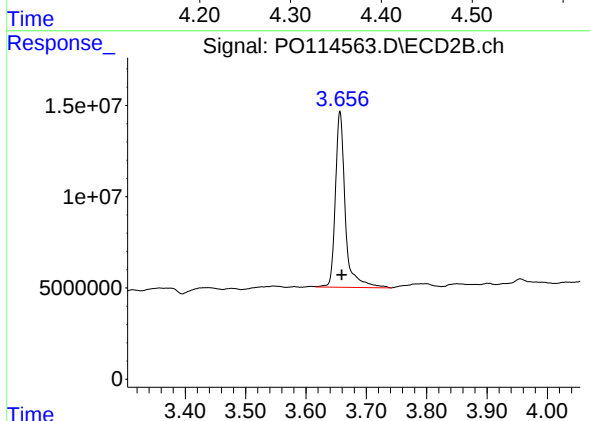


#1 Tetrachloro-m-xylene

R.T.: 3.656 min
Delta R.T.: -0.003 min
Response: 109870590
Conc: 27.45 ng/ml

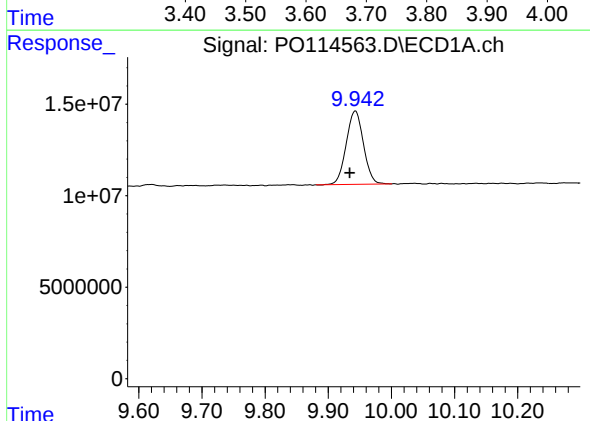

#2 Decachlorobiphenyl

R.T.: 9.943 min
Delta R.T.: 0.009 min
Response: 76114124
Conc: 20.90 ng/ml

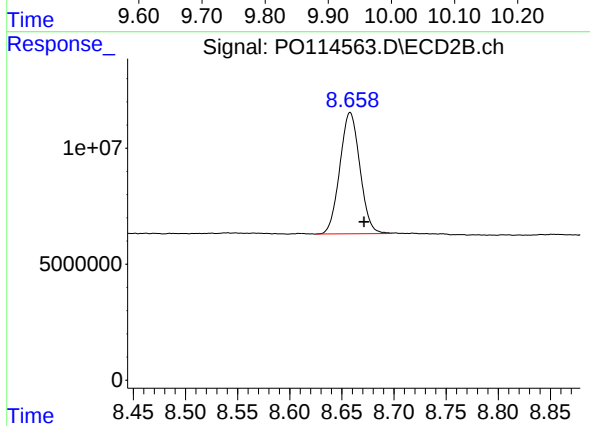

#2 Decachlorobiphenyl

R.T.: 8.658 min
Delta R.T.: -0.013 min
Response: 70108643
Conc: 21.03 ng/ml