


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102125\
Data File : BF144008.D
Acq On : 21 Oct 2025 12:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 06 15:29:47 2025

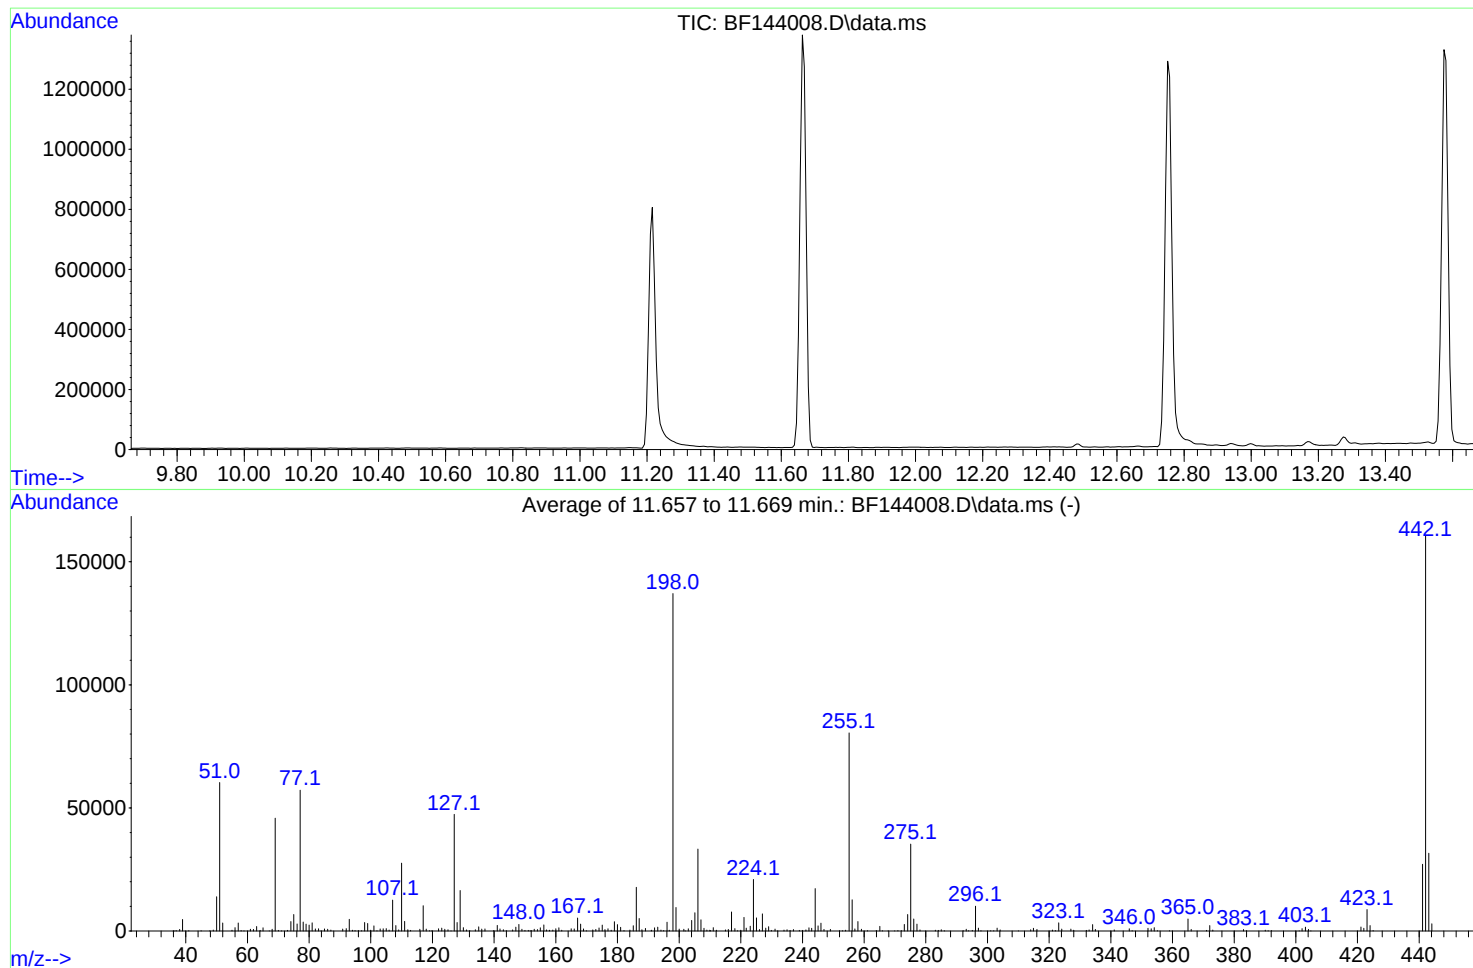

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1603

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	715	PASS
69	69	100	100	100.0	45819	PASS
70	69	0.00	2	0.5	248	PASS
197	198	0.00	2	0.2	322	PASS
198	198	100	100	100.0	137115	PASS
199	198	5	9	7.0	9565	PASS
365	198	1	100	3.6	4896	PASS
441	443	0.01	150	85.7	27087	PASS
442	442	100	100	100.0	160408	PASS
443	442	15	24	19.7	31611	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/21/2025	BNA_F	<u>BF144008.D</u>
Compound Name	Response	Retention Time
DDT	371363	13.58
DDD	9829	13.274
DDE	2408	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12237	383600	3.19

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102125\
Data File : BF144008.D
Acq On : 21 Oct 2025 12:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 21 13:56:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

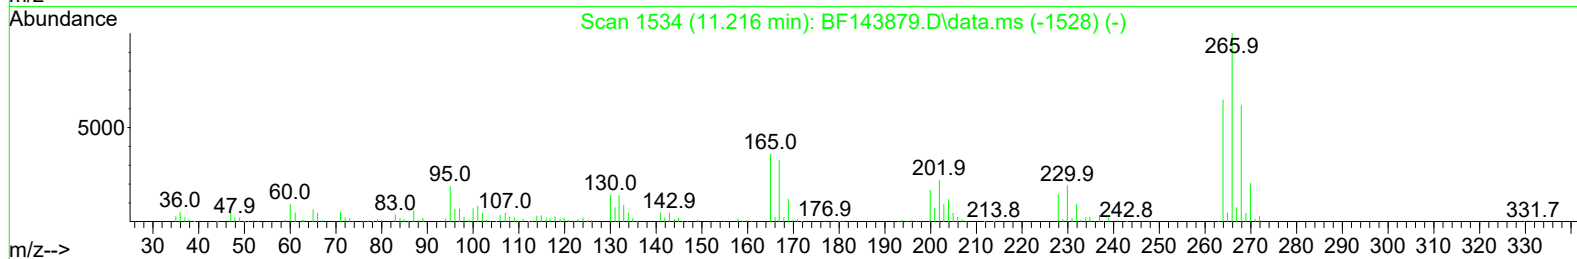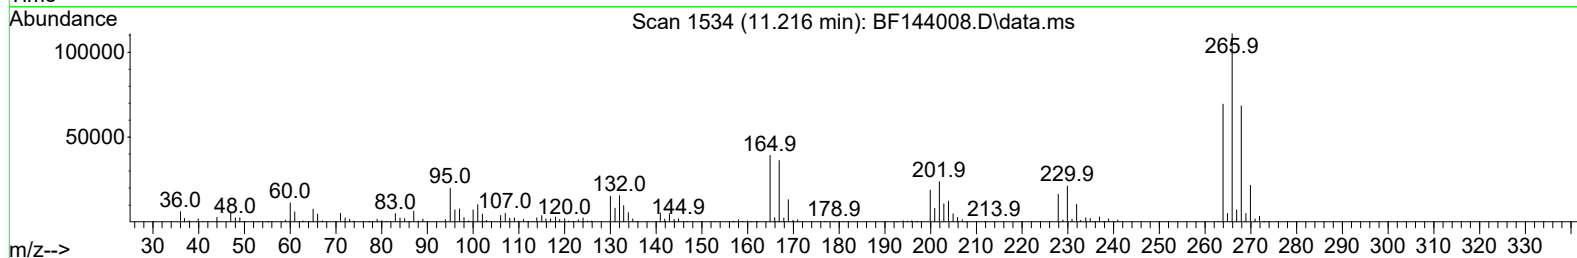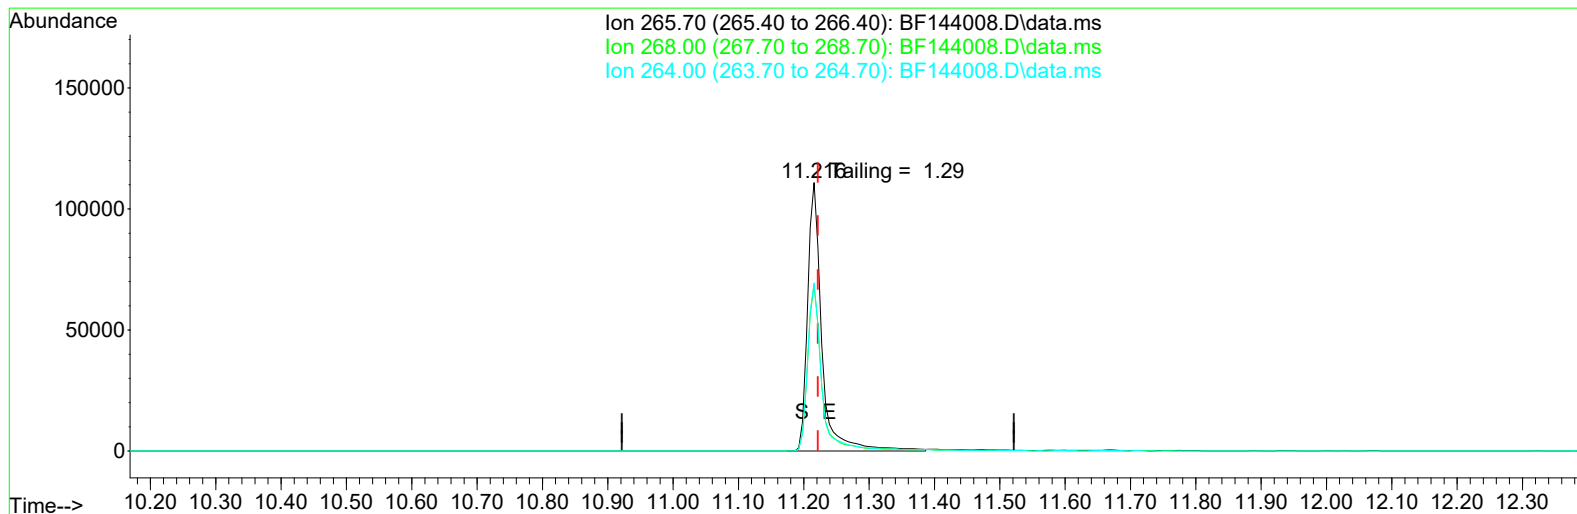

TIC: BF144008.D\data.ms

(70) Pentachlorophenol (C)




11.216min (-0.006) 31834.77 ng

response 169131

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	61.71
264.00	64.70	62.61
0.00	0.00	0.00

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 21 13:56:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

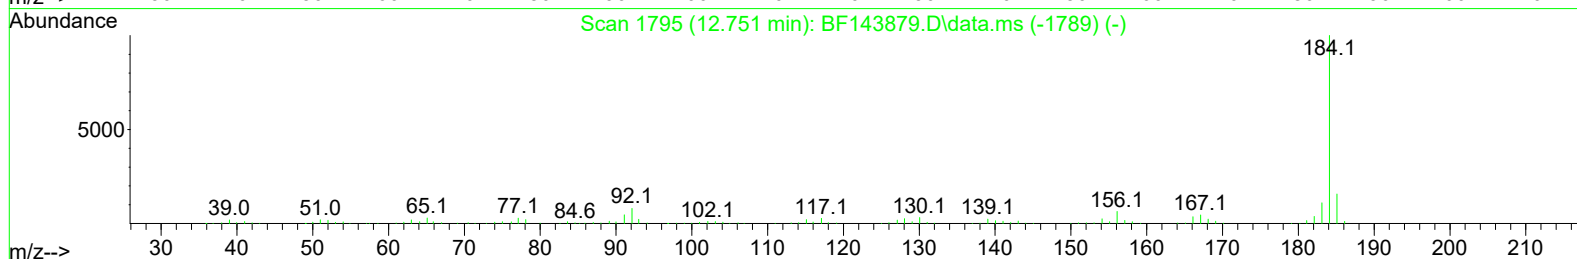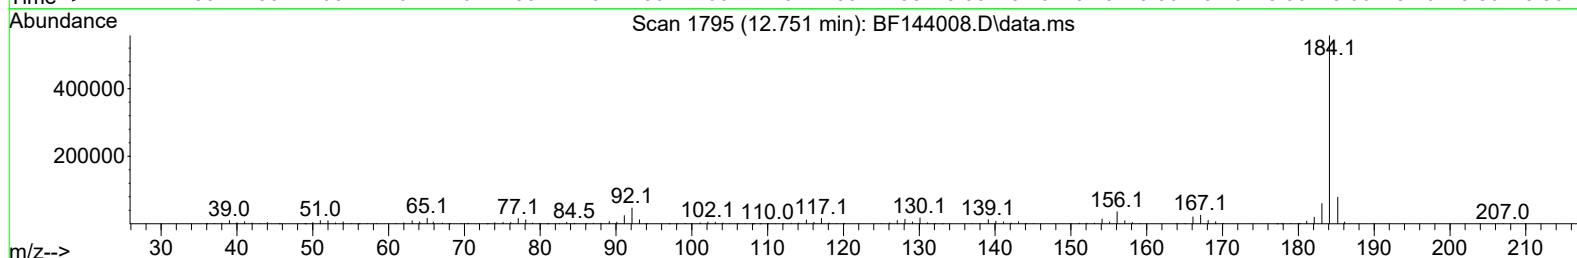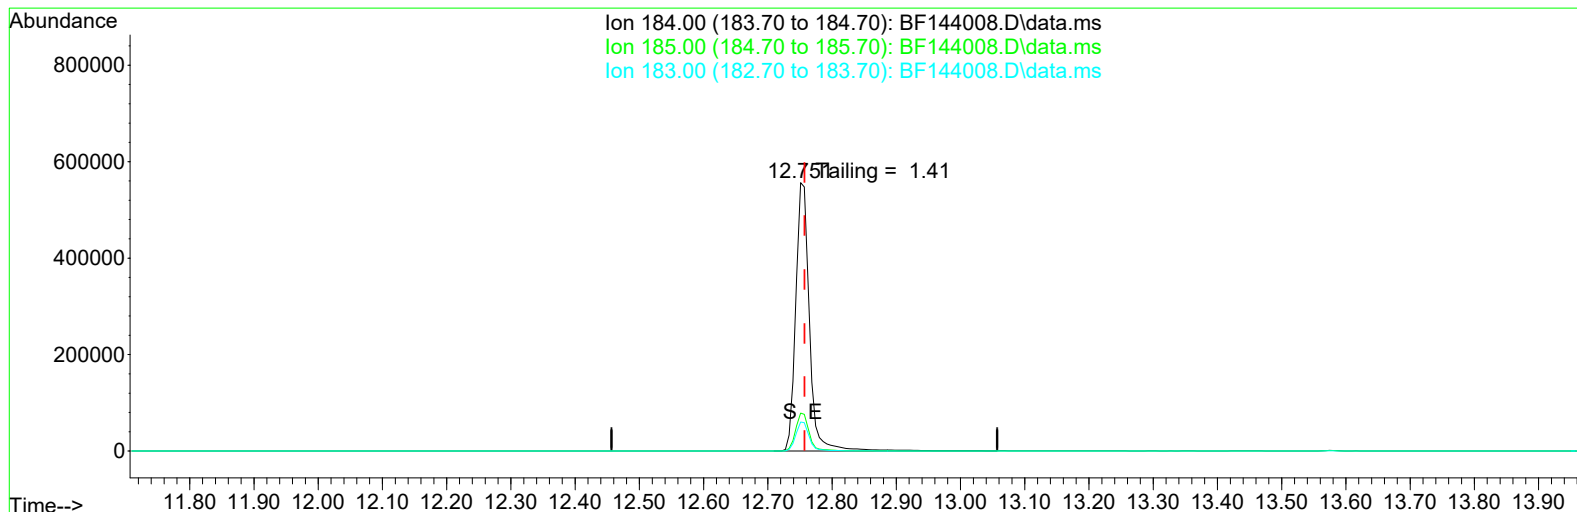

TIC: BF144008.D\data.ms

(77) Benzidine

12.751min (-0.006) 0.00 ng

response 827233

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.17
183.00	11.00	10.79
0.00	0.00	0.00