


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102225\
Data File : BF144031.D
Acq On : 22 Oct 2025 09:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 06 15:29:47 2025

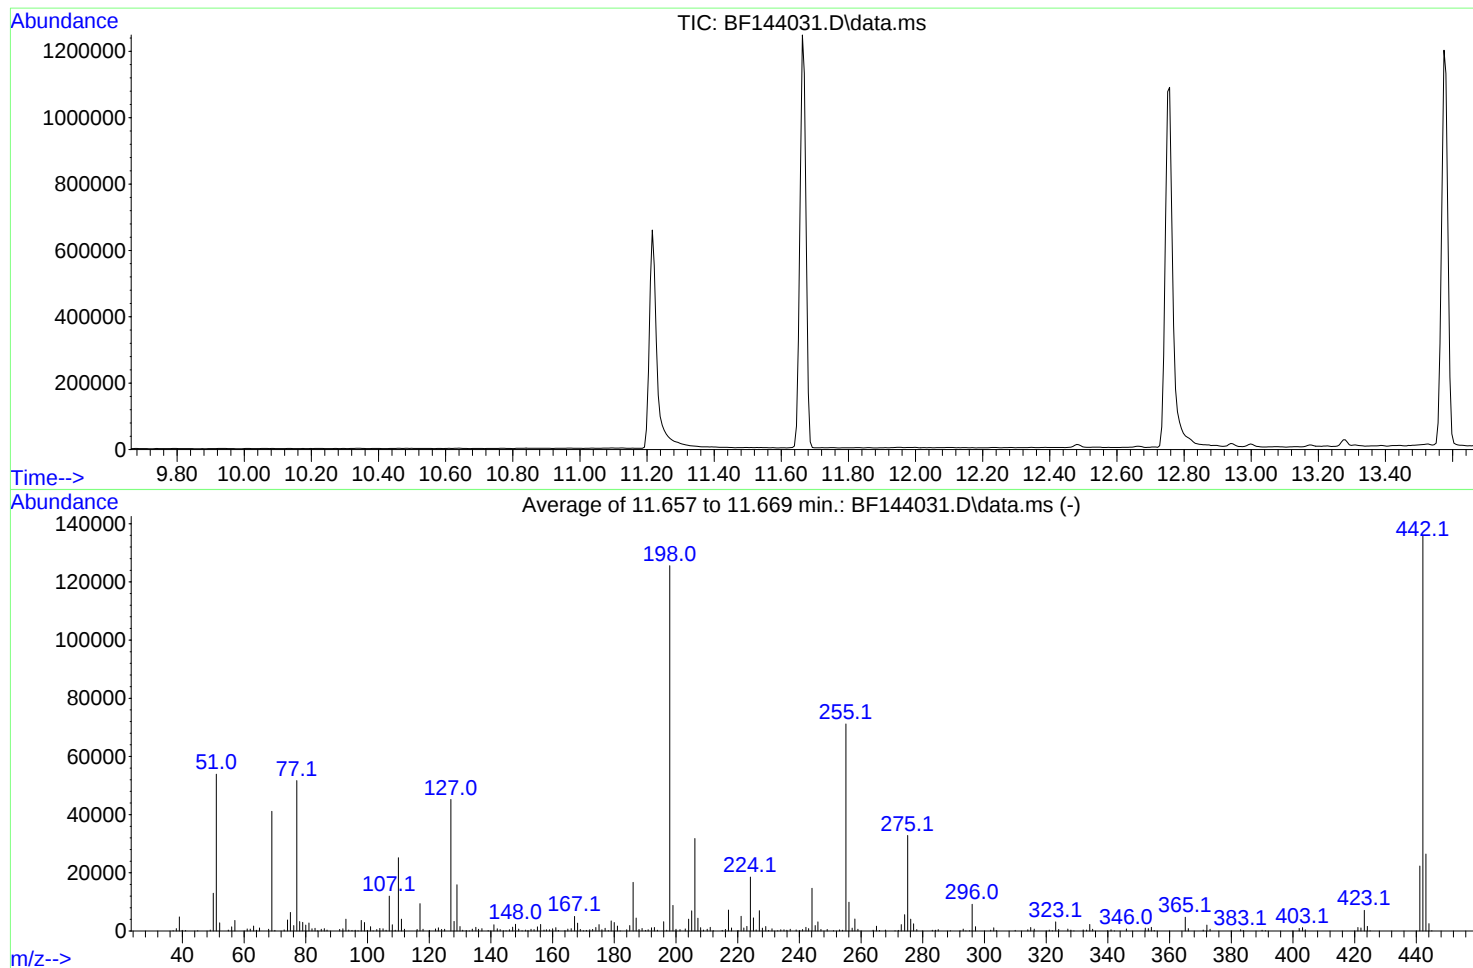

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1603

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.5	610	PASS
69	69	100	100	100.0	41155	PASS
70	69	0.00	2	0.6	235	PASS
197	198	0.00	2	0.2	273	PASS
198	198	100	100	100.0	125584	PASS
199	198	5	9	7.0	8799	PASS
365	198	1	100	3.8	4712	PASS
441	443	0.01	150	84.6	22367	PASS
442	442	100	100	100.0	135728	PASS
443	442	15	24	19.5	26434	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/22/2025	BNA_F	<u>BF144031.D</u>
Compound Name	Response	Retention Time
DDT	316043	13.574
DDD	8713	13.28
DDE	2730	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11443	327486	3.49

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102225\
Data File : BF144031.D
Acq On : 22 Oct 2025 09:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 22 12:25:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

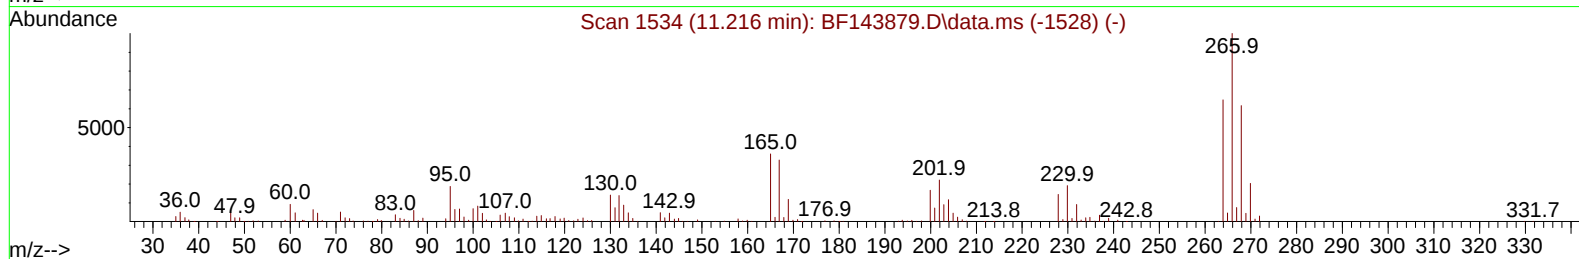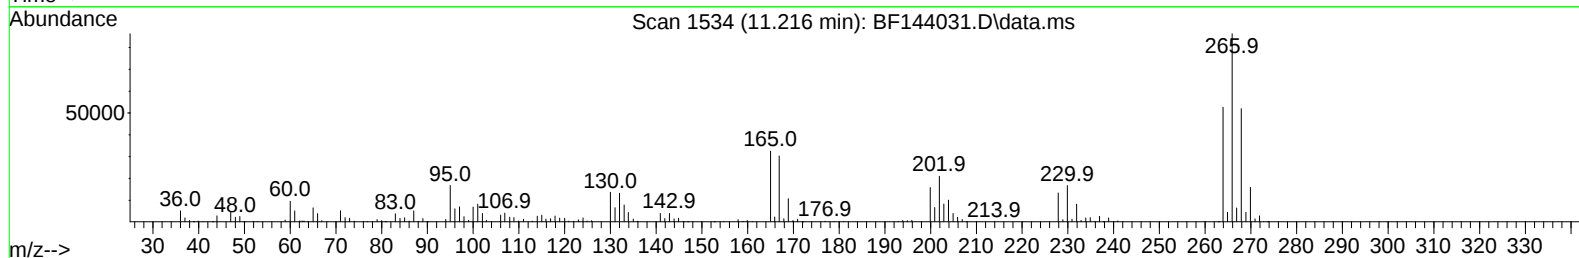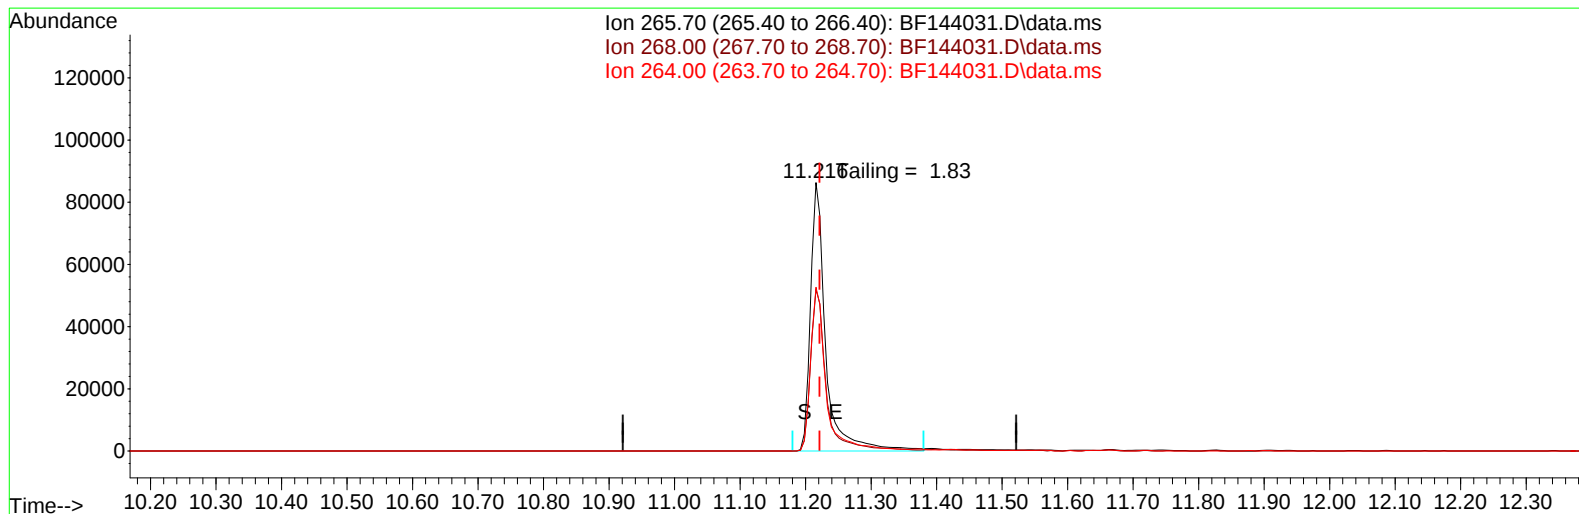

TIC: BF144031.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.006) 25307.30 ng




response 139659

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	60.26
264.00	64.70	61.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102225\
Data File : BF144031.D
Acq On : 22 Oct 2025 09:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 22 12:25:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

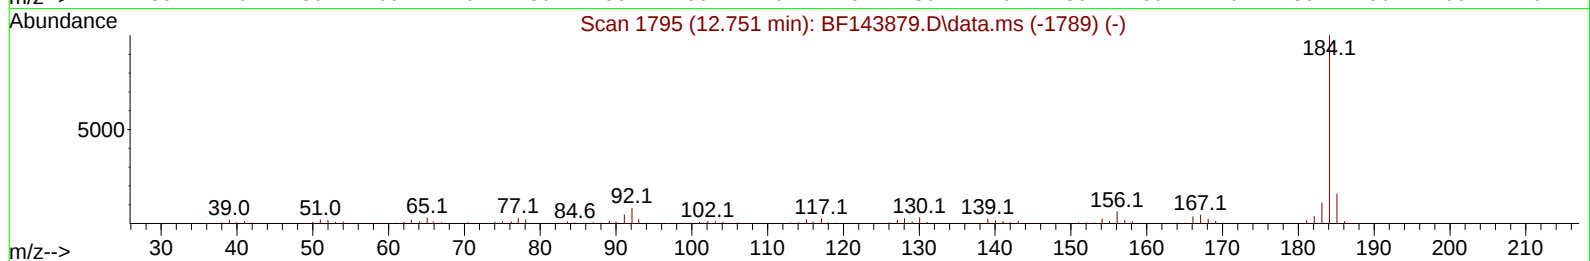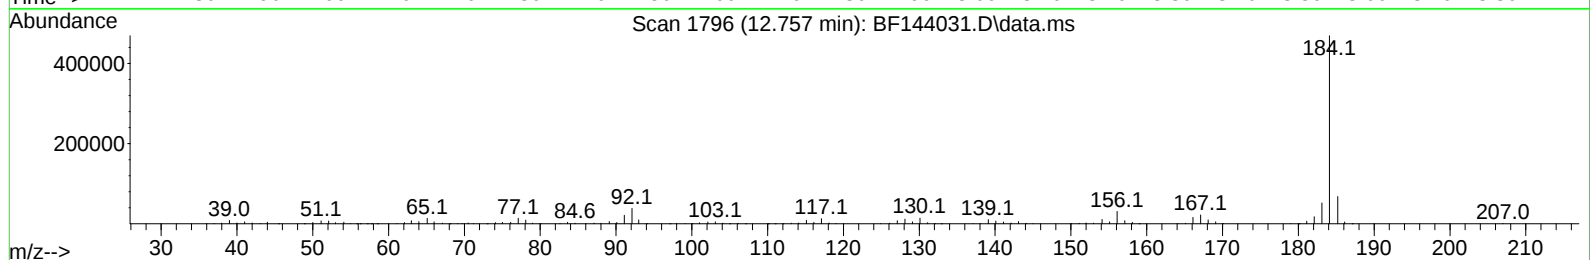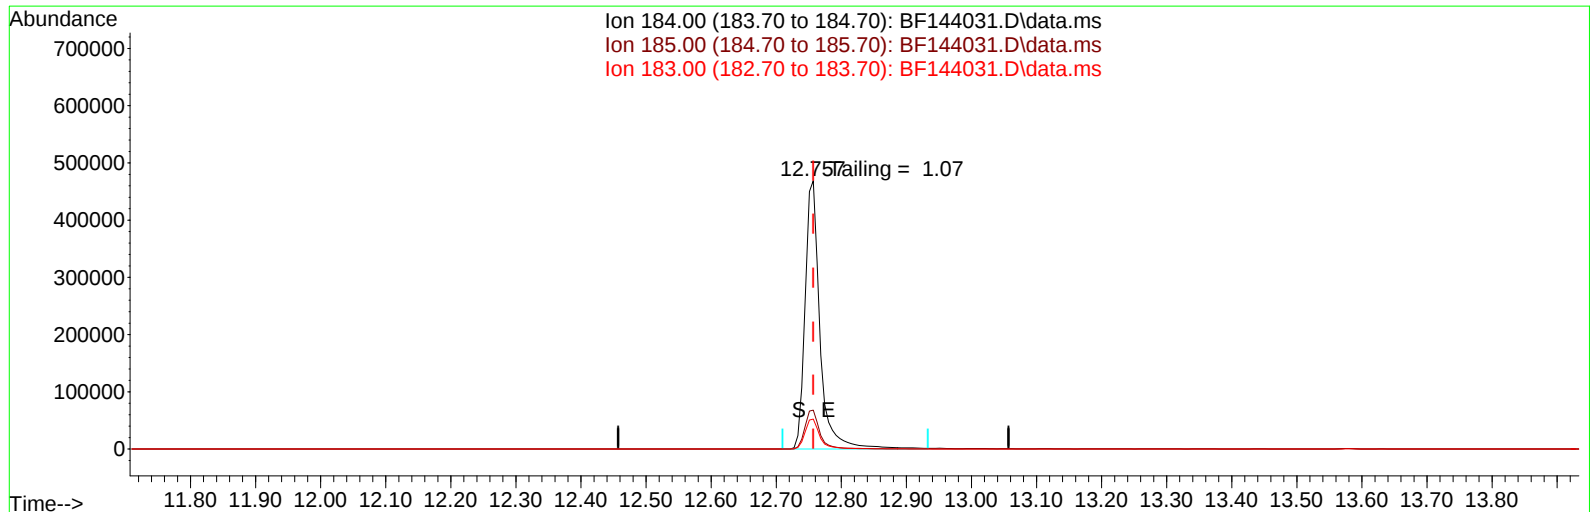

TIC: BF144031.D\data.ms

(77) Benzidine

12.757min (-0.000) 0.00 ng

response 749496

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.47
183.00	11.00	11.14
0.00	0.00	0.00