
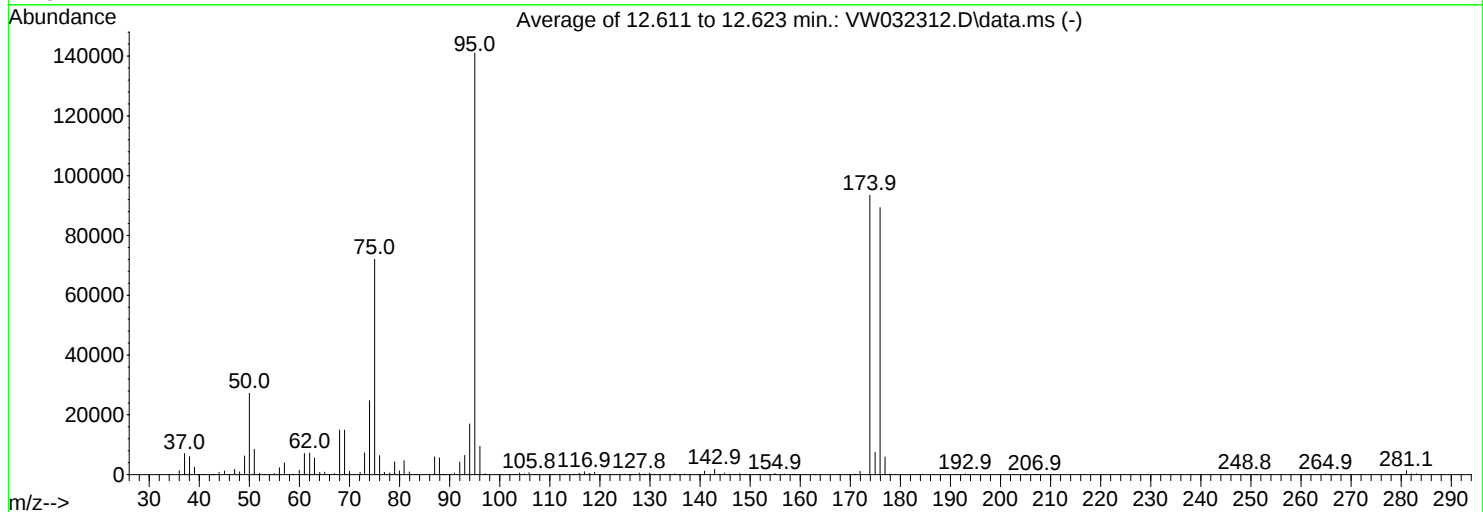


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100125\
 Data File : VW032312.D
 Acq On : 01 Oct 2025 08:12
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W100125S.M
 Title : SW846 8260
 Last Update : Thu Oct 02 21:24:16 2025

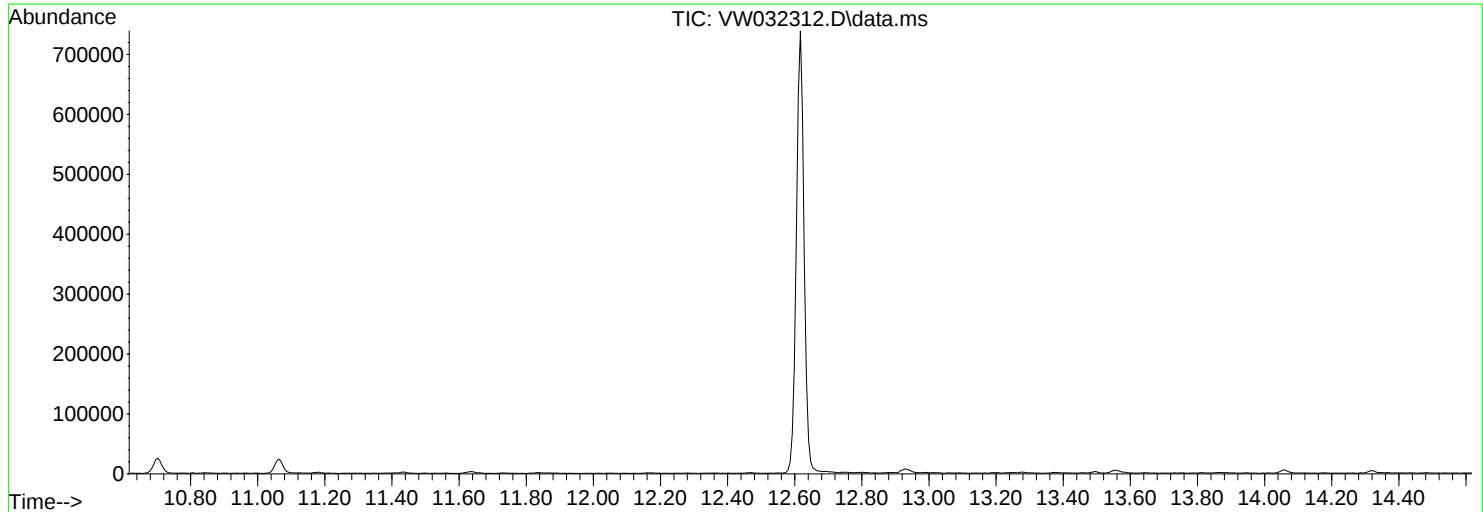

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	27221	PASS
75	95	30	60	51.1	72061	PASS
95	95	100	100	100.0	141091	PASS
96	95	5	9	6.7	9491	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	66.2	93424	PASS
175	174	5	9	8.0	7516	PASS
176	174	95	101	95.6	89325	PASS
177	176	5	9	6.6	5907	PASS