
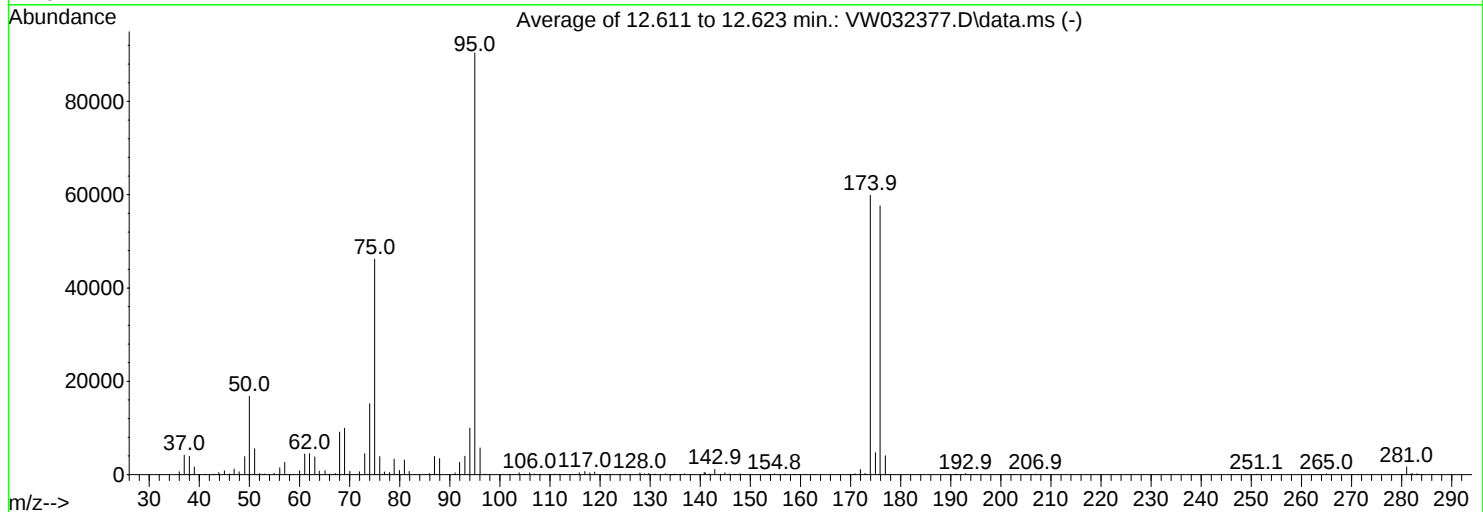


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102025\
Data File : VW032377.D
Acq On : 20 Oct 2025 09:36
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W100125S.M
Title : SW846 8260
Last Update : Thu Oct 02 21:24:16 2025

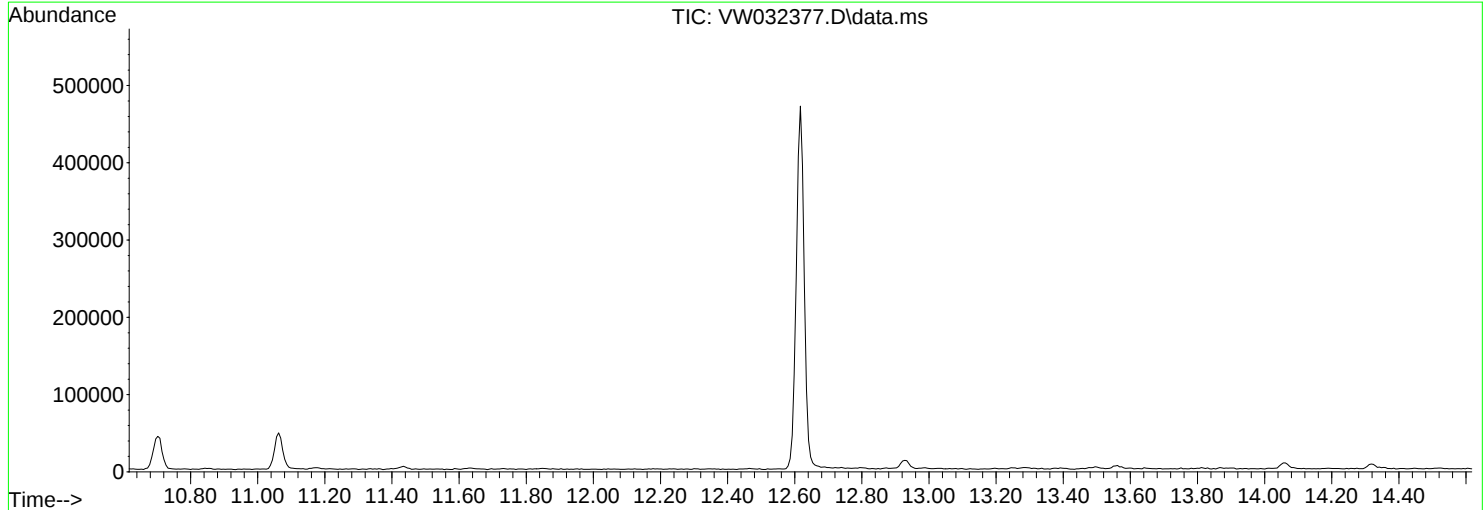

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	16809	PASS
75	95	30	60	51.1	46188	PASS
95	95	100	100	100.0	90408	PASS
96	95	5	9	6.3	5736	PASS
173	174	0.00	2	0.5	276	PASS
174	95	50	100	66.2	59875	PASS
175	174	5	9	7.8	4687	PASS
176	174	95	101	96.2	57613	PASS
177	176	5	9	7.0	4059	PASS