


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102725\
Data File : BF144073.D
Acq On : 27 Oct 2025 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 24 17:30:25 2025

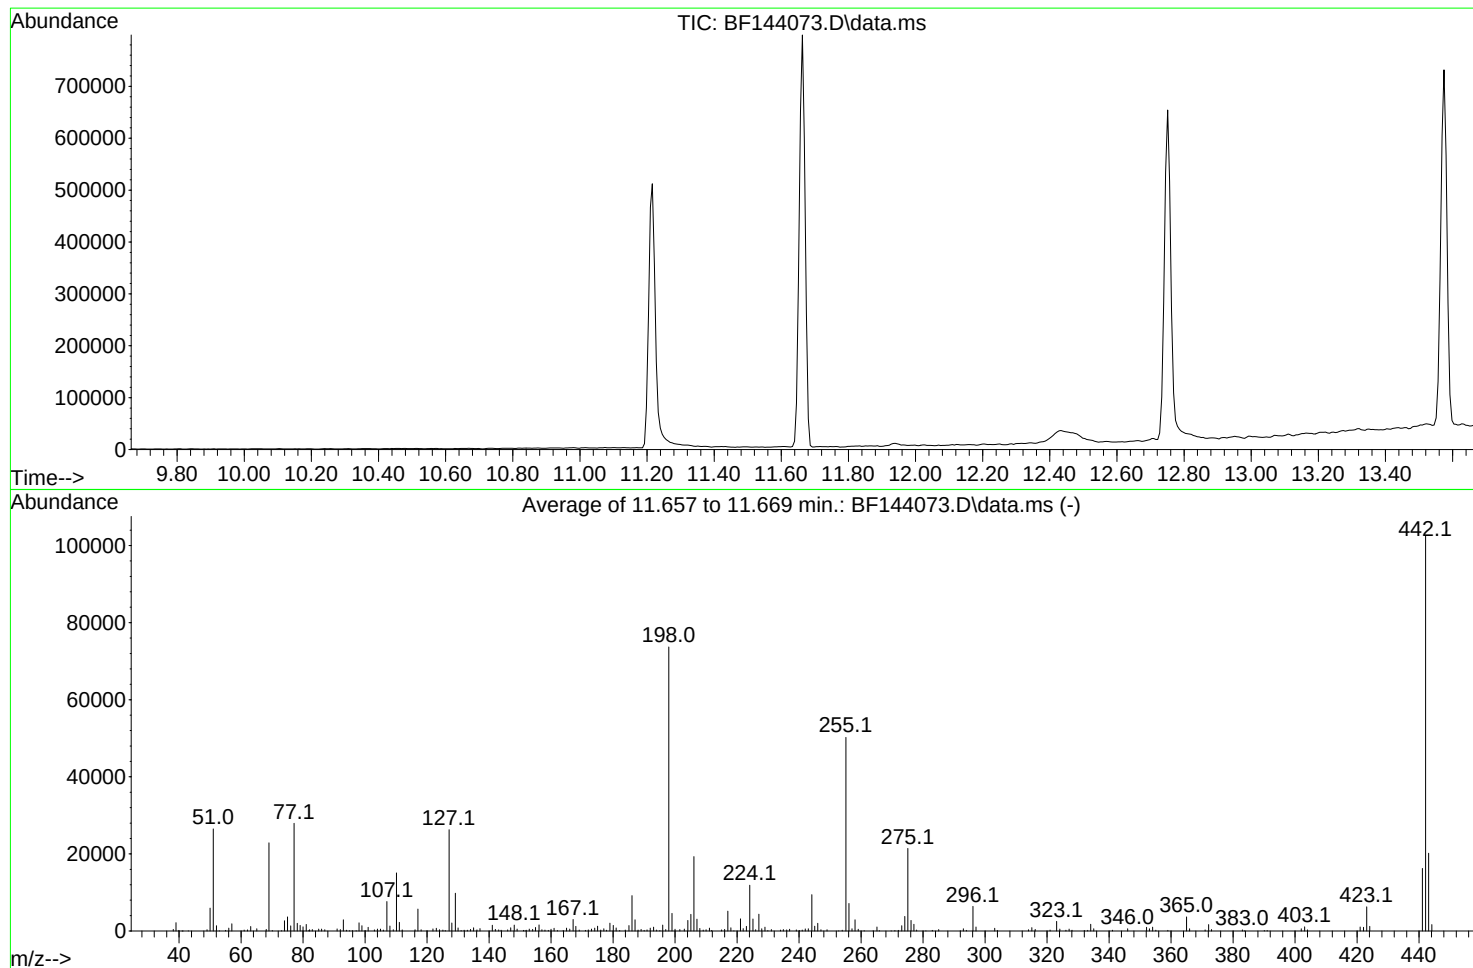




AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.9	439	PASS
69	69	100	100	100.0	22889	PASS
70	69	0.00	2	0.5	121	PASS
197	198	0.00	2	0.5	369	PASS
198	198	100	100	100.0	73707	PASS
199	198	5	9	6.2	4588	PASS
365	198	1	100	4.9	3647	PASS
441	443	0.01	150	80.6	16254	PASS
442	442	100	100	100.0	102437	PASS
443	442	15	24	19.7	20159	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102725\
Data File : BF144073.D
Acq On : 27 Oct 2025 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 27 11:44:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 17:30:25 2025
Response via : Initial Calibration

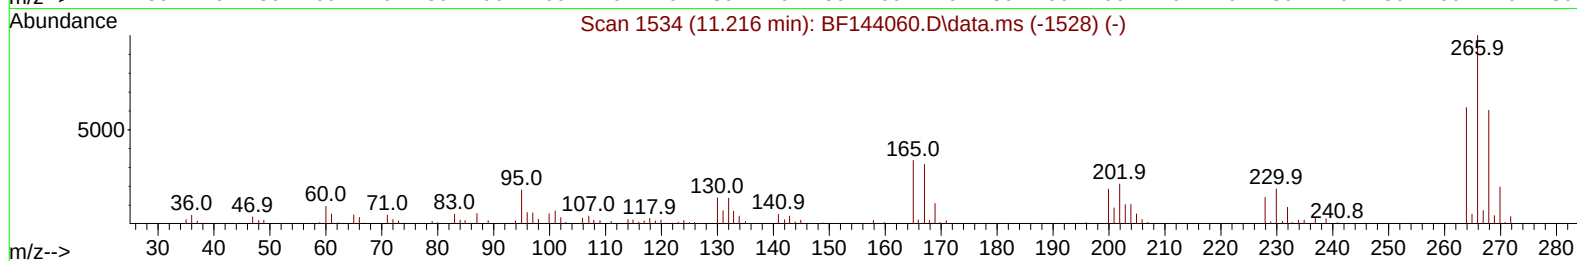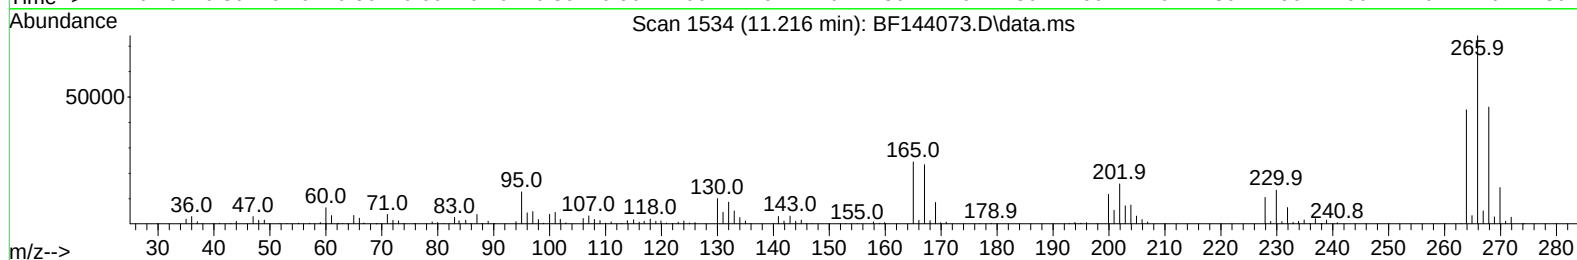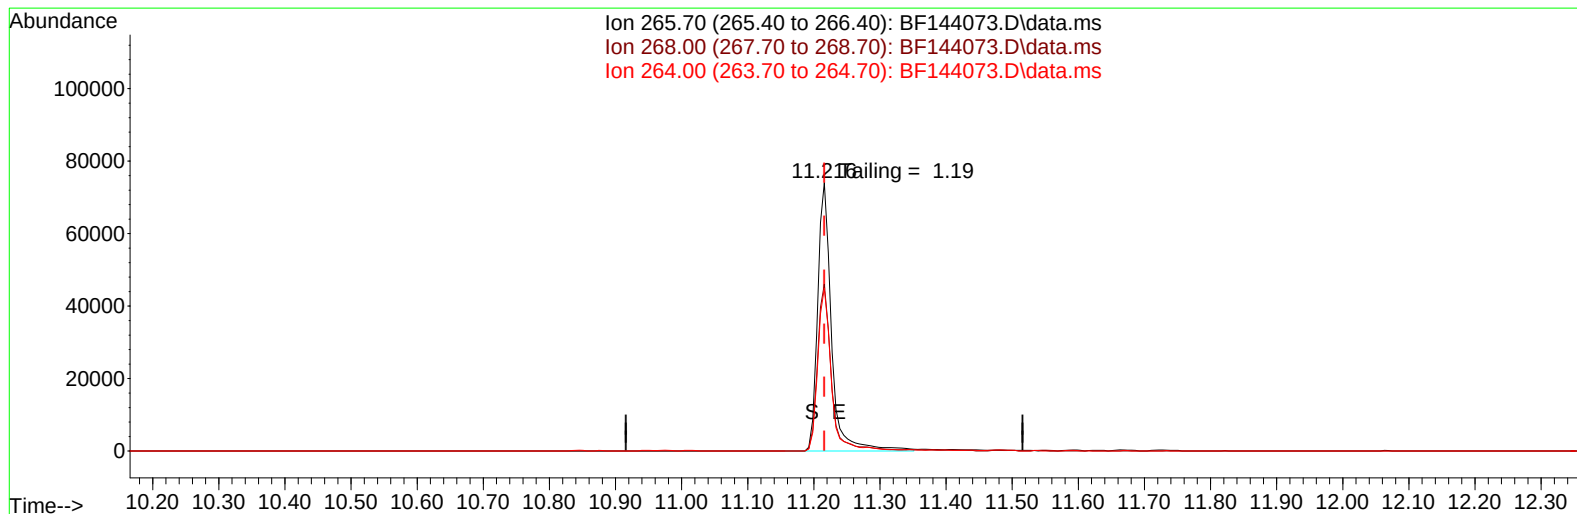

TIC: BF144073.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.000) 52871.76 ng




response 108593

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.30	62.12
264.00	61.70	60.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102725\
Data File : BF144073.D
Acq On : 27 Oct 2025 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 27 11:44:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 17:30:25 2025
Response via : Initial Calibration

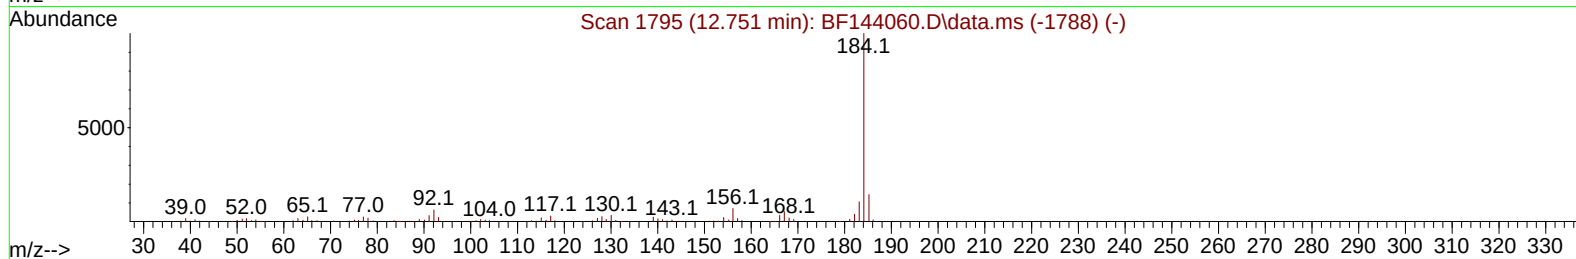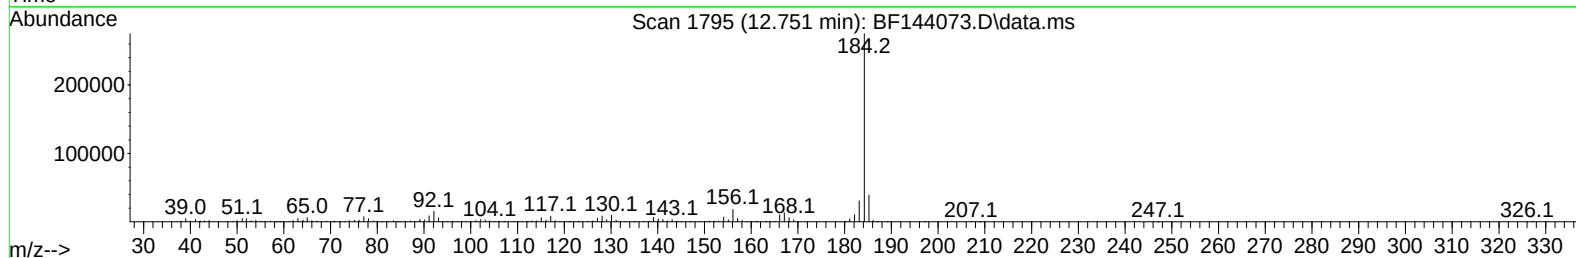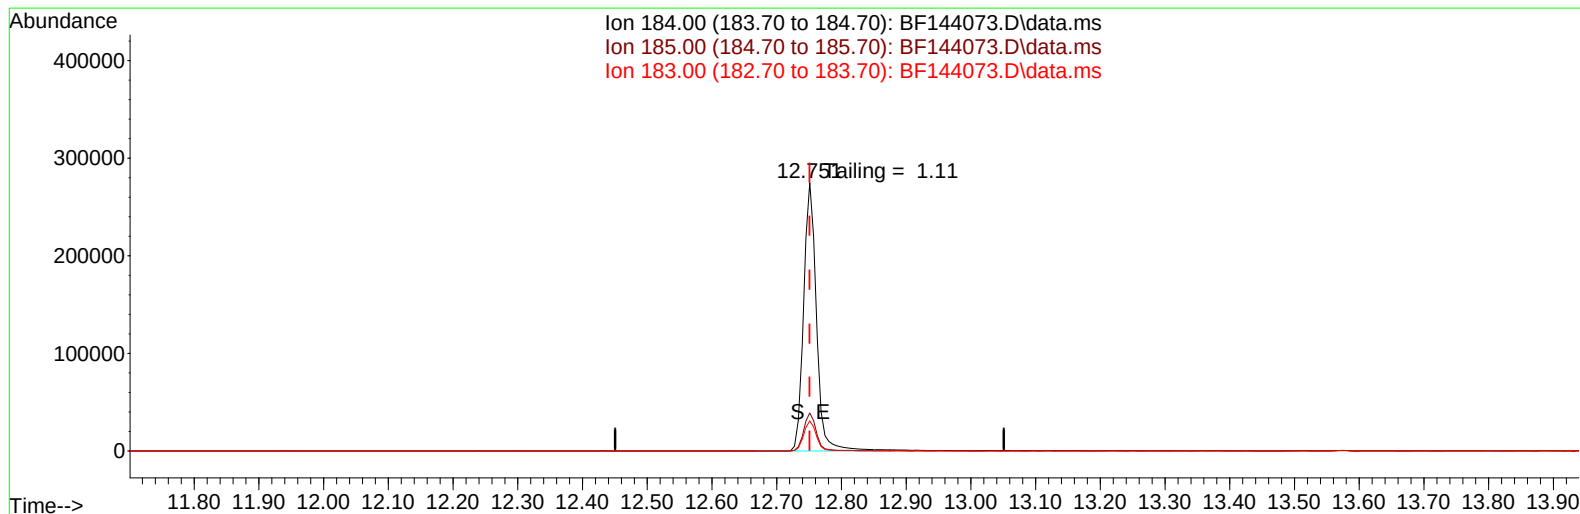

TIC: BF144073.D\data.ms

(77) Benzidine

12.751min (+ 0.000) 21247.29 ng m

response 380221

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.21
183.00	10.60	11.20
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/27/2025	BNA_F	<u>BF144073.D</u>
Compound Name	Response	Retention Time
DDT	178874	13.574
DDD	2782	13.275
DDE	115	12.992
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2897	181771	1.59

Instrument :
BNA_F
ClientSampleId :
DFTPP