

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102725\
 Data File : BF144086.D
 Acq On : 27 Oct 2025 16:33
 Operator : RC/JU
 Sample : Q3395-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PR132-S07-000102-22510170

Quant Time: Oct 27 17:06:05 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 24 17:30:25 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.881	152	49197	20.000	ng	0.00
21) Naphthalene-d8	8.163	136	182564	20.000	ng	0.00
39) Acenaphthene-d10	9.916	164	93912	20.000	ng	0.00
64) Phenanthrene-d10	11.410	188	147369	20.000	ng	0.00
76) Chrysene-d12	14.057	240	132745	20.000	ng	0.00
86) Perylene-d12	15.539	264	166960	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.498	112	284104	91.364	ng	0.00
7) Phenol-d6	6.504	99	322671	93.958	ng	0.00
23) Nitrobenzene-d5	7.439	82	204522	61.377	ng	0.00
42) 2,4,6-Tribromophenol	10.710	330	98872	82.651	ng	0.00
45) 2-Fluorobiphenyl	9.233	172	371566	55.677	ng	0.00
79) Terphenyl-d14	12.998	244	341415	44.964	ng	0.00
Target Compounds						
71) Phenanthrene	11.433	178	20215	2.761	ng	96
75) Fluoranthene	12.627	202	21112	2.610	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102725\
Data File : BF144086.D
Acq On : 27 Oct 2025 16:33
Operator : RC/JU
Sample : Q3395-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PR132-S07-000102-22510170

Quant Time: Oct 27 17:06:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 17:30:25 2025
Response via : Initial Calibration




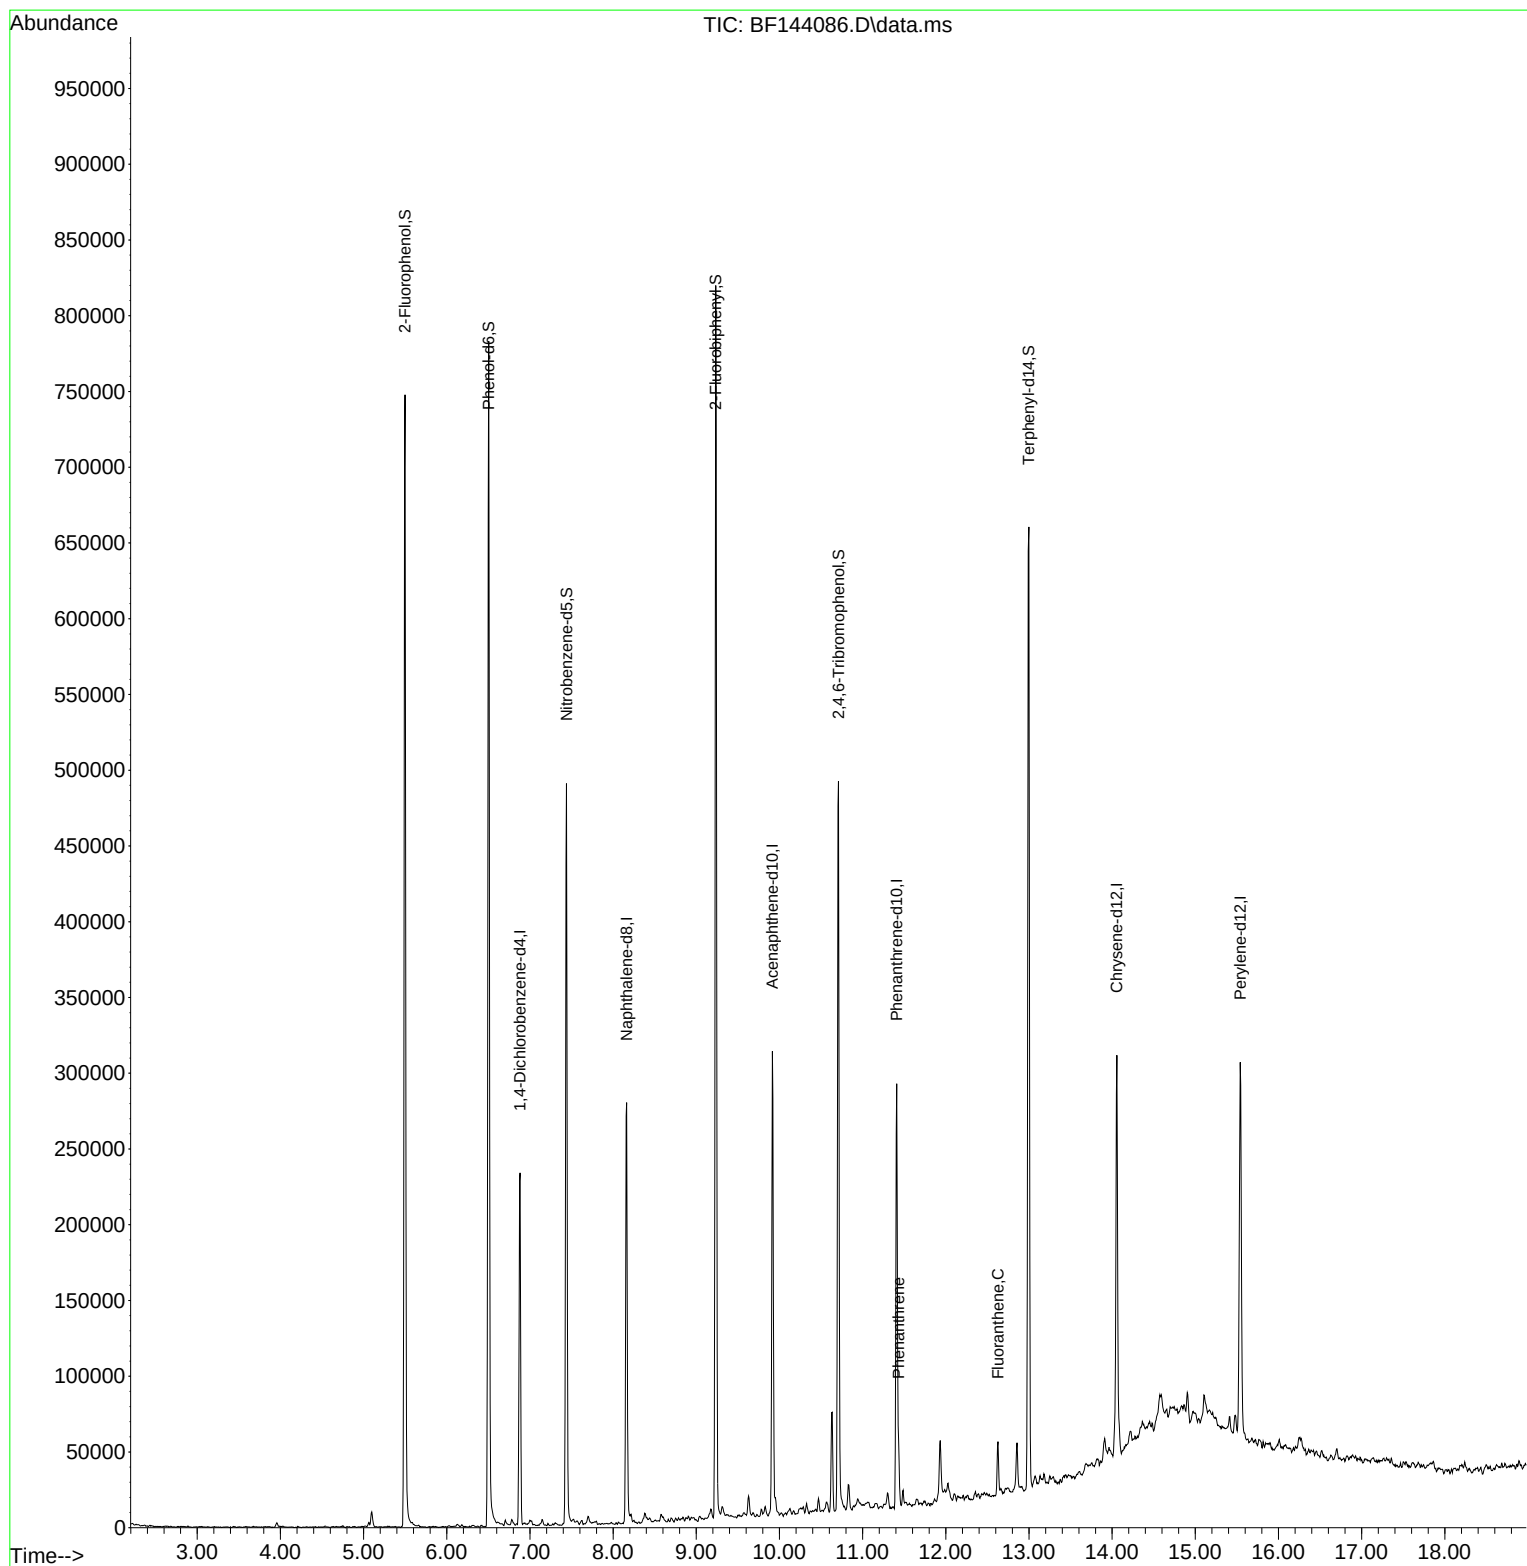


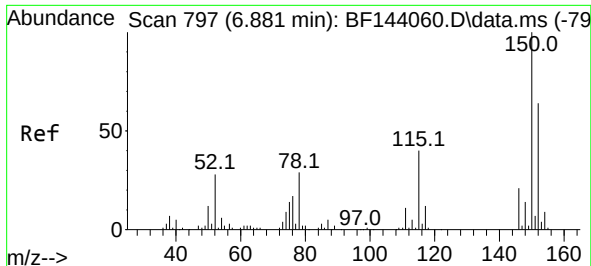

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.881 min Scan# 797
Delta R.T. -0.000 min
Lab File: BF144086.D
Acq: 27 Oct 2025 16:33




Instrument :
BNA_F
ClientSampleId :
PR132-S07-000102-22510170


Tgt Ion:152 Resp: 49197
Ion Ratio Lower Upper
152 100
150 159.3 124.4 186.6
115 59.6 49.4 74.0

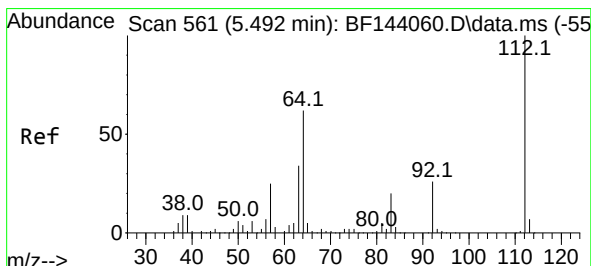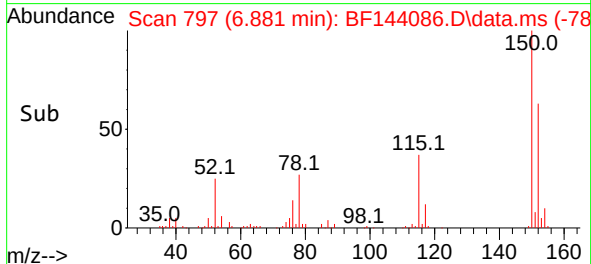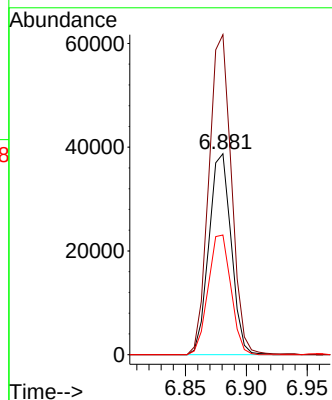

#5
2-Fluorophenol
Concen: 91.364 ng
RT: 5.498 min Scan# 562
Delta R.T. 0.006 min
Lab File: BF144086.D
Acq: 27 Oct 2025 16:33

Tgt Ion:112 Resp: 284104
Ion Ratio Lower Upper
112 100
64 58.6 49.8 74.8
63 31.9 27.4 41.2


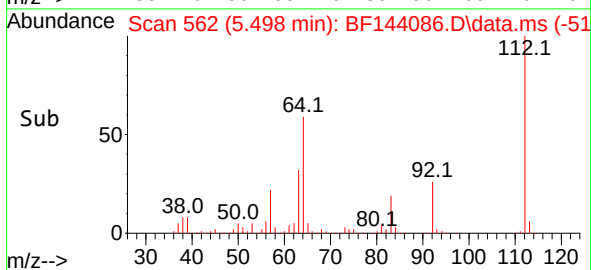
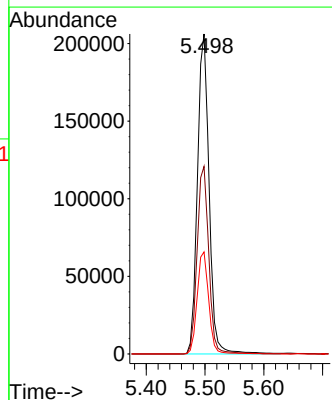
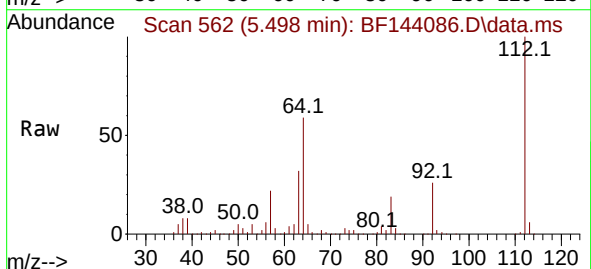


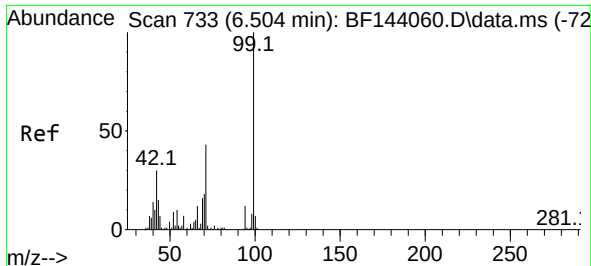

#7
Phenol-d6
Concen: 93.958 ng
RT: 6.504 min Scan# 71
Delta R.T. 0.000 min
Lab File: BF144086.D
Acq: 27 Oct 2025 16:33




Instrument :
BNA_F
ClientSampleId :
PR132-S07-000102-22510170


Tgt Ion: 99 Resp: 322671
Ion Ratio Lower Upper
99 100
42 27.7 23.9 35.9
71 41.2 34.4 51.6

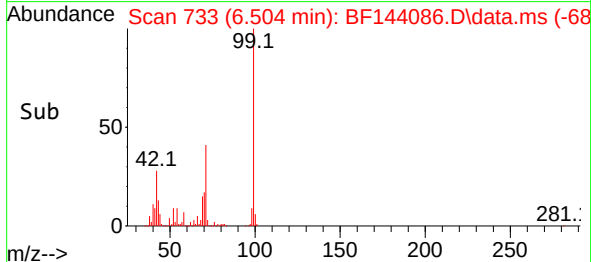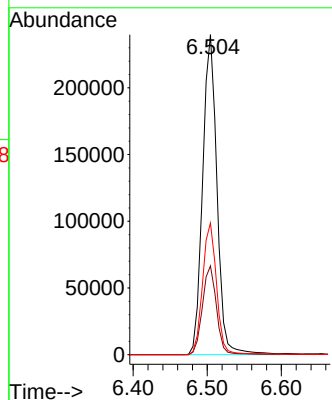

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.163 min Scan# 1015
Delta R.T. 0.000 min
Lab File: BF144086.D
Acq: 27 Oct 2025 16:33

Tgt Ion:136 Resp: 182564
Ion Ratio Lower Upper
136 100
137 10.9 8.6 13.0
54 8.3 6.6 9.8
68 5.0 4.6 6.8

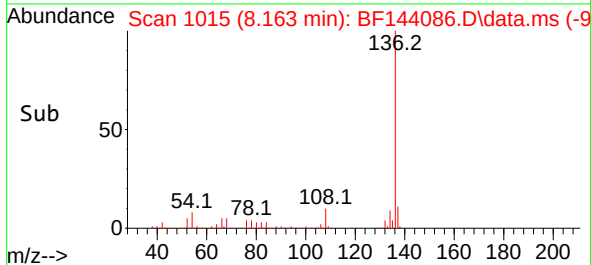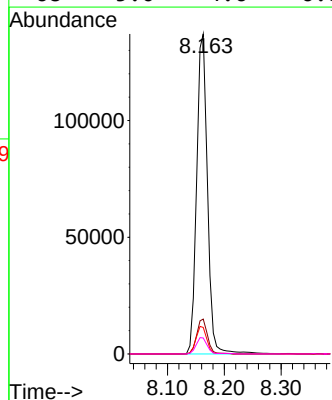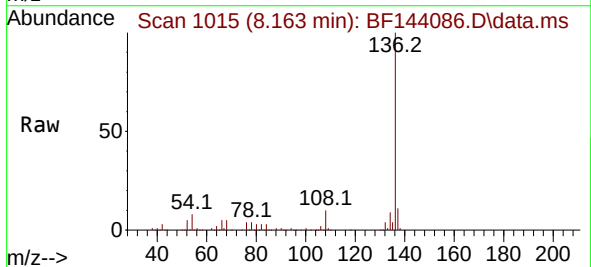

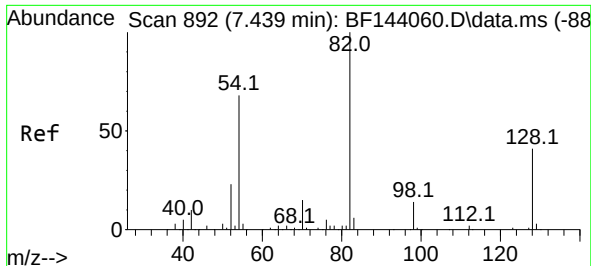

#23

Nitrobenzene-d5

Concen: 61.377 ng

RT: 7.439 min Scan# 892

Delta R.T. 0.000 min

Lab File: BF144086.D

Acq: 27 Oct 2025 16:33

Instrument :





BNA_F

ClientSampleId :

PR132-S07-000102-22510170

Tgt Ion: 82 Resp: 204522

Ion	Ratio	Lower	Upper
82	100		
128	43.5	32.4	48.6
54	63.8	54.0	81.0

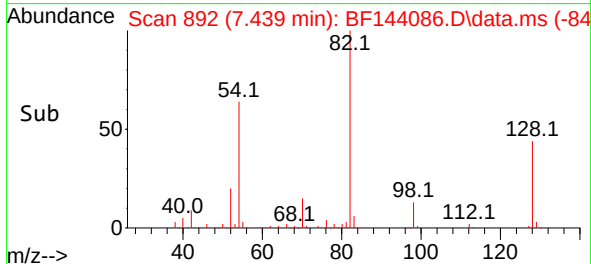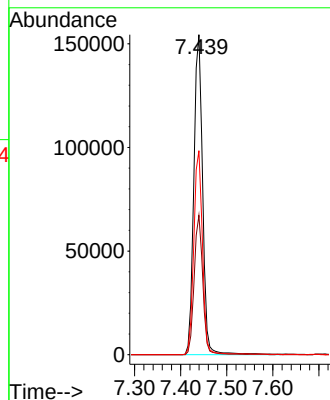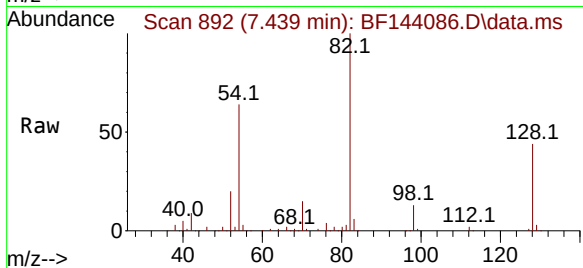

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.916 min Scan# 1313




Delta R.T. 0.000 min


Lab File: BF144086.D

Acq: 27 Oct 2025 16:33

Tgt Ion:164 Resp: 93912

Ion	Ratio	Lower	Upper
164	100		
162	100.1	79.4	119.2
160	45.3	36.7	55.1

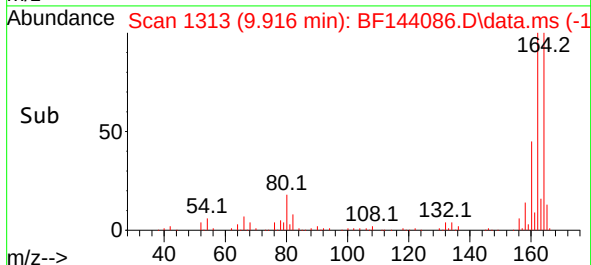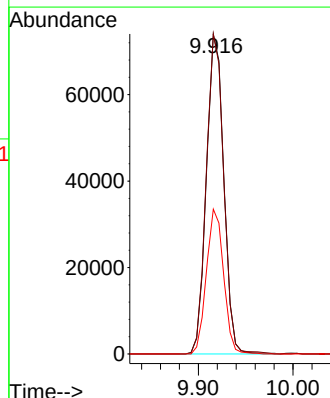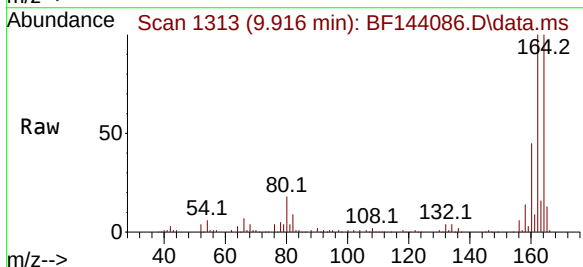

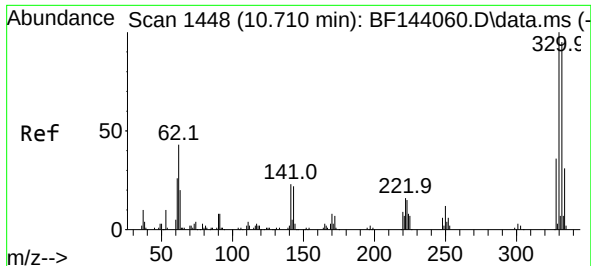

#42

2,4,6-Tribromophenol

Concen: 82.651 ng

RT: 10.710 min Scan# 1448

Delta R.T. 0.000 min

Lab File: BF144086.D


Acq: 27 Oct 2025 16:33

Instrument :

BNA_F

ClientSampleId :

PR132-S07-000102-22510170






Tgt Ion:330 Resp: 98872

Ion Ratio Lower Upper

330 100

332 96.8 77.0 115.6

141 24.6 19.4 29.0

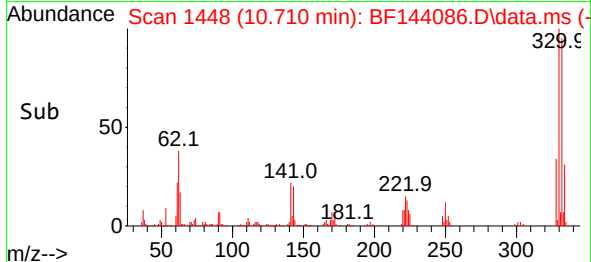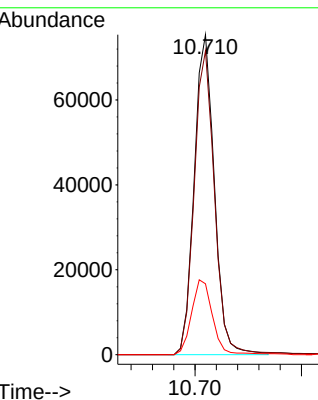

#45

2-Fluorobiphenyl

Concen: 55.677 ng

RT: 9.233 min Scan# 1197

Delta R.T. -0.006 min

Lab File: BF144086.D

Acq: 27 Oct 2025 16:33




Tgt Ion:172 Resp: 371566


Ion Ratio Lower Upper

172 100

171 34.9 27.5 41.3

170 24.2 19.0 28.6

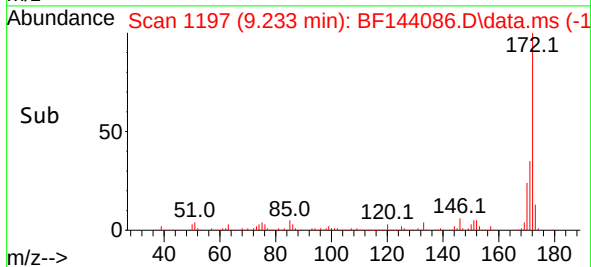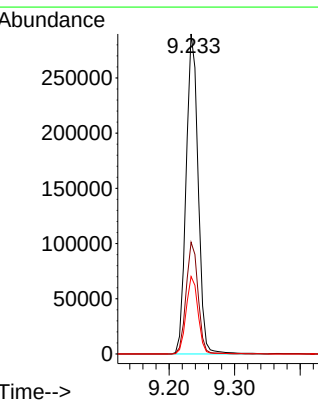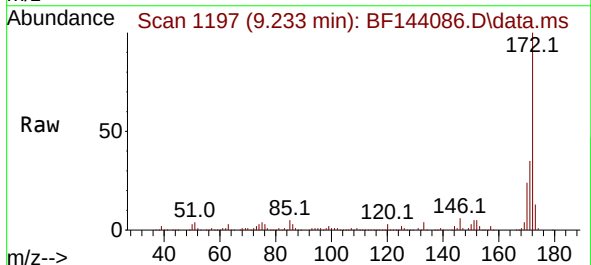



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.410 min Scan# 1567

Delta R.T. 0.000 min

Lab File: BF144086.D

Acq: 27 Oct 2025 16:33

Instrument :

BNA_F

ClientSampleId :

PR132-S07-000102-22510170





Tgt Ion:188 Resp: 147369

Ion Ratio Lower Upper

188 100

94 8.0 5.4 8.0

80 7.8 6.0 9.0

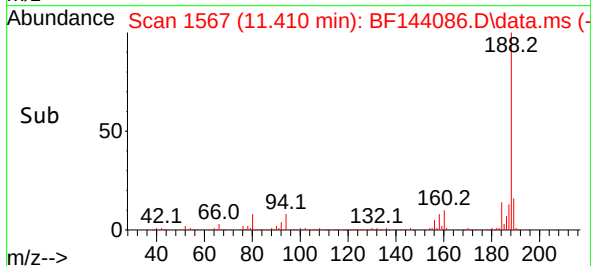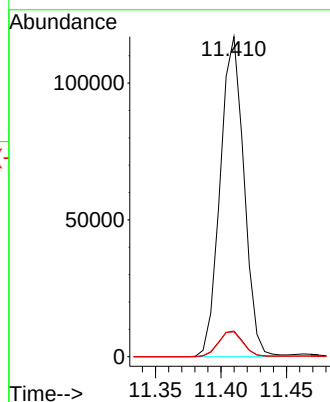

#71

Phenanthrene

Concen: 2.761 ng

RT: 11.433 min Scan# 1571

Delta R.T. 0.000 min

Lab File: BF144086.D

Acq: 27 Oct 2025 16:33




Tgt Ion:178 Resp: 20215


Ion Ratio Lower Upper

178 100

176 22.6 16.3 24.5

179 17.3 12.6 18.8


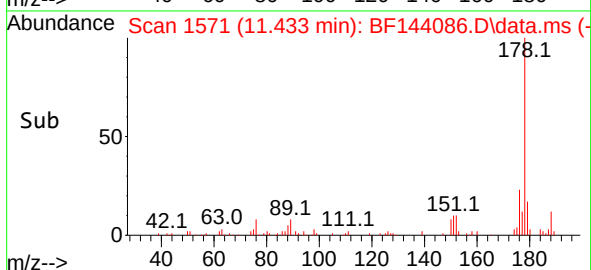
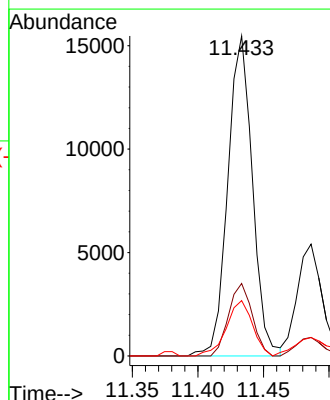
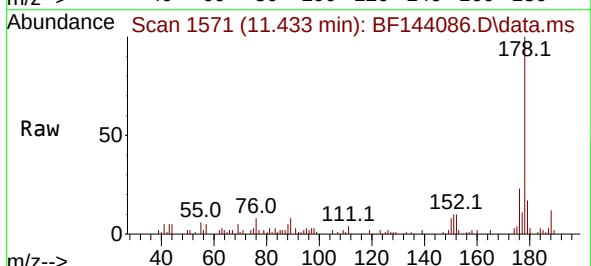


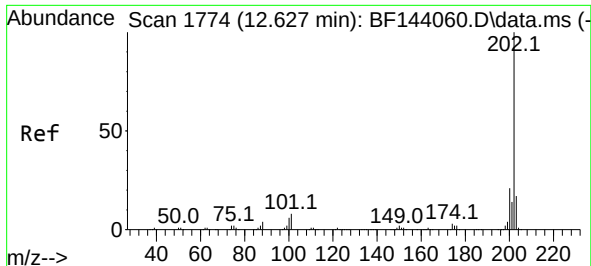

#75
Fluoranthene
Concen: 2.610 ng
RT: 12.627 min Scan# 11
Delta R.T. 0.000 min
Lab File: BF144086.D
Acq: 27 Oct 2025 16:33




Instrument :
BNA_F
ClientSampleId :
PR132-S07-000102-22510170


Tgt Ion:202 Resp: 21112
Ion Ratio Lower Upper
202 100
101 8.5 0.0 27.7
203 17.6 0.0 37.3

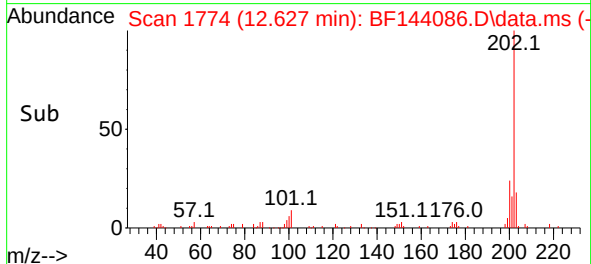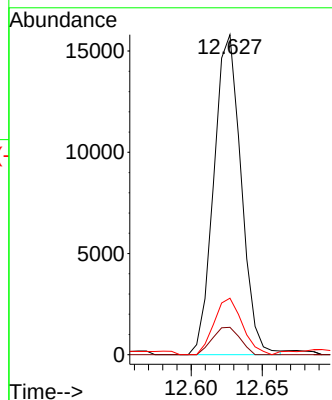

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.057 min Scan# 2017
Delta R.T. 0.000 min
Lab File: BF144086.D
Acq: 27 Oct 2025 16:33


Tgt Ion:240 Resp: 132745
Ion Ratio Lower Upper
240 100
120 8.1 6.5 9.7
236 24.3 20.1 30.1

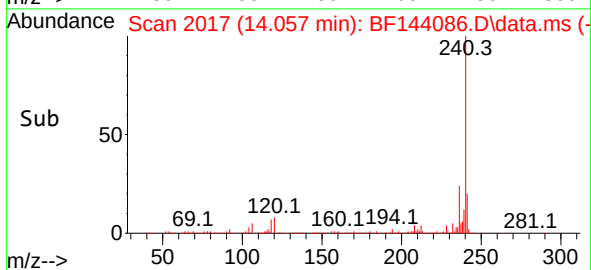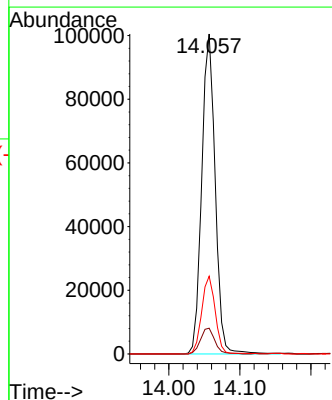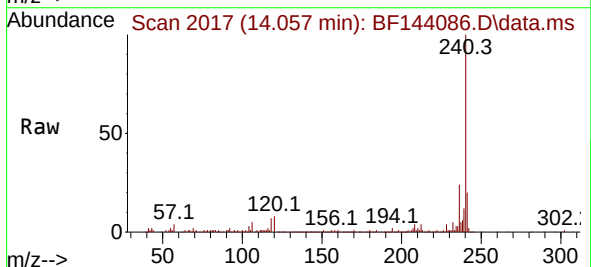



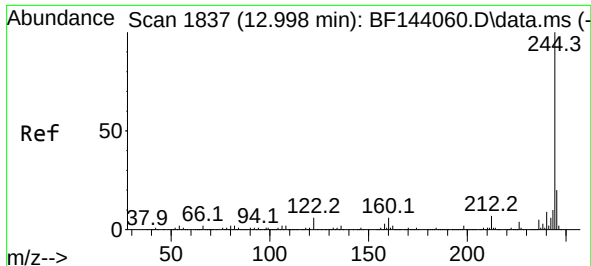


#79
 Terphenyl-d14
 Concen: 44.964 ng
 RT: 12.998 min Scan# 1837
 Delta R.T. 0.000 min
 Lab File: BF144086.D
 Acq: 27 Oct 2025 16:33


Instrument :
 BNA_F
 ClientSampleId :
 PR132-S07-000102-22510170



Tgt Ion:244 Resp: 341415
 Ion Ratio Lower Upper
 244 100
 212 6.3 5.8 8.6
 122 6.3 4.9 7.3

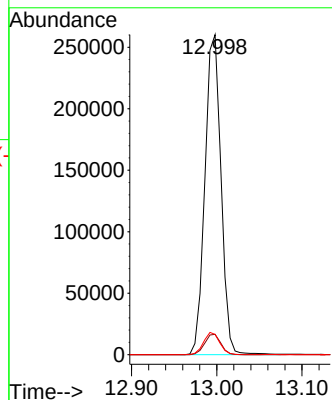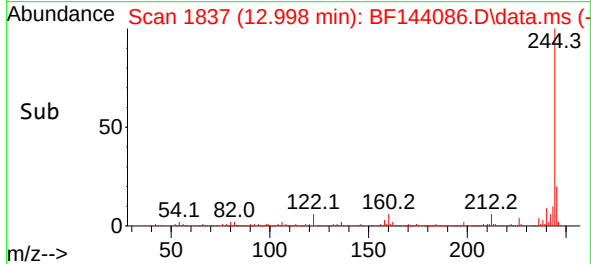

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.539 min Scan# 2269
 Delta R.T. 0.000 min
 Lab File: BF144086.D
 Acq: 27 Oct 2025 16:33

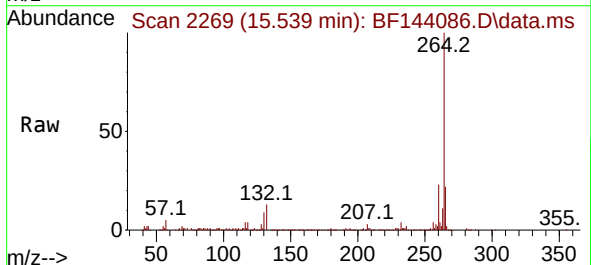

Tgt Ion:264 Resp: 166960
 Ion Ratio Lower Upper
 264 100
 260 23.1 17.0 25.4
 265 22.2 16.6 24.8

