

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102225\
 Data File : FF016597.D
 Signal(s) : FID2B.ch
 Acq On : 22 Oct 2025 15:13
 Operator : YP\AJ
 Sample : Q3399-01MS
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 COMP-ROLLOFFMS

Integration File: autoint1.e
 Quant Time: Oct 22 15:20:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102225.M
 Quant Title :
 QLast Update : Fri Oct 03 03:40:27 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.062	1217883	10.355 ug/ml
Target Compounds			
2) N-DECANE	4.576	1627447	13.537 ug/ml
3) N-DODECANE	6.754	1715883	14.078 ug/ml
4) N-TETRADECANE	8.587	1769814	14.379 ug/ml
5) N-HEXADECANE	10.197	1851051	14.791 ug/ml
6) N-OCTADECANE	11.643	1888261	14.531 ug/ml
7) N-EICOSANE	12.956	1933172	14.498 ug/ml
8) N-DOCOSANE	14.159	1874779	14.303 ug/ml
10) N-TETRACOSANE	15.266	1824860	13.777 ug/ml
11) N-HEXACOSANE	16.291	1787647	13.536 ug/ml
12) N-OCTACOSANE	17.246	1792982	13.652 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102225\
Data File : FF016597.D
Signal(s) : FID2B.ch
Acq On : 22 Oct 2025 15:13
Operator : YP\AJ
Sample : Q3399-01MS
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
COMP-ROLLOFFMS

Integration File: autoint1.e
Quant Time: Oct 22 15:20:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102225.M
Quant Title :
QLast Update : Fri Oct 03 03:40:27 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

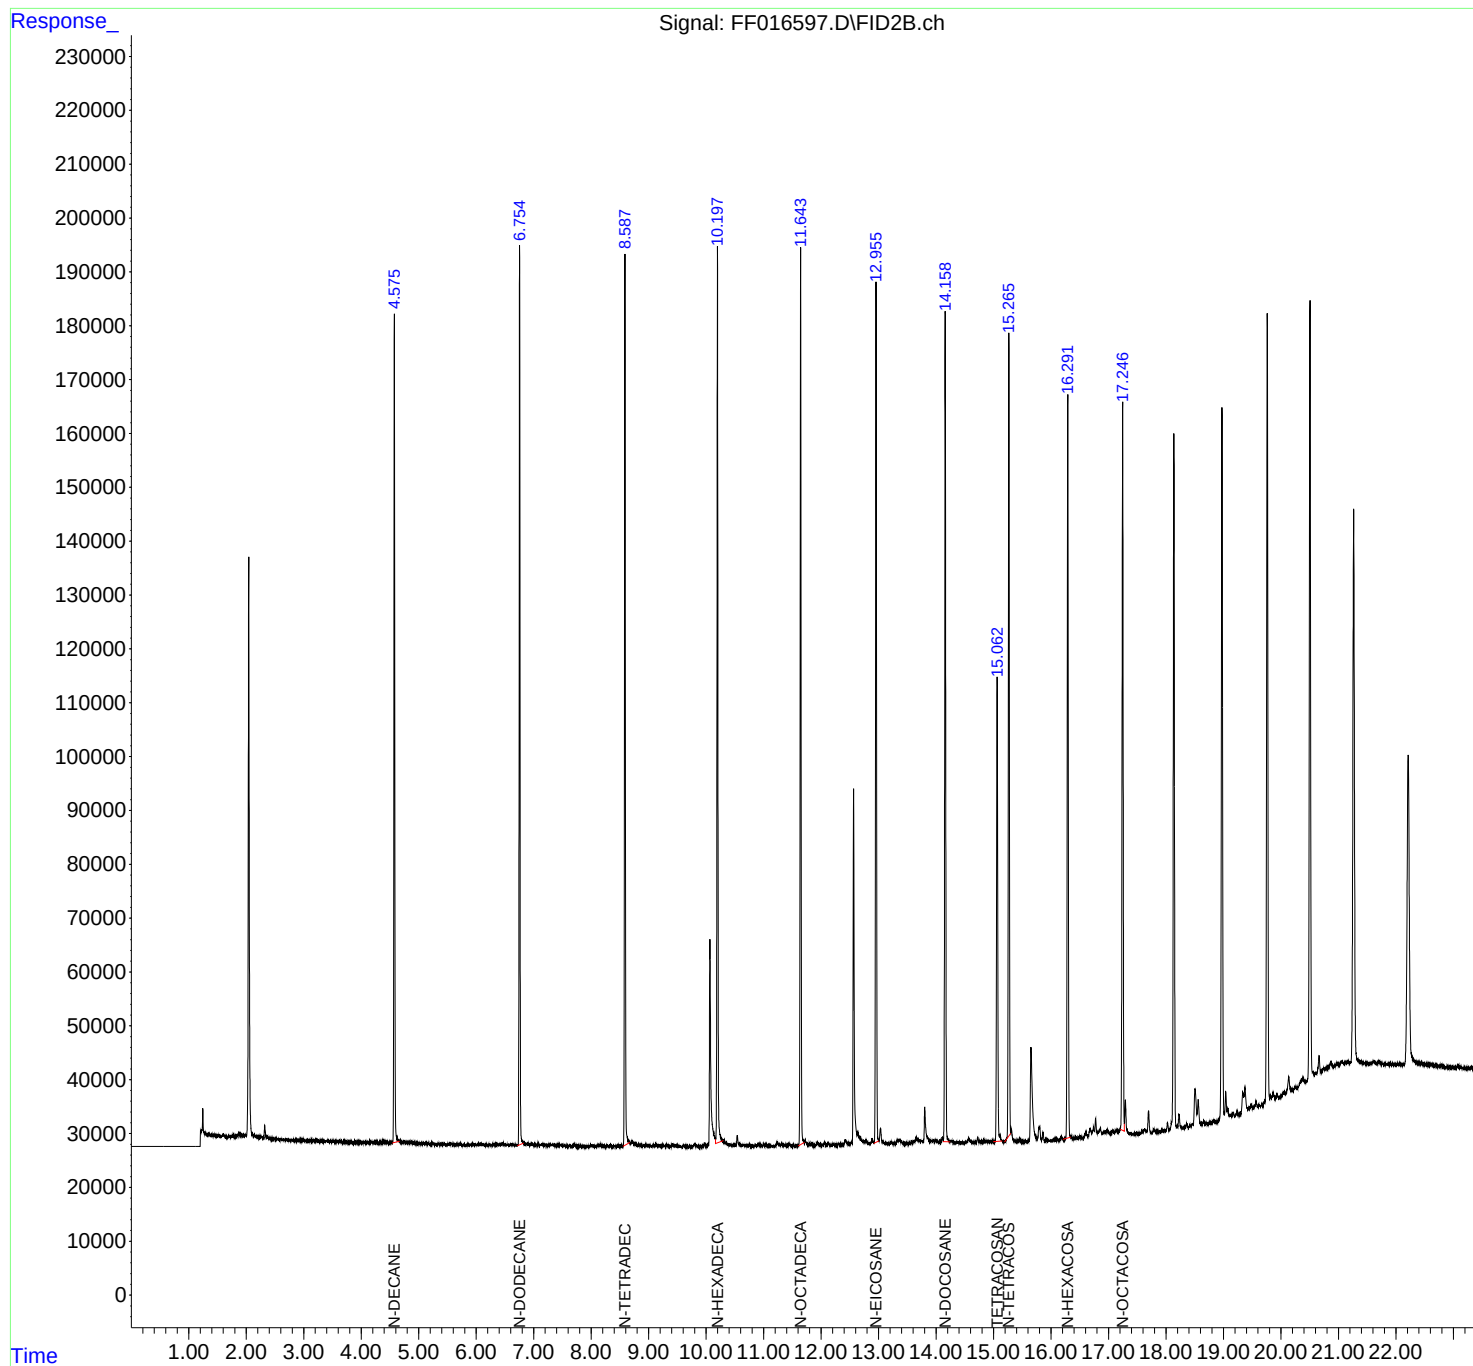


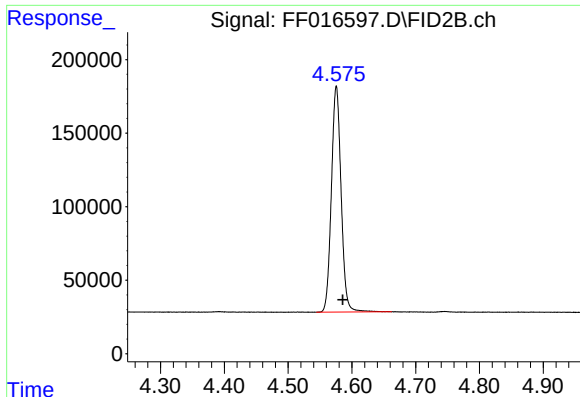

#2 N-DECANE


R.T.: 4.576 min
Delta R.T.: -0.010 min
Response: 1627447
Conc: 13.54 ug/ml

Instrument :
FID_F
ClientSampleId :
COMP-ROLLOFFMS

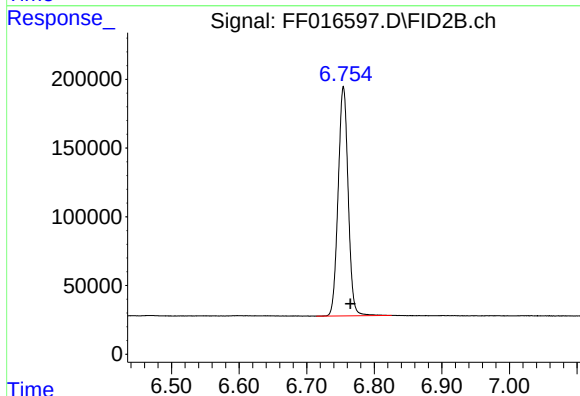


#3 N-DODECANE

R.T.: 6.754 min
Delta R.T.: -0.010 min
Response: 1715883
Conc: 14.08 ug/ml

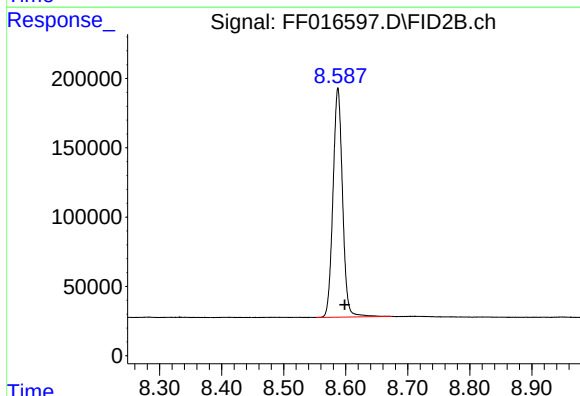


#4 N-TETRADECANE

R.T.: 8.587 min
Delta R.T.: -0.011 min
Response: 1769814
Conc: 14.38 ug/ml

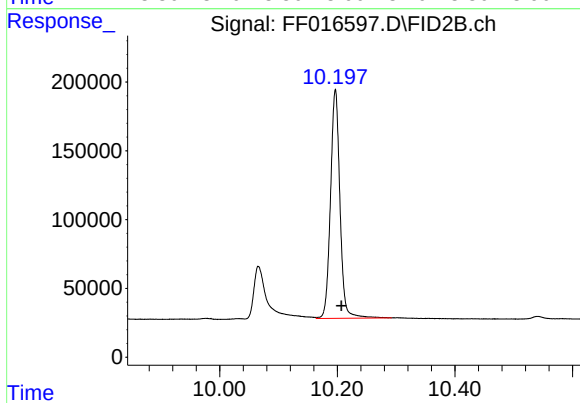

#5 N-HEXADECANE


R.T.: 10.197 min
Delta R.T.: -0.010 min
Response: 1851051
Conc: 14.79 ug/ml

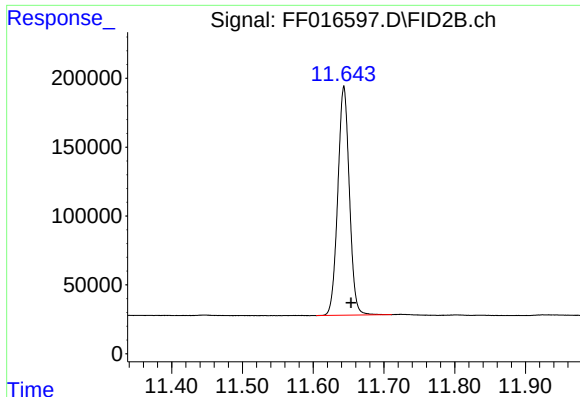

#6 N-OCTADECANE


R.T.: 11.643 min
Delta R.T.: -0.010 min
Response: 1888261
Conc: 14.53 ug/ml

Instrument :
FID_F
ClientSampleId :
COMP-ROLLOFFMS

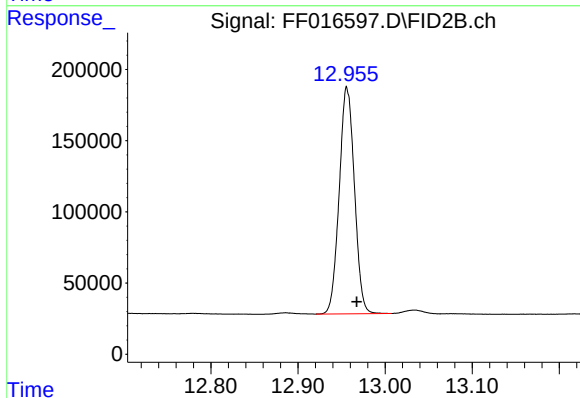


#7 N-EICOSANE

R.T.: 12.956 min
Delta R.T.: -0.011 min
Response: 1933172
Conc: 14.50 ug/ml

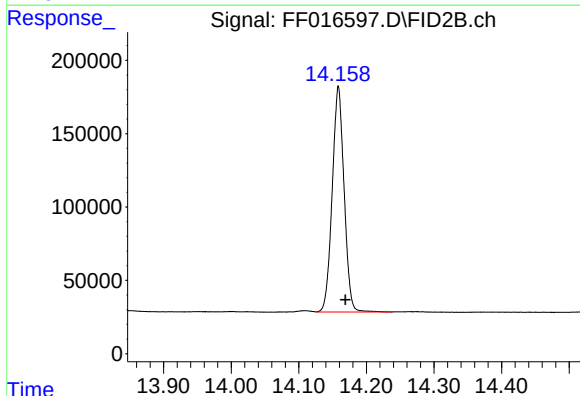


#8 N-DOCOSANE

R.T.: 14.159 min
Delta R.T.: -0.010 min
Response: 1874779
Conc: 14.30 ug/ml

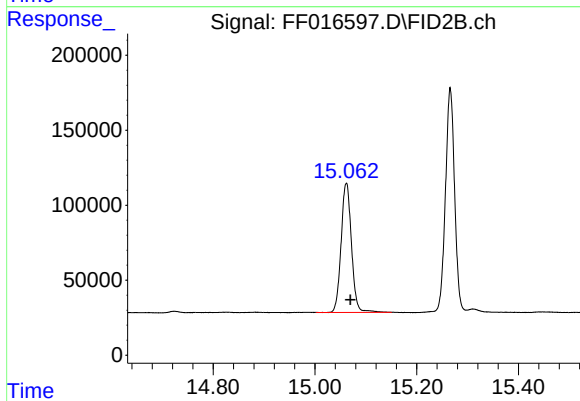

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.062 min
Delta R.T.: -0.008 min
Response: 1217883
Conc: 10.36 ug/ml

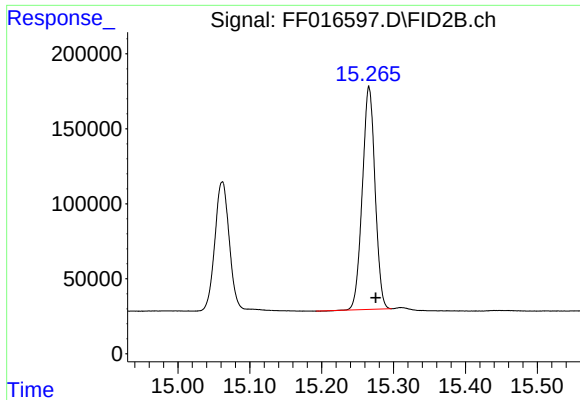

#10 N-TETRACOSANE


R.T.: 15.266 min
Delta R.T.: -0.009 min
Response: 1824860
Conc: 13.78 ug/ml

Instrument :
FID_F
ClientSampleId :
COMP-ROLLOFFMS

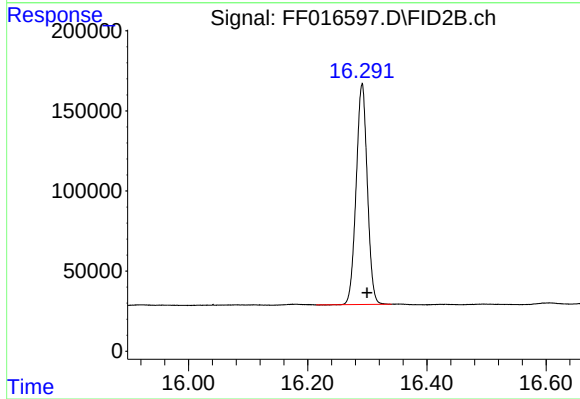

#11 N-HEXACOSANE

R.T.: 16.291 min
Delta R.T.: -0.008 min
Response: 1787647
Conc: 13.54 ug/ml

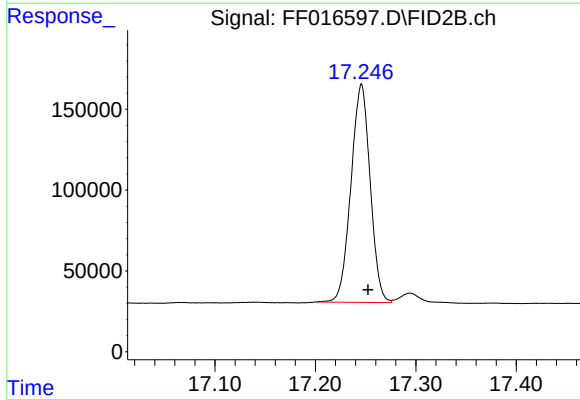

#12 N-OCTACOSANE

R.T.: 17.246 min
Delta R.T.: -0.006 min
Response: 1792982
Conc: 13.65 ug/ml