

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102325\
 Data File : PS032136.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2025 11:44
 Operator : AR\AJ
 Sample : Q3399-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-ROLLOFF

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/24/2025
 Supervised By :mohammad ahmed 10/28/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 17:31:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.278	7.743	1798.7E6	505.0E6	377.310m	458.930m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102325\
Data File : PS032136.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2025 11:44
Operator : AR\AJ
Sample : Q3399-02
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
COMP-ROLLOFF


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/24/2025
Supervised By : mohammad ahmed 10/28/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 17:31:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

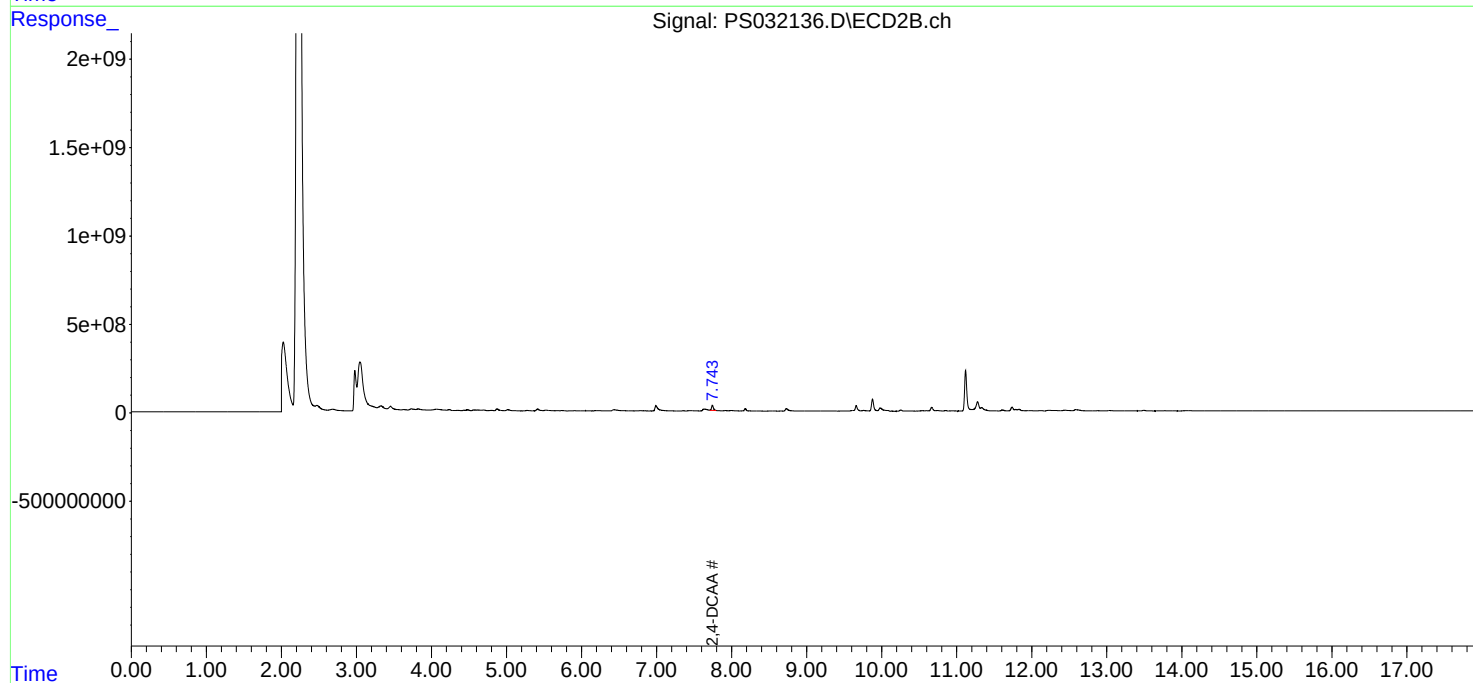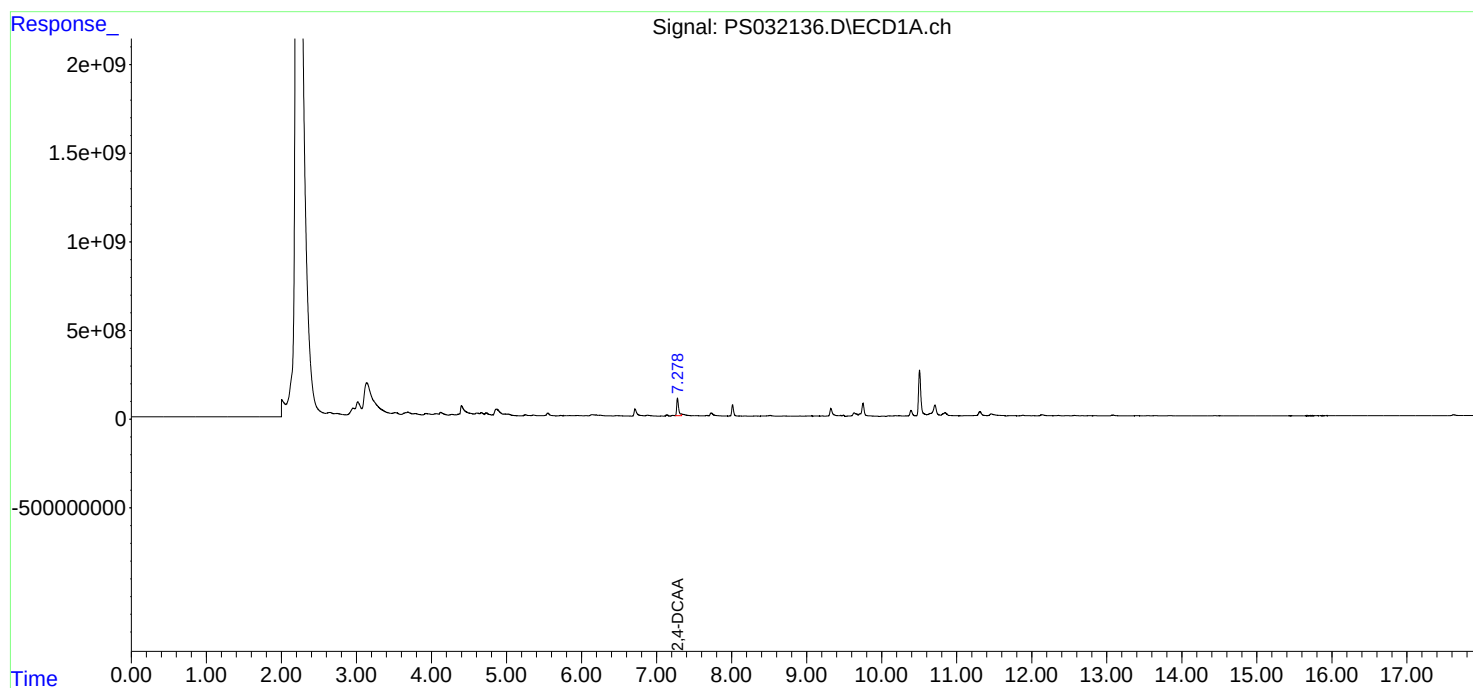

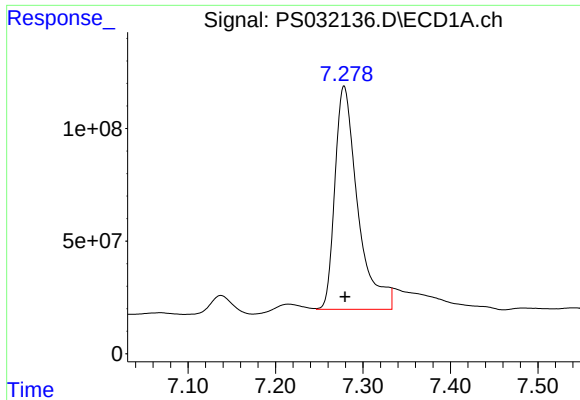


#4 2,4-DCAA

R.T.: 7.278 min
Delta R.T.: -0.002 min
Response: 1798651114
Conc: 377.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-ROLLOFF

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/24/2025
Supervised By :mohammad ahmed 10/28/2025

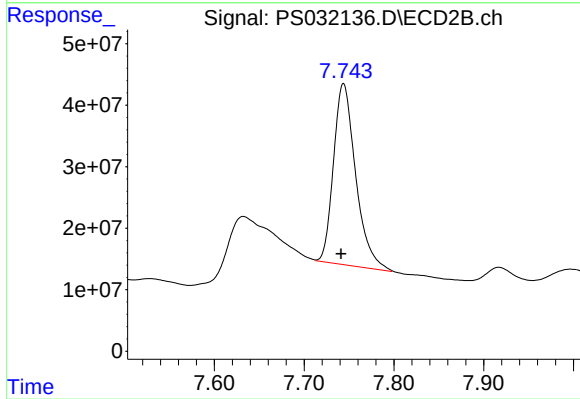

#4 2,4-DCAA

R.T.: 7.743 min
Delta R.T.: 0.002 min
Response: 504979181
Conc: 458.93 ng/ml m