


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110325\
Data File : BG064671.D
Acq On : 3 Nov 2025 13:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Nov 03 18:16:26 2025

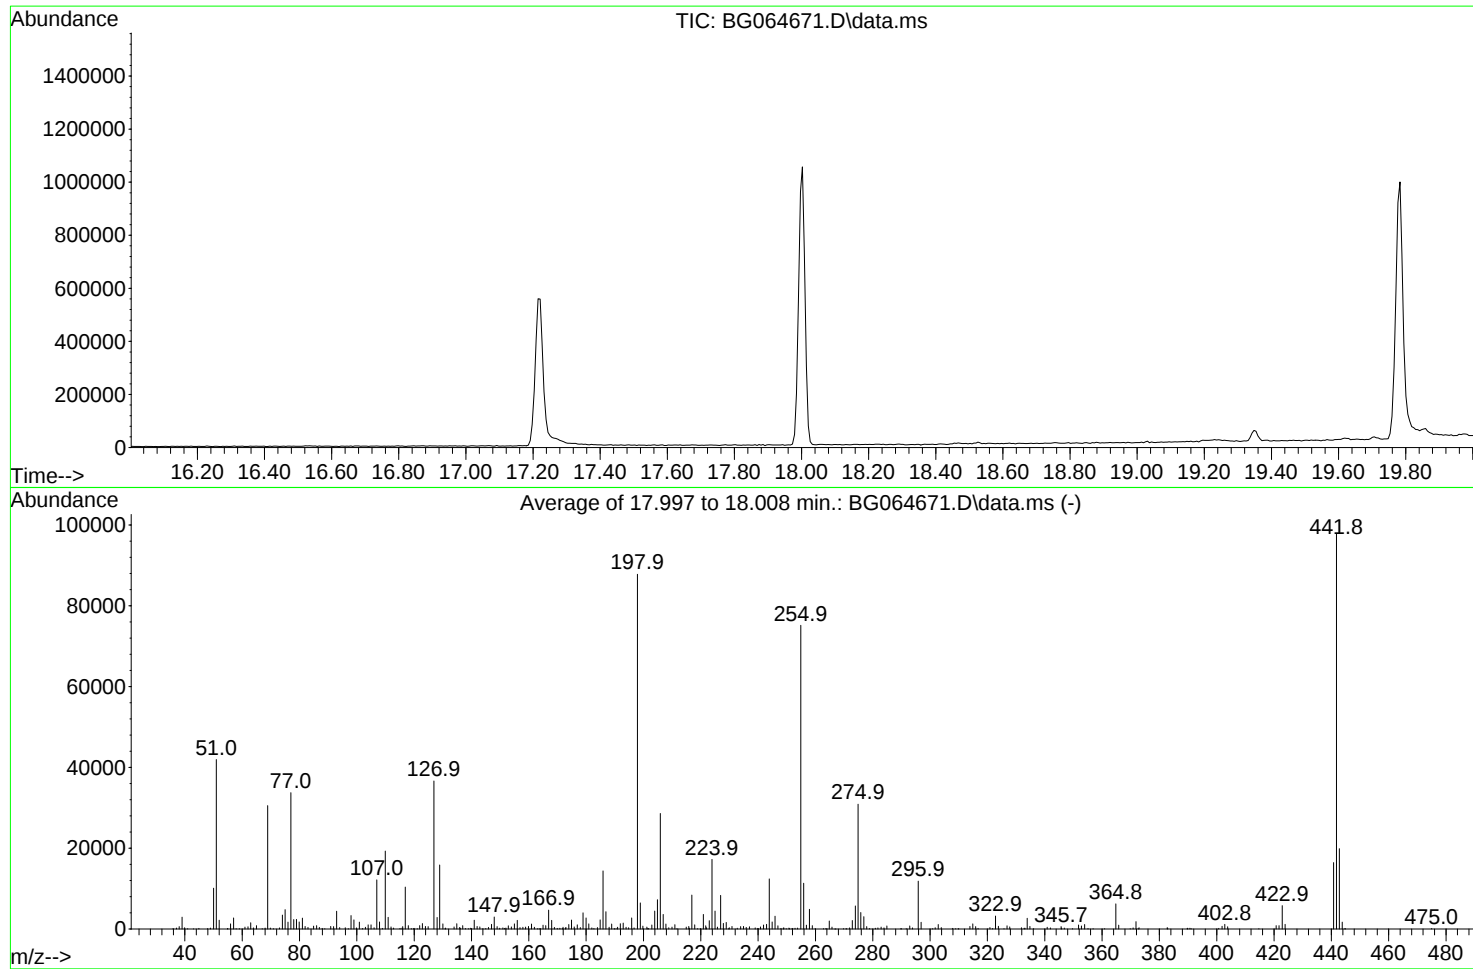




AutoFind: Scans 2537, 2538, 2539; Background Corrected with Scan 2530

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.7	205	PASS
69	69	100	100	100.0	30531	PASS
70	69	0.00	2	0.7	206	PASS
197	198	0.00	2	0.3	270	PASS
198	198	100	100	100.0	87816	PASS
199	198	5	9	7.4	6455	PASS
365	198	1	100	7.1	6206	PASS
441	443	0.01	150	82.8	16441	PASS
442	442	100	100	100.0	97760	PASS
443	442	15	24	20.3	19856	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110325\
Data File : BG064671.D
Acq On : 3 Nov 2025 13:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 04 01:35:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 03 18:16:26 2025
Response via : Initial Calibration

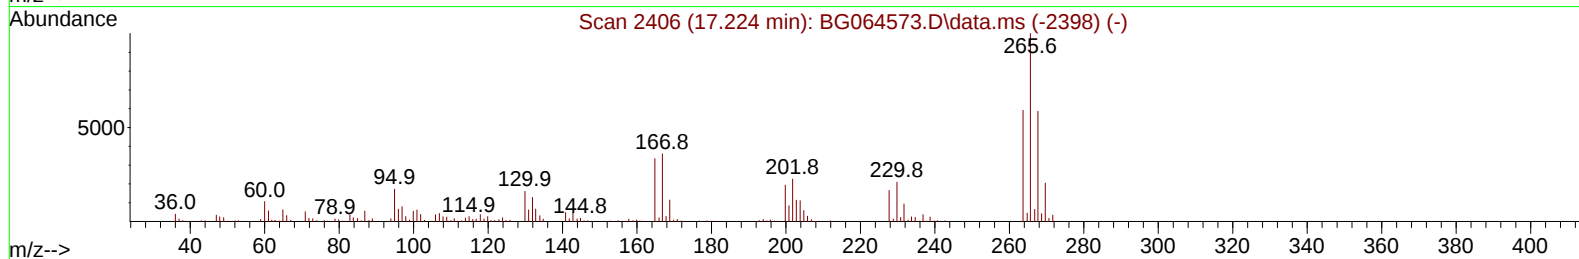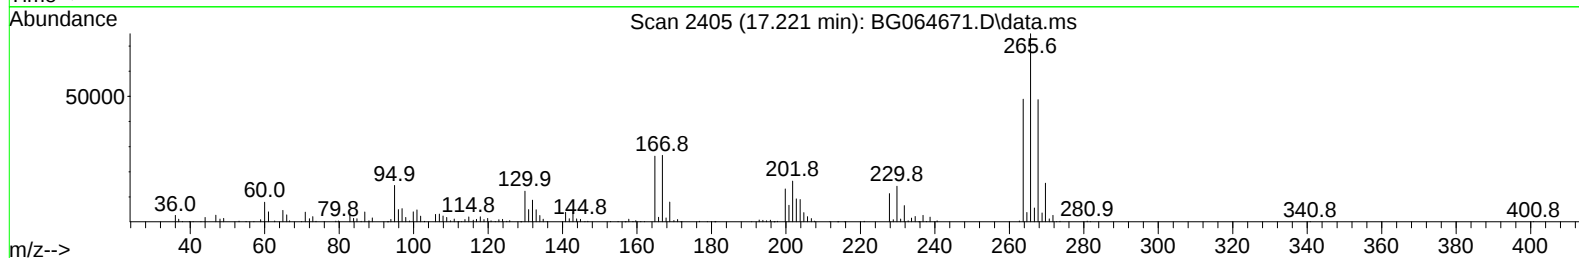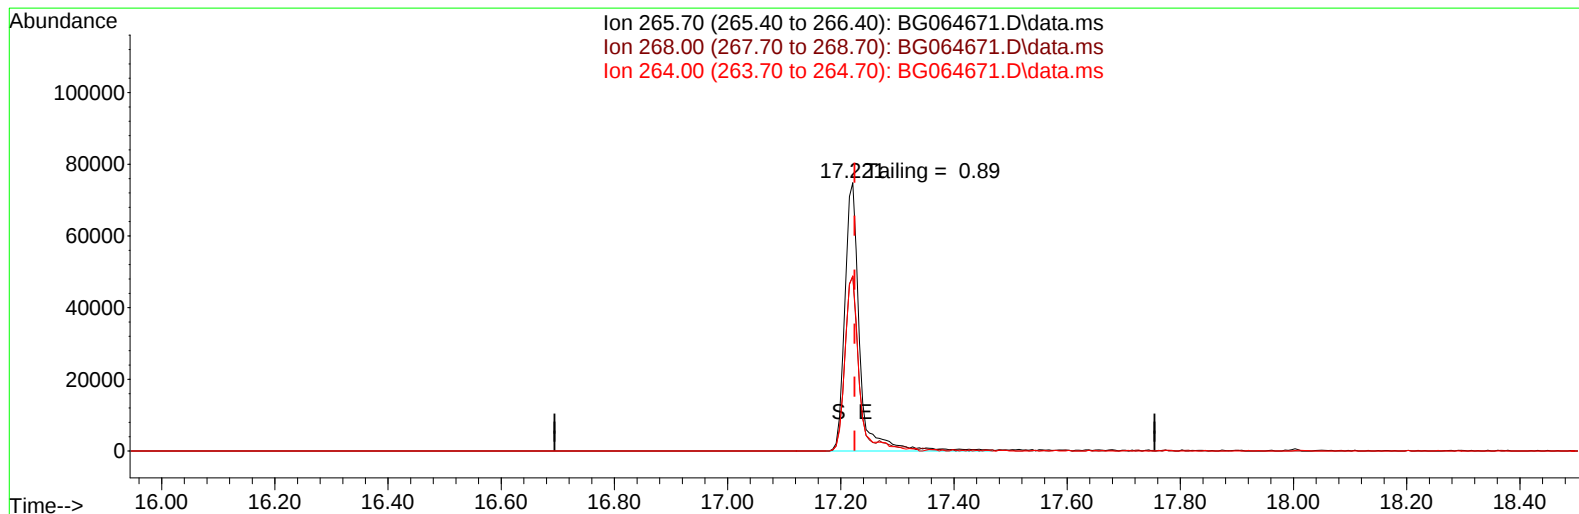

TIC: BG064671.D\data.ms

(70) Pentachlorophenol (C)

17.221min (-0.003) 285068.28 ng




response 132179

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	65.04
264.00	59.10	70.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110325\
Data File : BG064671.D
Acq On : 3 Nov 2025 13:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 04 01:35:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 03 18:16:26 2025
Response via : Initial Calibration

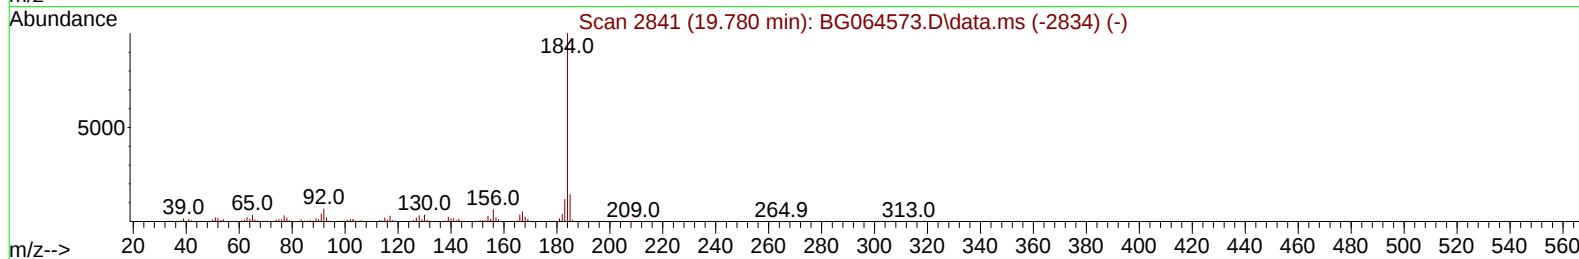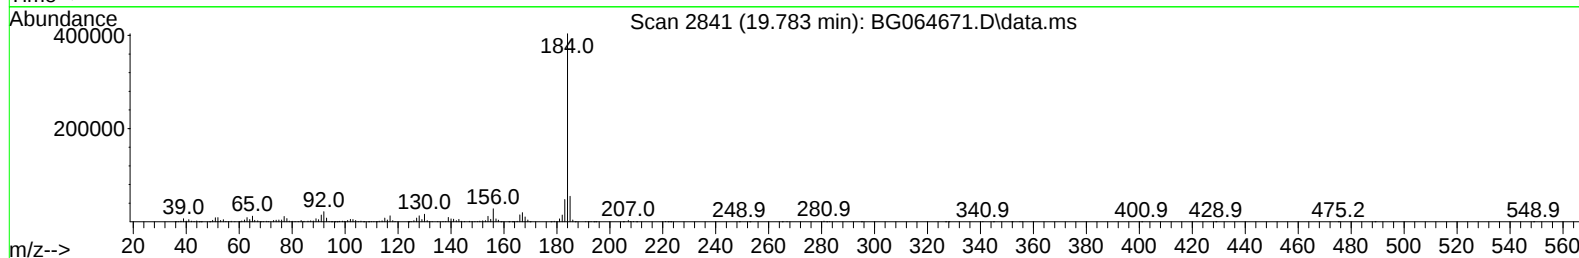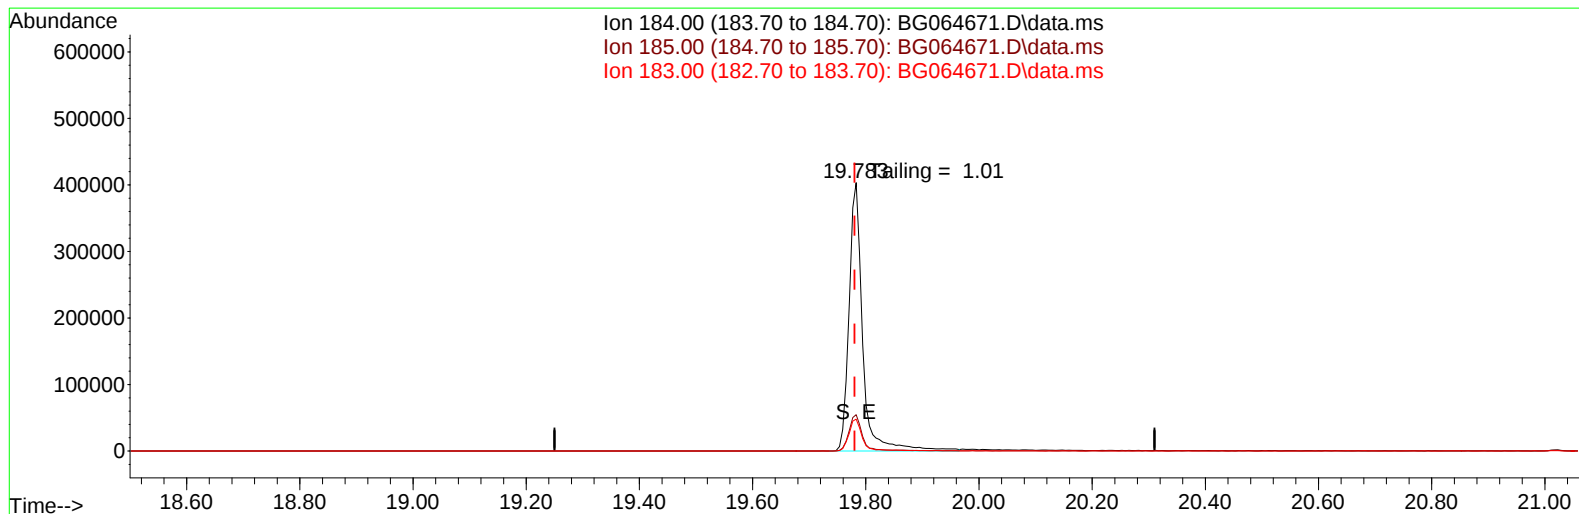

TIC: BG064671.D\data.ms

(77) Benzidine

19.783min (+ 0.003) 139043.84 ng

response 672874

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.55
183.00	11.80	11.90
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/3/2025	BNA_G	<u>BG064671.D</u>
Compound Name	Response	Retention Time
DDT	399376	21.017
DDD	4583	20.57
DDE	760	20.071
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5343	404719	1.32

Instrument :
BNA_G
ClientSampleId :
DFTPP