



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102425\
Data File : VX048338.D
Acq On : 24 Oct 2025 08:19
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102025W.M
Title : SW846 8260
Last Update : Mon Oct 20 14:13:59 2025

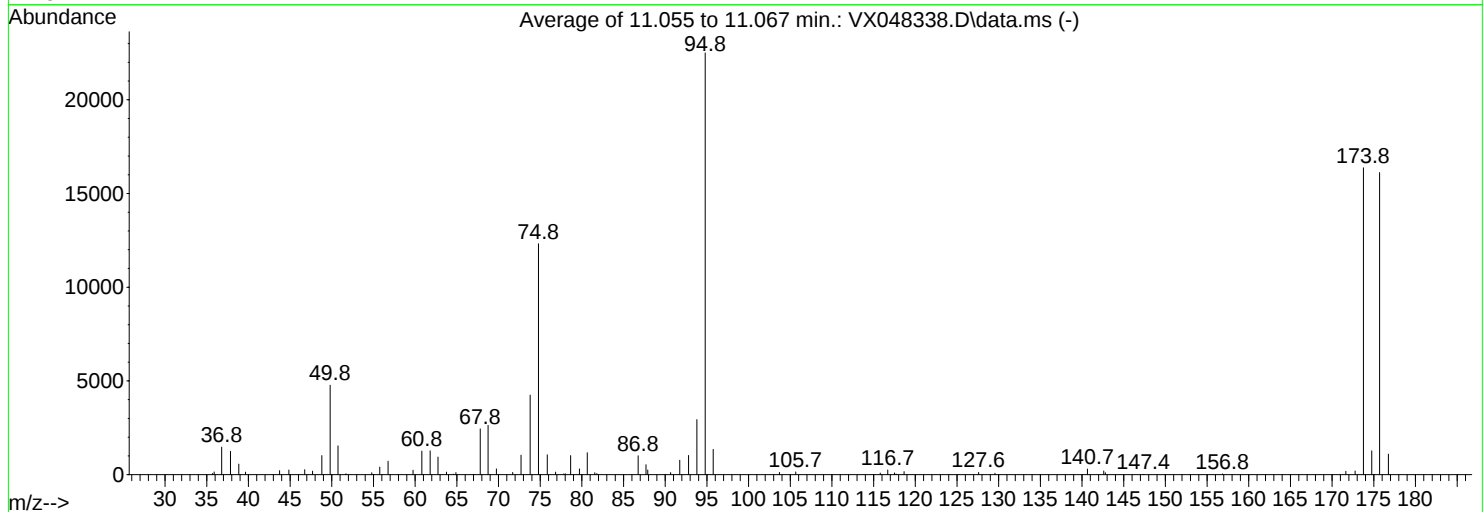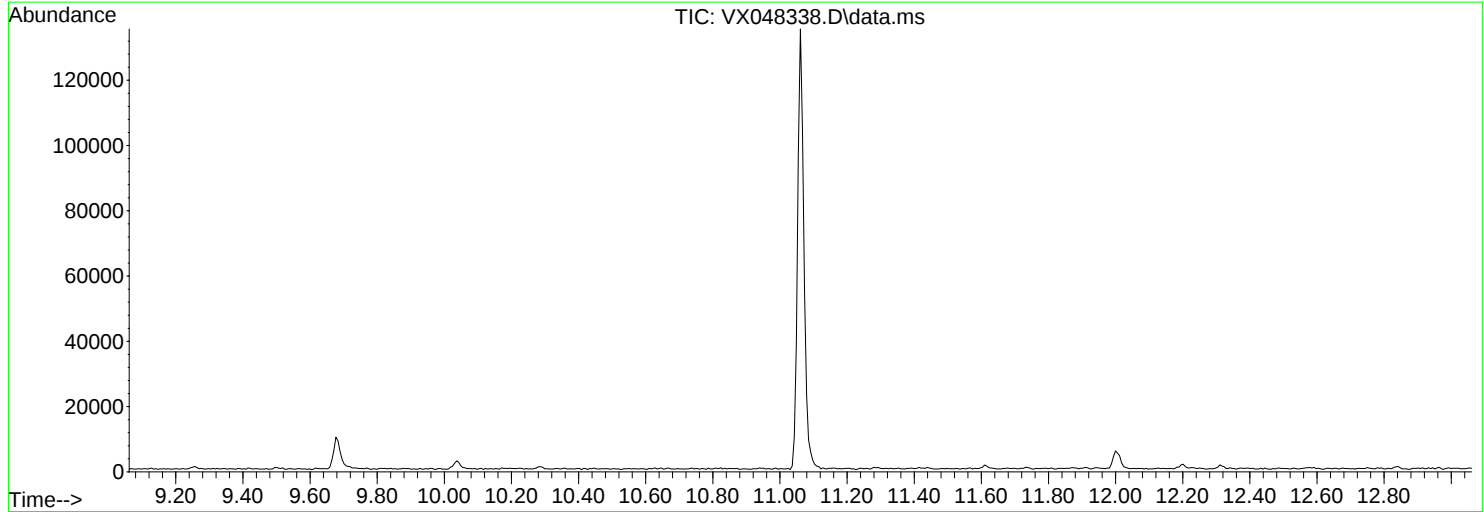

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	4772	PASS
75	95	30	60	54.7	12319	PASS
95	95	100	100	100.0	22504	PASS
96	95	5	9	6.0	1351	PASS
173	174	0.00	2	1.2	197	PASS
174	95	50	100	72.8	16374	PASS
175	174	5	9	7.8	1269	PASS
176	174	95	101	98.4	16118	PASS
177	176	5	9	6.8	1089	PASS