



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102125\
Data File : VX048251.D
Acq On : 21 Oct 2025 08:12
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102025W.M
Title : SW846 8260
Last Update : Mon Oct 20 14:13:59 2025

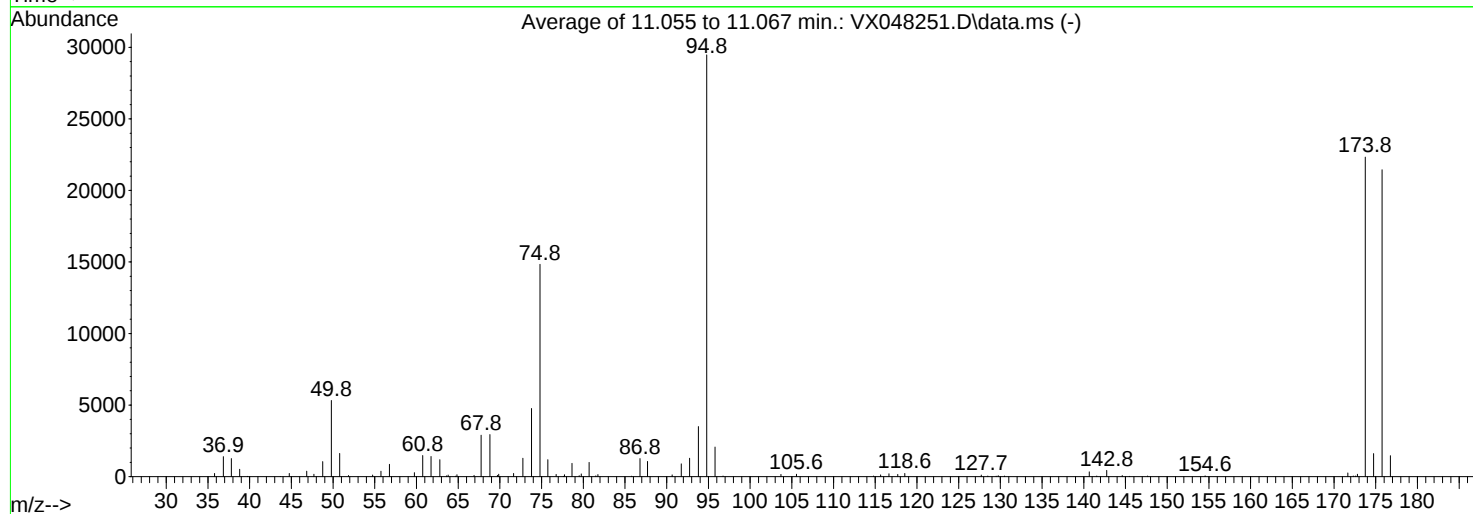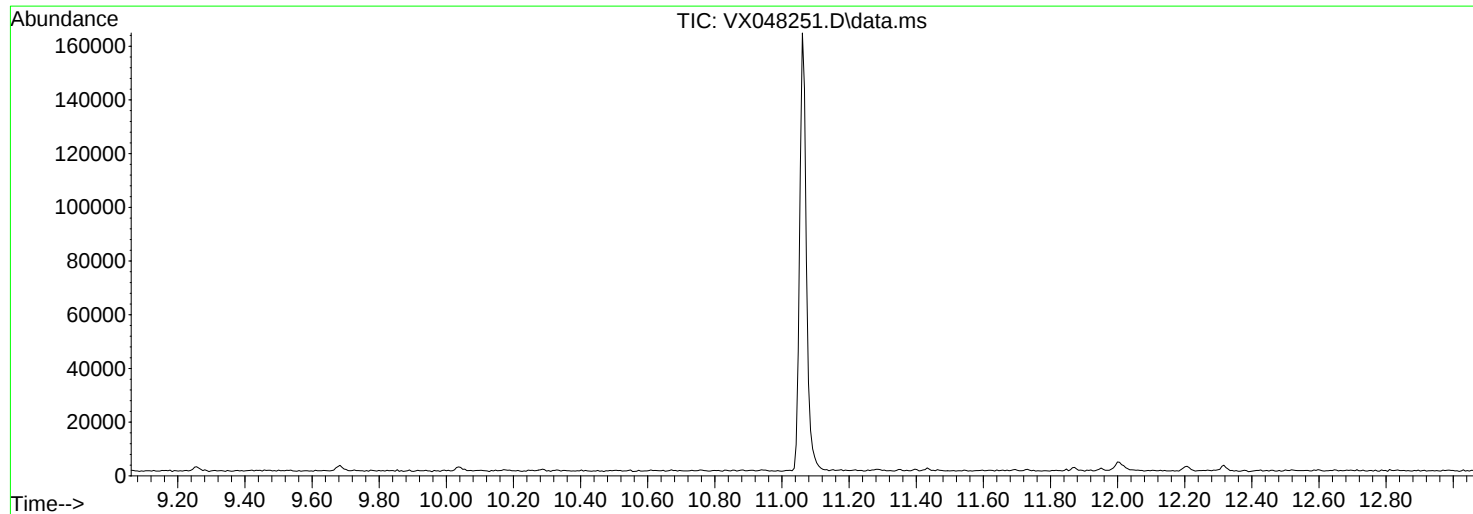

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1629

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.0	5318	PASS
75	95	30	60	50.3	14833	PASS
95	95	100	100	100.0	29475	PASS
96	95	5	9	7.0	2071	PASS
173	174	0.00	2	0.7	166	PASS
174	95	50	100	75.8	22330	PASS
175	174	5	9	7.2	1615	PASS
176	174	95	101	96.1	21451	PASS
177	176	5	9	6.8	1462	PASS