

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following “ Results Qualifiers” are used:

Value	If the result is a value greater than or equal to the detection limit, report the value
U	Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. “10 U”. This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
ND	Indicates the analyte was analyzed for, but not detected
J	Indicates an estimated value. This flag is used: (1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.) (2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
B	Indicates the analyte was found in the blank as well as the sample report as “12 B”.
E	Indicates the analyte ‘s concentration exceeds the calibrated range of the instrument for that specific analysis.
D	This flag identifies all compounds identified in an analysis at a secondary dilution factor.
P	This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a “P”.
N	This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
A	This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
Q	Indicates the LCS did not meet the control limits requirements



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

LAB CHRONICLE

OrderID:	Q3410	OrderDate:	10/20/2025 4:05:00 PM
Client:	Sciacca General Contractors, LLC	Project:	49 Moore Place Belleville
Contact:	Rosanne Scirica	Location:	J11,VOA Lab

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q3410-02	VOC	SOIL	VOC-TCLVOA-10	8260D	10/20/25		10/21/25	10/20/25



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Hit Summary Sheet
SW-846

SDG No.: Q3410

Client: Sciacca General Contractors, LLC

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units
-----------	-----------	--------	-----------	---------------	---	-----	-----	-------

Client ID:

0

Total Voc :

Total Concentration:



QC SUMMARY

Surrogate Summary

SDG No.: Q3410

Client: Sciacca General Contractors, LLC

Analytical Method: SW8260D

Lab Sample ID	Client ID	Parameter	Spike	Result	Recovery (%)	Qual	Limits (%)	
							Low	High
Q3410-02	VOC	1,2-Dichloroethane-d4	50	51.4	103		63	155
		Dibromofluoromethane	50	51.0	102		70	134
		Toluene-d8	50	48.2	96		74	123
		4-Bromofluorobenzene	50	39.1	78		17	146
VY1021SBL01	VY1021SBL01	1,2-Dichloroethane-d4	50	46.0	92		63	155
		Dibromofluoromethane	50	49.7	99		70	134
		Toluene-d8	50	48.1	96		74	123
		4-Bromofluorobenzene	50	36.4	73		17	146
VY1021SBS01	VY1021SBS01	1,2-Dichloroethane-d4	50	46.9	94		63	155
		Dibromofluoromethane	50	50.9	102		70	134
		Toluene-d8	50	51.3	103		74	123
		4-Bromofluorobenzene	50	49.9	100		17	146
VY1021SBSD01	VY1021SBSD01	1,2-Dichloroethane-d4	50	45.6	91		63	155
		Dibromofluoromethane	50	49.6	99		70	134
		Toluene-d8	50	49.7	99		74	123
		4-Bromofluorobenzene	50	47.6	95		17	146

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.:	<u>Q3410</u>	Analytical Method:	<u>SW8260D</u>
Client:	<u>Sciacca General Contractors, LLC</u>	Datafile :	<u>VY023523.D</u>

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Low	Limits High	RPD
VY1021SBS01	Dichlorodifluoromethane	20	20.3	ug/Kg	102			64	136	
	Chloromethane	20	19.5	ug/Kg	98			52	151	
	Vinyl chloride	20	20.2	ug/Kg	101			56	148	
	Bromomethane	20	21.5	ug/Kg	108			58	141	
	Chloroethane	20	21.2	ug/Kg	106			69	130	
	Trichlorofluoromethane	20	20.4	ug/Kg	102			69	134	
	1,1,2-Trichlorotrifluoroethane	20	21.1	ug/Kg	106			81	123	
	1,1-Dichloroethene	20	20.2	ug/Kg	101			79	121	
	Acetone	100	120	ug/Kg	120			40	171	
	Carbon disulfide	20	20.2	ug/Kg	101			59	130	
	Methyl tert-butyl Ether	20	18.0	ug/Kg	90			77	129	
	Methyl Acetate	20	15.9	ug/Kg	79			69	149	
	Methylene Chloride	20	19.0	ug/Kg	95			72	131	
	trans-1,2-Dichloroethene	20	21.0	ug/Kg	105			80	123	
	1,1-Dichloroethane	20	20.5	ug/Kg	103			82	123	
	Cyclohexane	20	18.8	ug/Kg	94			76	122	
	2-Butanone	100	100	ug/Kg	100			69	131	
	Carbon Tetrachloride	20	21.7	ug/Kg	109			76	129	
	cis-1,2-Dichloroethene	20	20.7	ug/Kg	104			82	123	
	Bromochloromethane	20	19.7	ug/Kg	99			80	127	
	Chloroform	20	21.5	ug/Kg	108			82	125	
	1,1,1-Trichloroethane	20	21.1	ug/Kg	106			80	126	
	Methylcyclohexane	20	19.8	ug/Kg	99			77	123	
	Benzene	20	21.6	ug/Kg	108			84	121	
	1,2-Dichloroethane	20	20.0	ug/Kg	100			81	126	
	Trichloroethene	20	21.9	ug/Kg	110			83	122	
	1,2-Dichloropropane	20	21.5	ug/Kg	108			83	122	
	Bromodichloromethane	20	21.3	ug/Kg	106			82	123	
	4-Methyl-2-Pentanone	100	86.7	ug/Kg	87			70	135	
	Toluene	20	21.9	ug/Kg	110			83	122	
	t-1,3-Dichloropropene	20	19.9	ug/Kg	100			78	124	
	cis-1,3-Dichloropropene	20	20.8	ug/Kg	104			81	122	
	1,1,2-Trichloroethane	20	21.0	ug/Kg	105			82	125	
	2-Hexanone	100	95.9	ug/Kg	96			66	138	
	Dibromochloromethane	20	20.8	ug/Kg	104			79	125	
	1,2-Dibromoethane	20	20.1	ug/Kg	101			80	125	
	Tetrachloroethene	20	22.0	ug/Kg	110			83	125	
	Chlorobenzene	20	21.2	ug/Kg	106			84	122	
	Ethyl Benzene	20	21.0	ug/Kg	105			82	124	
	m/p-Xylenes	40	43.1	ug/Kg	108			83	124	
	o-Xylene	20	20.6	ug/Kg	103			83	123	
	Styrene	20	21.0	ug/Kg	105			82	124	
	Bromoform	20	19.5	ug/Kg	98			75	127	
	Isopropylbenzene	20	20.3	ug/Kg	102			82	124	
	1,1,2,2-Tetrachloroethane	20	18.2	ug/Kg	91			77	127	
	1,3-Dichlorobenzene	20	20.7	ug/Kg	104			83	122	
	1,4-Dichlorobenzene	20	20.5	ug/Kg	103			84	121	
	1,2-Dichlorobenzene	20	20.5	ug/Kg	103			83	124	

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: Q3410

Analytical Method: SW8260D

Client: Sciacca General Contractors, LLC

Datafile : VY023523.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Low	Limits	RPD
									High	
VY1021SBS01	1,2-Dibromo-3-Chloropropane	20	17.0	ug/Kg	85			66	134	
	1,2,4-Trichlorobenzene	20	18.0	ug/Kg	90			78	127	
	1,2,3-Trichlorobenzene	20	18.1	ug/Kg	91			70	137	

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.:	<u>Q3410</u>	Analytical Method:	<u>SW8260D</u>
Client:	<u>Sciaccia General Contractors, LLC</u>	Datafile :	<u>VY023524.D</u>

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Low	Limits High	RPD
VY1021SBSD01	Dichlorodifluoromethane	20	20.9	ug/Kg	104	2		64	136	20
	Chloromethane	20	19.3	ug/Kg	97	1		52	151	20
	Vinyl chloride	20	20.0	ug/Kg	100	1		56	148	20
	Bromomethane	20	20.7	ug/Kg	104	4		58	141	20
	Chloroethane	20	21.4	ug/Kg	107	1		69	130	20
	Trichlorofluoromethane	20	20.6	ug/Kg	103	1		69	134	20
	1,1,2-Trichlorotrifluoroethane	20	20.7	ug/Kg	104	2		81	123	20
	1,1-Dichloroethene	20	20.6	ug/Kg	103	2		79	121	20
	Acetone	100	120	ug/Kg	120	0		40	171	20
	Carbon disulfide	20	19.7	ug/Kg	99	2		59	130	20
	Methyl tert-butyl Ether	20	18.2	ug/Kg	91	1		77	129	20
	Methyl Acetate	20	15.6	ug/Kg	78	1		69	149	20
	Methylene Chloride	20	18.9	ug/Kg	95	0		72	131	20
	trans-1,2-Dichloroethene	20	20.6	ug/Kg	103	2		80	123	20
	1,1-Dichloroethane	20	20.6	ug/Kg	103	0		82	123	20
	Cyclohexane	20	18.6	ug/Kg	93	1		76	122	20
	2-Butanone	100	100	ug/Kg	100	0		69	131	20
	Carbon Tetrachloride	20	21.0	ug/Kg	105	4		76	129	20
	cis-1,2-Dichloroethene	20	20.5	ug/Kg	103	1		82	123	20
	Bromochloromethane	20	19.6	ug/Kg	98	1		80	127	20
	Chloroform	20	21.0	ug/Kg	105	3		82	125	20
	1,1,1-Trichloroethane	20	20.8	ug/Kg	104	2		80	126	20
	Methylcyclohexane	20	19.5	ug/Kg	98	1		77	123	20
	Benzene	20	21.6	ug/Kg	108	0		84	121	20
	1,2-Dichloroethane	20	20.0	ug/Kg	100	0		81	126	20
	Trichloroethene	20	21.2	ug/Kg	106	4		83	122	20
	1,2-Dichloropropane	20	20.7	ug/Kg	104	4		83	122	20
	Bromodichloromethane	20	21.2	ug/Kg	106	0		82	123	20
	4-Methyl-2-Pentanone	100	86.8	ug/Kg	87	0		70	135	20
	Toluene	20	21.4	ug/Kg	107	3		83	122	20
	t-1,3-Dichloropropene	20	19.5	ug/Kg	98	2		78	124	20
	cis-1,3-Dichloropropene	20	20.2	ug/Kg	101	3		81	122	20
	1,1,2-Trichloroethane	20	20.2	ug/Kg	101	4		82	125	20
	2-Hexanone	100	96.5	ug/Kg	97	1		66	138	20
	Dibromochloromethane	20	20.5	ug/Kg	103	1		79	125	20
	1,2-Dibromoethane	20	20.2	ug/Kg	101	0		80	125	20
	Tetrachloroethene	20	22.1	ug/Kg	111	1		83	125	20
	Chlorobenzene	20	21.2	ug/Kg	106	0		84	122	20
	Ethyl Benzene	20	20.8	ug/Kg	104	1		82	124	20
	m/p-Xylenes	40	42.7	ug/Kg	107	1		83	124	20
	o-Xylene	20	20.7	ug/Kg	104	1		83	123	20
	Styrene	20	20.5	ug/Kg	103	2		82	124	20
	Bromoform	20	19.6	ug/Kg	98	0		75	127	20
	Isopropylbenzene	20	20.3	ug/Kg	102	0		82	124	20
	1,1,2,2-Tetrachloroethane	20	18.8	ug/Kg	94	3		77	127	20
	1,3-Dichlorobenzene	20	20.8	ug/Kg	104	0		83	122	20
	1,4-Dichlorobenzene	20	20.6	ug/Kg	103	0		84	121	20
	1,2-Dichlorobenzene	20	20.5	ug/Kg	103	0		83	124	20

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.:	<u>Q3410</u>	Analytical Method:	<u>SW8260D</u>
Client:	<u>Sciacca General Contractors, LLC</u>	Datafile :	<u>VY023524.D</u>

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Low	Limits High	RPD
VY1021SBSD01	1,2-Dibromo-3-Chloropropane	20	17.3	ug/Kg	86	1		66	134	20
	1,2,4-Trichlorobenzene	20	19.1	ug/Kg	96	6		78	127	20
	1,2,3-Trichlorobenzene	20	18.8	ug/Kg	94	3		70	137	20

VOLATILE METHOD BLANK SUMMARY

Client ID

VY1021SBL01

Lab Name: Alliance

Contract: SCIA01

Lab Code: ACE

SDG NO.: Q3410

Lab File ID: VY023522.D

Lab Sample ID: VY1021SBL01

Date Analyzed: 10/21/2025

Time Analyzed: 09:34

GC Column: RXI-624 ID: 0.25 (mm)

Heated Purge: (Y/N) Y

Instrument ID: MSVOA_Y

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
VY1021SBS01	VY1021SBS01	VY023523.D	10/21/2025
VY1021SBSD01	VY1021SBSD01	VY023524.D	10/21/2025
VOC	Q3410-02	VY023535.D	10/21/2025

COMMENTS: _____



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
BROMOFLUOROBENZENE (BFB)

Lab Name: Alliance

Contract: SCIA01

Lab Code: ACE

SDG NO.: Q3410

Lab File ID: VY023383.D

BFB Injection Date: 10/07/2025

Instrument ID: MSVOA_Y

BFB Injection Time: 08:43

GC Column: RXI-624 ID: 0.25 (mm)

Heated Purge: Y/N Y

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
50	15.0 - 40.0% of mass 95	16.9
75	30.0 - 60.0% of mass 95	48.1
95	Base Peak, 100% relative abundance	100
96	5.0 - 9.0% of mass 95	6.6
173	Less than 2.0% of mass 174	0.9 (0.9) 1
174	50.0 - 100.0% of mass 95	99.1
175	5.0 - 9.0% of mass 174	7.3 (7.4) 1
176	95.0 - 101.0% of mass 174	95.4 (96.2) 1
177	5.0 - 9.0% of mass 176	6.3 (6.6) 2

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

CLIENT ID	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
VSTDIC005	VSTDIC005	VY023384.D	10/07/2025	09:17
VSTDIC010	VSTDIC010	VY023385.D	10/07/2025	10:02
VSTDIC020	VSTDIC020	VY023386.D	10/07/2025	11:24
VSTDIC050	VSTDIC050	VY023387.D	10/07/2025	11:47
VSTDIC100	VSTDIC100	VY023388.D	10/07/2025	12:09
VSTDIC150	VSTDIC150	VY023389.D	10/07/2025	12:32



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
BROMOFLUOROBENZENE (BFB)

Lab Name: Alliance

Contract: SCIA01

Lab Code: ACE

SDG NO.: Q3410

Lab File ID: VY023520.D

BFB Injection Date: 10/21/2025

Instrument ID: MSVOA_Y

BFB Injection Time: 08:29

GC Column: RXI-624 ID: 0.25 (mm)

Heated Purge: Y/N Y

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
50	15.0 - 40.0% of mass 95	16.5
75	30.0 - 60.0% of mass 95	48.5
95	Base Peak, 100% relative abundance	100
96	5.0 - 9.0% of mass 95	6.7
173	Less than 2.0% of mass 174	1.3 (1.4) 1
174	50.0 - 100.0% of mass 95	94.7
175	5.0 - 9.0% of mass 174	6.8 (7.1) 1
176	95.0 - 101.0% of mass 174	92.5 (97.7) 1
177	5.0 - 9.0% of mass 176	6.2 (6.7) 2

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

CLIENT ID	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
VSTDCCC050	VSTDCCC050	VY023521.D	10/21/2025	09:05
VY1021SBL01	VY1021SBL01	VY023522.D	10/21/2025	09:34
VY1021SBS01	VY1021SBS01	VY023523.D	10/21/2025	10:04
VY1021SBSD01	VY1021SBSD01	VY023524.D	10/21/2025	10:27
VOC	Q3410-02	VY023535.D	10/21/2025	15:22

VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: Alliance Contract: SCIA01
 Lab Code: ACE SDG NO.: Q3410
 Lab File ID: VY023521.D Date Analyzed: 10/21/2025
 Instrument ID: MSVOA_Y Time Analyzed: 09:05
 GC Column: RXI-624 ID: 0.25 (mm) Heated Purge: (Y/N) Y

	IS1 AREA #	RT #	IS2 AREA #	RT #	IS3 AREA #	RT #
12 HOUR STD	499961	7.71	698196	8.62	642915	11.42
UPPER LIMIT	999922	8.213	1396390	9.116	1285830	11.92
LOWER LIMIT	249981	7.213	349098	8.116	321458	10.92
EPA SAMPLE NO.						
VOC	730922	7.71	1192245	8.62	968962	11.41
VY1021SBL01	767531	7.71	1271980	8.62	1000258	11.42
VY1021SBS01	494016	7.71	712868	8.62	635785	11.41
VY1021SBSD01	507725	7.71	737688	8.62	649036	11.41

IS1 = Pentafluorobenzene
 IS2 = 1,4-Difluorobenzene
 IS3 = Chlorobenzene-d5

AREA UPPER LIMIT = +100% of internal standard area
 AREA LOWER LIMIT = -50% of internal standard area
 RT UPPER LIMIT = +0.50 minutes of internal standard RT
 RT LOWER LIMIT = -0.50 minutes of internal standard RT

Column used to flag values outside QC limits with an asterisk.
 * Values outside of QC limits.

VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: Alliance Contract: SCIA01
 Lab Code: ACE SDG NO.: Q3410
 Lab File ID: VY023521.D Date Analyzed: 10/21/2025
 Instrument ID: MSVOA_Y Time Analyzed: 09:05
 GC Column: RXI-624 ID: 0.25 (mm) Heated Purge: (Y/N) Y

	IS4 AREA #	RT #				
12 HOUR STD	341616	13.347				
UPPER LIMIT	683232	13.847				
LOWER LIMIT	170808	12.847				
EPA SAMPLE NO.						
VOC	369934	13.35				
VY1021SBL01	378610	13.35				
VY1021SBS01	341398	13.35				
VY1021SBSD01	345630	13.35				

IS4 = 1,4-Dichlorobenzene-d4

AREA UPPER LIMIT = +100% of internal standard area
 AREA LOWER LIMIT = -50% of internal standard area
 RT UPPER LIMIT = +0.50 minutes of internal standard RT
 RT LOWER LIMIT = -0.50 minutes of internal standard RT

Column used to flag values outside QC limits with an asterisk.
 * Values outside of QC limits.



SAMPLE DATA

Report of Analysis

Client: Sciacca General Contractors, LLC

Project: 49 Moore Place Belleville

Client Sample ID: VOC

Lab Sample ID: Q3410-02

Analytical Method: 8260D

Sample Wt/Vol: 5.02 g

Level: LOW

Final Vol: 5000 uL

Date Collected: 10/20/25

Date Received: 10/20/25

SDG No.: Q3410

Matrix: SOIL

% Solid: 80.5

Test: VOC-TCLVOA-10

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Date Ana.	BatchID
TARGETS									
75-71-8	Dichlorodifluoromethane	1.40	U	1	1.40	6.20	ug/Kg	10/21/25 15:22	VY102125
74-87-3	Chloromethane	1.40	U	1	1.40	6.20	ug/Kg	10/21/25 15:22	VY102125
75-01-4	Vinyl Chloride	0.98	U	1	0.98	6.20	ug/Kg	10/21/25 15:22	VY102125
74-83-9	Bromomethane	1.30	U	1	1.30	6.20	ug/Kg	10/21/25 15:22	VY102125
75-00-3	Chloroethane	1.60	U	1	1.60	6.20	ug/Kg	10/21/25 15:22	VY102125
75-69-4	Trichlorofluoromethane	1.50	U	1	1.50	6.20	ug/Kg	10/21/25 15:22	VY102125
76-13-1	1,1,2-Trichlorotrifluoroethane	1.30	U	1	1.30	6.20	ug/Kg	10/21/25 15:22	VY102125
75-35-4	1,1-Dichloroethene	1.20	U	1	1.20	6.20	ug/Kg	10/21/25 15:22	VY102125
67-64-1	Acetone	5.90	U	1	5.90	30.9	ug/Kg	10/21/25 15:22	VY102125
75-15-0	Carbon Disulfide	1.30	U	1	1.30	6.20	ug/Kg	10/21/25 15:22	VY102125
1634-04-4	Methyl tert-butyl Ether	0.90	U	1	0.90	6.20	ug/Kg	10/21/25 15:22	VY102125
79-20-9	Methyl Acetate	1.90	U	1	1.90	6.20	ug/Kg	10/21/25 15:22	VY102125
75-09-2	Methylene Chloride	4.40	U	1	4.40	12.4	ug/Kg	10/21/25 15:22	VY102125
156-60-5	trans-1,2-Dichloroethene	1.10	U	1	1.10	6.20	ug/Kg	10/21/25 15:22	VY102125
75-34-3	1,1-Dichloroethane	0.99	U	1	0.99	6.20	ug/Kg	10/21/25 15:22	VY102125
110-82-7	Cyclohexane	0.98	U	1	0.98	6.20	ug/Kg	10/21/25 15:22	VY102125
78-93-3	2-Butanone	8.10	U	1	8.10	30.9	ug/Kg	10/21/25 15:22	VY102125
56-23-5	Carbon Tetrachloride	1.20	U	1	1.20	6.20	ug/Kg	10/21/25 15:22	VY102125
156-59-2	cis-1,2-Dichloroethene	0.93	U	1	0.93	6.20	ug/Kg	10/21/25 15:22	VY102125
74-97-5	Bromochloromethane	1.40	U	1	1.40	6.20	ug/Kg	10/21/25 15:22	VY102125
67-66-3	Chloroform	1.00	U	1	1.00	6.20	ug/Kg	10/21/25 15:22	VY102125
71-55-6	1,1,1-Trichloroethane	1.20	U	1	1.20	6.20	ug/Kg	10/21/25 15:22	VY102125
108-87-2	Methylcyclohexane	1.10	U	1	1.10	6.20	ug/Kg	10/21/25 15:22	VY102125
71-43-2	Benzene	0.98	U	1	0.98	6.20	ug/Kg	10/21/25 15:22	VY102125
107-06-2	1,2-Dichloroethane	0.98	U	1	0.98	6.20	ug/Kg	10/21/25 15:22	VY102125
79-01-6	Trichloroethene	1.00	U	1	1.00	6.20	ug/Kg	10/21/25 15:22	VY102125
78-87-5	1,2-Dichloropropane	1.10	U	1	1.10	6.20	ug/Kg	10/21/25 15:22	VY102125
75-27-4	Bromodichloromethane	0.97	U	1	0.97	6.20	ug/Kg	10/21/25 15:22	VY102125
108-10-1	4-Methyl-2-Pentanone	4.40	U	1	4.40	30.9	ug/Kg	10/21/25 15:22	VY102125
108-88-3	Toluene	0.97	U	1	0.97	6.20	ug/Kg	10/21/25 15:22	VY102125
10061-02-6	t-1,3-Dichloropropene	0.80	U	1	0.80	6.20	ug/Kg	10/21/25 15:22	VY102125
10061-01-5	cis-1,3-Dichloropropene	0.77	U	1	0.77	6.20	ug/Kg	10/21/25 15:22	VY102125
79-00-5	1,1,2-Trichloroethane	1.10	U	1	1.10	6.20	ug/Kg	10/21/25 15:22	VY102125
591-78-6	2-Hexanone	4.60	U	1	4.60	30.9	ug/Kg	10/21/25 15:22	VY102125
124-48-1	Dibromochloromethane	1.10	U	1	1.10	6.20	ug/Kg	10/21/25 15:22	VY102125
106-93-4	1,2-Dibromoethane	1.10	U	1	1.10	6.20	ug/Kg	10/21/25 15:22	VY102125
127-18-4	Tetrachloroethene	1.30	U	1	1.30	6.20	ug/Kg	10/21/25 15:22	VY102125
108-90-7	Chlorobenzene	1.10	U	1	1.10	6.20	ug/Kg	10/21/25 15:22	VY102125
100-41-4	Ethyl Benzene	0.83	U	1	0.83	6.20	ug/Kg	10/21/25 15:22	VY102125
179601-23-1	m/p-Xylenes	1.50	U	1	1.50	12.4	ug/Kg	10/21/25 15:22	VY102125
95-47-6	o-Xylene	1.00	U	1	1.00	6.20	ug/Kg	10/21/25 15:22	VY102125
100-42-5	Styrene	0.88	U	1	0.88	6.20	ug/Kg	10/21/25 15:22	VY102125
75-25-2	Bromoform	1.10	U	1	1.10	6.20	ug/Kg	10/21/25 15:22	VY102125



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client: Sciacca General Contractors, LLC

Project: 49 Moore Place Belleville

Client Sample ID: VOC

Lab Sample ID: Q3410-02

Analytical Method: 8260D

Sample Wt/Vol: 5.02 g

Level : LOW

Final Vol: 5000 uL

Date Collected: 10/20/25

Date Received: 10/20/25

SDG No.: Q3410

Matrix: SOIL

% Solid: 80.5

Test: VOC-TCLVOA-10

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Date Ana.	BatchID
98-82-8	Isopropylbenzene	0.97	U	1	0.97	6.20	ug/Kg	10/21/25 15:22	VY102125
79-34-5	1,1,2,2-Tetrachloroethane	1.50	U	1	1.50	6.20	ug/Kg	10/21/25 15:22	VY102125
541-73-1	1,3-Dichlorobenzene	2.10	U	1	2.10	6.20	ug/Kg	10/21/25 15:22	VY102125
106-46-7	1,4-Dichlorobenzene	1.90	U	1	1.90	6.20	ug/Kg	10/21/25 15:22	VY102125
95-50-1	1,2-Dichlorobenzene	1.80	U	1	1.80	6.20	ug/Kg	10/21/25 15:22	VY102125
96-12-8	1,2-Dibromo-3-Chloropropane	2.30	U	1	2.30	6.20	ug/Kg	10/21/25 15:22	VY102125
120-82-1	1,2,4-Trichlorobenzene	3.70	U	1	3.70	6.20	ug/Kg	10/21/25 15:22	VY102125
87-61-6	1,2,3-Trichlorobenzene	3.90	U	1	3.90	6.20	ug/Kg	10/21/25 15:22	VY102125
SURROGATES									
17060-07-0	1,2-Dichloroethane-d4	51.4			63 - 155	103%	SPK: 50		
1868-53-7	Dibromofluoromethane	51.0			70 - 134	102%	SPK: 50		
2037-26-5	Toluene-d8	48.2			74 - 123	96%	SPK: 50		
460-00-4	4-Bromofluorobenzene	39.1			17 - 146	78%	SPK: 50		
INTERNAL STANDARDS									
		Area Count							
363-72-4	Pentafluorobenzene	731000							
540-36-3	1,4-Difluorobenzene	1190000							
3114-55-4	Chlorobenzene-d5	969000							
3855-82-1	1,4-Dichlorobenzene-d4	370000							

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
 Data File : VY023535.D
 Acq On : 21 Oct 2025 15:22
 Operator : SY/MD
 Sample : Q3410-02
 Misc : 5.02g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VOC

Quant Time: Oct 24 01:37:14 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.713	168	730922	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	1192245	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	968962	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	369934	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.067	65	314071	51.385	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	102.780%
35) Dibromofluoromethane	7.634	113	373961	51.047	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	102.100%
50) Toluene-d8	10.109	98	1314151	48.169	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	96.340%
62) 4-Bromofluorobenzene	12.408	95	352021	39.083	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	78.160%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
Data File : VY023535.D
Acq On : 21 Oct 2025 15:22
Operator : SY/MD
Sample : Q3410-02
Misc : 5.02g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VOC

Quant Time: Oct 24 01:37:14 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 05:12:50 2025
Response via : Initial Calibration




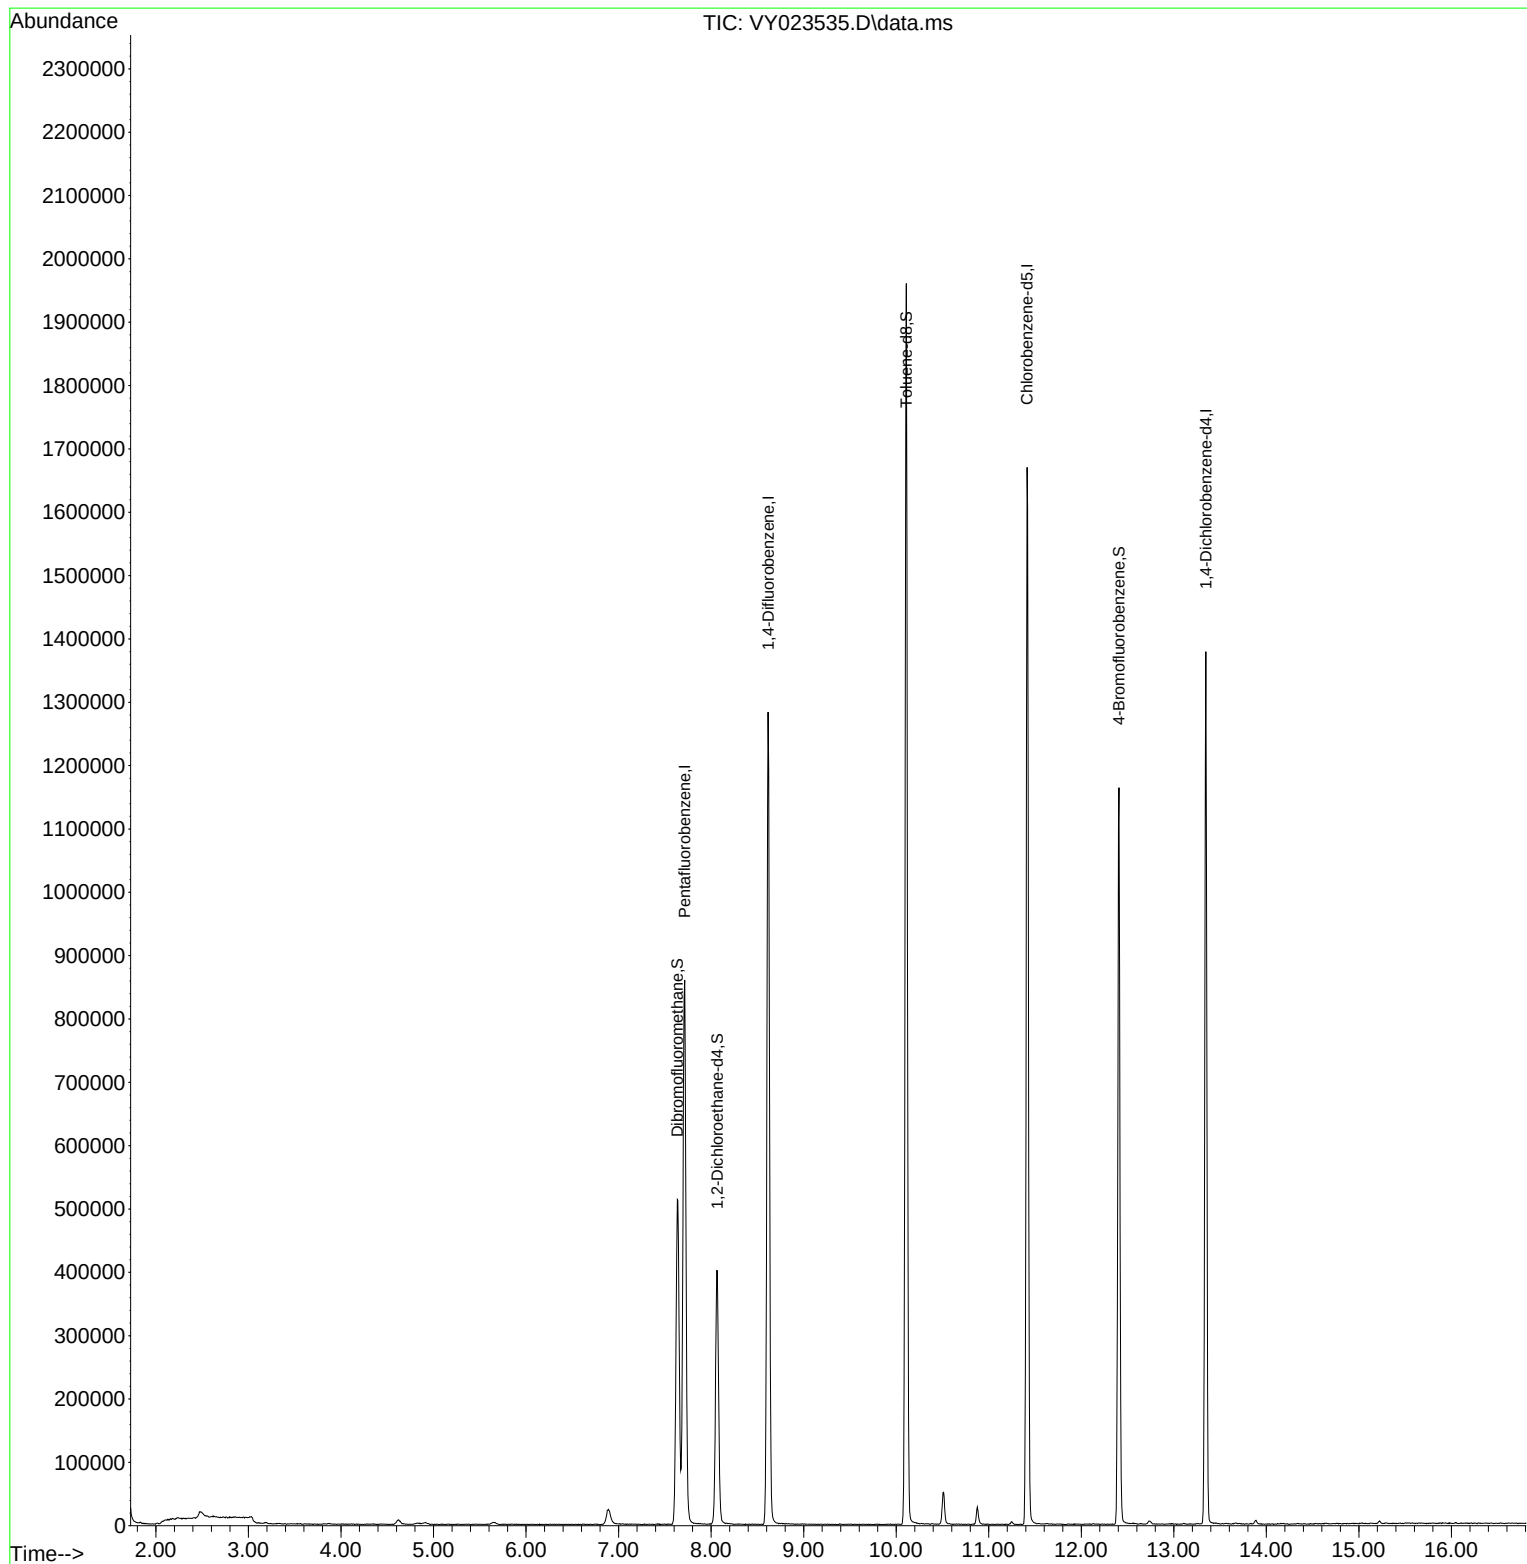


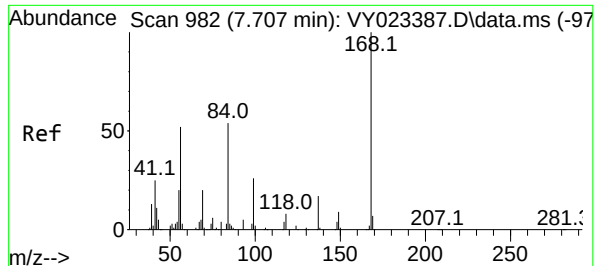

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 99
Delta R.T. 0.006 min
Lab File: VY023535.D
Acq: 21 Oct 2025 15:22




Instrument :
MSVOA_Y
ClientSampleId :
VOC


Tgt Ion:168 Resp: 730922
Ion Ratio Lower Upper
168 100
99 47.4 39.7 59.5

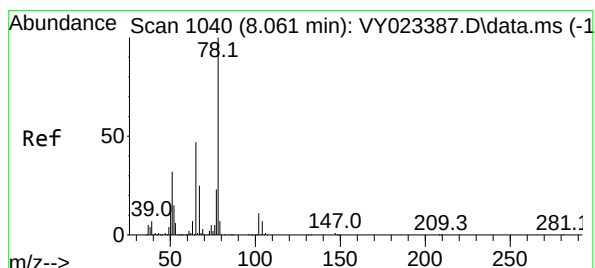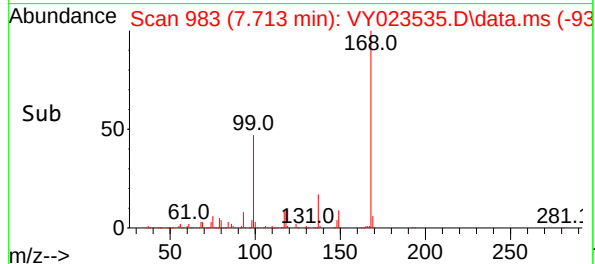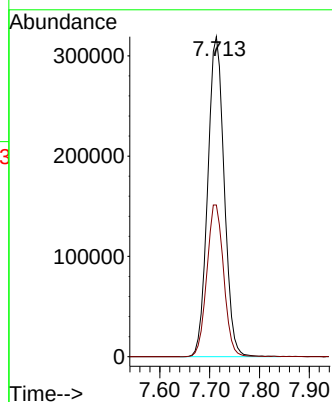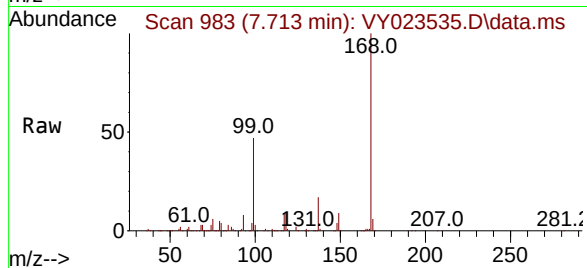

#33
1,2-Dichloroethane-d4
Concen: 51.385 ug/l
RT: 8.067 min Scan# 1041
Delta R.T. 0.006 min
Lab File: VY023535.D
Acq: 21 Oct 2025 15:22

Tgt Ion: 65 Resp: 314071
Ion Ratio Lower Upper
65 100
67 53.6 0.0 105.8

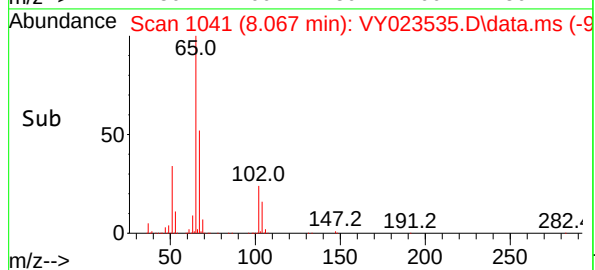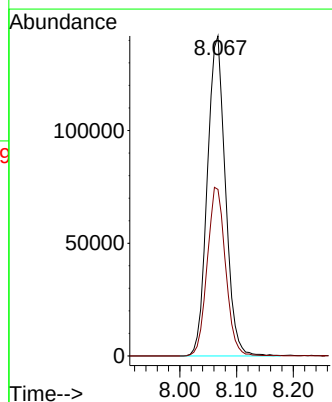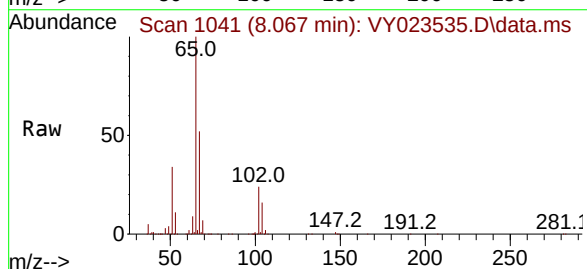

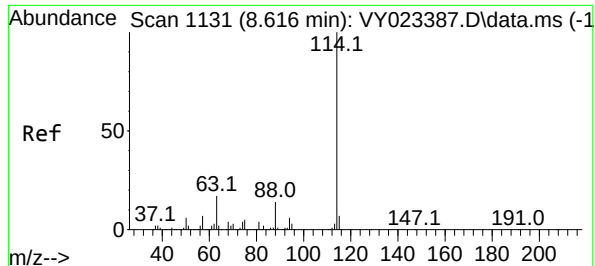

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.616 min Scan# 1131

Delta R.T. 0.000 min

Lab File: VY023535.D

Acq: 21 Oct 2025 15:22

Instrument :

MSVOA_Y

ClientSampleId :

VOC





Tgt Ion:114 Resp: 1192245

Ion Ratio Lower Upper

114 100

63 16.0 0.0 34.2

88 14.4 0.0 28.4

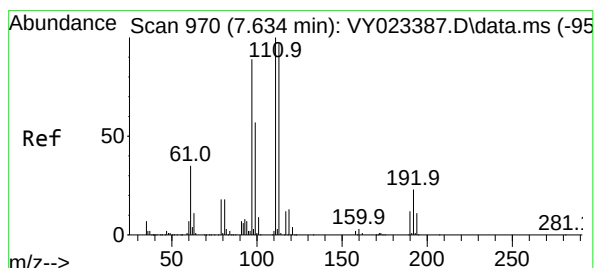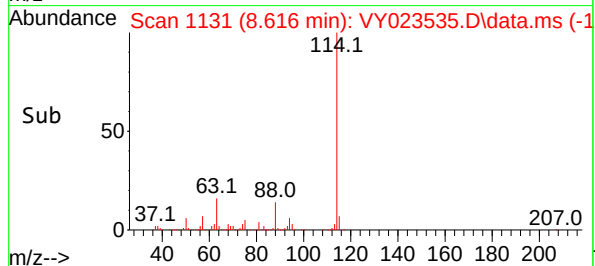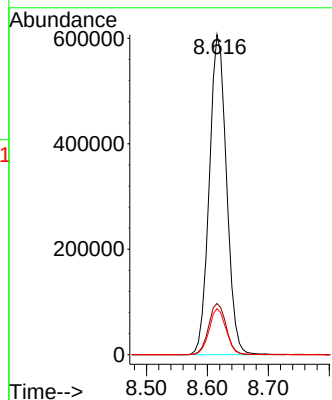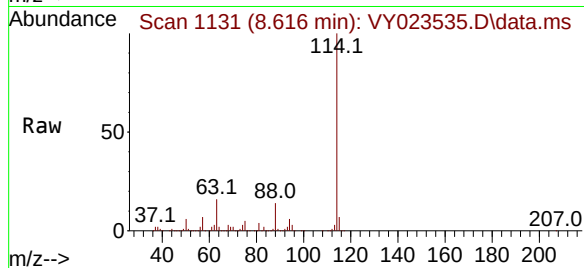

#35

Dibromofluoromethane

Concen: 51.047 ug/l

RT: 7.634 min Scan# 970

Delta R.T. 0.000 min

Lab File: VY023535.D

Acq: 21 Oct 2025 15:22




Tgt Ion:113 Resp: 373961


Ion Ratio Lower Upper

113 100

111 101.7 81.8 122.6

192 22.1 18.0 27.0


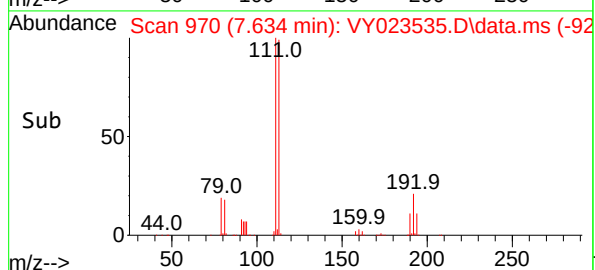
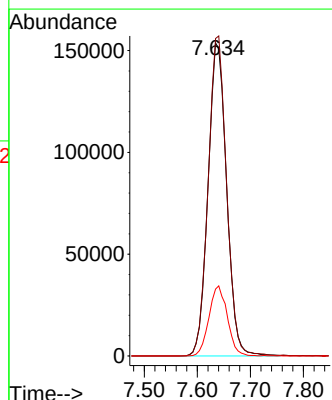
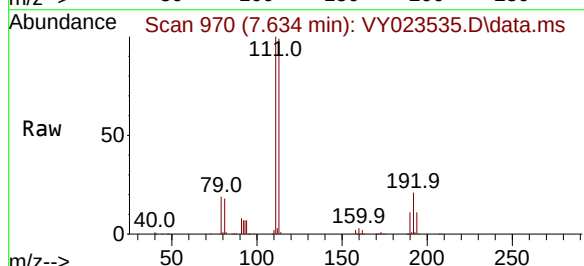


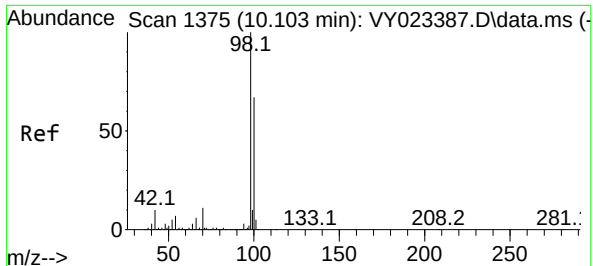

#50
Toluene-d8
Concen: 48.169 ug/l
RT: 10.109 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY023535.D
Acq: 21 Oct 2025 15:22




Instrument :
MSVOA_Y
ClientSampleId :
VOC


Tgt Ion: 98 Resp: 1314151
Ion Ratio Lower Upper
98 100
100 65.4 53.0 79.4

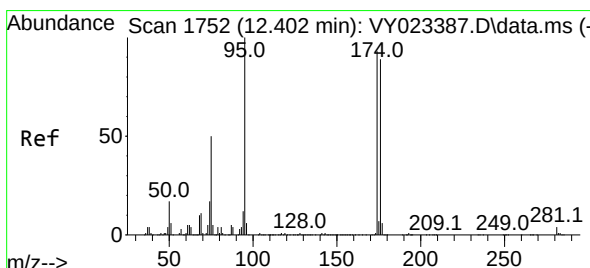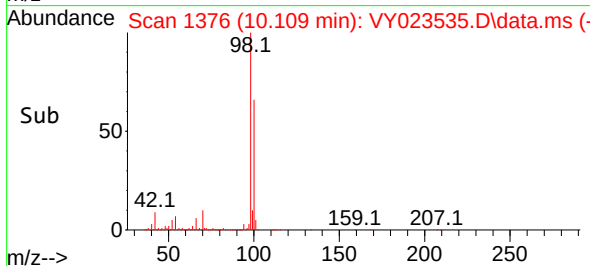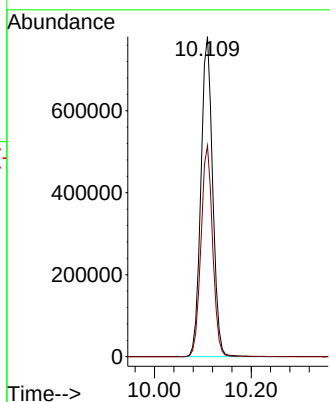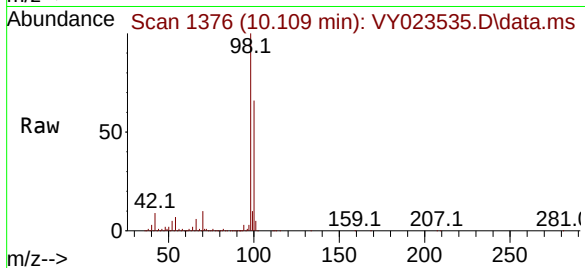

#62
4-Bromofluorobenzene
Concen: 39.083 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.006 min
Lab File: VY023535.D
Acq: 21 Oct 2025 15:22

Tgt Ion: 95 Resp: 352021
Ion Ratio Lower Upper
95 100
174 97.7 0.0 192.8
176 93.1 0.0 187.6

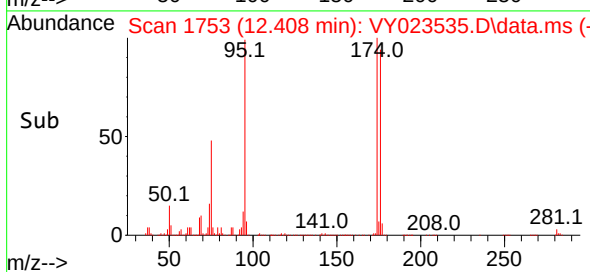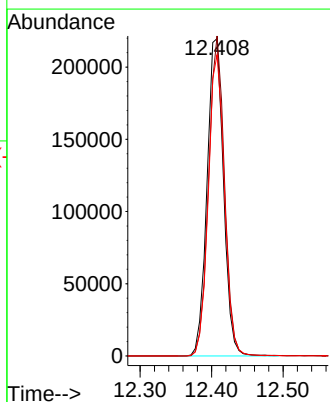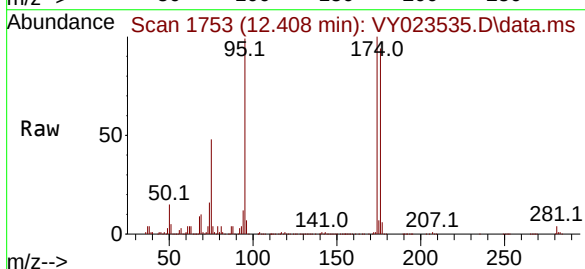

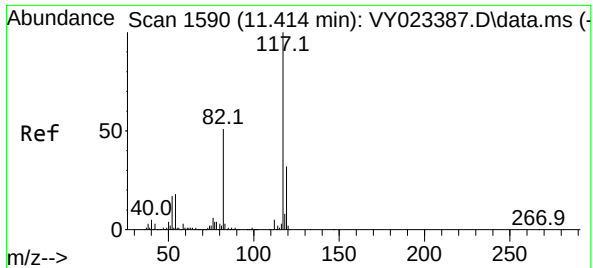

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY023535.D

Acq: 21 Oct 2025 15:22

Instrument :

MSVOA_Y

ClientSampleId :

VOC





Tgt Ion:117 Resp: 968962

Ion Ratio Lower Upper

117 100

82 50.0 41.0 61.4

119 32.2 25.6 38.4

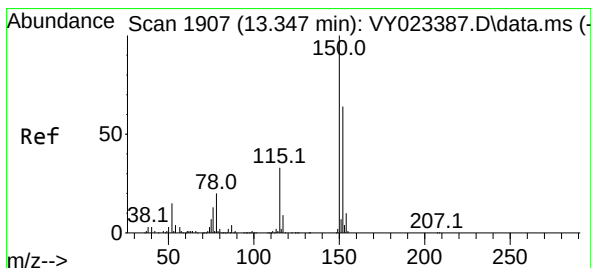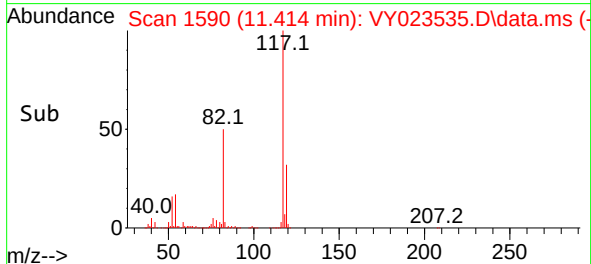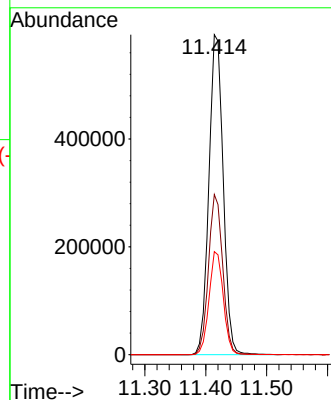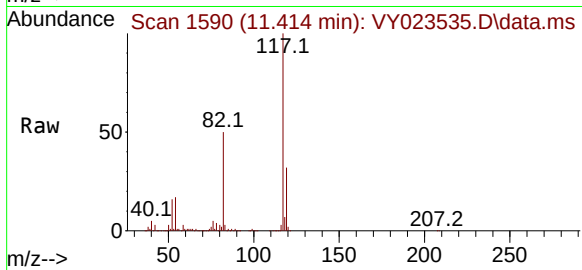

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.347 min Scan# 1907

Delta R.T. 0.000 min

Lab File: VY023535.D

Acq: 21 Oct 2025 15:22




Tgt Ion:152 Resp: 369934

Ion Ratio Lower Upper

152 100

115 54.2 27.1 81.2

150 157.1 0.0 347.4

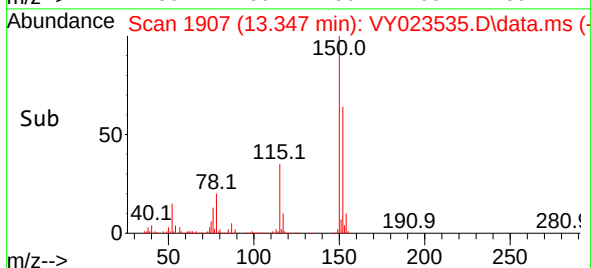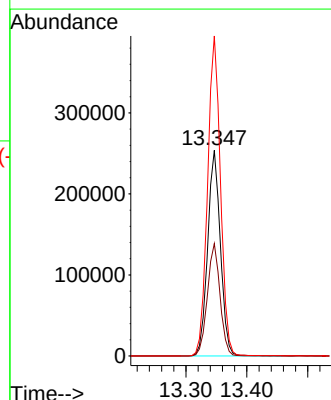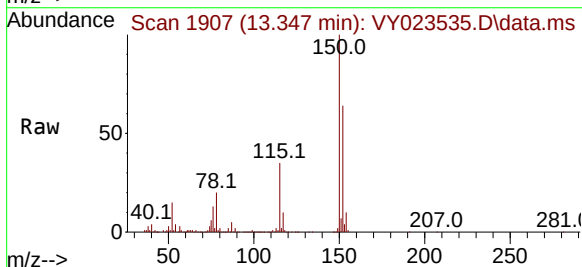

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
Data File : VY023535.D
Acq On : 21 Oct 2025 15:22
Operator : SY/MD
Sample : Q3410-02
Misc : 5.02g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VOC

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M

Title : SW846 8260

Signal : TIC: VY023535.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.470	116	123	133	rBV8	10460	39327	1.18%	0.232%
2	6.890	836	848	862	rBV2	24039	82669	2.49%	0.487%
3	7.634	960	970	976	rBV	512872	1228938	36.97%	7.245%
4	7.713	976	983	999	rVB	858456	1993542	59.98%	11.753%
5	8.061	1030	1040	1055	rBV	400553	928093	27.92%	5.472%
6	8.616	1122	1131	1147	rBV	1282709	2547104	76.63%	15.017%
7	10.109	1366	1376	1394	rBV	1959151	3323898	100.00%	19.597%
8	10.512	1433	1442	1451	rBV2	50638	97023	2.92%	0.572%
9	10.878	1495	1502	1511	rBV	27184	44942	1.35%	0.265%
10	11.414	1582	1590	1607	rBV	1668842	2735789	82.31%	16.129%
11	12.408	1744	1753	1765	rBV	1163058	1881570	56.61%	11.093%
12	13.347	1896	1907	1920	rBV	1377228	2058621	61.93%	12.137%




Sum of corrected areas: 16961516

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
Data File : VY023535.D
Acq On : 21 Oct 2025 15:22
Operator : SY/MD
Sample : Q3410-02
Misc : 5.02g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VOC

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

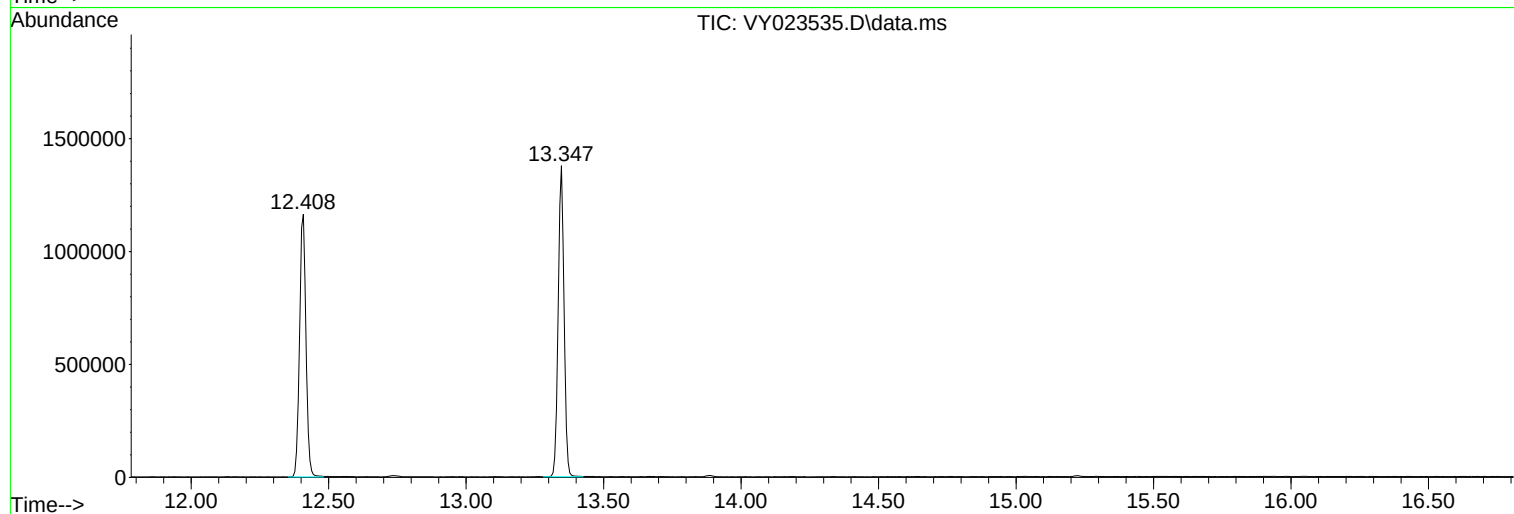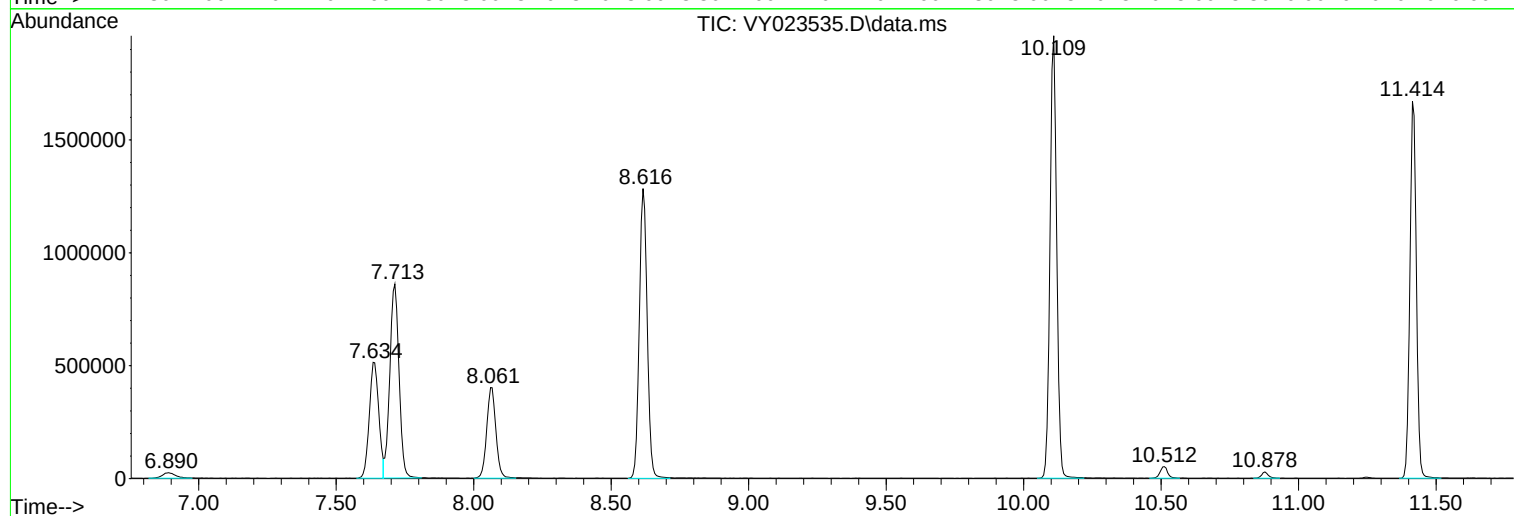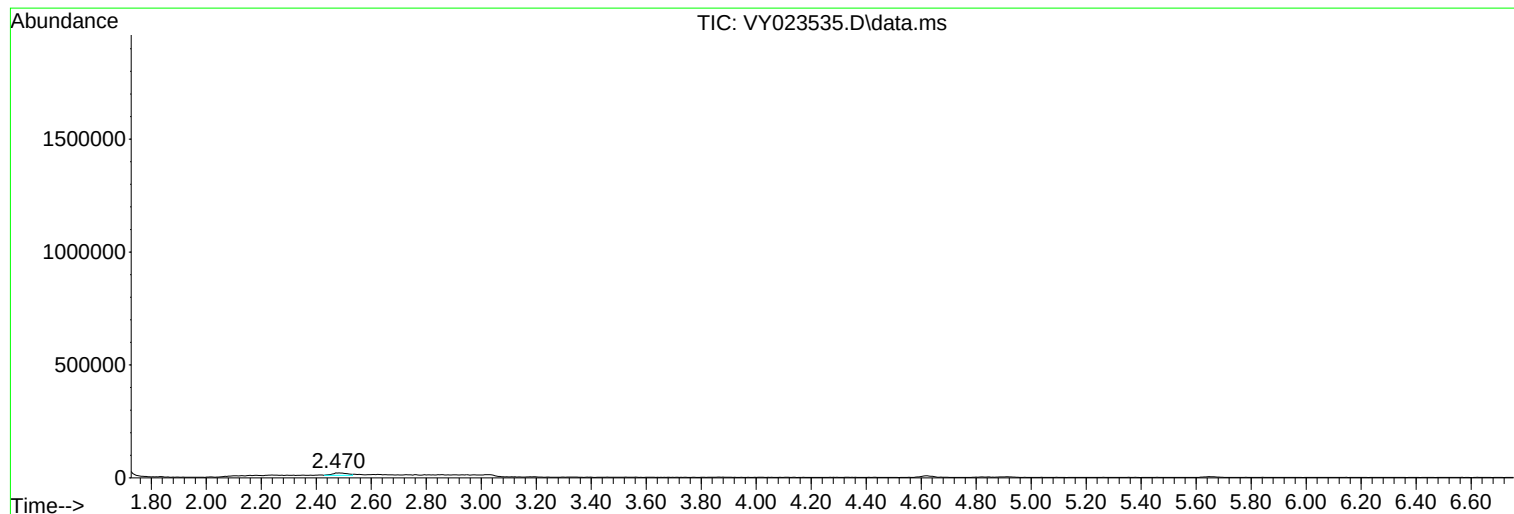

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
Data File : VY023535.D
Acq On : 21 Oct 2025 15:22
Operator : SY/MD
Sample : Q3410-02
Misc : 5.02g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VOC

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
Data File : VY023535.D
Acq On : 21 Oct 2025 15:22
Operator : SY/MD
Sample : Q3410-02
Misc : 5.02g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VOC

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------



CALIBRATION SUMMARY



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE ORGANICS INITIAL CALIBRATION DATA

Lab Name: Alliance Contract: SCIA01
 Lab Code: ACE SDG No.: Q3410
 Instrument ID: MSVOA_Y Calibration Date(s): 10/07/2025 10/07/2025
 Heated Purge: (Y/N) Y Calibration Time(s): 09:17 12:32
 GC Column: RXI-624 ID: 0.25 (mm)

LAB FILE ID:		RRF005 = VY023384.D		RRF010 = VY023385.D		RRF020 = VY023386.D			
		RRF050 = VY023387.D		RRF100 = VY023388.D		RRF150 = VY023389.D			
COMPOUND	RRF005	RRF010	RRF020	RRF050	RRF100	RRF150	RRF	% RSD	
Dichlorodifluoromethane	0.397	0.399	0.400	0.321	0.310	0.333	0.360	12	
Chloromethane	0.518	0.557	0.512	0.449	0.438	0.467	0.490	9.4	
Vinyl Chloride	0.660	0.684	0.659	0.598	0.597	0.633	0.639	5.6	
Bromomethane	0.601	0.596	0.548	0.469	0.483	0.518	0.536	10.4	
Chloroethane	0.441	0.462	0.453	0.414	0.413	0.429	0.435	4.7	
Trichlorofluoromethane	0.884	0.920	0.946	0.842	0.850	0.877	0.887	4.5	
1,1,2-Trichlorotrifluoroethane	0.484	0.486	0.479	0.437	0.429	0.445	0.460	5.6	
1,1-Dichloroethene	0.449	0.475	0.456	0.427	0.426	0.443	0.446	4.1	
Acetone	0.128	0.117	0.094	0.084	0.085	0.089	0.100	18.7	
Carbon Disulfide	1.291	1.367	1.320	1.225	1.210	1.246	1.277	4.7	
Methyl tert-butyl Ether	1.006	1.075	1.075	1.020	1.091	1.165	1.072	5.3	
Methyl Acetate	0.244	0.265	0.260	0.245	0.266	0.286	0.261	6	
Methylene Chloride	0.625	0.634	0.576	0.458	0.463	0.473	0.538	15.4	
trans-1,2-Dichloroethene	0.494	0.504	0.507	0.470	0.478	0.494	0.491	2.9	
1,1-Dichloroethane	0.800	0.835	0.827	0.759	0.765	0.792	0.796	3.9	
Cyclohexane	0.797	0.717	0.697	0.643	0.644	0.676	0.696	8.3	
2-Butanone	0.133	0.134	0.115	0.105	0.115	0.126	0.122	9.6	
Carbon Tetrachloride	0.483	0.501	0.504	0.481	0.487	0.503	0.493	2.1	
cis-1,2-Dichloroethene	0.542	0.584	0.582	0.542	0.563	0.591	0.567	3.8	
Bromochloromethane	0.332	0.323	0.320	0.267	0.270	0.273	0.297	10.2	
Chloroform	0.886	0.912	0.901	0.835	0.842	0.874	0.875	3.5	
1,1,1-Trichloroethane	0.808	0.814	0.822	0.767	0.764	0.796	0.795	3.1	
Methylcyclohexane	0.491	0.486	0.537	0.527	0.554	0.583	0.530	7	
Benzene	1.253	1.302	1.322	1.259	1.281	1.312	1.288	2.2	
1,2-Dichloroethane	0.328	0.346	0.343	0.315	0.324	0.338	0.332	3.6	
Trichloroethene	0.380	0.381	0.386	0.367	0.372	0.376	0.377	1.8	
1,2-Dichloropropane	0.276	0.289	0.292	0.274	0.283	0.293	0.285	2.9	
Bromodichloromethane	0.440	0.463	0.459	0.439	0.449	0.468	0.453	2.7	
4-Methyl-2-Pentanone	0.141	0.159	0.161	0.159	0.180	0.196	0.166	11.6	
Toluene	0.777	0.818	0.855	0.827	0.855	0.885	0.836	4.5	

* Compounds with required minimum RRF and maximum %RSD values.
 All other compounds must meet a minimum RRF of 0.010.
 RRF of 1,4-Dioxane = Value should be divide by 1000.



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE ORGANICS INITIAL CALIBRATION DATA

Lab Name: Alliance Contract: SCIA01
 Lab Code: ACE SDG No.: Q3410
 Instrument ID: MSVOA_Y Calibration Date(s): 10/07/2025 10/07/2025
 Heated Purge: (Y/N) Y Calibration Time(s): 09:17 12:32
 GC Column: RXI-624 ID: 0.25 (mm)

LAB FILE ID:	RRF005 = VY023384.D			RRF010 = VY023385.D		RRF020 = VY023386.D		RRF050 = VY023387.D		RRF100 = VY023388.D		RRF150 = VY023389.D	
COMPOUND	RRF005	RRF010	RRF020	RRF050	RRF100	RRF150	RRF	% RSD					
t-1,3-Dichloropropene	0.357	0.380	0.390	0.385	0.415	0.438	0.394	7.2					
cis-1,3-Dichloropropene	0.424	0.460	0.465	0.455	0.481	0.505	0.465	5.9					
1,1,2-Trichloroethane	0.234	0.247	0.241	0.231	0.244	0.254	0.242	3.5					
2-Hexanone	0.108	0.117	0.110	0.112	0.126	0.138	0.119	9.9					
Dibromochloromethane	0.319	0.337	0.340	0.327	0.347	0.365	0.339	4.7					
1,2-Dibromoethane	0.215	0.229	0.231	0.223	0.237	0.249	0.231	5.2					
Tetrachloroethene	0.538	0.517	0.561	0.523	0.502	0.456	0.516	6.9					
Chlorobenzene	1.086	1.095	1.092	1.053	1.083	1.116	1.087	1.9					
Ethyl Benzene	1.606	1.711	1.753	1.777	1.824	1.891	1.760	5.5					
m/p-Xylenes	0.632	0.675	0.715	0.719	0.734	0.763	0.706	6.5					
o-Xylene	0.588	0.623	0.653	0.670	0.701	0.738	0.662	8.1					
Styrene	0.902	1.026	1.098	1.109	1.166	1.233	1.089	10.5					
Bromoform	0.225	0.242	0.238	0.230	0.244	0.262	0.240	5.4					
Isopropylbenzene	2.967	3.153	3.353	3.317	3.425	3.555	3.295	6.3					
1,1,2,2-Tetrachloroethane	0.530	0.548	0.502	0.499	0.543	0.611	0.539	7.6					
1,3-Dichlorobenzene	1.667	1.698	1.718	1.657	1.701	1.794	1.706	2.9					
1,4-Dichlorobenzene	1.703	1.703	1.694	1.624	1.653	1.732	1.685	2.3					
1,2-Dichlorobenzene	1.485	1.498	1.511	1.446	1.490	1.543	1.496	2.1					
1,2-Dibromo-3-Chloropropane	0.087	0.093	0.083	0.083	0.088	0.096	0.088	6.2					
1,2,4-Trichlorobenzene	0.846	0.867	0.901	0.918	1.007	1.054	0.932	8.7					
1,2,3-Trichlorobenzene	0.719	0.753	0.795	0.793	0.866	0.920	0.808	9.1					
1,2-Dichloroethane-d4	0.455	0.436	0.429	0.392	0.392	0.405	0.418	6.2					
Dibromofluoromethane	0.311	0.314	0.317	0.298	0.299	0.303	0.307	2.6					
Toluene-d8	1.132	1.170	1.177	1.129	1.122	1.135	1.144	2					
4-Bromofluorobenzene	0.401	0.370	0.373	0.365	0.372	0.386	0.378	3.5					

* Compounds with required minimum RRF and maximum %RSD values.
 All other compounds must meet a minimum RRF of 0.010.
 RRF of 1,4-Dioxane = Value should be divide by 1000.

Method Path : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\
 Method File : 82Y100725S.M
 Title : SW846 8260
 Last Update : Wed Oct 08 05:12:50 2025
 Response Via : Initial Calibration

Calibration Files

5 =VY023384.D 10 =VY023385.D 20 =VY023386.D 50 =VY023387.D 100 =VY023388.D 150 =VY023389.D

	Compound	5	10	20	50	100	150	Avg	%RSD
1) I	Pentafluorobenzene	-----ISTD-----							
2) T	Dichlorodifluo...	0.397	0.399	0.400	0.321	0.310	0.333	0.360	11.97
3) P	Chloromethane	0.518	0.557	0.512	0.449	0.438	0.467	0.490	9.45
4) C	Vinyl Chloride	0.660	0.684	0.659	0.598	0.597	0.633	0.639	5.59#
5) T	Bromomethane	0.601	0.596	0.548	0.469	0.483	0.518	0.536	10.42
6) T	Chloroethane	0.441	0.462	0.453	0.414	0.413	0.429	0.435	4.67
7) T	Trichlorofluor...	0.884	0.920	0.946	0.842	0.850	0.877	0.887	4.54
8) T	Diethyl Ether	0.240	0.239	0.236	0.215	0.224	0.237	0.232	4.42
9) T	1,1,2-Trichlor...	0.484	0.486	0.479	0.437	0.429	0.445	0.460	5.57
10) T	Methyl Iodide	0.404	0.503	0.518	0.538	0.547	0.562	0.512	11.09
11) T	Tert butyl alc...	0.033	0.037	0.030	0.025	0.029	0.033	0.031	13.08
12) CM	1,1-Dichloroet...	0.449	0.475	0.456	0.427	0.426	0.443	0.446	4.14#
13) T	Acrolein	0.045	0.043	0.042	0.042	0.044	0.048	0.044	5.27
14) T	Allyl chloride	0.540	0.555	0.546	0.526	0.535	0.560	0.544	2.33
15) T	Acrylonitrile	0.088	0.093	0.086	0.082	0.088	0.095	0.089	5.52
16) T	Acetone	0.128	0.117	0.094	0.084	0.085	0.089	0.100	18.67
17) T	Carbon Disulfide	1.291	1.367	1.320	1.225	1.210	1.246	1.277	4.74
18) T	Methyl Acetate	0.244	0.265	0.260	0.245	0.266	0.286	0.261	6.00
19) T	Methyl tert-bu...	1.006	1.075	1.075	1.020	1.091	1.165	1.072	5.30
20) T	Methylene Chlo...	0.625	0.634	0.576	0.458	0.463	0.473	0.538	15.41
21) T	trans-1,2-Dich...	0.494	0.504	0.507	0.470	0.478	0.494	0.491	2.95
22) T	Diisopropyl ether	1.107	1.238	1.255	1.163	1.195	1.257	1.202	4.95
23) T	Vinyl Acetate	0.594	0.646	0.651	0.625	0.667	0.722	0.651	6.65
24) P	1,1-Dichloroet...	0.800	0.835	0.827	0.759	0.765	0.792	0.796	3.90
25) T	2-Butanone	0.133	0.134	0.115	0.105	0.115	0.126	0.122	9.56
26) T	2,2-Dichloropr...	0.752	0.771	0.731	0.705	0.699	0.726	0.731	3.74
27) T	cis-1,2-Dichlo...	0.542	0.584	0.582	0.542	0.563	0.591	0.567	3.81
28) T	Bromochloromet...	0.332	0.323	0.320	0.267	0.270	0.273	0.297	10.22
29) T	Tetrahydrofuran	0.066	0.070	0.067	0.064	0.070	0.078	0.069	7.25
30) C	Chloroform	0.886	0.912	0.901	0.835	0.842	0.874	0.875	3.54#
31) T	Cyclohexane	0.797	0.717	0.697	0.643	0.644	0.676	0.696	8.27
32) T	1,1,1-Trichlor...	0.808	0.814	0.822	0.767	0.764	0.796	0.795	3.08
33) S	1,2-Dichloroet...	0.455	0.436	0.429	0.392	0.392	0.405	0.418	6.21
34) I	1,4-Difluorobenzene	-----ISTD-----							
35) S	Dibromofluorom...	0.311	0.314	0.317	0.298	0.299	0.303	0.307	2.62
36) T	1,1-Dichloropr...	0.395	0.413	0.413	0.397	0.405	0.417	0.407	2.20
37) T	Ethyl Acetate	0.148	0.162	0.163	0.150	0.164	0.179	0.161	6.94
38) T	Carbon Tetrach...	0.483	0.501	0.504	0.481	0.487	0.503	0.493	2.14
39) T	Methylcyclohexane	0.491	0.486	0.537	0.527	0.554	0.583	0.530	7.03
40) TM	Benzene	1.253	1.302	1.322	1.259	1.281	1.312	1.288	2.22
41) T	Methacrylonitrile	0.082	0.085	0.091	0.080	0.089	0.096	0.087	7.09
42) TM	1,2-Dichloroet...	0.328	0.346	0.343	0.315	0.324	0.338	0.332	3.59
43) T	Isopropyl Acetate	0.297	0.313	0.313	0.302	0.335	0.369	0.321	8.32
44) TM	Trichloroethene	0.380	0.381	0.386	0.367	0.372	0.376	0.377	1.81
45) C	1,2-Dichloropr...	0.276	0.289	0.292	0.274	0.283	0.293	0.285	2.89#
46) T	Dibromomethane	0.172	0.182	0.183	0.173	0.181	0.188	0.180	3.43
47) T	Bromodichlorom...	0.440	0.463	0.459	0.439	0.449	0.468	0.453	2.70
48) T	Methyl methacr...	0.125	0.139	0.149	0.148	0.165	0.181	0.151	12.98
49) T	1,4-Dioxane	0.002	0.002	0.002	0.002	0.002	0.002	0.002	10.06
50) S	Toluene-d8	1.132	1.170	1.177	1.129	1.122	1.135	1.144	2.03
51) T	4-Methyl-2-Pen...	0.141	0.159	0.161	0.159	0.180	0.196	0.166	11.55
52) CM	Toluene	0.777	0.818	0.855	0.827	0.855	0.885	0.836	4.49#
53) T	t-1,3-Dichloro...	0.357	0.380	0.390	0.385	0.415	0.438	0.394	7.24
54) T	cis-1,3-Dichlo...	0.424	0.460	0.465	0.455	0.481	0.505	0.465	5.86
55) T	1,1,2-Trichlor...	0.234	0.247	0.241	0.231	0.244	0.254	0.242	3.52
56) T	Ethyl methacry...	0.219	0.248	0.262	0.279	0.321	0.345	0.279	16.80

Method Path : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\
 Method File : 82Y100725S.M

57)	T	1,3-Dichloropr...	0.361	0.381	0.383	0.374	0.392	0.409	0.383	4.26
58)	T	2-Chloroethyl ...	0.093	0.112	0.112	0.129	0.145	0.159	0.125	19.35
59)	T	2-Hexanone	0.108	0.117	0.110	0.112	0.126	0.138	0.119	9.86
60)	T	Dibromochlorom...	0.319	0.337	0.340	0.327	0.347	0.365	0.339	4.69
61)	T	1,2-Dibromoethane	0.215	0.229	0.231	0.223	0.237	0.249	0.231	5.16
62)	S	4-Bromofluorob...	0.401	0.370	0.373	0.365	0.372	0.386	0.378	3.51
63)	I	Chlorobenzene-d5	-----ISTD-----							
64)	T	Tetrachloroethene	0.538	0.517	0.561	0.523	0.502	0.456	0.516	6.92
65)	PM	Chlorobenzene	1.086	1.095	1.092	1.053	1.083	1.116	1.087	1.89
66)	T	1,1,1,2-Tetrac...	0.388	0.389	0.390	0.373	0.384	0.402	0.388	2.44
67)	C	Ethyl Benzene	1.606	1.711	1.753	1.777	1.824	1.891	1.760	5.54#
68)	T	m/p-Xylenes	0.632	0.675	0.715	0.719	0.734	0.763	0.706	6.54
69)	T	o-Xylene	0.588	0.623	0.653	0.670	0.701	0.738	0.662	8.15
70)	T	Styrene	0.902	1.026	1.098	1.109	1.166	1.233	1.089	10.55
71)	P	Bromoform	0.225	0.242	0.238	0.230	0.244	0.262	0.240	5.41
72)	I	1,4-Dichlorobenzen...	-----ISTD-----							
73)	T	Isopropylbenzene	2.967	3.153	3.353	3.317	3.425	3.555	3.295	6.30
74)	T	N-amyl acetate	0.477	0.535	0.556	0.581	0.665	0.738	0.592	15.95
75)	P	1,1,2,2-Tetrac...	0.530	0.548	0.502	0.499	0.543	0.611	0.539	7.60
76)	T	1,2,3-Trichlor...	0.406	0.399	0.484	0.433	0.455	0.469	0.441	7.76
77)	T	Bromobenzene	0.849	0.880	0.885	0.845	0.877	0.921	0.876	3.14
78)	T	n-propylbenzene	3.373	3.676	3.906	3.883	3.955	4.086	3.813	6.64
79)	T	2-Chlorotoluene	2.095	2.208	2.282	2.227	2.249	2.338	2.233	3.66
80)	T	1,3,5-Trimethy...	2.309	2.557	2.736	2.706	2.772	2.896	2.663	7.70
81)	T	trans-1,4-Dich...	0.171	0.175	0.176	0.169	0.185	0.203	0.180	7.04
82)	T	4-Chlorotoluene	2.173	2.266	2.362	2.276	2.316	2.404	2.300	3.52
83)	T	tert-Butylbenzene	2.199	2.363	2.465	2.522	2.533	2.668	2.458	6.55
84)	T	1,2,4-Trimethy...	2.301	2.552	2.701	2.706	2.782	2.903	2.657	7.86
85)	T	sec-Butylbenzene	3.175	3.388	3.571	3.583	3.664	3.778	3.527	6.08
86)	T	p-Isopropyltol...	2.575	2.804	3.032	3.087	3.183	3.334	3.003	9.09
87)	T	1,3-Dichlorobe...	1.667	1.698	1.718	1.657	1.701	1.794	1.706	2.85
88)	T	1,4-Dichlorobe...	1.703	1.703	1.694	1.624	1.653	1.732	1.685	2.33
89)	T	n-Butylbenzene	2.279	2.428	2.626	2.682	2.778	2.904	2.616	8.76
90)	T	Hexachloroethane	0.667	0.631	0.647	0.625	0.643	0.662	0.646	2.54
91)	T	1,2-Dichlorobe...	1.485	1.498	1.511	1.446	1.490	1.543	1.496	2.13
92)	T	1,2-Dibromo-3-...	0.087	0.093	0.083	0.083	0.088	0.096	0.088	6.18
93)	T	1,2,4-Trichlor...	0.846	0.867	0.901	0.918	1.007	1.054	0.932	8.75
94)	T	Hexachlorobuta...	0.590	0.571	0.572	0.577	0.587	0.590	0.581	1.52
95)	T	Naphthalene	1.206	1.281	1.346	1.466	1.722	1.887	1.485	17.98
96)	T	1,2,3-Trichlor...	0.719	0.753	0.795	0.793	0.866	0.920	0.808	9.14

(#) = Out of Range

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
 Data File : VY023384.D
 Acq On : 07 Oct 2025 09:17
 Operator : SY/MD
 Sample : VSTDICC005
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICC005

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025
 Supervised By :Mahesh Dadoda 10/10/2025

Quant Time: Oct 08 04:39:47 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 04:39:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	585717	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.615	114	882488	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	753398	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	378104	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	26670	5.258	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery =	10.520%#		
35) Dibromofluoromethane	7.634	113	27455	5.126	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery =	10.260%#		
50) Toluene-d8	10.103	98	99905	4.946	ug/l	0.00
Spiked Amount 50.000	Range 58 - 134		Recovery =	9.900%#		
62) 4-Bromofluorobenzene	12.401	95	35355	5.548	ug/l	0.00
Spiked Amount 50.000	Range 30 - 143		Recovery =	11.100%#		
Target Compounds					Qvalue	
2) Dichlorodifluoromethane	1.867	85	23245	5.038	ug/l	92
3) Chloromethane	2.074	50	30346	4.627	ug/l	94
4) Vinyl Chloride	2.202	62	38657	4.668	ug/l	95
5) Bromomethane	2.598	94	35214	5.184	ug/l	94
6) Chloroethane	2.732	64	25848	4.597	ug/l	98
7) Trichlorofluoromethane	3.055	101	51797	4.869	ug/l	98
8) Diethyl Ether	3.452	74	14079	5.060	ug/l	96
9) 1,1,2-Trichlorotrifluo...	3.818	101	28368	4.989	ug/l	99
10) Methyl Iodide	4.007	142	23692	3.606	ug/l	99
11) Tert butyl alcohol	4.854	59	9774	32.746	ug/l #	80
12) 1,1-Dichloroethene	3.787	96	26290	4.806	ug/l	94
13) Acrolein	3.653	56	13176	26.054	ug/l	100
14) Allyl chloride	4.385	41	31614	4.616	ug/l	98
15) Acrylonitrile	5.055	53	25891	23.754	ug/l	99
16) Acetone	3.866	43	37573	32.940	ug/l	96
17) Carbon Disulfide	4.104	76	75645	4.432	ug/l	99
18) Methyl Acetate	4.391	43	14279	4.926	ug/l	98
19) Methyl tert-butyl Ether	5.116	73	58919	4.600	ug/l	95
20) Methylene Chloride	4.616	84	36598	5.917	ug/l	100
21) trans-1,2-Dichloroethene	5.110	96	28923	4.754	ug/l	99
22) Diisopropyl ether	6.018	45	64833	4.269	ug/l	94
23) Vinyl Acetate	5.964	43	173851	20.824	ug/l	99
24) 1,1-Dichloroethane	5.909	63	46850	4.679	ug/l	100
25) 2-Butanone	6.890	43	38990	27.656	ug/l	93
26) 2,2-Dichloropropane	6.884	77	44062	4.953	ug/l	98
27) cis-1,2-Dichloroethene	6.884	96	31743	4.600	ug/l	98
28) Bromochloromethane	7.244	49	19445	5.006	ug/l	99
29) Tetrahydrofuran	7.262	42	19296	23.059	ug/l	98
30) Chloroform	7.421	83	51887	4.806	ug/l	97
31) Cyclohexane	7.707	56	46675	5.279	ug/l #	79
32) 1,1,1-Trichloroethane	7.616	97	47305	4.881	ug/l	99
36) 1,1-Dichloropropene	7.835	75	34888	4.617	ug/l	98
37) Ethyl Acetate	6.982	43	13082	4.379	ug/l #	93
38) Carbon Tetrachloride	7.817	117	42654	4.859	ug/l	95
39) Methylcyclohexane	9.109	83	43329	4.479	ug/l	98
40) Benzene	8.079	78	110551	4.693	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
 Data File : VY023384.D
 Acq On : 07 Oct 2025 09:17
 Operator : SY/MD
 Sample : VSTDICC005
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICC005

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025
 Supervised By :Mahesh Dadoda 10/10/2025

Quant Time: Oct 08 04:39:47 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 04:39:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	7.225	41	7226m	4.658	ug/l	
42) 1,2-Dichloroethane	8.158	62	28940	4.828	ug/l	100
43) Isopropyl Acetate	8.201	43	26166	4.503	ug/l	99
44) Trichloroethene	8.859	130	33564	5.077	ug/l	99
45) 1,2-Dichloropropane	9.140	63	24358	4.595	ug/l	92
46) Dibromomethane	9.231	93	15179	4.682	ug/l	97
47) Bromodichloromethane	9.420	83	38813	4.756	ug/l	93
48) Methyl methacrylate	9.219	41	11038	4.071	ug/l	98
49) 1,4-Dioxane	9.219	88	3255	96.953	ug/l #	86
51) 4-Methyl-2-Pentanone	9.999	43	62279	20.925	ug/l	98
52) Toluene	10.170	92	68550	4.585	ug/l	99
53) t-1,3-Dichloropropene	10.396	75	31477	4.491	ug/l	99
54) cis-1,3-Dichloropropene	9.853	75	37392	4.463	ug/l	96
55) 1,1,2-Trichloroethane	10.572	97	20641	4.786	ug/l	97
56) Ethyl methacrylate	10.438	69	19324	3.891	ug/l	94
57) 1,3-Dichloropropane	10.719	76	31831	4.560	ug/l	96
58) 2-Chloroethyl Vinyl ether	9.713	63	41054m	18.894	ug/l	
59) 2-Hexanone	10.761	43	47778	23.185	ug/l	97
60) Dibromochloromethane	10.908	129	28135	4.783	ug/l	97
61) 1,2-Dibromoethane	11.017	107	18957	4.673	ug/l	97
64) Tetrachloroethene	10.646	164	40570	5.383	ug/l	98
65) Chlorobenzene	11.444	112	81802	4.997	ug/l	98
66) 1,1,1,2-Tetrachloroethane	11.517	131	29222	5.075	ug/l	97
67) Ethyl Benzene	11.517	91	121005	4.529	ug/l	99
68) m/p-Xylenes	11.633	106	95176	8.887	ug/l	100
69) o-Xylene	11.956	106	44280	4.466	ug/l	98
70) Styrene	11.969	104	67960	4.152	ug/l	99
71) Bromoform	12.133	173	16988	4.929	ug/l #	99
73) Isopropylbenzene	12.255	105	112194	4.455	ug/l	99
74) N-amyl acetate	12.066	43	18041	3.833	ug/l #	96
75) 1,1,2,2-Tetrachloroethane	12.505	83	20052	4.773	ug/l	100
76) 1,2,3-Trichloropropane	12.554	75	15359m	4.118	ug/l	
77) Bromobenzene	12.529	156	32106	4.967	ug/l	99
78) n-propylbenzene	12.596	91	127521	4.305	ug/l	99
79) 2-Chlorotoluene	12.676	91	79199	4.631	ug/l	99
80) 1,3,5-Trimethylbenzene	12.737	105	87297	4.264	ug/l	100
81) trans-1,4-Dichloro-2-b...	12.304	75	6474	4.680	ug/l	98
82) 4-Chlorotoluene	12.779	91	82155	4.600	ug/l	100
83) tert-Butylbenzene	12.999	119	83151	4.457	ug/l	100
84) 1,2,4-Trimethylbenzene	13.042	105	86988	4.294	ug/l	99
85) sec-Butylbenzene	13.176	105	120061	4.443	ug/l	99
86) p-Isopropyltoluene	13.291	119	97377	4.264	ug/l	99
87) 1,3-Dichlorobenzene	13.285	146	63027	4.936	ug/l	100
88) 1,4-Dichlorobenzene	13.365	146	64389	5.085	ug/l	95
89) n-Butylbenzene	13.615	91	86179	4.274	ug/l	99
90) Hexachloroethane	13.877	117	25204	5.084	ug/l	97
91) 1,2-Dichlorobenzene	13.657	146	56167	5.041	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	14.273	75	3305	4.964	ug/l	95
93) 1,2,4-Trichlorobenzene	14.919	180	32000	4.875	ug/l	99
94) Hexachlorobutadiene	15.023	225	22316	5.456	ug/l	99
95) Naphthalene	15.145	128	45598	4.360	ug/l	99
96) 1,2,3-Trichlorobenzene	15.328	180	27176	4.772	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
Data File : VY023384.D
Acq On : 07 Oct 2025 09:17
Operator : SY/MD
Sample : VSTDICC005
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICC005

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025
Supervised By :Mahesh Dadoda 10/10/2025

Quant Time: Oct 08 04:39:47 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 04:39:16 2025
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICC005

Manual Integrations

Reviewed By :Semsettin Yesilyurt 10/10/2025
Supervised By :Mahesh Dadoda 10/10/2025

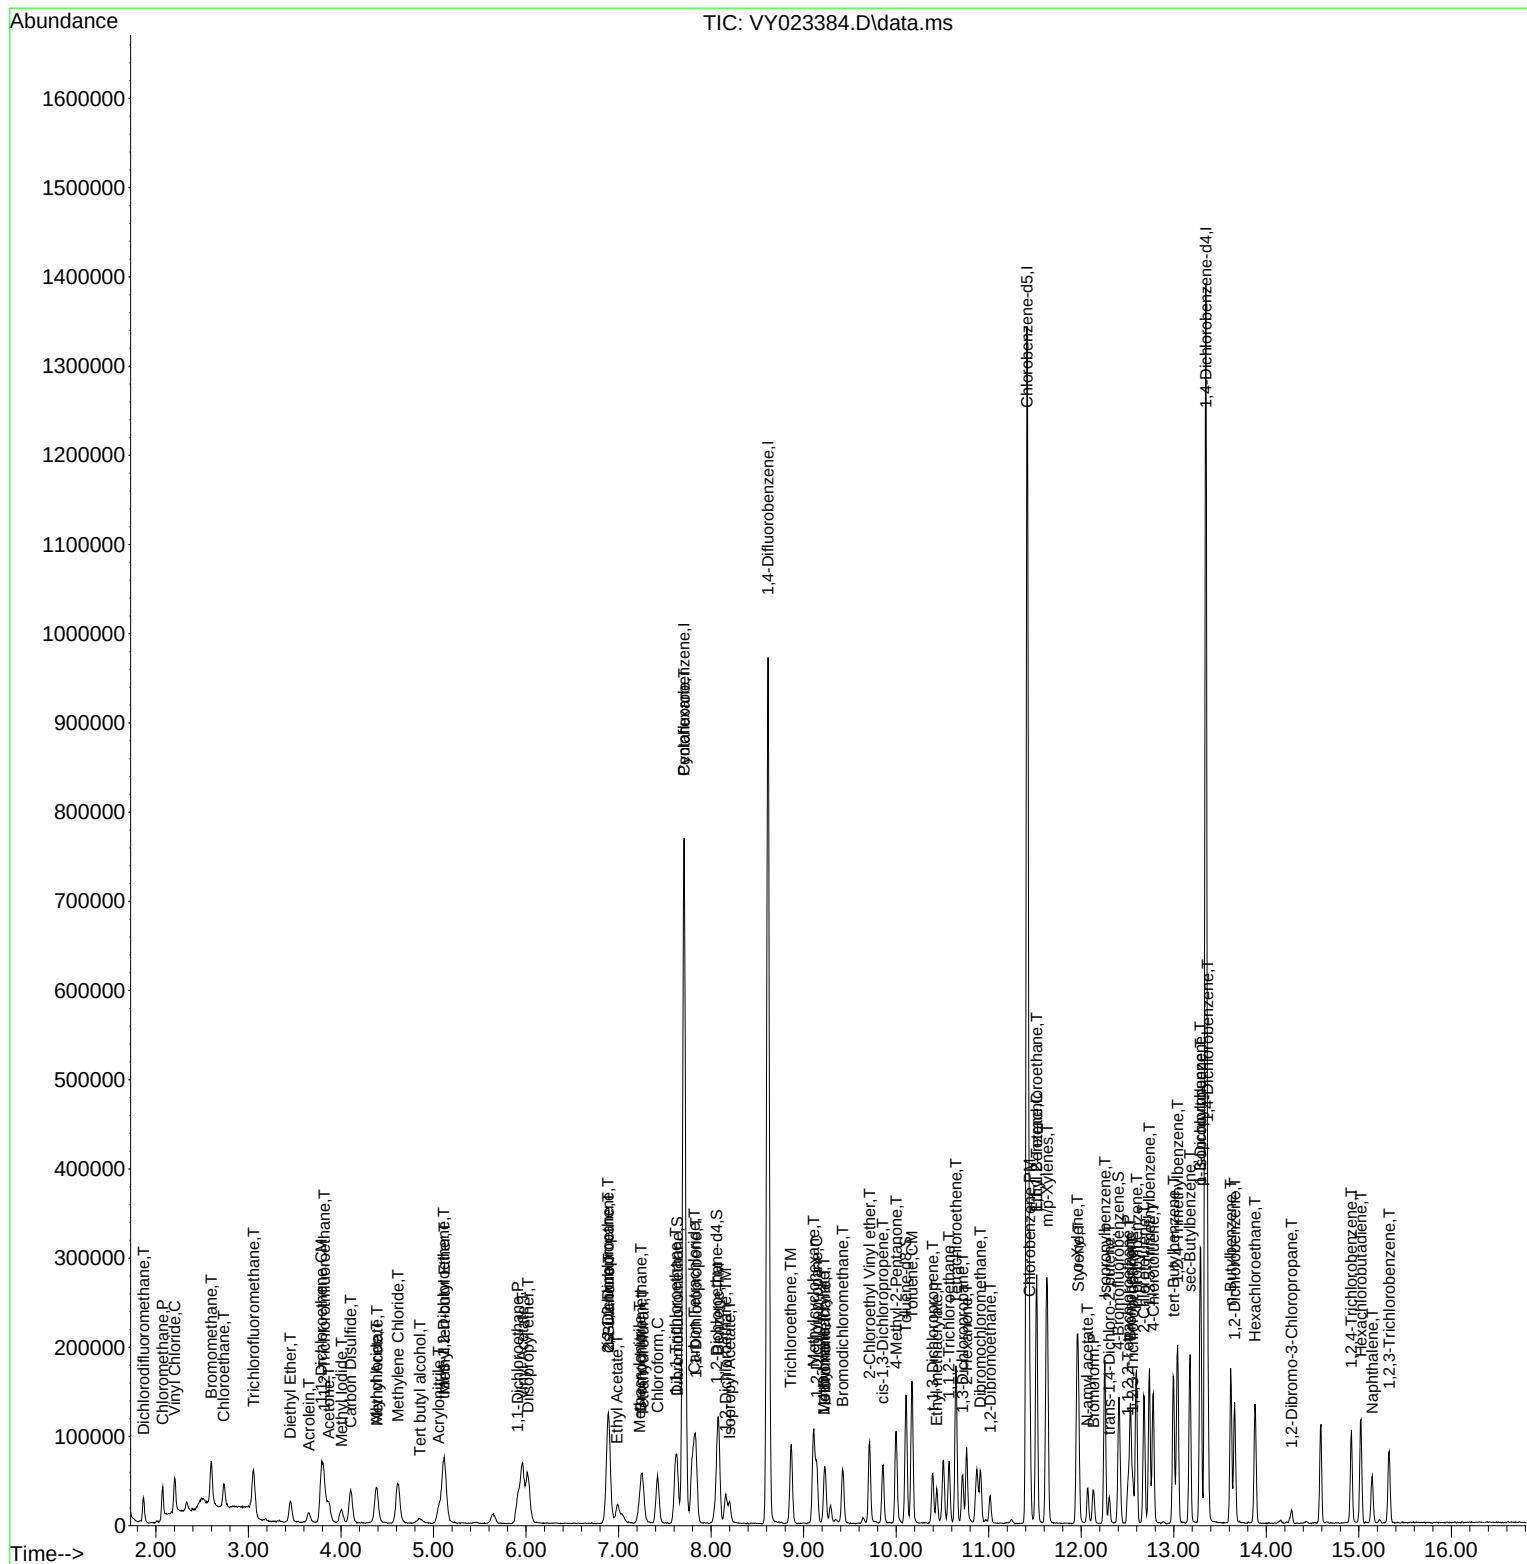

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
 Data File : VY023385.D
 Acq On : 07 Oct 2025 10:02
 Operator : SY/MD
 Sample : VSTDICC010
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICC010

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025
 Supervised By :Mahesh Dadoda 10/10/2025

Quant Time: Oct 08 04:40:53 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 04:39:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.713	168	559828	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.615	114	847077	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	736152	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	374998	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.067	65	48826	10.071	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery =	20.140%#		
35) Dibromofluoromethane	7.634	113	53279	10.364	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery =	20.720%#		
50) Toluene-d8	10.109	98	198242	10.225	ug/l	0.00
Spiked Amount 50.000	Range 58 - 134		Recovery =	20.460%#		
62) 4-Bromofluorobenzene	12.401	95	62601	10.235	ug/l	0.00
Spiked Amount 50.000	Range 30 - 143		Recovery =	20.460%#		
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.867	85	44666	10.129	ug/l	97
3) Chloromethane	2.068	50	62413	9.957	ug/l	97
4) Vinyl Chloride	2.202	62	76587	9.676	ug/l	99
5) Bromomethane	2.592	94	66689	10.271	ug/l	90
6) Chloroethane	2.732	64	51757	9.632	ug/l	92
7) Trichlorofluoromethane	3.055	101	102972	10.128	ug/l	99
8) Diethyl Ether	3.458	74	26719	10.047	ug/l	96
9) 1,1,2-Trichlorotrifluo...	3.818	101	54405	10.011	ug/l	99
10) Methyl Iodide	4.007	142	56313	8.967	ug/l	99
11) Tert butyl alcohol	4.854	59	20540	71.998	ug/l #	89
12) 1,1-Dichloroethene	3.793	96	53191	10.173	ug/l	98
13) Acrolein	3.653	56	24014	49.681	ug/l	94
14) Allyl chloride	4.385	41	62154	9.494	ug/l	99
15) Acrylonitrile	5.061	53	51937	49.854	ug/l	99
16) Acetone	3.872	43	65410	59.997	ug/l	94
17) Carbon Disulfide	4.104	76	153055	9.382	ug/l	100
18) Methyl Acetate	4.391	43	29725	10.728	ug/l	100
19) Methyl tert-butyl Ether	5.116	73	120347	9.830	ug/l	100
20) Methylene Chloride	4.616	84	71034	12.016	ug/l	96
21) trans-1,2-Dichloroethene	5.116	96	56465	9.710	ug/l	97
22) Diisopropyl ether	6.024	45	138589	9.547	ug/l	98
23) Vinyl Acetate	5.963	43	361478	45.300	ug/l	99
24) 1,1-Dichloroethane	5.915	63	93512	9.772	ug/l	98
25) 2-Butanone	6.890	43	75171	55.784	ug/l	92
26) 2,2-Dichloropropane	6.890	77	86325	10.153	ug/l	99
27) cis-1,2-Dichloroethene	6.896	96	65335	9.905	ug/l	99
28) Bromochloromethane	7.244	49	36132	9.733	ug/l	99
29) Tetrahydrofuran	7.262	42	38990	48.749	ug/l	99
30) Chloroform	7.421	83	102058	9.890	ug/l	99
31) Cyclohexane	7.701	56	80245	9.495	ug/l #	88
32) 1,1,1-Trichloroethane	7.622	97	91186	9.844	ug/l	99
36) 1,1-Dichloropropene	7.835	75	69913	9.639	ug/l	99
37) Ethyl Acetate	6.988	43	27388	9.551	ug/l	96
38) Carbon Tetrachloride	7.817	117	84799	10.065	ug/l	99
39) Methylcyclohexane	9.109	83	82275	8.860	ug/l	95
40) Benzene	8.079	78	220629	9.758	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
 Data File : VY023385.D
 Acq On : 07 Oct 2025 10:02
 Operator : SY/MD
 Sample : VSTDICC010
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICC010

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025
 Supervised By :Mahesh Dadoda 10/10/2025

Quant Time: Oct 08 04:40:53 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 04:39:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	7.225	41	14344	9.632	ug/l #	92
42) 1,2-Dichloroethane	8.158	62	58541	10.174	ug/l	99
43) Isopropyl Acetate	8.201	43	53042	9.510	ug/l	98
44) Trichloroethene	8.865	130	64537	10.171	ug/l	96
45) 1,2-Dichloropropane	9.140	63	49009	9.632	ug/l	100
46) Dibromomethane	9.231	93	30780	9.890	ug/l	99
47) Bromodichloromethane	9.426	83	78392	10.007	ug/l	99
48) Methyl methacrylate	9.225	41	23484	9.023	ug/l	97
49) 1,4-Dioxane	9.231	88	6822	211.693	ug/l	94
51) 4-Methyl-2-Pentanone	9.999	43	134746	47.165	ug/l	99
52) Toluene	10.170	92	138662	9.661	ug/l	100
53) t-1,3-Dichloropropene	10.396	75	64315	9.559	ug/l	96
54) cis-1,3-Dichloropropene	9.853	75	77905	9.687	ug/l	98
55) 1,1,2-Trichloroethane	10.572	97	41881	10.118	ug/l	92
56) Ethyl methacrylate	10.438	69	42096	8.830	ug/l	98
57) 1,3-Dichloropropane	10.719	76	64537	9.633	ug/l	98
58) 2-Chloroethyl Vinyl ether	9.713	63	94970m	45.535	ug/l	
59) 2-Hexanone	10.761	43	99175	50.138	ug/l	96
60) Dibromochloromethane	10.908	129	57151	10.123	ug/l	97
61) 1,2-Dibromoethane	11.011	107	38861	9.979	ug/l	99
64) Tetrachloroethene	10.646	164	76110	10.335	ug/l	98
65) Chlorobenzene	11.438	112	161155	10.074	ug/l	96
66) 1,1,1,2-Tetrachloroethane	11.517	131	57233	10.173	ug/l	98
67) Ethyl Benzene	11.517	91	251958	9.651	ug/l	98
68) m/p-Xylenes	11.627	106	198866	19.004	ug/l	99
69) o-Xylene	11.950	106	91710	9.467	ug/l	100
70) Styrene	11.969	104	151094	9.446	ug/l	99
71) Bromoform	12.133	173	35681	10.595	ug/l #	94
73) Isopropylbenzene	12.249	105	236489	9.467	ug/l	99
74) N-amyl acetate	12.066	43	40098	8.590	ug/l	97
75) 1,1,2,2-Tetrachloroethane	12.505	83	41130	9.871	ug/l	97
76) 1,2,3-Trichloropropane	12.554	75	29944m	8.095	ug/l	
77) Bromobenzene	12.529	156	66002	10.295	ug/l	99
78) n-propylbenzene	12.590	91	275671	9.384	ug/l	100
79) 2-Chlorotoluene	12.676	91	165582	9.762	ug/l	100
80) 1,3,5-Trimethylbenzene	12.731	105	191799	9.445	ug/l	100
81) trans-1,4-Dichloro-2-b...	12.298	75	13110	9.556	ug/l	99
82) 4-Chlorotoluene	12.773	91	169968	9.595	ug/l	100
83) tert-Butylbenzene	12.993	119	177250	9.579	ug/l	99
84) 1,2,4-Trimethylbenzene	13.041	105	191423	9.528	ug/l	98
85) sec-Butylbenzene	13.170	105	254134	9.483	ug/l	100
86) p-Isopropyltoluene	13.285	119	210320	9.287	ug/l	100
87) 1,3-Dichlorobenzene	13.285	146	127377	10.058	ug/l	99
88) 1,4-Dichlorobenzene	13.365	146	127757	10.172	ug/l	98
89) n-Butylbenzene	13.615	91	182116	9.107	ug/l	98
90) Hexachloroethane	13.877	117	47355	9.630	ug/l	97
91) 1,2-Dichlorobenzene	13.657	146	112325	10.165	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	14.273	75	7005	10.608	ug/l	94
93) 1,2,4-Trichlorobenzene	14.919	180	65050	9.992	ug/l	98
94) Hexachlorobutadiene	15.023	225	42813	10.554	ug/l	97
95) Naphthalene	15.139	128	96092	9.264	ug/l	99
96) 1,2,3-Trichlorobenzene	15.328	180	56499	10.004	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
Data File : VY023385.D
Acq On : 07 Oct 2025 10:02
Operator : SY/MD
Sample : VSTDICC010
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICC010

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025
Supervised By :Mahesh Dadoda 10/10/2025

Quant Time: Oct 08 04:40:53 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 04:39:16 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICC010

Manual Integrations APPROVED

Abundance

TIC: VY023385.D\data.ms

Time-->

2.00 3.00 4.00 5.00 6.00 7.00 8.00 9.00 10.00 11.00 12.00 13.00 14.00 15.00 16.00

1600000

1500000

1400000

1300000

1200000

1100000

1000000

900000

800000

700000

600000

500000

400000

300000

200000

100000

0

Dichlorodifluoromethane, T

Chloromethane, P

Vinyl Chloride, C

Bromomethane, T

Chloroethane, T

Trichlorofluoromethane, T

Diethyl Ether, T

Acrolein, T

1,1,2,2-Tetrachloroethane, T

Acetone, T

Methylsulfoxide, T

Methylacetate, T

Methylene Chloride, T

Tert butyl alcohol, T

Acrylonitrile, T

1,2-Dichloroethane, T

1,1-Dichloroethane, T

Diisopropyl ether, T

Ethyl Acetate, T

Methoxybenzene, T

Chloroform, C

1,2-Dichlorobenzene, S

Carbon disulfide, T

Isopropyl acetate, T

1,2-Dichloroethane, T

1,4-Difluorobenzene, I

1,4-Difluorobenzene, I

Trichloroethene, TM

1,2-Dichlorobenzene, T

Bromodichloromethane, T

2-Chloroethyl Vinyl ether, T

cis-1,3-Dichloropropene, T

4-Methylpentan-2-one, T

1,2-Dichloroethane, T

Ethyl hexachlorocyclopentene, T

1,3-Dichlorobenzene, T

Dibromochloromethane, T

1,2-Dibromoethane, T

Chlorobenzene, PM

Ethyl hexachlorocyclopentane, T

m-Xylenes, T

Isopropyl acetate, T

trans-1,4-Dichloro-2-butene, T

trans-1,4-Dichloro-2-butene, S

1,2-Dichlorobenzene, T

1,2-Dichlorobenzene, T

2-Chlorobenzonitrile, T

tert-Butyl peroxide, T

sec-Butylbenzene, T

1,4-Dichlorobenzene, T

1,2-Dichlorobenzene, T

Hexachloroethane, T

1,2-Dibromo-3-Chloropropane, T

1,2,4-Trichlorobenzene, T

Naphthalene, T

1,2,3-Trichlorobenzene, T

1,4-Dichlorobenzene-d4, I

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
 Data File : VY023386.D
 Acq On : 07 Oct 2025 11:24
 Operator : SY/MD
 Sample : VSTDICC020
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICC020

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025
 Supervised By :Mahesh Dadoda 10/10/2025

Quant Time: Oct 08 04:41:57 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 04:39:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	574363	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.615	114	851961	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	746872	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	382604	50.000	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	8.061	65	98481	19.798	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	39.600%#
35) Dibromofluoromethane	7.634	113	108034	20.895	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	41.800%#
50) Toluene-d8	10.103	98	401067	20.568	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	41.140%#
62) 4-Bromofluorobenzene	12.401	95	127216	20.680	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	41.360%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.867	85	91924	20.318	ug/l	98
3) Chloromethane	2.074	50	117585	18.284	ug/l	100
4) Vinyl Chloride	2.202	62	151460	18.652	ug/l	99
5) Bromomethane	2.586	94	125948	18.907	ug/l	97
6) Chloroethane	2.732	64	103973	18.859	ug/l	94
7) Trichlorofluoromethane	3.049	101	217452	20.846	ug/l	99
8) Diethyl Ether	3.452	74	54124	19.837	ug/l	99
9) 1,1,2-Trichlorotrifluo...	3.811	101	109936	19.718	ug/l	99
10) Methyl Iodide	4.007	142	119083	18.482	ug/l	99
11) Tert butyl alcohol	4.854	59	34346	117.345	ug/l	98
12) 1,1-Dichloroethene	3.787	96	104778	19.531	ug/l	98
13) Acrolein	3.653	56	48115	97.023	ug/l	98
14) Allyl chloride	4.384	41	125424	18.674	ug/l	98
15) Acrylonitrile	5.055	53	99018	92.641	ug/l	100
16) Acetone	3.866	43	108209	96.742	ug/l	96
17) Carbon Disulfide	4.104	76	303284	18.121	ug/l	99
18) Methyl Acetate	4.384	43	59704	21.002	ug/l	97
19) Methyl tert-butyl Ether	5.116	73	247030	19.667	ug/l	97
20) Methylene Chloride	4.616	84	132229	21.801	ug/l	98
21) trans-1,2-Dichloroethene	5.110	96	116410	19.512	ug/l	95
22) Diisopropyl ether	6.018	45	288429	19.366	ug/l	98
23) Vinyl Acetate	5.957	43	748048	91.373	ug/l	99
24) 1,1-Dichloroethane	5.915	63	190012	19.354	ug/l	99
25) 2-Butanone	6.896	43	132159	95.593	ug/l	93
26) 2,2-Dichloropropane	6.884	77	167903	19.247	ug/l	99
27) cis-1,2-Dichloroethene	6.890	96	133634	19.747	ug/l	99
28) Bromochloromethane	7.244	49	73407	19.273	ug/l	98
29) Tetrahydrofuran	7.262	42	76502	93.229	ug/l	99
30) Chloroform	7.421	83	207096	19.562	ug/l	100
31) Cyclohexane	7.701	56	160159	18.472	ug/l	97
32) 1,1,1-Trichloroethane	7.616	97	188861	19.873	ug/l	100
36) 1,1-Dichloropropene	7.835	75	140912	19.317	ug/l	100
37) Ethyl Acetate	6.982	43	55705	19.315	ug/l	98
38) Carbon Tetrachloride	7.817	117	171925	20.289	ug/l	99
39) Methylcyclohexane	9.109	83	182831	19.576	ug/l	99
40) Benzene	8.079	78	450471	19.809	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
 Data File : VY023386.D
 Acq On : 07 Oct 2025 11:24
 Operator : SY/MD
 Sample : VSTDICC020
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :

MSVOA_Y

ClientSampleId :

VSTDICC020

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025

Supervised By :Mahesh Dadoda 10/10/2025

Quant Time: Oct 08 04:41:57 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M

Quant Title : SW846 8260

QLast Update : Wed Oct 08 04:39:16 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	7.225	41	31129m	20.783	ug/l	
42) 1,2-Dichloroethane	8.158	62	116941	20.206	ug/l	99
43) Isopropyl Acetate	8.195	43	106595	19.002	ug/l #	87
44) Trichloroethene	8.865	130	131459	20.598	ug/l	98
45) 1,2-Dichloropropane	9.140	63	99363	19.417	ug/l	98
46) Dibromomethane	9.231	93	62277	19.896	ug/l	98
47) Bromodichloromethane	9.420	83	156426	19.854	ug/l	98
48) Methyl methacrylate	9.219	41	50661	19.352	ug/l	99
49) 1,4-Dioxane	9.225	88	13636	420.712	ug/l	99
51) 4-Methyl-2-Pentanone	9.999	43	274059	95.378	ug/l	100
52) Toluene	10.170	92	291453	20.191	ug/l	100
53) t-1,3-Dichloropropene	10.390	75	132848	19.632	ug/l	99
54) cis-1,3-Dichloropropene	9.853	75	158580	19.606	ug/l	95
55) 1,1,2-Trichloroethane	10.572	97	82183	19.740	ug/l	96
56) Ethyl methacrylate	10.438	69	89244	18.613	ug/l	99
57) 1,3-Dichloropropane	10.719	76	130650	19.389	ug/l	98
58) 2-Chloroethyl Vinyl ether	9.713	63	190850m	90.982	ug/l	
59) 2-Hexanone	10.761	43	187387	94.190	ug/l	99
60) Dibromochloromethane	10.908	129	115907	20.412	ug/l	100
61) 1,2-Dibromoethane	11.011	107	78579	20.062	ug/l	100
64) Tetrachloroethene	10.646	164	167648	22.438	ug/l	97
65) Chlorobenzene	11.438	112	326360	20.109	ug/l	99
66) 1,1,1,2-Tetrachloroethane	11.517	131	116412	20.396	ug/l	99
67) Ethyl Benzene	11.517	91	523606	19.768	ug/l	99
68) m/p-Xylenes	11.627	106	426913	40.211	ug/l	100
69) o-Xylene	11.956	106	195021	19.843	ug/l	96
70) Styrene	11.968	104	327934	20.208	ug/l	99
71) Bromoform	12.133	173	71119	20.814	ug/l #	99
73) Isopropylbenzene	12.255	105	513183	20.136	ug/l	99
74) N-amyl acetate	12.072	43	85063	17.860	ug/l	98
75) 1,1,2,2-Tetrachloroethane	12.505	83	76821	18.069	ug/l	99
76) 1,2,3-Trichloropropane	12.554	75	74100m	19.634	ug/l	
77) Bromobenzene	12.529	156	135402	20.700	ug/l	98
78) n-propylbenzene	12.596	91	597829	19.945	ug/l	100
79) 2-Chlorotoluene	12.676	91	349203	20.179	ug/l	100
80) 1,3,5-Trimethylbenzene	12.737	105	418684	20.208	ug/l	100
81) trans-1,4-Dichloro-2-b...	12.304	75	26922	19.234	ug/l	98
82) 4-Chlorotoluene	12.773	91	361458	20.000	ug/l	99
83) tert-Butylbenzene	12.993	119	377277	19.983	ug/l	99
84) 1,2,4-Trimethylbenzene	13.041	105	413292	20.162	ug/l	100
85) sec-Butylbenzene	13.176	105	546582	19.990	ug/l	100
86) p-Isopropyltoluene	13.291	119	464005	20.081	ug/l	100
87) 1,3-Dichlorobenzene	13.285	146	262901	20.347	ug/l	99
88) 1,4-Dichlorobenzene	13.365	146	259217	20.230	ug/l	99
89) n-Butylbenzene	13.615	91	401893	19.697	ug/l	98
90) Hexachloroethane	13.877	117	98983	19.730	ug/l	97
91) 1,2-Dichlorobenzene	13.657	146	231199	20.507	ug/l	100
92) 1,2-Dibromo-3-Chloropr...	14.273	75	12668	18.802	ug/l	99
93) 1,2,4-Trichlorobenzene	14.919	180	137963	20.770	ug/l	99
94) Hexachlorobutadiene	15.023	225	87575	21.159	ug/l	99
95) Naphthalene	15.145	128	206017	19.467	ug/l	100
96) 1,2,3-Trichlorobenzene	15.328	180	121656	21.113	ug/l	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
Data File : VY023386.D
Acq On : 07 Oct 2025 11:24
Operator : SY/MD
Sample : VSTDICC020
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICC020

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025
Supervised By :Mahesh Dadoda 10/10/2025

Quant Time: Oct 08 04:41:57 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 04:39:16 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed



```
Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
Data File : VY023386.D
Acq On    : 07 Oct 2025  11:24
Operator  : SY/MD
Sample    : VSTDIC020
Misc      : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial  : 5      Sample Multiplier: 1
```

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICC020

Quant Time: Oct 08 04:41:57 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 04:39:16 2025
Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025
Supervised By :Mahesh Dadoda 10/10/2025

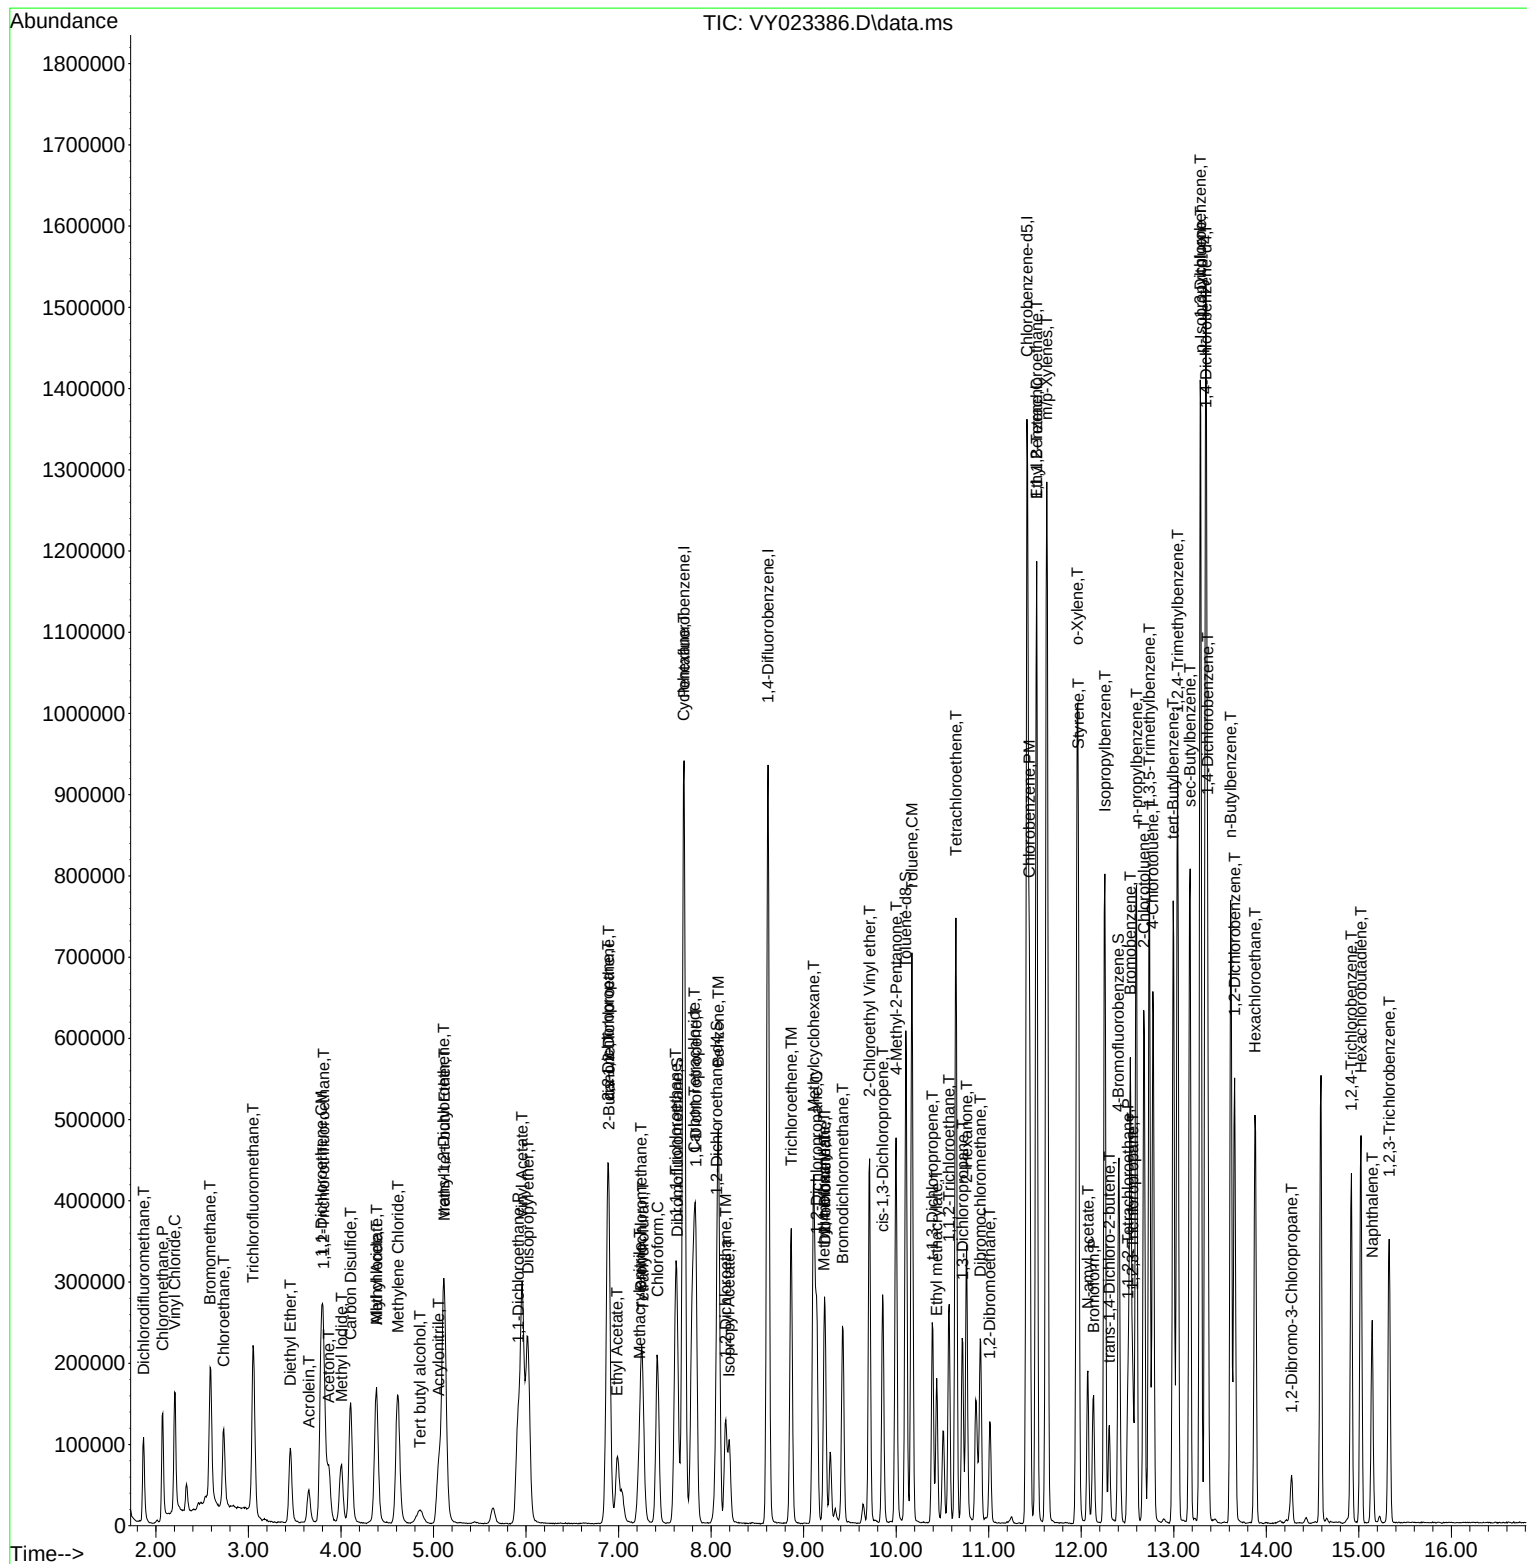

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
 Data File : VY023387.D
 Acq On : 07 Oct 2025 11:47
 Operator : SY/MD
 Sample : VSTDICCC050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICCC050

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025
 Supervised By :Mahesh Dadoda 10/10/2025

Quant Time: Oct 08 04:43:02 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 04:39:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	590340	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	858767	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	749869	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	392169	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	231295	45.240	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery =	90.480%		
35) Dibromofluoromethane	7.634	113	256331	49.185	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery =	98.360%		
50) Toluene-d8	10.103	98	969649	49.334	ug/l	0.00
Spiked Amount 50.000	Range 58 - 134		Recovery =	98.660%		
62) 4-Bromofluorobenzene	12.402	95	313426	50.546	ug/l	0.00
Spiked Amount 50.000	Range 30 - 143		Recovery =	101.100%		
Target Compounds					Qvalue	
2) Dichlorodifluoromethane	1.867	85	189467	40.745	ug/l	100
3) Chloromethane	2.068	50	265142	40.113	ug/l	100
4) Vinyl Chloride	2.202	62	352993	42.293	ug/l	100
5) Bromomethane	2.592	94	277005	40.458	ug/l	100
6) Chloroethane	2.733	64	244551	43.157	ug/l	100
7) Trichlorofluoromethane	3.056	101	496981	46.354	ug/l	100
8) Diethyl Ether	3.452	74	126634	45.158	ug/l	100
9) 1,1,2-Trichlorotrifluo...	3.812	101	258100	45.039	ug/l	100
10) Methyl Iodide	4.001	142	317731	47.979	ug/l	100
11) Tert butyl alcohol	4.860	59	73642	244.793	ug/l	100
12) 1,1-Dichloroethene	3.787	96	252190	45.738	ug/l	100
13) Acrolein	3.647	56	123642	242.575	ug/l	100
14) Allyl chloride	4.379	41	310569	44.989	ug/l	100
15) Acrylonitrile	5.055	53	240668	219.075	ug/l	100
16) Acetone	3.866	43	247122	214.955	ug/l	100
17) Carbon Disulfide	4.104	76	722982	42.028	ug/l	100
18) Methyl Acetate	4.385	43	144816	49.563	ug/l	100
19) Methyl tert-butyl Ether	5.116	73	601934	46.626	ug/l	100
20) Methylene Chloride	4.616	84	270612	43.409	ug/l	100
21) trans-1,2-Dichloroethene	5.110	96	277516	45.256	ug/l	100
22) Diisopropyl ether	6.019	45	686481	44.844	ug/l	100
23) Vinyl Acetate	5.958	43	1843784	219.119	ug/l	100
24) 1,1-Dichloroethane	5.915	63	448267	44.423	ug/l	100
25) 2-Butanone	6.890	43	310237	218.327	ug/l	100
26) 2,2-Dichloropropane	6.884	77	416391	46.440	ug/l	100
27) cis-1,2-Dichloroethene	6.890	96	320028	46.010	ug/l	100
28) Bromochloromethane	7.244	49	157414	40.211	ug/l	100
29) Tetrahydrofuran	7.262	42	187787	222.653	ug/l	100
30) Chloroform	7.421	83	493098	45.316	ug/l	100
31) Cyclohexane	7.701	56	379644	42.602	ug/l	100
32) 1,1,1-Trichloroethane	7.616	97	452713	46.347	ug/l	100
36) 1,1-Dichloropropene	7.835	75	341353	46.424	ug/l	100
37) Ethyl Acetate	6.982	43	129053	44.394	ug/l	100
38) Carbon Tetrachloride	7.817	117	413187	48.374	ug/l	100
39) Methylcyclohexane	9.109	83	452959	48.113	ug/l	100
40) Benzene	8.079	78	1080883	47.154	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
 Data File : VY023387.D
 Acq On : 07 Oct 2025 11:47
 Operator : SY/MD
 Sample : VSTDICCC050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICCC050

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025
 Supervised By :Mahesh Dadoda 10/10/2025

Quant Time: Oct 08 04:43:02 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 04:39:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	7.220	41	68542	45.399	ug/l	100
42) 1,2-Dichloroethane	8.152	62	270387	46.350	ug/l	100
43) Isopropyl Acetate	8.195	43	259041	45.811	ug/l	100
44) Trichloroethene	8.866	130	315104	48.982	ug/l	100
45) 1,2-Dichloropropane	9.140	63	234978	45.555	ug/l	100
46) Dibromomethane	9.231	93	148914	47.198	ug/l	100
47) Bromodichloromethane	9.420	83	377084	47.482	ug/l	100
48) Methyl methacrylate	9.219	41	126732	48.027	ug/l	100
49) 1,4-Dioxane	9.225	88	34053	1042.312	ug/l	100
51) 4-Methyl-2-Pentanone	9.993	43	682879	235.772	ug/l	100
52) Toluene	10.170	92	710404	48.824	ug/l	100
53) t-1,3-Dichloropropene	10.390	75	330392	48.438	ug/l	100
54) cis-1,3-Dichloropropene	9.853	75	390619	47.910	ug/l	100
55) 1,1,2-Trichloroethane	10.573	97	198478	47.296	ug/l	100
56) Ethyl methacrylate	10.438	69	239407	49.535	ug/l	100
57) 1,3-Dichloropropane	10.713	76	321276	47.301	ug/l	100
58) 2-Chloroethyl Vinyl ether	9.707	63	553816	261.921	ug/l	100
59) 2-Hexanone	10.756	43	479606	239.162	ug/l	100
60) Dibromochloromethane	10.908	129	281047	49.103	ug/l	100
61) 1,2-Dibromoethane	11.012	107	191356	48.468	ug/l	100
64) Tetrachloroethene	10.646	164	392056	52.264	ug/l	100
65) Chlorobenzene	11.438	112	789650	48.460	ug/l	100
66) 1,1,1,2-Tetrachloroethane	11.511	131	279583	48.788	ug/l	100
67) Ethyl Benzene	11.518	91	1332350	50.099	ug/l	100
68) m/p-Xylenes	11.627	106	1077583	101.092	ug/l	100
69) o-Xylene	11.950	106	502722	50.946	ug/l	100
70) Styrene	11.969	104	831908	51.059	ug/l	100
71) Bromoform	12.127	173	172315	50.229	ug/l #	100
73) Isopropylbenzene	12.249	105	1301009	49.803	ug/l	100
74) N-amyl acetate	12.066	43	227684	46.640	ug/l	100
75) 1,1,2,2-Tetrachloroethane	12.505	83	195565	44.878	ug/l	100
76) 1,2,3-Trichloropropane	12.554	75	169814m	43.898	ug/l	100
77) Bromobenzene	12.530	156	331331	49.419	ug/l	100
78) n-propylbenzene	12.591	91	1522965	49.572	ug/l	100
79) 2-Chlorotoluene	12.676	91	873335	49.235	ug/l	100
80) 1,3,5-Trimethylbenzene	12.731	105	1061112	49.966	ug/l	100
81) trans-1,4-Dichloro-2-b...	12.298	75	66299	46.212	ug/l	100
82) 4-Chlorotoluene	12.773	91	892764	48.192	ug/l	100
83) tert-Butylbenzene	12.993	119	988936	51.104	ug/l	100
84) 1,2,4-Trimethylbenzene	13.042	105	1061159	50.505	ug/l	100
85) sec-Butylbenzene	13.170	105	1405003	50.133	ug/l	100
86) p-Isopropyltoluene	13.286	119	1210644	51.115	ug/l	100
87) 1,3-Dichlorobenzene	13.286	146	649899	49.072	ug/l	100
88) 1,4-Dichlorobenzene	13.365	146	636694	48.476	ug/l	100
89) n-Butylbenzene	13.615	91	1051949	50.299	ug/l	100
90) Hexachloroethane	13.877	117	245108	47.664	ug/l	100
91) 1,2-Dichlorobenzene	13.657	146	567114	49.075	ug/l	100
92) 1,2-Dibromo-3-Chloropr...	14.273	75	32585	47.184	ug/l	100
93) 1,2,4-Trichlorobenzene	14.919	180	359833	52.852	ug/l	100
94) Hexachlorobutadiene	15.017	225	226316	53.346	ug/l	100
95) Naphthalene	15.139	128	575044	53.012	ug/l	100
96) 1,2,3-Trichlorobenzene	15.328	180	310831	52.628	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
Data File : VY023387.D
Acq On : 07 Oct 2025 11:47
Operator : SY/MD
Sample : VSTDICCC050
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICCC050

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025
Supervised By :Mahesh Dadoda 10/10/2025

Quant Time: Oct 08 04:43:02 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 04:39:16 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
 Data File : VY023387.D
 Acq On : 07 Oct 2025 11:47
 Operator : SY/MD
 Sample : VSTDICCC050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICCC050

Quant Time: Oct 08 04:43:02 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 04:39:16 2025
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 10/10/2025
 Supervised By : Mahesh Dadoda 10/10/2025

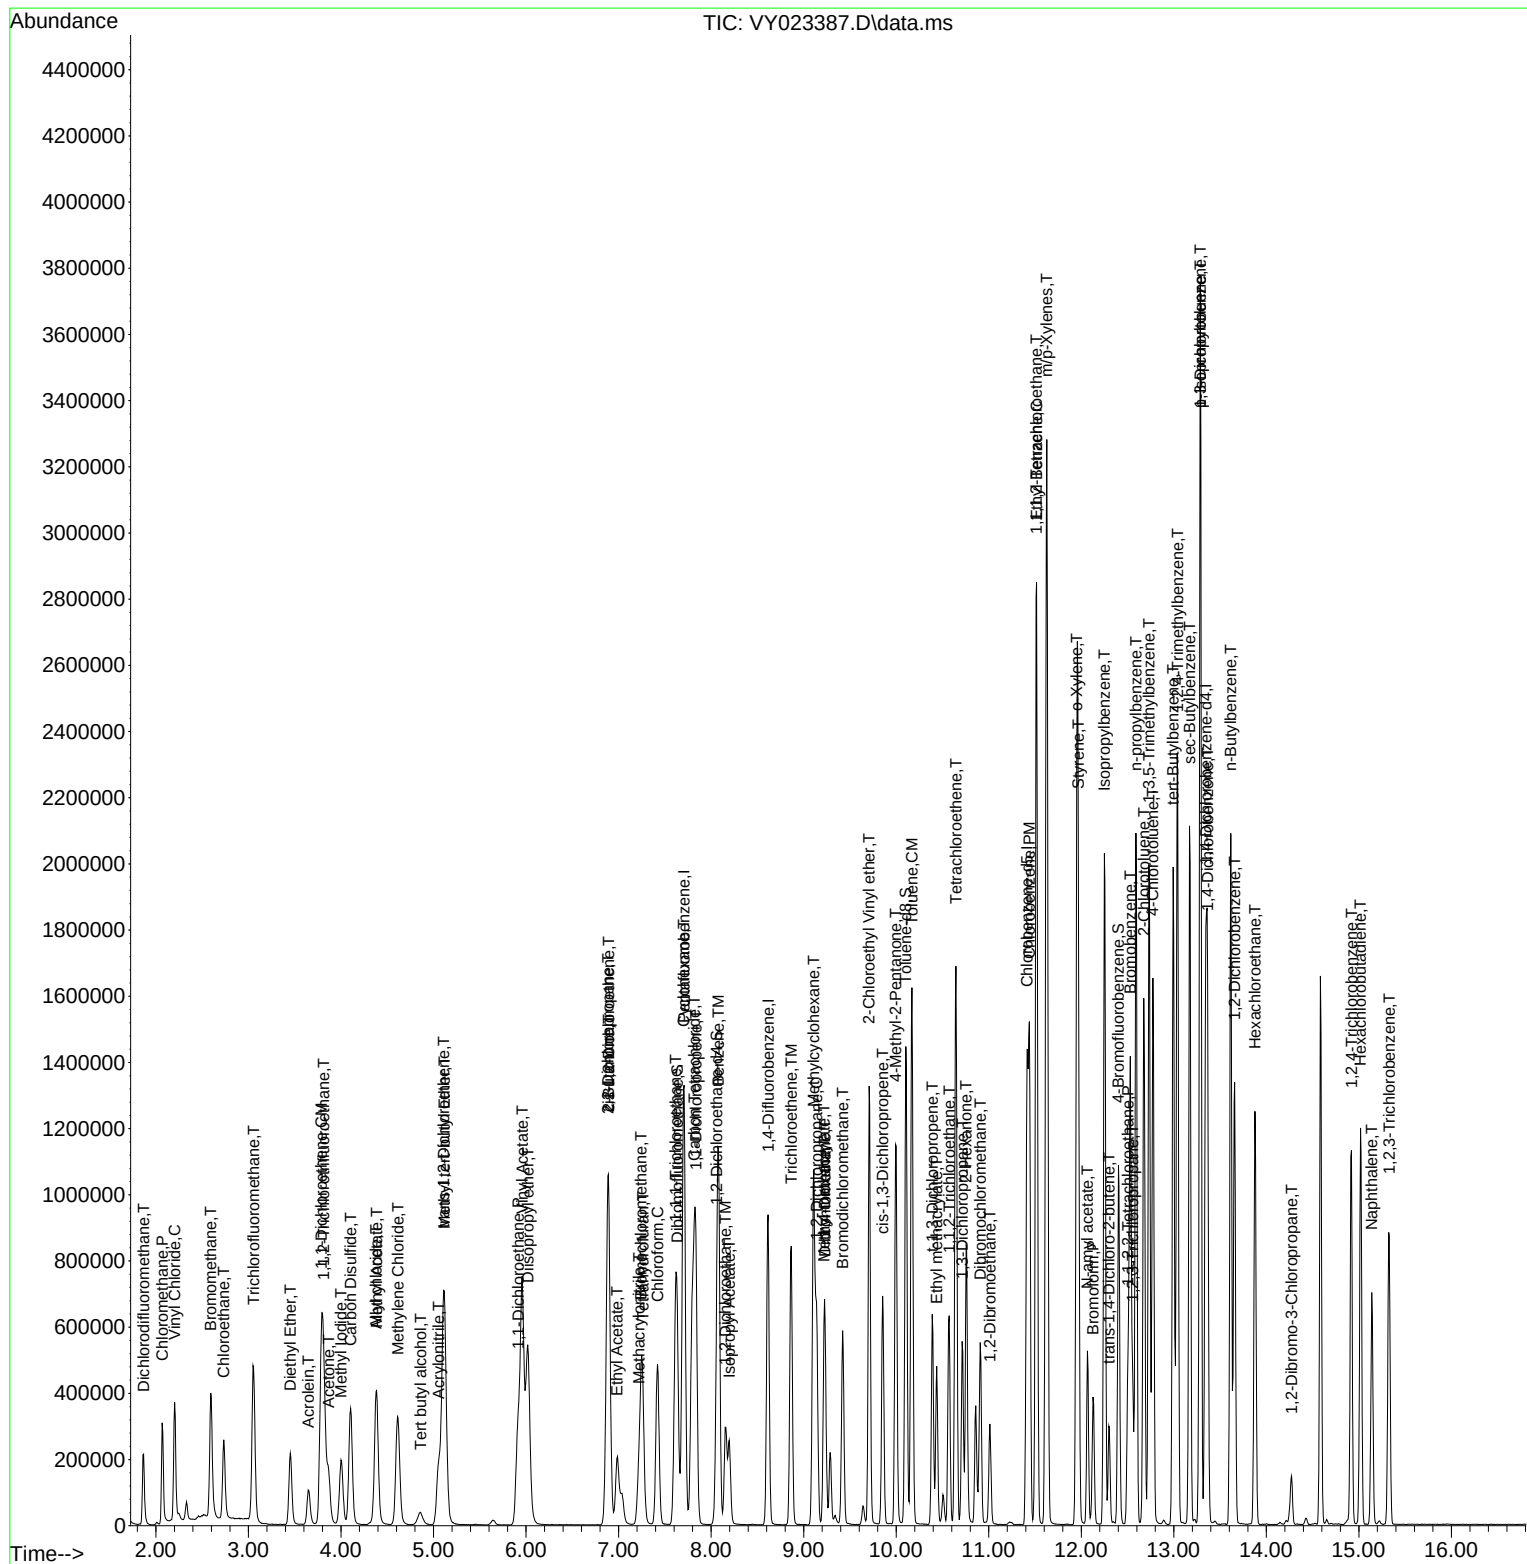

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
 Data File : VY023388.D
 Acq On : 07 Oct 2025 12:09
 Operator : SY/MD
 Sample : VSTDICC100
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICC100

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 10/10/2025
 Supervised By : Mahesh Dadoda 10/10/2025

Quant Time: Oct 08 04:44:07 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 04:39:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	595770	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	855682	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	764361	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.340	152	400285	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	467005	90.510	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 181.020%#			
35) Dibromofluoromethane	7.634	113	511478	98.497	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 197.000%#			
50) Toluene-d8	10.103	98	1919872	98.031	ug/l	0.00
Spiked Amount 50.000	Range 58 - 134		Recovery = 196.060%#			
62) 4-Bromofluorobenzene	12.401	95	636435	103.007	ug/l	0.00
Spiked Amount 50.000	Range 30 - 143		Recovery = 206.020%#			
Target Compounds					Qvalue	
2) Dichlorodifluoromethane	1.867	85	368985	78.627	ug/l	96
3) Chloromethane	2.068	50	521606	78.195	ug/l	96
4) Vinyl Chloride	2.202	62	711235	84.438	ug/l	100
5) Bromomethane	2.586	94	574957	83.210	ug/l	99
6) Chloroethane	2.732	64	491625	85.968	ug/l	99
7) Trichlorofluoromethane	3.049	101	1012851	93.610	ug/l	99
8) Diethyl Ether	3.452	74	266779	94.266	ug/l	100
9) 1,1,2-Trichlorotrifluo...	3.812	101	511482	88.441	ug/l	100
10) Methyl Iodide	4.001	142	651575	97.495	ug/l	99
11) Tert butyl alcohol	4.866	59	172718	568.898	ug/l	99
12) 1,1-Dichloroethene	3.787	96	508059	91.303	ug/l	96
13) Acrolein	3.647	56	262636	510.573	ug/l	99
14) Allyl chloride	4.378	41	637073	91.446	ug/l	99
15) Acrylonitrile	5.055	53	522511	471.296	ug/l	100
16) Acetone	3.866	43	504700	435.004	ug/l	98
17) Carbon Disulfide	4.104	76	1442005	83.061	ug/l	99
18) Methyl Acetate	4.385	43	316911	107.474	ug/l	98
19) Methyl tert-butyl Ether	5.116	73	1300206	99.797	ug/l	97
20) Methylene Chloride	4.610	84	552018	87.742	ug/l	98
21) trans-1,2-Dichloroethene	5.110	96	569334	91.999	ug/l	96
22) Diisopropyl ether	6.018	45	1423347	92.133	ug/l	97
23) Vinyl Acetate	5.957	43	3975052	468.098	ug/l	99
24) 1,1-Dichloroethane	5.915	63	911619	89.517	ug/l	99
25) 2-Butanone	6.890	43	685693	478.154	ug/l	99
26) 2,2-Dichloropropane	6.884	77	833452	92.108	ug/l	98
27) cis-1,2-Dichloroethene	6.890	96	670773	95.557	ug/l	98
28) Bromochloromethane	7.244	49	321657	81.418	ug/l	99
29) Tetrahydrofuran	7.262	42	415867	488.587	ug/l	99
30) Chloroform	7.421	83	1003722	91.401	ug/l	100
31) Cyclohexane	7.701	56	767083	85.293	ug/l	98
32) 1,1,1-Trichloroethane	7.616	97	910837	92.399	ug/l	100
36) 1,1-Dichloropropene	7.835	75	692477	94.516	ug/l	99
37) Ethyl Acetate	6.982	43	280560	96.859	ug/l	98
38) Carbon Tetrachloride	7.817	117	833170	97.894	ug/l	99
39) Methylcyclohexane	9.109	83	947664	101.024	ug/l	99
40) Benzene	8.079	78	2192645	96.000	ug/l	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
 Data File : VY023388.D
 Acq On : 07 Oct 2025 12:09
 Operator : SY/MD
 Sample : VSTDICC100
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICC100

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025
 Supervised By :Mahesh Dadoda 10/10/2025

Quant Time: Oct 08 04:44:07 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 04:39:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	7.219	41	152239	101.200	ug/l	98
42) 1,2-Dichloroethane	8.158	62	554810	95.449	ug/l	100
43) Isopropyl Acetate	8.195	43	573653	101.815	ug/l	99
44) Trichloroethene	8.866	130	636149	99.245	ug/l	100
45) 1,2-Dichloropropane	9.140	63	485084	94.381	ug/l	99
46) Dibromomethane	9.231	93	309964	98.596	ug/l	99
47) Bromodichloromethane	9.420	83	769238	97.210	ug/l	99
48) Methyl methacrylate	9.219	41	282582	107.476	ug/l	99
49) 1,4-Dioxane	9.225	88	77305	2374.722	ug/l	99
51) 4-Methyl-2-Pentanone	9.993	43	1539324	533.386	ug/l	100
52) Toluene	10.170	92	1462927	100.905	ug/l	99
53) t-1,3-Dichloropropene	10.390	75	710475	104.537	ug/l	98
54) cis-1,3-Dichloropropene	9.853	75	822967	101.302	ug/l	98
55) 1,1,2-Trichloroethane	10.573	97	417623	99.875	ug/l	96
56) Ethyl methacrylate	10.438	69	549366	114.077	ug/l	99
57) 1,3-Dichloropropane	10.713	76	670961	99.140	ug/l	100
58) 2-Chloroethyl Vinyl ether	9.707	63	1240361	588.731	ug/l	99
59) 2-Hexanone	10.755	43	1081568	541.284	ug/l	99
60) Dibromochloromethane	10.908	129	593878	104.133	ug/l	100
61) 1,2-Dibromoethane	11.011	107	406293	103.280	ug/l	99
64) Tetrachloroethene	10.646	164	767753	100.406	ug/l	99
65) Chlorobenzene	11.438	112	1655143	99.649	ug/l	99
66) 1,1,1,2-Tetrachloroethane	11.511	131	586878	100.470	ug/l	99
67) Ethyl Benzene	11.517	91	2788252	102.856	ug/l	98
68) m/p-Xylenes	11.627	106	2243033	206.437	ug/l	100
69) o-Xylene	11.950	106	1072335	106.611	ug/l	99
70) Styrene	11.969	104	1782757	107.344	ug/l	100
71) Bromoform	12.127	173	373208	106.727	ug/l #	100
73) Isopropylbenzene	12.249	105	2741698	102.825	ug/l	100
74) N-amyl acetate	12.066	43	532255	106.818	ug/l	99
75) 1,1,2,2-Tetrachloroethane	12.505	83	434720	97.735	ug/l	98
76) 1,2,3-Trichloropropane	12.554	75	364622m	92.345	ug/l	
77) Bromobenzene	12.529	156	701741	102.545	ug/l	100
78) n-propylbenzene	12.590	91	3165894	100.958	ug/l	99
79) 2-Chlorotoluene	12.676	91	1800124	99.426	ug/l	100
80) 1,3,5-Trimethylbenzene	12.731	105	2219080	102.374	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.298	75	148302	101.273	ug/l	98
82) 4-Chlorotoluene	12.773	91	1854165	98.060	ug/l	99
83) tert-Butylbenzene	12.993	119	2028198	102.684	ug/l	97
84) 1,2,4-Trimethylbenzene	13.042	105	2227197	103.853	ug/l	100
85) sec-Butylbenzene	13.170	105	2932949	102.530	ug/l	100
86) p-Isopropyltoluene	13.285	119	2548220	105.408	ug/l	100
87) 1,3-Dichlorobenzene	13.285	146	1361716	100.735	ug/l	100
88) 1,4-Dichlorobenzene	13.365	146	1323618	98.734	ug/l	100
89) n-Butylbenzene	13.615	91	2223744	104.174	ug/l	99
90) Hexachloroethane	13.877	117	514746	98.069	ug/l	99
91) 1,2-Dichlorobenzene	13.657	146	1193043	101.146	ug/l	100
92) 1,2-Dibromo-3-Chloropr...	14.267	75	70107	99.458	ug/l	94
93) 1,2,4-Trichlorobenzene	14.919	180	806328	116.031	ug/l	99
94) Hexachlorobutadiene	15.017	225	470072	108.557	ug/l	99
95) Naphthalene	15.139	128	1378291	124.485	ug/l	100
96) 1,2,3-Trichlorobenzene	15.322	180	693477	115.034	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
Data File : VY023388.D
Acq On : 07 Oct 2025 12:09
Operator : SY/MD
Sample : VSTDICC100
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICC100

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025
Supervised By :Mahesh Dadoda 10/10/2025

Quant Time: Oct 08 04:44:07 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 04:39:16 2025
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICC100

Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025
Supervised By :Mahesh Dadoda 10/10/2025

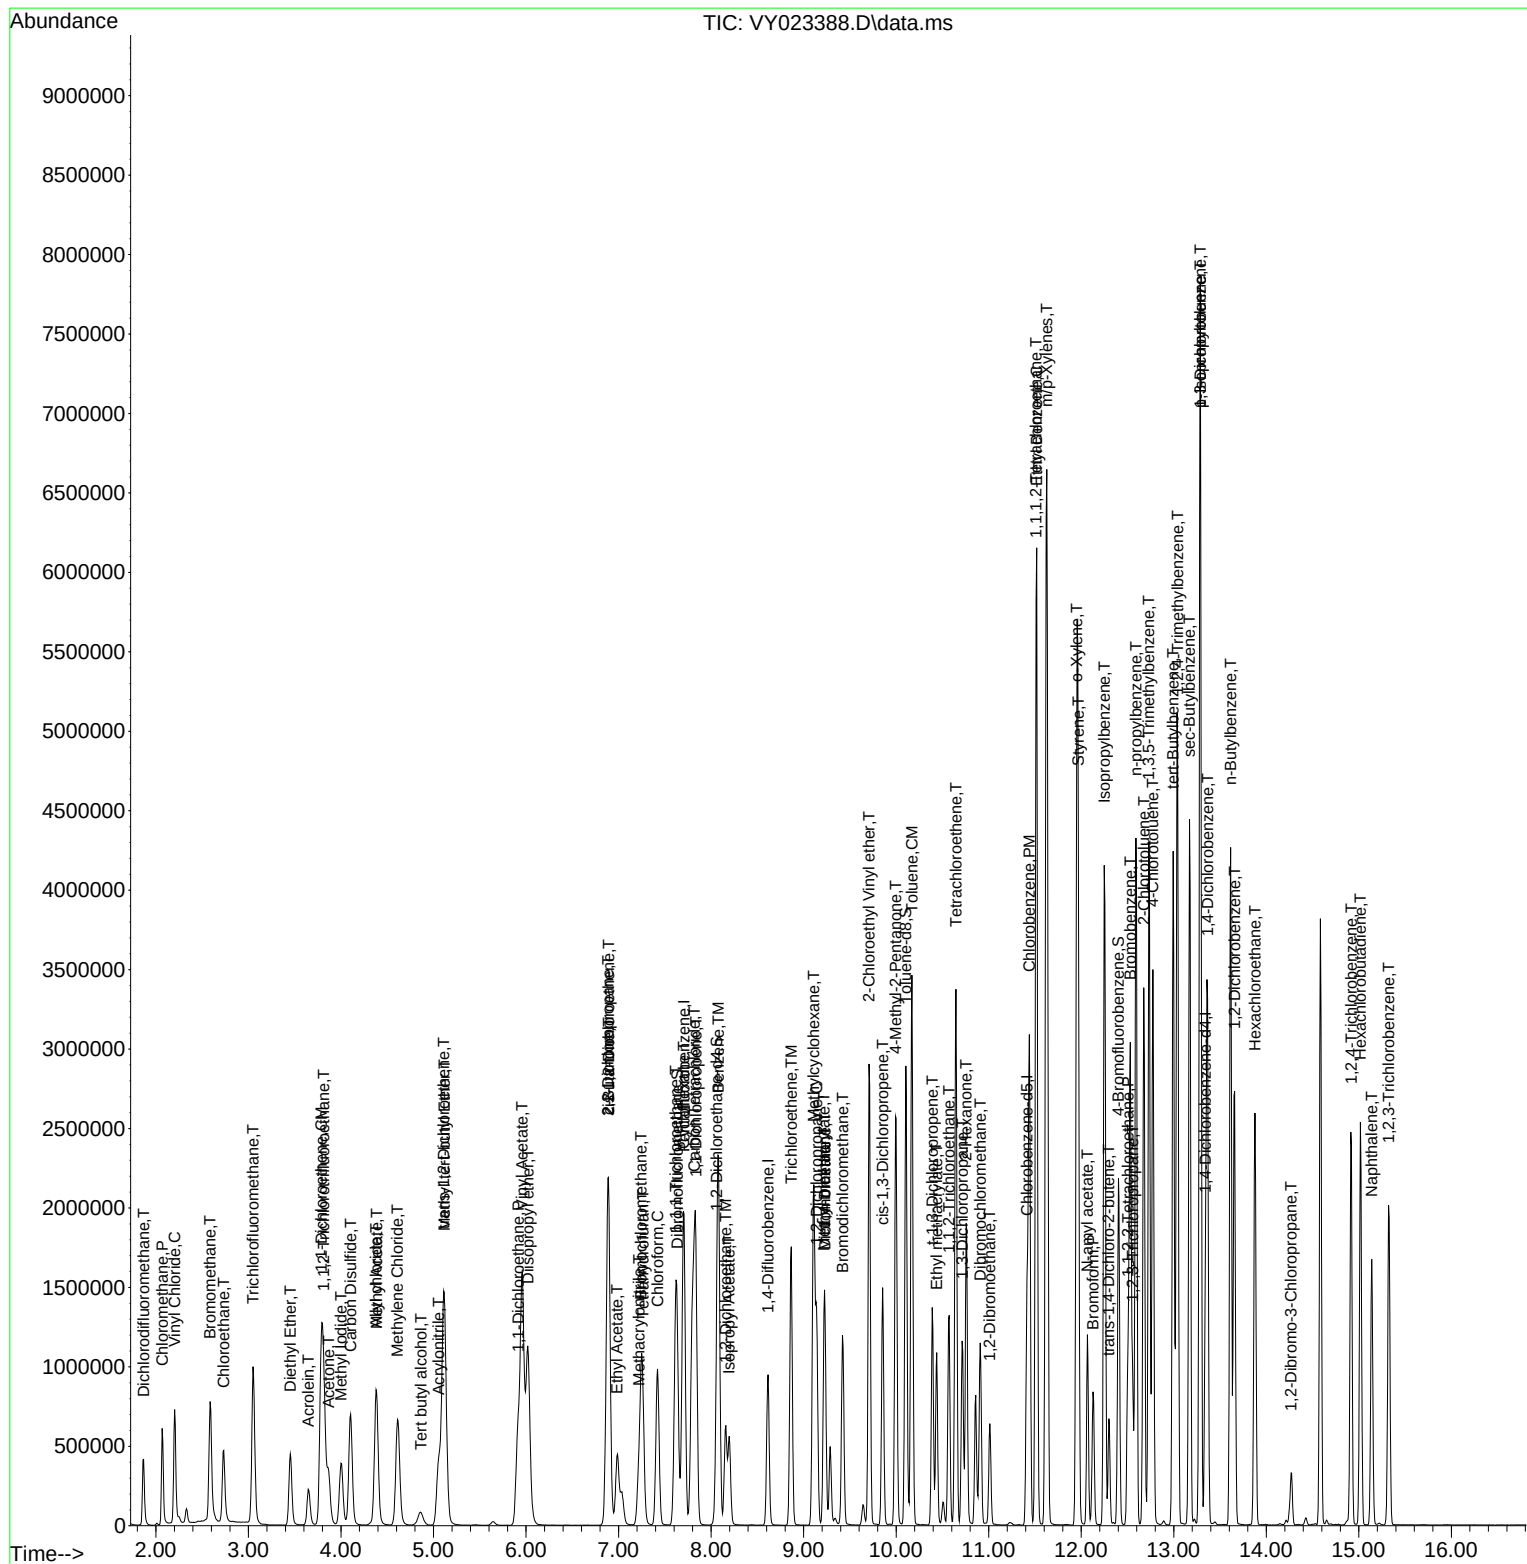

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
 Data File : VY023389.D
 Acq On : 07 Oct 2025 12:32
 Operator : SY/MD
 Sample : VSTDICC150
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICC150

Quant Time: Oct 08 04:45:15 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 04:39:16 2025
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 10/10/2025
 Supervised By : Mahesh Dadoda 10/10/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	588489	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	855488	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	765357	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	402368	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	714730	140.236	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 280.480%#			
35) Dibromofluoromethane	7.634	113	778632	149.977	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 299.960%#			
50) Toluene-d8	10.103	98	2912319	148.741	ug/l	0.00
Spiked Amount 50.000	Range 58 - 134		Recovery = 297.480%#			
62) 4-Bromofluorobenzene	12.402	95	990964	160.423	ug/l	0.00
Spiked Amount 50.000	Range 30 - 143		Recovery = 320.840%#			
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.867	85	587619	126.766	ug/l	97
3) Chloromethane	2.068	50	825167	125.233	ug/l	100
4) Vinyl Chloride	2.208	62	1118134	134.387	ug/l	100
5) Bromomethane	2.580	94	915389	134.118	ug/l	98
6) Chloroethane	2.726	64	756912	133.994	ug/l	99
7) Trichlorofluoromethane	3.050	101	1549160	144.948	ug/l	100
8) Diethyl Ether	3.452	74	418615	149.747	ug/l	100
9) 1,1,2-Trichlorotrifluo...	3.812	101	786278	137.639	ug/l	99
10) Methyl Iodide	4.007	142	992925	150.409	ug/l	99
11) Tert butyl alcohol	4.866	59	288878	963.279	ug/l	99
12) 1,1-Dichloroethene	3.787	96	781235	142.133	ug/l	97
13) Acrolein	3.653	56	423418	833.323	ug/l	100
14) Allyl chloride	4.385	41	988378	143.628	ug/l	99
15) Acrylonitrile	5.055	53	841857	768.735	ug/l	99
16) Acetone	3.866	43	789668	689.040	ug/l	99
17) Carbon Disulfide	4.104	76	2199339	128.252	ug/l	100
18) Methyl Acetate	4.385	43	505344	173.497	ug/l	99
19) Methyl tert-butyl Ether	5.116	73	2056533	159.802	ug/l	97
20) Methylene Chloride	4.616	84	835005	134.365	ug/l	98
21) trans-1,2-Dichloroethene	5.116	96	871380	142.549	ug/l	98
22) Diisopropyl ether	6.019	45	2218430	145.375	ug/l	99
23) Vinyl Acetate	5.958	43	6377047	760.246	ug/l	99
24) 1,1-Dichloroethane	5.915	63	1398477	139.024	ug/l	98
25) 2-Butanone	6.890	43	1116343	788.091	ug/l	97
26) 2,2-Dichloropropane	6.884	77	1281633	143.391	ug/l	99
27) cis-1,2-Dichloroethene	6.890	96	1043574	150.505	ug/l	98
28) Bromochloromethane	7.244	49	482210	123.567	ug/l	99
29) Tetrahydrofuran	7.262	42	687719	817.972	ug/l	100
30) Chloroform	7.421	83	1542715	142.221	ug/l	99
31) Cyclohexane	7.701	56	1192778	134.268	ug/l	98
32) 1,1,1-Trichloroethane	7.616	97	1405131	144.305	ug/l	100
36) 1,1-Dichloropropene	7.835	75	1069665	146.031	ug/l	100
37) Ethyl Acetate	6.982	43	460027	158.853	ug/l	98
38) Carbon Tetrachloride	7.817	117	1290353	151.646	ug/l	99
39) Methylcyclohexane	9.109	83	1496612	159.580	ug/l	99
40) Benzene	8.079	78	3366812	147.442	ug/l	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
 Data File : VY023389.D
 Acq On : 07 Oct 2025 12:32
 Operator : SY/MD
 Sample : VSTDICC150
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICC150

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025
 Supervised By :Mahesh Dadoda 10/10/2025

Quant Time: Oct 08 04:45:15 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 04:39:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	7.220	41	246974	164.212	ug/l	98
42) 1,2-Dichloroethane	8.158	62	866250	149.063	ug/l	100
43) Isopropyl Acetate	8.195	43	946087	167.955	ug/l	100
44) Trichloroethene	8.866	130	966011	150.740	ug/l	99
45) 1,2-Dichloropropane	9.140	63	752286	146.403	ug/l	99
46) Dibromomethane	9.231	93	483702	153.895	ug/l	99
47) Bromodichloromethane	9.420	83	1202247	151.965	ug/l	98
48) Methyl methacrylate	9.219	41	463614	176.368	ug/l	100
49) 1,4-Dioxane	9.225	88	123991	3809.726	ug/l	97
51) 4-Methyl-2-Pentanone	9.993	43	2516107	872.045	ug/l	100
52) Toluene	10.170	92	2272574	156.786	ug/l	98
53) t-1,3-Dichloropropene	10.390	75	1123644	165.367	ug/l	100
54) cis-1,3-Dichloropropene	9.853	75	1296713	159.654	ug/l	99
55) 1,1,2-Trichloroethane	10.573	97	652242	156.020	ug/l	96
56) Ethyl methacrylate	10.438	69	886127	184.048	ug/l	100
57) 1,3-Dichloropropane	10.713	76	1049593	155.122	ug/l	100
58) 2-Chloroethyl Vinyl ether	9.707	63	2040136	968.559	ug/l	100
59) 2-Hexanone	10.755	43	1776032	889.038	ug/l	99
60) Dibromochloromethane	10.908	129	935577	164.084	ug/l	99
61) 1,2-Dibromoethane	11.012	107	639895	162.699	ug/l	99
64) Tetrachloroethene	10.646	164	1046931	136.739	ug/l	98
65) Chlorobenzene	11.438	112	2563176	154.117	ug/l	99
66) 1,1,1,2-Tetrachloroethane	11.511	131	923367	157.870	ug/l	99
67) Ethyl Benzene	11.518	91	4341801	159.957	ug/l	97
68) m/p-Xylenes	11.627	106	3502137	321.899	ug/l	99
69) o-Xylene	11.950	106	1694987	168.295	ug/l	98
70) Styrene	11.969	104	2830398	170.203	ug/l	99
71) Bromoform	12.127	173	602644	172.115	ug/l #	99
73) Isopropylbenzene	12.249	105	4290662	160.084	ug/l	100
74) N-amyl acetate	12.066	43	890882	177.866	ug/l	98
75) 1,1,2,2-Tetrachloroethane	12.505	83	737773	165.010	ug/l	99
76) 1,2,3-Trichloropropane	12.554	75	565754m	142.542	ug/l	
77) Bromobenzene	12.530	156	1111318	161.555	ug/l	100
78) n-propylbenzene	12.591	91	4932015	156.465	ug/l	99
79) 2-Chlorotoluene	12.676	91	2822049	155.063	ug/l	100
80) 1,3,5-Trimethylbenzene	12.731	105	3496249	160.460	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.298	75	245190	166.570	ug/l	98
82) 4-Chlorotoluene	12.773	91	2902371	152.701	ug/l	99
83) tert-Butylbenzene	12.993	119	3220384	162.197	ug/l	97
84) 1,2,4-Trimethylbenzene	13.042	105	3503639	162.527	ug/l	99
85) sec-Butylbenzene	13.170	105	4560715	158.609	ug/l	99
86) p-Isopropyltoluene	13.286	119	4024712	165.622	ug/l	100
87) 1,3-Dichlorobenzene	13.286	146	2165278	159.350	ug/l	100
88) 1,4-Dichlorobenzene	13.365	146	2090133	155.104	ug/l	100
89) n-Butylbenzene	13.615	91	3505715	163.379	ug/l	99
90) Hexachloroethane	13.877	117	799264	151.487	ug/l	99
91) 1,2-Dichlorobenzene	13.657	146	1862691	157.101	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	14.267	75	116273	164.099	ug/l	96
93) 1,2,4-Trichlorobenzene	14.913	180	1272621	182.183	ug/l	100
94) Hexachlorobutadiene	15.017	225	711748	163.518	ug/l	98
95) Naphthalene	15.139	128	2277549	204.639	ug/l	100
96) 1,2,3-Trichlorobenzene	15.322	180	1110193	183.206	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
Data File : VY023389.D
Acq On : 07 Oct 2025 12:32
Operator : SY/MD
Sample : VSTDICC150
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICC150

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025
Supervised By :Mahesh Dadoda 10/10/2025

Quant Time: Oct 08 04:45:15 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 04:39:16 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
Data File : VY023389.D
Acq On : 07 Oct 2025 12:32
Operator : SY/MD
Sample : VSTDICC150
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICC150

Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025
Supervised By :Mahesh Dadoda 10/10/2025

Quant Time: Oct 08 04:45:15 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 04:39:16 2025
Response via : Initial Calibration

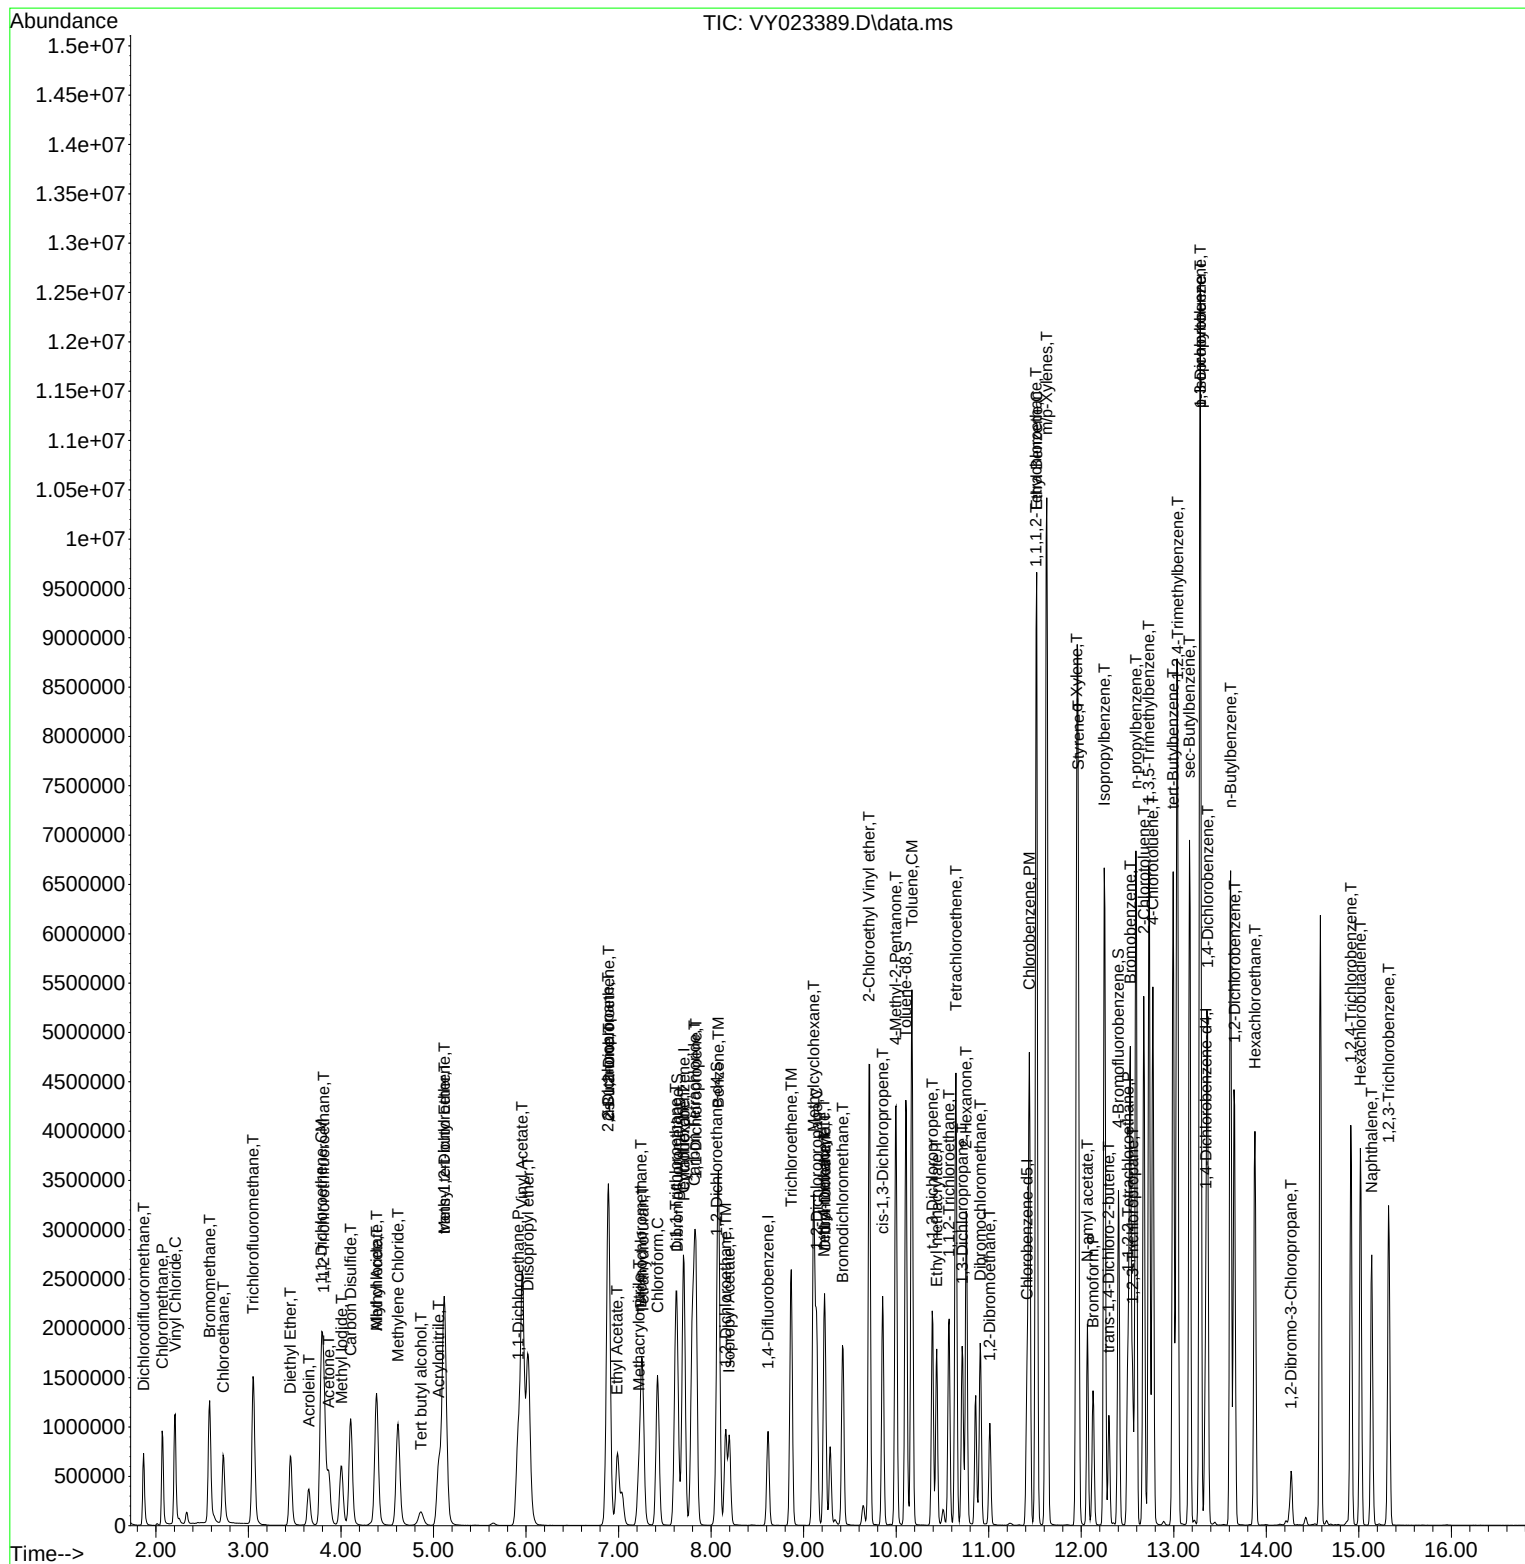

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
 Data File : VY023391.D
 Acq On : 07 Oct 2025 14:12
 Operator : SY/MD
 Sample : VSTDICV050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 ICVVY100725

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025
 Supervised By :Mahesh Dadoda 10/10/2025

Quant Time: Oct 08 05:15:49 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	574332	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	861639	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	771372	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	405636	50.000	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	8.061	65	237493	49.450	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	98.900%
35) Dibromofluoromethane	7.634	113	260038	49.116	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	98.240%
50) Toluene-d8	10.103	98	970614	49.228	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	98.460%
62) 4-Bromofluorobenzene	12.402	95	324700	49.881	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	99.760%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.867	85	185683	44.916	ug/l	99
3) Chloromethane	2.068	50	295766	52.519	ug/l	98
4) Vinyl Chloride	2.208	62	362714	49.449	ug/l	100
5) Bromomethane	2.598	94	300735	48.856	ug/l	98
6) Chloroethane	2.739	64	256831	51.367	ug/l	99
7) Trichlorofluoromethane	3.056	101	494789	48.582	ug/l	99
8) Diethyl Ether	3.458	74	135857	51.050	ug/l	100
9) 1,1,2-Trichlorotrifluo...	3.812	101	257524	48.728	ug/l	100
10) Methyl Iodide	4.007	142	305209	51.875	ug/l	98
11) Tert butyl alcohol	4.860	59	82562	231.079	ug/l	100
12) 1,1-Dichloroethene	3.787	96	254382	49.653	ug/l	97
13) Acrolein	3.653	56	124288	246.184	ug/l	99
14) Allyl chloride	4.385	41	316213	50.645	ug/l	99
15) Acrylonitrile	5.055	53	256219	251.575	ug/l	99
16) Acetone	3.866	43	243433	212.910	ug/l	98
17) Carbon Disulfide	4.104	76	733457	50.021	ug/l	100
18) Methyl Acetate	4.385	43	151281	50.439	ug/l	100
19) Methyl tert-butyl Ether	5.116	73	643111	52.230	ug/l	97
20) Methylene Chloride	4.616	84	324604	52.503	ug/l	97
21) trans-1,2-Dichloroethene	5.116	96	290384	51.482	ug/l	98
22) Diisopropyl ether	6.019	45	709381	51.364	ug/l	99
23) Vinyl Acetate	5.958	43	1950969	260.981	ug/l	99
24) 1,1-Dichloroethane	5.915	63	464207	50.742	ug/l	98
25) 2-Butanone	6.890	43	325351	233.083	ug/l	99
26) 2,2-Dichloropropane	6.884	77	416585	49.626	ug/l	99
27) cis-1,2-Dichloroethene	6.890	96	341964	52.485	ug/l	97
28) Bromochloromethane	7.244	49	155146	45.427	ug/l	100
29) Tetrahydrofuran	7.262	42	200513	253.317	ug/l	99
30) Chloroform	7.421	83	513997	51.137	ug/l	98
31) Cyclohexane	7.701	56	378819	47.416	ug/l	98
32) 1,1,1-Trichloroethane	7.616	97	456112	49.934	ug/l	100
36) 1,1-Dichloropropene	7.835	75	348786	49.761	ug/l	99
37) Ethyl Acetate	6.982	43	138119	49.740	ug/l	98
38) Carbon Tetrachloride	7.817	117	413653	48.671	ug/l	99
39) Methylcyclohexane	9.109	83	456031	49.970	ug/l	99
40) Benzene	8.079	78	1107790	49.906	ug/l	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
 Data File : VY023391.D
 Acq On : 07 Oct 2025 14:12
 Operator : SY/MD
 Sample : VSTDICV050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 ICVVY100725

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025
 Supervised By :Mahesh Dadoda 10/10/2025

Quant Time: Oct 08 05:15:49 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	7.220	41	72100	48.008	ug/l	96
42) 1,2-Dichloroethane	8.158	62	282332	49.318	ug/l	99
43) Isopropyl Acetate	8.195	43	279887	50.548	ug/l	100
44) Trichloroethene	8.866	130	319131	49.120	ug/l	98
45) 1,2-Dichloropropane	9.140	63	246887	50.355	ug/l	100
46) Dibromomethane	9.231	93	157758	50.885	ug/l	98
47) Bromodichloromethane	9.420	83	393918	50.450	ug/l	99
48) Methyl methacrylate	9.219	41	128606	49.440	ug/l	95
49) 1,4-Dioxane	9.231	88	37356	1039.252	ug/l	97
51) 4-Methyl-2-Pentanone	10.000	43	724992	253.421	ug/l	100
52) Toluene	10.170	92	743055	51.556	ug/l	99
53) t-1,3-Dichloropropene	10.390	75	347336	51.160	ug/l	99
54) cis-1,3-Dichloropropene	9.853	75	413860	51.649	ug/l	99
55) 1,1,2-Trichloroethane	10.573	97	210245	50.430	ug/l	97
56) Ethyl methacrylate	10.438	69	256731	53.385	ug/l	99
57) 1,3-Dichloropropane	10.713	76	337673	51.113	ug/l	99
58) 2-Chloroethyl Vinyl ether	9.713	63	586266	272.133	ug/l	100
59) 2-Hexanone	10.762	43	501877	245.480	ug/l	99
60) Dibromochloromethane	10.908	129	297946	50.974	ug/l	99
61) 1,2-Dibromoethane	11.018	107	201415	50.658	ug/l	100
64) Tetrachloroethene	10.646	164	382998	48.087	ug/l	99
65) Chlorobenzene	11.438	112	828466	49.381	ug/l	100
66) 1,1,1,2-Tetrachloroethane	11.518	131	296157	49.537	ug/l	99
67) Ethyl Benzene	11.518	91	1380691	50.841	ug/l	100
68) m/p-Xylenes	11.627	106	1108386	101.757	ug/l	100
69) o-Xylene	11.950	106	526954	51.577	ug/l	100
70) Styrene	11.969	104	875709	52.122	ug/l	100
71) Bromoform	12.133	173	185682	50.070	ug/l #	98
73) Isopropylbenzene	12.255	105	1345109	50.318	ug/l	100
74) N-amyl acetate	12.066	43	245291	51.087	ug/l	99
75) 1,1,2,2-Tetrachloroethane	12.505	83	217245	49.688	ug/l	99
76) 1,2,3-Trichloropropane	12.554	75	153438m	42.874	ug/l	
77) Bromobenzene	12.530	156	352420	49.590	ug/l	99
78) n-propylbenzene	12.591	91	1568180	50.694	ug/l	100
79) 2-Chlorotoluene	12.676	91	906610	50.047	ug/l	100
80) 1,3,5-Trimethylbenzene	12.737	105	1106664	51.231	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.304	75	67959	46.566	ug/l	97
82) 4-Chlorotoluene	12.773	91	941314	50.455	ug/l	100
83) tert-Butylbenzene	12.993	119	1037510	52.019	ug/l	99
84) 1,2,4-Trimethylbenzene	13.042	105	1110672	51.520	ug/l	99
85) sec-Butylbenzene	13.176	105	1454774	50.848	ug/l	100
86) p-Isopropyltoluene	13.292	119	1263377	51.864	ug/l	99
87) 1,3-Dichlorobenzene	13.286	146	686854	49.632	ug/l	99
88) 1,4-Dichlorobenzene	13.365	146	671644	49.140	ug/l	100
89) n-Butylbenzene	13.615	91	1100086	51.829	ug/l	99
90) Hexachloroethane	13.877	117	257335	49.116	ug/l	98
91) 1,2-Dichlorobenzene	13.657	146	602989	49.698	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	14.273	75	34928	48.687	ug/l	99
93) 1,2,4-Trichlorobenzene	14.919	180	386806	51.138	ug/l	100
94) Hexachlorobutadiene	15.023	225	236040	50.061	ug/l	99
95) Naphthalene	15.139	128	628190	52.154	ug/l	100
96) 1,2,3-Trichlorobenzene	15.328	180	335267	51.172	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
Data File : VY023391.D
Acq On : 07 Oct 2025 14:12
Operator : SY/MD
Sample : VSTDICV050
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
ICVVY100725

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025
Supervised By :Mahesh Dadoda 10/10/2025

Quant Time: Oct 08 05:15:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 05:12:50 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
 Data File : VY023391.D
 Acq On : 07 Oct 2025 14:12
 Operator : SY/MD
 Sample : VSTDICV050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :

MSVOA_Y

ClientSampleId :

ICVVY100725

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 10/10/2025
 Supervised By :Mahesh Dadoda 10/10/2025


Quant Time: Oct 08 05:15:49 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M

Quant Title : SW846 8260

QLast Update : Wed Oct 08 05:12:50 2025

Response via : Initial Calibration

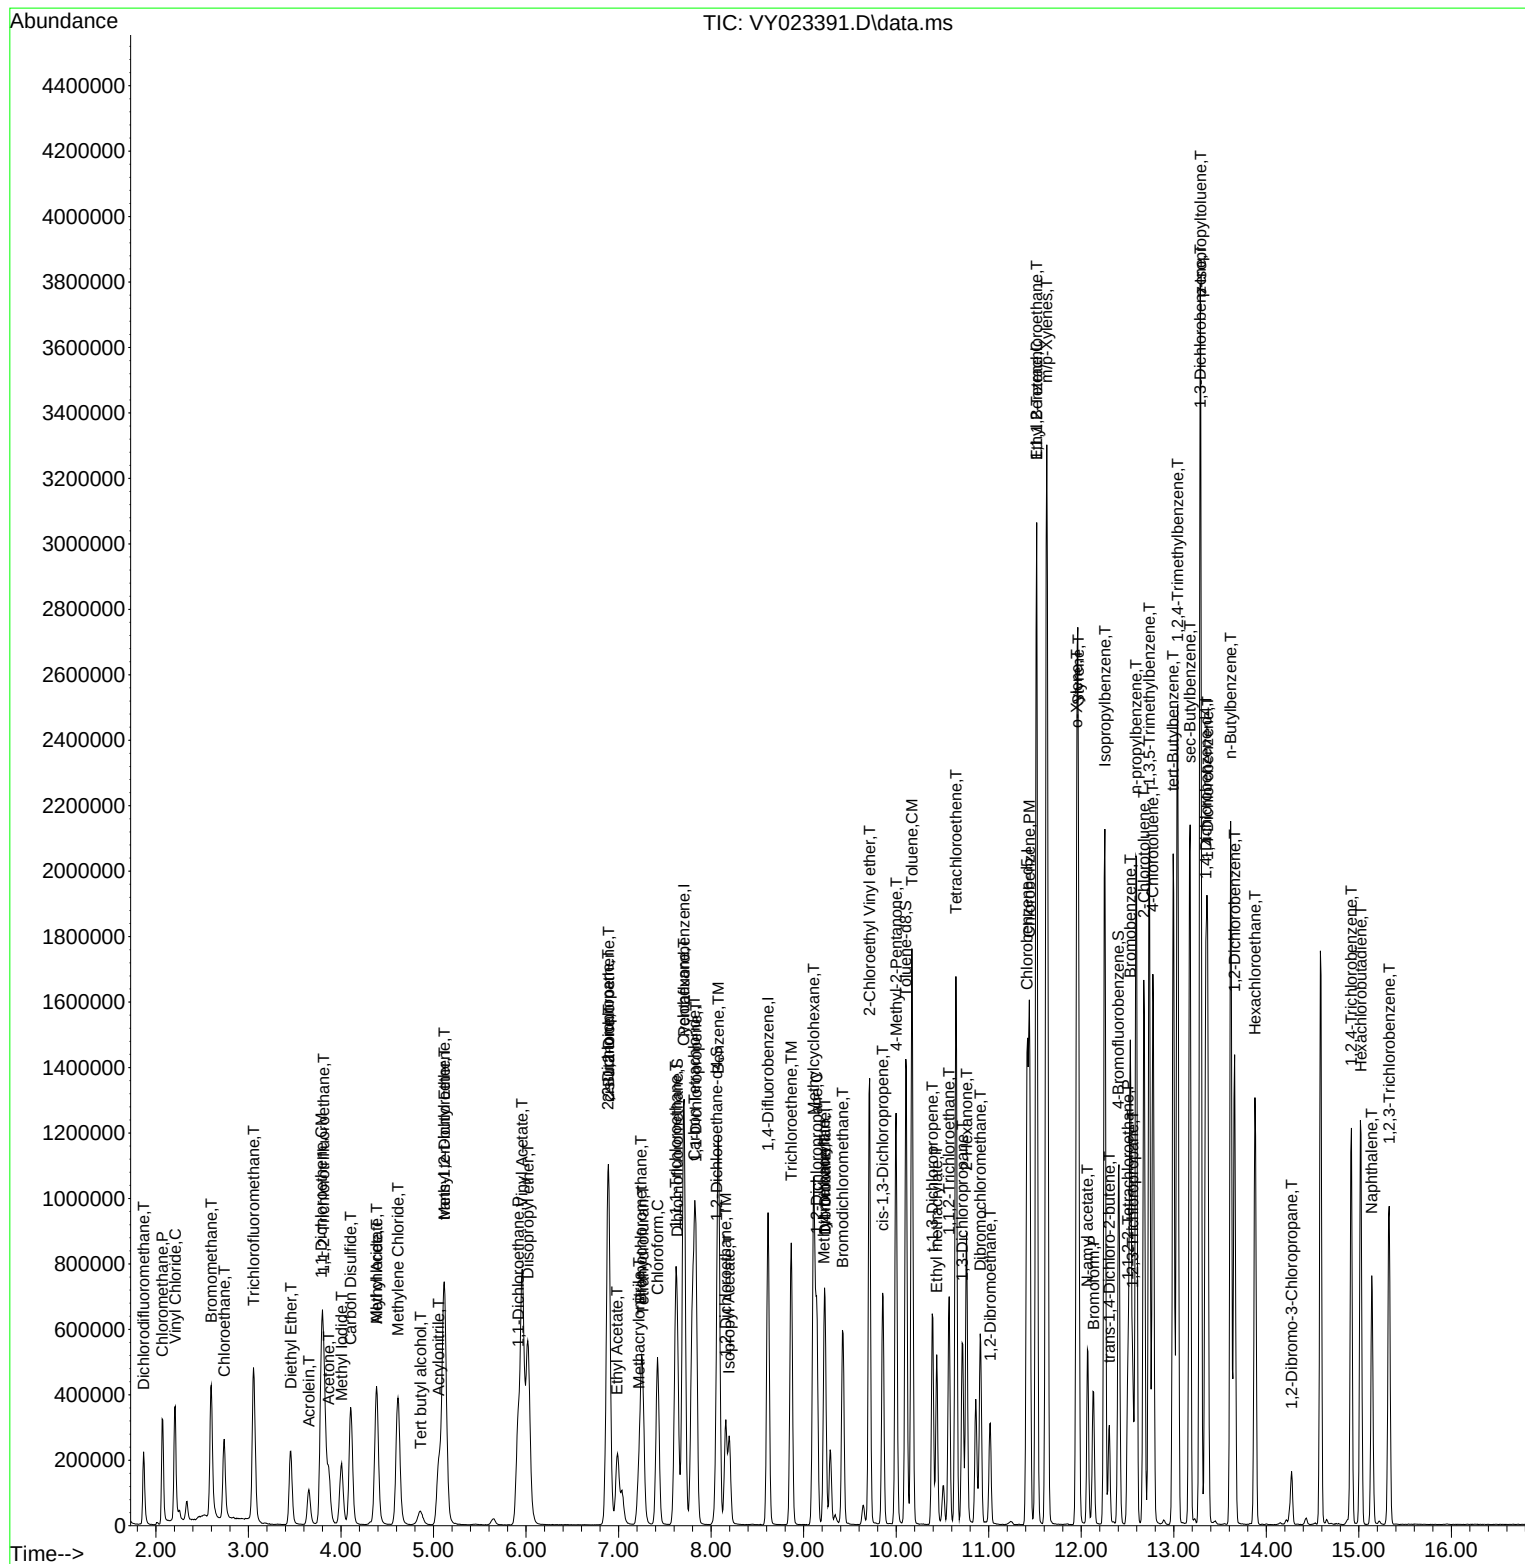

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
 Data File : VY023391.D
 Acq On : 07 Oct 2025 14:12
 Operator : SY/MD
 Sample : VSTDICV050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 ICVVY100725

Quant Time: Oct 08 05:15:49 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	50.000	50.000	0.0	97	0.00
2 T	Dichlorodifluoromethane	50.000	44.916	10.2	98	0.00
3 P	Chloromethane	50.000	52.519	-5.0	112	0.00
4 C	Vinyl Chloride	50.000	49.449	1.1#	103	0.00
5 T	Bromomethane	50.000	48.856	2.3	109	0.00
6 T	Chloroethane	50.000	51.367	-2.7	105	0.00
7 T	Trichlorofluoromethane	50.000	48.582	2.8	100	0.00
8 T	Diethyl Ether	50.000	51.050	-2.1	107	0.00
9 T	1,1,2-Trichlorotrifluoroeth	50.000	48.728	2.5	100	0.00
10 T	Methyl Iodide	50.000	51.875	-3.8	96	0.00
11 T	Tert butyl alcohol	250.000	231.079	7.6	112	0.00
12 CM	1,1-Dichloroethene	50.000	49.653	0.7#	101	0.00
13 T	Acrolein	250.000	246.184	1.5	101	0.00
14 T	Allyl chloride	50.000	50.645	-1.3	102	0.00
15 T	Acrylonitrile	250.000	251.575	-0.6	106	0.00
16 T	Acetone	250.000	212.910	14.8	99	0.00
17 T	Carbon Disulfide	50.000	50.021	-0.0	101	0.00
18 T	Methyl Acetate	50.000	50.439	-0.9	104	0.00
19 T	Methyl tert-butyl Ether	50.000	52.230	-4.5	107	0.00
20 T	Methylene Chloride	50.000	52.503	-5.0	120	0.00
21 T	trans-1,2-Dichloroethene	50.000	51.482	-3.0	105	0.00
22 T	Diisopropyl ether	50.000	51.364	-2.7	103	0.00
23 T	Vinyl Acetate	250.000	260.981	-4.4	106	0.00
24 P	1,1-Dichloroethane	50.000	50.742	-1.5	104	0.00
25 T	2-Butanone	250.000	233.083	6.8	105	0.00
26 T	2,2-Dichloropropane	50.000	49.626	0.7	100	0.00
27 T	cis-1,2-Dichloroethene	50.000	52.485	-5.0	107	0.00
28 T	Bromochloromethane	50.000	45.427	9.1	99	0.00
29 T	Tetrahydrofuran	250.000	253.317	-1.3	107	0.00
30 C	Chloroform	50.000	51.137	-2.3#	104	0.00
31 T	Cyclohexane	50.000	47.416	5.2	100	0.00
32 T	1,1,1-Trichloroethane	50.000	49.934	0.1	101	0.00
33 S	1,2-Dichloroethane-d4	50.000	49.450	1.1	103	0.00
34 I	1,4-Difluorobenzene	50.000	50.000	0.0	100	0.00
35 S	Dibromofluoromethane	50.000	49.116	1.8	101	0.00
36 T	1,1-Dichloropropene	50.000	49.761	0.5	102	0.00
37 T	Ethyl Acetate	50.000	49.740	0.5	107	0.00
38 T	Carbon Tetrachloride	50.000	48.671	2.7	100	0.00
39 T	Methylcyclohexane	50.000	49.970	0.1	101	0.00
40 TM	Benzene	50.000	49.906	0.2	102	0.00
41 T	Methacrylonitrile	50.000	48.008	4.0	105	0.00
42 TM	1,2-Dichloroethane	50.000	49.318	1.4	104	0.00
43 T	Isopropyl Acetate	50.000	50.548	-1.1	108	0.00
44 TM	Trichloroethene	50.000	49.120	1.8	101	0.00
45 C	1,2-Dichloropropane	50.000	50.355	-0.7#	105	0.00
46 T	Dibromomethane	50.000	50.885	-1.8	106	0.00
47 T	Bromodichloromethane	50.000	50.450	-0.9	104	0.00
48 T	Methyl methacrylate	50.000	49.440	1.1	101	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
 Data File : VY023391.D
 Acq On : 07 Oct 2025 14:12
 Operator : SY/MD
 Sample : VSTDICV050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 ICVVY100725

Quant Time: Oct 08 05:15:49 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	1000.000	1039.252	-3.9	110	0.00
50 S	Toluene-d8	50.000	49.228	1.5	100	0.00
51 T	4-Methyl-2-Pentanone	250.000	253.421	-1.4	106	0.00
52 CM	Toluene	50.000	51.556	-3.1#	105	0.00
53 T	t-1,3-Dichloropropene	50.000	51.160	-2.3	105	0.00
54 T	cis-1,3-Dichloropropene	50.000	51.649	-3.3	106	0.00
55 T	1,1,2-Trichloroethane	50.000	50.430	-0.9	106	0.00
56 T	Ethyl methacrylate	50.000	53.385	-6.8	107	0.00
57 T	1,3-Dichloropropane	50.000	51.113	-2.2	105	0.00
58 T	2-Chloroethyl Vinyl ether	250.000	272.133	-8.9	106	0.00
59 T	2-Hexanone	250.000	245.480	1.8	105	0.00
60 T	Dibromochloromethane	50.000	50.974	-1.9	106	0.00
61 T	1,2-Dibromoethane	50.000	50.658	-1.3	105	0.00
62 S	4-Bromofluorobenzene	50.000	49.881	0.2	104	0.00
63 I	Chlorobenzene-d5	50.000	50.000	0.0	103	0.00
64 T	Tetrachloroethene	50.000	48.087	3.8	98	0.00
65 PM	Chlorobenzene	50.000	49.381	1.2	105	0.00
66 T	1,1,1,2-Tetrachloroethane	50.000	49.537	0.9	106	0.00
67 C	Ethyl Benzene	50.000	50.841	-1.7#	104	0.00
68 T	m/p-Xylenes	100.000	101.757	-1.8	103	0.00
69 T	o-Xylene	50.000	51.577	-3.2	105	0.00
70 T	Styrene	50.000	52.122	-4.2	105	0.00
71 P	Bromoform	50.000	50.070	-0.1	108	0.00
72 I	1,4-Dichlorobenzene-d4	50.000	50.000	0.0	103	0.00
73 T	Isopropylbenzene	50.000	50.318	-0.6	103	0.00
74 T	N-ethyl acetate	50.000	51.087	-2.2	108	0.00
75 P	1,1,2,2-Tetrachloroethane	50.000	49.688	0.6	111	0.00
76 T	1,2,3-Trichloropropane	50.000	42.874	14.3	90	0.00
77 T	Bromobenzene	50.000	49.590	0.8	106	0.00
78 T	n-propylbenzene	50.000	50.694	-1.4	103	0.00
79 T	2-Chlorotoluene	50.000	50.047	-0.1	104	0.00
80 T	1,3,5-Trimethylbenzene	50.000	51.231	-2.5	104	0.00
81 T	trans-1,4-Dichloro-2-butene	50.000	46.566	6.9	103	0.00
82 T	4-Chlorotoluene	50.000	50.455	-0.9	105	0.00
83 T	tert-Butylbenzene	50.000	52.019	-4.0	105	0.00
84 T	1,2,4-Trimethylbenzene	50.000	51.520	-3.0	105	0.00
85 T	sec-Butylbenzene	50.000	50.848	-1.7	104	0.00
86 T	p-Isopropyltoluene	50.000	51.864	-3.7	104	0.00
87 T	1,3-Dichlorobenzene	50.000	49.632	0.7	106	0.00
88 T	1,4-Dichlorobenzene	50.000	49.140	1.7	105	0.00
89 T	n-Butylbenzene	50.000	51.829	-3.7	105	0.00
90 T	Hexachloroethane	50.000	49.116	1.8	105	0.00
91 T	1,2-Dichlorobenzene	50.000	49.698	0.6	106	0.00
92 T	1,2-Dibromo-3-Chloropropane	50.000	48.687	2.6	107	0.00
93 T	1,2,4-Trichlorobenzene	50.000	51.138	-2.3	107	0.00
94 T	Hexachlorobutadiene	50.000	50.061	-0.1	104	0.00
95 T	Naphthalene	50.000	52.154	-4.3	109	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
Data File : VY023391.D
Acq On : 07 Oct 2025 14:12
Operator : SY/MD
Sample : VSTDICV050
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
ICVVY100725

Quant Time: Oct 08 05:15:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 05:12:50 2025
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
96 T	1,2,3-Trichlorobenzene	50.000	51.172	-2.3	108	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 6

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
 Data File : VY023391.D
 Acq On : 07 Oct 2025 14:12
 Operator : SY/MD
 Sample : VSTDICV050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 ICVVY100725

Quant Time: Oct 08 05:15:49 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	1.000	1.000	0.0	97	0.00
2 T	Dichlorodifluoromethane	0.360	0.323	10.3	98	0.00
3 P	Chloromethane	0.490	0.515	-5.1	112	0.00
4 C	Vinyl Chloride	0.639	0.632	1.1#	103	0.00
5 T	Bromomethane	0.536	0.524	2.2	109	0.00
6 T	Chloroethane	0.435	0.447	-2.8	105	0.00
7 T	Trichlorofluoromethane	0.887	0.862	2.8	100	0.00
8 T	Diethyl Ether	0.232	0.237	-2.2	107	0.00
9 T	1,1,2-Trichlorotrifluoroeth	0.460	0.448	2.6	100	0.00
10 T	Methyl Iodide	0.512	0.531	-3.7	96	0.00
11 T	Tert butyl alcohol	0.031	0.029	6.5	112	0.00
12 CM	1,1-Dichloroethene	0.446	0.443	0.7#	101	0.00
13 T	Acrolein	0.044	0.043	2.3	101	0.00
14 T	Allyl chloride	0.544	0.551	-1.3	102	0.00
15 T	Acrylonitrile	0.089	0.089	0.0	106	0.00
16 T	Acetone	0.100	0.085	15.0	99	0.00
17 T	Carbon Disulfide	1.277	1.277	0.0	101	0.00
18 T	Methyl Acetate	0.261	0.263	-0.8	104	0.00
19 T	Methyl tert-butyl Ether	1.072	1.120	-4.5	107	0.00
20 T	Methylene Chloride	0.538	0.565	-5.0	120	0.00
21 T	trans-1,2-Dichloroethene	0.491	0.506	-3.1	105	0.00
22 T	Diisopropyl ether	1.202	1.235	-2.7	103	0.00
23 T	Vinyl Acetate	0.651	0.679	-4.3	106	0.00
24 P	1,1-Dichloroethane	0.796	0.808	-1.5	104	0.00
25 T	2-Butanone	0.122	0.113	7.4	105	0.00
26 T	2,2-Dichloropropane	0.731	0.725	0.8	100	0.00
27 T	cis-1,2-Dichloroethene	0.567	0.595	-4.9	107	0.00
28 T	Bromochloromethane	0.297	0.270	9.1	99	0.00
29 T	Tetrahydrofuran	0.069	0.070	-1.4	107	0.00
30 C	Chloroform	0.875	0.895	-2.3#	104	0.00
31 T	Cyclohexane	0.696	0.660	5.2	100	0.00
32 T	1,1,1-Trichloroethane	0.795	0.794	0.1	101	0.00
33 S	1,2-Dichloroethane-d4	0.418	0.414	1.0	103	0.00
34 I	1,4-Difluorobenzene	1.000	1.000	0.0	100	0.00
35 S	Dibromofluoromethane	0.307	0.302	1.6	101	0.00
36 T	1,1-Dichloropropene	0.407	0.405	0.5	102	0.00
37 T	Ethyl Acetate	0.161	0.160	0.6	107	0.00
38 T	Carbon Tetrachloride	0.493	0.480	2.6	100	0.00
39 T	Methylcyclohexane	0.530	0.529	0.2	101	0.00
40 TM	Benzene	1.288	1.286	0.2	102	0.00
41 T	Methacrylonitrile	0.087	0.084	3.4	105	0.00
42 TM	1,2-Dichloroethane	0.332	0.328	1.2	104	0.00
43 T	Isopropyl Acetate	0.321	0.325	-1.2	108	0.00
44 TM	Trichloroethene	0.377	0.370	1.9	101	0.00
45 C	1,2-Dichloropropane	0.285	0.287	-0.7#	105	0.00
46 T	Dibromomethane	0.180	0.183	-1.7	106	0.00
47 T	Bromodichloromethane	0.453	0.457	-0.9	104	0.00
48 T	Methyl methacrylate	0.151	0.149	1.3	101	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
 Data File : VY023391.D
 Acq On : 07 Oct 2025 14:12
 Operator : SY/MD
 Sample : VSTDICV050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 ICVVY100725

Quant Time: Oct 08 05:15:49 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	0.002	0.002	0.0	110	0.00
50 S	Toluene-d8	1.144	1.126	1.6	100	0.00
51 T	4-Methyl-2-Pentanone	0.166	0.168	-1.2	106	0.00
52 CM	Toluene	0.836	0.862	-3.1#	105	0.00
53 T	t-1,3-Dichloropropene	0.394	0.403	-2.3	105	0.00
54 T	cis-1,3-Dichloropropene	0.465	0.480	-3.2	106	0.00
55 T	1,1,2-Trichloroethane	0.242	0.244	-0.8	106	0.00
56 T	Ethyl methacrylate	0.279	0.298	-6.8	107	0.00
57 T	1,3-Dichloropropane	0.383	0.392	-2.3	105	0.00
58 T	2-Chloroethyl Vinyl ether	0.125	0.136	-8.8	106	0.00
59 T	2-Hexanone	0.119	0.116	2.5	105	0.00
60 T	Dibromochloromethane	0.339	0.346	-2.1	106	0.00
61 T	1,2-Dibromoethane	0.231	0.234	-1.3	105	0.00
62 S	4-Bromofluorobenzene	0.378	0.377	0.3	104	0.00
63 I	Chlorobenzene-d5	1.000	1.000	0.0	103	0.00
64 T	Tetrachloroethene	0.516	0.497	3.7	98	0.00
65 PM	Chlorobenzene	1.087	1.074	1.2	105	0.00
66 T	1,1,1,2-Tetrachloroethane	0.388	0.384	1.0	106	0.00
67 C	Ethyl Benzene	1.760	1.790	-1.7#	104	0.00
68 T	m/p-Xylenes	0.706	0.718	-1.7	103	0.00
69 T	o-Xylene	0.662	0.683	-3.2	105	0.00
70 T	Styrene	1.089	1.135	-4.2	105	0.00
71 P	Bromoform	0.240	0.241	-0.4	108	0.00
72 I	1,4-Dichlorobenzene-d4	1.000	1.000	0.0	103	0.00
73 T	Isopropylbenzene	3.295	3.316	-0.6	103	0.00
74 T	N-amyl acetate	0.592	0.605	-2.2	108	0.00
75 P	1,1,2,2-Tetrachloroethane	0.539	0.536	0.6	111	0.00
76 T	1,2,3-Trichloropropane	0.441	0.378	14.3	90	0.00
77 T	Bromobenzene	0.876	0.869	0.8	106	0.00
78 T	n-propylbenzene	3.813	3.866	-1.4	103	0.00
79 T	2-Chlorotoluene	2.233	2.235	-0.1	104	0.00
80 T	1,3,5-Trimethylbenzene	2.663	2.728	-2.4	104	0.00
81 T	trans-1,4-Dichloro-2-butene	0.180	0.168	6.7	103	0.00
82 T	4-Chlorotoluene	2.300	2.321	-0.9	105	0.00
83 T	tert-Butylbenzene	2.458	2.558	-4.1	105	0.00
84 T	1,2,4-Trimethylbenzene	2.657	2.738	-3.0	105	0.00
85 T	sec-Butylbenzene	3.527	3.586	-1.7	104	0.00
86 T	p-Isopropyltoluene	3.003	3.115	-3.7	104	0.00
87 T	1,3-Dichlorobenzene	1.706	1.693	0.8	106	0.00
88 T	1,4-Dichlorobenzene	1.685	1.656	1.7	105	0.00
89 T	n-Butylbenzene	2.616	2.712	-3.7	105	0.00
90 T	Hexachloroethane	0.646	0.634	1.9	105	0.00
91 T	1,2-Dichlorobenzene	1.496	1.487	0.6	106	0.00
92 T	1,2-Dibromo-3-Chloropropane	0.088	0.086	2.3	107	0.00
93 T	1,2,4-Trichlorobenzene	0.932	0.954	-2.4	107	0.00
94 T	Hexachlorobutadiene	0.581	0.582	-0.2	104	0.00
95 T	Naphthalene	1.485	1.549	-4.3	109	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
Data File : VY023391.D
Acq On : 07 Oct 2025 14:12
Operator : SY/MD
Sample : VSTDICV050
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
ICVVY100725

Quant Time: Oct 08 05:15:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 05:12:50 2025
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
96 T	1,2,3-Trichlorobenzene	0.808	0.827	-2.4	108	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 6



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE CONTINUING CALIBRATION CHECK

Lab Name:	<u>Alliance</u>	Contract:	<u>SCIA01</u>
Lab Code:	<u>ACE</u>	SDG No.:	<u>Q3410</u>
Instrument ID:	<u>MSVOA_Y</u>	Calibration Date/Time:	<u>10/21/2025 09:05</u>
Lab File ID:	<u>VY023521.D</u>	Init. Calib. Date(s):	<u>10/07/2025 10/07/2025</u>
Heated Purge: (Y/N)	<u>Y</u>	Init. Calib. Time(s):	<u>09:17 12:32</u>
GC Column:	<u>RXI-624</u>	ID:	<u>0.25</u> (mm)

COMPOUND	RRF	RRF050	MIN RRF	%D	MAX%D
Dichlorodifluoromethane	0.360	0.323		-10.28	20
Chloromethane	0.490	0.450	0.1	-8.16	20
Vinyl Chloride	0.639	0.605		-5.32	20
Bromomethane	0.536	0.513		-4.29	20
Chloroethane	0.435	0.447		2.76	20
Trichlorofluoromethane	0.887	0.883		-0.45	20
1,1,2-Trichlorotrifluoroethane	0.460	0.490		6.52	20
1,1-Dichloroethene	0.446	0.455		2.02	20
Acetone	0.100	0.113		13	20
Carbon Disulfide	1.277	1.260		-1.33	20
Methyl tert-butyl Ether	1.072	1.116		4.1	20
Methyl Acetate	0.261	0.303		16.09	20
Methylene Chloride	0.538	0.509		-5.39	20
trans-1,2-Dichloroethene	0.491	0.520		5.91	20
1,1-Dichloroethane	0.796	0.840	0.1	5.53	20
Cyclohexane	0.696	0.643		-7.61	20
2-Butanone	0.122	0.124		1.64	20
Carbon Tetrachloride	0.493	0.562		14	20
cis-1,2-Dichloroethene	0.567	0.614		8.29	20
Bromochloromethane	0.297	0.269		-9.43	20
Chloroform	0.875	0.960		9.71	20
1,1,1-Trichloroethane	0.795	0.859		8.05	20
Methylcyclohexane	0.530	0.568		7.17	20
Benzene	1.288	1.448		12.42	20
1,2-Dichloroethane	0.332	0.360		8.43	20
Trichloroethene	0.377	0.421		11.67	20
1,2-Dichloropropane	0.285	0.320		12.28	20
Bromodichloromethane	0.453	0.522		15.23	20
4-Methyl-2-Pentanone	0.166	0.186		12.05	20
Toluene	0.836	0.967		15.67	20
t-1,3-Dichloropropene	0.394	0.441		11.93	20
cis-1,3-Dichloropropene	0.465	0.524		12.69	20
1,1,2-Trichloroethane	0.242	0.285		17.77	20
2-Hexanone	0.119	0.135		13.44	20
Dibromochloromethane	0.339	0.403		18.88	20
1,2-Dibromoethane	0.231	0.269		16.45	20
Tetrachloroethene	0.516	0.575		11.43	20
Chlorobenzene	1.087	1.181	0.3	8.65	20

All other compounds must meet a minimum RRF of 0.010.
RRF of 1,4-Dioxane = Value should be divide by 1000.



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE CONTINUING CALIBRATION CHECK

Lab Name:	<u>Alliance</u>	Contract:	<u>SCIA01</u>
Lab Code:	<u>ACE</u>	SDG No.:	<u>Q3410</u>
Instrument ID:	<u>MSVOA_Y</u>	Calibration Date/Time:	<u>10/21/2025 09:05</u>
Lab File ID:	<u>VY023521.D</u>	Init. Calib. Date(s):	<u>10/07/2025 10/07/2025</u>
Heated Purge: (Y/N)	<u>Y</u>	Init. Calib. Time(s):	<u>09:17 12:32</u>
GC Column:	<u>RXI-624</u>	ID:	<u>0.25</u> (mm)

COMPOUND	RRF	RRF050	MIN RRF	%D	MAX%D
Ethyl Benzene	1.760	1.961		11.42	20
m/p-Xylenes	0.706	0.799		13.17	20
o-Xylene	0.662	0.739		11.63	20
Styrene	1.089	1.261		15.79	20
Bromoform	0.240	0.269	0.1	12.08	20
Isopropylbenzene	3.295	3.640		10.47	20
1,1,2,2-Tetrachloroethane	0.539	0.571	0.3	5.94	20
1,3-Dichlorobenzene	1.706	1.887		10.61	20
1,4-Dichlorobenzene	1.685	1.813		7.6	20
1,2-Dichlorobenzene	1.496	1.634		9.23	20
1,2-Dibromo-3-Chloropropane	0.088	0.088		0	20
1,2,4-Trichlorobenzene	0.932	0.982		5.36	20
1,2,3-Trichlorobenzene	0.808	0.843		4.33	20
1,2-Dichloroethane-d4	0.418	0.408		-2.39	20
Dibromofluoromethane	0.307	0.331		7.82	20
Toluene-d8	1.144	1.218		6.47	20
4-Bromofluorobenzene	0.378	0.405		7.14	20

All other compounds must meet a minimum RRF of 0.010.
RRF of 1,4-Dioxane = Value should be divide by 1000.

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
 Data File : VY023521.D
 Acq On : 21 Oct 2025 09:05
 Operator : SY/MD
 Sample : VSTDCCC050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDCCC050

Manual Integrations
 APPROVED

Reviewed By :Amit Patel 10/24/2025
 Supervised By :Mahesh Dadoda 10/27/2025

Quant Time: Oct 24 01:20:49 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.713	168	499961	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	698196	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	642915	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	341616	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.067	65	203881	48.767	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery =	97.540%		
35) Dibromofluoromethane	7.640	113	231392	53.936	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery =	107.880%		
50) Toluene-d8	10.109	98	850239	53.217	ug/l	0.00
Spiked Amount 50.000	Range 58 - 134		Recovery =	106.440%		
62) 4-Bromofluorobenzene	12.408	95	283018	53.656	ug/l	0.00
Spiked Amount 50.000	Range 30 - 143		Recovery =	107.320%		
Target Compounds					Qvalue	
2) Dichlorodifluoromethane	1.867	85	161266	44.813	ug/l	99
3) Chloromethane	2.074	50	225042	45.905	ug/l	98
4) Vinyl Chloride	2.208	62	302535	47.380	ug/l	98
5) Bromomethane	2.599	94	256539	47.876	ug/l	99
6) Chloroethane	2.739	64	223248	51.292	ug/l	98
7) Trichlorofluoromethane	3.062	101	441619	49.812	ug/l	100
8) Diethyl Ether	3.458	74	116040	50.089	ug/l	97
9) 1,1,2-Trichlorotrifluo...	3.818	101	245222	53.302	ug/l	100
10) Methyl Iodide	4.013	142	289234	56.473	ug/l	100
11) Tert butyl alcohol	4.848	59	86251	277.313	ug/l	97
12) 1,1-Dichloroethene	3.793	96	227578	51.029	ug/l	97
13) Acrolein	3.653	56	37204	84.654	ug/l	97
14) Allyl chloride	4.391	41	261207	48.058	ug/l	97
15) Acrylonitrile	5.062	53	233934	263.862	ug/l	99
16) Acetone	3.867	43	282507	283.840	ug/l	100
17) Carbon Disulfide	4.110	76	629852	49.345	ug/l	99
18) Methyl Acetate	4.385	43	151375	57.978	ug/l	100
19) Methyl tert-butyl Ether	5.122	73	557973	52.056	ug/l	97
20) Methylene Chloride	4.616	84	254490	47.285	ug/l	98
21) trans-1,2-Dichloroethene	5.116	96	259786	52.909	ug/l	97
22) Diisopropyl ether	6.025	45	622406	51.770	ug/l	98
23) Vinyl Acetate	5.964	43	1615658	248.276	ug/l	96
24) 1,1-Dichloroethane	5.921	63	420141	52.756	ug/l	98
25) 2-Butanone	6.897	43	310606	255.620	ug/l	99
26) 2,2-Dichloropropane	6.890	77	391432	53.566	ug/l	99
27) cis-1,2-Dichloroethene	6.897	96	307121	54.150	ug/l	96
28) Bromochloromethane	7.250	49	134434	45.218	ug/l	95
29) Tetrahydrofuran	7.262	42	171000	248.167	ug/l	94
30) Chloroform	7.427	83	479911	54.848	ug/l	100
31) Cyclohexane	7.707	56	321670	46.252	ug/l	94
32) 1,1,1-Trichloroethane	7.622	97	429628	54.031	ug/l	100
36) 1,1-Dichloropropene	7.841	75	318835	56.137	ug/l	100
37) Ethyl Acetate	6.988	43	120965	53.760	ug/l	99
38) Carbon Tetrachloride	7.823	117	392576	57.004	ug/l	98
39) Methylcyclohexane	9.110	83	396680	53.642	ug/l	100
40) Benzene	8.085	78	1010667	56.189	ug/l	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
 Data File : VY023521.D
 Acq On : 21 Oct 2025 09:05
 Operator : SY/MD
 Sample : VSTDCCC050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDCCC050

Manual Integrations
 APPROVED

Reviewed By :Amit Patel 10/24/2025
 Supervised By :Mahesh Dadoda 10/27/2025

Quant Time: Oct 24 01:20:49 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	7.220	41	56462	46.396	ug/l #	88
42) 1,2-Dichloroethane	8.159	62	251229	54.158	ug/l	98
43) Isopropyl Acetate	8.201	43	231909	51.687	ug/l #	85
44) Trichloroethene	8.866	130	294037	55.852	ug/l	99
45) 1,2-Dichloropropane	9.140	63	223488	56.253	ug/l	98
46) Dibromomethane	9.232	93	146935	58.489	ug/l	98
47) Bromodichloromethane	9.427	83	364567	57.621	ug/l	98
48) Methyl methacrylate	9.225	41	110852	52.590	ug/l	94
49) 1,4-Dioxane	9.225	88	30619	1051.234	ug/l	97
51) 4-Methyl-2-Pentanone	10.000	43	649884	280.345	ug/l	99
52) Toluene	10.170	92	675233	57.818	ug/l	99
53) t-1,3-Dichloropropene	10.396	75	307992	55.984	ug/l	98
54) cis-1,3-Dichloropropene	9.859	75	366195	56.399	ug/l	99
55) 1,1,2-Trichloroethane	10.573	97	198692	58.815	ug/l	95
56) Ethyl methacrylate	10.439	69	222590	57.121	ug/l	97
57) 1,3-Dichloropropane	10.719	76	307111	57.370	ug/l	100
58) 2-Chloroethyl Vinyl ether	9.713	63	488816	280.014	ug/l	99
59) 2-Hexanone	10.762	43	472202	285.033	ug/l	99
60) Dibromochloromethane	10.914	129	281057	59.341	ug/l	100
61) 1,2-Dibromoethane	11.018	107	187844	58.304	ug/l	100
64) Tetrachloroethene	10.646	164	369674	55.688	ug/l	99
65) Chlorobenzene	11.445	112	759409	54.309	ug/l	98
66) 1,1,1,2-Tetrachloroethane	11.518	131	280381	56.268	ug/l	99
67) Ethyl Benzene	11.518	91	1261040	55.713	ug/l	99
68) m/p-Xylenes	11.627	106	1027756	113.207	ug/l	99
69) o-Xylene	11.957	106	475420	55.830	ug/l	99
70) Styrene	11.969	104	810694	57.893	ug/l	99
71) Bromoform	12.133	173	173149	56.019	ug/l #	98
73) Isopropylbenzene	12.255	105	1243608	55.240	ug/l	100
74) N-amyl acetate	12.072	43	202085	49.976	ug/l	97
75) 1,1,2,2-Tetrachloroethane	12.505	83	195187	53.009	ug/l	99
76) 1,2,3-Trichloropropane	12.560	75	151087m	50.129	ug/l	
77) Bromobenzene	12.530	156	324603	54.235	ug/l	99
78) n-propylbenzene	12.597	91	1457896	55.961	ug/l	99
79) 2-Chlorotoluene	12.682	91	830894	54.463	ug/l	99
80) 1,3,5-Trimethylbenzene	12.737	105	1026971	56.451	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.304	75	61955	50.407	ug/l	99
82) 4-Chlorotoluene	12.780	91	868701	55.289	ug/l	100
83) tert-Butylbenzene	12.999	119	937982	55.842	ug/l	99
84) 1,2,4-Trimethylbenzene	13.042	105	1024486	56.428	ug/l	100
85) sec-Butylbenzene	13.176	105	1359841	56.437	ug/l	100
86) p-Isopropyltoluene	13.292	119	1176613	57.354	ug/l	100
87) 1,3-Dichlorobenzene	13.286	146	644461	55.296	ug/l	100
88) 1,4-Dichlorobenzene	13.365	146	619278	53.800	ug/l	100
89) n-Butylbenzene	13.615	91	1006298	56.295	ug/l	99
90) Hexachloroethane	13.877	117	238499	54.052	ug/l	99
91) 1,2-Dichlorobenzene	13.658	146	558110	54.620	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	14.273	75	29948	49.569	ug/l	96
93) 1,2,4-Trichlorobenzene	14.919	180	335488	52.665	ug/l	99
94) Hexachlorobutadiene	15.023	225	215262	54.210	ug/l	100
95) Naphthalene	15.145	128	523602	51.618	ug/l	100
96) 1,2,3-Trichlorobenzene	15.328	180	288040	52.203	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
Data File : VY023521.D
Acq On : 21 Oct 2025 09:05
Operator : SY/MD
Sample : VSTDCCC050
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Amit Patel 10/24/2025
Supervised By :Mahesh Dadoda 10/27/2025

Quant Time: Oct 24 01:20:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 05:12:50 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
 Data File : VY023521.D
 Acq On : 21 Oct 2025 09:05
 Operator : SY/MD
 Sample : VSTDCCC050
 Misc : 5.00g/5.0mL/MSVOA_Y/soil
 ALS Vial : 2 Sample Multiplier: 1

Instrument :

MSVOA_Y

ClientSampleId :

VSTDCCC050

Manual Integrations

APPROVED

Reviewed By :Amit Patel 10/24/2025

Supervised By :Mahesh Dadoda 10/27/2025


Quant Time: Oct 24 01:20:49 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M

Quant Title : SW846 8260

QLast Update : Wed Oct 08 05:12:50 2025

Response via : Initial Calibration

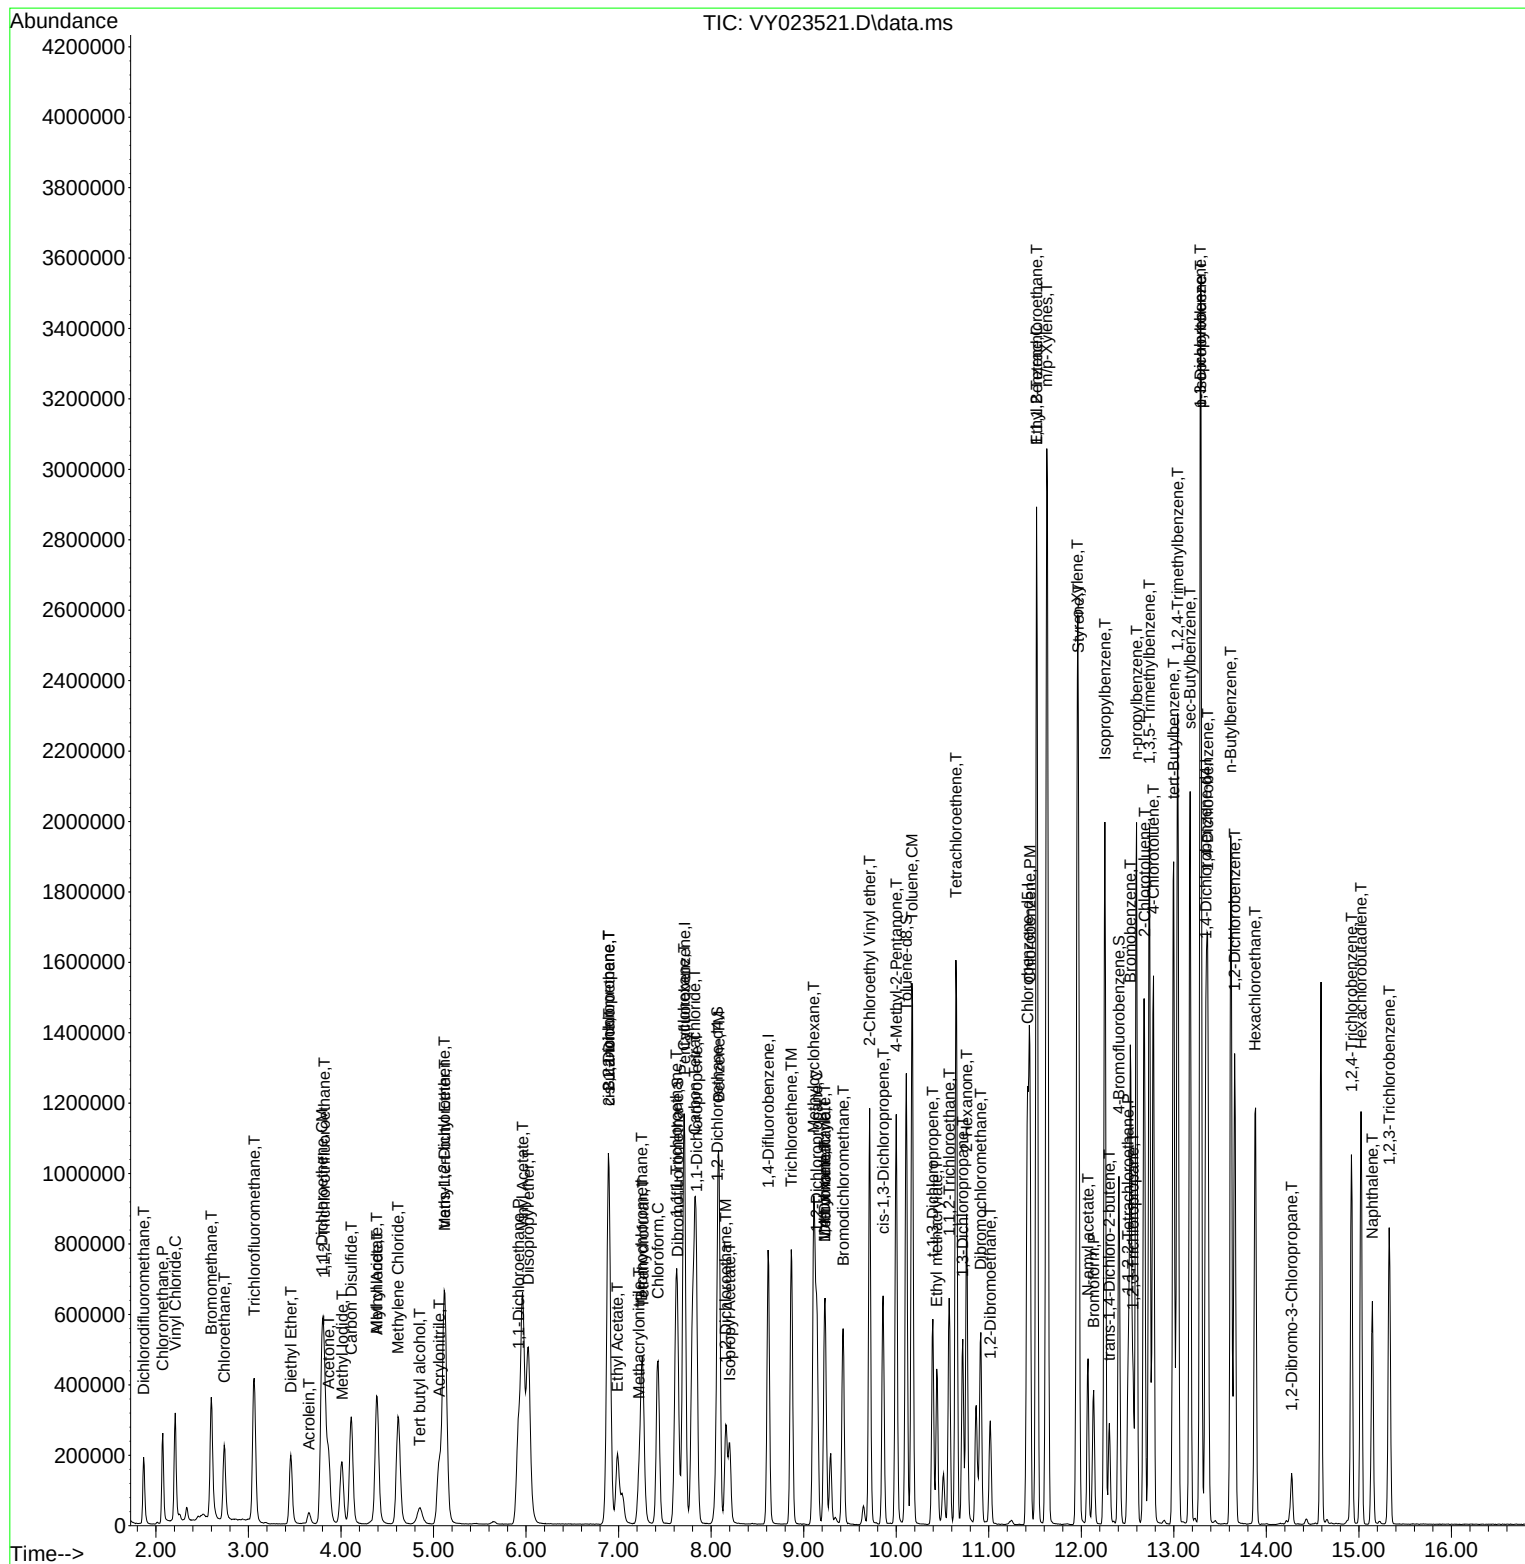

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
 Data File : VY023521.D
 Acq On : 21 Oct 2025 09:05
 Operator : SY/MD
 Sample : VSTDCCC050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 LabSampleId :
 VSTDCCC050

Quant Time: Oct 24 01:20:49 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	1.000	1.000	0.0	85	0.00
2 T	Dichlorodifluoromethane	0.360	0.323	10.3	85	0.00
3 P	Chloromethane	0.490	0.450	8.2	85	0.00
4 C	Vinyl Chloride	0.639	0.605	5.3#	86	0.00
5 T	Bromomethane	0.536	0.513	4.3	93	0.00
6 T	Chloroethane	0.435	0.447	-2.8	91	0.00
7 T	Trichlorofluoromethane	0.887	0.883	0.5	89	0.00
8 T	Diethyl Ether	0.232	0.232	0.0	92	0.00
9 T	1,1,2-Trichlorotrifluoroeth	0.460	0.490	-6.5	95	0.00
10 T	Methyl Iodide	0.512	0.579	-13.1	91	0.01
11 T	Tert butyl alcohol	0.031	0.035	-12.9	117	-0.01
12 CM	1,1-Dichloroethene	0.446	0.455	-2.0#	90	0.00
13 T	Acrolein	0.044	0.015	65.9#	30#	0.00
14 T	Allyl chloride	0.544	0.522	4.0	84	0.01
15 T	Acrylonitrile	0.089	0.094	-5.6	97	0.00
16 T	Acetone	0.100	0.113	-13.0	114	0.00
17 T	Carbon Disulfide	1.277	1.260	1.3	87	0.00
18 T	Methyl Acetate	0.261	0.303	-16.1	105	0.00
19 T	Methyl tert-butyl Ether	1.072	1.116	-4.1	93	0.00
20 T	Methylene Chloride	0.538	0.509	5.4	94	0.00
21 T	trans-1,2-Dichloroethene	0.491	0.520	-5.9	94	0.00
22 T	Diisopropyl ether	1.202	1.245	-3.6	91	0.00
23 T	Vinyl Acetate	0.651	0.646	0.8	88	0.00
24 P	1,1-Dichloroethane	0.796	0.840	-5.5	94	0.00
25 T	2-Butanone	0.122	0.124	-1.6	100	0.00
26 T	2,2-Dichloropropane	0.731	0.783	-7.1	94	0.00
27 T	cis-1,2-Dichloroethene	0.567	0.614	-8.3	96	0.00
28 T	Bromochloromethane	0.297	0.269	9.4	85	0.00
29 T	Tetrahydrofuran	0.069	0.068	1.4	91	0.00
30 C	Chloroform	0.875	0.960	-9.7#	97	0.00
31 T	Cyclohexane	0.696	0.643	7.6	85	0.00
32 T	1,1,1-Trichloroethane	0.795	0.859	-8.1	95	0.00
33 S	1,2-Dichloroethane-d4	0.418	0.408	2.4	88	0.00
34 I	1,4-Difluorobenzene	1.000	1.000	0.0	81	0.00
35 S	Dibromofluoromethane	0.307	0.331	-7.8	90	0.00
36 T	1,1-Dichloropropene	0.407	0.457	-12.3	93	0.00
37 T	Ethyl Acetate	0.161	0.173	-7.5	94	0.00
38 T	Carbon Tetrachloride	0.493	0.562	-14.0	95	0.00
39 T	Methylcyclohexane	0.530	0.568	-7.2	88	0.00
40 TM	Benzene	1.288	1.448	-12.4	94	0.00
41 T	Methacrylonitrile	0.087	0.081	6.9	82	0.00
42 TM	1,2-Dichloroethane	0.332	0.360	-8.4	93	0.00
43 T	Isopropyl Acetate	0.321	0.332	-3.4	90	0.00
44 TM	Trichloroethene	0.377	0.421	-11.7	93	0.00
45 C	1,2-Dichloropropane	0.285	0.320	-12.3#	95	0.00
46 T	Dibromomethane	0.180	0.210	-16.7	99	0.00
47 T	Bromodichloromethane	0.453	0.522	-15.2	97	0.00
48 T	Methyl methacrylate	0.151	0.159	-5.3	87	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
 Data File : VY023521.D
 Acq On : 21 Oct 2025 09:05
 Operator : SY/MD
 Sample : VSTDCCC050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 LabSampleId :
 VSTDCCC050

Quant Time: Oct 24 01:20:49 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	0.002	0.002	0.0	90	0.00
50 S	Toluene-d8	1.144	1.218	-6.5	88	0.00
51 T	4-Methyl-2-Pentanone	0.166	0.186	-12.0	95	0.00
52 CM	Toluene	0.836	0.967	-15.7#	95	0.00
53 T	t-1,3-Dichloropropene	0.394	0.441	-11.9	93	0.00
54 T	cis-1,3-Dichloropropene	0.465	0.524	-12.7	94	0.00
55 T	1,1,2-Trichloroethane	0.242	0.285	-17.8	100	0.00
56 T	Ethyl methacrylate	0.279	0.319	-14.3	93	0.00
57 T	1,3-Dichloropropane	0.383	0.440	-14.9	96	0.00
58 T	2-Chloroethyl Vinyl ether	0.125	0.140	-12.0	88	0.00
59 T	2-Hexanone	0.119	0.135	-13.4	98	0.00
60 T	Dibromochloromethane	0.339	0.403	-18.9	100	0.00
61 T	1,2-Dibromoethane	0.231	0.269	-16.5	98	0.00
62 S	4-Bromofluorobenzene	0.378	0.405	-7.1	90	0.00
63 I	Chlorobenzene-d5	1.000	1.000	0.0	86	0.00
64 T	Tetrachloroethene	0.516	0.575	-11.4	94	0.00
65 PM	Chlorobenzene	1.087	1.181	-8.6	96	0.00
66 T	1,1,1,2-Tetrachloroethane	0.388	0.436	-12.4	100	0.00
67 C	Ethyl Benzene	1.760	1.961	-11.4#	95	0.00
68 T	m/p-Xylenes	0.706	0.799	-13.2	95	0.00
69 T	o-Xylene	0.662	0.739	-11.6	95	0.00
70 T	Styrene	1.089	1.261	-15.8	97	0.00
71 P	Bromoform	0.240	0.269	-12.1	100	0.00
72 I	1,4-Dichlorobenzene-d4	1.000	1.000	0.0	87	0.00
73 T	Isopropylbenzene	3.295	3.640	-10.5	96	0.00
74 T	N-amyl acetate	0.592	0.592	0.0	89	0.00
75 P	1,1,2,2-Tetrachloroethane	0.539	0.571	-5.9	100	0.00
76 T	1,2,3-Trichloropropane	0.441	0.442	-0.2	89	0.00
77 T	Bromobenzene	0.876	0.950	-8.4	98	0.00
78 T	n-propylbenzene	3.813	4.268	-11.9	96	0.00
79 T	2-Chlorotoluene	2.233	2.432	-8.9	95	0.00
80 T	1,3,5-Trimethylbenzene	2.663	3.006	-12.9	97	0.00
81 T	trans-1,4-Dichloro-2-butene	0.180	0.181	-0.6	93	0.00
82 T	4-Chlorotoluene	2.300	2.543	-10.6	97	0.00
83 T	tert-Butylbenzene	2.458	2.746	-11.7	95	0.00
84 T	1,2,4-Trimethylbenzene	2.657	2.999	-12.9	97	0.00
85 T	sec-Butylbenzene	3.527	3.981	-12.9	97	0.00
86 T	p-Isopropyltoluene	3.003	3.444	-14.7	97	0.00
87 T	1,3-Dichlorobenzene	1.706	1.887	-10.6	99	0.00
88 T	1,4-Dichlorobenzene	1.685	1.813	-7.6	97	0.00
89 T	n-Butylbenzene	2.616	2.946	-12.6	96	0.00
90 T	Hexachloroethane	0.646	0.698	-8.0	97	0.00
91 T	1,2-Dichlorobenzene	1.496	1.634	-9.2	98	0.00
92 T	1,2-Dibromo-3-Chloropropane	0.088	0.088	0.0	92	0.00
93 T	1,2,4-Trichlorobenzene	0.932	0.982	-5.4	93	0.00
94 T	Hexachlorobutadiene	0.581	0.630	-8.4	95	0.00
95 T	Naphthalene	1.485	1.533	-3.2	91	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
Data File : VY023521.D
Acq On : 21 Oct 2025 09:05
Operator : SY/MD
Sample : VSTDCCC050
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_Y
LabSampleId :
VSTDCCC050

Quant Time: Oct 24 01:20:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 05:12:50 2025
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
96 T	1,2,3-Trichlorobenzene	0.808	0.843	-4.3	93	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 6

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
 Data File : VY023521.D
 Acq On : 21 Oct 2025 09:05
 Operator : SY/MD
 Sample : VSTDCCC050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 LabSampleId :
 VSTDCCC050

Quant Time: Oct 24 01:20:49 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	50.000	50.000	0.0	85	0.00
2 T	Dichlorodifluoromethane	50.000	44.813	10.4	85	0.00
3 P	Chloromethane	50.000	45.905	8.2	85	0.00
4 C	Vinyl Chloride	50.000	47.380	5.2#	86	0.00
5 T	Bromomethane	50.000	47.876	4.2	93	0.00
6 T	Chloroethane	50.000	51.292	-2.6	91	0.00
7 T	Trichlorofluoromethane	50.000	49.812	0.4	89	0.00
8 T	Diethyl Ether	50.000	50.089	-0.2	92	0.00
9 T	1,1,2-Trichlorotrifluoroeth	50.000	53.302	-6.6	95	0.00
10 T	Methyl Iodide	50.000	56.473	-12.9	91	0.01
11 T	Tert butyl alcohol	250.000	277.313	-10.9	117	-0.01
12 CM	1,1-Dichloroethene	50.000	51.029	-2.1#	90	0.00
13 T	Acrolein	250.000	84.654	66.1#	30	0.00
14 T	Allyl chloride	50.000	48.058	3.9	84	0.01
15 T	Acrylonitrile	250.000	263.862	-5.5	97	0.00
16 T	Acetone	250.000	283.840	-13.5	114	0.00
17 T	Carbon Disulfide	50.000	49.345	1.3	87	0.00
18 T	Methyl Acetate	50.000	57.978	-16.0	105	0.00
19 T	Methyl tert-butyl Ether	50.000	52.056	-4.1	93	0.00
20 T	Methylene Chloride	50.000	47.285	5.4	94	0.00
21 T	trans-1,2-Dichloroethene	50.000	52.909	-5.8	94	0.00
22 T	Diisopropyl ether	50.000	51.770	-3.5	91	0.00
23 T	Vinyl Acetate	250.000	248.276	0.7	88	0.00
24 P	1,1-Dichloroethane	50.000	52.756	-5.5	94	0.00
25 T	2-Butanone	250.000	255.620	-2.2	100	0.00
26 T	2,2-Dichloropropane	50.000	53.566	-7.1	94	0.00
27 T	cis-1,2-Dichloroethene	50.000	54.150	-8.3	96	0.00
28 T	Bromochloromethane	50.000	45.218	9.6	85	0.00
29 T	Tetrahydrofuran	250.000	248.167	0.7	91	0.00
30 C	Chloroform	50.000	54.848	-9.7#	97	0.00
31 T	Cyclohexane	50.000	46.252	7.5	85	0.00
32 T	1,1,1-Trichloroethane	50.000	54.031	-8.1	95	0.00
33 S	1,2-Dichloroethane-d4	50.000	48.767	2.5	88	0.00
34 I	1,4-Difluorobenzene	50.000	50.000	0.0	81	0.00
35 S	Dibromofluoromethane	50.000	53.936	-7.9	90	0.00
36 T	1,1-Dichloropropene	50.000	56.137	-12.3	93	0.00
37 T	Ethyl Acetate	50.000	53.760	-7.5	94	0.00
38 T	Carbon Tetrachloride	50.000	57.004	-14.0	95	0.00
39 T	Methylcyclohexane	50.000	53.642	-7.3	88	0.00
40 TM	Benzene	50.000	56.189	-12.4	94	0.00
41 T	Methacrylonitrile	50.000	46.396	7.2	82	0.00
42 TM	1,2-Dichloroethane	50.000	54.158	-8.3	93	0.00
43 T	Isopropyl Acetate	50.000	51.687	-3.4	90	0.00
44 TM	Trichloroethene	50.000	55.852	-11.7	93	0.00
45 C	1,2-Dichloropropane	50.000	56.253	-12.5#	95	0.00
46 T	Dibromomethane	50.000	58.489	-17.0	99	0.00
47 T	Bromodichloromethane	50.000	57.621	-15.2	97	0.00
48 T	Methyl methacrylate	50.000	52.590	-5.2	87	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
 Data File : VY023521.D
 Acq On : 21 Oct 2025 09:05
 Operator : SY/MD
 Sample : VSTDCCC050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 LabSampleId :
 VSTDCCC050

Quant Time: Oct 24 01:20:49 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	1000.000	1051.234	-5.1	90	0.00
50 S	Toluene-d8	50.000	53.217	-6.4	88	0.00
51 T	4-Methyl-2-Pentanone	250.000	280.345	-12.1	95	0.00
52 CM	Toluene	50.000	57.818	-15.6#	95	0.00
53 T	t-1,3-Dichloropropene	50.000	55.984	-12.0	93	0.00
54 T	cis-1,3-Dichloropropene	50.000	56.399	-12.8	94	0.00
55 T	1,1,2-Trichloroethane	50.000	58.815	-17.6	100	0.00
56 T	Ethyl methacrylate	50.000	57.121	-14.2	93	0.00
57 T	1,3-Dichloropropane	50.000	57.370	-14.7	96	0.00
58 T	2-Chloroethyl Vinyl ether	250.000	280.014	-12.0	88	0.00
59 T	2-Hexanone	250.000	285.033	-14.0	98	0.00
60 T	Dibromochloromethane	50.000	59.341	-18.7	100	0.00
61 T	1,2-Dibromoethane	50.000	58.304	-16.6	98	0.00
62 S	4-Bromofluorobenzene	50.000	53.656	-7.3	90	0.00
63 I	Chlorobenzene-d5	50.000	50.000	0.0	86	0.00
64 T	Tetrachloroethene	50.000	55.688	-11.4	94	0.00
65 PM	Chlorobenzene	50.000	54.309	-8.6	96	0.00
66 T	1,1,1,2-Tetrachloroethane	50.000	56.268	-12.5	100	0.00
67 C	Ethyl Benzene	50.000	55.713	-11.4#	95	0.00
68 T	m/p-Xylenes	100.000	113.207	-13.2	95	0.00
69 T	o-Xylene	50.000	55.830	-11.7	95	0.00
70 T	Styrene	50.000	57.893	-15.8	97	0.00
71 P	Bromoform	50.000	56.019	-12.0	100	0.00
72 I	1,4-Dichlorobenzene-d4	50.000	50.000	0.0	87	0.00
73 T	Isopropylbenzene	50.000	55.240	-10.5	96	0.00
74 T	N-amyl acetate	50.000	49.976	0.0	89	0.00
75 P	1,1,2,2-Tetrachloroethane	50.000	53.009	-6.0	100	0.00
76 T	1,2,3-Trichloropropane	50.000	50.129	-0.3	89	0.00
77 T	Bromobenzene	50.000	54.235	-8.5	98	0.00
78 T	n-propylbenzene	50.000	55.961	-11.9	96	0.00
79 T	2-Chlorotoluene	50.000	54.463	-8.9	95	0.00
80 T	1,3,5-Trimethylbenzene	50.000	56.451	-12.9	97	0.00
81 T	trans-1,4-Dichloro-2-butene	50.000	50.407	-0.8	93	0.00
82 T	4-Chlorotoluene	50.000	55.289	-10.6	97	0.00
83 T	tert-Butylbenzene	50.000	55.842	-11.7	95	0.00
84 T	1,2,4-Trimethylbenzene	50.000	56.428	-12.9	97	0.00
85 T	sec-Butylbenzene	50.000	56.437	-12.9	97	0.00
86 T	p-Isopropyltoluene	50.000	57.354	-14.7	97	0.00
87 T	1,3-Dichlorobenzene	50.000	55.296	-10.6	99	0.00
88 T	1,4-Dichlorobenzene	50.000	53.800	-7.6	97	0.00
89 T	n-Butylbenzene	50.000	56.295	-12.6	96	0.00
90 T	Hexachloroethane	50.000	54.052	-8.1	97	0.00
91 T	1,2-Dichlorobenzene	50.000	54.620	-9.2	98	0.00
92 T	1,2-Dibromo-3-Chloropropane	50.000	49.569	0.9	92	0.00
93 T	1,2,4-Trichlorobenzene	50.000	52.665	-5.3	93	0.00
94 T	Hexachlorobutadiene	50.000	54.210	-8.4	95	0.00
95 T	Naphthalene	50.000	51.618	-3.2	91	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
Data File : VY023521.D
Acq On : 21 Oct 2025 09:05
Operator : SY/MD
Sample : VSTDCCC050
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_Y
LabSampleId :
VSTDCCC050

Quant Time: Oct 24 01:20:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 05:12:50 2025
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
96 T	1,2,3-Trichlorobenzene	50.000	52.203	-4.4	93	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 6




QC SAMPLE DATA

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100725\
Data File : VY023383.D
Acq On : 07 Oct 2025 08:43
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Title : SW846 8260
Last Update : Wed Oct 08 05:12:50 2025

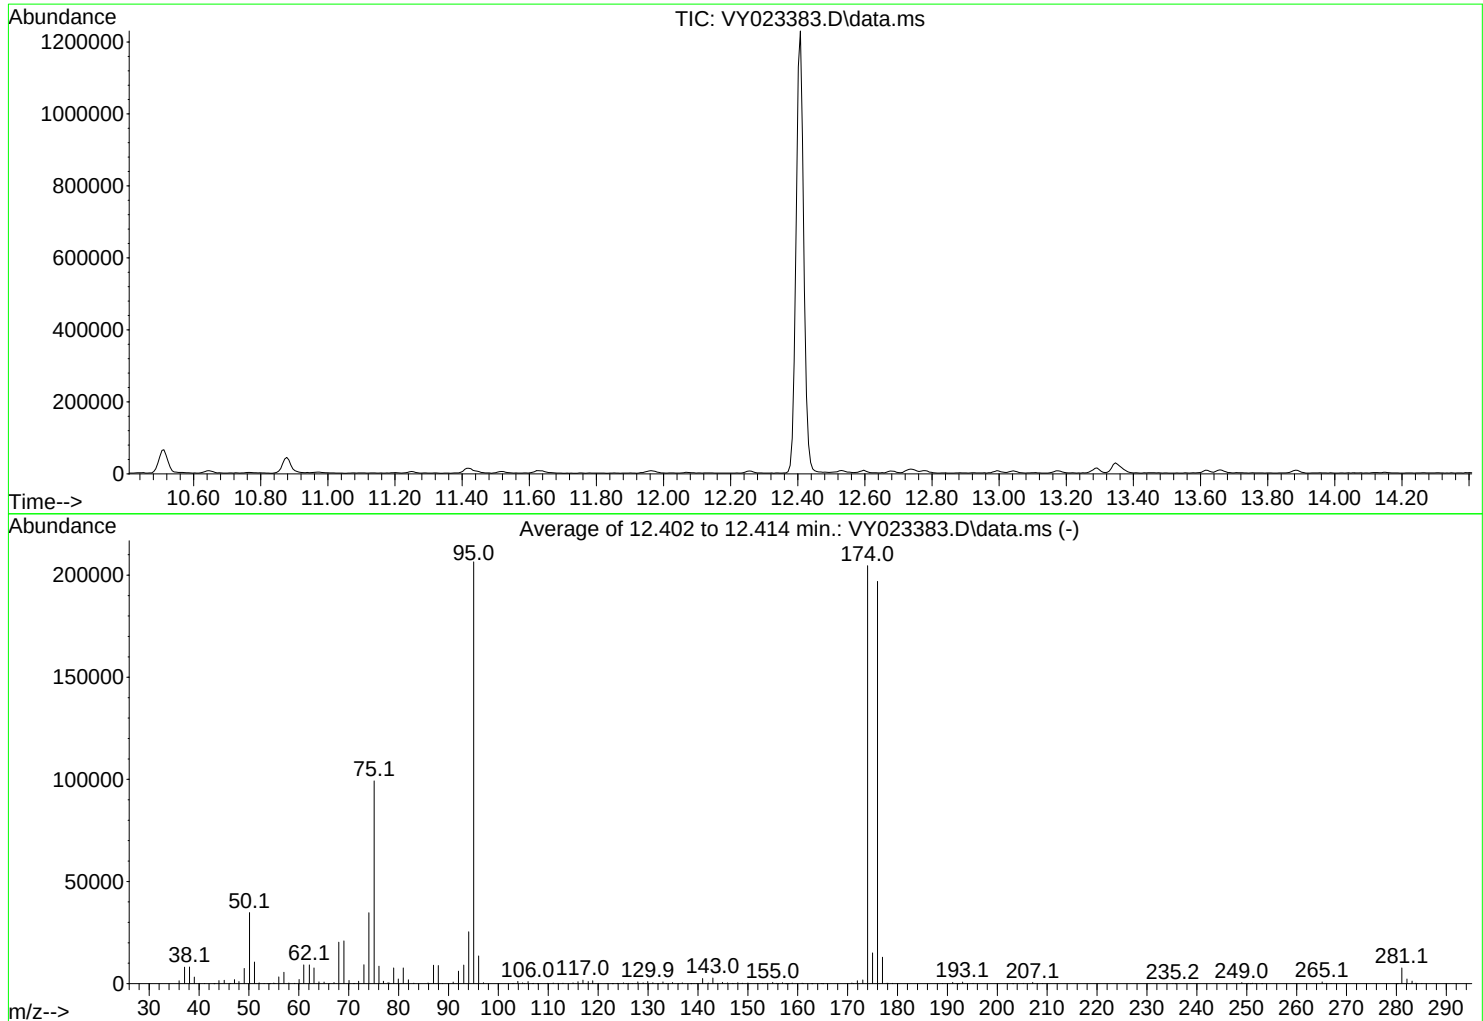

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743



Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.9	34816	PASS
75	95	30	60	48.1	99264	PASS
95	95	100	100	100.0	206507	PASS
96	95	5	9	6.6	13540	PASS
173	174	0.00	2	0.9	1817	PASS
174	95	50	100	99.1	204629	PASS
175	174	5	9	7.4	15059	PASS
176	174	95	101	96.2	196949	PASS
177	176	5	9	6.6	12912	PASS

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
Data File : VY023520.D
Acq On : 21 Oct 2025 08:29
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Title : SW846 8260
Last Update : Wed Oct 08 05:12:50 2025

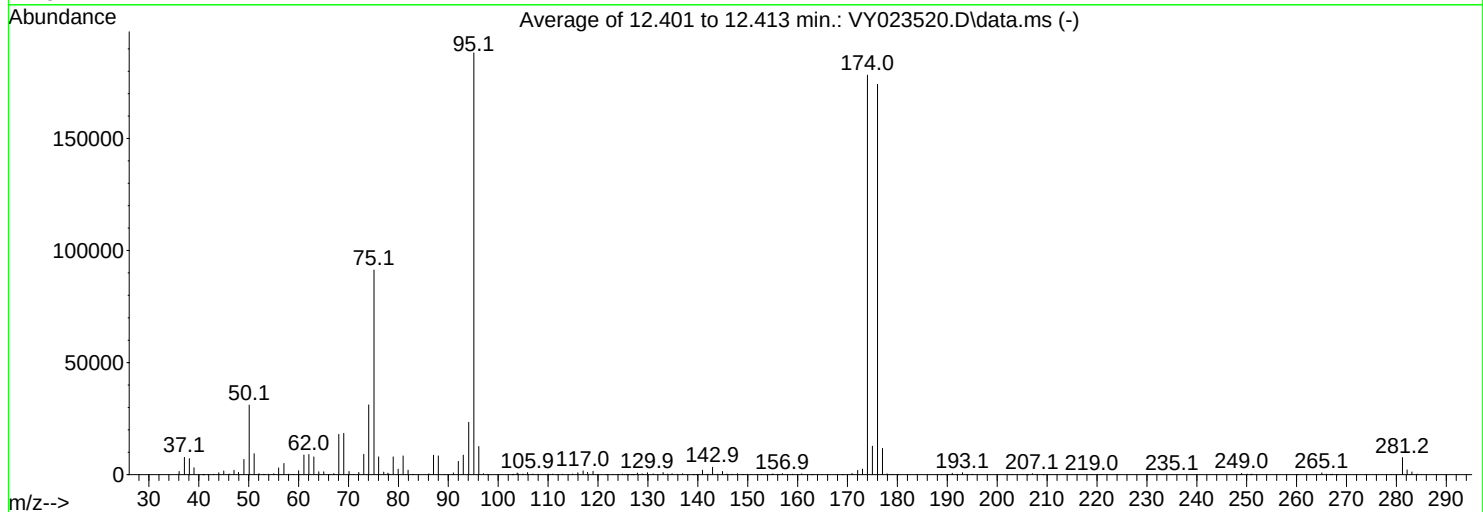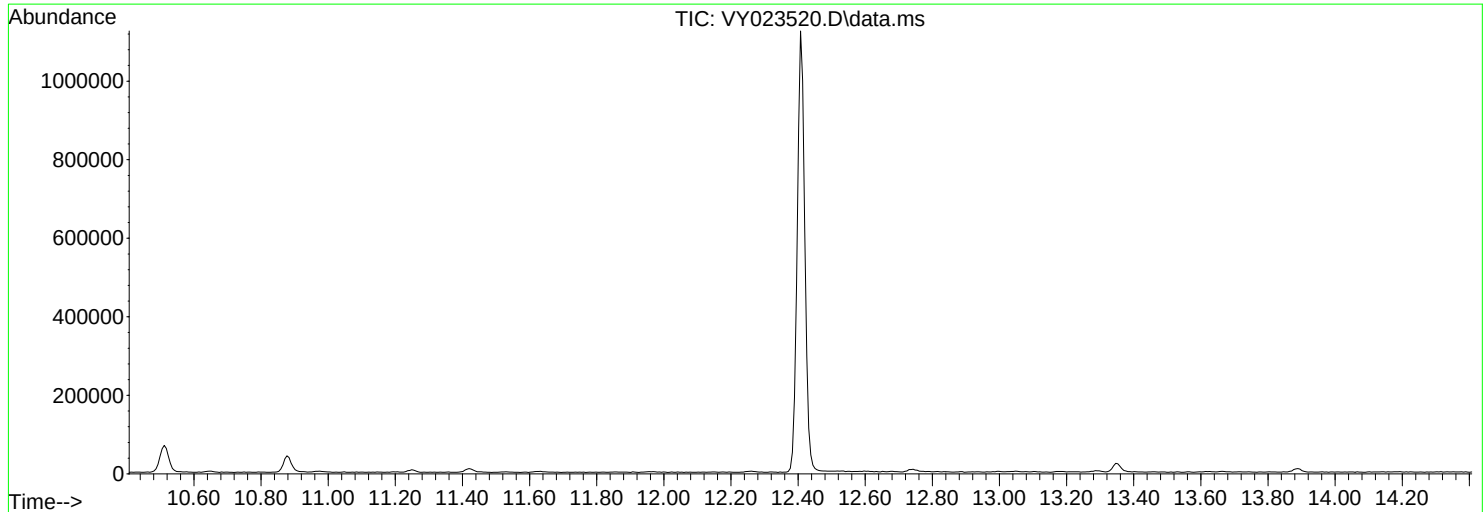

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	31051	PASS
75	95	30	60	48.5	91288	PASS
95	95	100	100	100.0	188203	PASS
96	95	5	9	6.7	12595	PASS
173	174	0.00	2	1.4	2489	PASS
174	95	50	100	94.7	178283	PASS
175	174	5	9	7.1	12726	PASS
176	174	95	101	97.7	174101	PASS
177	176	5	9	6.7	11711	PASS

Report of Analysis

Client: Sciacca General Contractors, LLC

Project: 49 Moore Place Belleville

Client Sample ID: VY1021SBL01

Lab Sample ID: VY1021SBL01

Analytical Method: 8260D

Sample Wt/Vol: 5 g

Level: LOW

Final Vol: 5000 uL

Date Collected:

Date Received:

SDG No.: Q3410

Matrix: SOIL

% Solid: 100

Test: VOC-TCLVOA-10

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Date Ana.	BatchID
TARGETS									
75-71-8	Dichlorodifluoromethane	1.10	U	1	1.10	5.00	ug/Kg	10/21/25 09:34	VY102125
74-87-3	Chloromethane	1.10	U	1	1.10	5.00	ug/Kg	10/21/25 09:34	VY102125
75-01-4	Vinyl Chloride	0.79	U	1	0.79	5.00	ug/Kg	10/21/25 09:34	VY102125
74-83-9	Bromomethane	1.10	U	1	1.10	5.00	ug/Kg	10/21/25 09:34	VY102125
75-00-3	Chloroethane	1.30	U	1	1.30	5.00	ug/Kg	10/21/25 09:34	VY102125
75-69-4	Trichlorofluoromethane	1.20	U	1	1.20	5.00	ug/Kg	10/21/25 09:34	VY102125
76-13-1	1,1,2-Trichlorotrifluoroethane	1.10	U	1	1.10	5.00	ug/Kg	10/21/25 09:34	VY102125
75-35-4	1,1-Dichloroethene	1.00	U	1	1.00	5.00	ug/Kg	10/21/25 09:34	VY102125
67-64-1	Acetone	4.70	U	1	4.70	25.0	ug/Kg	10/21/25 09:34	VY102125
75-15-0	Carbon Disulfide	1.10	U	1	1.10	5.00	ug/Kg	10/21/25 09:34	VY102125
1634-04-4	Methyl tert-butyl Ether	0.73	U	1	0.73	5.00	ug/Kg	10/21/25 09:34	VY102125
79-20-9	Methyl Acetate	1.50	U	1	1.50	5.00	ug/Kg	10/21/25 09:34	VY102125
75-09-2	Methylene Chloride	3.50	U	1	3.50	10.0	ug/Kg	10/21/25 09:34	VY102125
156-60-5	trans-1,2-Dichloroethene	0.86	U	1	0.86	5.00	ug/Kg	10/21/25 09:34	VY102125
75-34-3	1,1-Dichloroethane	0.80	U	1	0.80	5.00	ug/Kg	10/21/25 09:34	VY102125
110-82-7	Cyclohexane	0.79	U	1	0.79	5.00	ug/Kg	10/21/25 09:34	VY102125
78-93-3	2-Butanone	6.50	U	1	6.50	25.0	ug/Kg	10/21/25 09:34	VY102125
56-23-5	Carbon Tetrachloride	0.97	U	1	0.97	5.00	ug/Kg	10/21/25 09:34	VY102125
156-59-2	cis-1,2-Dichloroethene	0.75	U	1	0.75	5.00	ug/Kg	10/21/25 09:34	VY102125
74-97-5	Bromochloromethane	1.20	U	1	1.20	5.00	ug/Kg	10/21/25 09:34	VY102125
67-66-3	Chloroform	0.84	U	1	0.84	5.00	ug/Kg	10/21/25 09:34	VY102125
71-55-6	1,1,1-Trichloroethane	0.93	U	1	0.93	5.00	ug/Kg	10/21/25 09:34	VY102125
108-87-2	Methylcyclohexane	0.91	U	1	0.91	5.00	ug/Kg	10/21/25 09:34	VY102125
71-43-2	Benzene	0.79	U	1	0.79	5.00	ug/Kg	10/21/25 09:34	VY102125
107-06-2	1,2-Dichloroethane	0.79	U	1	0.79	5.00	ug/Kg	10/21/25 09:34	VY102125
79-01-6	Trichloroethene	0.81	U	1	0.81	5.00	ug/Kg	10/21/25 09:34	VY102125
78-87-5	1,2-Dichloropropane	0.91	U	1	0.91	5.00	ug/Kg	10/21/25 09:34	VY102125
75-27-4	Bromodichloromethane	0.78	U	1	0.78	5.00	ug/Kg	10/21/25 09:34	VY102125
108-10-1	4-Methyl-2-Pentanone	3.60	U	1	3.60	25.0	ug/Kg	10/21/25 09:34	VY102125
108-88-3	Toluene	0.78	U	1	0.78	5.00	ug/Kg	10/21/25 09:34	VY102125
10061-02-6	t-1,3-Dichloropropene	0.65	U	1	0.65	5.00	ug/Kg	10/21/25 09:34	VY102125
10061-01-5	cis-1,3-Dichloropropene	0.62	U	1	0.62	5.00	ug/Kg	10/21/25 09:34	VY102125
79-00-5	1,1,2-Trichloroethane	0.92	U	1	0.92	5.00	ug/Kg	10/21/25 09:34	VY102125
591-78-6	2-Hexanone	3.70	U	1	3.70	25.0	ug/Kg	10/21/25 09:34	VY102125
124-48-1	Dibromochloromethane	0.87	U	1	0.87	5.00	ug/Kg	10/21/25 09:34	VY102125
106-93-4	1,2-Dibromoethane	0.88	U	1	0.88	5.00	ug/Kg	10/21/25 09:34	VY102125
127-18-4	Tetrachloroethene	1.10	U	1	1.10	5.00	ug/Kg	10/21/25 09:34	VY102125
108-90-7	Chlorobenzene	0.91	U	1	0.91	5.00	ug/Kg	10/21/25 09:34	VY102125
100-41-4	Ethyl Benzene	0.67	U	1	0.67	5.00	ug/Kg	10/21/25 09:34	VY102125
179601-23-1	m/p-Xylenes	1.20	U	1	1.20	10.0	ug/Kg	10/21/25 09:34	VY102125
95-47-6	o-Xylene	0.82	U	1	0.82	5.00	ug/Kg	10/21/25 09:34	VY102125
100-42-5	Styrene	0.71	U	1	0.71	5.00	ug/Kg	10/21/25 09:34	VY102125
75-25-2	Bromoform	0.86	U	1	0.86	5.00	ug/Kg	10/21/25 09:34	VY102125



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client: Sciacca General Contractors, LLC

Project: 49 Moore Place Belleville

Client Sample ID: VY1021SBL01

Lab Sample ID: VY1021SBL01

Analytical Method: 8260D

Sample Wt/Vol: 5 g

Level : LOW

Final Vol: 5000 uL

Date Collected:

Date Received:

SDG No.: Q3410

Matrix: SOIL

% Solid: 100

Test: VOC-TCLVOA-10

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Date Ana.	BatchID
98-82-8	Isopropylbenzene	0.78	U	1	0.78	5.00	ug/Kg	10/21/25 09:34	VY102125
79-34-5	1,1,2,2-Tetrachloroethane	1.20	U	1	1.20	5.00	ug/Kg	10/21/25 09:34	VY102125
541-73-1	1,3-Dichlorobenzene	1.70	U	1	1.70	5.00	ug/Kg	10/21/25 09:34	VY102125
106-46-7	1,4-Dichlorobenzene	1.60	U	1	1.60	5.00	ug/Kg	10/21/25 09:34	VY102125
95-50-1	1,2-Dichlorobenzene	1.50	U	1	1.50	5.00	ug/Kg	10/21/25 09:34	VY102125
96-12-8	1,2-Dibromo-3-Chloropropane	1.80	U	1	1.80	5.00	ug/Kg	10/21/25 09:34	VY102125
120-82-1	1,2,4-Trichlorobenzene	3.00	U	1	3.00	5.00	ug/Kg	10/21/25 09:34	VY102125
87-61-6	1,2,3-Trichlorobenzene	3.20	U	1	3.20	5.00	ug/Kg	10/21/25 09:34	VY102125
SURROGATES									
17060-07-0	1,2-Dichloroethane-d4	46.0			63 - 155	92%	SPK: 50		
1868-53-7	Dibromofluoromethane	49.7			70 - 134	99%	SPK: 50		
2037-26-5	Toluene-d8	48.1			74 - 123	96%	SPK: 50		
460-00-4	4-Bromofluorobenzene	36.4			17 - 146	73%	SPK: 50		
INTERNAL STANDARDS									
		Area Count							
363-72-4	Pentafluorobenzene	768000							
540-36-3	1,4-Difluorobenzene	1270000							
3114-55-4	Chlorobenzene-d5	1000000							
3855-82-1	1,4-Dichlorobenzene-d4	379000							

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
 Data File : VY023522.D
 Acq On : 21 Oct 2025 09:34
 Operator : SY/MD
 Sample : VY1021SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY1021SBL01

Quant Time: Oct 24 01:21:50 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.713	168	767531	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	1271980	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	1000258	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	378610	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	295141	45.985	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	91.960%
35) Dibromofluoromethane	7.640	113	388671	49.729	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	99.460%
50) Toluene-d8	10.109	98	1399310	48.076	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	96.160%
62) 4-Bromofluorobenzene	12.408	95	349784	36.400	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	72.800%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
Data File : VY023522.D
Acq On : 21 Oct 2025 09:34
Operator : SY/MD
Sample : VY1021SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY1021SBL01

Quant Time: Oct 24 01:21:50 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 05:12:50 2025
Response via : Initial Calibration




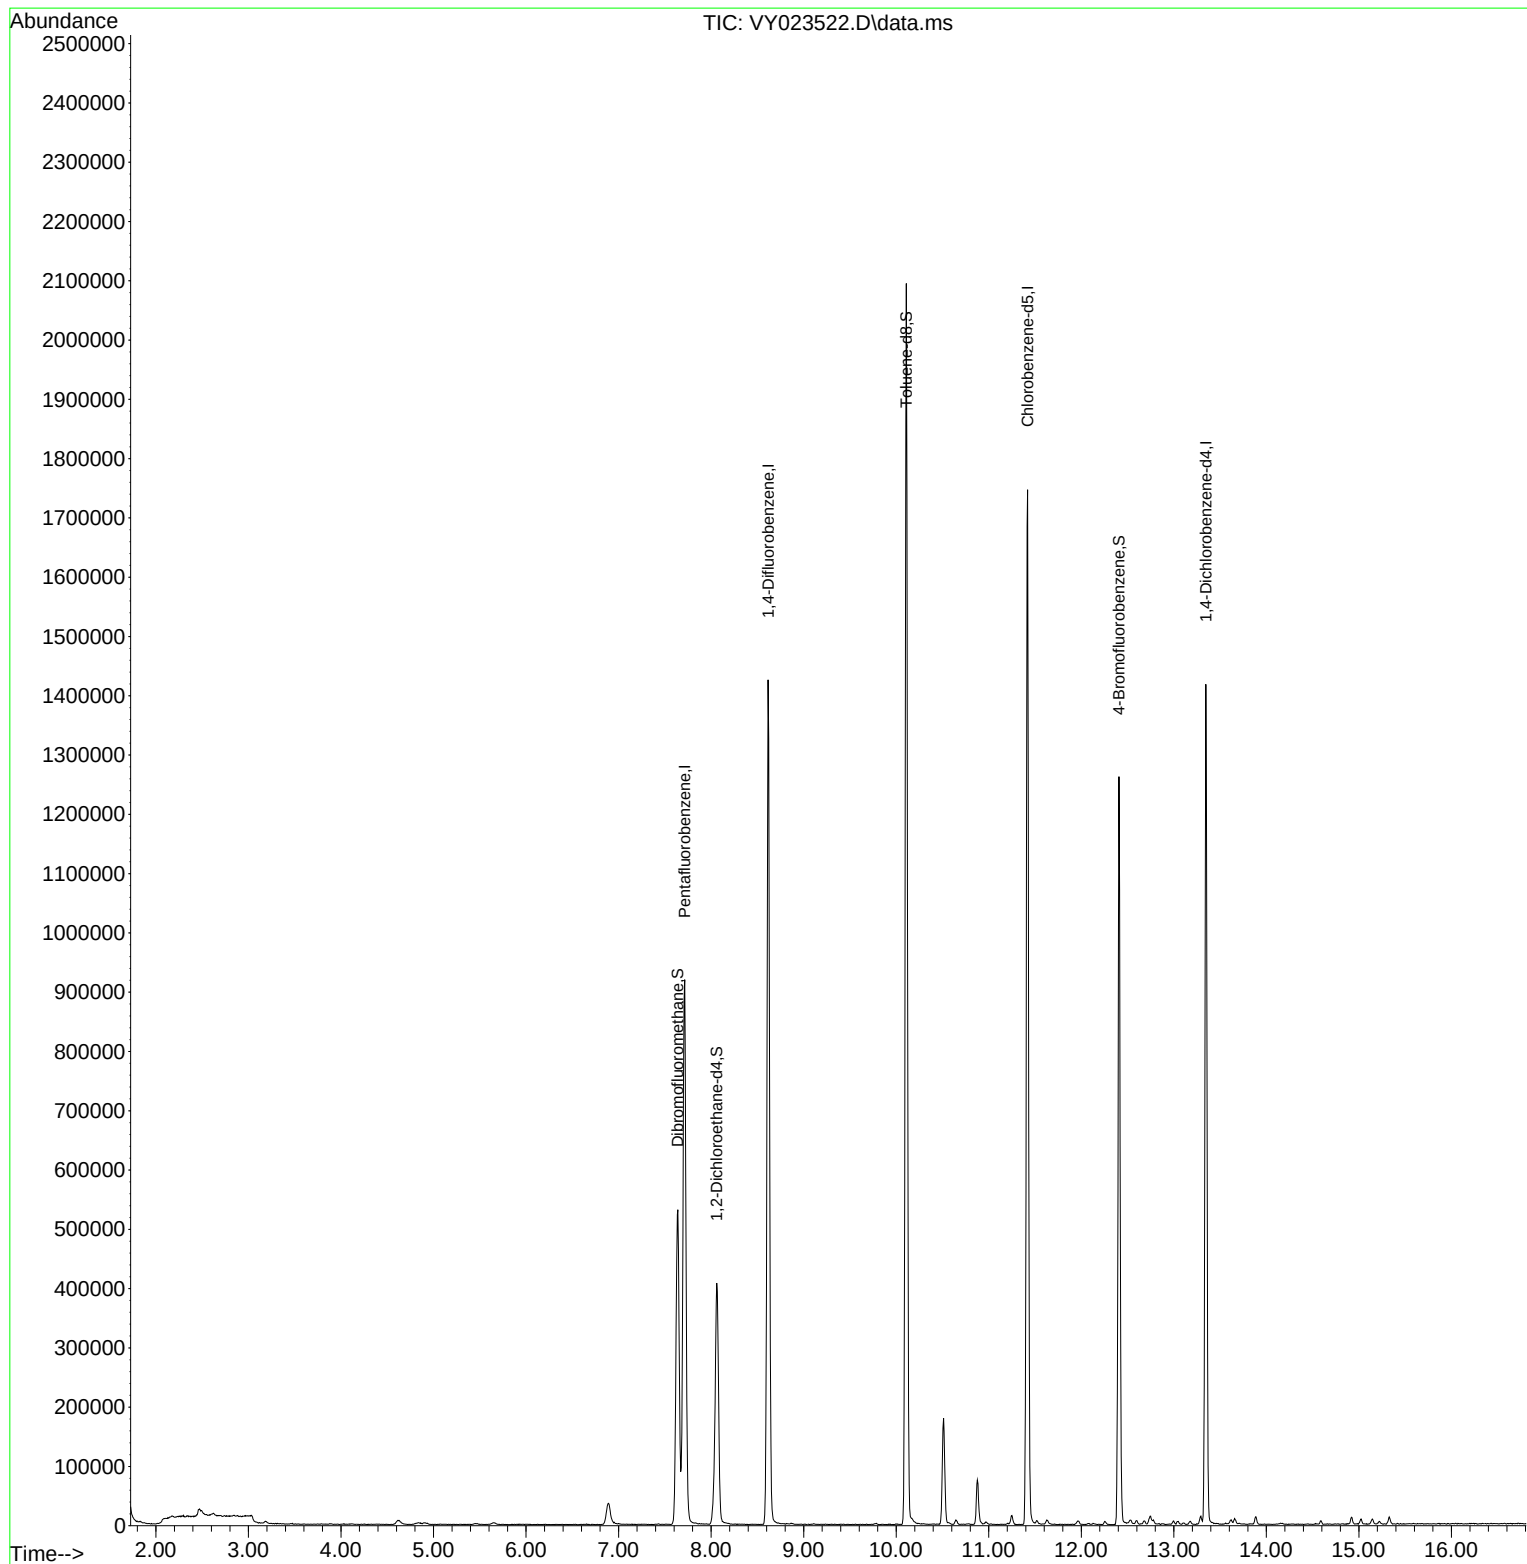


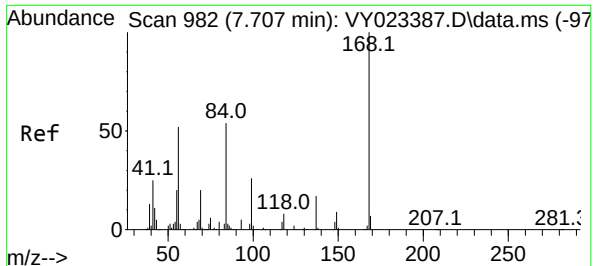

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 99
Delta R.T. 0.006 min
Lab File: VY023522.D
Acq: 21 Oct 2025 09:34




Instrument :
MSVOA_Y
ClientSampleId :
VY1021SBL01


Tgt Ion:168 Resp: 767531
Ion Ratio Lower Upper
168 100
99 47.8 39.7 59.5

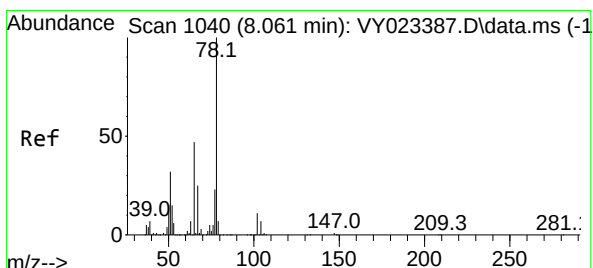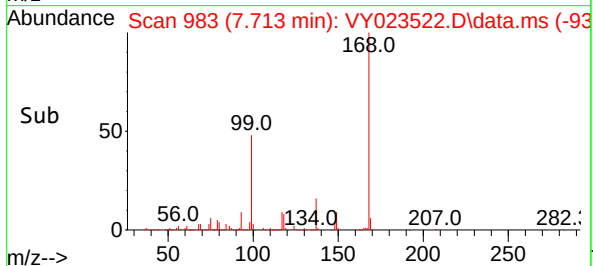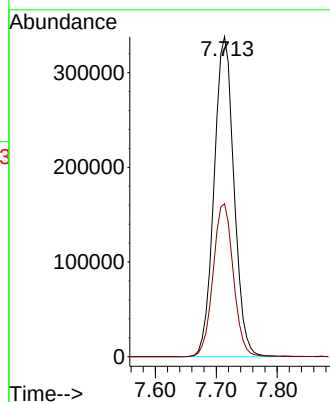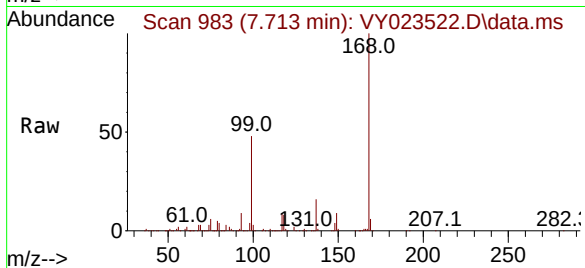

#33
1,2-Dichloroethane-d4
Concen: 45.985 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY023522.D
Acq: 21 Oct 2025 09:34

Tgt Ion: 65 Resp: 295141
Ion Ratio Lower Upper
65 100
67 52.8 0.0 105.8

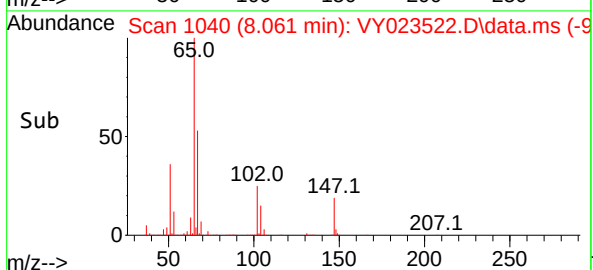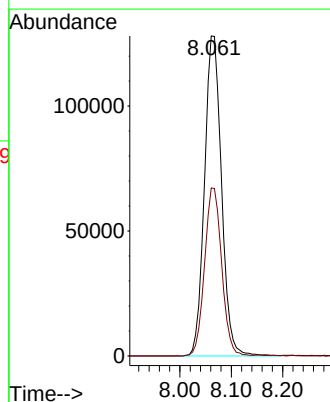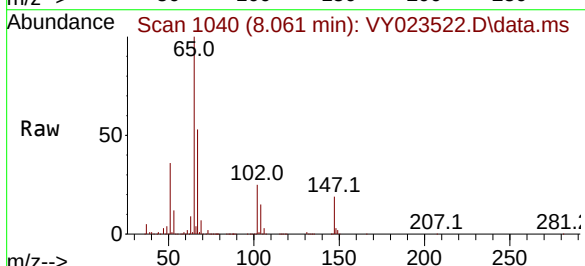

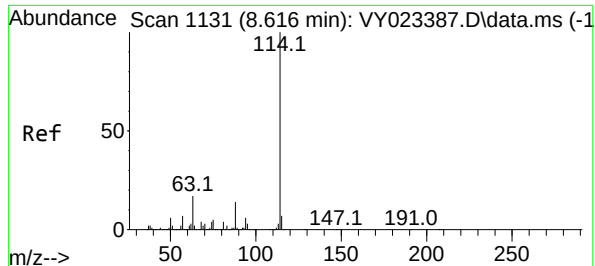

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.616 min Scan# 1131

Delta R.T. 0.000 min

Lab File: VY023522.D

Acq: 21 Oct 2025 09:34

Instrument :

MSVOA_Y

ClientSampleId :

VY1021SBL01





Tgt Ion:114 Resp: 1271980

Ion Ratio Lower Upper

114 100

63 17.5 0.0 34.2

88 14.2 0.0 28.4

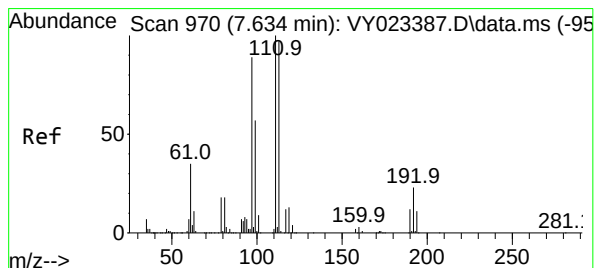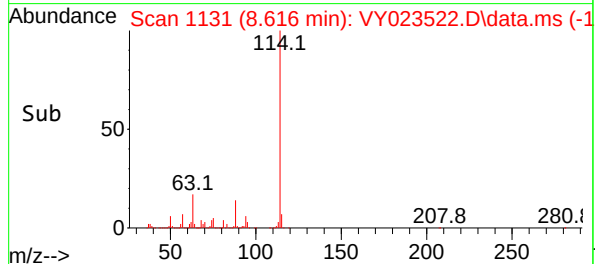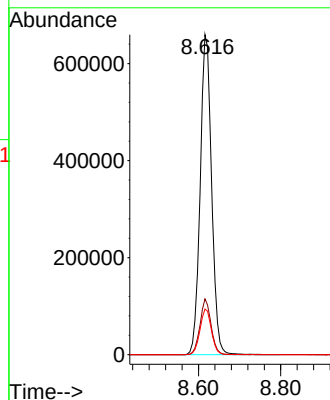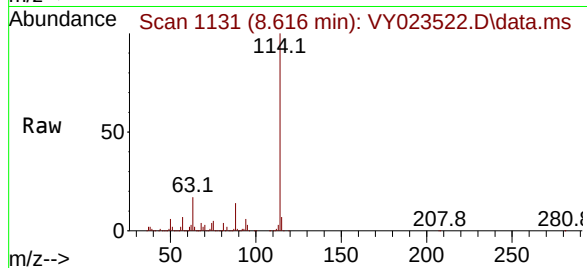

#35

Dibromofluoromethane

Concen: 49.729 ug/l

RT: 7.640 min Scan# 971

Delta R.T. 0.006 min

Lab File: VY023522.D

Acq: 21 Oct 2025 09:34




Tgt Ion:113 Resp: 388671


Ion Ratio Lower Upper

113 100

111 101.1 81.8 122.6

192 21.8 18.0 27.0


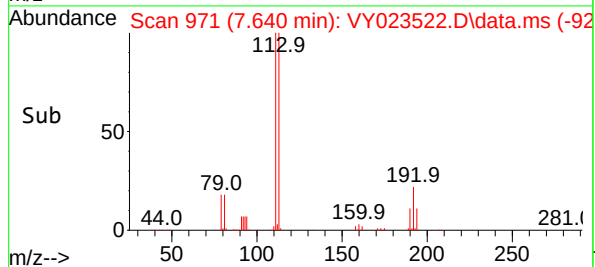
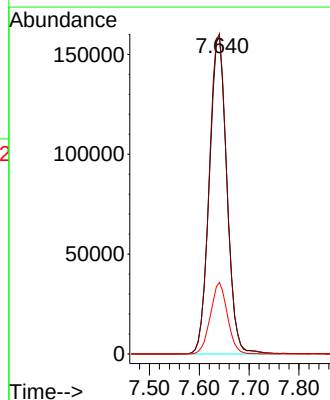
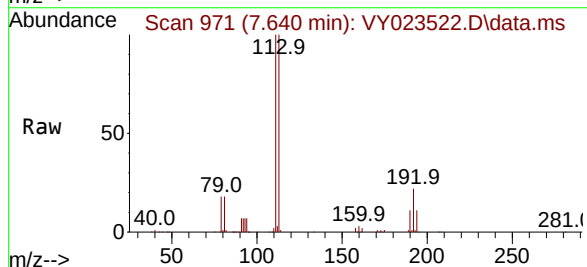


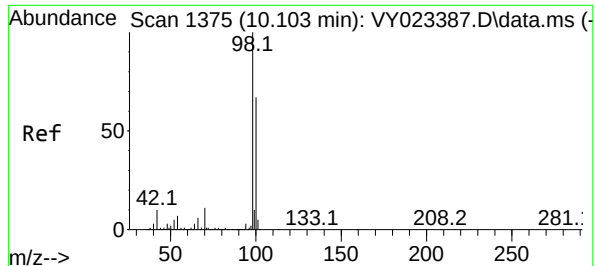

#50
Toluene-d8
Concen: 48.076 ug/l
RT: 10.109 min Scan# 1375
Delta R.T. 0.006 min
Lab File: VY023522.D
Acq: 21 Oct 2025 09:34




Instrument :
MSVOA_Y
ClientSampleId :
VY1021SBL01


Tgt Ion: 98 Resp: 1399310
Ion Ratio Lower Upper
98 100
100 65.2 53.0 79.4

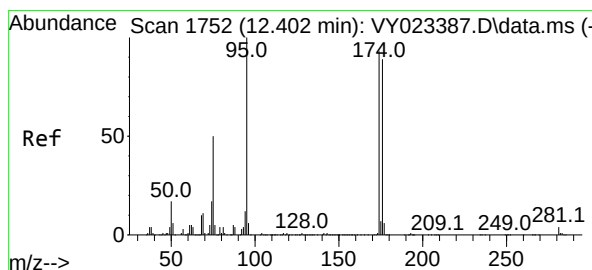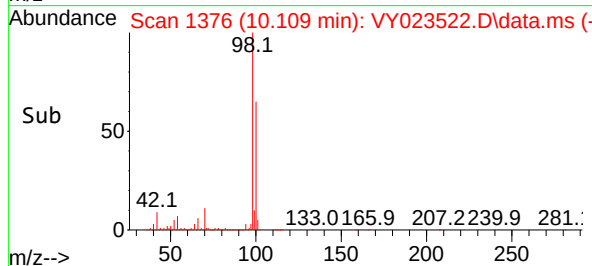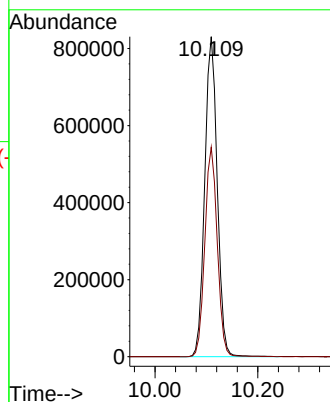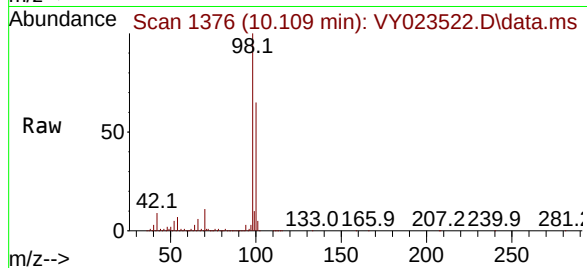

#62
4-Bromofluorobenzene
Concen: 36.400 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.006 min
Lab File: VY023522.D
Acq: 21 Oct 2025 09:34

Tgt Ion: 95 Resp: 349784
Ion Ratio Lower Upper
95 100
174 98.0 0.0 192.8
176 93.7 0.0 187.6

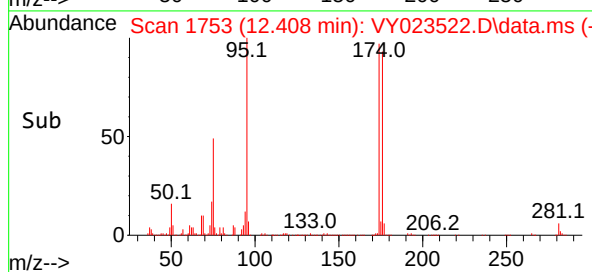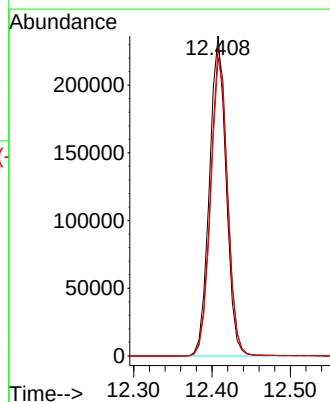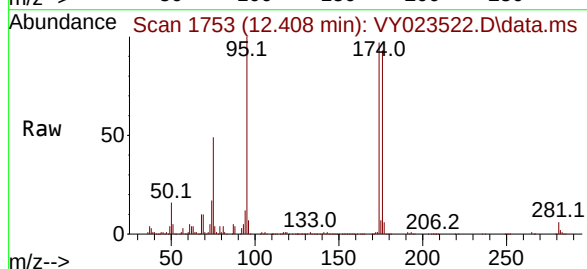

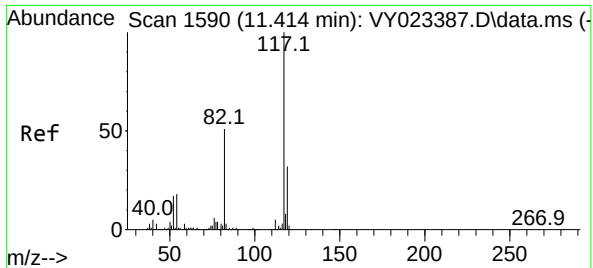

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.420 min Scan# 11

Delta R.T. 0.006 min

Lab File: VY023522.D

Acq: 21 Oct 2025 09:34

Instrument :

MSVOA_Y

ClientSampleId :

VY1021SBL01





Tgt Ion:117 Resp: 1000258

Ion Ratio Lower Upper

117 100

82 50.0 41.0 61.4

119 32.6 25.6 38.4

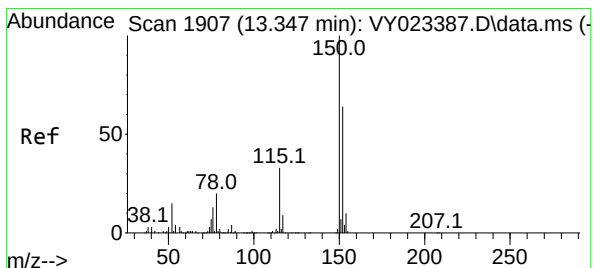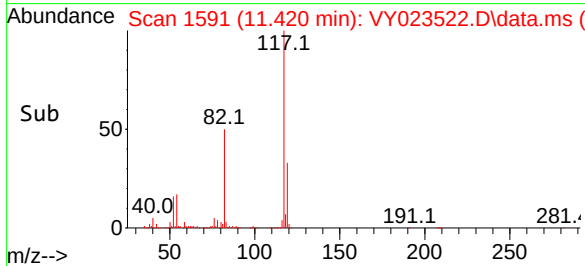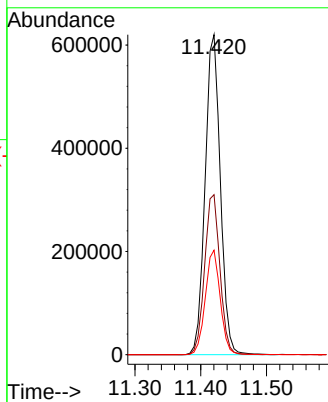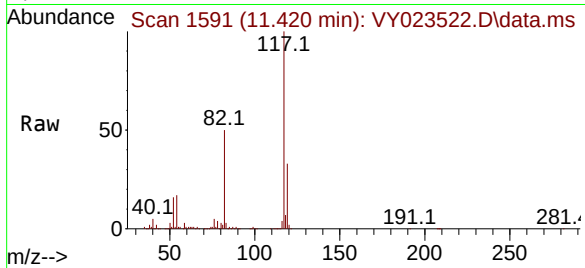

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.347 min Scan# 1907

Delta R.T. 0.000 min

Lab File: VY023522.D

Acq: 21 Oct 2025 09:34




Tgt Ion:152 Resp: 378610

Ion Ratio Lower Upper

152 100

115 53.8 27.1 81.2

150 156.0 0.0 347.4

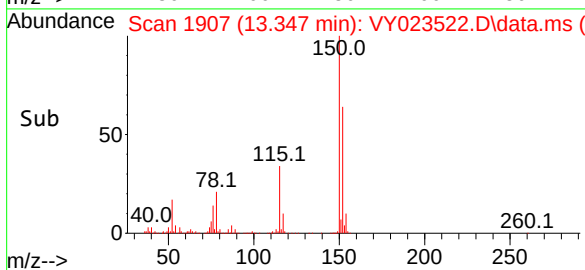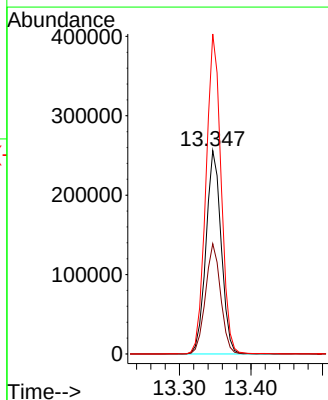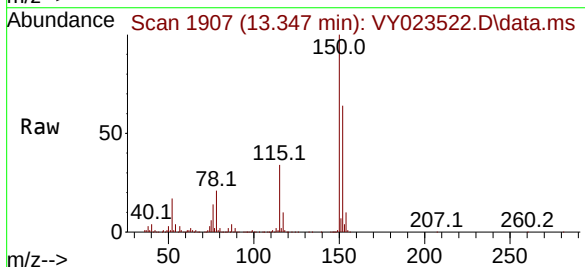

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
Data File : VY023522.D
Acq On : 21 Oct 2025 09:34
Operator : SY/MD
Sample : VY1021SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY1021SBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M

Title : SW846 8260

Signal : TIC: VY023522.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.890	838	848	857	rBV	35400	111624	3.14%	0.612%
2	7.640	959	971	976	rBV	531008	1277186	35.90%	6.997%
3	7.713	976	983	1000	rVB	917366	2109123	59.28%	11.555%
4	8.061	1027	1040	1064	rBV2	406960	1071893	30.13%	5.872%
5	8.616	1122	1131	1147	rBV	1424841	2733100	76.81%	14.973%
6	10.109	1367	1376	1396	rBV	2093314	3558053	100.00%	19.492%
7	10.512	1435	1442	1449	rBV	178794	329732	9.27%	1.806%
8	10.878	1494	1502	1511	rBV	75256	134524	3.78%	0.737%
9	11.420	1583	1591	1604	rBV	1745395	2851605	80.15%	15.622%
10	12.408	1746	1753	1763	rBV2	1261596	1957774	55.02%	10.725%
11	13.347	1901	1907	1921	rVB	1416131	2119051	59.56%	11.609%




Sum of corrected areas: 18253665

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
Data File : VY023522.D
Acq On : 21 Oct 2025 09:34
Operator : SY/MD
Sample : VY1021SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY1021SBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

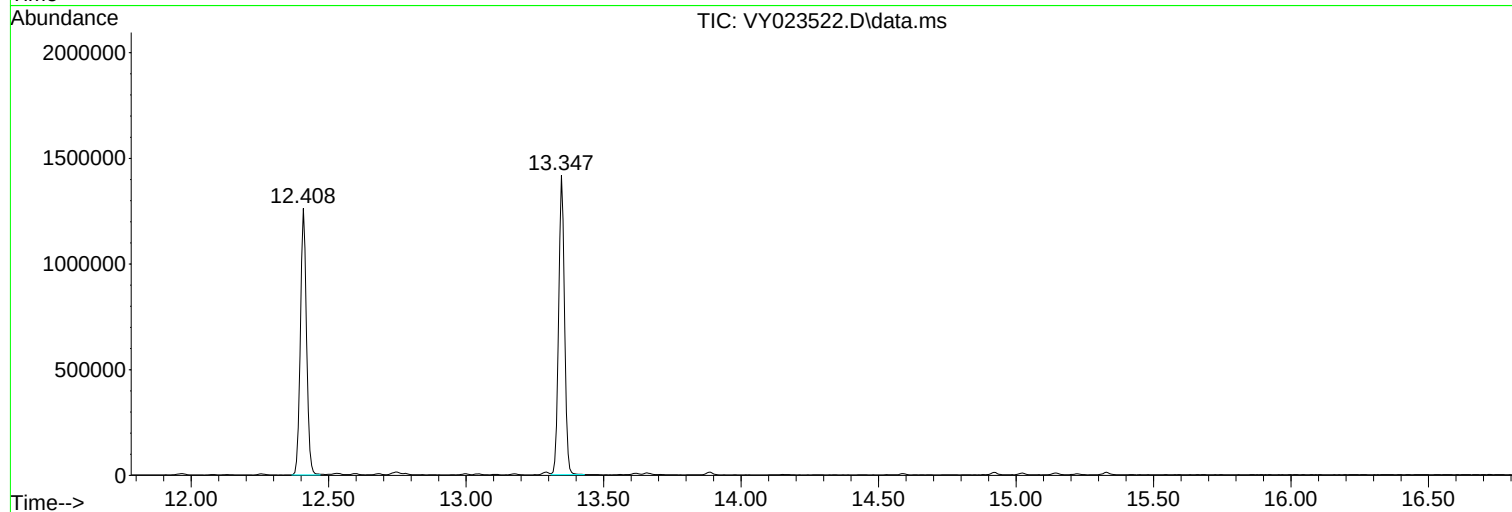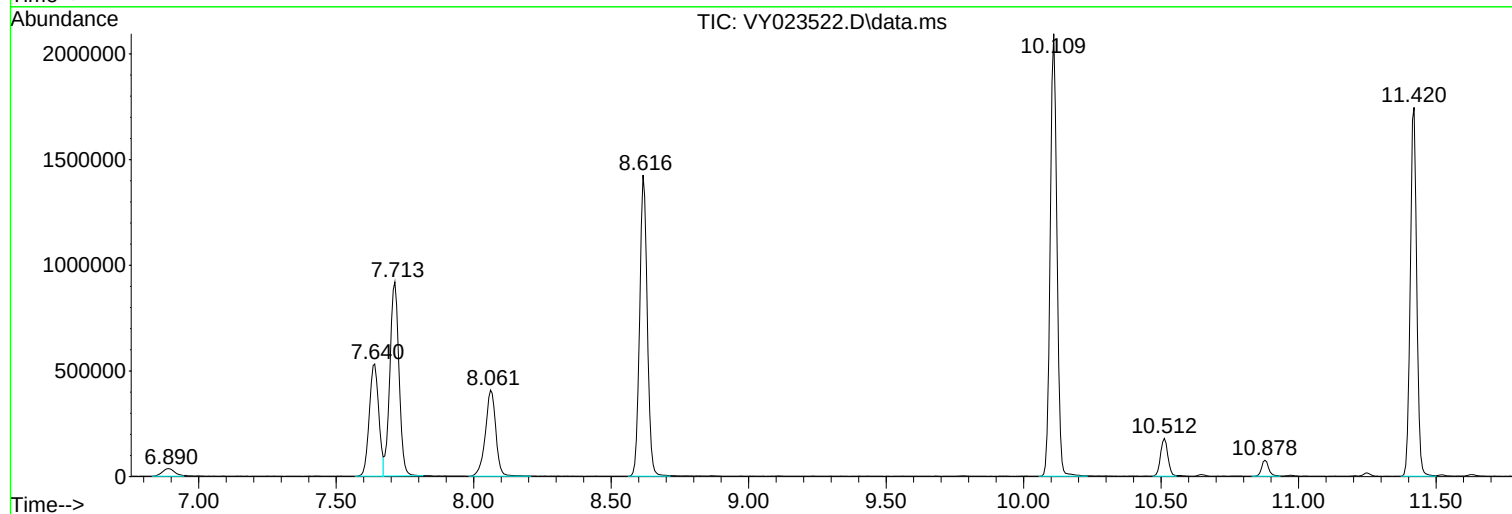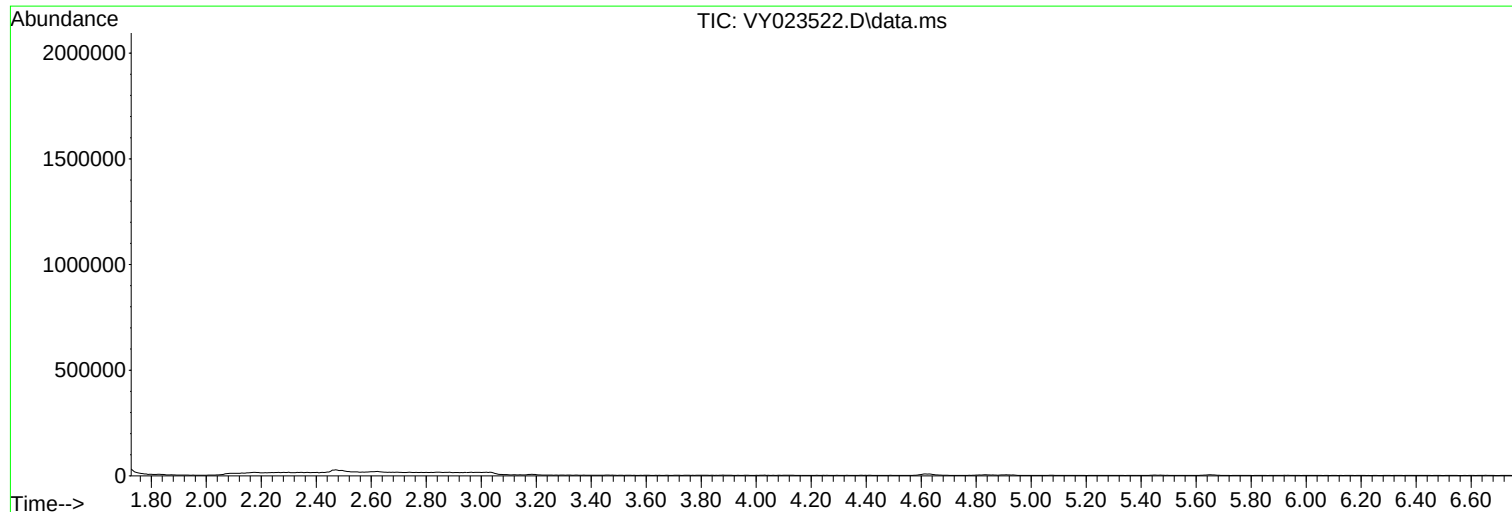

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
Data File : VY023522.D
Acq On : 21 Oct 2025 09:34
Operator : SY/MD
Sample : VY1021SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY1021SBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
Data File : VY023522.D
Acq On : 21 Oct 2025 09:34
Operator : SY/MD
Sample : VY1021SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY1021SBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc

Report of Analysis

Client: Sciacca General Contractors, LLC

Project: 49 Moore Place Belleville

Client Sample ID: VY1021SBS01

Lab Sample ID: VY1021SBS01

Analytical Method: 8260D

Level : LOW

Sample Wt/Vol: 5 g

Final Vol: 5000 uL

Date Collected:

Date Received:

SDG No.: Q3410

Matrix: SOIL

% Solid: 100

Test: VOC-TCLVOA-10

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Date Ana.	BatchID
TARGETS									
75-71-8	Dichlorodifluoromethane	20.3		1	1.10	5.00	ug/Kg	10/21/25 10:04	VY102125
74-87-3	Chloromethane	19.5		1	1.10	5.00	ug/Kg	10/21/25 10:04	VY102125
75-01-4	Vinyl Chloride	20.2		1	0.79	5.00	ug/Kg	10/21/25 10:04	VY102125
74-83-9	Bromomethane	21.5		1	1.10	5.00	ug/Kg	10/21/25 10:04	VY102125
75-00-3	Chloroethane	21.2		1	1.30	5.00	ug/Kg	10/21/25 10:04	VY102125
75-69-4	Trichlorofluoromethane	20.4		1	1.20	5.00	ug/Kg	10/21/25 10:04	VY102125
76-13-1	1,1,2-Trichlorotrifluoroethane	21.1		1	1.10	5.00	ug/Kg	10/21/25 10:04	VY102125
75-35-4	1,1-Dichloroethene	20.2		1	1.00	5.00	ug/Kg	10/21/25 10:04	VY102125
67-64-1	Acetone	120		1	4.70	25.0	ug/Kg	10/21/25 10:04	VY102125
75-15-0	Carbon Disulfide	20.2		1	1.10	5.00	ug/Kg	10/21/25 10:04	VY102125
1634-04-4	Methyl tert-butyl Ether	18.0		1	0.73	5.00	ug/Kg	10/21/25 10:04	VY102125
79-20-9	Methyl Acetate	15.9		1	1.50	5.00	ug/Kg	10/21/25 10:04	VY102125
75-09-2	Methylene Chloride	19.0		1	3.50	10.0	ug/Kg	10/21/25 10:04	VY102125
156-60-5	trans-1,2-Dichloroethene	21.0		1	0.86	5.00	ug/Kg	10/21/25 10:04	VY102125
75-34-3	1,1-Dichloroethane	20.5		1	0.80	5.00	ug/Kg	10/21/25 10:04	VY102125
110-82-7	Cyclohexane	18.8		1	0.79	5.00	ug/Kg	10/21/25 10:04	VY102125
78-93-3	2-Butanone	100		1	6.50	25.0	ug/Kg	10/21/25 10:04	VY102125
56-23-5	Carbon Tetrachloride	21.7		1	0.97	5.00	ug/Kg	10/21/25 10:04	VY102125
156-59-2	cis-1,2-Dichloroethene	20.7		1	0.75	5.00	ug/Kg	10/21/25 10:04	VY102125
74-97-5	Bromochloromethane	19.7		1	1.20	5.00	ug/Kg	10/21/25 10:04	VY102125
67-66-3	Chloroform	21.5		1	0.84	5.00	ug/Kg	10/21/25 10:04	VY102125
71-55-6	1,1,1-Trichloroethane	21.1		1	0.93	5.00	ug/Kg	10/21/25 10:04	VY102125
108-87-2	Methylcyclohexane	19.8		1	0.91	5.00	ug/Kg	10/21/25 10:04	VY102125
71-43-2	Benzene	21.6		1	0.79	5.00	ug/Kg	10/21/25 10:04	VY102125
107-06-2	1,2-Dichloroethane	20.0		1	0.79	5.00	ug/Kg	10/21/25 10:04	VY102125
79-01-6	Trichloroethene	21.9		1	0.81	5.00	ug/Kg	10/21/25 10:04	VY102125
78-87-5	1,2-Dichloropropane	21.5		1	0.91	5.00	ug/Kg	10/21/25 10:04	VY102125
75-27-4	Bromodichloromethane	21.3		1	0.78	5.00	ug/Kg	10/21/25 10:04	VY102125
108-10-1	4-Methyl-2-Pentanone	86.7		1	3.60	25.0	ug/Kg	10/21/25 10:04	VY102125
108-88-3	Toluene	21.9		1	0.78	5.00	ug/Kg	10/21/25 10:04	VY102125
10061-02-6	t-1,3-Dichloropropene	19.9		1	0.65	5.00	ug/Kg	10/21/25 10:04	VY102125
10061-01-5	cis-1,3-Dichloropropene	20.8		1	0.62	5.00	ug/Kg	10/21/25 10:04	VY102125
79-00-5	1,1,2-Trichloroethane	21.0		1	0.92	5.00	ug/Kg	10/21/25 10:04	VY102125
591-78-6	2-Hexanone	95.9		1	3.70	25.0	ug/Kg	10/21/25 10:04	VY102125
124-48-1	Dibromochloromethane	20.8		1	0.87	5.00	ug/Kg	10/21/25 10:04	VY102125
106-93-4	1,2-Dibromoethane	20.1		1	0.88	5.00	ug/Kg	10/21/25 10:04	VY102125
127-18-4	Tetrachloroethene	22.0		1	1.10	5.00	ug/Kg	10/21/25 10:04	VY102125
108-90-7	Chlorobenzene	21.2		1	0.91	5.00	ug/Kg	10/21/25 10:04	VY102125
100-41-4	Ethyl Benzene	21.0		1	0.67	5.00	ug/Kg	10/21/25 10:04	VY102125
179601-23-1	m/p-Xylenes	43.1		1	1.20	10.0	ug/Kg	10/21/25 10:04	VY102125
95-47-6	o-Xylene	20.6		1	0.82	5.00	ug/Kg	10/21/25 10:04	VY102125
100-42-5	Styrene	21.0		1	0.71	5.00	ug/Kg	10/21/25 10:04	VY102125
75-25-2	Bromoform	19.5		1	0.86	5.00	ug/Kg	10/21/25 10:04	VY102125



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client: Sciacca General Contractors, LLC

Project: 49 Moore Place Belleville

Client Sample ID: VY1021SBS01

Lab Sample ID: VY1021SBS01

Analytical Method: 8260D

Sample Wt/Vol: 5 g

Level : LOW

Final Vol: 5000 uL

Date Collected:

Date Received:

SDG No.: Q3410

Matrix: SOIL

% Solid: 100

Test: VOC-TCLVOA-10

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Date Ana.	BatchID
98-82-8	Isopropylbenzene	20.3		1	0.78	5.00	ug/Kg	10/21/25 10:04	VY102125
79-34-5	1,1,2,2-Tetrachloroethane	18.2		1	1.20	5.00	ug/Kg	10/21/25 10:04	VY102125
541-73-1	1,3-Dichlorobenzene	20.7		1	1.70	5.00	ug/Kg	10/21/25 10:04	VY102125
106-46-7	1,4-Dichlorobenzene	20.5		1	1.60	5.00	ug/Kg	10/21/25 10:04	VY102125
95-50-1	1,2-Dichlorobenzene	20.5		1	1.50	5.00	ug/Kg	10/21/25 10:04	VY102125
96-12-8	1,2-Dibromo-3-Chloropropane	17.0		1	1.80	5.00	ug/Kg	10/21/25 10:04	VY102125
120-82-1	1,2,4-Trichlorobenzene	18.0		1	3.00	5.00	ug/Kg	10/21/25 10:04	VY102125
87-61-6	1,2,3-Trichlorobenzene	18.1		1	3.20	5.00	ug/Kg	10/21/25 10:04	VY102125
SURROGATES									
17060-07-0	1,2-Dichloroethane-d4	46.9			63 - 155	94%	SPK: 50		
1868-53-7	Dibromofluoromethane	50.9			70 - 134	102%	SPK: 50		
2037-26-5	Toluene-d8	51.3			74 - 123	103%	SPK: 50		
460-00-4	4-Bromofluorobenzene	49.9			17 - 146	100%	SPK: 50		
INTERNAL STANDARDS									
		Area Count							
363-72-4	Pentafluorobenzene	494000							
540-36-3	1,4-Difluorobenzene	713000							
3114-55-4	Chlorobenzene-d5	636000							
3855-82-1	1,4-Dichlorobenzene-d4	341000							

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
 Data File : VY023523.D
 Acq On : 21 Oct 2025 10:04
 Operator : SY/MD
 Sample : VY1021SBS01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY1021SBS01

Manual Integrations
 APPROVED

Reviewed By :Amit Patel 10/24/2025
 Supervised By :Mahesh Dadoda 10/27/2025

Quant Time: Oct 24 01:22:08 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.713	168	494016	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	712868	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	635785	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	341398	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	193871	46.930	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery =	93.860%		
35) Dibromofluoromethane	7.634	113	222986	50.907	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery =	101.820%		
50) Toluene-d8	10.109	98	837402	51.335	ug/l	0.00
Spiked Amount 50.000	Range 58 - 134		Recovery =	102.680%		
62) 4-Bromofluorobenzene	12.408	95	268965	49.942	ug/l	0.00
Spiked Amount 50.000	Range 30 - 143		Recovery =	99.880%		
Target Compounds					Qvalue	
2) Dichlorodifluoromethane	1.867	85	72214	20.308	ug/l	96
3) Chloromethane	2.074	50	94488	19.506	ug/l	99
4) Vinyl Chloride	2.208	62	127704	20.240	ug/l	98
5) Bromomethane	2.592	94	113644	21.464	ug/l	96
6) Chloroethane	2.732	64	91163	21.197	ug/l	99
7) Trichlorofluoromethane	3.056	101	179067	20.441	ug/l	100
8) Diethyl Ether	3.458	74	42637	18.626	ug/l	95
9) 1,1,2-Trichlorotrifluo...	3.812	101	96083	21.136	ug/l	99
10) Methyl Iodide	4.007	142	95981	18.966	ug/l	100
11) Tert butyl alcohol	4.848	59	34552	112.428	ug/l #	89
12) 1,1-Dichloroethene	3.787	96	89008	20.198	ug/l	95
13) Acrolein	3.653	56	21612	49.768	ug/l	98
14) Allyl chloride	4.385	41	99926	18.606	ug/l	96
15) Acrylonitrile	5.061	53	79043	90.228	ug/l	99
16) Acetone	3.866	43	119380	121.387	ug/l	99
17) Carbon Disulfide	4.110	76	254170	20.152	ug/l	99
18) Methyl Acetate	4.385	43	40953	15.874	ug/l	100
19) Methyl tert-butyl Ether	5.116	73	190637	17.999	ug/l	96
20) Methylene Chloride	4.616	84	101259	19.041	ug/l	99
21) trans-1,2-Dichloroethene	5.116	96	101665	20.955	ug/l	97
22) Diisopropyl ether	6.018	45	232353	19.559	ug/l	93
23) Vinyl Acetate	5.964	43	586288	91.178	ug/l	97
24) 1,1-Dichloroethane	5.915	63	161044	20.465	ug/l	99
25) 2-Butanone	6.896	43	122251	101.820	ug/l	96
26) 2,2-Dichloropropane	6.884	77	149940	20.766	ug/l	98
27) cis-1,2-Dichloroethene	6.890	96	115907	20.682	ug/l	98
28) Bromochloromethane	7.250	49	57916	19.715	ug/l	93
29) Tetrahydrofuran	7.262	42	54688	80.322	ug/l	97
30) Chloroform	7.421	83	186069	21.521	ug/l	100
31) Cyclohexane	7.701	56	129108	18.787	ug/l	95
32) 1,1,1-Trichloroethane	7.616	97	165772	21.099	ug/l	100
36) 1,1-Dichloropropene	7.835	75	122511	21.126	ug/l	99
37) Ethyl Acetate	6.988	43	42544	18.518	ug/l	98
38) Carbon Tetrachloride	7.823	117	152907	21.746	ug/l	99
39) Methylcyclohexane	9.109	83	149816	19.842	ug/l	96
40) Benzene	8.079	78	396525	21.591	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
 Data File : VY023523.D
 Acq On : 21 Oct 2025 10:04
 Operator : SY/MD
 Sample : VY1021SBS01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY1021SBS01

Manual Integrations
 APPROVED

Reviewed By :Amit Patel 10/24/2025
 Supervised By :Mahesh Dadoda 10/27/2025

Quant Time: Oct 24 01:22:08 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	7.238	41	24936m	20.069	ug/l	
42) 1,2-Dichloroethane	8.158	62	94656	19.985	ug/l	97
43) Isopropyl Acetate	8.201	43	79352	17.322	ug/l	99
44) Trichloroethene	8.865	130	117801	21.916	ug/l	97
45) 1,2-Dichloropropane	9.140	63	87109	21.475	ug/l	100
46) Dibromomethane	9.231	93	52865	20.610	ug/l	98
47) Bromodichloromethane	9.426	83	137492	21.284	ug/l	100
48) Methyl methacrylate	9.219	41	34583	16.069	ug/l	89
49) 1,4-Dioxane	9.231	88	10115	340.128	ug/l	98
51) 4-Methyl-2-Pentanone	9.999	43	205212	86.702	ug/l	100
52) Toluene	10.170	92	260667	21.861	ug/l	100
53) t-1,3-Dichloropropene	10.396	75	111956	19.932	ug/l	99
54) cis-1,3-Dichloropropene	9.859	75	137908	20.802	ug/l	98
55) 1,1,2-Trichloroethane	10.573	97	72400	20.990	ug/l	95
56) Ethyl methacrylate	10.438	69	68512	17.220	ug/l	96
57) 1,3-Dichloropropane	10.719	76	110943	20.298	ug/l	100
58) 2-Chloroethyl Vinyl ether	9.713	63	161119	90.396	ug/l	100
59) 2-Hexanone	10.761	43	162182	95.882	ug/l	100
60) Dibromochloromethane	10.914	129	100658	20.815	ug/l	99
61) 1,2-Dibromoethane	11.011	107	66140	20.106	ug/l	100
64) Tetrachloroethene	10.646	164	144595	22.026	ug/l	96
65) Chlorobenzene	11.444	112	292874	21.180	ug/l	98
66) 1,1,1,2-Tetrachloroethane	11.517	131	105517	21.413	ug/l	99
67) Ethyl Benzene	11.517	91	469417	20.972	ug/l	99
68) m/p-Xylenes	11.627	106	386672	43.069	ug/l	98
69) o-Xylene	11.956	106	173158	20.563	ug/l	100
70) Styrene	11.969	104	290368	20.968	ug/l	100
71) Bromoform	12.133	173	59594	19.497	ug/l #	99
73) Isopropylbenzene	12.255	105	457435	20.332	ug/l	99
74) N-amyl acetate	12.072	43	63675	15.757	ug/l	96
75) 1,1,2,2-Tetrachloroethane	12.505	83	67088	18.231	ug/l	100
76) 1,2,3-Trichloropropane	12.554	75	51352m	17.049	ug/l	
77) Bromobenzene	12.529	156	120941	20.220	ug/l	97
78) n-propylbenzene	12.597	91	544028	20.896	ug/l	100
79) 2-Chlorotoluene	12.682	91	314616	20.636	ug/l	100
80) 1,3,5-Trimethylbenzene	12.737	105	382336	21.030	ug/l	100
81) trans-1,4-Dichloro-2-b...	12.304	75	21535	17.532	ug/l	99
82) 4-Chlorotoluene	12.779	91	333366	21.231	ug/l	100
83) tert-Butylbenzene	12.999	119	342878	20.426	ug/l	99
84) 1,2,4-Trimethylbenzene	13.042	105	382715	21.093	ug/l	99
85) sec-Butylbenzene	13.176	105	504696	20.959	ug/l	100
86) p-Isopropyltoluene	13.292	119	427597	20.856	ug/l	100
87) 1,3-Dichlorobenzene	13.285	146	241546	20.738	ug/l	100
88) 1,4-Dichlorobenzene	13.365	146	236089	20.523	ug/l	98
89) n-Butylbenzene	13.615	91	360818	20.198	ug/l	99
90) Hexachloroethane	13.877	117	93382	21.177	ug/l	97
91) 1,2-Dichlorobenzene	13.657	146	209046	20.472	ug/l	100
92) 1,2-Dibromo-3-Chloropr...	14.273	75	10278	17.023	ug/l	96
93) 1,2,4-Trichlorobenzene	14.919	180	114772	18.029	ug/l	99
94) Hexachlorobutadiene	15.023	225	80710	20.338	ug/l	97
95) Naphthalene	15.145	128	155957	15.384	ug/l	99
96) 1,2,3-Trichlorobenzene	15.328	180	99805	18.100	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
Data File : VY023523.D
Acq On : 21 Oct 2025 10:04
Operator : SY/MD
Sample : VY1021SBS01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY1021SBS01

Manual Integrations
APPROVED

Reviewed By :Amit Patel 10/24/2025
Supervised By :Mahesh Dadoda 10/27/2025

Quant Time: Oct 24 01:22:08 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 05:12:50 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
 Data File : VY023523.D
 Acq On : 21 Oct 2025 10:04
 Operator : SY/MD
 Sample : VY1021SBS01
 Misc : 5.00g/5.0mL/MSVOA_Y/soil
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY1021SBS01

Manual Integrations APPROVED

Reviewed By :Amit Patel 10/24/2025
 Supervised By :Mahesh Dadoda 10/27/2025

Quant Time: Oct 24 01:22:08 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

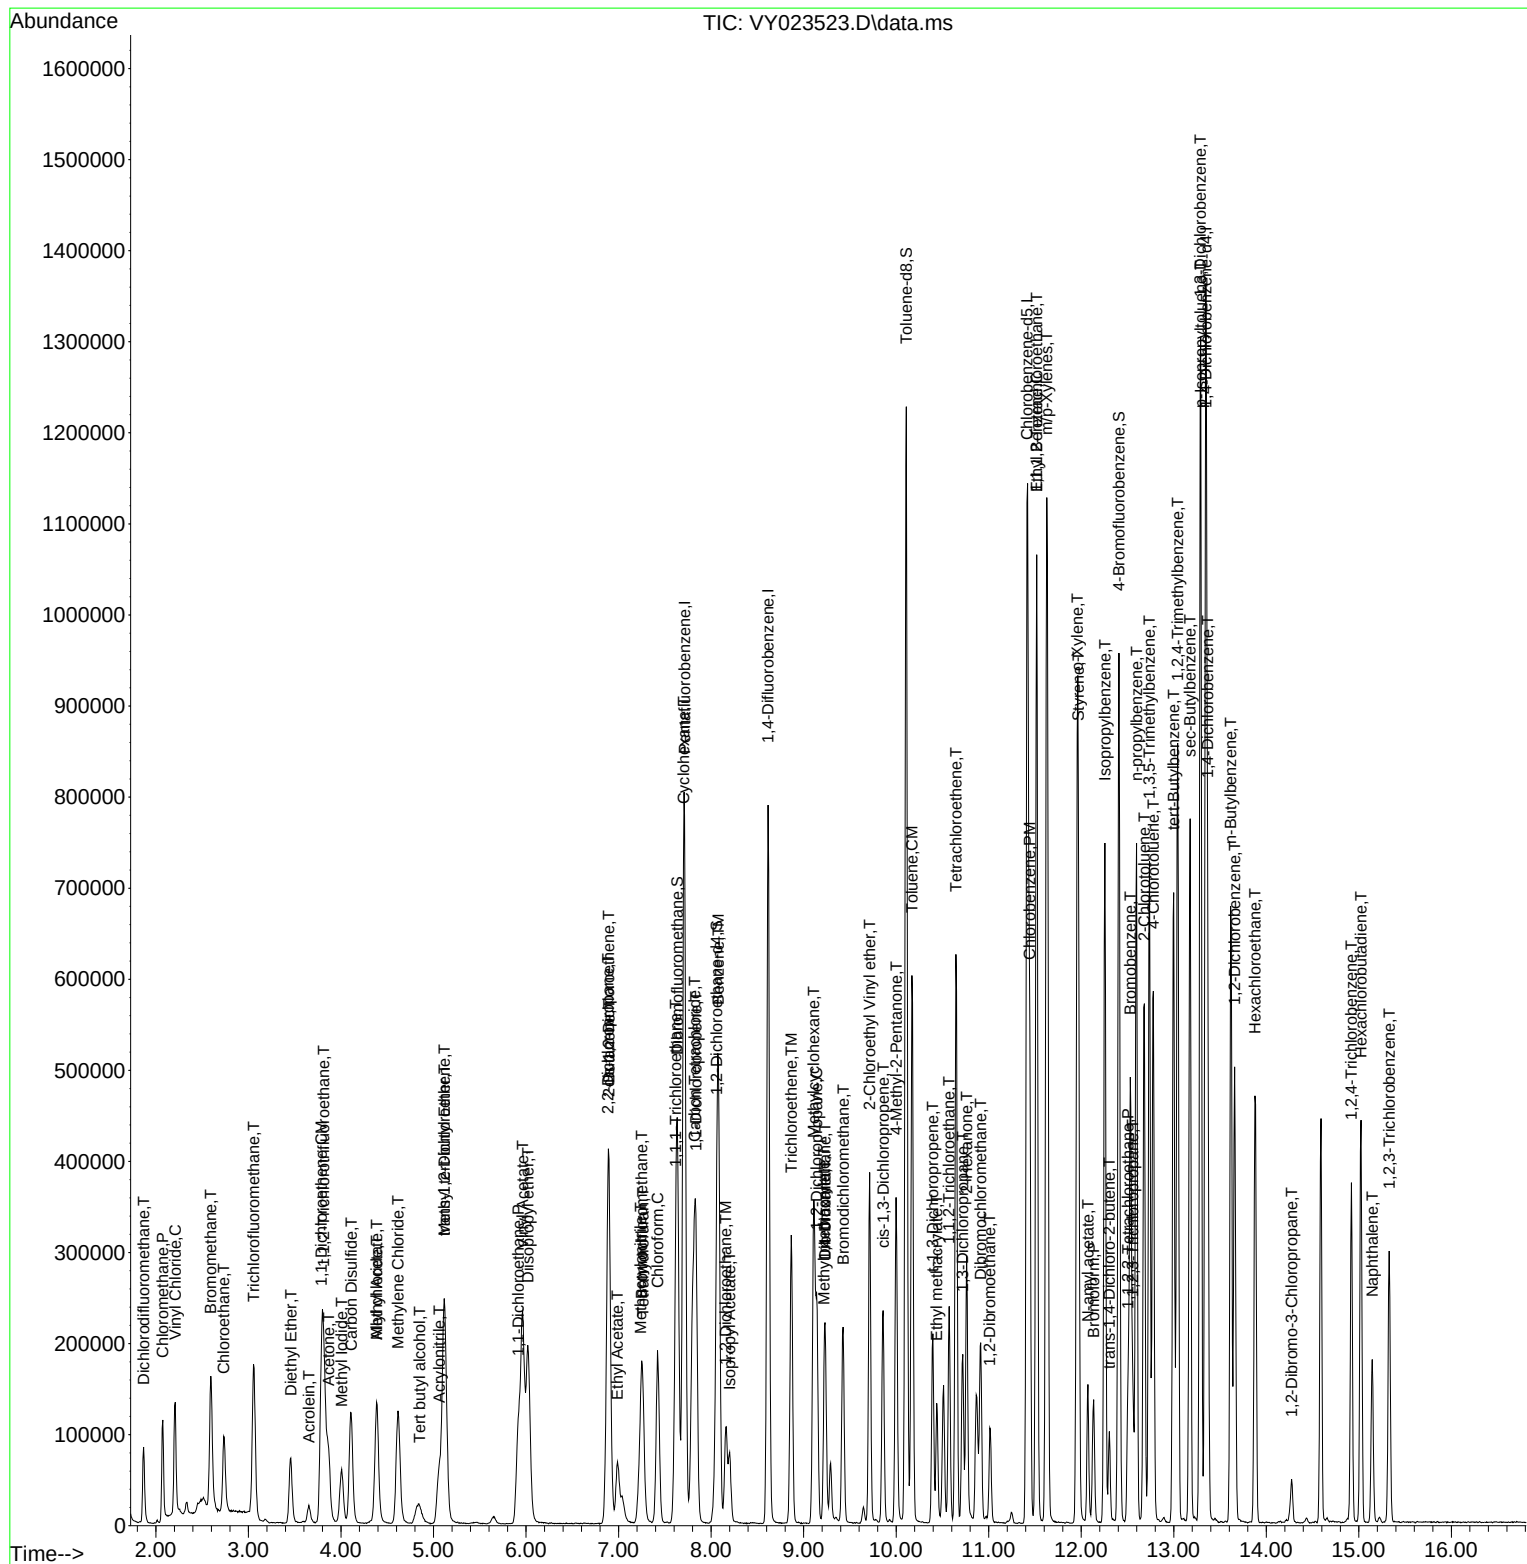

Report of Analysis

Client: Sciacca General Contractors, LLC

Project: 49 Moore Place Belleville

Client Sample ID: VY1021SBSD01

Lab Sample ID: VY1021SBSD01

Analytical Method: 8260D

Level : LOW

Sample Wt/Vol: 5 g

Final Vol: 5000 uL

Date Collected:

Date Received:

SDG No.: Q3410

Matrix: SOIL

% Solid: 100

Test: VOC-TCLVOA-10

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Date Ana.	BatchID
TARGETS									
75-71-8	Dichlorodifluoromethane	20.9		1	1.10	5.00	ug/Kg	10/21/25 10:27	VY102125
74-87-3	Chloromethane	19.3		1	1.10	5.00	ug/Kg	10/21/25 10:27	VY102125
75-01-4	Vinyl Chloride	20.0		1	0.79	5.00	ug/Kg	10/21/25 10:27	VY102125
74-83-9	Bromomethane	20.7		1	1.10	5.00	ug/Kg	10/21/25 10:27	VY102125
75-00-3	Chloroethane	21.4		1	1.30	5.00	ug/Kg	10/21/25 10:27	VY102125
75-69-4	Trichlorofluoromethane	20.6		1	1.20	5.00	ug/Kg	10/21/25 10:27	VY102125
76-13-1	1,1,2-Trichlorotrifluoroethane	20.7		1	1.10	5.00	ug/Kg	10/21/25 10:27	VY102125
75-35-4	1,1-Dichloroethene	20.6		1	1.00	5.00	ug/Kg	10/21/25 10:27	VY102125
67-64-1	Acetone	120		1	4.70	25.0	ug/Kg	10/21/25 10:27	VY102125
75-15-0	Carbon Disulfide	19.7		1	1.10	5.00	ug/Kg	10/21/25 10:27	VY102125
1634-04-4	Methyl tert-butyl Ether	18.2		1	0.73	5.00	ug/Kg	10/21/25 10:27	VY102125
79-20-9	Methyl Acetate	15.6		1	1.50	5.00	ug/Kg	10/21/25 10:27	VY102125
75-09-2	Methylene Chloride	18.9		1	3.50	10.0	ug/Kg	10/21/25 10:27	VY102125
156-60-5	trans-1,2-Dichloroethene	20.6		1	0.86	5.00	ug/Kg	10/21/25 10:27	VY102125
75-34-3	1,1-Dichloroethane	20.6		1	0.80	5.00	ug/Kg	10/21/25 10:27	VY102125
110-82-7	Cyclohexane	18.6		1	0.79	5.00	ug/Kg	10/21/25 10:27	VY102125
78-93-3	2-Butanone	100		1	6.50	25.0	ug/Kg	10/21/25 10:27	VY102125
56-23-5	Carbon Tetrachloride	21.0		1	0.97	5.00	ug/Kg	10/21/25 10:27	VY102125
156-59-2	cis-1,2-Dichloroethene	20.5		1	0.75	5.00	ug/Kg	10/21/25 10:27	VY102125
74-97-5	Bromochloromethane	19.6		1	1.20	5.00	ug/Kg	10/21/25 10:27	VY102125
67-66-3	Chloroform	21.0		1	0.84	5.00	ug/Kg	10/21/25 10:27	VY102125
71-55-6	1,1,1-Trichloroethane	20.8		1	0.93	5.00	ug/Kg	10/21/25 10:27	VY102125
108-87-2	Methylcyclohexane	19.5		1	0.91	5.00	ug/Kg	10/21/25 10:27	VY102125
71-43-2	Benzene	21.6		1	0.79	5.00	ug/Kg	10/21/25 10:27	VY102125
107-06-2	1,2-Dichloroethane	20.0		1	0.79	5.00	ug/Kg	10/21/25 10:27	VY102125
79-01-6	Trichloroethene	21.2		1	0.81	5.00	ug/Kg	10/21/25 10:27	VY102125
78-87-5	1,2-Dichloropropane	20.7		1	0.91	5.00	ug/Kg	10/21/25 10:27	VY102125
75-27-4	Bromodichloromethane	21.2		1	0.78	5.00	ug/Kg	10/21/25 10:27	VY102125
108-10-1	4-Methyl-2-Pentanone	86.8		1	3.60	25.0	ug/Kg	10/21/25 10:27	VY102125
108-88-3	Toluene	21.4		1	0.78	5.00	ug/Kg	10/21/25 10:27	VY102125
10061-02-6	t-1,3-Dichloropropene	19.5		1	0.65	5.00	ug/Kg	10/21/25 10:27	VY102125
10061-01-5	cis-1,3-Dichloropropene	20.2		1	0.62	5.00	ug/Kg	10/21/25 10:27	VY102125
79-00-5	1,1,2-Trichloroethane	20.2		1	0.92	5.00	ug/Kg	10/21/25 10:27	VY102125
591-78-6	2-Hexanone	96.5		1	3.70	25.0	ug/Kg	10/21/25 10:27	VY102125
124-48-1	Dibromochloromethane	20.5		1	0.87	5.00	ug/Kg	10/21/25 10:27	VY102125
106-93-4	1,2-Dibromoethane	20.2		1	0.88	5.00	ug/Kg	10/21/25 10:27	VY102125
127-18-4	Tetrachloroethene	22.1		1	1.10	5.00	ug/Kg	10/21/25 10:27	VY102125
108-90-7	Chlorobenzene	21.2		1	0.91	5.00	ug/Kg	10/21/25 10:27	VY102125
100-41-4	Ethyl Benzene	20.8		1	0.67	5.00	ug/Kg	10/21/25 10:27	VY102125
179601-23-1	m/p-Xylenes	42.7		1	1.20	10.0	ug/Kg	10/21/25 10:27	VY102125
95-47-6	o-Xylene	20.7		1	0.82	5.00	ug/Kg	10/21/25 10:27	VY102125
100-42-5	Styrene	20.5		1	0.71	5.00	ug/Kg	10/21/25 10:27	VY102125
75-25-2	Bromoform	19.6		1	0.86	5.00	ug/Kg	10/21/25 10:27	VY102125



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client: Sciacca General Contractors, LLC

Project: 49 Moore Place Belleville

Client Sample ID: VY1021SBSD01

Lab Sample ID: VY1021SBSD01

Analytical Method: 8260D

Sample Wt/Vol: 5 g

Level : LOW

Final Vol: 5000 uL

Date Collected:

Date Received:

SDG No.: Q3410

Matrix: SOIL

% Solid: 100

Test: VOC-TCLVOA-10

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Date Ana.	BatchID
98-82-8	Isopropylbenzene	20.3		1	0.78	5.00	ug/Kg	10/21/25 10:27	VY102125
79-34-5	1,1,2,2-Tetrachloroethane	18.8		1	1.20	5.00	ug/Kg	10/21/25 10:27	VY102125
541-73-1	1,3-Dichlorobenzene	20.8		1	1.70	5.00	ug/Kg	10/21/25 10:27	VY102125
106-46-7	1,4-Dichlorobenzene	20.6		1	1.60	5.00	ug/Kg	10/21/25 10:27	VY102125
95-50-1	1,2-Dichlorobenzene	20.5		1	1.50	5.00	ug/Kg	10/21/25 10:27	VY102125
96-12-8	1,2-Dibromo-3-Chloropropane	17.3		1	1.80	5.00	ug/Kg	10/21/25 10:27	VY102125
120-82-1	1,2,4-Trichlorobenzene	19.1		1	3.00	5.00	ug/Kg	10/21/25 10:27	VY102125
87-61-6	1,2,3-Trichlorobenzene	18.8		1	3.20	5.00	ug/Kg	10/21/25 10:27	VY102125

SURROGATES

17060-07-0	1,2-Dichloroethane-d4	45.6			63 - 155	91%	SPK: 50
1868-53-7	Dibromofluoromethane	49.6			70 - 134	99%	SPK: 50
2037-26-5	Toluene-d8	49.7			74 - 123	99%	SPK: 50
460-00-4	4-Bromofluorobenzene	47.7			17 - 146	95%	SPK: 50

INTERNAL STANDARDS

Area Count

363-72-4	Pentafluorobenzene	508000
540-36-3	1,4-Difluorobenzene	738000
3114-55-4	Chlorobenzene-d5	649000
3855-82-1	1,4-Dichlorobenzene-d4	346000

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
 Data File : VY023524.D
 Acq On : 21 Oct 2025 10:27
 Operator : SY/MD
 Sample : VY1021SBS01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY1021SBS01

Manual Integrations
 APPROVED

Reviewed By :Amit Patel 10/24/2025
 Supervised By :Mahesh Dadoda 10/27/2025

Quant Time: Oct 24 01:22:56 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.713	168	507725	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.615	114	737688	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	649036	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	345630	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	193552	45.588	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery =	91.180%		
35) Dibromofluoromethane	7.640	113	224981	49.635	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery =	99.260%		
50) Toluene-d8	10.109	98	839480	49.731	ug/l	0.00
Spiked Amount 50.000	Range 58 - 134		Recovery =	99.460%		
62) 4-Bromofluorobenzene	12.407	95	265572	47.653	ug/l	0.00
Spiked Amount 50.000	Range 30 - 143		Recovery =	95.300%		
Target Compounds					Qvalue	
2) Dichlorodifluoromethane	1.867	85	76535	20.942	ug/l	97
3) Chloromethane	2.074	50	96007	19.285	ug/l	94
4) Vinyl Chloride	2.208	62	129832	20.022	ug/l	98
5) Bromomethane	2.592	94	112639	20.700	ug/l	95
6) Chloroethane	2.732	64	94469	21.373	ug/l	95
7) Trichlorofluoromethane	3.055	101	185484	20.601	ug/l	99
8) Diethyl Ether	3.458	74	43119	18.328	ug/l	100
9) 1,1,2-Trichlorotrifluo...	3.818	101	96666	20.690	ug/l	98
10) Methyl Iodide	4.007	142	105061	20.199	ug/l	99
11) Tert butyl alcohol	4.854	59	29782	94.291	ug/l #	86
12) 1,1-Dichloroethene	3.787	96	93147	20.567	ug/l	97
13) Acrolein	3.653	56	22812	51.113	ug/l	100
14) Allyl chloride	4.391	41	104298	18.896	ug/l	98
15) Acrylonitrile	5.067	53	80058	88.919	ug/l	100
16) Acetone	3.866	43	119903	118.627	ug/l	99
17) Carbon Disulfide	4.110	76	255071	19.677	ug/l	100
18) Methyl Acetate	4.385	43	41344	15.593	ug/l	99
19) Methyl tert-butyl Ether	5.122	73	198449	18.231	ug/l	99
20) Methylene Chloride	4.622	84	103156	18.874	ug/l	98
21) trans-1,2-Dichloroethene	5.122	96	102505	20.557	ug/l	95
22) Diisopropyl ether	6.024	45	241142	19.751	ug/l	100
23) Vinyl Acetate	5.963	43	608978	92.150	ug/l	99
24) 1,1-Dichloroethane	5.915	63	166872	20.633	ug/l	99
25) 2-Butanone	6.896	43	123377	99.983	ug/l	97
26) 2,2-Dichloropropane	6.884	77	153398	20.671	ug/l	100
27) cis-1,2-Dichloroethene	6.890	96	118114	20.507	ug/l	98
28) Bromochloromethane	7.244	49	59036	19.554	ug/l	99
29) Tetrahydrofuran	7.262	42	56628	80.926	ug/l	98
30) Chloroform	7.427	83	186548	20.994	ug/l	98
31) Cyclohexane	7.707	56	131398	18.604	ug/l #	88
32) 1,1,1-Trichloroethane	7.622	97	167846	20.786	ug/l	99
36) 1,1-Dichloropropene	7.835	75	125854	20.973	ug/l	99
37) Ethyl Acetate	6.988	43	42506	17.879	ug/l	97
38) Carbon Tetrachloride	7.817	117	152959	21.021	ug/l	99
39) Methylcyclohexane	9.109	83	152680	19.541	ug/l	97
40) Benzene	8.085	78	409670	21.557	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
 Data File : VY023524.D
 Acq On : 21 Oct 2025 10:27
 Operator : SY/MD
 Sample : VY1021SBSD01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY1021SBSD01

Manual Integrations
 APPROVED

Reviewed By :Amit Patel 10/24/2025
 Supervised By :Mahesh Dadoda 10/27/2025

Quant Time: Oct 24 01:22:56 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	7.244	41	25328m	19.698	ug/l	
42) 1,2-Dichloroethane	8.158	62	97868	19.968	ug/l	98
43) Isopropyl Acetate	8.201	43	83604	17.636	ug/l	96
44) Trichloroethene	8.865	130	117839	21.185	ug/l	97
45) 1,2-Dichloropropane	9.140	63	86878	20.697	ug/l	96
46) Dibromomethane	9.231	93	54393	20.493	ug/l	98
47) Bromodichloromethane	9.426	83	141737	21.203	ug/l	97
48) Methyl methacrylate	9.225	41	36374	16.333	ug/l	93
49) 1,4-Dioxane	9.231	88	11187	363.519	ug/l	94
51) 4-Methyl-2-Pentanone	9.999	43	212509	86.764	ug/l	99
52) Toluene	10.170	92	264651	21.448	ug/l	99
53) t-1,3-Dichloropropene	10.396	75	113570	19.539	ug/l	99
54) cis-1,3-Dichloropropene	9.859	75	138303	20.160	ug/l	96
55) 1,1,2-Trichloroethane	10.572	97	72099	20.200	ug/l	96
56) Ethyl methacrylate	10.438	69	71577	17.385	ug/l	97
57) 1,3-Dichloropropane	10.719	76	115753	20.466	ug/l	100
58) 2-Chloroethyl Vinyl ether	9.713	63	157950	85.637	ug/l	99
59) 2-Hexanone	10.761	43	168854	96.468	ug/l	99
60) Dibromochloromethane	10.914	129	102818	20.546	ug/l	99
61) 1,2-Dibromoethane	11.011	107	68658	20.170	ug/l	98
64) Tetrachloroethene	10.646	164	148305	22.130	ug/l	96
65) Chlorobenzene	11.444	112	298892	21.174	ug/l	100
66) 1,1,1,2-Tetrachloroethane	11.517	131	105088	20.891	ug/l	99
67) Ethyl Benzene	11.517	91	475071	20.791	ug/l	100
68) m/p-Xylenes	11.627	106	391375	42.703	ug/l	100
69) o-Xylene	11.956	106	178360	20.748	ug/l	98
70) Styrene	11.969	104	290473	20.548	ug/l	99
71) Bromoform	12.133	173	61136	19.593	ug/l #	100
73) Isopropylbenzene	12.255	105	463044	20.329	ug/l	100
74) N-amyl acetate	12.072	43	68201	16.670	ug/l	97
75) 1,1,2,2-Tetrachloroethane	12.505	83	70214	18.847	ug/l	100
76) 1,2,3-Trichloropropane	12.554	75	63070m	20.683	ug/l	
77) Bromobenzene	12.529	156	123338	20.368	ug/l	98
78) n-propylbenzene	12.596	91	549380	20.843	ug/l	100
79) 2-Chlorotoluene	12.676	91	317913	20.597	ug/l	99
80) 1,3,5-Trimethylbenzene	12.737	105	383903	20.858	ug/l	100
81) trans-1,4-Dichloro-2-b...	12.304	75	22311	17.942	ug/l	97
82) 4-Chlorotoluene	12.773	91	329355	20.719	ug/l	99
83) tert-Butylbenzene	12.999	119	348123	20.485	ug/l	99
84) 1,2,4-Trimethylbenzene	13.041	105	381863	20.789	ug/l	100
85) sec-Butylbenzene	13.176	105	513781	21.075	ug/l	99
86) p-Isopropyltoluene	13.291	119	434529	20.935	ug/l	99
87) 1,3-Dichlorobenzene	13.285	146	245648	20.832	ug/l	98
88) 1,4-Dichlorobenzene	13.365	146	239545	20.569	ug/l	99
89) n-Butylbenzene	13.615	91	366353	20.257	ug/l	99
90) Hexachloroethane	13.877	117	92759	20.778	ug/l	98
91) 1,2-Dichlorobenzene	13.657	146	212289	20.535	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	14.273	75	10564	17.282	ug/l	99
93) 1,2,4-Trichlorobenzene	14.919	180	123359	19.140	ug/l	99
94) Hexachlorobutadiene	15.023	225	84356	20.997	ug/l	100
95) Naphthalene	15.145	128	169169	16.483	ug/l	99
96) 1,2,3-Trichlorobenzene	15.328	180	104991	18.807	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
Data File : VY023524.D
Acq On : 21 Oct 2025 10:27
Operator : SY/MD
Sample : VY1021SBSD01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY1021SBSD01

Manual Integrations
APPROVED

Reviewed By :Amit Patel 10/24/2025
Supervised By :Mahesh Dadoda 10/27/2025

Quant Time: Oct 24 01:22:56 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 05:12:50 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102125\
Data File : VY023524.D
Acq On : 21 Oct 2025 10:27
Operator : SY/MD
Sample : VY1021SBSD01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY1021SBSD01

Manual Integrations

Reviewed By :Amit Patel 10/24/2025
Supervised By :Mahesh Dadoda 10/27/2025

Quant Time: Oct 24 01:22:56 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 05:12:50 2025
Response via : Initial Calibration

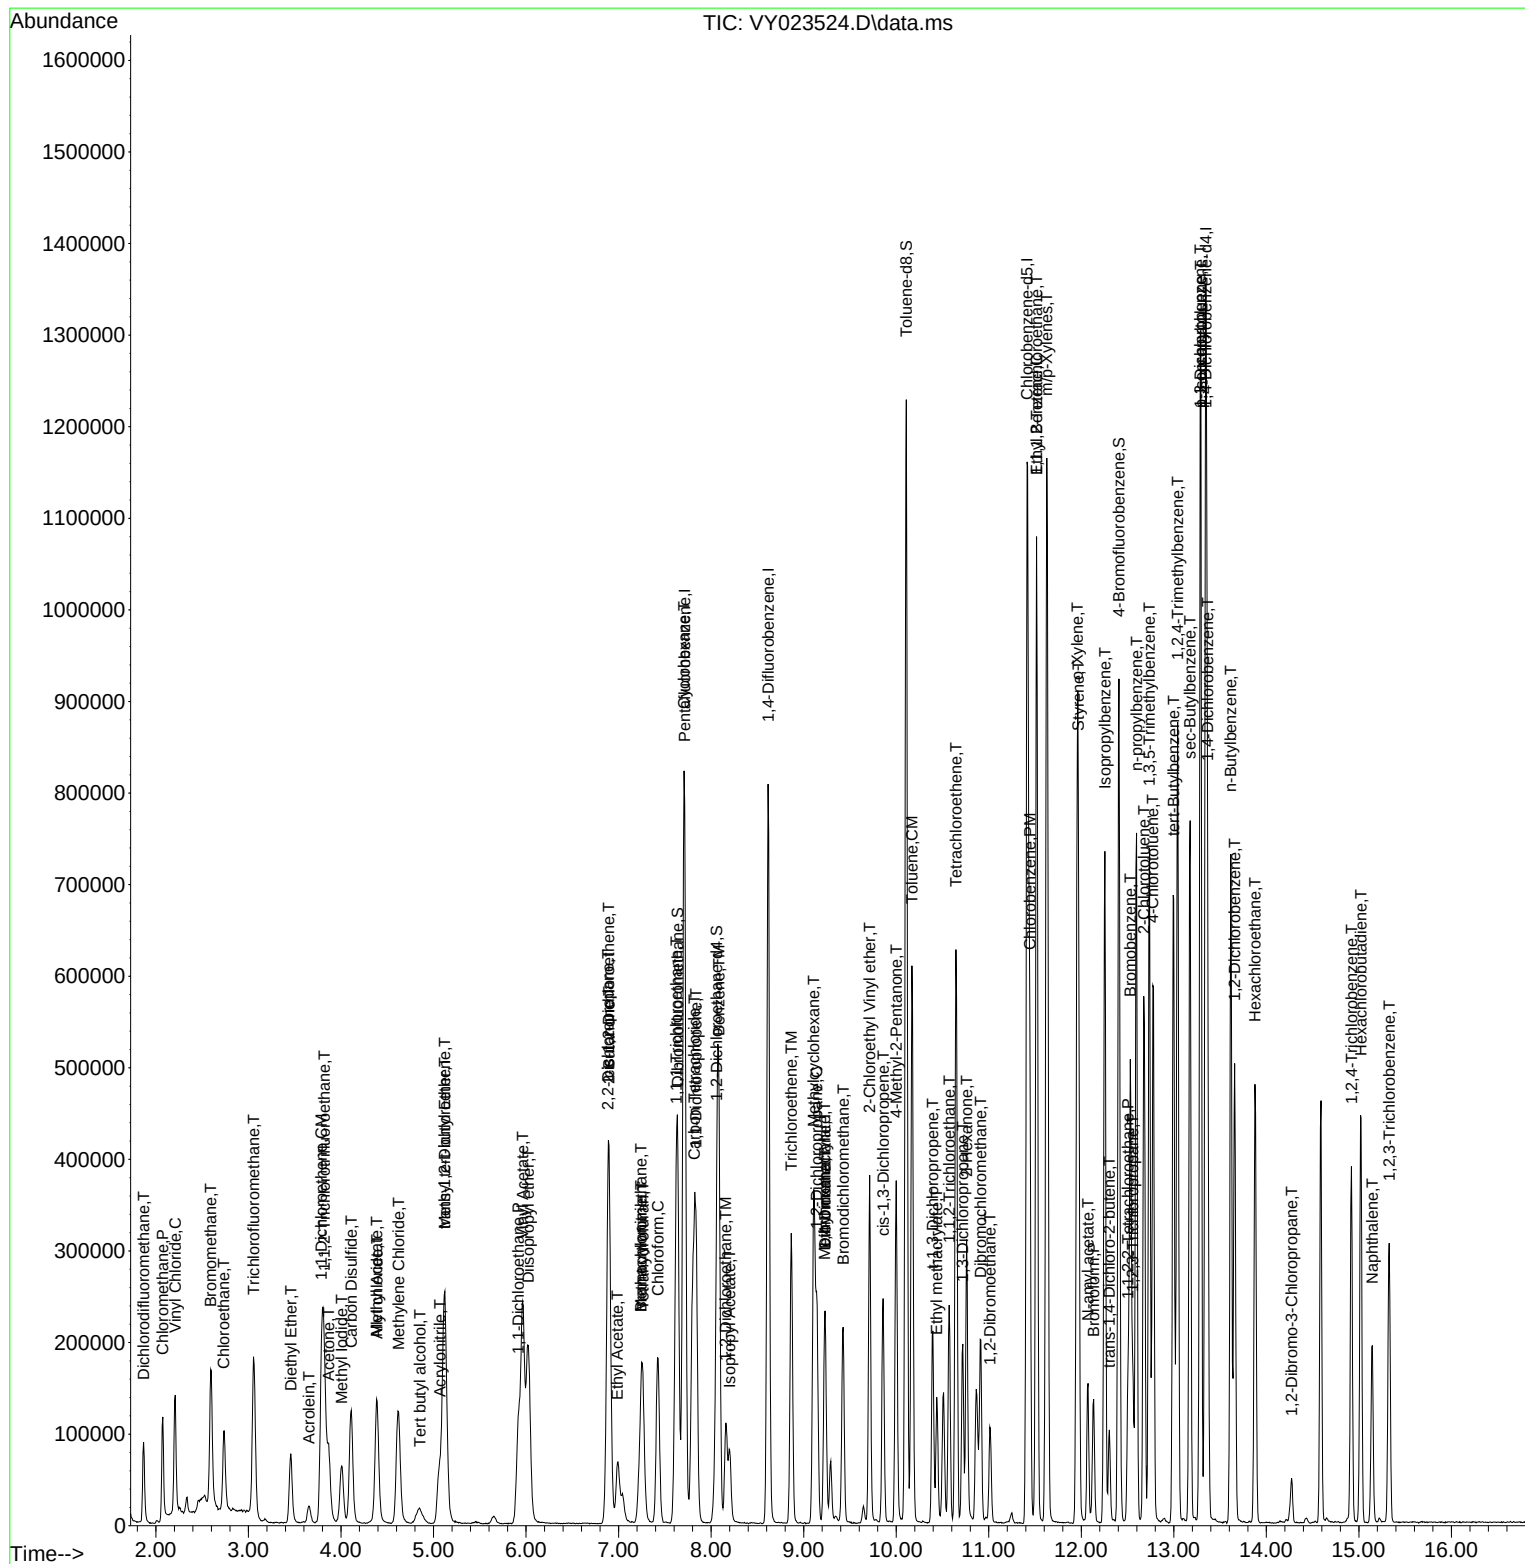

Manual Integration Report

Sequence:	VY100725	Instrument	MSVOA_y
-----------	----------	------------	---------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
VSTDICC005	VY023384.D	1,2,3-Trichloropropane	sam	10/10/2025 2:59:48 AM	MMdadoda	10/10/2025 4:37:28 AM	Peak Integrated by Software
VSTDICC005	VY023384.D	2-Chloroethyl Vinyl ether	sam	10/10/2025 2:59:48 AM	MMdadoda	10/10/2025 4:37:28 AM	Peak Integrated by Software
VSTDICC005	VY023384.D	Methacrylonitrile	sam	10/10/2025 2:59:48 AM	MMdadoda	10/10/2025 4:37:28 AM	Peak Integrated by Software
VSTDICC010	VY023385.D	1,2,3-Trichloropropane	sam	10/10/2025 2:59:52 AM	MMdadoda	10/10/2025 4:37:33 AM	Peak Integrated by Software
VSTDICC010	VY023385.D	2-Chloroethyl Vinyl ether	sam	10/10/2025 2:59:52 AM	MMdadoda	10/10/2025 4:37:33 AM	Peak Integrated by Software
VSTDICC020	VY023386.D	1,2,3-Trichloropropane	sam	10/10/2025 2:59:56 AM	MMdadoda	10/10/2025 4:37:37 AM	Peak Integrated by Software
VSTDICC020	VY023386.D	2-Chloroethyl Vinyl ether	sam	10/10/2025 2:59:56 AM	MMdadoda	10/10/2025 4:37:37 AM	Peak Integrated by Software
VSTDICC020	VY023386.D	Methacrylonitrile	sam	10/10/2025 2:59:56 AM	MMdadoda	10/10/2025 4:37:37 AM	Peak Integrated by Software
VSTDICCC050	VY023387.D	1,2,3-Trichloropropane	sam	10/10/2025 3:00:01 AM	MMdadoda	10/10/2025 4:37:41 AM	Peak Integrated by Software
VSTDICC100	VY023388.D	1,2,3-Trichloropropane	sam	10/10/2025 3:00:05 AM	MMdadoda	10/10/2025 4:37:46 AM	Peak Integrated by Software
VSTDICC150	VY023389.D	1,2,3-Trichloropropane	sam	10/10/2025 3:00:09 AM	MMdadoda	10/10/2025 4:37:51 AM	Peak Integrated by Software
VSTDICV050	VY023391.D	1,2,3-Trichloropropane	sam	10/10/2025 3:00:14 AM	MMdadoda	10/10/2025 4:37:55 AM	Peak Integrated by Software



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

Manual Integration Report

Sequence:

VY100725

Instrument

MSVOA_y

Sample ID

File ID

Parameter

Review By

Review On

Supervised
By

Supervised On

Reason

Manual Integration Report

Sequence:

VY102125

Instrument

MSVOA_y

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
VSTDCCC050	VY023521.D	1,2,3-Trichloropropane	Amit	10/24/2025 11:55:48 AM	 	 	Peak Integrated by Software
VY1021SBS01	VY023523.D	1,2,3-Trichloropropane	Amit	10/24/2025 11:55:53 AM	 	 	Peak Integrated by Software
VY1021SBS01	VY023523.D	Methacrylonitrile	Amit	10/24/2025 11:55:53 AM	 	 	Peak Integrated by Software
VY1021SBSD0 1	VY023524.D	1,2,3-Trichloropropane	Amit	10/24/2025 11:55:57 AM	 	 	Peak Integrated by Software
VY1021SBSD0 1	VY023524.D	Methacrylonitrile	Amit	10/24/2025 11:55:57 AM	 	 	Peak Integrated by Software

Instrument ID: **MSVOA_Y**

Daily Analysis Runlog For Sequence/QC Batch ID # VY100725

Review By	Semsettin Yesilyurt	Review On	10/10/2025 3:00:22 AM		
Supervise By	Maresh Dadoda	Supervise On	10/10/2025 4:38:02 AM		
SubDirectory	VY100725	HP Acquire Method	MSVOA_Y	HP Processing Method	82y100725s.m
STD. NAME		STD REF.#			
Tune/Reschk		VP135766			
Initial Calibration Stds		VP135767,VP135768,VP135769,VP135770,VP135771,VP135772			
CCC					
Internal Standard/PEM		VP133934			
ICV/I.BLK		VP135773			
Surrogate Standard					
MS/MSD Standard					
LCS Standard					

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VY023383.D	07 Oct 2025 08:43	SY/MD	Ok
2	VSTDIC005	VY023384.D	07 Oct 2025 09:17	SY/MD	Ok,M
3	VSTDIC010	VY023385.D	07 Oct 2025 10:02	SY/MD	Ok,M
4	VSTDIC020	VY023386.D	07 Oct 2025 11:24	SY/MD	Ok,M
5	VSTDIC050	VY023387.D	07 Oct 2025 11:47	SY/MD	Ok,M
6	VSTDIC100	VY023388.D	07 Oct 2025 12:09	SY/MD	Ok,M
7	VSTDIC150	VY023389.D	07 Oct 2025 12:32	SY/MD	Ok,M
8	VIBLK	VY023390.D	07 Oct 2025 13:02	SY/MD	Ok
9	VSTDICV050	VY023391.D	07 Oct 2025 14:12	SY/MD	Ok,M

M : Manual Integration

Instrument ID: **MSVOA_Y**

Daily Analysis Runlog For Sequence/QC Batch ID # VY102125

Review By	John Carlone	Review On	10/24/2025 2:07:04 PM
Supervise By		Supervise On	
SubDirectory	VY102125	HP Acquire Method	MSVOA_Y
		HP Processing Method	82y100725s.m
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP135871		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP135872,VP135873 VP133934		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VY023520.D	21 Oct 2025 08:29	SY/MD	Ok
2	VSTDCCC050	VY023521.D	21 Oct 2025 09:05	SY/MD	Ok,NS
3	VY1021SBL01	VY023522.D	21 Oct 2025 09:34	SY/MD	Ok
4	VY1021SBS01	VY023523.D	21 Oct 2025 10:04	SY/MD	Ok,NS
5	VY1021SBSD01	VY023524.D	21 Oct 2025 10:27	SY/MD	Ok,NS
6	Q3383-01	VY023525.D	21 Oct 2025 11:03	SY/MD	Ok
7	Q3382-01	VY023526.D	21 Oct 2025 11:26	SY/MD	Ok
8	Q3386-01RE	VY023527.D	21 Oct 2025 11:50	SY/MD	Confirms
9	Q3376-02	VY023528.D	21 Oct 2025 12:14	SY/MD	Ok
10	Q3393-03	VY023529.D	21 Oct 2025 12:38	SY/MD	Ok
11	Q3402-01	VY023530.D	21 Oct 2025 13:04	SY/MD	Ok
12	Q3402-04	VY023531.D	21 Oct 2025 13:48	SY/MD	Ok
13	Q3402-07	VY023532.D	21 Oct 2025 14:12	SY/MD	Ok
14	Q3402-10	VY023533.D	21 Oct 2025 14:35	SY/MD	Ok
15	Q3399-03	VY023534.D	21 Oct 2025 14:59	SY/MD	Ok
16	Q3410-02	VY023535.D	21 Oct 2025 15:22	SY/MD	Ok
17	Q3403-03	VY023536.D	21 Oct 2025 15:47	SY/MD	Ok
18	Q3406-01	VY023537.D	21 Oct 2025 16:10	SY/MD	Ok
19	Q3413-01	VY023538.D	21 Oct 2025 16:34	SY/MD	Not Ok
20	Q3412-03	VY023539.D	21 Oct 2025 16:57	SY/MD	Ok
21	Q3404-01	VY023540.D	21 Oct 2025 17:21	SY/MD	ReRun

Instrument ID: MSVOA_Y

Daily Analysis Runlog For Sequence/QCBatch ID # VY102125

Review By	John Carlone	Review On	10/24/2025 2:07:04 PM
Supervise By		Supervise On	
SubDirectory	VY102125	HP Acquire Method	MSVOA_Y
		HP Processing Method	82y100725s.m
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP135871		
CCC	VP135872,VP135873		
Internal Standard/PEM	VP133934		
ICV/I.BLK			
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	Q3395-03MS	VY023541.D	21 Oct 2025 17:44	SY/MD	Not Ok
----	------------	------------	-------------------	-------	--------

M : Manual Integration

Instrument ID: MSVOA_Y

Daily Analysis Runlog For Sequence/QC Batch ID # VY100725

Review By	Semsettin Yesilyurt	Review On	10/10/2025 3:00:22 AM
Supervise By	Maresh Dadoda	Supervise On	10/10/2025 4:38:02 AM
SubDirectory	VY100725	HP Acquire Method	MSVOA_Y HP Processing Method 82y100725s.m

STD. NAME	STD REF.#
Tune/Reschk	VP135766
Initial Calibration Stds	VP135767,VP135768,VP135769,VP135770,VP135771,VP135772
CCC	
Internal Standard/PEM	VP133934
ICV/I.BLK	VP135773
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleID	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	BFB	BFB	VY023383.D	07 Oct 2025 08:43		SY/MD	Ok
2	VSTDICC005	VSTDICC005	VY023384.D	07 Oct 2025 09:17		SY/MD	Ok,M
3	VSTDICC010	VSTDICC010	VY023385.D	07 Oct 2025 10:02		SY/MD	Ok,M
4	VSTDICC020	VSTDICC020	VY023386.D	07 Oct 2025 11:24		SY/MD	Ok,M
5	VSTDICCC050	VSTDICCC050	VY023387.D	07 Oct 2025 11:47		SY/MD	Ok,M
6	VSTDICC100	VSTDICC100	VY023388.D	07 Oct 2025 12:09		SY/MD	Ok,M
7	VSTDICC150	VSTDICC150	VY023389.D	07 Oct 2025 12:32		SY/MD	Ok,M
8	VIBLK	VIBLK	VY023390.D	07 Oct 2025 13:02		SY/MD	Ok
9	VSTDICV050	ICVVY100725	VY023391.D	07 Oct 2025 14:12		SY/MD	Ok,M

M : Manual Integration

Instrument ID: MSVOA_Y

Daily Analysis Runlog For Sequence/QC Batch ID # VY102125

Review By	John Carlone	Review On	10/24/2025 2:07:04 PM
Supervise By		Supervise On	
SubDirectory	VY102125	HP Acquire Method	MSVOA_Y HP Processing Method 82y100725s.m

STD. NAME	STD REF.#
Tune/Reschk Initial Calibration Stds	VP135871
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP135872,VP135873 VP133934

Sr#	SampleID	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	BFB	BFB	VY023520.D	21 Oct 2025 08:29		SY/MD	Ok
2	VSTDCCC050	VSTDCCC050	VY023521.D	21 Oct 2025 09:05		SY/MD	Ok,NS
3	VY1021SBL01	VY1021SBL01	VY023522.D	21 Oct 2025 09:34		SY/MD	Ok
4	VY1021SBS01	VY1021SBS01	VY023523.D	21 Oct 2025 10:04		SY/MD	Ok,NS
5	VY1021SBSD01	VY1021SBSD01	VY023524.D	21 Oct 2025 10:27		SY/MD	Ok,NS
6	Q3383-01	OR-03-101725	VY023525.D	21 Oct 2025 11:03	vial-B	SY/MD	Ok
7	Q3382-01	CENTRAL-AVE-TP	VY023526.D	21 Oct 2025 11:26	vial-B Internal Standard Fail	SY/MD	Ok
8	Q3386-01RE	237RE	VY023527.D	21 Oct 2025 11:50	vial-B Internal Standard Fail	SY/MD	Confirms
9	Q3376-02	PR132-DP01-20251016	VY023528.D	21 Oct 2025 12:14	vial-B	SY/MD	Ok
10	Q3393-03	PR132-S08-013038-20	VY023529.D	21 Oct 2025 12:38	vial-B	SY/MD	Ok
11	Q3402-01	41-LA	VY023530.D	21 Oct 2025 13:04	vial-A	SY/MD	Ok
12	Q3402-04	41-RA	VY023531.D	21 Oct 2025 13:48	vial-A	SY/MD	Ok
13	Q3402-07	41-LB	VY023532.D	21 Oct 2025 14:12	vial-A	SY/MD	Ok
14	Q3402-10	41-RB	VY023533.D	21 Oct 2025 14:35	vial-A	SY/MD	Ok
15	Q3399-03	COMP-ROLLOFF	VY023534.D	21 Oct 2025 14:59	vial-A	SY/MD	Ok
16	Q3410-02	VOC	VY023535.D	21 Oct 2025 15:22	vial-A	SY/MD	Ok
17	Q3403-03	MH-18-VOC	VY023536.D	21 Oct 2025 15:47	vial-A	SY/MD	Ok
18	Q3406-01	ARS20-0037	VY023537.D	21 Oct 2025 16:10	vial-A	SY/MD	Ok

Instrument ID: MSVOA_Y

Daily Analysis Runlog For Sequence/QC Batch ID # VY102125

Review By	John Carlone	Review On	10/24/2025 2:07:04 PM
Supervise By		Supervise On	
SubDirectory	VY102125	HP Acquire Method	MSVOA_Y
		HP Processing Method	82y100725s.m
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP135871		
CCC	VP135872,VP135873		
Internal Standard/PEM	VP133934		
ICV/I.BLK			
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

19	Q3413-01	BP-VPB-184-GW-980-S	VY023538.D	21 Oct 2025 16:34	vial-A End CCC Missing	SY/MD	Not Ok
20	Q3412-03	TP-6-VOC	VY023539.D	21 Oct 2025 16:57	vial-A	SY/MD	Ok
21	Q3404-01	MOO-25-0285-0288	VY023540.D	21 Oct 2025 17:21	vial-A Internal standard fail	SY/MD	ReRun
22	Q3395-03MS	PR132-S07-000102-20	VY023541.D	21 Oct 2025 17:44	vial-B Internal Standard Fail	SY/MD	Not Ok

M : Manual Integration

PERCENT SOLID

Supervisor: Iwona
Analyst: jignesh
Date: 10/22/2025

OVENTEMP IN Celsius(°C): 107
Time IN: 17:15
In Date: 10/21/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 104
Time OUT: 08:15
Out Date: 10/22/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID-OVEN

QC:LB137592

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
Q3399-01	COMP-ROLLOFF	13	1.15	10.96	12.11	11.00	89.9	
Q3401-01	41-CONCRETE	1	1.00	1.00	2.00	2.00	100.0	Concrete sample
Q3402-01	41-LA	2	1.15	10.90	12.05	8.69	69.2	
Q3402-02	41-LA-E2	3	1.13	10.64	11.77	10.2	85.2	
Q3402-04	41-RA	4	1.16	10.73	11.89	7.61	60.1	
Q3402-05	41-RA-E2	5	1.16	10.98	12.14	7.39	56.7	
Q3402-07	41-LB	6	1.16	10.77	11.93	8.26	65.9	
Q3402-08	41-LB-E2	7	1.16	10.95	12.11	6.22	46.2	
Q3402-10	41-RB	8	1.11	10.87	11.98	7.01	54.3	
Q3402-11	41-RB-E2	9	1.15	10.68	11.83	9.78	80.8	
Q3403-01	MH-18	10	1.19	10.49	11.68	10.75	91.1	
Q3403-02	MH-18-EPH	11	1.16	10.66	11.82	10.8	90.4	
Q3403-03	MH-18-VOC	12	1.19	11.37	12.56	11.59	91.5	
Q3404-01	MOO-25-0285-0288	14	1.15	10.74	11.89	10.22	84.5	
Q3404-03	MOO-25-0285-0288-E2	15	1.19	10.42	11.61	9.77	82.3	
Q3404-04	MOO-25-0292	16	1.18	10.22	11.4	10.5	91.2	
Q3404-07	MOO-25-0292-EPH-2	17	1.14	10.27	11.41	10.44	90.6	
Q3405-01	PAD-10-20-25-A	18	1.00	1.00	2.00	2.00	100.0	Concrete sample
Q3405-02	PAD-10-20-25-B	19	1.00	1.00	2.00	2.00	100.0	Concrete sample
Q3405-03	PAD-10-20-25-C	20	1.00	1.00	2.00	2.00	100.0	Concrete sample
Q3405-04	SW-10-20-25-A	21	1.00	1.00	2.00	2.00	100.0	Concrete sample
Q3406-01	ARS20-0037	22	1.18	11.19	12.37	11.24	89.9	
Q3406-03	ARS20-0037-E2	23	1.18	11.48	12.66	11.4	89.0	
Q3407-01	L35-A	24	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-02	L35-B	25	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-03	L36-A	26	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-04	L36-B	27	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-05	L37-A	28	1.00	1.00	2.00	2.00	100.0	PILC



PERCENT SOLID

Supervisor: Iwona
Analyst: jignesh
Date: 10/22/2025

OVENTEMP IN Celsius(°C): 107
Time IN: 17:15
In Date: 10/21/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 104
Time OUT: 08:15
Out Date: 10/22/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID-OVEN

QC:LB137592

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
Q3407-06	L37-B	29	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-07	L38-A	30	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-08	L38-B	31	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-09	L39-A	32	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-10	L39-B	33	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-11	L40-A	34	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-12	L40-B	35	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-13	L41-A	36	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-14	L41-B	37	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-15	L42-A	38	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-16	L42-B	39	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-17	L43-A	40	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-18	L43-B	41	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-19	L44-A	42	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-20	L44-B	43	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-21	L45-A	44	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-22	L45-B	45	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-23	L46-A	46	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-24	L46-B	47	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-25	L47-A	48	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-26	L47-B	49	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-27	L48-A	50	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-28	L48-B	51	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-29	L49-A	52	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-30	L49-B	53	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-31	L50-A	54	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-32	L50-B	55	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-33	L51-A	56	1.00	1.00	2.00	2.00	100.0	PILC



PERCENT SOLID

Supervisor: Iwona
Analyst: jignesh
Date: 10/22/2025

OVENTEMP IN Celsius(°C): 107
Time IN: 17:15
In Date: 10/21/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 104
Time OUT: 08:15
Out Date: 10/22/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID-OVEN

QC:LB137592

Lab ID	Client SampleID	Dish #	Dish Wt (g) (A)	Sample Wt (g)	Dish + Sample Wt (g) (B)	Dish+Dry Sample Wt (g) (C)	% Solid	Comments
Q3407-34	L51-B	57	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-35	L52-A	58	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-36	L52-B	59	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-37	L53-A	60	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-38	L53-B	61	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-39	245F69-A	62	1.00	1.00	2.00	2.00	100.0	PILC
Q3407-40	245F69-B	63	1.00	1.00	2.00	2.00	100.0	PILC
Q3408-01	ASPHALT-A	64	1.00	1.00	2.00	2.00	100.0	ASPHALT
Q3408-02	ASPHALT-B	65	1.00	1.00	2.00	2.00	100.0	ASPHALT
Q3408-03	ASPHALT-C	66	1.00	1.00	2.00	2.00	100.0	ASPHALT
Q3408-04	ASPHALT-D	67	1.00	1.00	2.00	2.00	100.0	ASPHALT
Q3409-01	EXCAVATION-AREA-A	68	1.00	1.00	2.00	2.00	100.0	Concreate sample
Q3409-02	EXCAVATION-AREA-B	69	1.00	1.00	2.00	2.00	100.0	Concreate sample
Q3410-01	WASTE	70	1.14	10.45	11.59	9.59	80.9	
Q3410-02	VOC	71	1.15	10.55	11.7	9.64	80.5	
Q3410-03	1	72	1.15	10.97	12.12	9.89	79.7	
Q3410-04	2	73	1.13	11.27	12.4	11.24	89.7	
Q3410-05	3	74	1.16	10.62	11.78	9.6	79.5	
Q3410-06	4	75	1.12	10.50	11.62	9.76	82.3	
Q3410-07	5	76	1.16	10.50	11.66	9.43	78.8	
Q3412-01	TP-6	77	1.14	10.81	11.95	10.84	89.7	
Q3412-02	TP-6-EPH	78	1.18	10.73	11.91	10.7	88.7	
Q3412-03	TP-6-VOC	79	1.15	10.52	11.67	10.38	87.7	
Q3413-01	BP-VPB-184-GW-980-982	80	1.14	11.55	12.69	2.00	7.4	sludge sample
Q3414-01	SB-1	81	1.13	10.12	11.25	11.17	99.2	
Q3414-02	SB-2	82	1.15	10.62	11.77	11.6	98.4	
Q3414-03	SB-3	83	1.13	10.53	11.66	11.4	97.5	
Q3414-04	SB-4	84	1.14	10.28	11.42	11.3	98.8	



PERCENT SOLID

Supervisor: Iwona
Analyst: jignesh
Date: 10/22/2025

OVENTEMP IN Celsius(°C): 107
Time IN: 17:15
In Date: 10/21/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 104
Time OUT: 08:15
Out Date: 10/22/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID-OVEN

QC:LB137592

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
Q3414-05	SB-5	85	1.16	10.25	11.41	11.34	99.3	
Q3414-06	SB-6	86	1.18	10.36	11.54	11.49	99.5	
Q3414-07	SB-7	87	1.15	10.25	11.4	11.26	98.6	
Q3414-08	SB-8	88	1.19	10.25	11.44	11.14	97.1	
Q3414-09	SB-9	89	1.16	10.31	11.47	11.18	97.2	
Q3414-10	SB-10	90	1.14	10.55	11.69	11.6	99.1	
Q3414-11	SB-11	91	1.19	10.20	11.39	11.04	96.6	
Q3414-12	SB-12	92	1.18	10.10	11.28	10.9	96.2	
Q3414-13	SB-13	93	1.14	10.06	11.2	10.85	96.5	
Q3415-01	50841	94	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q3415-02	50842	95	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q3415-03	50843	96	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q3416-01	NB-08-10212025	97	1.15	10.52	11.67	11.02	93.8	
Q3416-02	NB-08-10212025-E2	98	1.18	10.92	12.1	11.43	93.9	

$$\% \text{ Solid} = \frac{(C-A) * 100}{(B-A)}$$

WORKLIST(Hardcopy Internal Chain)

137592

WorkList Name : %1-102125 WorkList ID : 192565 Department : Wet-Chemistry Date : 10-21-2025 08:08:50

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q3399-01	COMP-ROLLOFF	Solid	Percent Solids	Cool 4 deg C	ICES02	D41	10/20/2025	Chemtech -SO
Q3401-01	41-CONCRETE	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3402-01	41-LA	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3402-02	41-LA-E2	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3402-04	41-RA	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3402-05	41-RA-E2	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3402-07	41-LB	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3402-08	41-LB-E2	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3402-10	41-RB	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3402-11	41-RB-E2	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3403-01	MH-18	Solid	Percent Solids	Cool 4 deg C	PSEG03	D41	10/20/2025	Chemtech -SO
Q3403-02	MH-18-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	D41	10/20/2025	Chemtech -SO
Q3403-03	MH-18-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	D41	10/20/2025	Chemtech -SO
Q3404-01	MOO-25-0285-0288	Solid	Percent Solids	Cool 4 deg C	PSEG03	D41	10/20/2025	Chemtech -SO
Q3404-03	MOO-25-0285-0288-E2	Solid	Percent Solids	Cool 4 deg C	PSEG03	D41	10/20/2025	Chemtech -SO
Q3404-04	MOO-25-0292	Solid	Percent Solids	Cool 4 deg C	PSEG03	D41	10/20/2025	Chemtech -SO
Q3404-07	MOO-25-0292-EPH-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	D41	10/20/2025	Chemtech -SO
Q3405-01	PAD-10-20-25-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3405-02	PAD-10-20-25-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3405-03	PAD-10-20-25-C	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3405-04	SW-10-20-25-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO

Date/Time 10/21/25 15:00 Date/Time 10/21/25 Date/Time 17130
 Raw Sample Received by: 88 WOC Raw Sample Received by: CP 8 Raw Sample Received by: 88 WOC
 Raw Sample Relinquished by: CP 8 Raw Sample Relinquished by: 88 WOC

WORKLIST(Hardcopy Internal Chain)

137592

WorkList Name : %1-102125 WorkList ID : 192565 Department : Wet-Chemistry Date : 10-21-2025 08:08:50

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q3406-01	ARS20-0037	Solid	Percent Solids	Cool 4 deg C	PSEG03	D41	10/20/2025	Chemtech -SO
Q3406-03	ARS20-0037-E2	Solid	Percent Solids	Cool 4 deg C	PSEG03	D41	10/20/2025	Chemtech -SO
Q3407-01	L35-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-02	L35-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-03	L36-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-04	L36-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-05	L37-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-06	L37-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-07	L38-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-08	L38-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-09	L39-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-10	L39-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-11	L40-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-12	L40-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-13	L41-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-14	L41-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-15	L42-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-16	L42-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-17	L43-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-18	L43-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-19	L44-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO

Date/Time 10/21/25 15:00
 Raw Sample Received by: SS WOC
 Raw Sample Relinquished by: QFS

Date/Time 10/21/25 17:30
 Raw Sample Received by: QFS
 Raw Sample Relinquished by: SS WOC

WORKLIST(Hardcopy Internal Chain)

137592

WorkList Name : %1-102125 WorkList ID : 192565 Department : Wet-Chemistry Date : 10-21-2025 08:08:50

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q3407-20	L44-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-21	L45-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-22	L45-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-23	L46-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-24	L46-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-25	L47-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-26	L47-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-27	L48-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-28	L48-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-29	L49-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-30	L49-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-31	L50-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-32	L50-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-33	L51-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-34	L51-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-35	L52-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-36	L52-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-37	L53-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-38	L53-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-39	245F69-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3407-40	245F69-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO

Date/Time 10/21/25 151.00
 Raw Sample Received by: [Signature]
 Raw Sample Relinquished by: [Signature]

Date/Time 10/21/25 17130
 Raw Sample Received by: [Signature]
 Raw Sample Relinquished by: [Signature]

WORKLIST(Hardcopy Internal Chain)

137592

WorkList Name : %1-102125 WorkList ID : 192565 Department : Wet-Chemistry Date : 10-21-2025 08:08:50

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q3408-01	ASPHALT-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D41	10/20/2025	Chemtech -SO
Q3408-02	ASPHALT-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D41	10/20/2025	Chemtech -SO
Q3408-03	ASPHALT-C	Solid	Percent Solids	Cool 4 deg C	PSEG03	D41	10/20/2025	Chemtech -SO
Q3408-04	ASPHALT-D	Solid	Percent Solids	Cool 4 deg C	PSEG03	D41	10/20/2025	Chemtech -SO
Q3409-01	EXCAVATION-AREA-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D41	10/20/2025	Chemtech -SO
Q3409-02	EXCAVATION-AREA-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D41	10/20/2025	Chemtech -SO
Q3410-01	WASTE	Solid	Percent Solids	Cool 4 deg C	SCIA01	J11	10/20/2025	Chemtech -SO
Q3410-02	VOC	Solid	Percent Solids	Cool 4 deg C	SCIA01	J11	10/20/2025	Chemtech -SO
Q3410-03	1	Solid	Percent Solids	Cool 4 deg C	SCIA01	J11	10/20/2025	Chemtech -SO
Q3410-04	2	Solid	Percent Solids	Cool 4 deg C	SCIA01	J11	10/20/2025	Chemtech -SO
Q3410-05	3	Solid	Percent Solids	Cool 4 deg C	SCIA01	J11	10/20/2025	Chemtech -SO
Q3410-06	4	Solid	Percent Solids	Cool 4 deg C	SCIA01	J11	10/20/2025	Chemtech -SO
Q3410-07	5	Solid	Percent Solids	Cool 4 deg C	SCIA01	J11	10/20/2025	Chemtech -SO
Q3412-01	TP-6	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3412-02	TP-6-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3412-03	TP-6-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/20/2025	Chemtech -SO
Q3413-01	BP-VPB-184-GW-980-982	Solid	Percent Solids	Cool 4 deg C	TETR06	D31	10/20/2025	Chemtech -SO
Q3414-01	SB-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	D32	10/21/2025	Chemtech -SO
Q3414-02	SB-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	D32	10/21/2025	Chemtech -SO
Q3414-03	SB-3	Solid	Percent Solids	Cool 4 deg C	PSEG03	D32	10/21/2025	Chemtech -SO
Q3414-04	SB-4	Solid	Percent Solids	Cool 4 deg C	PSEG03	D32	10/21/2025	Chemtech -SO

Date/Time

10/21/25 15:00

Raw Sample Received by:

TS WWC

Raw Sample Relinquished by:

OPSN

Date/Time

10/21/25 17:20

Raw Sample Received by:

CP SN

Raw Sample Relinquished by:

TS WWC

WORKLIST(Hardcopy Internal Chain)

W-137592

WorkList Name : %1-102125 WorkList ID : 192565 Department : Wet-Chemistry Date : 10-21-2025 08:08:50

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q3414-05	SB-5	Solid	Percent Solids	Cool 4 deg C	PSEG03	D32	10/21/2025	Chemtech -SO
Q3414-06	SB-6	Solid	Percent Solids	Cool 4 deg C	PSEG03	D32	10/21/2025	Chemtech -SO
Q3414-07	SB-7	Solid	Percent Solids	Cool 4 deg C	PSEG03	D32	10/21/2025	Chemtech -SO
Q3414-08	SB-8	Solid	Percent Solids	Cool 4 deg C	PSEG03	D32	10/21/2025	Chemtech -SO
Q3414-09	SB-9	Solid	Percent Solids	Cool 4 deg C	PSEG03	D32	10/21/2025	Chemtech -SO
Q3414-10	SB-10	Solid	Percent Solids	Cool 4 deg C	PSEG03	D32	10/21/2025	Chemtech -SO
Q3414-11	SB-11	Solid	Percent Solids	Cool 4 deg C	PSEG03	D32	10/21/2025	Chemtech -SO
Q3414-12	SB-12	Solid	Percent Solids	Cool 4 deg C	PSEG03	D32	10/21/2025	Chemtech -SO
Q3414-13	SB-13	Solid	Percent Solids	Cool 4 deg C	PSEG03	D32	10/21/2025	Chemtech -SO
Q3415-01	50841	Solid	Percent Solids	Cool 4 deg C	PSEG03	D41	10/21/2025	Chemtech -SO
Q3415-02	50842	Solid	Percent Solids	Cool 4 deg C	PSEG03	D41	10/21/2025	Chemtech -SO
Q3415-03	50843	Solid	Percent Solids	Cool 4 deg C	PSEG03	D41	10/21/2025	Chemtech -SO
Q3416-01	NB-08-10212025	Solid	Percent Solids	Cool 4 deg C	PSEG05	D31	10/21/2025	Chemtech -SO
Q3416-02	NB-08-10212025-E2	Solid	Percent Solids	Cool 4 deg C	PSEG05	D31	10/21/2025	Chemtech -SO
Q3418-01	101725	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/21/2025	Chemtech -SO
Q3418-02	101725-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/21/2025	Chemtech -SO
Q3418-03	101725-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	10/21/2025	Chemtech -SO

Date/Time 10/21/25 15:00
 Raw Sample Received by: SB wcc
 Raw Sample Relinquished by: cd sm

Date/Time 10/21/25 17:30
 Raw Sample Received by: cd sm
 Raw Sample Relinquished by: SB wcc

Prep Standard - Chemical Standard Summary

Order ID : Q3410

Test : VOC-TCLVOA-10

Prepbatch ID :

Sequence ID/Qc Batch ID: VY102125,

Standard ID :

VP133934,VP134147,VP134149,VP134150,VP134934,VP134957,VP135552,VP135553,VP135834,VP135835,VP135871,VP135872,VP135873,

Chemical ID :

V13391,V14200,V14204,V14205,V14290,V14509,V14510,V14531,V14532,V14625,V14636,V14637,V14638,V14639,V14673,V14727,V14728,V14803,V14815,V14844,V14906,V14921,V14928,V14929,V14951,V14952,V15073,V15074,V15075,W3112,

VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1917	8260 Internal standard 50 ppm	VP133934	05/16/2025	11/12/2025	Semsettin Yesilyurt	None	None	Maresh Dadoda
								05/21/2025

FROM 0.10000ml of V14290 + 49.90000ml of V14921 = Final Quantity: 50.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
252	8260 Working STD (BCM)-First source, 100PPM	VP134147	06/06/2025	12/06/2025	Semsettin Yesilyurt	None	None	Maresh Dadoda
								06/10/2025

FROM 1.00000ml of V14673 + 19.00000ml of V14929 = Final Quantity: 20.000 ml



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1810	8260 Working Std(2-CVE)-800ppm	VP134149	06/06/2025	12/06/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 06/10/2025
<u>FROM</u>	1.00000ml of V14636 + 1.00000ml of V14637 + 1.00000ml of V14638 + 1.00000ml of V14639 + 46.00000ml of V14929 = Final Quantity: 50.000 ml							

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1811	8260 Working Std(2-CVE)-500ppm	VP134150	06/06/2025	12/06/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 06/10/2025
<u>FROM</u> 7.50000ml of V14929 + 12.50000ml of VP134149 = Final Quantity: 20.000 ml								

VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
249	8260 Surrogate, 100PPM	VP134934	07/29/2025	01/29/2026	Semsettin Yesilyurt	None	None	Maresh Dadoda
08/06/2025								

FROM 0.10000ml of V14906 + 24.90000ml of V14625 = Final Quantity: 25.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
218	BFB, 25PPM	VP134957	08/01/2025	11/22/2025	Semsettin Yesilyurt	None	None	Maresh Dadoda
08/06/2025								

FROM 0.50000ml of V13391 + 49.50000ml of V14625 = Final Quantity: 50.000 ml



VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
257	8260 Calibration Working STD Mix-First source, 160PPM	VP135552	09/22/2025	11/03/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 09/26/2025

FROM 0.40000ml of V14844 + 1.00000ml of V14200 + 1.00000ml of V14509 + 1.00000ml of V14510 + 1.00000ml of V14531 + 1.00000ml of V14532 + 1.00000ml of V14727 + 1.00000ml of V14728 + 1.00000ml of V14803 + 1.00000ml of V14815 + 1.00000ml of V14951 + 1.00000ml of V14952 + 1.50000ml of V14204 + 1.50000ml of V14205 + 10.60000ml of V14928 = Final Quantity: 25.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
244	8260 Calibration Working STD Mix-First source, 100PPM	VP135553	09/22/2025	11/03/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 09/26/2025

FROM 5.62500ml of V14928 + 9.37500ml of VP135552 = Final Quantity: 15.000 ml

VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
51	8260 Working STD (Acrolein) -first source, 800PPM	VP135834	10/17/2025	11/16/2025	Semsettin Yesilyurt	None	None	Maresh Dadoda
								10/17/2025

FROM 1.00000ml of V15073 + 1.50000ml of V15074 + 1.50000ml of V15075 + 21.00000ml of V14928 = Final Quantity: 25.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
56	8260 Working STD (Acrolein) -first source, 500PPM	VP135835	10/17/2025	11/16/2025	Semsettin Yesilyurt	None	None	Maresh Dadoda
								10/17/2025

FROM 7.50000ml of V14928 + 12.50000ml of VP135834 = Final Quantity: 20.000 ml

VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
732	BFB TUNE CHECK - SOIL	VP135871	10/21/2025	10/22/2025	Amit Patel	None	None	Maresh Dadoda
								10/21/2025

FROM 4.99800ml of W3112 + 0.00200ml of VP134957 = Final Quantity: 5.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
773	50 PPB CCC, 8260-SOIL	VP135872	10/21/2025	10/22/2025	Amit Patel	None	None	Maresh Dadoda
								10/21/2025

FROM 4.98000ml of W3112 + 0.00250ml of VP134147 + 0.00250ml of VP134150 + 0.00250ml of VP134934 + 0.00250ml of VP135553
+ 0.00250ml of VP135835 + 0.00500ml of VP133934 = Final Quantity: 5.000 ml



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
773	50 PPB CCC, 8260-SOIL	VP135873	10/21/2025	10/22/2025	Amit Patel	None	None	Mahesh Dadoda 10/21/2025
FROM 4.98000ml of W3112 + 0.00250ml of VP134147 + 0.00250ml of VP134150 + 0.00250ml of VP134934 + 0.00250ml of VP135553 + 0.00250ml of VP135835 + 0.00500ml of VP133934 = Final Quantity: 5.000 ml								

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30067 / BFB tuneing solution	A0191805	11/22/2025	11/22/2024 / SAM	01/13/2023 / SAM	V13391

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30006 / VOA Mix, CLP method Calibration Std #1 ketones 5000uq/ml, PTM, 1ml	A0200785	03/22/2026	09/22/2025 / sam	02/28/2024 / SAM	V14200

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30006 / VOA Mix, CLP method Calibration Std #1 ketones 5000uq/ml, PTM, 1ml	A0200785	03/22/2026	09/22/2025 / sam	02/28/2024 / SAM	V14204

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30006 / VOA Mix, CLP method Calibration Std #1 ketones 5000uq/ml, PTM, 1ml	A0200785	03/22/2026	09/22/2025 / sam	02/28/2024 / SAM	V14205

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	555581 / Custom Standard, 8260 Internal Std [CS 5179-1]	A0210184	12/12/2025	12/12/2024 / SAM	04/15/2024 / SAM	V14290

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	95317 / Universal VOA Mega Mix (Min order = 5)	021624	03/22/2026	09/22/2025 / sam	09/17/2024 / SAM	V14509

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	95317 / Universal VOA Mega Mix (Min order = 5)	021624	03/22/2026	09/22/2025 / sam	09/17/2024 / SAM	V14510

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	95319 / Revised Additions Mix (Min = 5)	091724	03/22/2026	09/22/2025 / sam	09/18/2024 / SAM	V14531

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	95319 / Revised Additions Mix (Min = 5)	091724	03/22/2026	09/22/2025 / sam	09/18/2024 / SAM	V14532

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	2310762004	01/29/2026	07/29/2025 / SAM	11/26/2024 / SAM	V14625

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ 2-Chloroethyl vinyl ether	120524	12/06/2025	06/06/2025 / SAM	12/06/2024 / SAM	V14636

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ 2-Chloroethyl vinyl ether	120524	12/06/2025	06/06/2025 / SAM	12/06/2024 / SAM	V14637

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ 2-Chloroethyl vinyl ether	120524	12/06/2025	06/06/2025 / SAM	12/06/2024 / SAM	V14638

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ 2-Chloroethyl vinyl ether	120524	12/06/2025	06/06/2025 / SAM	12/06/2024 / SAM	V14639

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30225 / VOA Mix, bromochloromethane, 2000ug/mL, P&TM, 1mL/ampul	A0214960	12/06/2025	06/06/2025 / SAM	12/09/2024 / SAM	V14673

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30042 / VOA Mix,500 series method 502.2 Calibration Std #1 gases, 2000uq/ml, PTM, 1ml	A0216826	03/22/2026	09/22/2025 / sam	12/17/2024 / SAM	V14727

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30042 / VOA Mix,500 series method 502.2 Calibration Std #1 gases, 2000uq/ml, PTM, 1ml	A0216826	03/22/2026	09/22/2025 / sam	12/17/2024 / SAM	V14728

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	555408 / Custom Standard, Vinyl Acetate Standard w/ Grav [CS 5066-6] TWO SEPARATE	A0220471	03/22/2026	09/22/2025 / sam	01/08/2025 / SAM	V14803

LOTS

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	555408 / Custom Standard, Vinyl Acetate Standard w/ Grav [CS 5066-6] TWO SEPARATE	A0220471	03/22/2026	09/22/2025 / sam	01/08/2025 / SAM	V14815

LOTS

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30470 / VOA Stock Solution, tert-butanol std, 1mL, P&TM	A0217535	03/22/2026	09/22/2025 / sam	01/21/2025 / SAM	V14844

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	555582 / Custom Mixture, 8260 A/B Surrogate Mix [CS 5179-2]	A0223904	07/29/2026	07/29/2025 / SAM	03/24/2025 / SAM	V14906

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	24G0262002	11/12/2025	05/12/2025 / SAM	05/09/2025 / SAM	V14921

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	24G0262002	03/22/2026	09/22/2025 / sam	05/09/2025 / SAM	V14928

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	24G0262002	12/06/2025	06/06/2025 / SAM	05/09/2025 / SAM	V14929

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30489 / VOA Mix, 8260B Acetates Mix, P&TM, 1mL	A0222076	03/22/2026	09/22/2025 / sam	05/19/2025 / SAM	V14951

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30489 / VOA Mix, 8260B Acetates Mix, P&TM, 1mL	A0222076	03/22/2026	09/22/2025 / sam	05/19/2025 / SAM	V14952

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	91980 / Acrolin Std (Min = 5)	101625	11/16/2025	10/17/2025 / sam	10/17/2025 / sam	V15073

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	91980 / Acrolin Std (Min = 5)	101625	11/16/2025	10/17/2025 / sam	10/17/2025 / sam	V15074

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	91980 / Acrolin Std (Min = 5)	101625	11/16/2025	10/17/2025 / sam	10/17/2025 / sam	V15075

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / lwona	07/03/2024 / lwona	W3112

Methanol
ULTRA RESI-ANALYZED
For Purge and Trap Analysis



Material No.: 9077-02
Batch No.: 23I0762004
Manufactured Date: 2023-08-11
Expiration Date: 2026-08-10
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay (CH ₃ OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.5 ppm
Titration Acid (μeq/g)	≤ 0.3	0.2
Titration Base (μeq/g)	≤ 0.10	0.01
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis – Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use
Performance Tested for Use in EPA Methods
500 Series for Drinking Water
600 Series for Wastewater
846 for Solid Waste

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Ken Koehnlein
Sr. Manager, Quality Assurance



Ree 03117/24

CERTIFIED WEIGHT REPORT

Part Number: 95317

Lot Number: 021624

Description: Universal VOA Megamix

69 components

Expiration Date: 021627

Recommended Storage: Freezer (0 °C)

Nominal Concentration (µg/mL): 2000

NIST Test ID#: BUTB

Solvent(s): Lot#
Methanol EG359-USQ12Weight(s) shown below were combined and diluted to (mL): 100.0 0.021 Balance Uncertainty
Flask Uncertainty


Formulated By:	Prashant Chauhan	021624
Reviewed By:	Pedro L. Renteria	021624

Compound	(K049)	Lot	Dir.	Initial	Initial	Nominal	Purity	Purity	Uncertainty	Target	Actual	Actual	Expanded	SDS Information				
	Part Number	Number	Factor	Vol. (mL)	Conc.(µg/mL)	Conc (µg/mL)	(%)	Uncertainty	Pipette (mL)	Weight(g)	Weight(g)	Conc (µg/mL)	Uncertainty	(+/-) (µg/mL)	(Solvent Safety Info. On Attached pg.)	CASE	OSHA PEL (TWA)	LD50
1. Acetonitrile	0324	021644	NA	NA	NA	2000	99.99	0.2	NA	0.20007	0.20020	2001.3	8.1	75-05-8	40 ppm (70mg/m3/8H)			or-rat 2450mg/kg
2. Allyl chloride (3-Chloropropene)	0325	102366	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20221	2001.4	8.2	107-05-1	1 ppm (3mg/m3/8H)			or-rat 700mg/kg
3. Carbon disulfide	0060	MKCR8561	NA	NA	NA	2000	99.99	0.2	NA	0.20007	0.20023	2001.6	8.1	75-15-0	4 ppm (12mg/m3) (skin)			or-rat 1200mg/kg
4. cis-1,4-Dichloro-2-butene	1196	14718EF	NA	NA	NA	2000	95	0.2	NA	0.21056	0.21069	2001.1	8.5	1478-11-5	NA			N/A
5. trans-1,4-Dichloro-2-butene	0486	MKBP6041V	NA	NA	NA	2000	96.5	0.2	NA	0.20731	0.20746	2001.7	8.4	110-57-6	NA			N/A
6. Diethyl ether	0153	IK18CAS000C	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20040	2001.5	8.1	60-29-7	NA			N/A
7. Ethyl methacrylate	0381	06126PX	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20230	2002.3	8.2	97-63-2	NA			or-rat 14800mg/kg
8. Iodomethane	0489	SHBF8718V	NA	NA	NA	2000	99.5	0.2	NA	0.20106	0.20121	2001.5	8.2	74-88-4	5 ppm(28mg/m3/8H)(skin)			or-rat 76mg/kg
9. 2-Methyl-1-propanol	0445	15241EB	NA	NA	NA	2000	99.5	0.2	NA	0.20106	0.20120	2001.4	8.1	78-83-1	50 ppm (150mg/m3/8H)			or-rat 2460mg/kg
10. Methacrylonitrile	0442	00427ET	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20221	2001.4	8.2	128-98-7	1 ppm (3mg/m3/8H)(skin)			or-rat 120mg/kg
11. Methyl acrylate	1075	SHBK0679	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20040	2001.5	8.1	96-33-3	10 ppm(35mg/m3/8H)(skin)			or-rat 277mg/kg
12. Methyl methacrylate	0404	MKGW6137V	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20041	2001.6	8.1	80-62-6	100 ppm (410mg/m3/8H)			or-rat 7872mg/kg
13. Nitrobenzene	0228	01213TV	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20220	2001.3	8.2	98-95-3	1 ppm (5mg/m3/8H)(skin)			or-rat 780mg/kg
14. 2-Nitropropane	0461	14002JX	NA	NA	NA	2000	97.3	0.2	NA	0.20560	0.20577	2001.6	8.3	78-46-9	10 ppm (30mg/m3/8H)			or-rat 720mg/kg
15. Perchloroethane	0460	HGA01	NA	NA	NA	2000	98	0.2	NA	0.20413	0.20430	2001.6	8.3	78-01-7	NA			N/A
16. 1,1,2-Trichlorotrifluoroethane	0474	18930	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20225	2001.8	8.2	76-13-1	1000 ppm (7600mg/m3/8H)			or-rat 43g/kg
17. Bromodichloromethane	35171	101623	0.05	5.00	40001.7	2000	NA	NA	0.017	NA	NA	1999.6	22.9	75-27-4	NA			or-rat 915mg/kg
18. Dibromochloromethane	35171	101623	0.05	5.00	40002.1	2000	NA	NA	0.017	NA	NA	1999.6	23.0	124-48-1	NA			or-rat 848mg/kg
19. cis-1,2-Dichloroethene	35171	101623	0.05	5.00	40003.1	2000	NA	NA	0.017	NA	NA	1999.7	22.9	156-59-2	NA			N/A
20. trans-1,2-Dichloroethene	35171	101623	0.05	5.00	40002.4	2000	NA	NA	0.017	NA	NA	1999.6	23.0	156-60-5	NA			N/A
21. Methylene chloride	35171	101623	0.05	5.00	40002.8	2000	NA	NA	0.017	NA	NA	1999.6	22.9	75-09-2	500 ppm			or-rat 1235mg/kg
22. 1,1-Dichloroethane	32251	102023	0.10	10.00	20001.6	2000	NA	NA	0.042	NA	NA	1999.7	20.4	75-35-4	1 ppm (4mg/m3/8H)			or-rat 820mg/kg
23. Bromoform	95321	020724	0.10	10.00	20003.2	2000	NA	NA	0.042	NA	NA	1999.8	20.5	75-25-2	0.5 ppm (5mg/m3) (skin)			or-rat 200mg/kg
24. Carbon tetrachloride	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.4	56-23-5	2 ppm (12.6mg/m3/8H)			or-rat 933mg/kg
25. Chloroform	95321	020724	0.10	10.00	20004.0	2000	NA	NA	0.042	NA	NA	1999.8	20.5	67-68-3	60 ppm (240mg/m3) (CL)			or-rat 2350mg/kg
26. Dibromomethane	95321	020724	0.10	10.00	20002.9	2000	NA	NA	0.042	NA	NA	1999.8	20.5	74-95-3	NA			or-rat 908mg/kg
27. 1,1-Dichloroethane	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.5	74-95-3	NA			or-rat 106mg/kg
28. 2,2-Dichloropropane	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.5	75-34-3	100 ppm			or-rat 725mg/kg
29. Trichloroethene	95321	020724	0.10	10.00	20201.1	2000	NA	NA	0.042	NA	NA	1999.8	20.4	594-20-7	NA			N/A
30. 1,1,1-Trichloroethane	95321	020724	0.10	10.00	20003.0	2000	NA	NA	0.042	NA	NA	2019.8	20.8	127-18-4	25 ppm (170mg/m3/8H)(final)			or-rat 2629mg/kg
31. 1,2-Dibromo-3-chloropropane	35161	112322	0.05	5.00	40018.5	2000	NA	NA	0.017	NA	NA	1999.8	20.5	71-55-6	350 ppm (1900mg/m3/8H)			or-rat 10300mg/kg
32. 1,2-Dibromoethane	35161	112322	0.05	5.00	40024.8	2000	NA	NA	0.017	NA	NA	2000.3	22.9	96-12-8	0.001 ppm			or-rat 170mg/kg
33. 1,2-Dichloroethane	35161	112322	0.05	5.00	40018.0	2000	NA	NA	0.017	NA	NA	2000.7	22.9	106-93-4	20 ppm (8H)			or-rat 108mg/kg
34. 1,2-Dichloropropane	35161	112322	0.05	5.00	40051.0	2000	NA	NA	0.017	NA	NA	2000.4	22.9	107-06-2	50 ppm (8H)			or-rat 670mg/kg
35. 1,3-Dichloropropane	35161	112322	0.05	5.00	40005.9	2000	NA	NA	0.017	NA	NA	2002.0	22.9	78-87-5	75 ppm (350mg/m3/8H)			or-rat 1947mg/kg
36. 1,1-Dichloropropene	35161	112322	0.05	5.00	40012.1	2000	NA	NA	0.017	NA	NA	1999.8	22.9	142-28-9	NA			or-rat 3600mg/kg
37. cis-1,3-Dichloropropene	35161	112322	0.05	5.00	40010.0	2000	NA	NA	0.017	NA	NA	2000.1	28.7	563-58-6	NA			N/A
38. trans-1,3-Dichloropropene	35161	112322	0.05	5.00	40017.6	2000	NA	NA	0.017	NA	NA	2000.0	23.0	10061-01-5	NA			N/A
39. Hexachloro-1,3-butadiene	35161	112322	0.05	5.00	40017.6	2000	NA	NA	0.017	NA	NA	2000.4	23.0	10061-02-6	NA			N/A
40. 1,1,1,2-Tetrachloroethane	35161	112322	0.05	5.00	40011.9	2000	NA	NA	0.017	NA	NA	2000.6	29.7	87-68-3	0.02 ppm (0.24mg/m3/8H)			or-rat 82mg/kg
41. 1,1,2,2-Tetrachloroethane	35161	112322	0.05	5.00	40007.5	2000	NA	NA	0.017	NA	NA	2000.1	22.9	830-20-6	NA			or-rat 670mg/kg
42. 1,1,2-Trichloroethane	35161	112322	0.05	5.00	40007.5	2000	NA	NA	0.017	NA	NA	1999.9	22.9	79-34-5	5 ppm (35mg/m3/8H)(skin)			or-rat 800mg/kg
43. Trichloroethene	35161	112322	0.05	5.00	40006.6	2000	NA	NA	0.017	NA	NA	1999.8	23.0	79-00-5	10 ppm (45mg/m3/8H)(skin)			or-rat 936mg/kg
44. 1,2,3-Trichloropropane	35161	112322	0.05	5.00	40029.0	2000	NA	NA	0.017	NA	NA	2000.9	22.9	79-01-6	50 ppm (270mg/m3/8H)			or-rat 3402mg/kg
45. Benzene	35162	050823	0.05	5.00	40006.0	2000	NA	NA	0.017	NA	NA	1999.9	22.9	96-18-4	10 ppm (60mg/m3/8H)			or-rat 149.8mg/kg
46. Bromobenzene	35162	050823	0.05	5.00	40006.9	2000	NA	NA	0.017	NA	NA	1999.7	22.9	71-43-2	1 ppm			or-rat 4894mg/kg
47. n-Butyl benzene	35162	050823	0.05	5.00	40003.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-86-1	NA			or-rat 2699mg/kg
48. Ethyl benzene	35162	050823	0.05	5.00	40004.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	104-51-8	NA			N/A
49. p-Isopropyl toluene	35162	050823	0.05	5.00	40004.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	100-41-4	100 ppm (435mg/m3/8H)			or-rat >2000mg/kg
50. Naphthalene	35162	050823	0.05	5.00	40005.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	99-87-6	NA			or-rat 4750mg/kg
51. Styrene	35162	050823	0.05	5.00	40004.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	91-20-3	10 ppm (50mg/m3/8H)			or-rat 490mg/kg
52. Toluene	35162	050823	0.05	5.00	40006.2	2000	NA	NA	0.017	NA	NA	1999.7	22.9	100-42-5	100 ppm			or-rat 5000mg/kg
53. 1,2,3-Trichlorobenzene	35162	050823	0.05	5.00	40003.1	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-88-3	200 ppm			or-rat 5000mg/kg
54. 1,2,4-Trichlorobenzene	35162	050823	0.05	5.00	40001.6	2000	NA	NA	0.017	NA	NA	1999.7	22.9	87-61-6	NA			or-rat 1390mg/kg
55. 1,2,4-Trimethylbenzene	35162	050823	0.05	5.00	40001.6	2000	NA	NA	0.017	NA	NA	1999.8	22.9	120-82-1	5 ppm (CL) (40mg/m3)			or-rat 756mg/kg
56. 1,3,5-Trimethylbenzene	35162	050823	0.05	5.00	40006.7	2000	NA	NA	0.017	NA	NA	1999.6	23.0	95-63-6	NA			or-rat 5g/kg
57. m-Xylene	35162	050823	0.05	5.00	40005.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-87-8	NA			or-rat 5000mg/kg
58. tert-Butyl benzene	35163	101923	0.05	5.00	40001.2	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-38-3	100 ppm (435mg/m3/8H)			or-rat 5g/kg
59. sec-Butyl benzene	35163	101923	0.05	5.00	40002.4	2000	NA	NA	0.017	NA	NA	1999.8	22.9	98-06-6	NA			N/A
60. Chlorobenzene	35163	101923	0.05	5.00	40003.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	135-98-8	NA			or-rat 2240mg/kg
61. 2-Chlorotoluene	35163	101923	0.05	5.00	40003.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	108-90-7	75 ppm (350mg/m3/8H)			or-rat 2290mg/kg
62. 4-Chlorotoluene	35163	101923	0.05	5.00	40003.3													

Run 16, "P95317 L021624 (2000µg/mL in MeOH)"

Run Length: 60.00 min, 35998 points at 10 points/second.
Created: Sat, Feb 17, 2024 at 8:56:46 AM.
Sampled: Sequence "021624-GC5M1", Method "GC5-M1".
Analyzed using Method "GC5-M1".

Comments
GC5-M1 Analysis by Candice Warren
Column ID SPB-Vocol 105 meter X 0.53mm X 3.0µm film thickness
Flow rates: Total flow=290mL/min., Helium (carrier)=10mL/min.,
Helium(make-up)=10mL/min., Hydrogen(make-up)=40mL/min., Air(make-up)=230mL/min.
Oven Profile: Temp. 1=35°C (Time 1=10 min.), Temp 2=200°C (Time 2=8.75 min.),
Rate = 4°C/min., Total run time=60 min. Injector temp.=200°C, FID Temp.=200°C.
FID Signal = Edaq Channel 1
Standard injection = 0.5µL, Range=3

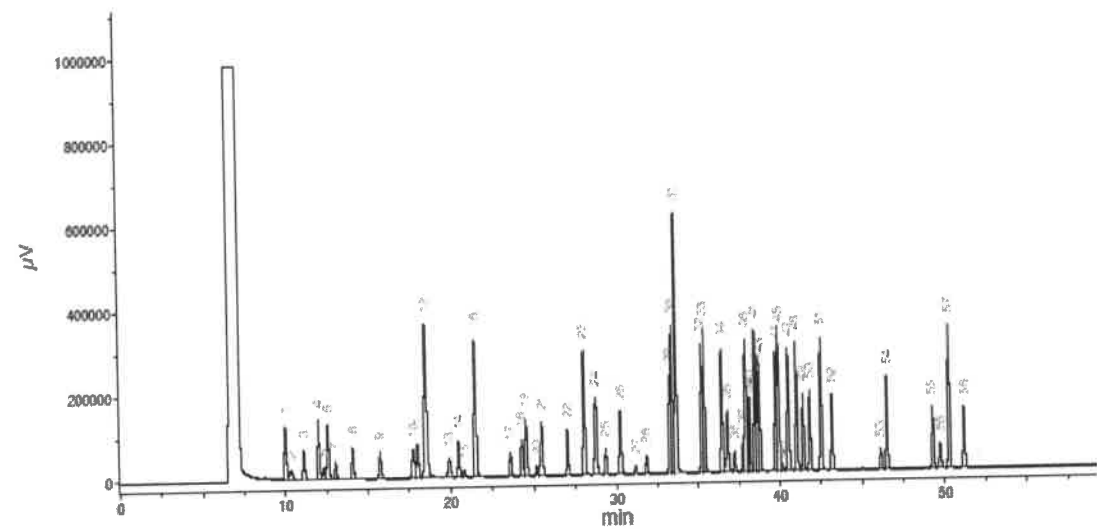

Peak #	Name	FID RT (min.)
1	Ether	9.97
2	1,1,2-Trichloro-1,2,2-trifluoroethane	10.53
3	1,1,1-Trichloroethane	11.10
4	Acetonitrile	12.60
5	Iodomethane	12.91
6	Allyl chloride	13.56
7	Carbon disulfide/Methylene chloride	13.94
8	trans-1,2-Dichloroethene	14.07
9	1,1-Dichloroethane	15.74
10	2,2-Dichloropropane	17.74
11	cis-1,2-Dichloroethene	18.00
12	Methoxyvinylbenzene/Methyl acrylate/Chloroform	18.49
13	Isobutene/1,1,1-Trichloroethane	18.91
14	1,1-Dichloropropane	20.46
15	Carbon tetrachloride	20.79
16	Benzene/1,2-Dichloroethane	21.48
17	Trichloroethene	23.88
18	1,2-Dichloropropane	24.52
19	Methyl methacrylate	25.13
20	Bromochloropropane	25.46
21	Dibromomethane/2-Pentene	27.07
22	cis-1,2-Dichloroethene	28.03
23	Toluene	28.73
24	Ethyl methacrylate/Trans-1,2-Dichloroethene	29.34
25	1,1,2-Trichloroethane	30.34
26	Tetrachloroethane/1,2-Dichloropropane	31.16
27	Dibromochloromethane	31.84
28	1,2-Dibromomethane	33.06
29	Chlorobenzene	33.40
30	Ethylbenzene/1,1,1,2-Tetrachloroethane	33.85
31	m-Xylene/p-Xylene	35.33
32	o-Xylene	35.70
33	Styrene	35.70
34	Isopropylbenzene/Bromofarm	36.48
35	cis-1,4-Dichloro-3-butene	36.80
36	1,1,2-Trichloropropane	37.23
37	n-Propylbenzene	37.77
38	trans-1,4-Dichloro-3-butene	37.92
39	Bromobenzene	38.05
40	1,3,5-Trimethylbenzene	38.14
41	2-Chlorobenzene	38.50
42	4-Chlorobenzene	38.63
43	tert-Butylbenzene	38.77
44	sec-Butylbenzene	39.76
45	1,2,4-Trimethylbenzene	40.17
46	1,2,4-Trimethylbenzene	40.52
47	p-Isopropylbenzene	41.02
48	1,3-Trichlorobenzene	41.42
49	1,4-Dichlorobenzene	41.83
50	n-Butylbenzene	42.52
51	1,2-Dichlorobenzene	42.18
52	1,2-Dichloropropane	46.12
53	1,2-Dichloro-3-methylpropane	46.40
54	Nitrobenzene	49.26
55	1,2,4-Trichlorobenzene	49.72
56	Hexachlorocyclopentadiene	50.56
57	Naphthalene	51.16
58	1,2,3-Trichlorobenzene	

Safety Data Sheet (SDS)

GHS/OSHA Compliant

Section I Product and Company Identification

IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr. Hamden CT, 06514	Emergency Telephone International	1-352-323-3500
		Date Prepared/Revised	January 1, 2024

Section II - Hazards Identification

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H225
H370
P271
P302,332

Highly Flammable Liquid and Vapor
Cause damage to organs
Use in ventilated area
If on skin, wash with soap and water

H301, 311, 331
H351
P280
P305,351,338

Toxic if swallowed, skin contact, inhaled
Suspected of causing cancer
Use gloves, eye protection/face shield
If in eyes, remove contacts, rinse with water



Signal Word: DANGER

Section III - Composition

Components (Specific Chemical Identity; Common Name(s))		
Methanol	METHYL ALCOHOL	CAS#: 67-56-1
		% (optional) > 97

See Certified Weight Report For Other Analytes Present At Trace Quantities.

INTENDED USE: REFERENCE MATERIAL

Section IV. FIRST AID MEASURES

General advice	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact	Wash with soap and water. Consult a physician.
In case of eye contact	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Flammability	Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.
Suitable extinguishing media	Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire	Wear self contained breathing apparatus for fire fighting if necessary.

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up	Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist.
Storage Conditions	Use ventilation. Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge. Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methanol	67-56-1 TWA 200 ppm
Skin notation	TWA 200 ppm
Potential for skin absorption, ingestion and inhalation.	
Personal protective equipment	Respiratory protection Handle with gloves. Gloves must be inspected prior to use. Eye protection.
Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.	

Section IX - Physical/Chemical Characteristics

Boiling Point	65°C	Specific Gravity (H ₂ O = 1)	0.79
Vapor Pressure (mm Hg)	96	Melting Point	-98°C
Vapor Density (AIR = 1)	1.11	Evaporation rate (Butyl Acetate = 1)	4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

Section X. STABILITY AND REACTIVITY

Chemical stability	Stable under recommended storage conditions.
Possibility of hazardous reactions	Vapours may form explosive mixture with air.
Conditions to avoid	Heat, flames, sparks, extreme temperature and sunlight.
Materials to avoid	Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids
Hazardous decomposition products formed under fire conditions.	- Carbon oxides

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - rat - 5,628 mg/kg
LC50 Inhalation - rat - 4 h - 64000 ppm
LD50 Dermal - rabbit - 15,800 mg/kg
Toxic if absorbed through skin. Causes skin irritation.
Eye damage/eye irritation
Toxic if inhaled. Causes respiratory tract irritation.
Toxic if swallowed.

Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.

LC50 15,400 mg/l - 96 h
EC50 24,500.00 mg/l - 48 h
EC100 10,000.00 mg/l - 24 h

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US)
UN number: 1230 Class: 3 Packing group: II
Proper shipping name: Methanol

IATA
UN number: 1230 Class: 3 Packing group: II
Proper shipping name: Methanol

Section XV. REGULATORY INFORMATION

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant
SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



Ree 03117/24

CERTIFIED WEIGHT REPORT

Part Number: 95317

Lot Number: 021624

Description: Universal VOA Megamix

69 components

Expiration Date: 021627

Recommended Storage: Freezer (0 °C)

Nominal Concentration (µg/mL): 2000

NIST Test ID#: BUTB

Solvent(s): Lot#
Methanol EG359-USQ12Weight(s) shown below were combined and diluted to (mL): 100.0 0.021 Balance Uncertainty
Flask Uncertainty

Formulated By:	Prashant Chauhan	021624
Reviewed By:	Pedro L. Renteria	021624
DATE		

Compound	(KME)	Lot	DIL	Initial Vol. (mL)	Initial Conc. (µg/mL)	Nominal Conc. (µg/mL)	Purity (%)	Purity Uncertainty	Uncertainty Pipette (mL)	Target Weight(g)	Actual Weight(g)	Actual Conc. (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information		
														(Solvent Safety Info. On Attached pg.)		
														Part Number	Number	Factor
1. Acetonitrile	(0324)	021644	NA	NA	NA	2000	99.99	0.2	NA	0.20007	0.20020	2001.3	8.1	75-05-8	40 ppm (70mg/m3/8H)	or-rat 2450mg/kg
2. Allyl chloride (3-Chloropropene)	(0325)	102396	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20221	2001.4	8.2	107-05-1	1 ppm (3mg/m3/8H)	or-rat 700mg/kg
3. Carbon disulfide	(0060)	MKCR8561	NA	NA	NA	2000	99.99	0.2	NA	0.20007	0.20023	2001.6	8.1	75-15-0	4 ppm (12mg/m3) (skin)	or-rat 1200mg/kg
4. cis-1,4-Dichloro-2-butene	(1196)	14718EF	NA	NA	NA	2000	95	0.2	NA	0.21056	0.21069	2001.1	8.5	1478-11-5	N/A	N/A
5. trans-1,4-Dichloro-2-butene	(0486)	MKBP6041V	NA	NA	NA	2000	96.5	0.2	NA	0.20731	0.20746	2001.7	8.4	110-57-6	N/A	N/A
6. Diethyl ether	(0153)	IK18CAS000C	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20040	2001.5	8.1	60-29-7	N/A	N/A
7. Ethyl methacrylate	(0381)	06128PX	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20230	2002.3	8.2	97-63-2	N/A	or-rat 14800mg/kg
8. Iodomethane	(0489)	SHBF8718V	NA	NA	NA	2000	99.5	0.2	NA	0.20106	0.20121	2001.5	8.2	74-88-4	5 ppm(28mg/m3/8H)(skin)	or-rat 75mg/kg
9. 2-Methyl-1-propanol	(0445)	15241EB	NA	NA	NA	2000	99.5	0.2	NA	0.20106	0.20120	2001.4	8.1	78-83-1	50 ppm (150mg/m3/8H)	or-rat 2460mg/kg
10. Methacrylonitrile	(0442)	00427ET	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20221	2001.4	8.2	128-98-7	1 ppm (3mg/m3/8H)(skin)	or-rat 120mg/kg
11. Methyl acrylate	(1075)	SHBK0679	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20040	2001.5	8.1	96-33-3	10 ppm(35mg/m3/8H)(skin)	or-rat 277mg/kg
12. Methyl methacrylate	(0404)	MKGW6137V	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20041	2001.6	8.1	80-62-6	100 ppm (410mg/m3/8H)	or-rat 7872mg/kg
13. Nitrobenzene	(0228)	01213TV	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20220	2001.3	8.2	98-95-3	1 ppm (5mg/m3/8H)(skin)	or-rat 780mg/kg
14. 2-Nitropropane	(0461)	14002JX	NA	NA	NA	2000	97.3	0.2	NA	0.20560	0.20577	2001.6	8.3	78-46-9	10 ppm (35mg/m3/8H)	or-rat 720mg/kg
15. Perchloroethane	(0460)	HGA01	NA	NA	NA	2000	98	0.2	NA	0.20413	0.20430	2001.6	8.3	78-01-7	N/A	N/A
16. 1,1,2-Trichlorotrifluoroethane	(0474)	18930	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20225	2001.8	8.2	76-13-1	1000 ppm (7600mg/m3/8H)	or-rat 435g/kg
17. Bromodichloromethane	35171	101623	0.05	5.00	40001.7	2000	NA	NA	0.017	NA	NA	1999.6	22.9	75-27-4	N/A	or-rat 915mg/kg
18. Dibromochloromethane	35171	101623	0.05	5.00	40002.1	2000	NA	NA	0.017	NA	NA	1999.6	23.0	124-48-1	N/A	or-rat 848mg/kg
19. cis-1,2-Dichloroethene	35171	101623	0.05	5.00	40003.1	2000	NA	NA	0.017	NA	NA	1999.7	22.9	156-59-2	N/A	N/A
20. trans-1,2-Dichloroethene	35171	101623	0.05	5.00	40003.2	2000	NA	NA	0.017	NA	NA	1999.6	23.0	156-60-5	N/A	or-rat 1235mg/kg
21. Methylene chloride	35171	101623	0.05	5.00	40002.8	2000	NA	NA	0.017	NA	NA	1999.6	22.9	75-09-2	500 ppm	or-rat 820mg/kg
22. 1,1-Dichloroethane	32261	102023	0.10	10.00	20001.6	2000	NA	NA	0.042	NA	NA	1999.7	20.4	75-35-4	1 ppm (4mg/m3/8H)	or-rat 200mg/kg
23. Bromoform	95321	020724	0.10	10.00	20003.2	2000	NA	NA	0.042	NA	NA	1999.8	20.5	75-25-2	0.5 ppm (5mg/m3) (skin)	or-rat 933mg/kg
24. Carbon tetrachloride	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.4	56-23-5	2 ppm (12.6mg/m3/8H)	or-rat 2350mg/kg
25. Chloroform	95321	020724	0.10	10.00	20002.9	2000	NA	NA	0.042	NA	NA	1999.8	20.5	67-68-3	60 ppm (240mg/m3) (CL)	or-rat 908mg/kg
26. Dibromomethane	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.5	74-95-3	N/A	or-rat 108mg/kg
27. 1,1-Dichloroethane	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.4	594-20-7	N/A	N/A
28. 2,2-Dichloropropane	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.4	594-20-7	N/A	N/A
29. Trichloroethene	95321	020724	0.10	10.00	20201.1	2000	NA	NA	0.042	NA	NA	2019.8	20.8	127-18-4	25 ppm (170mg/m3/8H)(final)	or-rat 2629mg/kg
30. 1,1,1-Trichloroethane	95321	020724	0.10	10.00	20003.0	2000	NA	NA	0.042	NA	NA	1999.8	20.5	71-55-6	350 ppm (1900mg/m3/8H)	or-rat 10300mg/kg
31. 1,2-Dibromo-3-chloropropane	35161	112322	0.05	5.00	40018.5	2000	NA	NA	0.017	NA	NA	2000.3	22.9	86-12-8	0.001 ppm	or-rat 170mg/kg
32. 1,2-Dibromoethane	35161	112322	0.05	5.00	40024.8	2000	NA	NA	0.017	NA	NA	2000.7	22.9	106-93-4	20 ppm (8H)	or-rat 108mg/kg
33. 1,2-Dichloroethane	35161	112322	0.05	5.00	40018.0	2000	NA	NA	0.017	NA	NA	2000.4	22.9	107-06-2	50 ppm (8H)	or-rat 670mg/kg
34. 1,2-Dichloropropane	35161	112322	0.05	5.00	40051.0	2000	NA	NA	0.017	NA	NA	2002.0	22.9	78-87-5	75 ppm (350mg/m3/8H)	or-rat 1947mg/kg
35. 1,3-Dichloropropane	35161	112322	0.05	5.00	40005.9	2000	NA	NA	0.017	NA	NA	1999.8	22.9	142-28-9	N/A	or-rat 3600mg/kg
36. 1,1-Dichloropropene	35161	112322	0.05	5.00	40012.1	2000	NA	NA	0.017	NA	NA	2000.1	28.7	563-58-6	N/A	N/A
37. cis-1,3-Dichloropropene	35161	112322	0.05	5.00	40010.0	2000	NA	NA	0.017	NA	NA	2000.0	23.0	10061-01-5	N/A	N/A
38. trans-1,3-Dichloropropene	35161	112322	0.05	5.00	40017.6	2000	NA	NA	0.017	NA	NA	2000.4	23.0	10061-02-6	N/A	N/A
39. Hexachloro-1,3-butadiene	35161	112322	0.05	5.00	40021.9	2000	NA	NA	0.017	NA	NA	2000.6	29.7	87-68-3	0.02 ppm (0.24mg/m3/8H)	or-rat 82mg/kg
40. 1,1,1,2-Tetrachloroethane	35161	112322	0.05	5.00	40011.9	2000	NA	NA	0.017	NA	NA	2000.1	22.9	830-20-6	N/A	or-rat 670mg/kg
41. 1,1,2,2-Tetrachloroethane	35161	112322	0.05	5.00	40007.5	2000	NA	NA	0.017	NA	NA	1999.9	22.9	79-34-5	5 ppm (35mg/m3/8H)(skin)	or-rat 800mg/kg
42. 1,1,2-Trichloroethane	35161	112322	0.05	5.00	40006.6	2000	NA	NA	0.017	NA	NA	1999.8	23.0	79-00-5	10 ppm (45mg/m3/8H)(skin)	or-rat 936mg/kg
43. Trichloroethene	35161	112322	0.05	5.00	40029.0	2000	NA	NA	0.017	NA	NA	2000.9	22.9	79-01-6	50 ppm (270mg/m3/8H)	or-mus 2402mg/kg
44. 1,2,3-Trichloropropane	35161	112322	0.05	5.00	40007.5	2000	NA	NA	0.017	NA	NA	1999.9	22.9	96-18-4	10 ppm (60mg/m3/8H)	or-rat 149.8mg/kg
45. Benzene	35162	050823	0.05	5.00	40006.0	2000	NA	NA	0.017	NA	NA	1999.7	22.9	71-43-2	1 ppm	or-rat 4894mg/kg
46. Bromobenzene	35162	050823	0.05	5.00	40003.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-88-1	N/A	or-rat 2699mg/kg
47. n-Butyl benzene	35162	050823	0.05	5.00	40003.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	104-51-8	N/A	N/A
48. Ethyl benzene	35162	050823	0.05	5.00	40004.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	100-41-4	100 ppm (435mg/m3/8H)	or-rat >2000mg/kg
49. p-Isopropyl toluene	35162	050823	0.05	5.00	40005.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	99-87-6	N/A	or-rat 4750mg/kg
50. Naphthalene	35162	050823	0.05	5.00	40005.2	2000	NA	NA	0.017	NA	NA	1999.8	22.9	91-20-3	10 ppm (50mg/m3/8H)	or-rat 490mg/kg
51. Styrene	35162	050823	0.05	5.00	40004.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	100-42-5	100 ppm	or-rat 5000mg/kg
52. Toluene	35162	050823	0.05	5.00	40008.2	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-88-3	200 ppm	or-rat 5000mg/kg
53. 1,2,3-Trichlorobenzene	35162	050823	0.05	5.00	40003.1	2000	NA	NA	0.017	NA	NA	1999.7	22.9	87-81-6	N/A	or-rat 1390mg/kg
54. 1,2,4-Trichlorobenzene	35162	050823	0.05	5.00	40006.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	120-82-1	5 ppm (CL) (40mg/m3)	or-rat 756mg/kg
55. 1,2,4-Trimethylbenzene	35162	050823	0.05	5.00	40001.8	2000	NA	NA	0.017	NA	NA	1999.8	23.0	95-63-6	N/A	or-rat 5g/kg
56. 1,3,5-Trimethylbenzene	35162	050823	0.05	5.00	40006.7	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-87-8	N/A	or-rat 5000mg/kg
57. m-Xylene	35162	050823	0.05	5.00	40005.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-38-3	100 ppm (435mg/m3/8H)	or-rat 5g/kg
58. tert-Butyl benzene	35163	101923	0.05	5.00	40001.2	2000	NA	NA	0.017	NA	NA	1999.8	22.9	96-06-6	N/A	N/A
59. sec-Butyl benzene	35163	101923	0.05	5.00	40002.4	2000	NA	NA	0.017	NA	NA	1999.8	22.9	135-98-6	N/A	or-rat 2240mg/kg
60. Chlorobenzene	35163	101923	0.05	5.00	40003.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	108-90-7	75 ppm (350mg/m3/8H)	or-rat 2290mg/kg
61. 2-Chlorotoluene	35163	101923	0.05	5.00	40003.3	2000	NA	NA	0.017	NA	NA	1999.5	22.9	95-49-8	50 ppm (250mg/m3/8H)	or-rat 3900mg/kg
62. 4-Chlorotoluene	35163	101923	0.05	5.00	40003.3	2000	NA	NA	0.017	NA	NA	1999.7	22.9	106-43-4	N/A	or-rat 2100mg/kg
63. 1,2-Dichlorobenzene	35163	101923	0.05	5.00	40003.3	2000	NA	NA	0.017	NA	NA	1999.6	23.0	95-50-1	50 ppm (300mg/m3) (CL)	or-rat 500mg/kg
64. 1,3-Dichlorobenzene	35163	101923	0.05	5.00	40001.7	2000	NA	NA	0.017	NA	NA	1999.6	23.0	541-73-1	N/A	or-mus 1060mg/kg
65. 1,4-Dichlorobenzene	35163	101923	0.05	5												




Run 16, "P95317 L021624 (2000µg/mL in MeOH)"

Run Length: 60.00 min, 35998 points at 10 points/second.
Created: Sat, Feb 17, 2024 at 8:56:46 AM.
Sampled: Sequence "021624-GC5M1", Method "GC5-M1".
Analyzed using Method "GC5-M1".

Comments

GC5-M1 Analysis by Candice Warren
Column ID SPB-Vocol 105 meter X 0.53mm X 3.0µm film thickness
Flow rates: Total flow=290mL/min., Helium (carrier)=10mL/min.,
Helium(make-up)=10mL/min., Hydrogen(make-up)=40mL/min., Air(make-up)=230mL/min.
Oven Profile: Temp. 1=35°C (Time 1=10 min.), Temp 2=200°C (Time 2=8.75 min.),
Rate = 4°C/min., Total run time=60 min. Injector temp.=200°C, FID Temp.=200°C.
FID Signal = Edaq Channel 1
Standard injection = 0.5µL, Range=3

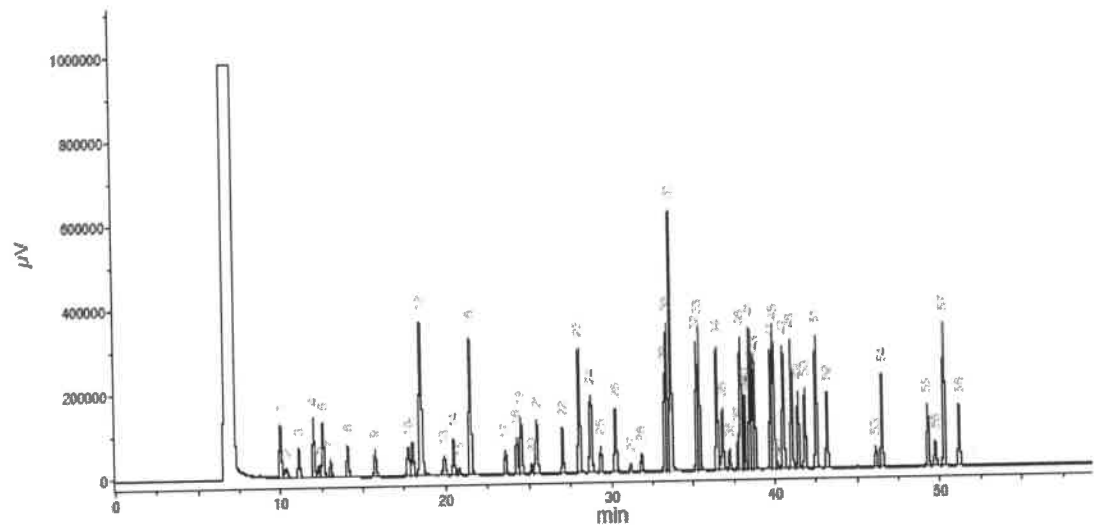

Peak #	Name	FID RT (min.)
1	Ether	9.97
2	1,1,2-Trichloro-1,2,2-trifluoroethane	10.53
3	1,1-Dichloroethane	11.10
4	Acetonitrile	12.60
5	Iodomethane	12.91
6	Allyl chloride	12.96
7	Carbon disulfide/Methylene chloride	13.04
8	trans-1,2-Dichloroethene	14.07
9	1,1-Dichloroethane	15.74
10	2,2-Dichloropropane	17.74
11	cis-1,2-Dichloroethene	18.00
12	Methoxyvinylbenzene/Methyl acrylate/Chloroform	18.49
13	Isobutene/1,1,1-Trichloroethane	18.91
14	1,1-Dichloropropane	20.46
15	Carbon tetrachloride	20.79
16	Benzene/1,2-Dichloroethane	21.48
17	Trichloroethene	23.88
18	1,2-Dichloropropane	24.52
19	Methyl methacrylate	25.13
20	Bromochloropropane	25.46
21	Dibromomethane/2,2-Dichloropropane	27.07
22	cis-1,2-Dichloroethene	28.03
23	Toluene	28.73
24	Ethyl methacrylate/trans-1,2-Dichloroethene	29.34
25	1,1,2-Trichloroethane	30.34
26	Tetrachloroethane/1,2-Dichloropropane	31.16
27	Dibromochloromethane	31.84
28	1,2-Dibromomethane	33.06
29	Chlorobenzene	33.40
30	Ethylbenzene/1,1,1,2-Tetrachloroethane	33.85
31	m-Xylene/p-Xylene	35.33
32	o-Xylene	35.70
33	Styrene	35.70
34	Isopropylbenzene/Bromofarm	36.48
35	cis-1,4-Dichloro-3-butene	36.80
36	1,1,2-Trichloropropane	37.23
37	n-Propylbenzene	37.77
38	trans-1,4-Dichloro-3-butene	37.92
39	Bromobenzene	38.05
40	1,3,5-Trimethylbenzene	38.14
41	1,3,5-Trimethylbenzene	38.50
42	Chlorobenzene	38.63
43	4-Chlorobenzene	38.77
44	tert-Butylbenzene	39.76
45	1,2,4-Trimethylbenzene	39.91
46	Pentachloroethane	40.17
47	sec-Butylbenzene	40.52
48	p-Isopropylbenzene	41.02
49	1,3-Dichlorobenzene	41.42
50	1,4-Dichlorobenzene	41.83
51	n-Butylbenzene	42.52
52	1,2-Dichlorobenzene	42.58
53	1,2-Dibromo-3-chloropropane	46.12
54	Nitrobenzene	46.40
55	1,2,4-Trifluorobenzene	49.26
56	Hexachlorocyclopentadiene	49.72
57	Naphthalene	50.56
58	1,2,3-Trichlorobenzene	51.16

Safety Data Sheet (SDS)

GHS/OSHA Compliant

Section I Product and Company Identification

IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr. Hamden CT, 06514	Emergency Telephone International	1-352-323-3500
		Date Prepared/Revised	January 1, 2024

Section II - Hazards Identification

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H225 H370 P271 P302,332	Highly Flammable Liquid and Vapor Cause damage to organs Use in ventilated area If on skin, wash with soap and water	H301, 311, 331 H351 P280 P305,351,338	Toxic if swallowed, skin contact, inhaled Suspected of causing cancer Use gloves, eye protection/face shield If in eyes, remove contacts, rinse with water
----------------------------------	---	--	---



Signal Word: DANGER

Section III - Composition

Components (Specific Chemical Identity; Common Name(s))	CAS#:	% (optional)
Methanol METHYL ALCOHOL	67-56-1	> 97

See Certified Weight Report For Other Analytes Present At Trace Quantities.

INTENDED USE: REFERENCE MATERIAL

Section IV. FIRST AID MEASURES

General advice	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact	Wash with soap and water. Consult a physician.
In case of eye contact	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Flammability	Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.
Suitable extinguishing media	Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire	Wear self contained breathing apparatus for fire fighting if necessary.

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up	Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist.
Storage Conditions	Use ventilation. Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge. Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methanol	67-56-1 TWA 200 ppm
Skin notation	TWA 200 ppm
Potential for skin absorption	ingestion and inhalation.
Personal protective equipment	Respiratory protection Handle with gloves. Gloves must be inspected prior to use. Eye protection.
Avoid contact with skin, eyes and clothing.	Wash hands thoroughly after handling the product.

Section IX - Physical/Chemical Characteristics

Boiling Point	65°C	Specific Gravity (H ₂ O = 1)	0.79
Vapor Pressure (mm Hg)	96	Melting Point	-98°C
Vapor Density (AIR = 1)	1.11	Evaporation rate (Butyl Acetate = 1)	4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

Section X. STABILITY AND REACTIVITY

Chemical stability	Stable under recommended storage conditions.
Possibility of hazardous reactions	Vapours may form explosive mixture with air.
Conditions to avoid	Heat, flames, sparks, extreme temperature and sunlight.
Materials to avoid	Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids
Hazardous decomposition products formed under fire conditions.	- Carbon oxides

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - rat - 5,628 mg/kg
LC50 Inhalation - rat - 4 h - 64000 ppm
LD50 Dermal - rabbit - 15,800 mg/kg
Toxic if absorbed through skin. Causes skin irritation.
Eye damage/eye irritation
Toxic if inhaled. Causes respiratory tract irritation.
Toxic if swallowed.

Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.

LC50 15,400 mg/l - 96 h
EC50 24,500.00 mg/l - 48 h
EC100 10,000.00 mg/l - 24 h

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US)
UN number: 1230 Class: 3 Packing group: II
Proper shipping name: Methanol

IATA
UN number: 1230 Class: 3 Packing group: II
Proper shipping name: Methanol

Section XV. REGULATORY INFORMATION

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant
SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



Certified Reference Material CRM



Dec 09/17/24

CERTIFIED WEIGHT REPORT

Part Number:
Lot Number:
Description:91980
091424
AcroleinSolvent(s):
WaterLot#
072324QExpiration Date:
Recommended Storage:
Nominal Concentration (µg/mL):
NIST Test ID#:101424
Refrigerate (4 °C)
5000
6UTBWeight(s) shown below were combined and diluted to (mL):
5E-05 Balance Uncertainty
0.001 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA)	LD50
----------	-----	------------	----------------------	------------	-------------	------------------	------------------	---------------------	------------------------------------	--	------	----------------	------

1. Acrolein 5 103755V10F 5000 97 0.5 0.05186 0.05175 5008.9 52.5 107-02-8 0.1 ppm ori-rat 46mg/kg

Method: GC/MSD-1, Detector: Mass Selective Detector (Scan mode). Columns: Vocol (60m X 0.25mm ID X 1.5µm film thickness), Oven Profile: Temp. 1 = 35°C (Time 1 = 0min.), Temp. 2 = 200°C (Time 2 = 8.75 min.), Rate = 4°C/min., Injector Temp. = 200°C, Detector Temp. = 220°C. Analyst: Pedro Rentas, NOTE: Due to the instability of acrolein in solution, all solutions thereof, should be used immediately. Long term storage is not recommended. Please contact our technical department if further information is required.

TIC: [BSB2]79005.D

Scan 232 (8.927 min): [BSB2]79005.D

Abundance

27

250000

8.93

200000

50000

56

150000

40000

30000

20000

50000

10000

37

Time-->

10.00 15.00 20.00 25.00 30.00 35.00 40.00 45.00 50.00 55.00 60.00

m/z-->

0

20 30 40 50 60 70 80 90 100 110 120 130 140 150 160 170

44 65 75 85 119 158 169

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Certified Reference Material CRM



Dec 09/17/24

CERTIFIED WEIGHT REPORT

Part Number:

91980

Lot Number:

091424

Description:

Acrolein

Solvent(s):

Water

Lot#

072324Q

Expiration Date:

101424

Recommended Storage:

Refrigerate (4 °C)

5000

Nominal Concentration (µg/mL):

6UTB

NIST Test ID#:

5E-05

Balance Uncertainty

Weight(s) shown below were combined and diluted to (mL):

10.0

0.001

Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	(Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LD50
----------	-----	------------	----------------------	------------	-------------	------------------	------------------	---------------------	------------------------------------	--	----------------	------

1. Acrolein	5	103755V10F	5000	97	0.5	0.05186	0.05175	5008.9	52.5	107-02-8	0.1 ppm	ori-rat 46mg/kg
-------------	---	------------	------	----	-----	---------	---------	--------	------	----------	---------	-----------------

Method: GC/MSD-1, Detector: Mass Selective Detector (Scan mode). Columns: Vocol (60m X 0.25mm ID X 1.5µm film thickness), Oven Profile: Temp. 1 = 35°C (Time 1 = 0min.), Temp. 2 = 200°C (Time 2 = 8.75 min.), Rate = 4°C/min., Injector Temp. = 200°C, Detector Temp. = 220°C. Analyst: Pedro Rentas, NOTE: Due to the instability of acrolein in solution, all solutions thereof, should be used immediately. Long term storage is not recommended. Please contact our technical department if further information is required.

TIC: [BSB2]79005.D

Scan 232 (8.927 min): [BSB2]79005.D

Abundance

27

250000

8.93

200000

50000

56

150000

40000

30000

20000

50000

10000

37

Time-->

0

10.00 15.00 20.00 25.00 30.00 35.00 40.00 45.00 50.00 55.00 60.00

m/z-->

0

44

65 75 85

119

158 169

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Dec 12/6/24
20 vial

CERTIFIED WEIGHT REPORT

Part Number: 95318
Lot Number: 120524
Description: 2-Chloroethyl vinyl ether

Solvent(s): Lot#
Methanol EJ143-US

Expiration Date: 120527
Recommended Storage: Refrigerate (4 °C)
Nominal Concentration (µg/mL): 10000
NIST Test ID#: 6UTB

✓ 14630 to
✓ 14649


Weight(s) shown below were combined and diluted to (mL):

5E-05 Balance Uncertainty
0.001 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	(Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LD50
----------	-----	------------	----------------------	------------	--------------------	-------------------	-------------------	---------------------	----------------------------------	--	----------------	------

1. 2-Chloroethyl vinyl ether	74	MKCD0033	10000	99	0.2	0.50536	0.50550	10002.9	40.5	110-75-8	N/A	or-rat 250mg/kg
------------------------------	----	----------	-------	----	-----	---------	---------	---------	------	----------	-----	-----------------

Method: GC6MSD-1.M. Detector: MSD. Column: (60m X 0.25mm X 1.5 µm). Oven Profile: Temp 1 = 35°C (Time 1=10min.), Temp 2 = 200°C (Time 2=8.75 min.), Rate = 4°C/min., Injector B Temp = 200°C, Detector B Temp. = 220°C. Analyst: Candice Warren.

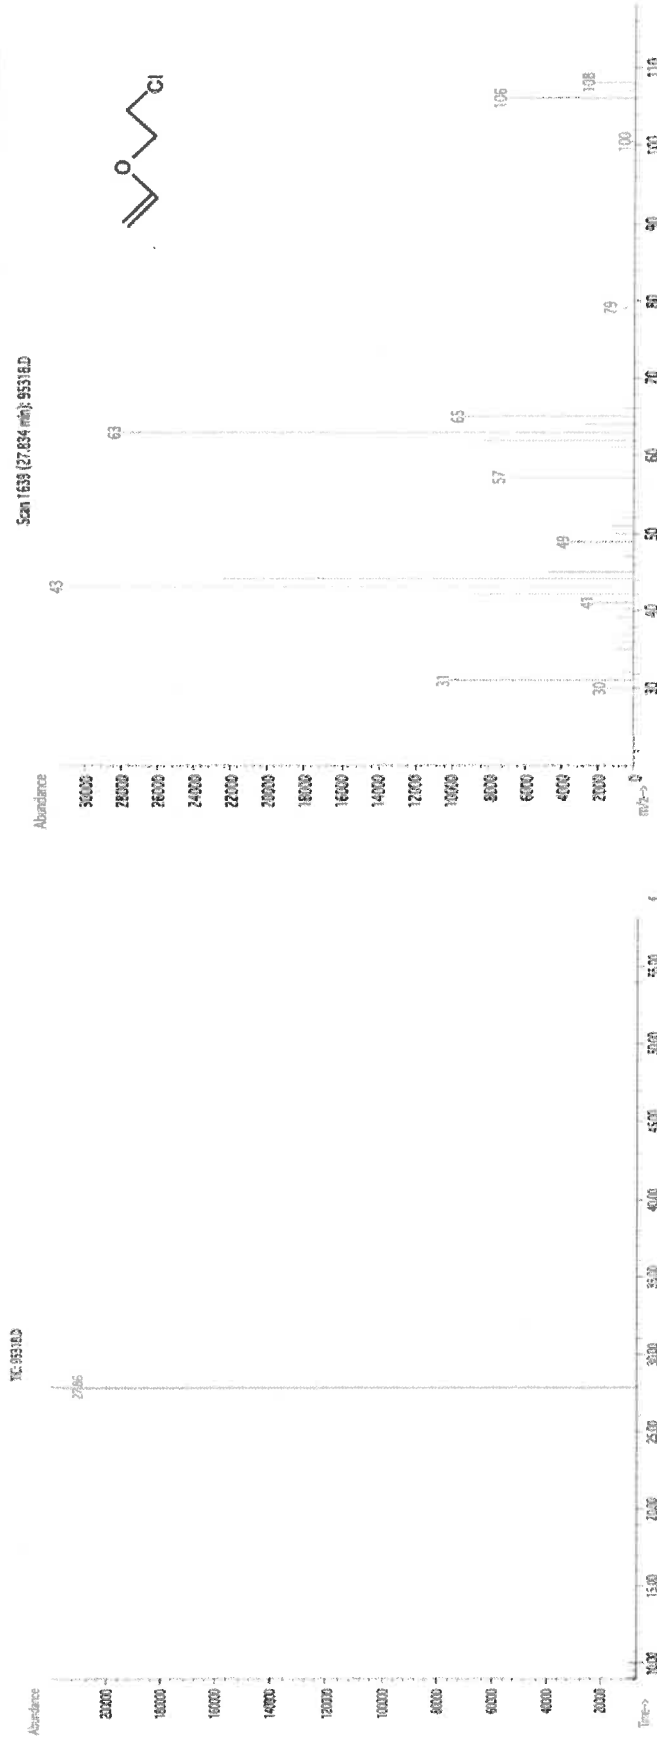

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (±) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Safety Data Sheet (SDS)

GHS/OSHA Compliant

Section I Product and Company Identification

IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr.	Emergency Telephone International	1-352-323-3500
	Hamden CT, 06514	Date Prepared/Revised	January 1, 2024

Section II - Hazards Identification

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H225	Highly Flammable Liquid and Vapor	H301, 311, 331	Toxic if swallowed, skin contact, inhaled
H370	Cause damage to organs	H351	Suspected of causing cancer
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302,332	If on skin, wash with soap and water	P305,351,338	If in eyes, remove contacts, rinse with water



Signal Word: DANGER

Section III - Composition

Components (Specific Chemical Identity; Common Name(s))		% (optional)
Methanol	METHYL ALCOHOL	> 97

See Certified Weight Report For Other Analytes Present At Trace Quantities.

INTENDED USE: REFERENCE MATERIAL

Section IV. FIRST AID MEASURES

General advice	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact	Wash with soap and water. Consult a physician.
In case of eye contact	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Flammability	Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.
Suitable extinguishing media	Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire	Wear self contained breathing apparatus for fire fighting if necessary.

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up	Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation. Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methanol	67-56-1	67-56-1	TWA 200 ppm
Skin notation			TWA 200 ppm
Potential for skin absorption, ingestion and inhalation.			
Personal protective equipment	Respiratory protection	Handle with gloves. Gloves must be inspected prior to use.	Eye protection.
Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.			

Section IX - Physical/Chemical Characteristics

Boiling Point	65°C	Specific Gravity (H ₂ O = 1)	0.79
Vapor Pressure (mm Hg)	96	Melting Point	-98°C
Vapor Density (AIR = 1)	1.11	Evaporation rate (Butyl Acetate = 1)	4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

Section X. STABILITY AND REACTIVITY

Chemical stability	Stable under recommended storage conditions.
Possibility of hazardous reactions	Vapours may form explosive mixture with air.
Conditions to avoid	Heat, flames, sparks, extreme temperature and sunlight.
Materials to avoid	Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids
Hazardous decomposition products formed under fire conditions.	- Carbon oxides

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - rat - 5,628 mg/kg
LC50 Inhalation - rat - 4 h - 64000 ppm
LD50 Dermal - rabbit - 15,800 mg/kg
Toxic if absorbed through skin. Causes skin irritation.
Eye damage/eye irritation
Toxic if inhaled. Causes respiratory tract irritation.
Toxic if swallowed.

Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.

LC50 15,400 mg/l - 96 h
EC50 24,500.00 mg/l - 48 h
EC100 10,000.00 mg/l - 24 h

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US)	IATA
UN number: 1230 Class: 3 Packing group: II	UN number: 1230 Class: 3 Packing group: II
Proper shipping name: Methanol	Proper shipping name: Methanol

Section XV. REGULATORY INFORMATION

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant
SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



Dec 12/6/24
20 vial

CERTIFIED WEIGHT REPORT

Part Number: 95318
Lot Number: 120524
Description: 2-Chloroethyl vinyl ether

Solvent(s): Lot#
Methanol EJ143-US

Expiration Date: 120527
Recommended Storage: Refrigerate (4 °C)
Nominal Concentration (µg/mL): 10000
NIST Test ID#: 6UTB

✓ 14630 to
✓ 14649


Weight(s) shown below were combined and diluted to (mL):

5E-05 Balance Uncertainty
0.001 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA)	LD50
----------	-----	------------	----------------------	------------	--------------------	-------------------	-------------------	---------------------	----------------------------------	--	------	----------------	------

1. 2-Chloroethyl vinyl ether	74	MKCD0033	10000	99	0.2	0.50536	0.50550	10002.9	40.5	110-75-8	N/A	or-rat 250mg/kg
------------------------------	----	----------	-------	----	-----	---------	---------	---------	------	----------	-----	-----------------

Method: GC6MSD-1.M. Detector: MSD. Column: (60m X 0.25mm X 1.5 µm). Oven Profile: Temp 1 = 35°C (Time 1=10min.), Temp 2 = 200°C (Time 2=8.75 min.), Rate = 4°C/min., Injector B Temp = 200°C, Detector B Temp. = 220°C. Analyst: Candice Warren.

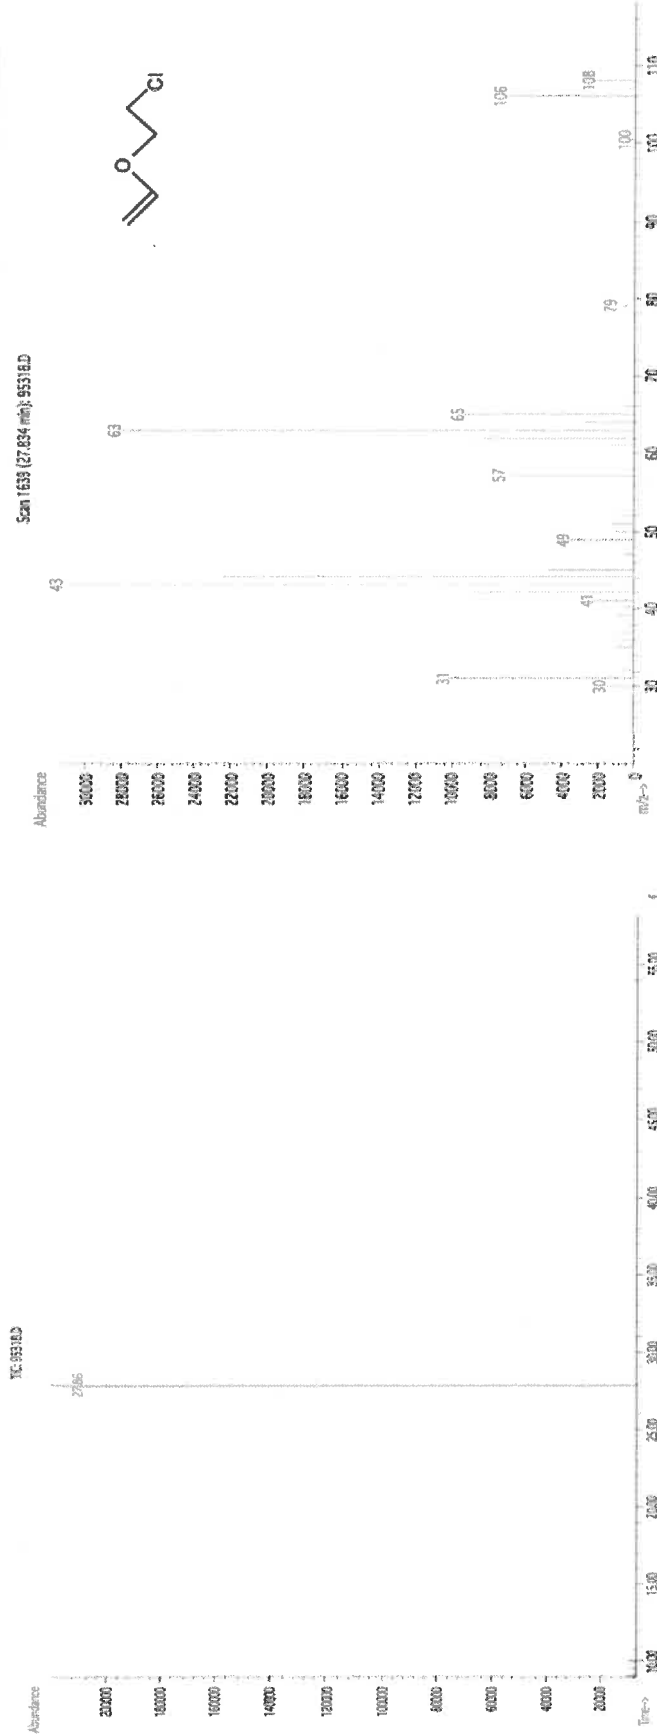

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (±) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Safety Data Sheet (SDS)

GHS/OSHA Compliant

Section I Product and Company Identification

IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr.	Emergency Telephone International	1-352-323-3500
	Hamden CT, 06514	Date Prepared/Revised	January 1, 2024

Section II - Hazards Identification

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H225	Highly Flammable Liquid and Vapor	H301, 311, 331	Toxic if swallowed, skin contact, inhaled
H370	Cause damage to organs	H351	Suspected of causing cancer
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302,332	If on skin, wash with soap and water	P305,351,338	If in eyes, remove contacts, rinse with water



Signal Word: DANGER

Section III - Composition

Components (Specific Chemical Identity; Common Name(s))		% (optional)
Methanol	METHYL ALCOHOL	> 97

See Certified Weight Report For Other Analytes Present At Trace Quantities.

INTENDED USE: REFERENCE MATERIAL

Section IV. FIRST AID MEASURES

General advice	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact	Wash with soap and water. Consult a physician.
In case of eye contact	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Flammability	Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.
Suitable extinguishing media	Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire	Wear self contained breathing apparatus for fire fighting if necessary.

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up	Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation. Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methanol	67-56-1	67-56-1	TWA 200 ppm
Skin notation			TWA 200 ppm
Potential for skin absorption, ingestion and inhalation.			
Personal protective equipment	Respiratory protection	Handle with gloves. Gloves must be inspected prior to use.	Eye protection.
Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.			

Section IX - Physical/Chemical Characteristics

Boiling Point	65°C	Specific Gravity (H ₂ O = 1)	0.79
Vapor Pressure (mm Hg)	96	Melting Point	-98°C
Vapor Density (AIR = 1)	1.11	Evaporation rate (Butyl Acetate = 1)	4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

Section X. STABILITY AND REACTIVITY

Chemical stability	Stable under recommended storage conditions.
Possibility of hazardous reactions	Vapours may form explosive mixture with air.
Conditions to avoid	Heat, flames, sparks, extreme temperature and sunlight.
Materials to avoid	Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids
Hazardous decomposition products formed under fire conditions.	- Carbon oxides

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - rat - 5,628 mg/kg
LC50 Inhalation - rat - 4 h - 64000 ppm
LD50 Dermal - rabbit - 15,800 mg/kg
Toxic if absorbed through skin. Causes skin irritation.
Eye damage/eye irritation
Toxic if inhaled. Causes respiratory tract irritation.
Toxic if swallowed.

Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.

LC50 15,400 mg/l - 96 h
EC50 24,500.00 mg/l - 48 h
EC100 10,000.00 mg/l - 24 h

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US)	IATA
UN number: 1230 Class: 3 Packing group: II	UN number: 1230 Class: 3 Packing group: II
Proper shipping name: Methanol	Proper shipping name: Methanol

Section XV. REGULATORY INFORMATION

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant
SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



Dec 12/6/24
20 vial

CERTIFIED WEIGHT REPORT

Part Number: 95318
Lot Number: 120524
Description: 2-Chloroethyl vinyl ether

Solvent(s): Lot#
Methanol EJ143-US

Expiration Date: 120527
Recommended Storage: Refrigerate (4 °C)
Nominal Concentration (µg/mL): 10000
NIST Test ID#: 6UTB

Weight(s) shown below were combined and diluted to (mL):


5E-05 Balance Uncertainty
0.001 Flask Uncertainty

Formulated By: Prashant Chauhan 120524
Reviewed By: Pedro L. Rentas 120524

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information	
										(Solvent Safety Info. On Attached pg.)	LD50

1. 2-Chloroethyl vinyl ether	74	MKCD0033	10000	99	0.2	0.50536	0.50550	10002.9	40.5	110-75-8	N/A	or-rat 250mg/kg
------------------------------	----	----------	-------	----	-----	---------	---------	---------	------	----------	-----	-----------------

Method: GC6MSD-1.M. Detector: MSD. Column: (60m X 0.25mm X 1.5 µm). Oven Profile: Temp 1 = 35°C (Time 1=10min.), Temp 2 = 200°C (Time 2=8.75 min.), Rate = 4°C/min., Injector B Temp = 200°C, Detector B Temp = 220°C. Analyst: Candice Warren.

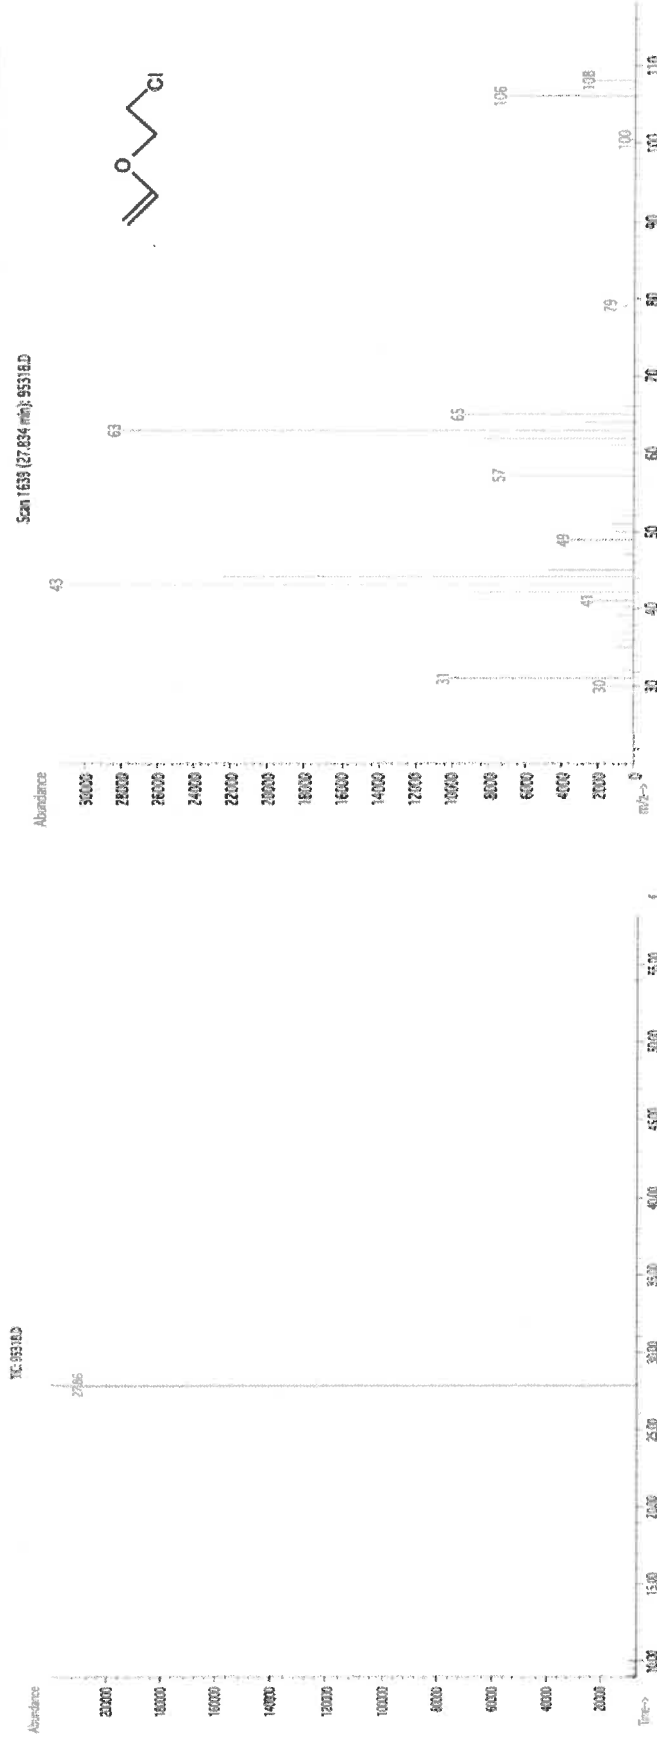

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

GHS/OSHA Compliant

Section I Product and Company Identification

IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rosotto Dr. Hamden CT. 06514	Emergency Telephone International Date Prepared/Revised	1-352-323-3500 January 1, 2024

Section II - Hazards Identification

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H225	Highly Flammable Liquid and Vapor	H301, 311, 331	Toxic if swallowed, skin contact, inhaled
H370	Cause damage to organs	H351	Suspected of causing cancer
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302,332	If on skin, wash with soap and water	P305,351,338	If in eyes, remove contacts, rinse with water



Signal Word: DANGER

Section III - Composition

Components (Specific Chemical Identity; Common Name(s))	CAS#	% (optional)
Methanol	METHYL ALCOHOL	> 97

See Certified Weight Report For Other Analytes Present At Trace Quantities.

INTENDED USE: REFERENCE MATERIAL

Section IV. FIRST AID MEASURES

General advice	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact	Wash with soap and water. Consult a physician.
In case of eye contact	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Flammability	Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.
Suitable extinguishing media	Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire	Wear self contained breathing apparatus for fire fighting if necessary.

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up	Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methanol 67-56-1 TWA 200 ppm
Skin notation TWA 200 ppm
Potential for skin absorption, ingestion and inhalation.
Personal protective equipment Respiratory protection Handle with gloves. Gloves must be inspected prior to use. Eye protection.
Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.

Section IX - Physical/Chemical Characteristics

Boiling Point	65°C	Specific Gravity (H ₂ O = 1)	0.79
Vapor Pressure (mm Hg)	96	Melting Point	-98°C
Vapor Density (AIR = 1)	1.11	Evaporation rate (Butyl Acetate = 1)	4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

Section X. STABILITY AND REACTIVITY

Chemical stability	Stable under recommended storage conditions.
Possibility of hazardous reactions	Vapours may form explosive mixture with air.
Conditions to avoid	Heat, flames, sparks, extreme temperature and sunlight.
Materials to avoid	Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids
Hazardous decomposition products formed under fire conditions.	- Carbon oxides

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - rat - 5,628 mg/kg
LC50 Inhalation - rat - 4 h - 64000 ppm
LD50 Dermal - rabbit - 15,800 mg/kg
Toxic if absorbed through skin. Causes skin irritation.
Eye damage/eye irritation
Toxic if inhaled. Causes respiratory tract irritation.
Toxic if swallowed.

Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.

LC50 15,400 mg/l - 96 h
EC50 24,500.00 mg/l - 48 h
EC100 10,000.00 mg/l - 24 h

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US)	IATA
UN number: 1230 Class: 3 Packing group: II	UN number: 1230 Class: 3 Packing group: II
Proper shipping name: Methanol	Proper shipping name: Methanol

Section XV. REGULATORY INFORMATION

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant
SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



Dec 12/6/24
20 vial

CERTIFIED WEIGHT REPORT

Part Number: 95318
Lot Number: 120524
Description: 2-Chloroethyl vinyl ether

Solvent(s): Lot#
Methanol EJ143-US

Expiration Date: 120527
Recommended Storage: Refrigerate (4 °C)
Nominal Concentration (µg/mL): 10000
NIST Test ID#: 6UTB

✓ 14630 to
✓ 14649


Weight(s) shown below were combined and diluted to (mL):

5E-05 Balance Uncertainty
0.001 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	(Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LD50
----------	-----	------------	----------------------	------------	--------------------	-------------------	-------------------	---------------------	----------------------------------	--	----------------	------

1. 2-Chloroethyl vinyl ether	74	MKCD0033	10000	99	0.2	0.50536	0.50550	10002.9	40.5	110-75-8	N/A	or-rat 250mg/kg
------------------------------	----	----------	-------	----	-----	---------	---------	---------	------	----------	-----	-----------------

Method: GC6MSD-1.M. Detector: MSD. Column: (60m X 0.25mm X 1.5 µm). Oven Profile: Temp 1 = 35°C (Time 1=10min.), Temp 2 = 200°C (Time 2=8.75 min.), Rate = 4°C/min., Injector B Temp = 200°C, Detector B Temp. = 220°C. Analyst: Candice Warren.

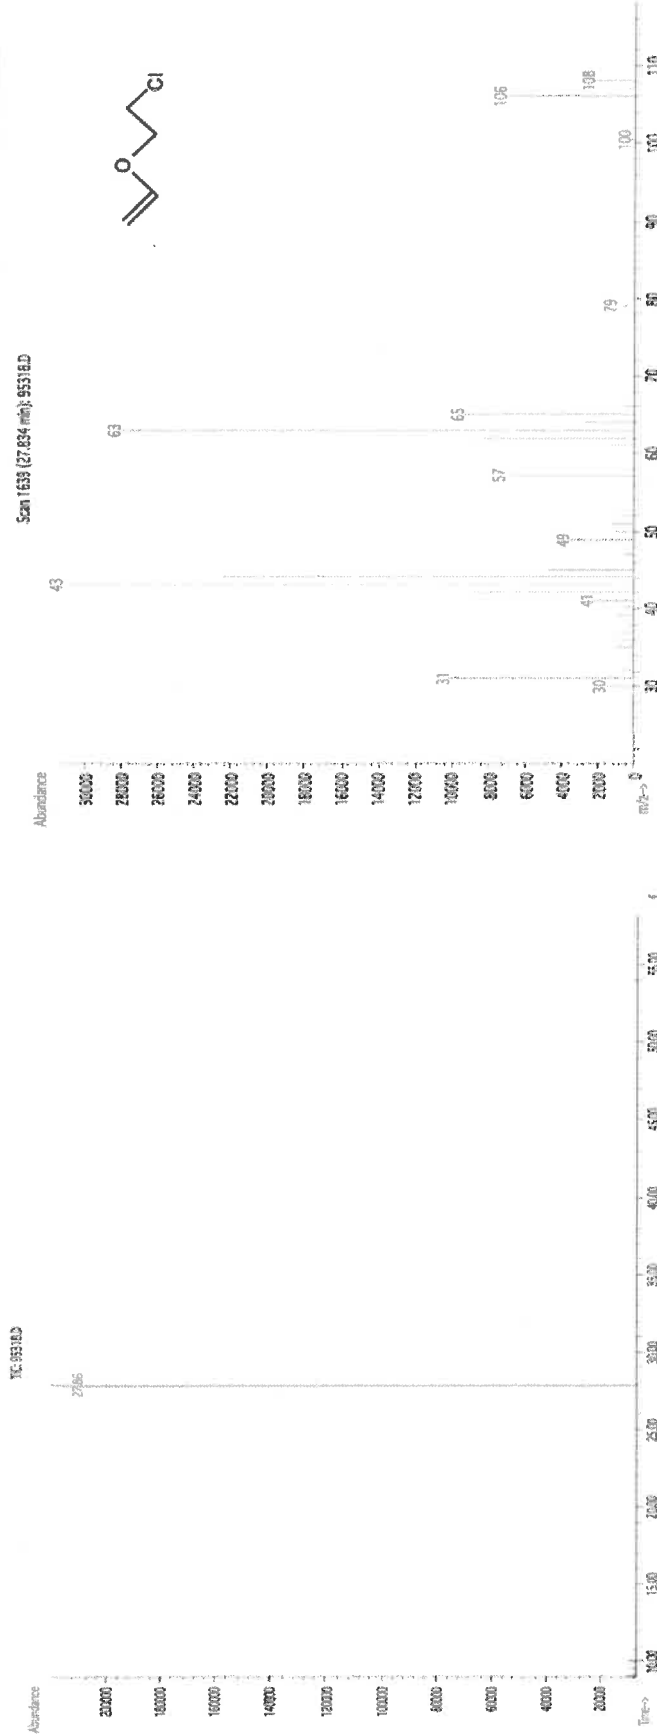

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (±) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Safety Data Sheet (SDS)

GHS/OSHA Compliant

Section I Product and Company Identification

IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr.	Emergency Telephone International	1-352-323-3500
	Hamden CT, 06514	Date Prepared/Revised	January 1, 2024

Section II - Hazards Identification

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H225	Highly Flammable Liquid and Vapor	H301, 311, 331	Toxic if swallowed, skin contact, inhaled
H370	Cause damage to organs	H351	Suspected of causing cancer
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302,332	If on skin, wash with soap and water	P305,351,338	If in eyes, remove contacts, rinse with water



Signal Word: DANGER

Section III - Composition

Components (Specific Chemical Identity; Common Name(s))		% (optional)
Methanol	METHYL ALCOHOL	> 97

See Certified Weight Report For Other Analytes Present At Trace Quantities.

INTENDED USE: REFERENCE MATERIAL

Section IV. FIRST AID MEASURES

General advice	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact	Wash with soap and water. Consult a physician.
In case of eye contact	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Flammability	Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.
Suitable extinguishing media	Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire	Wear self contained breathing apparatus for fire fighting if necessary.

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up	Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation. Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methanol	67-56-1	67-56-1	TWA 200 ppm
Skin notation			TWA 200 ppm
Potential for skin absorption, ingestion and inhalation.			
Personal protective equipment	Respiratory protection	Handle with gloves. Gloves must be inspected prior to use.	Eye protection.
Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.			

Section IX - Physical/Chemical Characteristics

Boiling Point	65°C	Specific Gravity (H ₂ O = 1)	0.79
Vapor Pressure (mm Hg)	96	Melting Point	-98°C
Vapor Density (AIR = 1)	1.11	Evaporation rate (Butyl Acetate = 1)	4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

Section X. STABILITY AND REACTIVITY

Chemical stability	Stable under recommended storage conditions.
Possibility of hazardous reactions	Vapours may form explosive mixture with air.
Conditions to avoid	Heat, flames, sparks, extreme temperature and sunlight.
Materials to avoid	Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids
Hazardous decomposition products formed under fire conditions.	- Carbon oxides

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - rat - 5,628 mg/kg
LC50 Inhalation - rat - 4 h - 64000 ppm
LD50 Dermal - rabbit - 15,800 mg/kg
Toxic if absorbed through skin. Causes skin irritation.
Eye damage/eye irritation
Toxic if inhaled. Causes respiratory tract irritation.
Toxic if swallowed.

Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.

LC50 15,400 mg/l - 96 h
EC50 24,500.00 mg/l - 48 h
EC100 10,000.00 mg/l - 24 h

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US)	IATA
UN number: 1230 Class: 3 Packing group: II	UN number: 1230 Class: 3 Packing group: II
Proper shipping name: Methanol	Proper shipping name: Methanol

Section XV. REGULATORY INFORMATION

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant
SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30067 **Lot No.:** A0191805

Description : 4-Bromofluorobenzene Standard

4-Bromofluorobenzene Standard 2,500µg/mL, P&T Methanol,
1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : November 30, 2027 **Storage:** 0°C or colder

Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Bromo-4-fluorobenzene (BFB)	460-00-4	184975	99%	2,483.9 µg/mL	+/- 139.5488

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:


40 ml/min

Inj. Vol

1µl

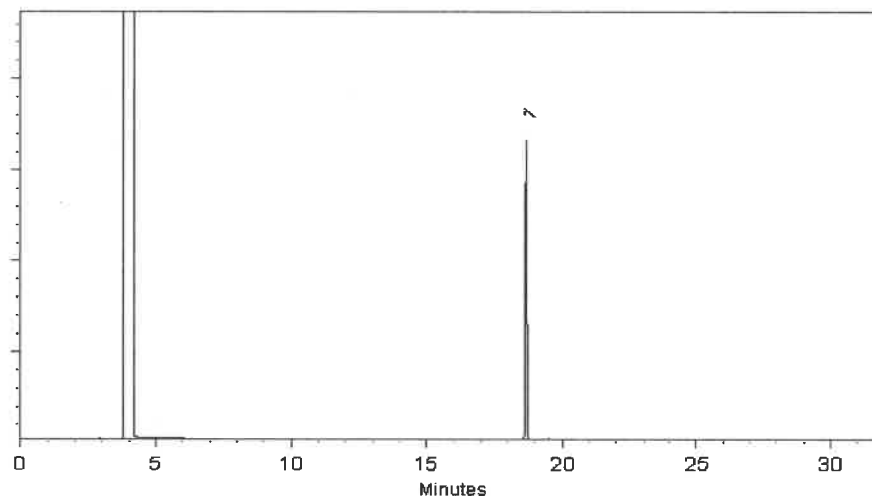

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Alicia Leathers - Operation Technician I

Date Mixed: 17-Nov-2022

Balance Serial # B251644995


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 21-Nov-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30006 **Lot No.:** A0200785

Description : VOA Calibration Mix #1

VOA Calibration Mix #1 5,000µg/mL, P&T Methanol/Water(90:10), 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : November 30, 2026 **Storage:** 0°C or colder

Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Acetone	67-64-1	SHBP8774	99%	5,018.5 µg/mL	+/- 173.4162
2	2-Butanone (MEK)	78-93-3	SHBL5543	99%	5,016.0 µg/mL	+/- 173.3298
3	4-Methyl-2-pentanone (MIBK)	108-10-1	SHBP4724	99%	5,010.7 µg/mL	+/- 173.1455
4	2-Hexanone	591-78-6	MKCQ6663	99%	5,015.0 µg/mL	+/- 173.2952

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol/Water (90:10)
CAS # 67-56-1/7732-18-5
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0 μ m
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:


40 ml/min

Inj. Vol

1 μ l

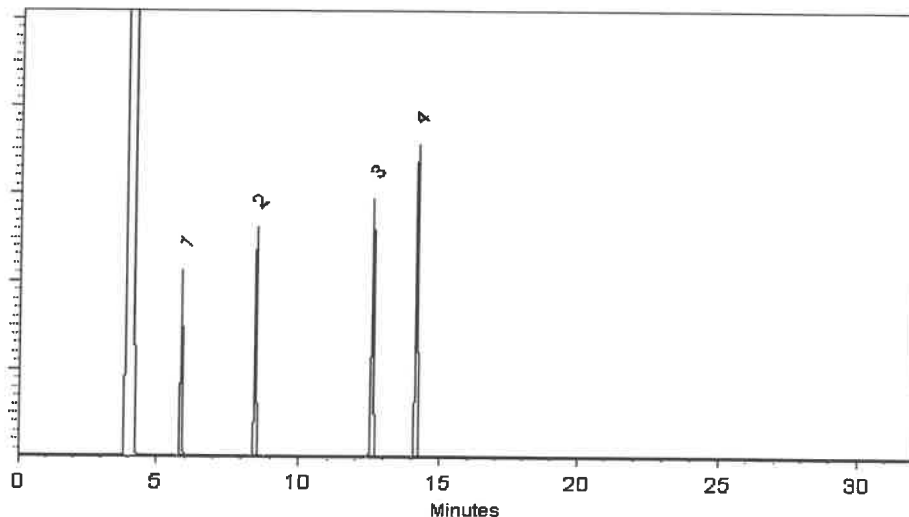

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 09-Aug-2023

Balance Serial # B707717271


Marlina Cowan - Operations Tech II ARM QC

Date Passed: 16-Aug-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30006 **Lot No.:** A0200785

Description : VOA Calibration Mix #1

VOA Calibration Mix #1 5,000µg/mL, P&T Methanol/Water(90:10), 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : November 30, 2026 **Storage:** 0°C or colder

Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Acetone	67-64-1	SHBP8774	99%	5,018.5 µg/mL	+/- 173.4162
2	2-Butanone (MEK)	78-93-3	SHBL5543	99%	5,016.0 µg/mL	+/- 173.3298
3	4-Methyl-2-pentanone (MIBK)	108-10-1	SHBP4724	99%	5,010.7 µg/mL	+/- 173.1455
4	2-Hexanone	591-78-6	MKCQ6663	99%	5,015.0 µg/mL	+/- 173.2952

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol/Water (90:10)
CAS # 67-56-1/7732-18-5
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:


40 ml/min

Inj. Vol

1µl

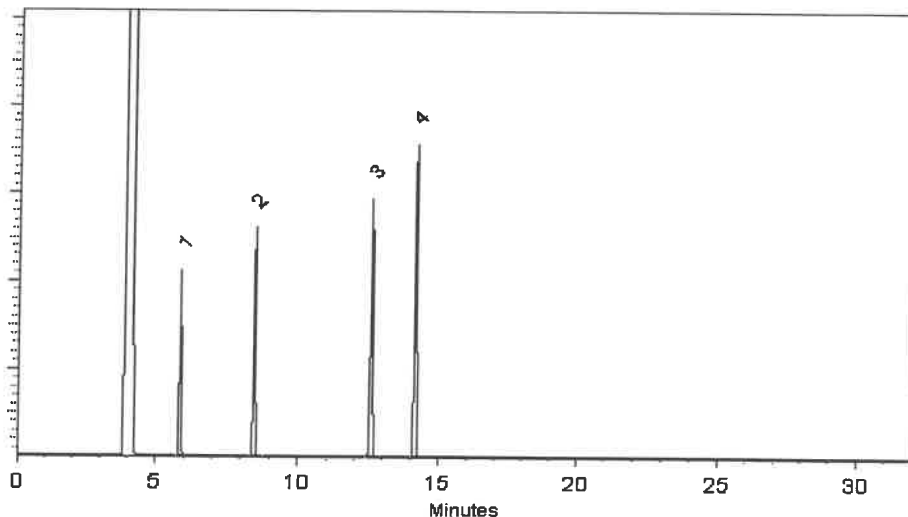

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 09-Aug-2023

Balance Serial # B707717271


Marlina Cowan - Operations Tech II ARM QC

Date Passed: 16-Aug-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30006 **Lot No.:** A0200785

Description : VOA Calibration Mix #1

VOA Calibration Mix #1 5,000µg/mL, P&T Methanol/Water(90:10), 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : November 30, 2026 **Storage:** 0°C or colder

Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Acetone	67-64-1	SHBP8774	99%	5,018.5 µg/mL	+/- 173.4162
2	2-Butanone (MEK)	78-93-3	SHBL5543	99%	5,016.0 µg/mL	+/- 173.3298
3	4-Methyl-2-pentanone (MIBK)	108-10-1	SHBP4724	99%	5,010.7 µg/mL	+/- 173.1455
4	2-Hexanone	591-78-6	MKCQ6663	99%	5,015.0 µg/mL	+/- 173.2952

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol/Water (90:10)
CAS # 67-56-1/7732-18-5
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:


40 ml/min

Inj. Vol

1µl

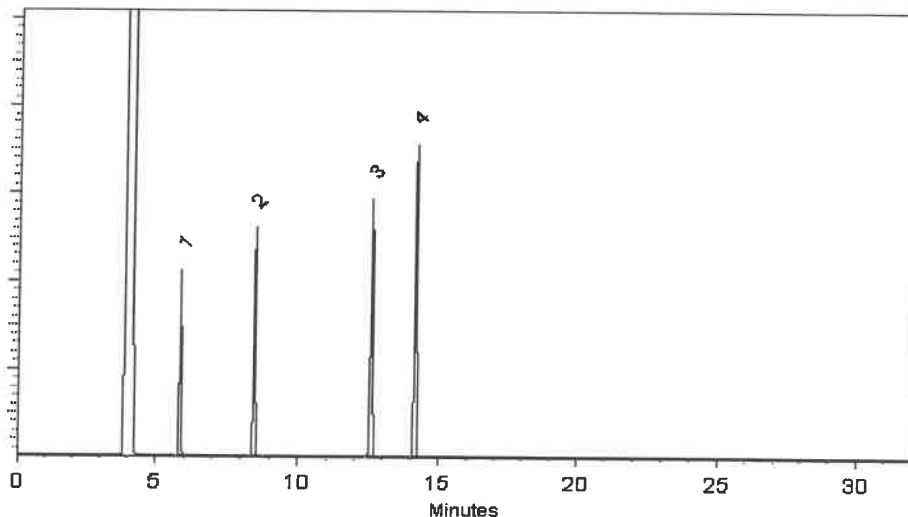

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 09-Aug-2023

Balance Serial # B707717271


Marlina Cowan - Operations Tech II ARM QC

Date Passed: 16-Aug-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 555581 Lot No.: A0210184

Description: Custom 8260 Internal Standard Mix

Custom 8260 Internal Standard Mix 25,000µg/mL, P&T Methanol, 1mL/ampul

Container Size: 2 mL Pkg Amt: > 1 mL

Expiration Date: April 30, 2027 Storage: 10°C or colder

Ship: Ambient

CERTIFIED VALUES

Component #	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,4-Dichlorobenzene-d4	3855-82-1	PR-30447	99%	25,212.0 µg/mL	+/- 1,427.8857
2	1,4-Difluorobenzene	540-36-3	MKCS8657	99%	25,220.0 µg/mL	+/- 1,428.3388
3	Chlorobenzene-d5	3114-55-4	PR-31132	99%	25,116.0 µg/mL	+/- 1,422.4487
4	Pentafluorobenzene	363-72-4	MKCR9383	99%	25,180.0 µg/mL	+/- 1,426.0734

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

John Friedline - Operations Technician I

Date Mixed: 11-Apr-2024 Balance: 11275.10105



Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

10 vial.
Dec: 12/09/24
CERTIFIED REFERENCE MATERIAL

Certificate of Analysis
chromatographic plus

V14667-5
V14676



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30225 **Lot No.:** A0214960
Description : Bromochloromethane Standard
Bromochloromethane 2000µg/mL, P&T Methanol, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : August 31, 2029 **Storage:** 0°C or colder
Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Bromochloromethane	74-97-5	SYN240416CTH	99%	2,012.0 µg/mL	+/- 113.0519

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1µl

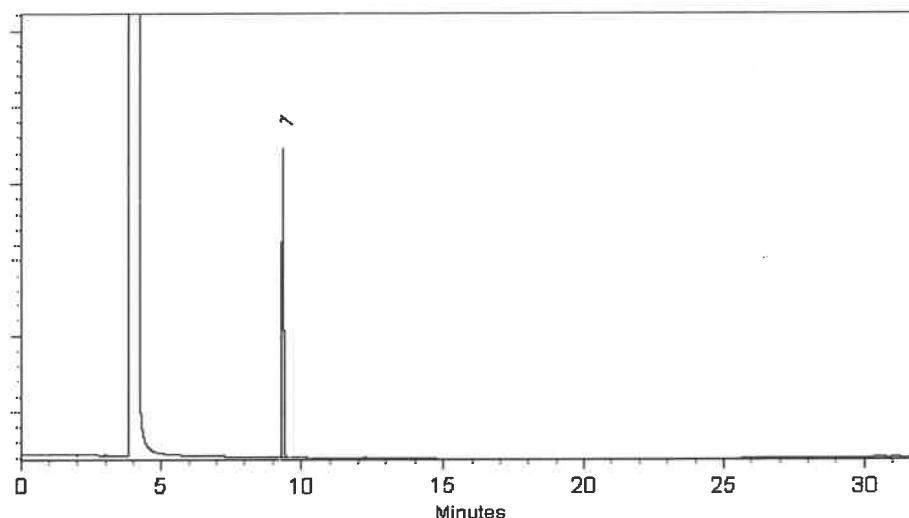

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Stacey Wanner - Operations Technician I

Date Mixed: 08-Aug-2024

Balance Serial # 1127510105

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 14-Aug-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

Rec 12/17/24
CERTIFIED REFERENCE MATERIAL

30 ml
Certificate of Analysis
chromatographic plus

V14727 to
V14756



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30042 **Lot No.:** A0216826
Description : 502.2 Calibration Mix #1
502.2 Calibration Mix #1 2,000µg/mL, P&T Methanol, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : May 31, 2031 **Storage:** 0°C or colder
Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Dichlorodifluoromethane (CFC-12)	75-71-8	00022922	99%	2,000.9 µg/mL	+/- 112.4144
2	Chloromethane (methyl chloride)	74-87-3	00022694	99%	2,000.7 µg/mL	+/- 112.3998
3	Vinyl chloride	75-01-4	00015559	99%	2,000.3 µg/mL	+/- 112.3779
4	Bromomethane (methyl bromide)	74-83-9	00017022	99%	2,001.8 µg/mL	+/- 112.4650
5	Chloroethane (ethyl chloride)	75-00-3	107-401039114-1	99%	2,000.1 µg/mL	+/- 112.3700
6	Trichlorofluoromethane (CFC-11)	75-69-4	MKCJ8658	99%	2,000.7 µg/mL	+/- 112.3992

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Quality Confirmation Test

Column:

60m x 0.25mm x 1.4µm
Rtx-502.2 (cat.#10916)

Carrier Gas:

helium-constant flow 2.0 mL/min.

Temp. Program:

40°C (hold 6 min.) to 100°C
@ 6°C/min.

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


MSD

Split Vent:

Split ratio 10:1

Inj. Vol

1µl

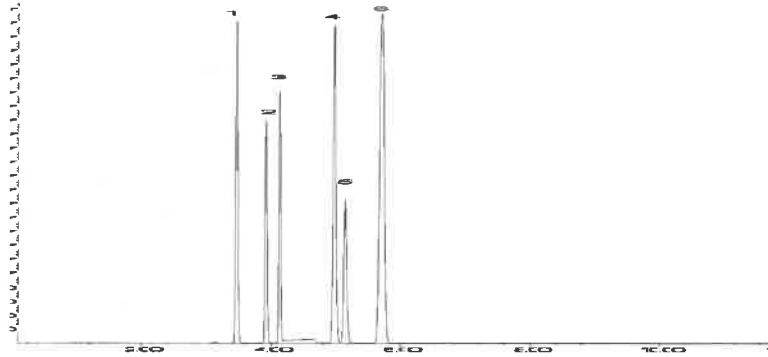

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Tom Suckal - Mix Technician

Date Mixed: 23-Sep-2024

Balance Serial # B707717271

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 04-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

Rec 12/17/24
CERTIFIED REFERENCE MATERIAL

30 ml
Certificate of Analysis
chromatographic plus

V14727 to
V14756



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30042 **Lot No.:** A0216826
Description : 502.2 Calibration Mix #1
502.2 Calibration Mix #1 2,000µg/mL, P&T Methanol, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : May 31, 2031 **Storage:** 0°C or colder
Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Dichlorodifluoromethane (CFC-12)	75-71-8	00022922	99%	2,000.9 µg/mL	+/- 112.4144
2	Chloromethane (methyl chloride)	74-87-3	00022694	99%	2,000.7 µg/mL	+/- 112.3998
3	Vinyl chloride	75-01-4	00015559	99%	2,000.3 µg/mL	+/- 112.3779
4	Bromomethane (methyl bromide)	74-83-9	00017022	99%	2,001.8 µg/mL	+/- 112.4650
5	Chloroethane (ethyl chloride)	75-00-3	107-401039114-1	99%	2,000.1 µg/mL	+/- 112.3700
6	Trichlorofluoromethane (CFC-11)	75-69-4	MKCJ8658	99%	2,000.7 µg/mL	+/- 112.3992

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Quality Confirmation Test

Column:

60m x 0.25mm x 1.4µm
Rtx-502.2 (cat.#10916)

Carrier Gas:

helium-constant flow 2.0 mL/min.

Temp. Program:

40°C (hold 6 min.) to 100°C
@ 6°C/min.

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


MSD

Split Vent:

Split ratio 10:1

Inj. Vol

1µl

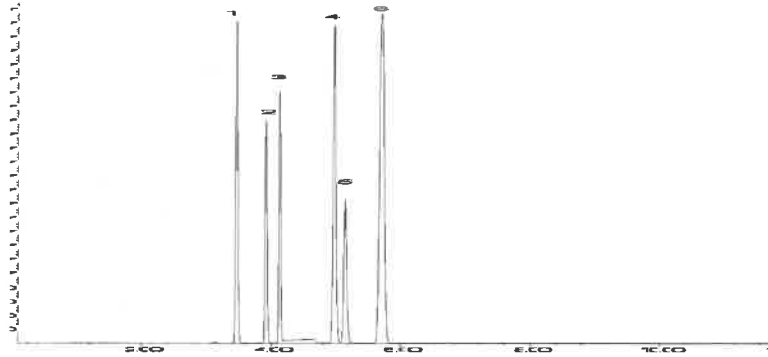

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Tom Suckal - Mix Technician

Date Mixed: 23-Sep-2024

Balance Serial # B707717271

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 04-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus

✓ 14842 to 14846



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30470 **Lot No.:** A0217535
Description : tert-Butanol Standard
tert-Butanol Std 50,000µg/mL, P&T Methanol, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : October 31, 2027 **Storage:** 0°C or colder
Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	tert-Butanol (TBA)	75-65-0	SHBQ8002-1	99%	50,007.5 µg/mL	+/- 717.6137

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1µl

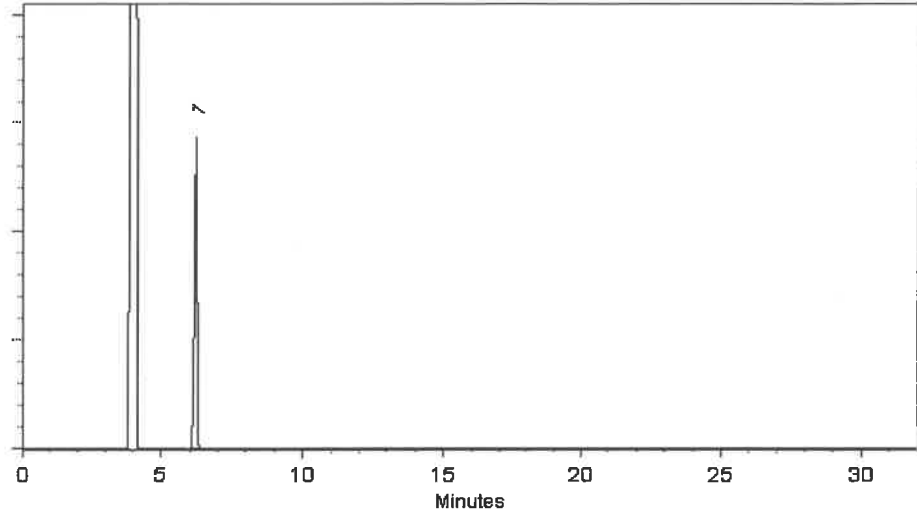

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

A. O. E.
Aaron Enyart - Operations Tech I

Date Mixed: 07-Oct-2024

Balance Serial # B251644995

Brittany Federinko
Brittany Federinko - Operations Tech I

Date Passed: 09-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

2014 Dec 01/08/21
CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic

V14803 - V14822



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 555408-SL **Lot No.:** A0220471
Description : Custom Vinyl Acetate Standard
Custom Vinyl Acetate Standard 8,000µg/mL, P&T Methanol, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : June 30, 2026 **Storage:** -20°C or colder
Handling: This product is photosensitive. **Ship:** On Ice

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Vinyl acetate	108-05-4	RD240423RSR	99%	8,066.0 µg/mL	+/- 278.7979

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Tech Tips:

Vinyl acetate is a volatile organic ester included in the target lists of several US EPA and other methods. Under acidic conditions, esters react with alcohols to form new esters (transesterification). Methanol-based mixes containing halogenated compounds are slightly acidic, so it is important to minimize exposure of vinyl acetate to mixes of halogenated compounds in methanol. For this reason, we offer vinyl acetate in individual solution, and suggest that it be introduced into the working level calibration solution immediately before use. This will minimize problems and ensure more consistent results.

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1µl

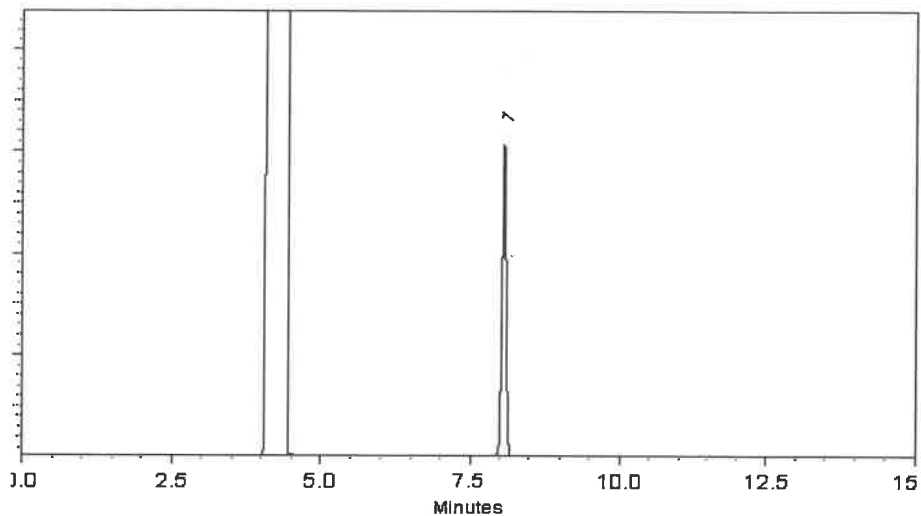

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ethan Winiarski - Operations Tech I

Date Mixed: 24-Dec-2024

Balance Serial # 1127510105

Dillan Murphy - Operations Technician I

Date Passed: 02-Jan-2025

REVIEWED
By Jennifer Pollock at 7:12 am, Jan 05, 2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

2014 Dec 01/08/21
CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic

V14803 - V14822



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 555408-SL **Lot No.:** A0220471
Description : Custom Vinyl Acetate Standard
Custom Vinyl Acetate Standard 8,000µg/mL, P&T Methanol, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : June 30, 2026 **Storage:** -20°C or colder
Handling: This product is photosensitive. **Ship:** On Ice

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Vinyl acetate	108-05-4	RD240423RSR	99%	8,066.0 µg/mL	+/- 278.7979

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Tech Tips:

Vinyl acetate is a volatile organic ester included in the target lists of several US EPA and other methods. Under acidic conditions, esters react with alcohols to form new esters (transesterification). Methanol-based mixes containing halogenated compounds are slightly acidic, so it is important to minimize exposure of vinyl acetate to mixes of halogenated compounds in methanol. For this reason, we offer vinyl acetate in individual solution, and suggest that it be introduced into the working level calibration solution immediately before use. This will minimize problems and ensure more consistent results.

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1µl

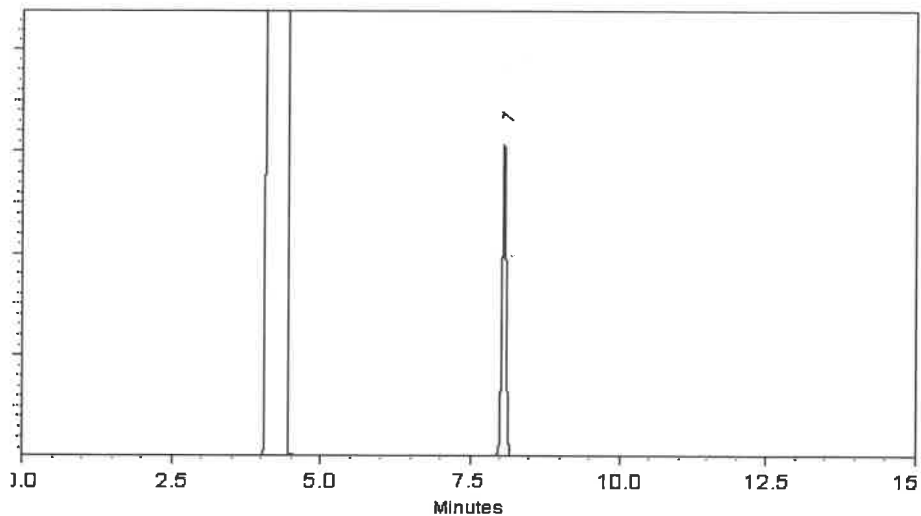

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ethan Winiarski - Operations Tech I

Date Mixed: 24-Dec-2024

Balance Serial # 1127510105

Dillan Murphy - Operations Technician I

Date Passed: 02-Jan-2025

REVIEWED
By Jennifer Pollock at 7:12 am, Jan 05, 2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

gravimetric

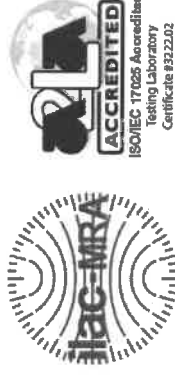

10 vial
See 03/31/25
V14904 to V14913

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 555582 Lot No.: A0223904

Description: Custom 8260A/B Surrogate Mix

Custom 8260A/B Surrogate Mix 25,000µg/mL, P&T Methanol, 1mL/ampul

Container Size: 2 mL Pkg Amt: > 1 mL

Expiration Date: March 31, 2028 Storage: 10°C or colder

Ship: Ambient

CERTIFIED VALUES

Component #	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	1,2-Dichloroethane-d4	17060-07-0	PR-33313	99%	25,108.0 µg/mL	+/- 1,421.9957
2	1-Bromo-4-fluorobenzene (BFB)	460-00-4	0000268853	99%	25,108.0 µg/mL	+/- 1,421.9957
3	Dibromofluoromethane	1868-53-7	VENKAT02	99%	25,232.0 µg/mL	+/- 1,429.0184
4	Toluene-d8	2037-26-5	PR-34141	99%	25,156.0 µg/mL	+/- 1,424.7141

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Brittany Federlino

Brittany Federlino - Operations Tech I

Date Mixed: 27-Mar-2025

Balance: B251644995

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.

Methanol
ULTRA RESI-ANALYZED
For Purge and Trap Analysis

Rec 05/09/25
Avantor™



*V14921 to
V14938*

Material No.: 9077-02
Batch No.: 24G0262002
Manufactured Date: 2024-05-14
Expiration Date: 2027-05-14
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay (CH ₃ OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.3 ppm
Titration Acid (μeq/g)	≤ 0.3	0.3
Titration Base (μeq/g)	≤ 0.10	0.03
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis - Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use
Performance Tested for Use in EPA Methods
500 Series for Drinking Water
600 Series for Wastewater
846 for Solid Waste

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Methanol
ULTRA RESI-ANALYZED
For Purge and Trap Analysis

Rec 05/09/25
Avantor™



*V14921 to
V14938*

Material No.: 9077-02
Batch No.: 24G0262002
Manufactured Date: 2024-05-14
Expiration Date: 2027-05-14
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay (CH ₃ OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.3 ppm
Titration Acid (μeq/g)	≤ 0.3	0.3
Titration Base (μeq/g)	≤ 0.10	0.03
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis - Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use
Performance Tested for Use in EPA Methods
500 Series for Drinking Water
600 Series for Wastewater
846 for Solid Waste

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Mark
Jamie Croak
Director Quality Operations, Bioscience Production

Methanol
ULTRA RESI-ANALYZED
For Purge and Trap Analysis

Rec 05/09/25
Avantor™



*V14921 to
V14938*

Material No.: 9077-02
Batch No.: 24G0262002
Manufactured Date: 2024-05-14
Expiration Date: 2027-05-14
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay (CH ₃ OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.3 ppm
Titration Acid (μeq/g)	≤ 0.3	0.3
Titration Base (μeq/g)	≤ 0.10	0.03
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis - Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use
Performance Tested for Use in EPA Methods
500 Series for Drinking Water
600 Series for Wastewater
846 for Solid Waste

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309
www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus

✓ 149516 ✓ 14970



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30489 Lot No.: A0222076

Description : 8260B Acetates Mix

8260B Acetates Mix 2,000 µg/mL, P&T Methanol, 1mL/ampul

Container Size : 2 mL Pkg Amt: > 1 mL

Expiration Date : August 31, 2026 Storage: -20°C or colder

Handling: This product is photosensitive. Ship: On Ice

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Methyl acetate	79-20-9	SHBR1889	99%	2,004.0 µg/mL	+/- 69.2674
2	Vinyl acetate	108-05-4	RD240423RSR	99%	2,010.0 µg/mL	+/- 69.4748
3	Ethyl acetate	141-78-6	SHBS3323	99%	2,019.3 µg/mL	+/- 69.7974
4	Isopropyl acetate	108-21-4	BCCG7069	99%	2,008.0 µg/mL	+/- 69.4057
5	Propyl acetate	109-60-4	P8XLN	99%	2,008.0 µg/mL	+/- 69.4057
6	Butyl acetate	123-86-4	SHBR2024	99%	2,008.0 µg/mL	+/- 69.4057
7	Amyl acetate	628-63-7	BCBT7442	99%	2,006.7 µg/mL	+/- 69.3596

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Tech Tips:

Vinyl acetate is a volatile organic ester included in the target lists of several US EPA and other methods. Under acidic conditions, esters react with alcohols to form new esters (transesterification). Methanol-based mixes containing halogenated compounds are slightly acidic, so it is important to minimize exposure of vinyl acetate to mixes of halogenated compounds in methanol. For this




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309
www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus

✓ 149516 ✓ 14970



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30489 Lot No.: A0222076

Description : 8260B Acetates Mix

8260B Acetates Mix 2,000 µg/mL, P&T Methanol, 1mL/ampul

Container Size : 2 mL Pkg Amt: > 1 mL

Expiration Date : August 31, 2026 Storage: -20°C or colder

Handling: This product is photosensitive. Ship: On Ice

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Methyl acetate	79-20-9	SHBR1889	99%	2,004.0 µg/mL	+/- 69.2674
2	Vinyl acetate	108-05-4	RD240423RSR	99%	2,010.0 µg/mL	+/- 69.4748
3	Ethyl acetate	141-78-6	SHBS3323	99%	2,019.3 µg/mL	+/- 69.7974
4	Isopropyl acetate	108-21-4	BCCG7069	99%	2,008.0 µg/mL	+/- 69.4057
5	Propyl acetate	109-60-4	P8XLN	99%	2,008.0 µg/mL	+/- 69.4057
6	Butyl acetate	123-86-4	SHBR2024	99%	2,008.0 µg/mL	+/- 69.4057
7	Amyl acetate	628-63-7	BCBT7442	99%	2,006.7 µg/mL	+/- 69.3596

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Tech Tips:

Vinyl acetate is a volatile organic ester included in the target lists of several US EPA and other methods. Under acidic conditions, esters react with alcohols to form new esters (transesterification). Methanol-based mixes containing halogenated compounds are slightly acidic, so it is important to minimize exposure of vinyl acetate to mixes of halogenated compounds in methanol. For this



Certified Reference Material CRM



Re 101625 5100

CERTIFIED WEIGHT REPORT

Part Number:
Lot Number:
Description:

91980
101625
Acrolein

Solvent(s):
Water

Lot#
041725Q

Expiration Date:
Recommended Storage:
Nominal Concentration (µg/mL):
NIST Test ID#:

111625
Refrigerate (2°C to 8°C)
5000
6UTB

5E-05 Balance Uncertainty
0.001 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL):


10.0

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
----------	-----	------------	----------------------	------------	-------------	------------------	------------------	---------------------	----------------------------------	------	----------------	------

1. Acrolein 5 103755V10F 5000 97 0.5 0.05166 0.05180 5013.7 52.6 107-02-8 0.1 ppm orl-rat 48mg/kg

Method: GC6MSD-1. Detector: Mass Selective Detector (Scan mode). Columns: Vool (60m X 0.25mm ID X 1.5µm film thickness). Oven Profile: Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2 = 200°C (Time 2 = 8.75 min.). Rate = 4°C/min., Injector Temp. = 200°C, Detector Temp. = 220°C. Analyst: Pedro Renteria. NOTE: Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately. Long term storage is not recommended. Please contact our technical department if further information is required.

TIC: [BSB2]79005.D

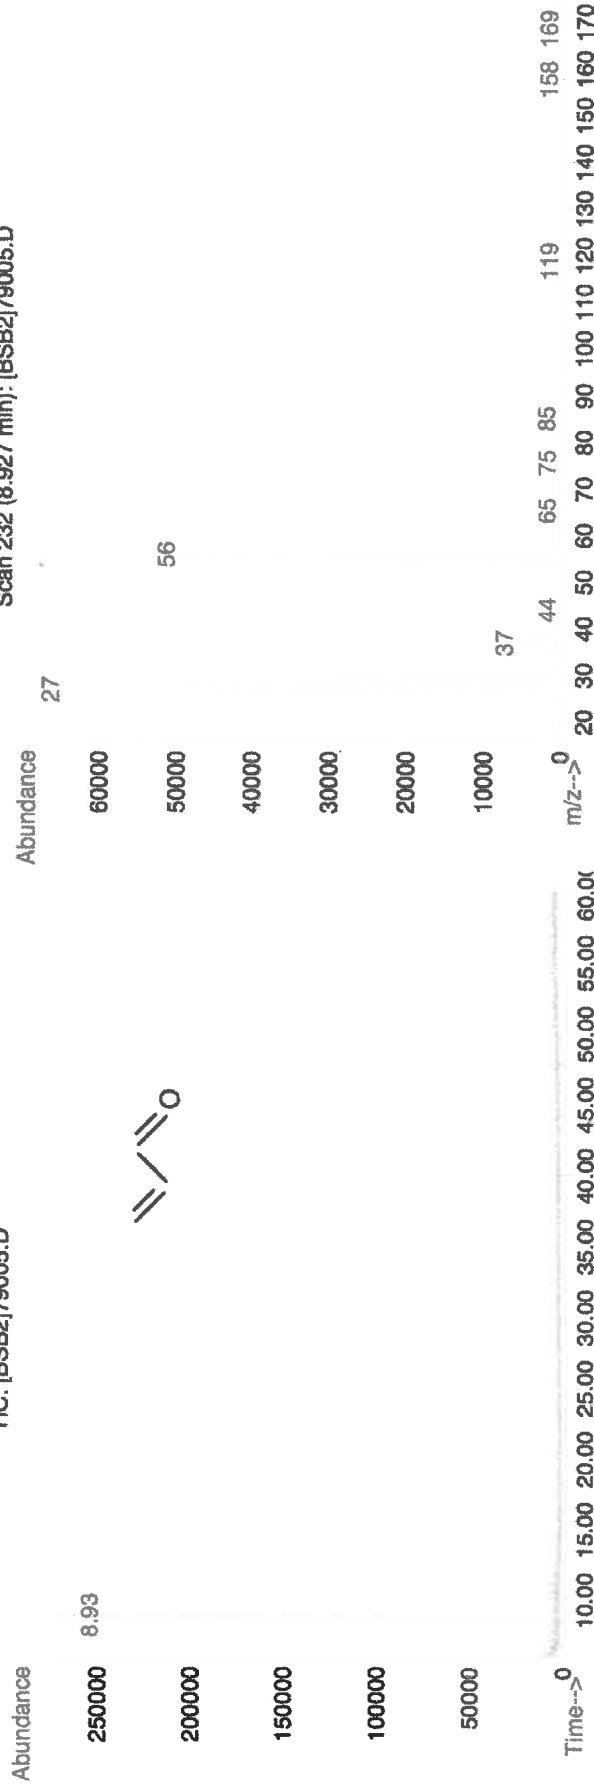

• The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
• Standards are prepared gravimetrically using balances that are calibrated by an ISO 17025 certified organization with weights traceable through NIST to the SI kilogram (see above).
• Standards are certified (±) 0.5% of the stated value, unless otherwise stated.
• All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
• Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).
Rev 1A, 2/25/2025



Certified Reference Material CRM



Re 101625 5109

CERTIFIED WEIGHT REPORT

Part Number:
Lot Number:
Description:

91980
101625
Acrolein

Solvent(s):
Water

Lot#
041725Q

Expiration Date:
Recommended Storage:
Nominal Concentration (µg/mL):
NIST Test ID#:

111625
Refrigerate (2°C to 8°C)
5000
6UTB

5E-05 Balance Uncertainty
0.001 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL):


10.0

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
----------	-----	------------	----------------------	------------	-------------	------------------	------------------	---------------------	----------------------------------	------	----------------	------

1. Acrolein 5 103755V10F 5000 97 0.5 0.05166 0.05180 5013.7 52.6 107-02-8 0.1 ppm orl-rat 48mg/kg

Method: GC6MSD-1. Detector: Mass Selective Detector (Scan mode). Columns: Vool (60m X 0.25mm ID X 1.5µm film thickness). Oven Profile: Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2 = 200°C (Time 2 = 8.75 min.). Rate = 4°C/min., Injector Temp. = 200°C, Detector Temp. = 220°C. Analyst: Pedro Renteria. NOTE: Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately. Long term storage is not recommended. Please contact our technical department if further information is required.

TIC: [BSB2]79005.D

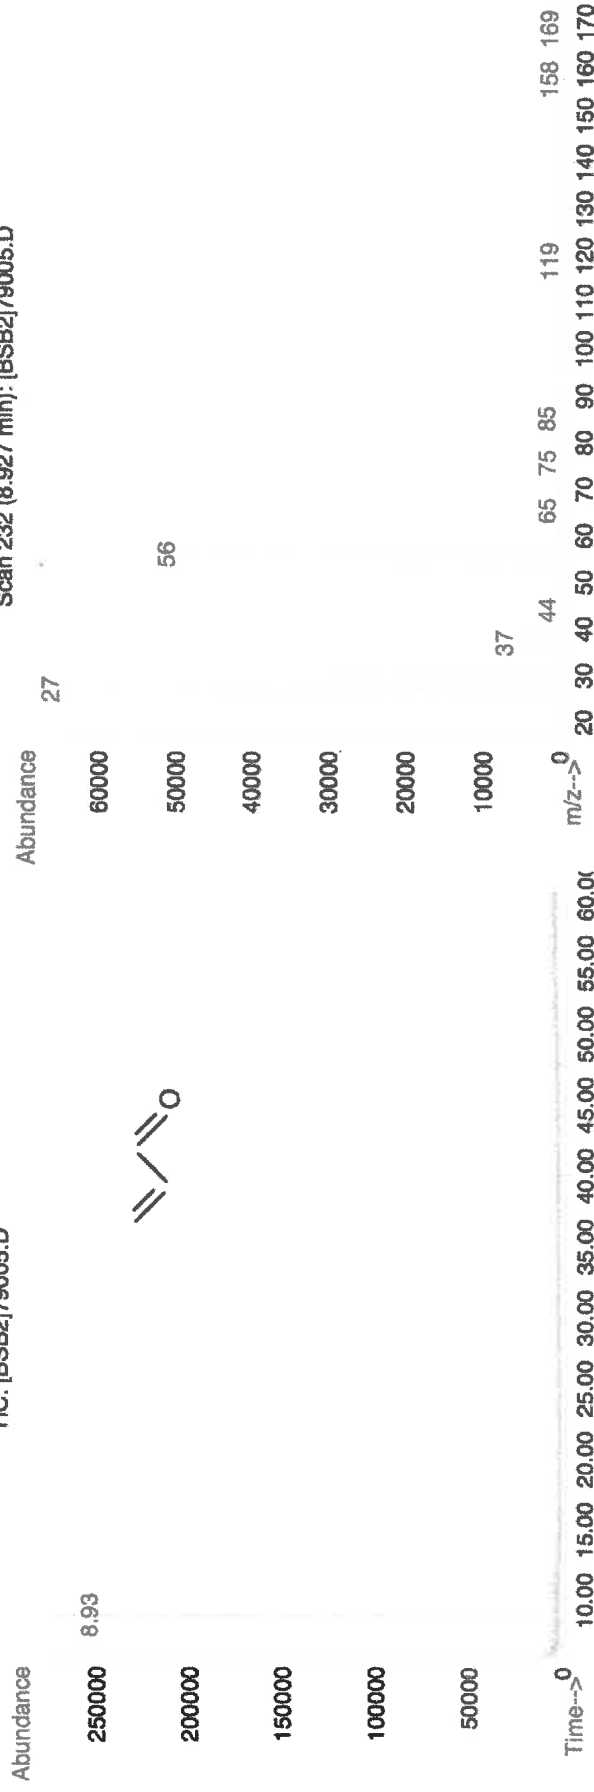

• The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
• Standards are prepared gravimetrically using balances that are calibrated by an ISO 17025 certified organization with weights traceable through NIST to the SI Kilogram (see above).
• Standards are certified (±) 0.5% of the stated value, unless otherwise stated.
• All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
• Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).
Rev 1A, 2/25/2025



Certified Reference Material CRM



Re 101625 5109

CERTIFIED WEIGHT REPORT

Part Number:
Lot Number:
Description:

91980
101625
Acrolein

Solvent(s):
Water

Lot#
041725Q

Expiration Date:
Recommended Storage:
Nominal Concentration (µg/mL):
NIST Test ID#:

111625
Refrigerate (2°C to 8°C)
5000
6UTB

5E-05 Balance Uncertainty
0.001 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL):


10.0

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
----------	-----	------------	----------------------	------------	-------------	------------------	------------------	---------------------	------------------------------------	------	----------------	------

1. Acrolein 5 103755V10F 5000 97 0.5 0.05166 0.05180 5013.7 52.6 107-02-8 0.1 ppm orl-rat 48mg/kg

Method: GC6MSD-1. Detector: Mass Selective Detector (Scan mode). Columns: Vool (60m X 0.25mm ID X 1.5µm film thickness). Oven Profile: Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C (Time 2 = 8.75 min.). Rate = 4°C/min., Injector Temp. = 200°C, Detector Temp. = 220°C. Analyst: Pedro Renteria. NOTE: Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately. Long term storage is not recommended. Please contact our technical department if further information is required.

TIC: [BSB2]79005.D

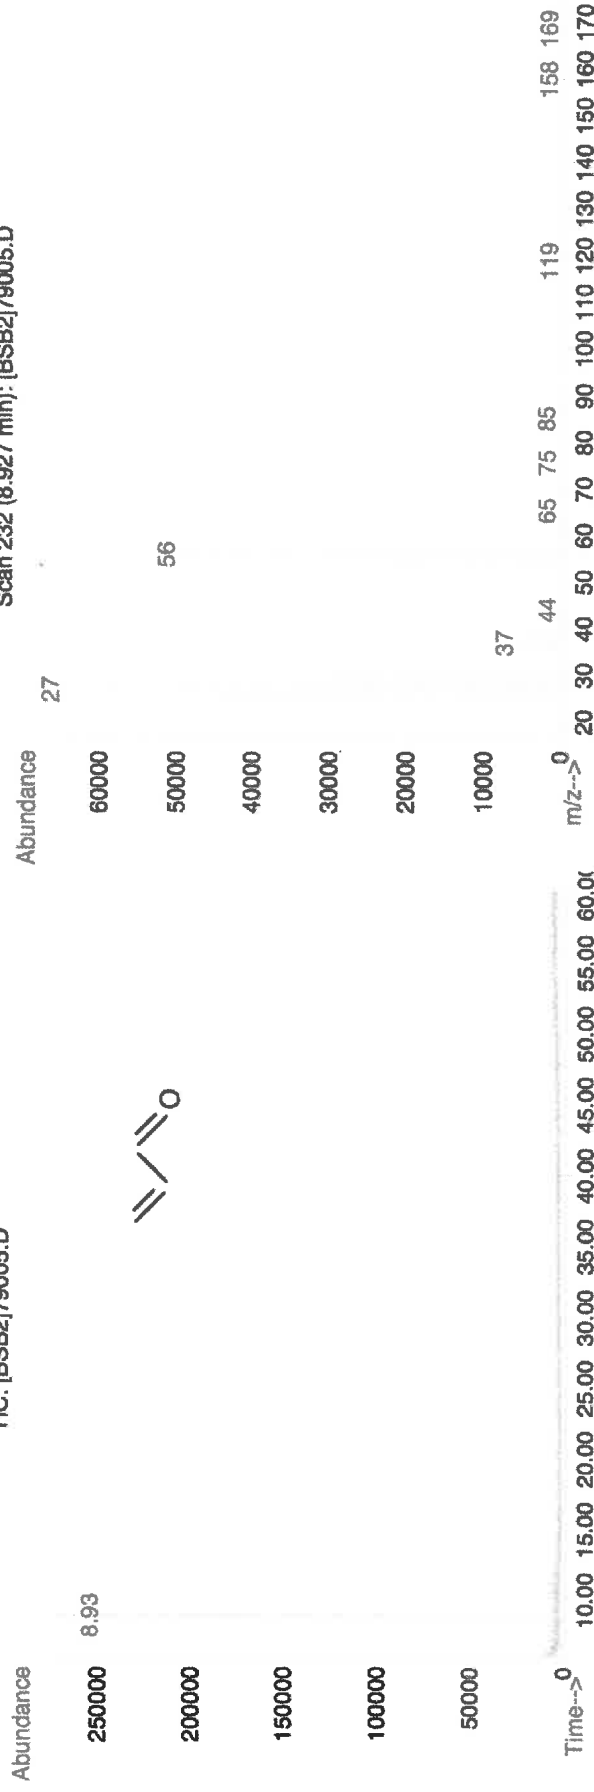

• The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
• Standards are prepared gravimetrically using balances that are calibrated by an ISO 17025 certified organization with weights traceable through NIST to the SI Kilogram (see above).
• Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
• All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
• Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).
Rev 1A, 2/25/2025

Preservation Log

BalanceID: VOA-SC-2

Review By: Amit

Supervise By: MMDadoda

Seq	LabID	Vial A Weight (g)	Vial A Time	Vial B Weight (g)	Vial B Time	Vial C Weight(g) with MeOH	Vial C Time	Methanol ID	Preservation Date	Comments
1	Q3410-02	5.02	10:00	5.03	10:01	4.51	10:02	V14921	10/21/2025	JAR SAMPLE 8260 STORED IN FRZ #2

Instructions : For medium Level analysis, 5ml MeOH added for CLP(SOM/SFAM) method and 10ml for regular 8260.

If the samples are not to be analyzed within 48hrs of sampling, preserve samples immediately, Vials A and B are stored in the VOA-FRZ-2.

Vial C - MeOH preserved vials are kept in VOA-REF #6.



SHIPPING DOCUMENTS

Q 3410

49 Moore Place

CHEMTECH

CHAIN OF CUSTODY RECORD

284 Sheffield Street, Mountainside, NJ 07092
(908) 789-8900 Fax (908) 789-8922
www.chemtech.net

Chemtech Project Number Belleville
COC Number Belleville

CLIENT INFORMATION		PROJECT INFORMATION		BILLING INFORMATION	
Report to be sent to:		PROJECT NAME:		BILL TO:	PO#
COMPANY:		PROJECT #:	LOCATION:	ADDRESS:	
ADDRESS:		PROJECT MANAGER:		CITY:	STATE: ZIP:
CITY:	STATE: ZIP:	E-MAIL:		ATTENTION:	
ATTENTION:		PHONE:	FAX:	PHONE:	
PHONE: FAX:					

DATA TURNAROUND INFORMATION		DATA DELIVERABLE INFORMATION		ANALYSIS	
FAX (RUSH):	DAYS*	☐ Level 1 (Results Only)	☐ Level 4 (QC + Full Raw Data)		
HARDCOPY (DATA PACKAGE):	DAYS*	☐ Level 2 (Results + QC)	☐ NJ Reduced ☐ US EPA CLP		
EDD:	DAYS*	☐ Level 3 (Results + QC + Raw Data)	☐ NYS ASP A ☐ NYS ASP B		
*TO BE APPROVED BY CHEMTECH		☐ EDD FORMAT	☐ Other		
STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS DAYS					

CHEMTECH SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# of Bottles	PRESERVATIVES									COMMENTS	
			COMP	GRAB	DATE	TIME		1	2	3	4	5	6	7	8	9		
1.	WASTE				10/20	2:30	1	X										
2.	VOC					8:30	1		X									
3.	1					10:30	1			X								
4.	2					10:45	1			X								
5.	3					2:45	1			X								
6.	4					2:45	1			X								
7.	5					9:15	1			X								
8.																		
9.																		
10.																		

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE PROSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER	DATE/TIME 1550	RECEIVED BY	1550	Conditions of bottles or colors at receipt: ☐ COMPLAINT ☐ NON COMPLAINT ☐ COOLER TEMP <u>3.5°</u>
1.	10-20-25	1.	10-20-25	Comments:
RELINQUISHED BY	DATE/TIME	RECEIVED BY		
2.		2.		
RELINQUISHED BY	DATE/TIME 1710	RECEIVED FOR LAB BY		CLIENT: ☐ Hand Delivered ☐ Other: _____
3.	10-20-25	3.		CHEMTECH: ☐ Picked Up
Page _____ of _____				Shipment Complete ☐ YES ☐ NO

10/20/18

WHITE - CHEMTECH COPY FOR RETURN TO CLIENT

YELLOW - CHEMTECH COPY

PINK - SAMPLER COPY


Laboratory Certification

Certified By	License No.
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255425
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	TX-C25-00189
Virginia	460312

LOGIN REPORT/SAMPLE TRANSFER

Order ID : Q3410	SCIA01	Order Date : 10/20/2025 4:05:00 PM	Project Mgr :
Client Name : Sciacca General Contractor:		Project Name : 49 Moore Place Belleville	Report Type : Results Only
Client Contact : Rosanne Scirica		Receive DateTime : 10/20/2025 5:00:00 PM	EDD Type : EXCEL NJCLEANUP
Invoice Name : Sciacca General Contractor:		Purchase Order : 5:10:00 	Hard Copy Date :
Invoice Contact : Rosanne Scirica			Date Signoff :

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DUE DATES
Q3410-02	VOC	Solid	10/20/2025	08:30	VOC-TCLVOA-10		8260D		10 Bus. Days

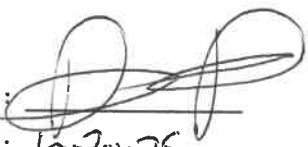Relinquished By : 

Date / Time : 10-20-25

Received By : 

Date / Time : 10/21/25 8:00

Storage Area : VOA Refridgerator Room

1846
P22